

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101323\
 Data File : PS024631.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2023 23:01
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 00:34:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.359	6.780	1005.7E6	331.6E6	488.856	479.624
Target Compounds							
1) T	Dalapon	2.511	2.572	7686262	3776595	3.111	3.375
5) T	DICAMBA	0.000	6.941	0	366522	N.D.	<MDL
6) T	MCP	6.683	6.984f	1539247	34652911	<MDL	17.585 #
7) T	MCPA	0.000	7.245	0	9231733	N.D.	2.881
8) T	DICHLORPROP	0.000	7.569	0	2537313	N.D.	3.374
9) T	2,4-D	7.249	7.787f	362.9E6	368117	131.350	<MDL #
10) T	Pentachlo...	0.000	8.264	0	1447284	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.622	0	1128314	N.D.	<MDL
12) T	2,4,5-T	0.000	8.995	0	1370760	N.D.	<MDL
13) T	2,4-DB	0.000	9.491	0	1107889	N.D.	2.174
14) T	DINOSEB	0.000	9.825	0	831675	N.D.	<MDL
15) T	Picloram	9.684	10.780	201.6E6	52712665	11.565	8.482 #
16) T	DCPA	0.000	10.780	0	52712665	N.D.	10.103



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101323\
Data File : PS024631.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2023 23:01
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 00:34:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

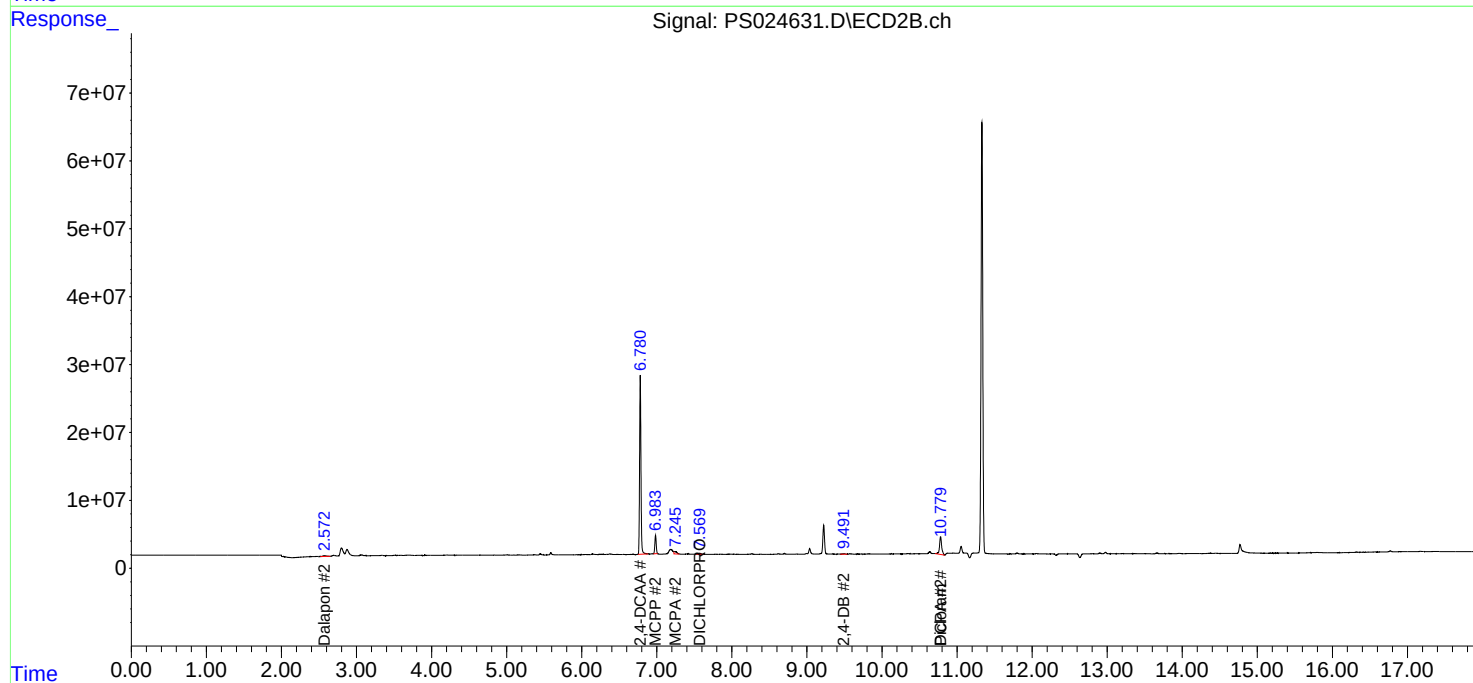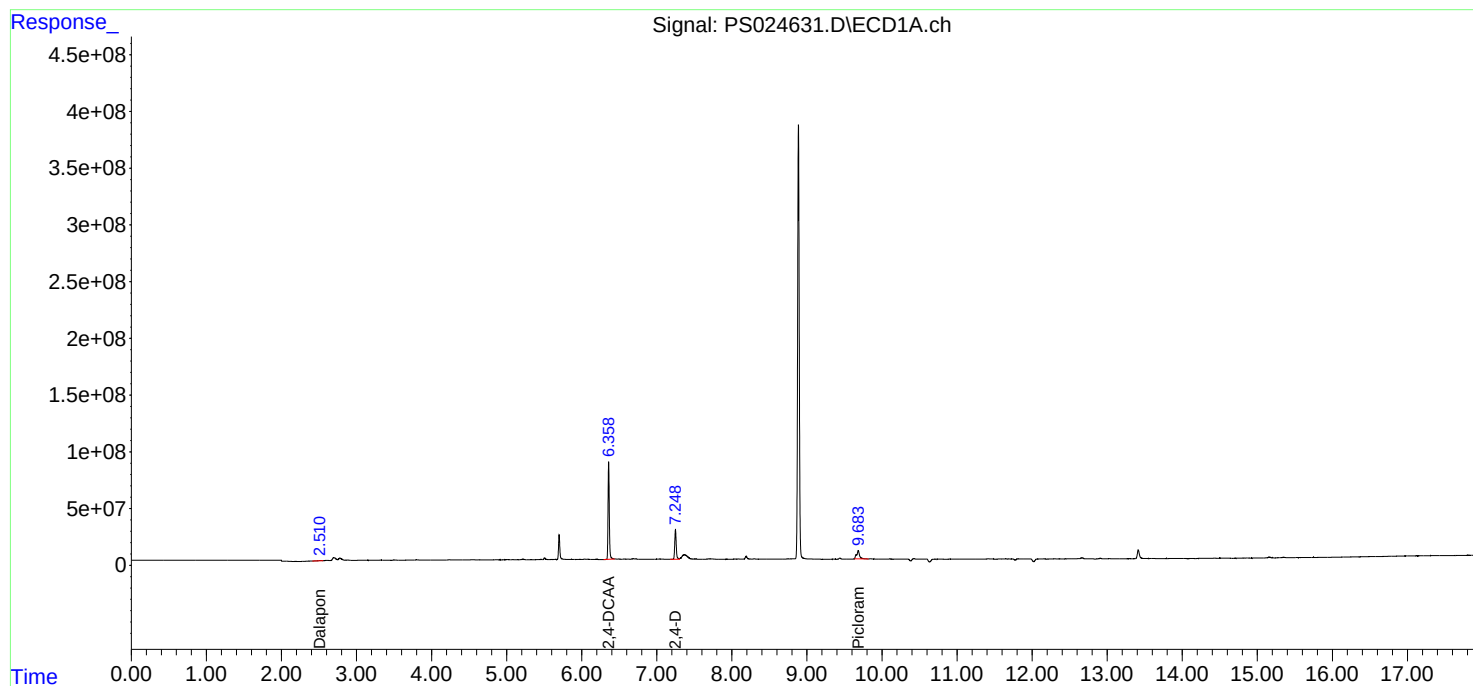


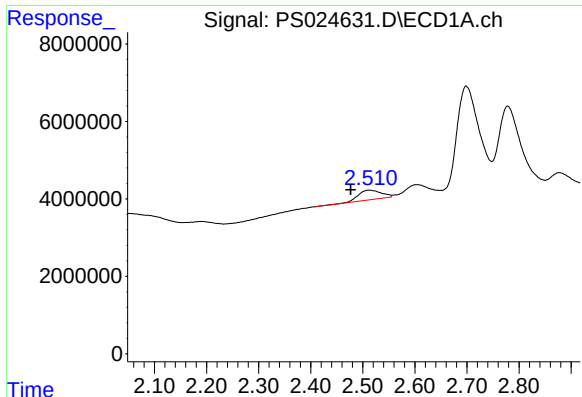

#1 Dalapon


R.T.: 2.511 min
Delta R.T.: 0.034 min
Response: 7686262
Conc: 3.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

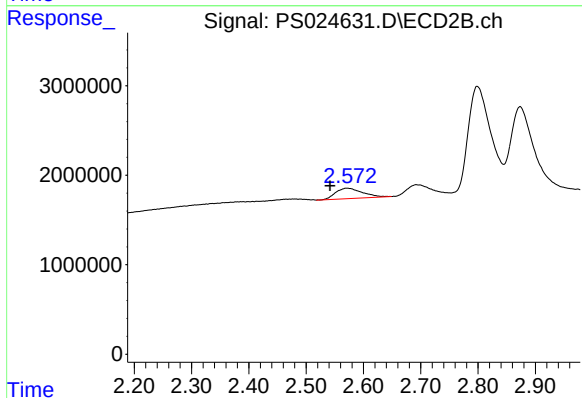


#1 Dalapon

R.T.: 2.572 min
Delta R.T.: 0.030 min
Response: 3776595
Conc: 3.37 ng/ml

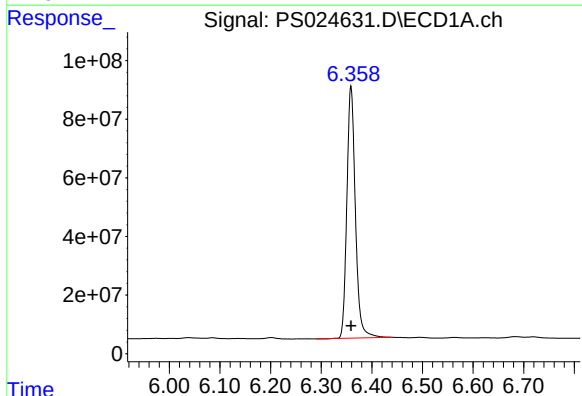


#4 2,4-DCAA

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 1005737747
Conc: 488.86 ng/ml

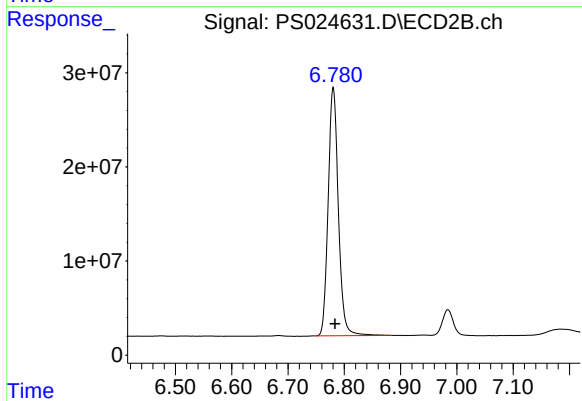

#4 2,4-DCAA


R.T.: 6.780 min
Delta R.T.: -0.003 min
Response: 331559796
Conc: 479.62 ng/ml

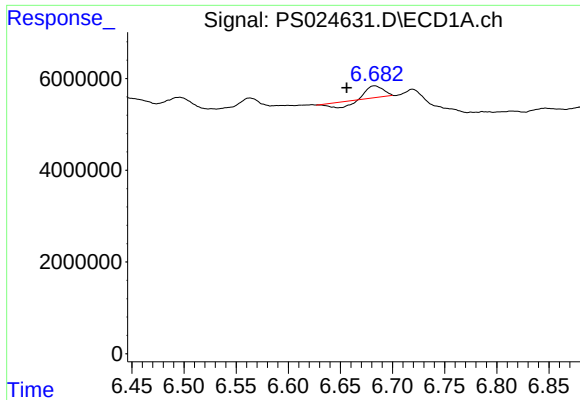

#6 MCP


R.T.: 6.683 min
Delta R.T.: 0.027 min
Response: 1539247
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

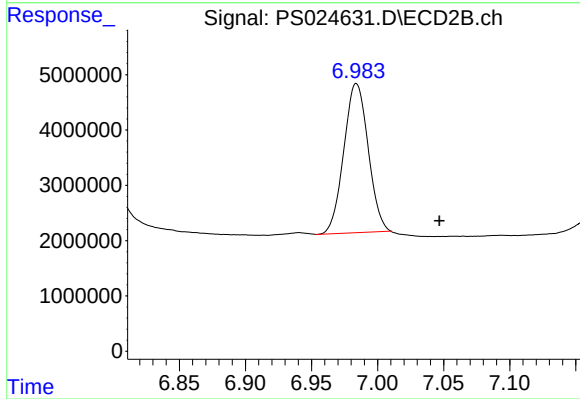


#6 MCP

R.T.: 6.984 min
Delta R.T.: -0.063 min
Response: 34652911
Conc: 17.58 ug/ml

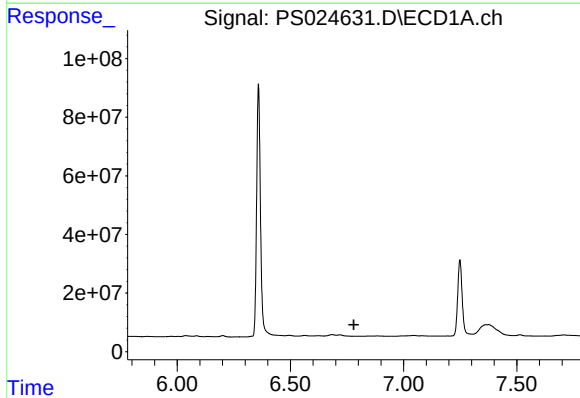


#7 MCP

R.T.: 0.000 min
Exp R.T. : 6.780 min
Response: 0
Conc: N.D.

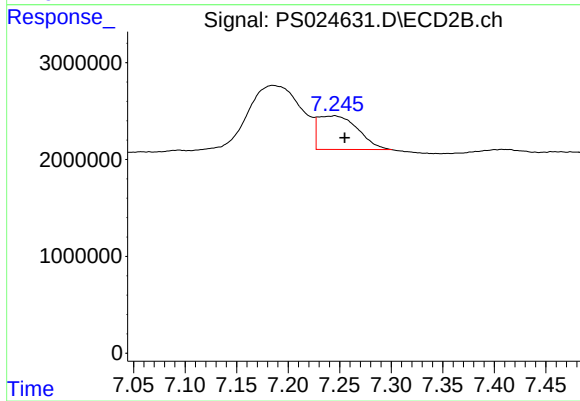

#7 MCP


R.T.: 7.245 min
Delta R.T.: -0.010 min
Response: 9231733
Conc: 2.88 ug/ml

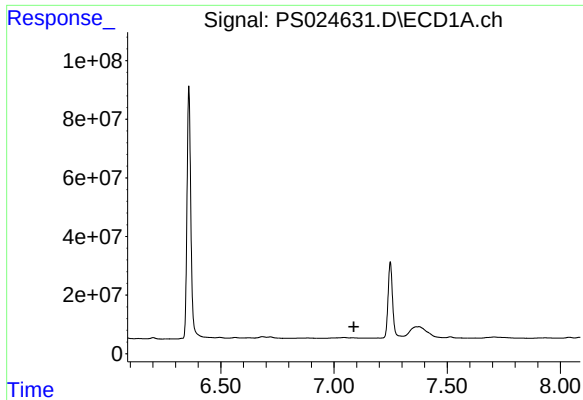

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

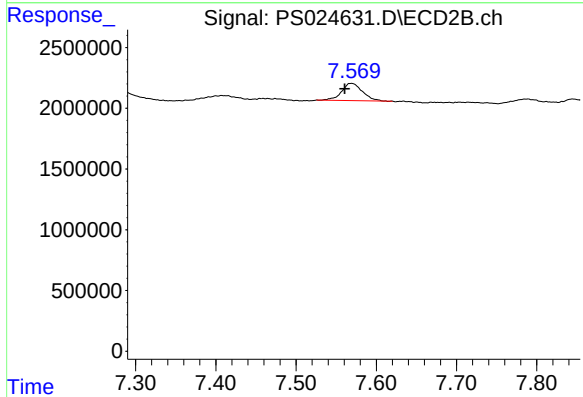


#8 DICHLORPROP

R.T.: 7.569 min
Delta R.T.: 0.008 min
Response: 2537313
Conc: 3.37 ng/ml

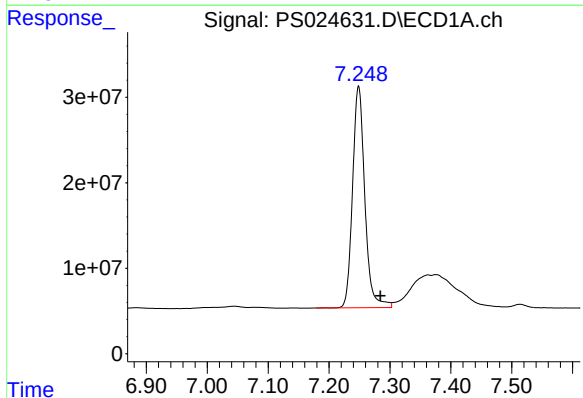


#9 2,4-D

R.T.: 7.249 min
Delta R.T.: -0.036 min
Response: 362919867
Conc: 131.35 ng/ml

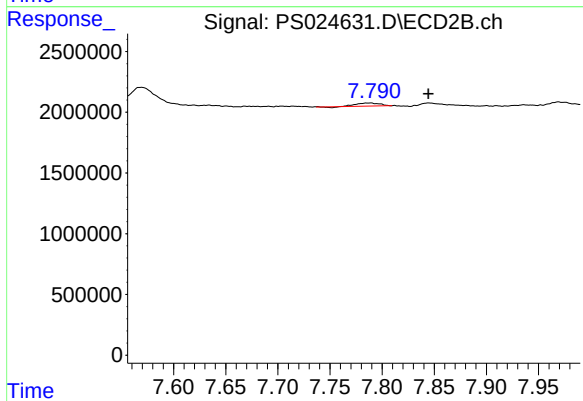

#9 2,4-D


R.T.: 7.787 min
Delta R.T.: -0.057 min
Response: 368117
Conc: N.D.

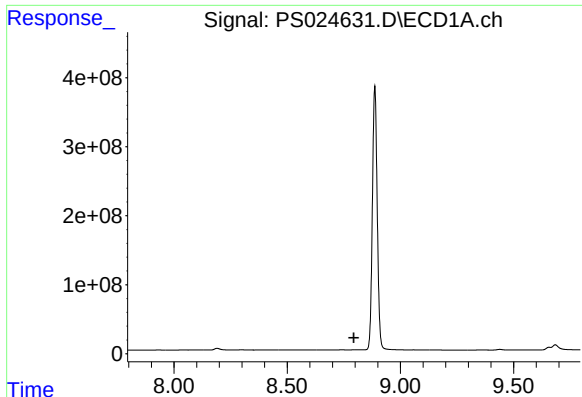

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

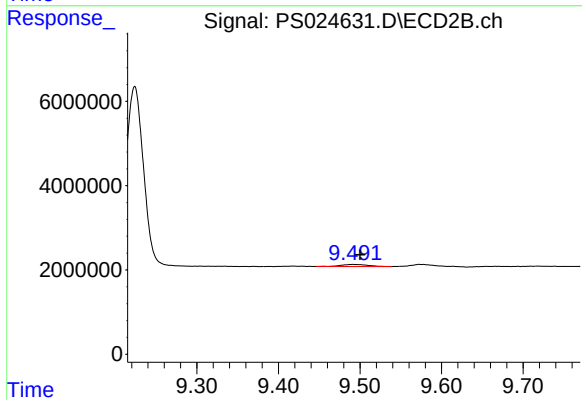


#13 2,4-DB

R.T.: 9.491 min
Delta R.T.: -0.009 min
Response: 1107889
Conc: 2.17 ng/ml

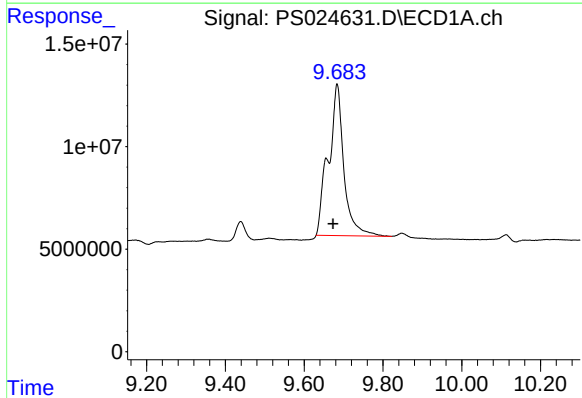


#15 Picloram

R.T.: 9.684 min
Delta R.T.: 0.011 min
Response: 201642577
Conc: 11.56 ng/ml

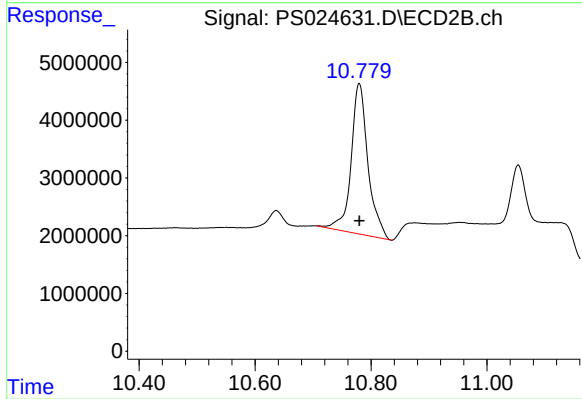

#15 Picloram


R.T.: 10.780 min
Delta R.T.: 0.000 min
Response: 52712665
Conc: 8.48 ng/ml

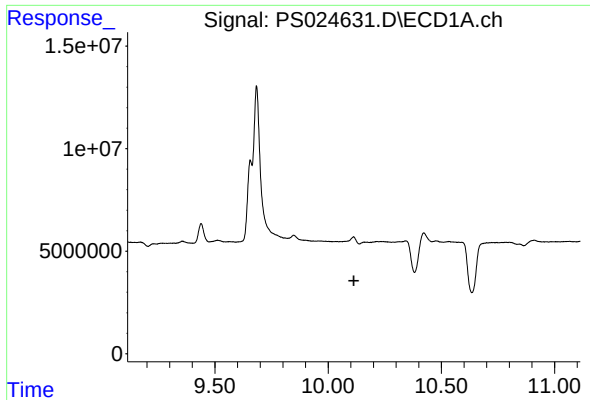

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

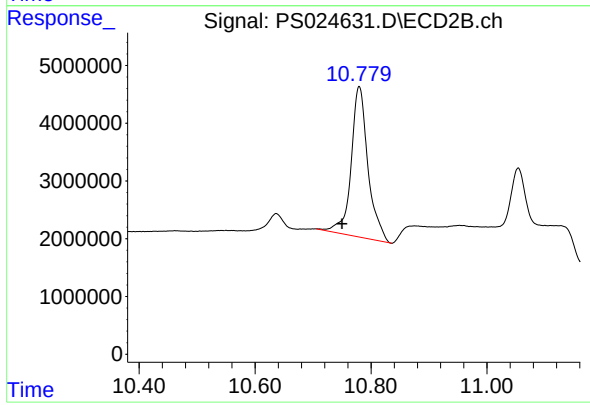

#16 DCPA

R.T.: 10.780 min
Delta R.T.: 0.030 min
Response: 52712665
Conc: 10.10 ng/ml