

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101325\
 Data File : PS031997.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2025 16:30
 Operator : AR\AJ
 Sample : Q3305-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 AU-06-100725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 09:06:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.285	7.750	434.7E6	143.6E6	91.183	130.526 #
Target Compounds							
1) T	Dalapon	2.638f	2.681	1698.7E6	1086.6E6	219.823	289.119 #
2) T	3,5-DICHL...	6.434	0.000	3451434	0	<MDL	N.D. #
3) T	4-Nitroph...	7.087	7.307	9041058	4012401	6.774	2.644 #
5) T	DICAMBA	7.481	0.000	3298849	0	<MDL	N.D. #
6) T	MCPD	7.680f	0.000	13986216	0	1.144	N.D. #
7) T	MCPA	7.800	8.262f	25651059	55994236	1.743	14.843 #
8) T	DICHLORPROP	0.000	8.663	0	12782903	N.D.	6.528
10) T	Pentachlo...	8.698	9.510	5644571	37476846	<MDL	<MDL #
11) T	2,4,5-TP ...	9.232f	9.882	15409666	287.3E6	<MDL	14.312 #
12) T	2,4,5-T	9.605f	10.327	294.3E6	342.7E6	11.659	19.990 #
13) T	2,4-DB	10.132	10.887	226.5E6	21587764	73.072	16.708 #
14) T	DINOSEB	11.311f	11.286	89873245	229.6E6	4.030	15.103 #
15) T	Picloram	11.165	0.000	22600794	0	<MDL	N.D. #
16) T	DCPA	11.629	0.000	66747411	0	1.817	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101325\
Data File : PS031997.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2025 16:30
Operator : AR\AJ
Sample : Q3305-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
AU-06-100725

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 09:06:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

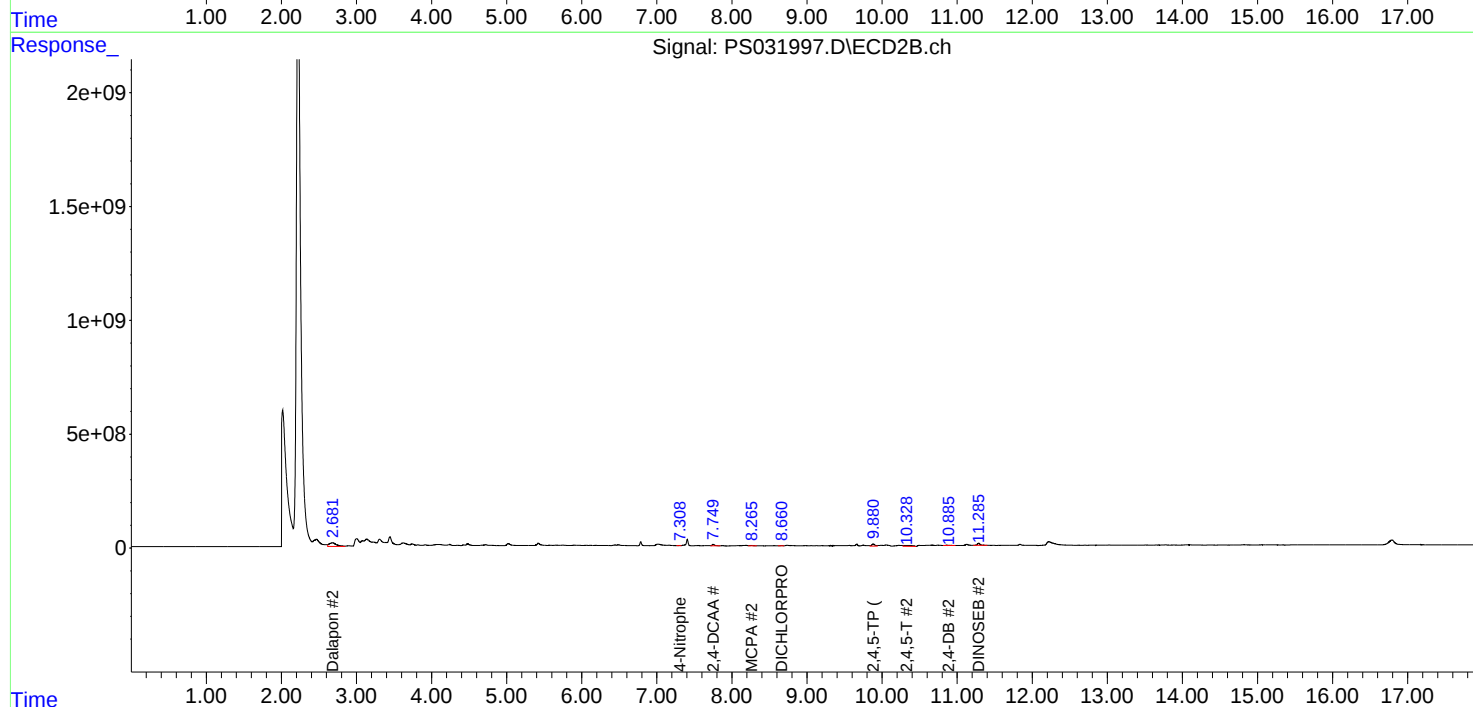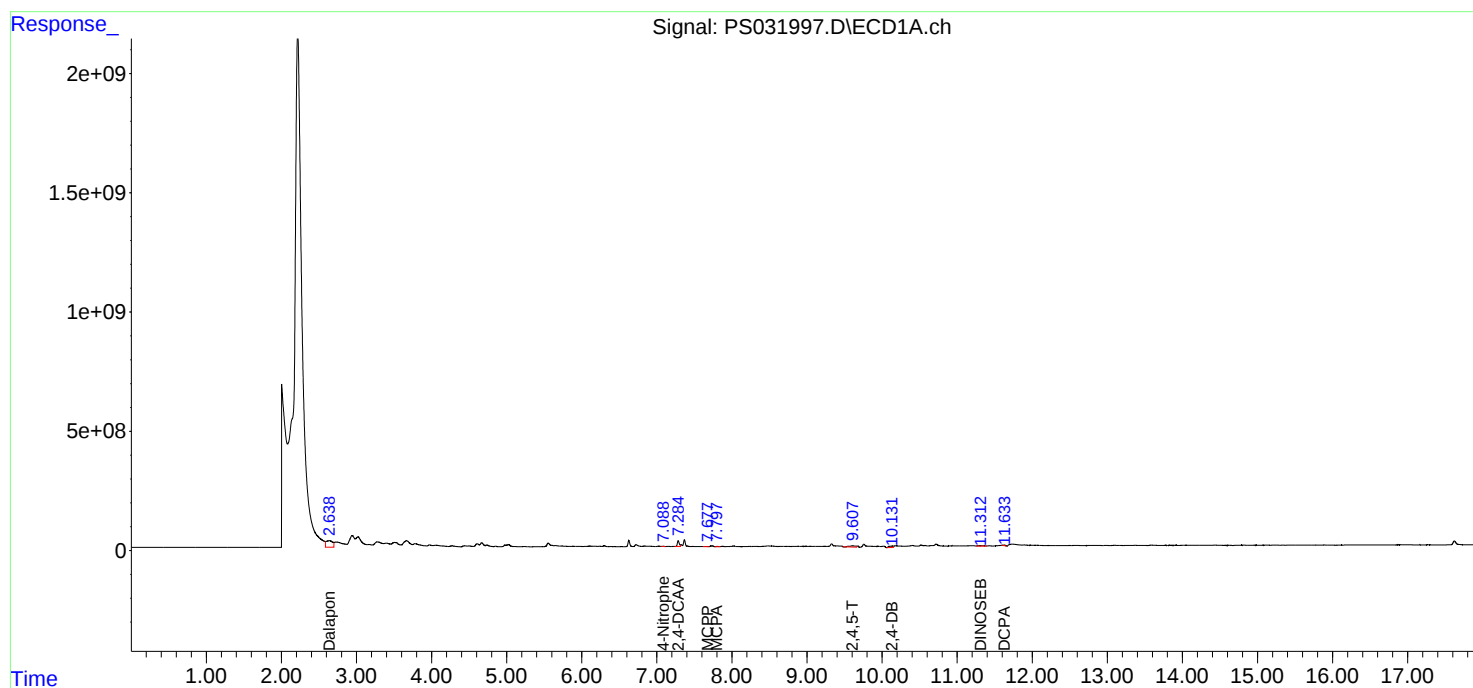


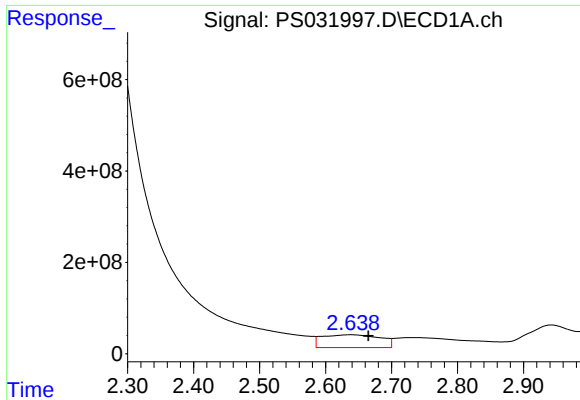

#1 Dalapon


R.T.: 2.638 min
Delta R.T.: -0.027 min
Response: 1698685606
Conc: 219.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-100725

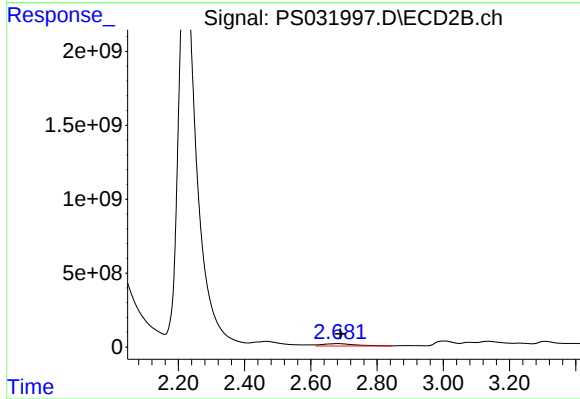


#1 Dalapon

R.T.: 2.681 min
Delta R.T.: -0.008 min
Response: 1086586688
Conc: 289.12 ng/ml

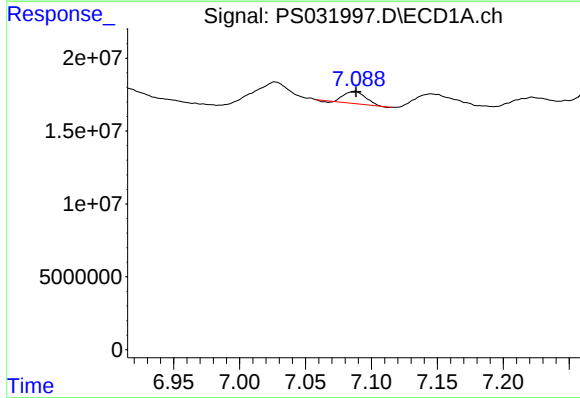


#3 4-Nitrophenol

R.T.: 7.087 min
Delta R.T.: -0.001 min
Response: 9041058
Conc: 6.77 ng/ml

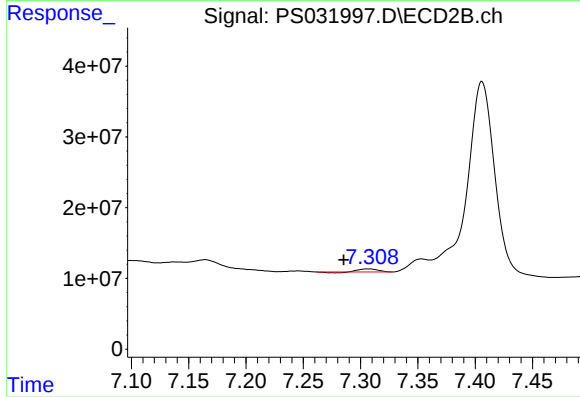

#3 4-Nitrophenol


R.T.: 7.307 min
Delta R.T.: 0.021 min
Response: 4012401
Conc: 2.64 ng/ml

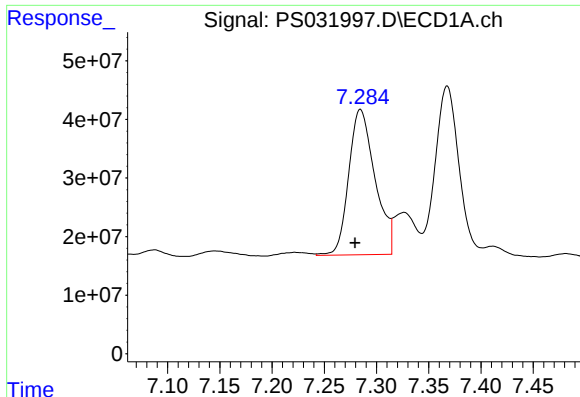

#4 2,4-DCAA


R.T.: 7.285 min
Delta R.T.: 0.005 min
Response: 434670832
Conc: 91.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-100725

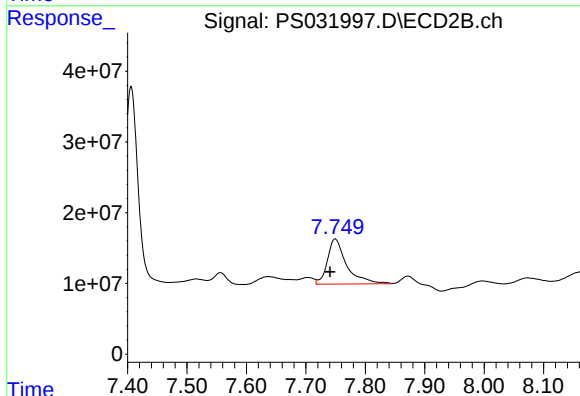


#4 2,4-DCAA

R.T.: 7.750 min
Delta R.T.: 0.009 min
Response: 143622744
Conc: 130.53 ng/ml

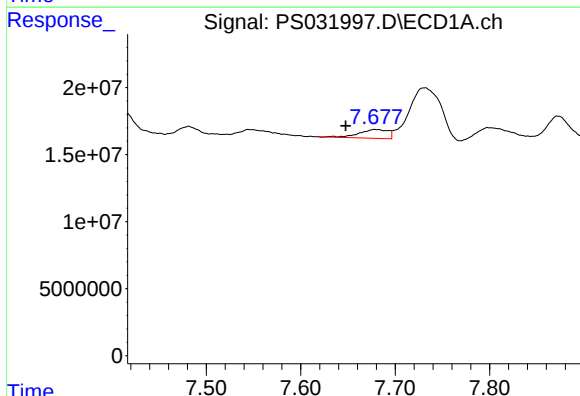


#6 MCPP

R.T.: 7.680 min
Delta R.T.: 0.032 min
Response: 13986216
Conc: 1.14 ug/ml

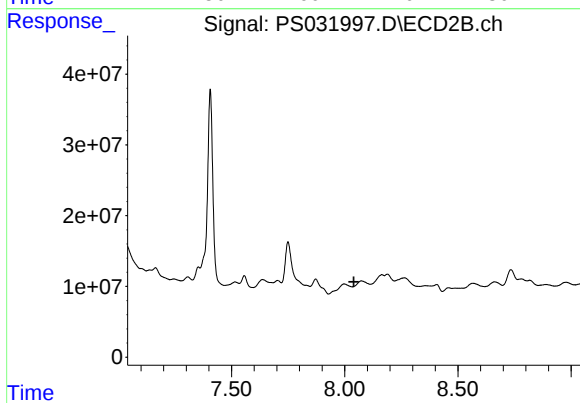

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 8.040 min
Response: 0
Conc: N.D.

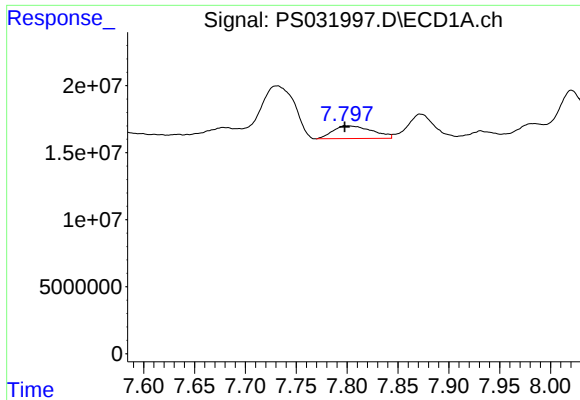

#7 MCPA


R.T.: 7.800 min
Delta R.T.: 0.003 min
Response: 25651059
Conc: 1.74 ug/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-100725

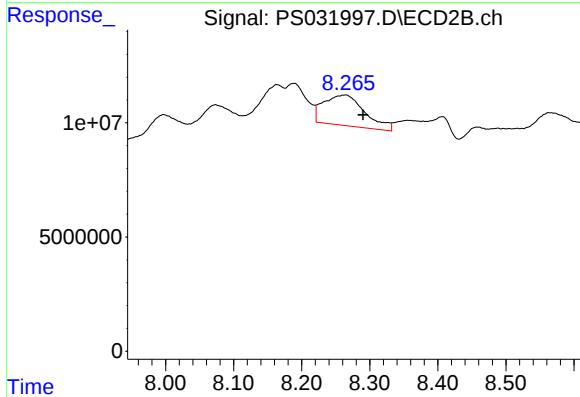


#7 MCPA

R.T.: 8.262 min
Delta R.T.: -0.029 min
Response: 55994236
Conc: 14.84 ug/ml

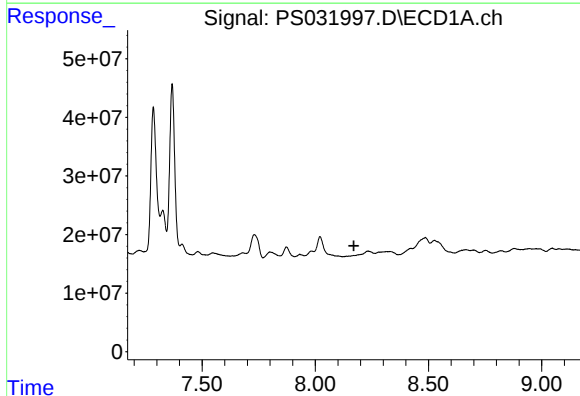


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.171 min
Response: 0
Conc: N.D.

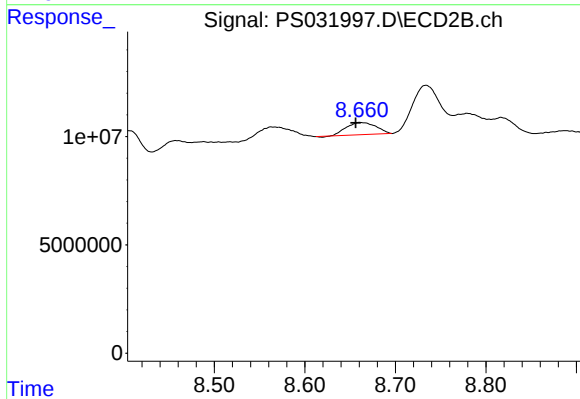

#8 DICHLORPROP


R.T.: 8.663 min
Delta R.T.: 0.007 min
Response: 12782903
Conc: 6.53 ng/ml

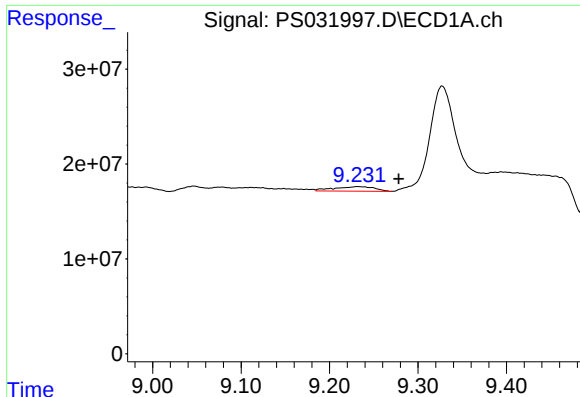

#11 2,4,5-TP (SILVEX)


R.T.: 9.232 min
Delta R.T.: -0.046 min
Response: 15409666
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
AU-06-100725

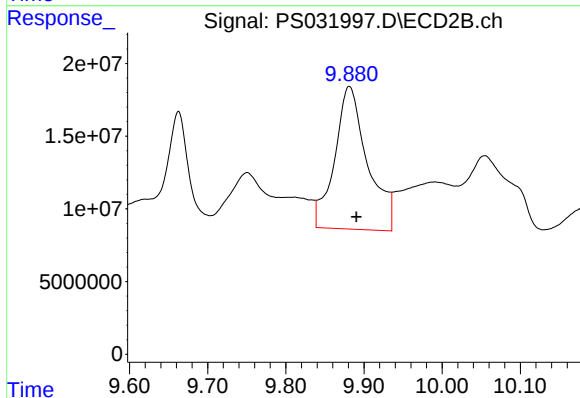


#11 2,4,5-TP (SILVEX)

R.T.: 9.882 min
Delta R.T.: -0.009 min
Response: 287317341
Conc: 14.31 ng/ml

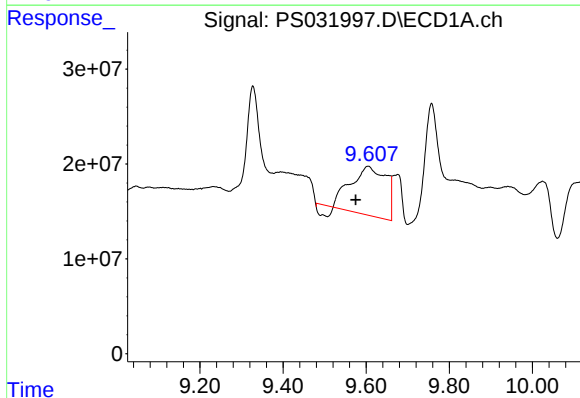


#12 2,4,5-T

R.T.: 9.605 min
Delta R.T.: 0.030 min
Response: 294315831
Conc: 11.66 ng/ml

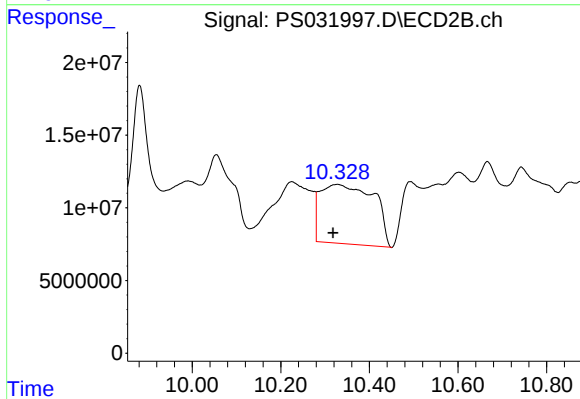

#12 2,4,5-T


R.T.: 10.327 min
Delta R.T.: 0.009 min
Response: 342725039
Conc: 19.99 ng/ml

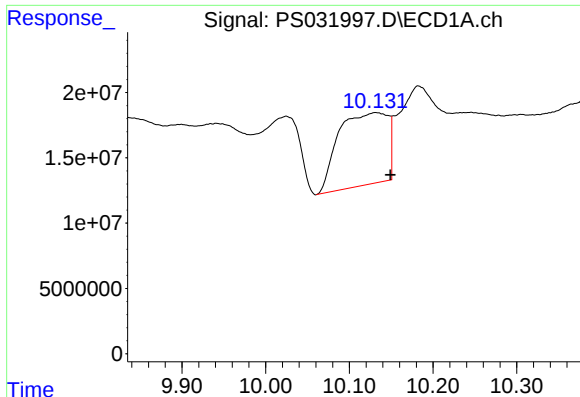

#13 2,4-DB


R.T.: 10.132 min
Delta R.T.: -0.017 min
Response: 226546319
Conc: 73.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-100725

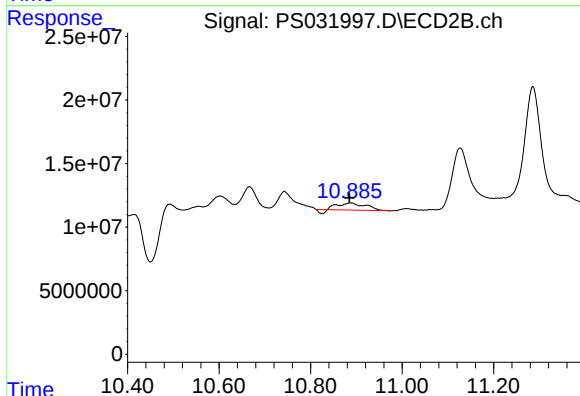


#13 2,4-DB

R.T.: 10.887 min
Delta R.T.: 0.002 min
Response: 21587764
Conc: 16.71 ng/ml

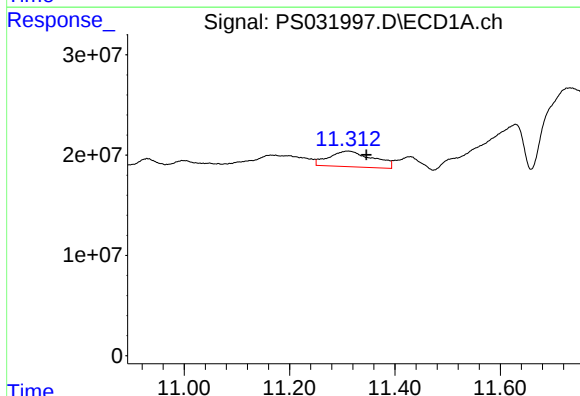


#14 DINOSEB

R.T.: 11.311 min
Delta R.T.: -0.035 min
Response: 89873245
Conc: 4.03 ng/ml

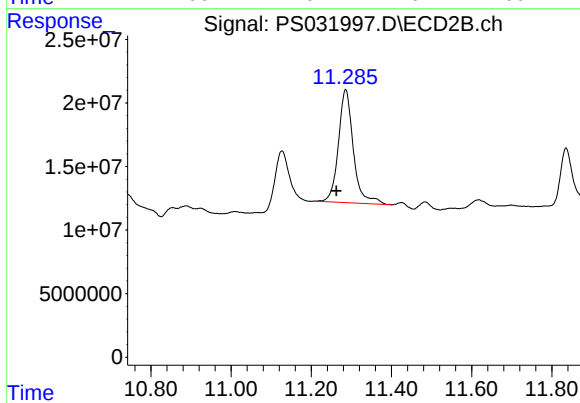

#14 DINOSEB


R.T.: 11.286 min
Delta R.T.: 0.023 min
Response: 229612845
Conc: 15.10 ng/ml

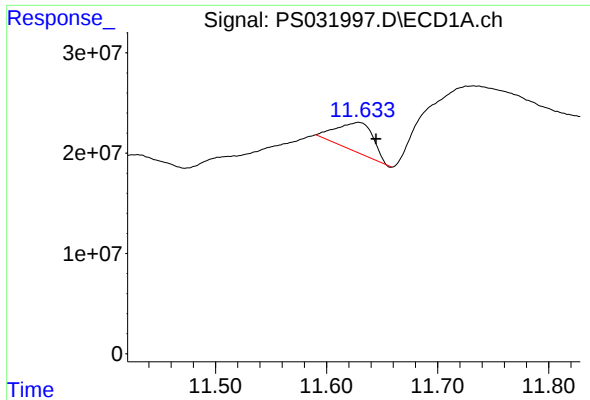

#16 DCPA

R.T.: 11.629 min
Delta R.T.: -0.016 min
Response: 66747411
Conc: 1.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
AU-06-100725

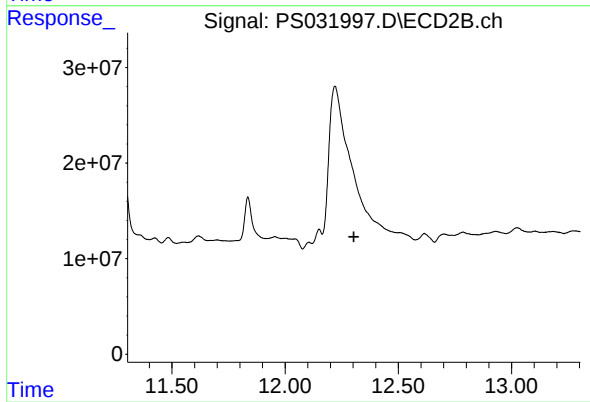

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 12.304 min
Response: 0
Conc: N.D.