

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101325\
 Data File : PS031998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Oct 2025 16:54
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 09:06:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.284	7.749	1688.9E6	457.7E6	354.294	415.967
Target Compounds							
1) T	Dalapon	0.000	2.647f	0	73157201	N.D.	19.466
2) T	3,5-DICHL...	6.446	0.000	10871380	0	1.544	N.D. #
7) T	MCPA	7.755f	8.243f	6654778	34501675	<MDL	9.146 #
8) T	DICHLORPROP	8.200f	0.000	1373539	0	<MDL	N.D. #
10) T	Pentachlo...	8.706	9.511	9397970	5734099	<MDL	<MDL #
11) T	2,4,5-TP ...	9.294	0.000	5435955	0	<MDL	N.D. #
12) T	2,4,5-T	9.620f	0.000	9149056	0	<MDL	N.D. #
13) T	2,4-DB	10.146	0.000	733005	0	<MDL	N.D. #
14) T	DINOSEB	11.347	0.000	6691447	0	<MDL	N.D. #
15) T	Picloram	11.181	0.000	8343602	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101325\
Data File : PS031998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Oct 2025 16:54
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 09:06:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

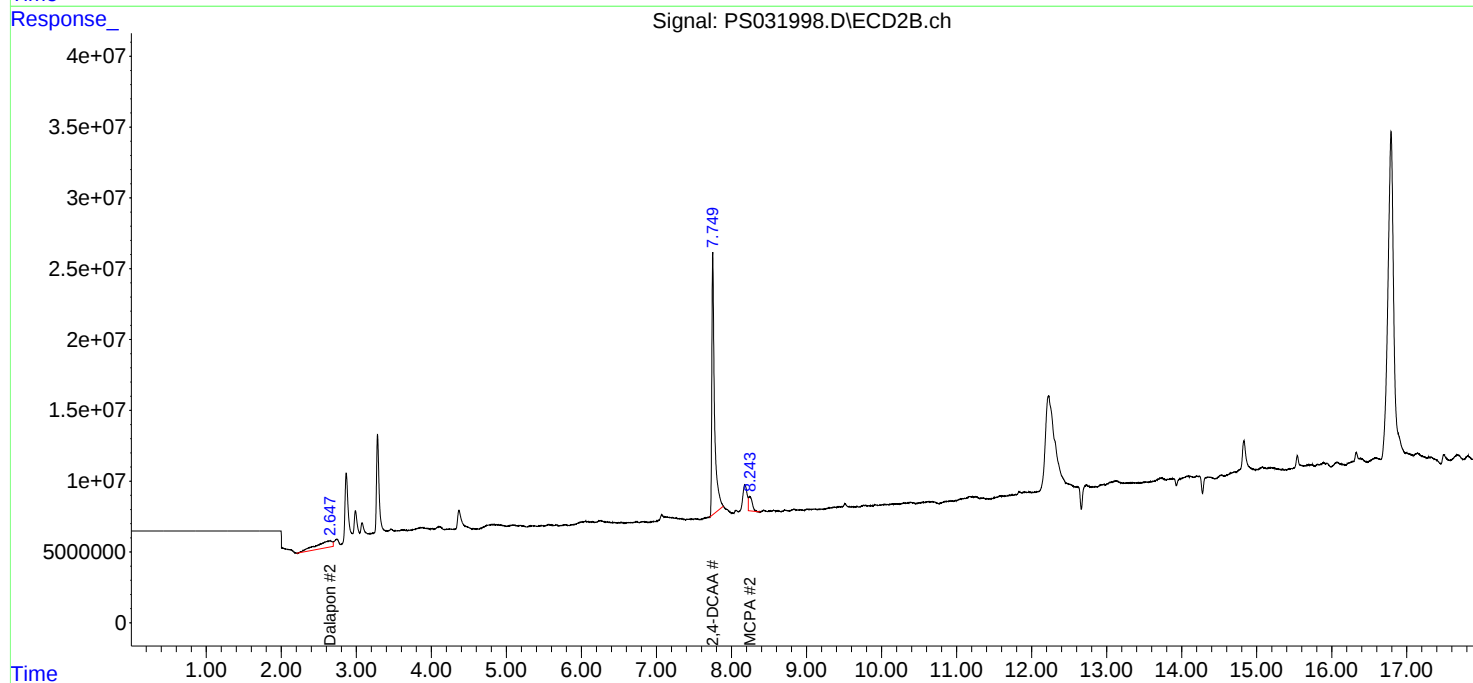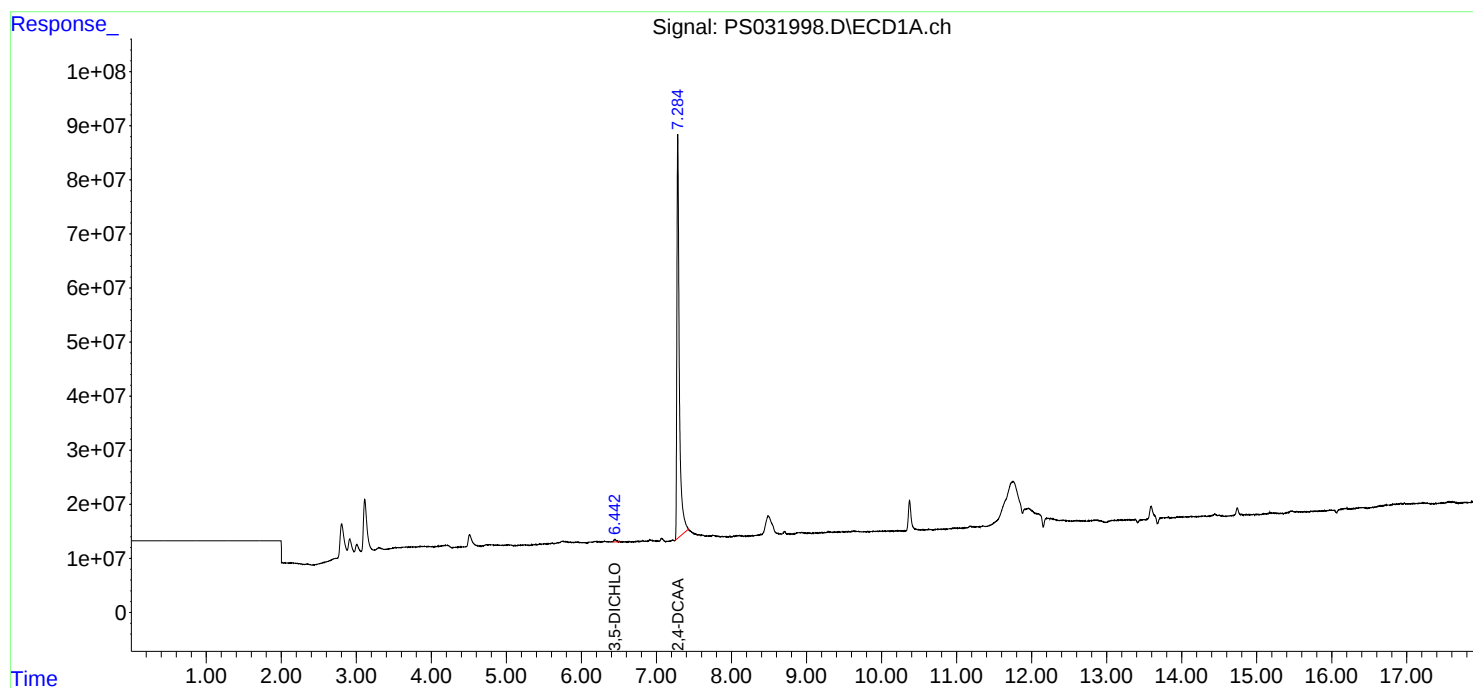


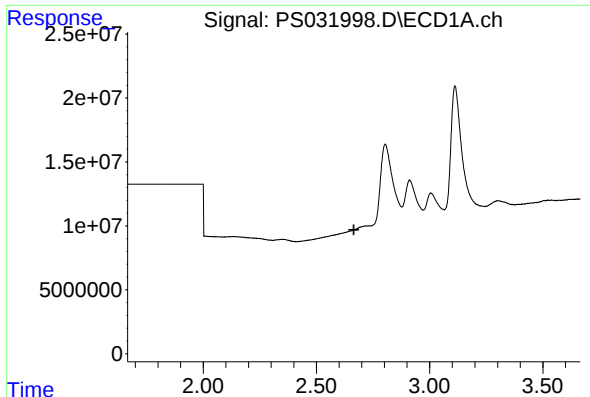

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.665 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

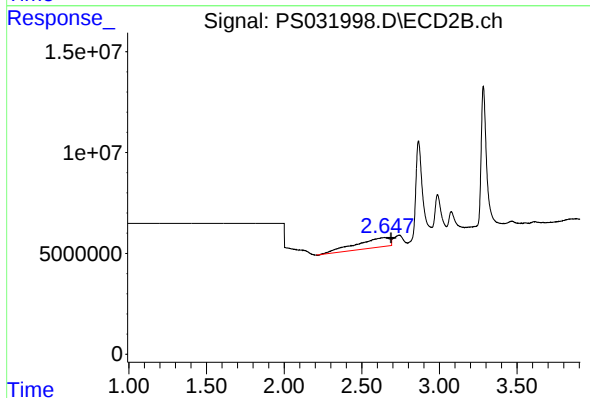


#1 Dalapon

R.T.: 2.647 min
Delta R.T.: -0.042 min
Response: 73157201
Conc: 19.47 ng/ml

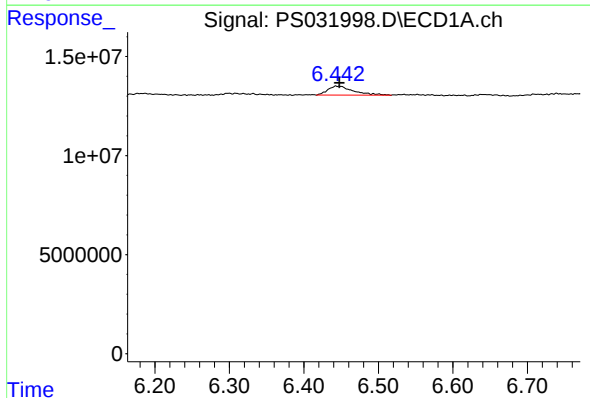


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.446 min
Delta R.T.: -0.002 min
Response: 10871380
Conc: 1.54 ng/ml

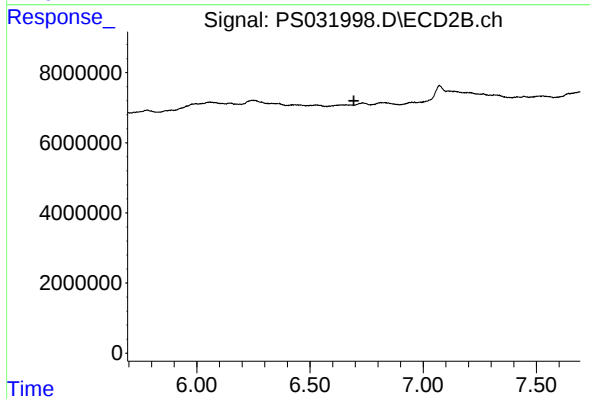

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.694 min
Response: 0
Conc: N.D.

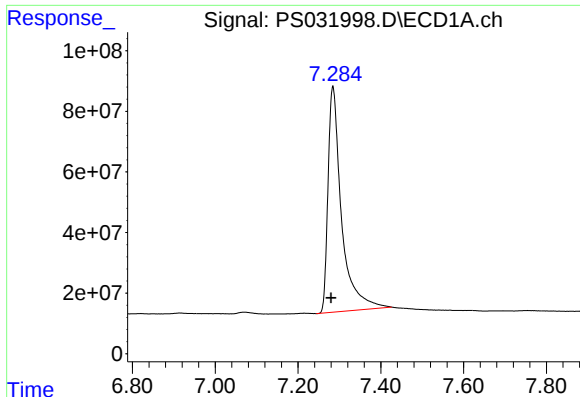

#4 2,4-DCAA


R.T.: 7.284 min
Delta R.T.: 0.005 min
Response: 1688934054
Conc: 354.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

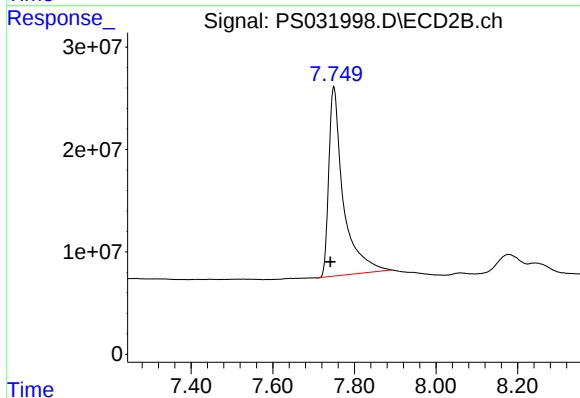


#4 2,4-DCAA

R.T.: 7.749 min
Delta R.T.: 0.008 min
Response: 457705118
Conc: 415.97 ng/ml

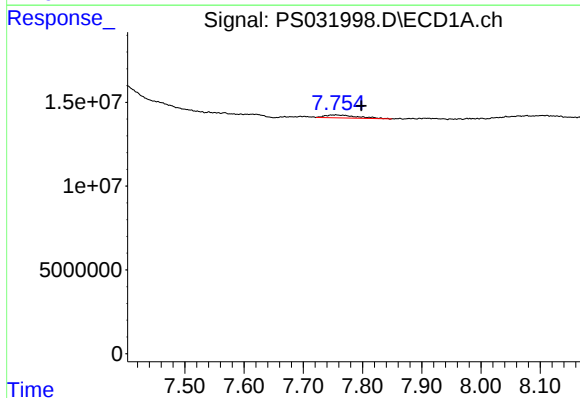

#7 MCPA

R.T.: 7.755 min
Delta R.T.: -0.043 min
Response: 6654778
Conc: N.D.

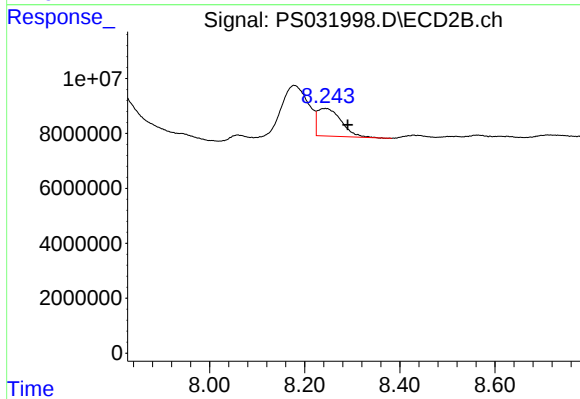

#7 MCPA

R.T.: 8.243 min
Delta R.T.: -0.047 min
Response: 34501675
Conc: 9.15 ug/ml