

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101419\
 Data File : PS007130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2019 14:56
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 17:44:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.443	5.174	504.5E6	297.7E6	368.572	423.305
Target Compounds							
5) T	DICAMBA	0.000	5.302	0	8441776	N.D.	3.244
7) T	MCPA	0.000	5.488	0	43785741	N.D.	15.062
9) T	2,4-D	6.493	0.000	72813773	0	59.086	N.D. #
10) T	Pentachlo...	0.000	6.468	0	13694836	N.D.	1.424
15) T	Picloram	8.998	8.934	80355548	104.1E6	7.280	16.960 #
16) T	DCPA	0.000	8.870	0	7568251	N.D.	1.509



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101419\
Data File : PS007130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2019 14:56
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 17:44:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

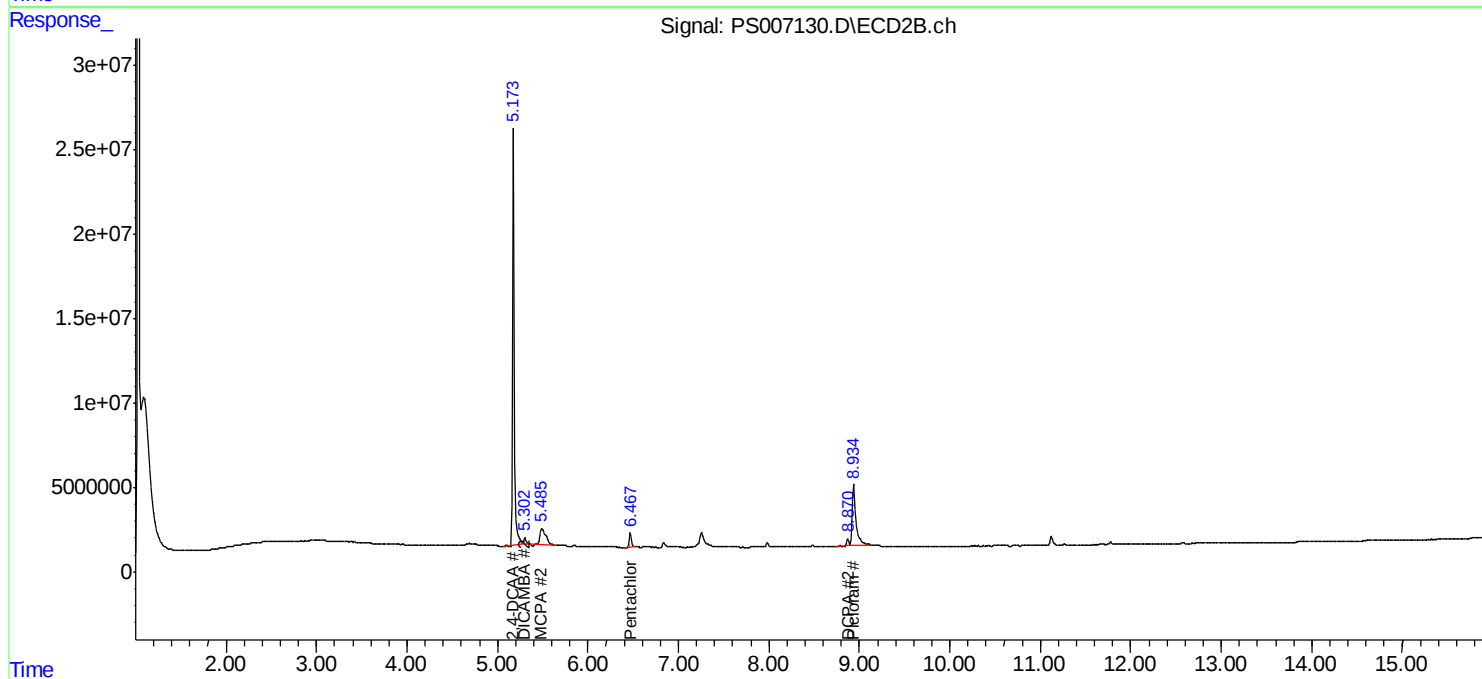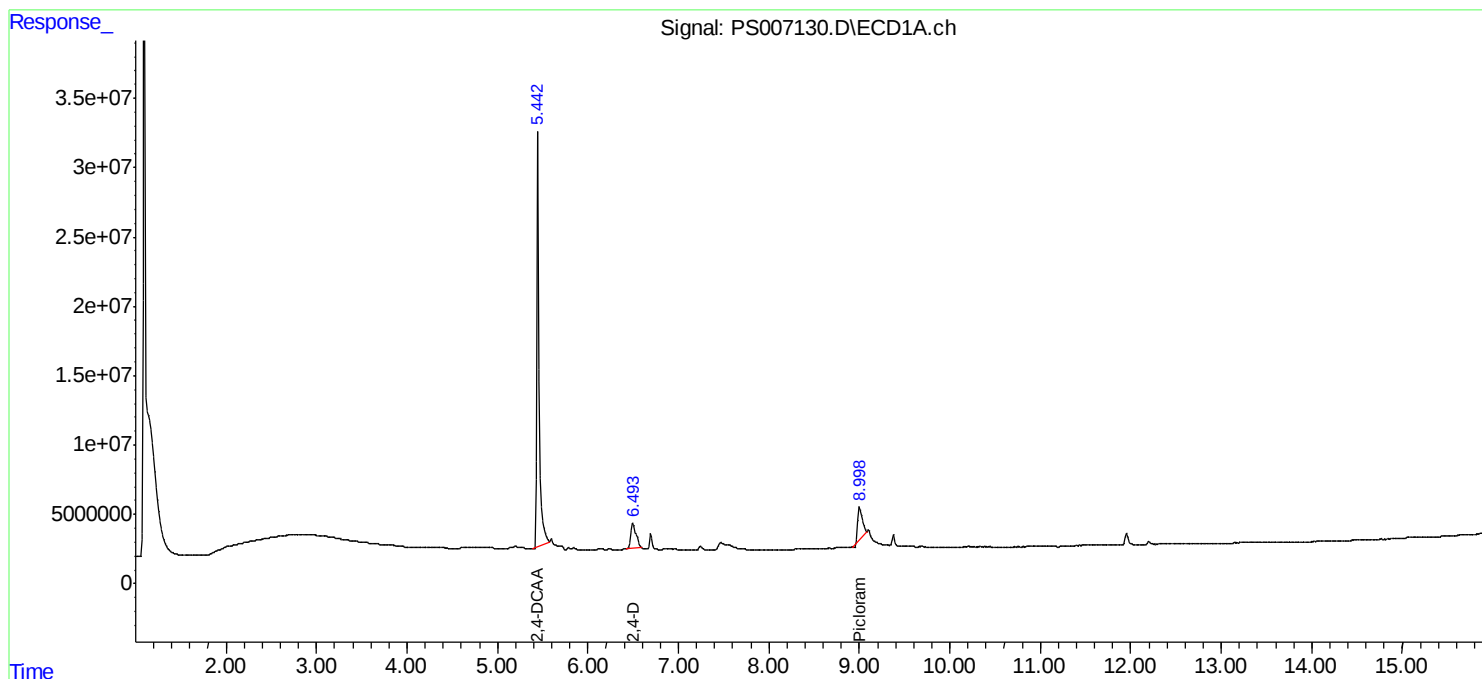


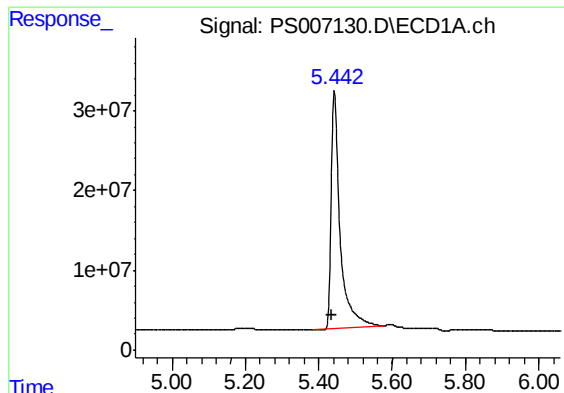

#4 2,4-DCAA


R.T.: 5.443 min
Delta R.T.: 0.007 min
Response: 504452514
Conc: 368.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

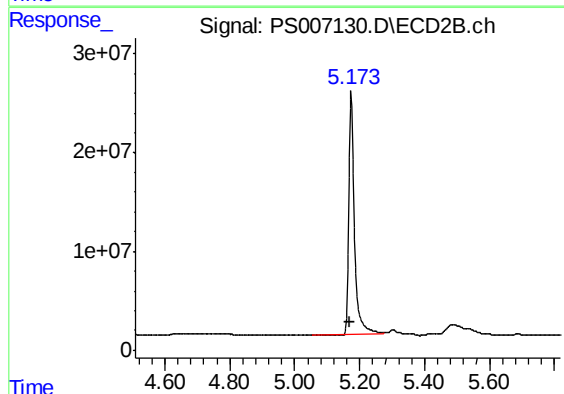


#4 2,4-DCAA

R.T.: 5.174 min
Delta R.T.: 0.005 min
Response: 297713246
Conc: 423.31 ng/ml

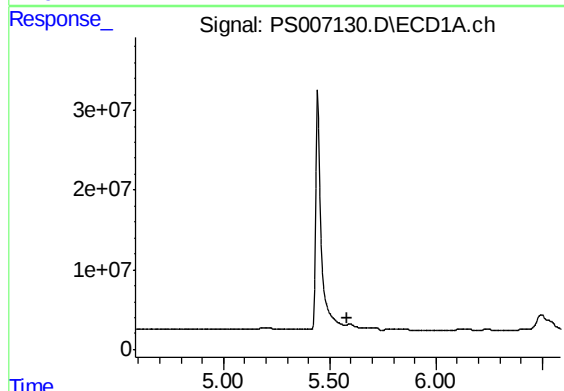


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.585 min
Response: 0
Conc: N.D.

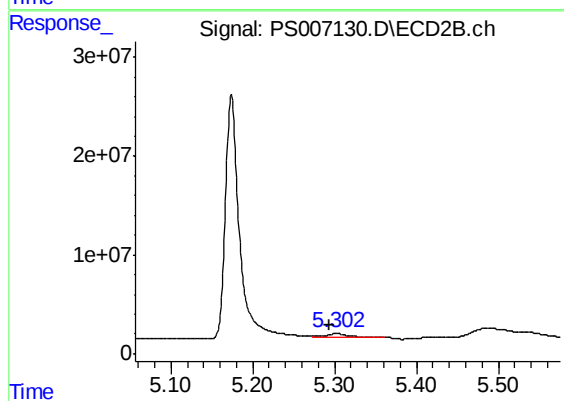

#5 DICAMBA


R.T.: 5.302 min
Delta R.T.: 0.008 min
Response: 8441776
Conc: 3.24 ng/ml

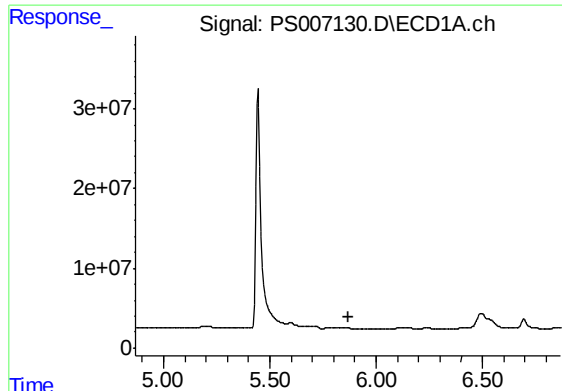

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

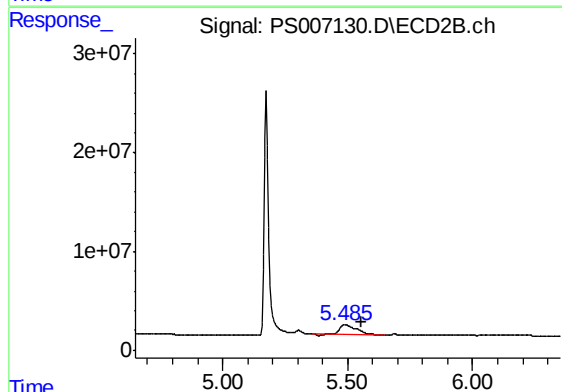


#7 MCPA

R.T.: 5.488 min
Delta R.T.: -0.067 min
Response: 43785741
Conc: 15.06 ug/ml

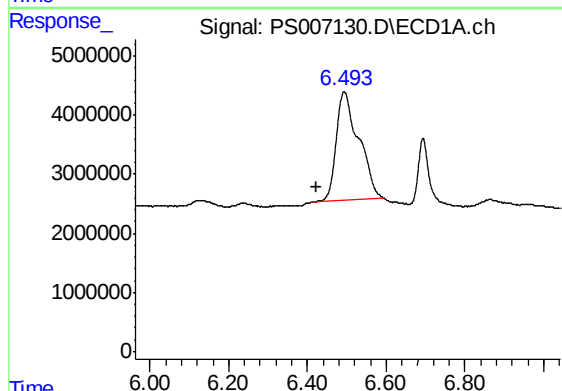


#9 2,4-D

R.T.: 6.493 min
Delta R.T.: 0.069 min
Response: 72813773
Conc: 59.09 ng/ml

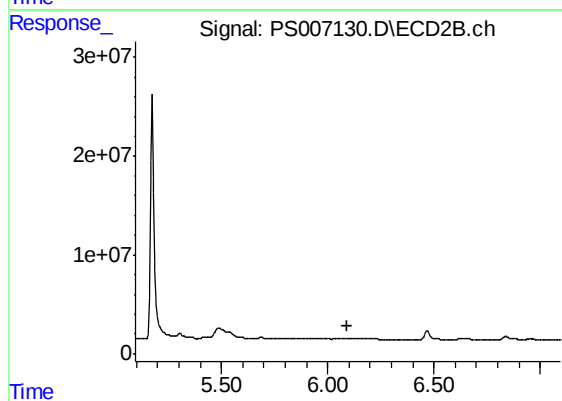

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.095 min
Response: 0
Conc: N.D.

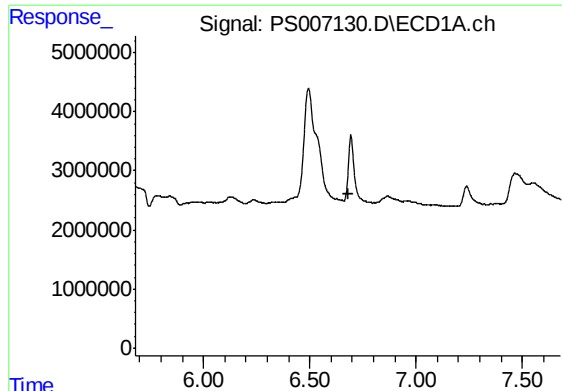

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

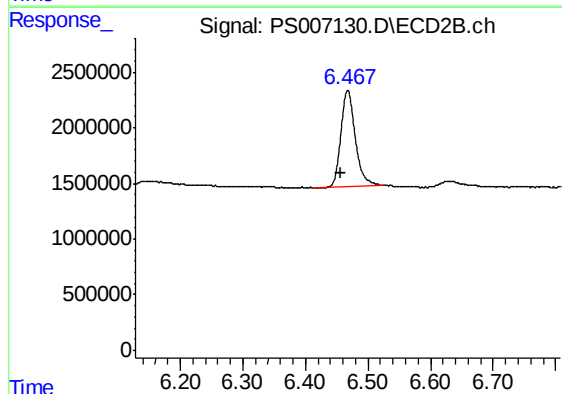


#10 Pentachlorophenol

R.T.: 6.468 min
Delta R.T.: 0.010 min
Response: 13694836
Conc: 1.42 ng/ml

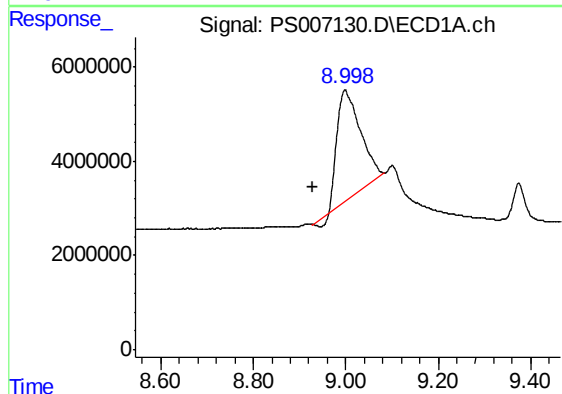


#15 Picloram

R.T.: 8.998 min
Delta R.T.: 0.069 min
Response: 80355548
Conc: 7.28 ng/ml

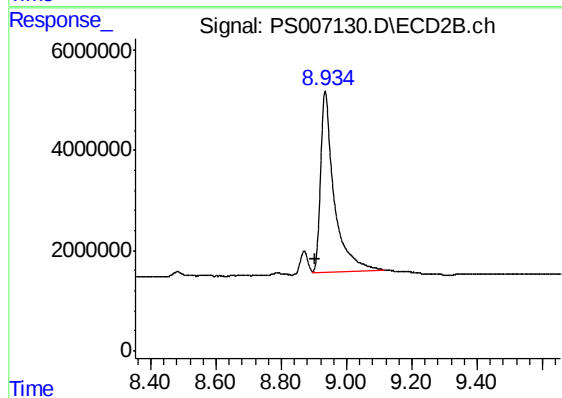

#15 Picloram


R.T.: 8.934 min
Delta R.T.: 0.030 min
Response: 104137590
Conc: 16.96 ng/ml

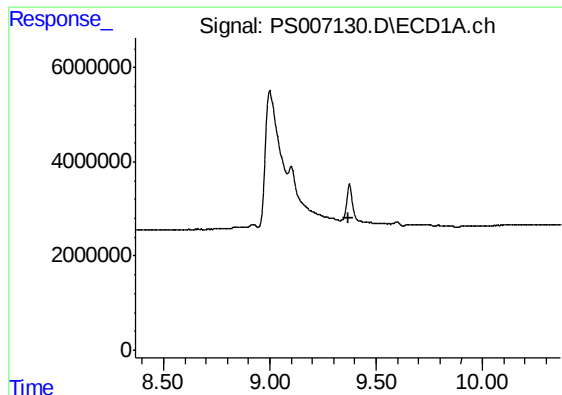

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

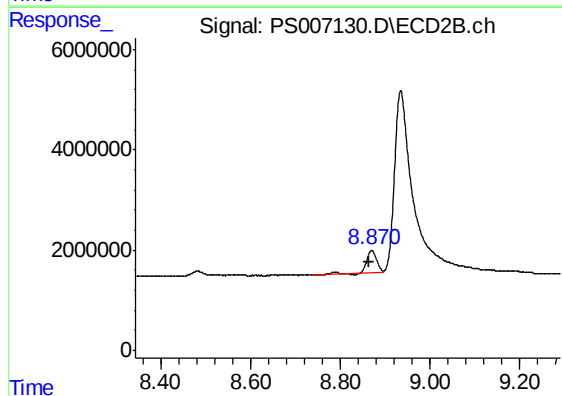

#16 DCPA

R.T.: 8.870 min
Delta R.T.: 0.007 min
Response: 7568251
Conc: 1.51 ng/ml