

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101419\
 Data File : PS007136.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2019 17:12
 Operator : SM\AJ
 Sample : PB123819BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB123819BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 17:46:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.442	5.173	487.4E6	275.7E6	356.112	391.967
Target Compounds							
7) T	MCPA	0.000	5.486	0 44789136		N.D.	15.407
9) T	2,4-D	6.491	0.000	70395408	0	57.123	N.D. #
15) T	Picloram	0.000	8.942	0 57046068		N.D.	9.291



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101419\
Data File : PS007136.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2019 17:12
Operator : SM\AJ
Sample : PB123819BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB123819BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 17:46:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

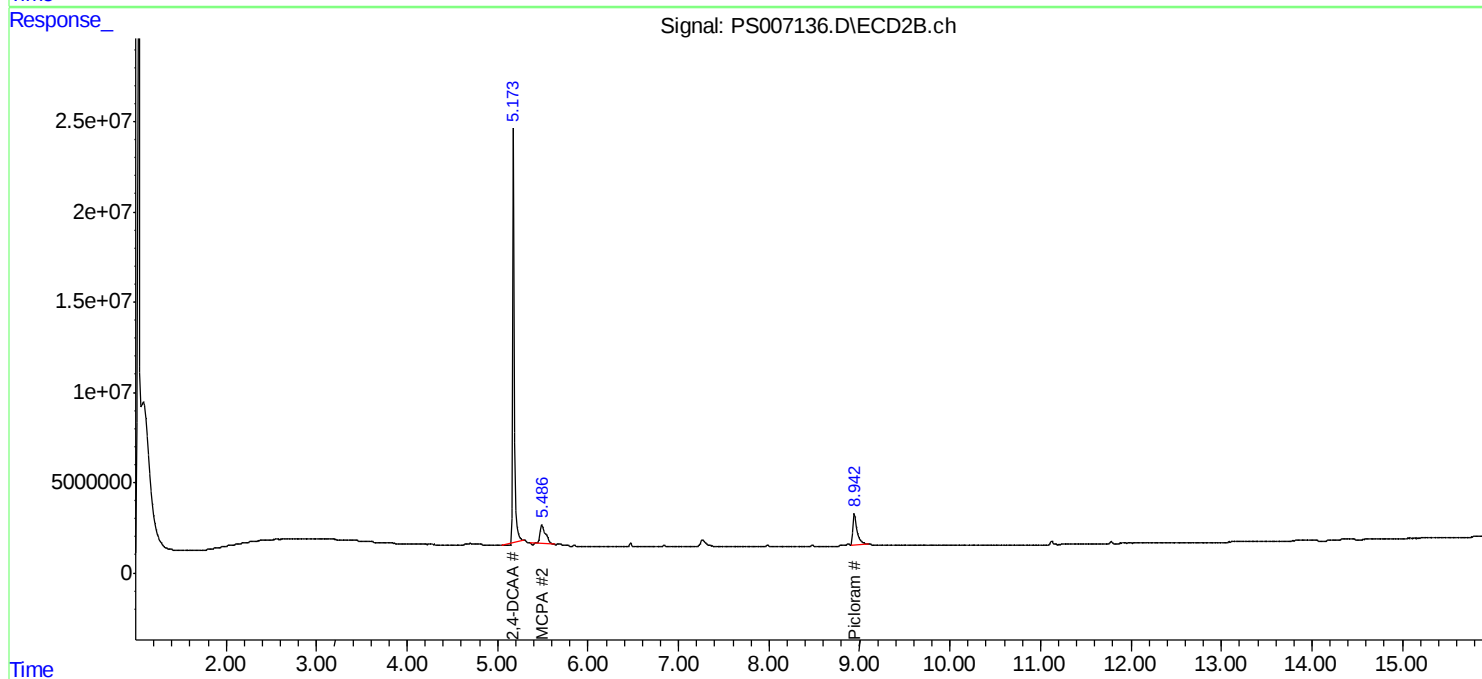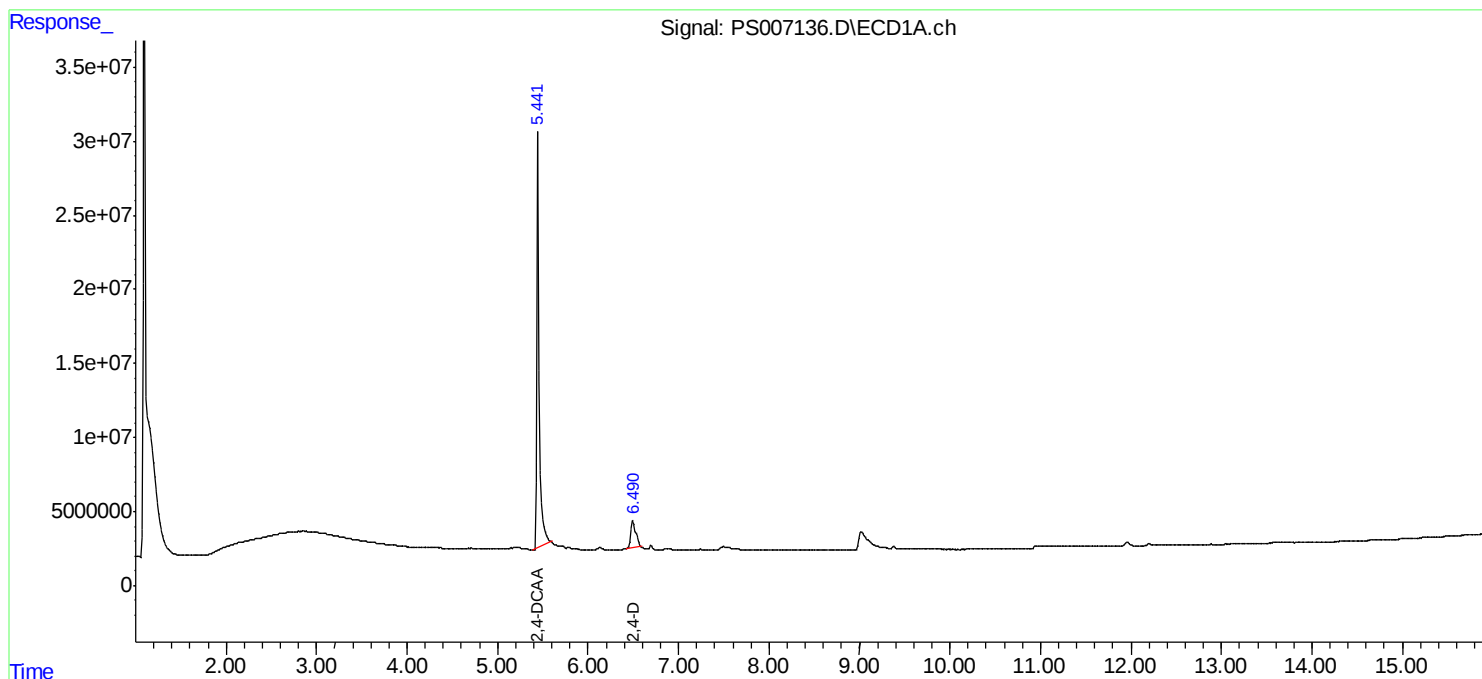


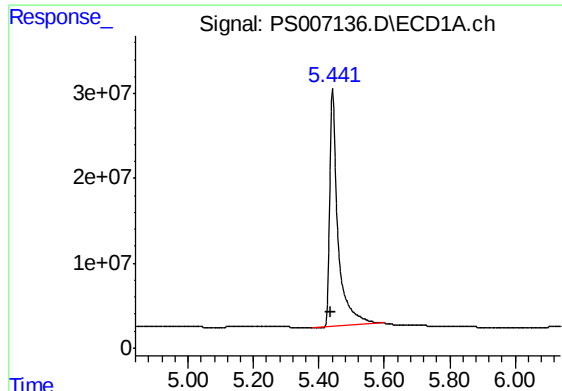

#4 2,4-DCAA


R.T.: 5.442 min
Delta R.T.: 0.006 min
Response: 487399851
Conc: 356.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123819BL

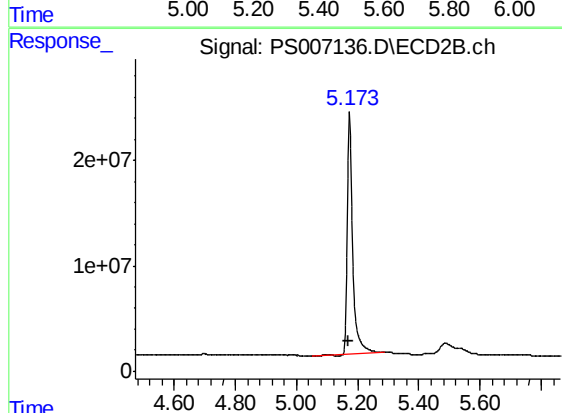


#4 2,4-DCAA

R.T.: 5.173 min
Delta R.T.: 0.005 min
Response: 275673054
Conc: 391.97 ng/ml

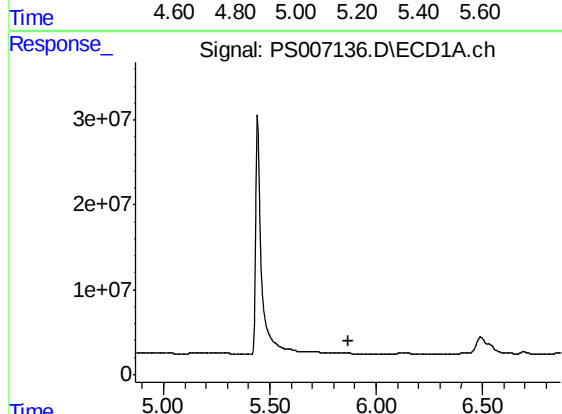


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

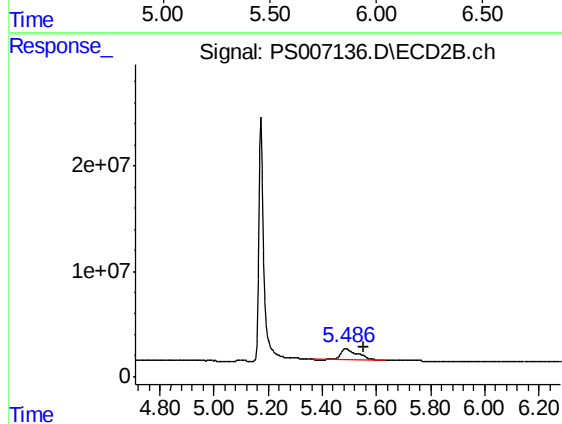

#7 MCPA


R.T.: 5.486 min
Delta R.T.: -0.069 min
Response: 44789136
Conc: 15.41 ug/ml

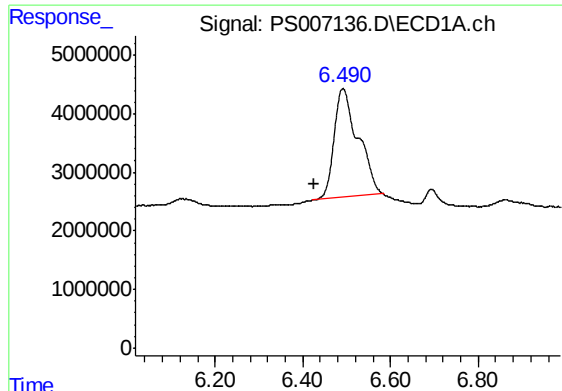

#9 2,4-D


R.T.: 6.491 min
Delta R.T.: 0.067 min
Response: 70395408
Conc: 57.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123819BL

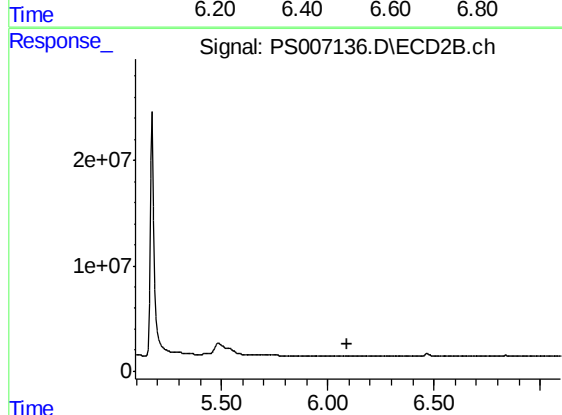


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

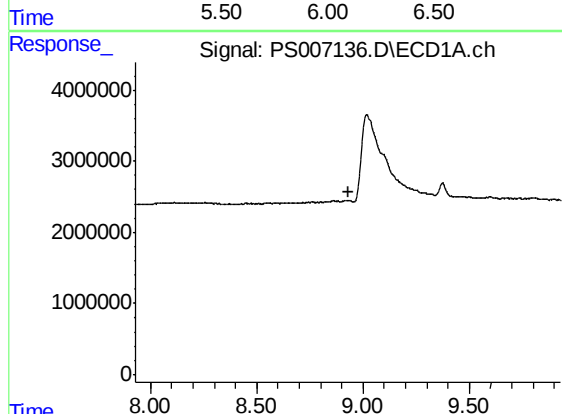

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

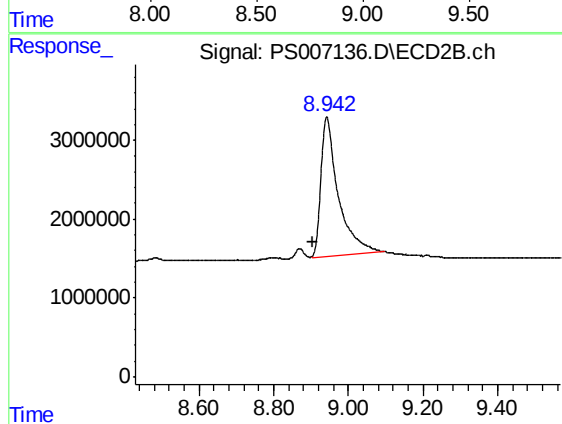

#15 Picloram

R.T.: 8.942 min
Delta R.T.: 0.037 min
Response: 57046068
Conc: 9.29 ng/ml