

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101419\
 Data File : PS007126.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2019 12:36
 Operator : SM\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 14 13:50:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:50:27 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.436	5.169	1012.6E6	520.9E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.011	1.721	1163.3E6	624.1E6	682.500	682.500
2) T	3,5-DICHL...	4.810	4.475	1197.3E6	603.7E6	697.500	697.500
3) T	4-Nitroph...	5.290	4.856	416.5E6	268.9E6	682.500	682.500
5) T	DICAMBA	5.585	5.294	3469.5E6	1844.4E6	705.000	705.000
6) T	MCPD	5.736	5.379	253.5E6	135.2E6	70.500	70.500
7) T	MCPA	5.867	5.555	354.5E6	200.0E6	69.750	69.750
8) T	DICHLORPROP	6.209	5.826	827.5E6	457.7E6	705.000	705.000
9) T	2,4-D	6.424	6.095	884.1E6	560.1E6	705.000	705.000
10) T	Pentachlo...	6.680	6.457	12760.8E6	6861.0E6	712.500	712.500
11) T	2,4,5-TP ...	7.214	6.821	4979.1E6	2715.5E6	712.500	712.500
12) T	2,4,5-T	7.486	7.178	5472.1E6	2537.3E6	712.500	712.500
13) T	2,4-DB	8.014	7.662	694.4E6	341.6E6	712.500	712.500
14) T	DINOSB	9.095	7.971	4110.5E6	1989.2E6	705.000	705.000
15) T	Picloram	8.929	8.905	8070.5E6	4423.6E6	712.500	712.500
16) T	DCPA	9.367	8.863	6463.7E6	3614.8E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101419\
Data File : PS007126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2019 12:36
Operator : SM\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 14 13:50:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:50:27 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

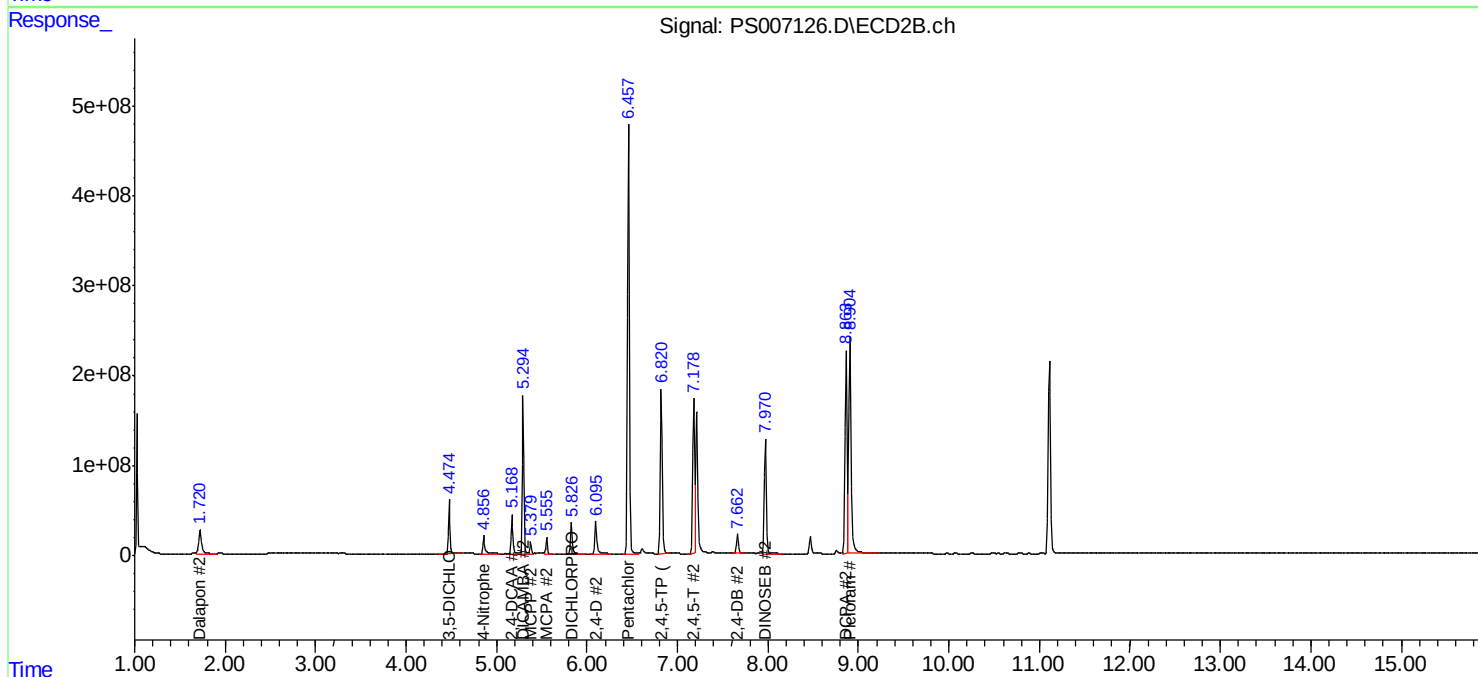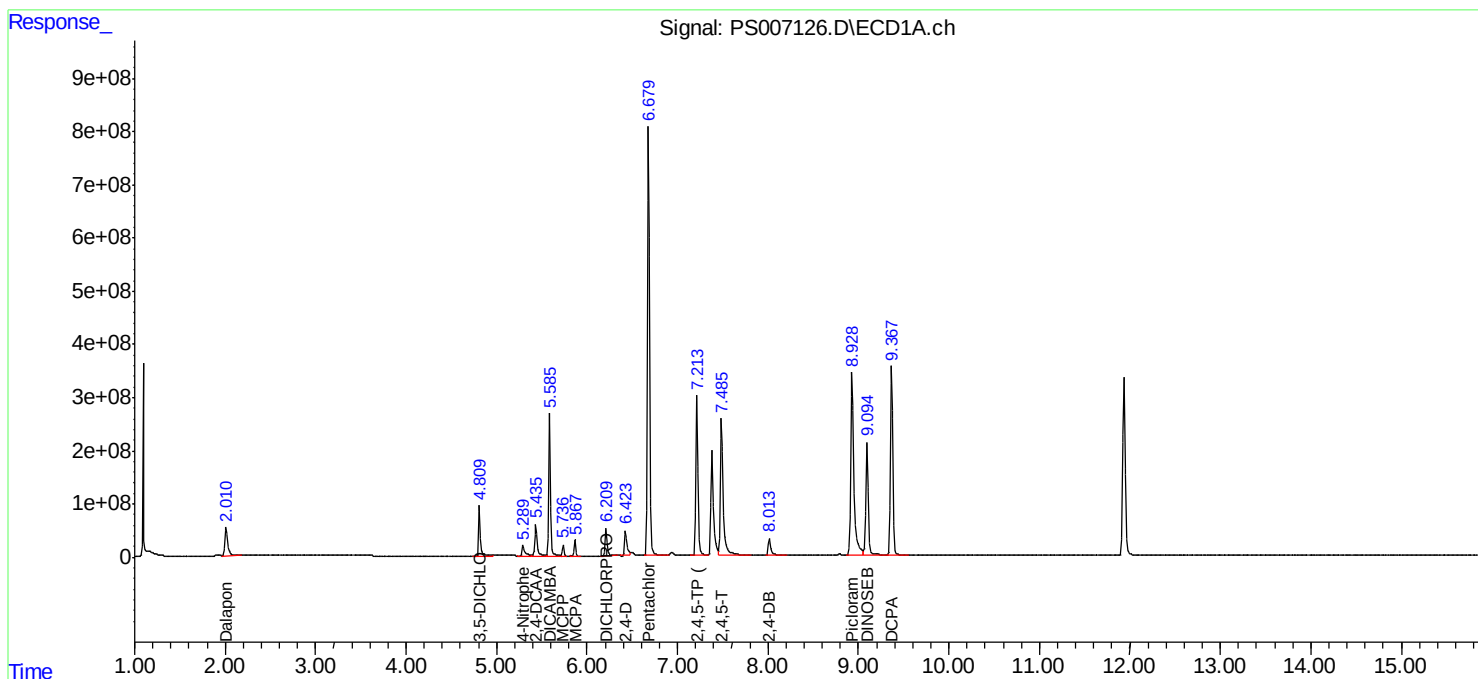


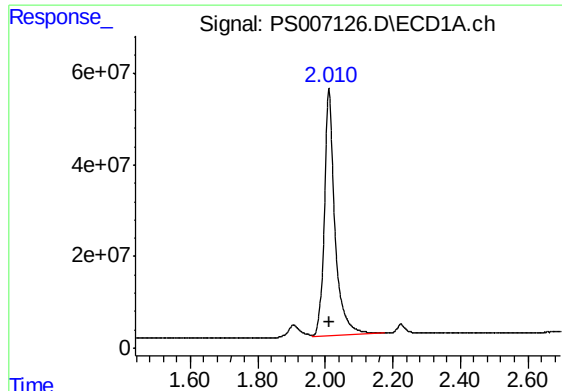

#1 Dalapon


R.T.: 2.011 min
Delta R.T.: 0.000 min
Response: 1163338245
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

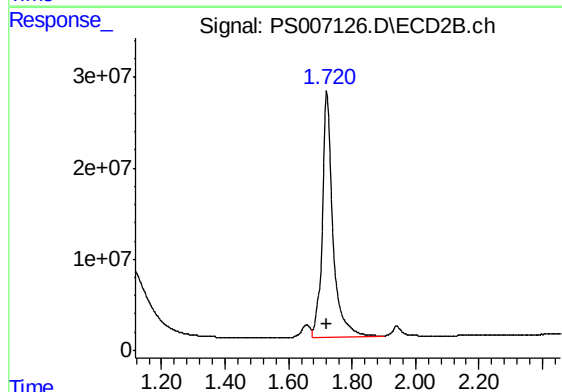


#1 Dalapon

R.T.: 1.721 min
Delta R.T.: 0.000 min
Response: 624059671
Conc: 682.50 ng/ml

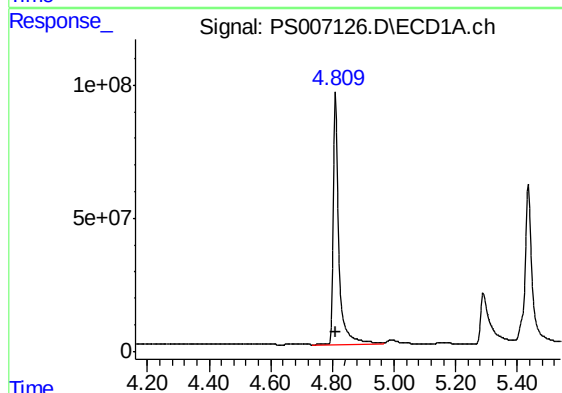


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.810 min
Delta R.T.: 0.000 min
Response: 1197265778
Conc: 697.50 ng/ml

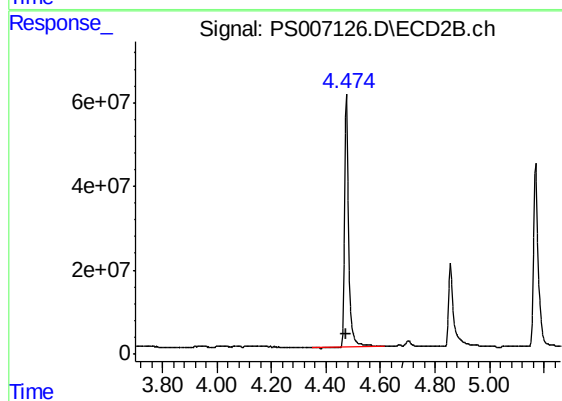

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.475 min
Delta R.T.: 0.000 min
Response: 603722397
Conc: 697.50 ng/ml

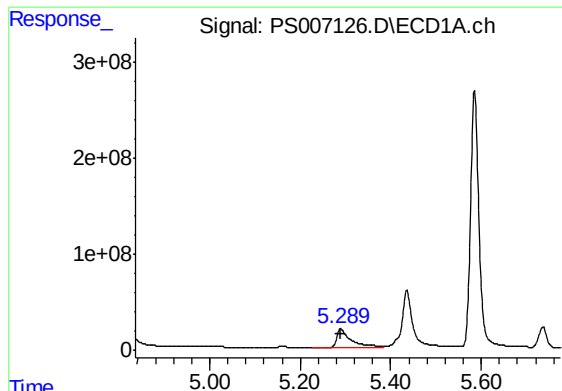

#3 4-Nitrophenol


R.T.: 5.290 min
Delta R.T.: 0.000 min
Response: 416458626
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

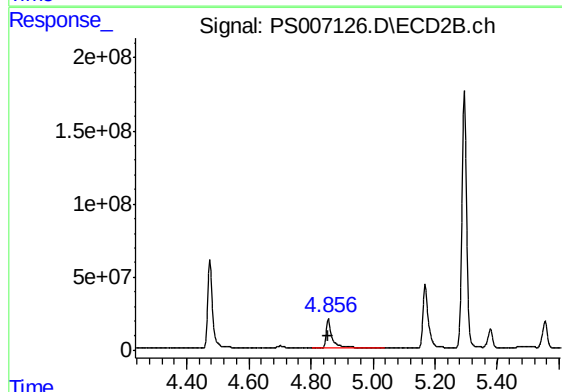


#3 4-Nitrophenol

R.T.: 4.856 min
Delta R.T.: 0.000 min
Response: 268907928
Conc: 682.50 ng/ml

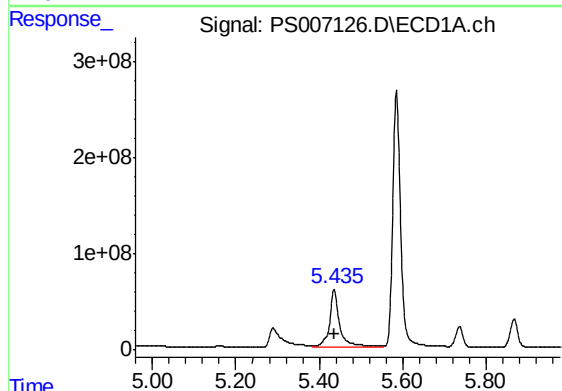


#4 2,4-DCAA

R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 1012643032
Conc: 750.00 ng/ml

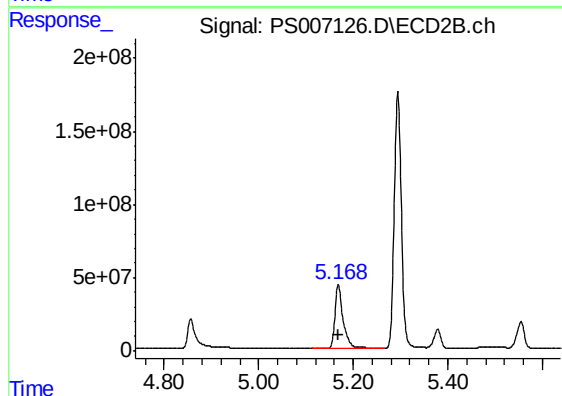

#4 2,4-DCAA


R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 520910917
Conc: 750.00 ng/ml

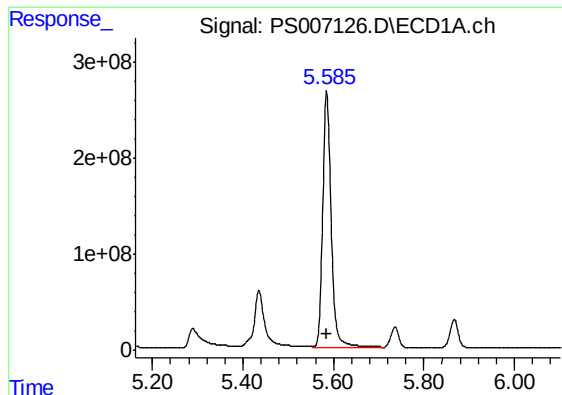

#5 DICAMBA


R.T.: 5.585 min
Delta R.T.: 0.000 min
Response: 3469476518
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

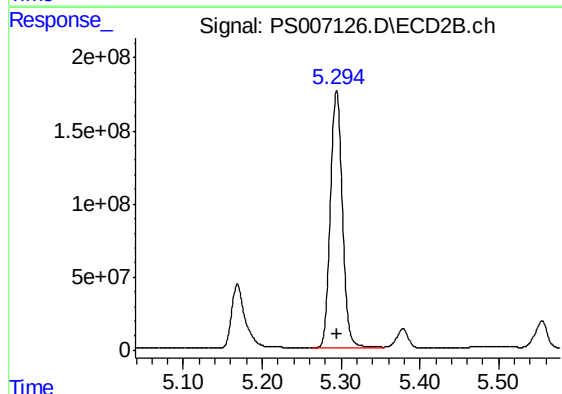


#5 DICAMBA

R.T.: 5.294 min
Delta R.T.: 0.000 min
Response: 1844416701
Conc: 705.00 ng/ml

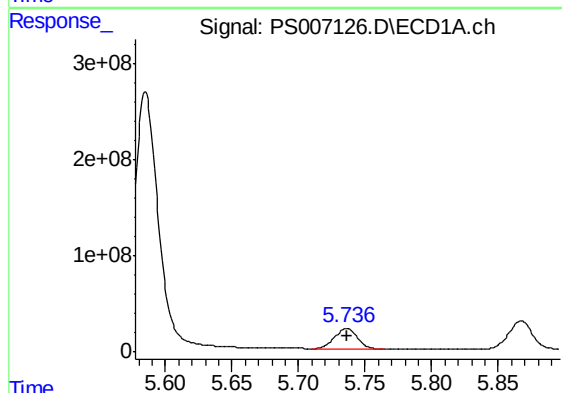


#6 MCPP

R.T.: 5.736 min
Delta R.T.: 0.000 min
Response: 253470335
Conc: 70.50 ug/ml

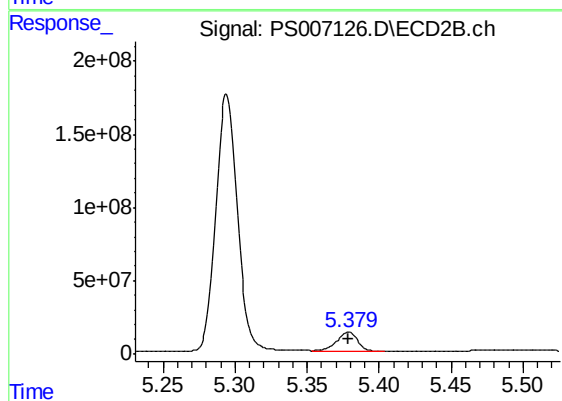

#6 MCPP


R.T.: 5.379 min
Delta R.T.: 0.000 min
Response: 135234793
Conc: 70.50 ug/ml

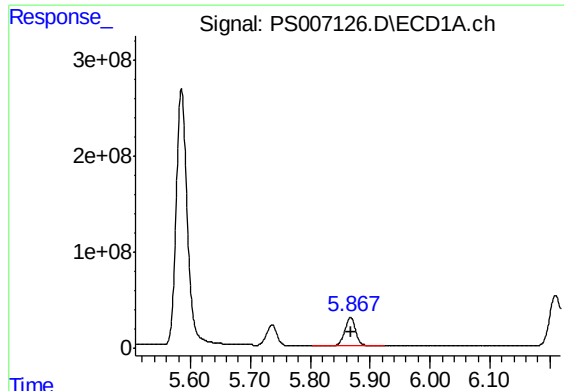

#7 MCPA


R.T.: 5.867 min
Delta R.T.: 0.000 min
Response: 354479020
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

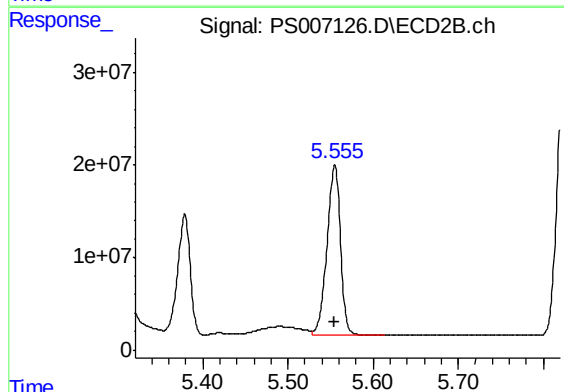


#7 MCPA

R.T.: 5.555 min
Delta R.T.: 0.000 min
Response: 199997204
Conc: 69.75 ug/ml

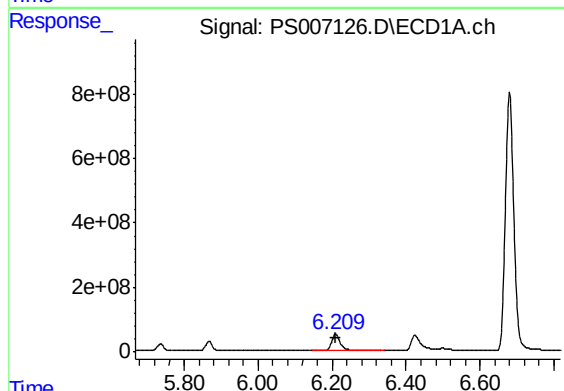


#8 DICHLORPROP

R.T.: 6.209 min
Delta R.T.: 0.000 min
Response: 827498247
Conc: 705.00 ng/ml

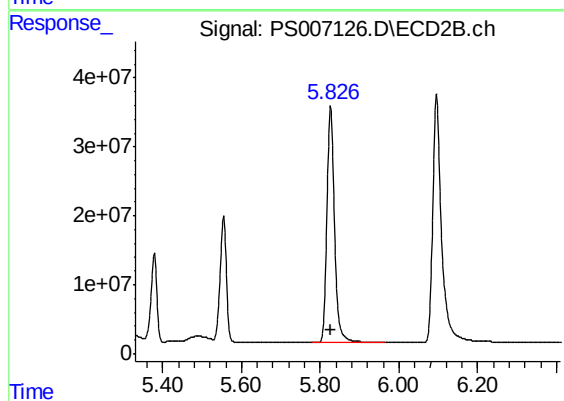

#8 DICHLORPROP


R.T.: 5.826 min
Delta R.T.: 0.000 min
Response: 457677423
Conc: 705.00 ng/ml

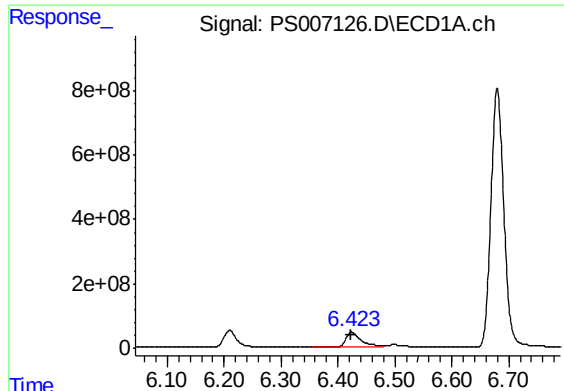

#9 2,4-D


R.T.: 6.424 min
Delta R.T.: 0.000 min
Response: 884071086
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

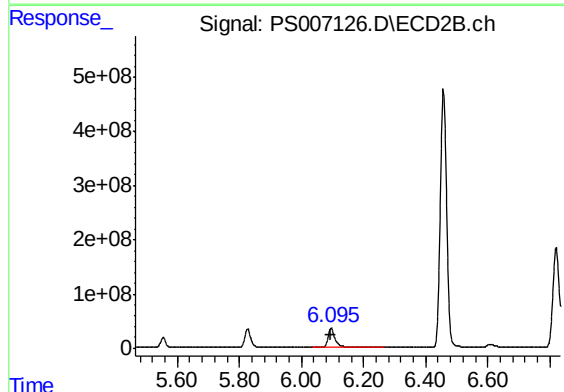


#9 2,4-D

R.T.: 6.095 min
Delta R.T.: 0.000 min
Response: 560118648
Conc: 705.00 ng/ml

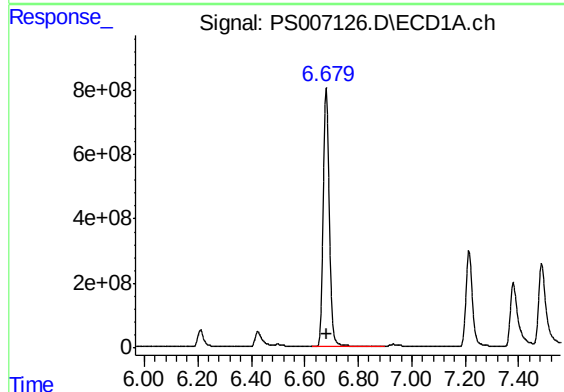


#10 Pentachlorophenol

R.T.: 6.680 min
Delta R.T.: 0.000 min
Response: 12760833223
Conc: 712.50 ng/ml

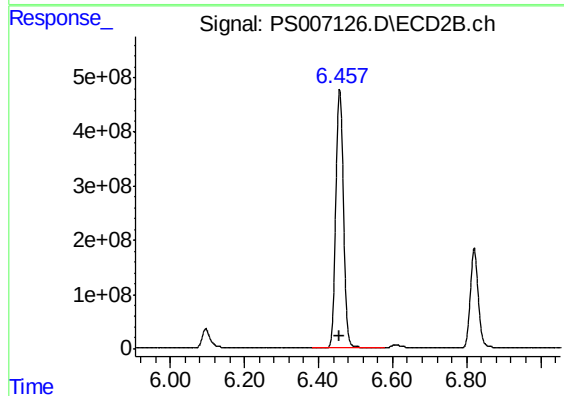

#10 Pentachlorophenol


R.T.: 6.457 min
Delta R.T.: 0.000 min
Response: 6860994964
Conc: 712.50 ng/ml

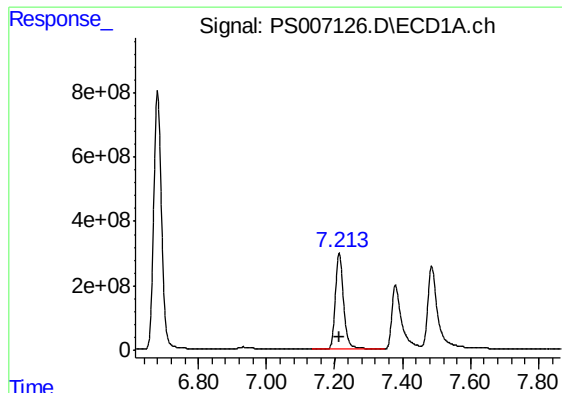

#11 2,4,5-TP (SILVEX)


R.T.: 7.214 min
Delta R.T.: 0.000 min
Response: 4979052440
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

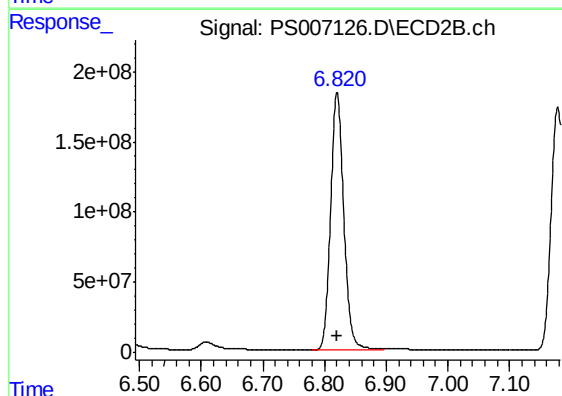


#11 2,4,5-TP (SILVEX)

R.T.: 6.821 min
Delta R.T.: 0.000 min
Response: 2715510377
Conc: 712.50 ng/ml

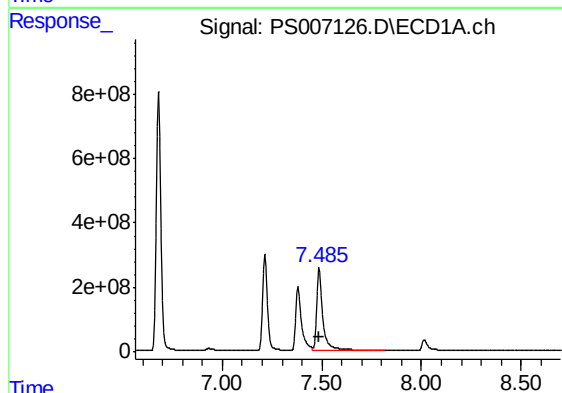


#12 2,4,5-T

R.T.: 7.486 min
Delta R.T.: 0.000 min
Response: 5472127539
Conc: 712.50 ng/ml

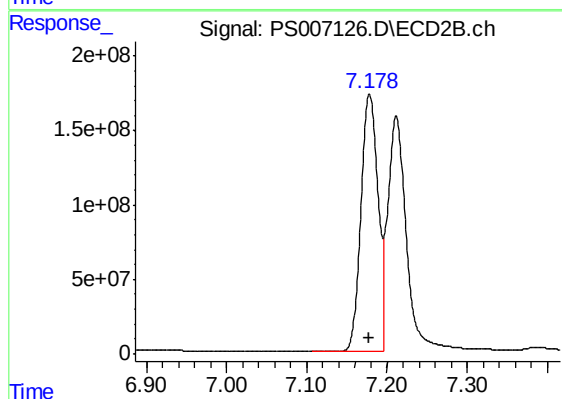

#12 2,4,5-T


R.T.: 7.178 min
Delta R.T.: 0.000 min
Response: 2537345522
Conc: 712.50 ng/ml

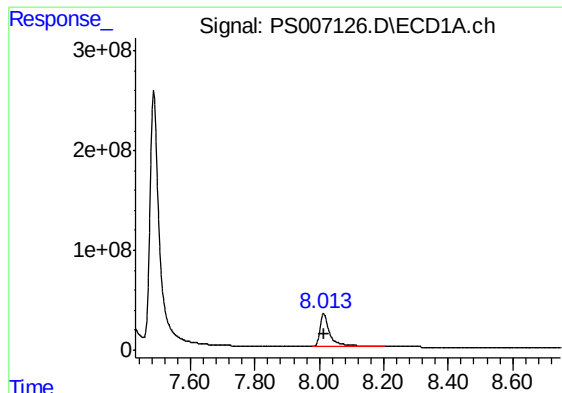

#13 2,4-DB


R.T.: 8.014 min
Delta R.T.: 0.000 min
Response: 694352341
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

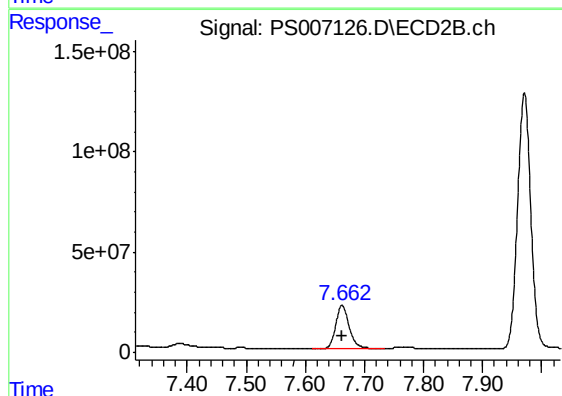


#13 2,4-DB

R.T.: 7.662 min
Delta R.T.: 0.000 min
Response: 341553365
Conc: 712.50 ng/ml

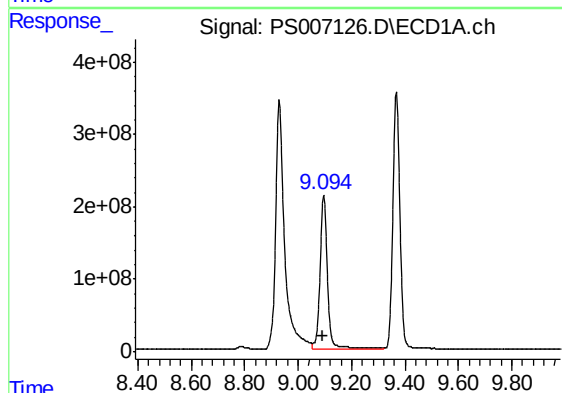


#14 DINOSEB

R.T.: 9.095 min
Delta R.T.: 0.000 min
Response: 4110468757
Conc: 705.00 ng/ml

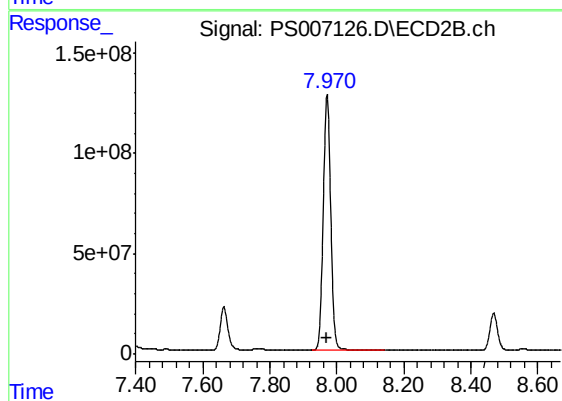

#14 DINOSEB


R.T.: 7.971 min
Delta R.T.: 0.000 min
Response: 1989193027
Conc: 705.00 ng/ml

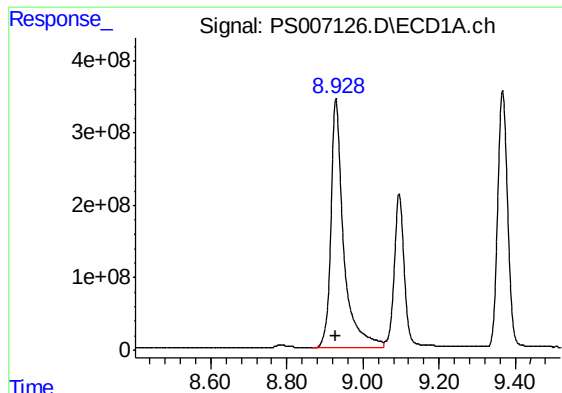

#15 Picloram


R.T.: 8.929 min
Delta R.T.: 0.000 min
Response: 8070460814
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

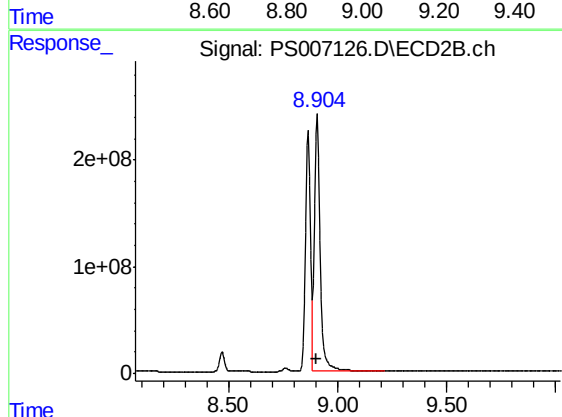


#15 Picloram

R.T.: 8.905 min
Delta R.T.: 0.000 min
Response: 4423600830
Conc: 712.50 ng/ml

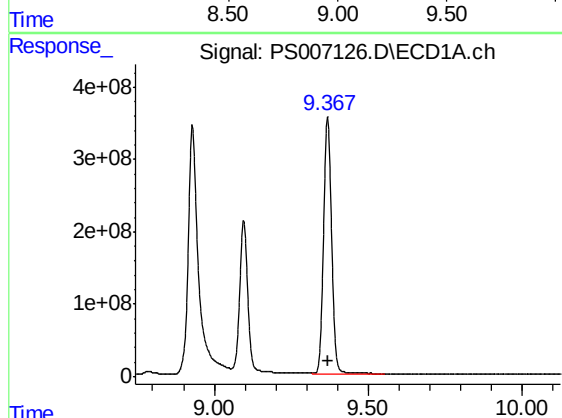

#16 DCPA

R.T.: 9.367 min
Delta R.T.: 0.000 min
Response: 6463708520
Conc: 720.00 ng/ml

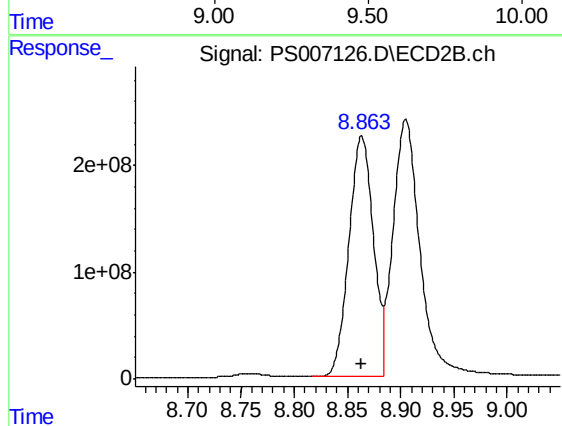

#16 DCPA

R.T.: 8.863 min
Delta R.T.: 0.000 min
Response: 3614844652
Conc: 720.00 ng/ml