

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101422\
 Data File : PS020796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 08:45
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:13:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.485f	0.000	1972092	0	1.045	N.D.	#
Target Compounds								
1) T	Dalapon	2.547	0.000	1120840	0	<MDL	N.D.	#
2) T	3,5-DICHL...	5.755	0.000	19755145	0	6.575	N.D.	#
5) T	DICAMBA	6.552	7.087f	246945	2237484	<MDL	<MDL	#
6) T	MCP	6.747	7.179f	5586051	-638047	<MDL	N.D.	#
7) T	MCPA	6.891	0.000	922514	0	<MDL	N.D.	#
8) T	DICHLORPROP	7.172	7.674	308727	1790432	<MDL	1.234	#
9) T	2,4-D	7.390	0.000	2848985	0	1.169	N.D.	#
10) T	Pentachlo...	7.618	8.354	319115	9213862	<MDL	<MDL	#
11) T	2,4,5-TP ...	8.138	8.801f	1998828	1557167	<MDL	<MDL	#
12) T	2,4,5-T	8.392	9.168	430816	1046624	<MDL	<MDL	#
13) T	2,4-DB	8.849f	0.000	2851001	0	1.248	N.D.	#
14) T	DINOSEB	9.982	0.000	727855	0	<MDL	N.D.	#
15) T	Picloram	9.772	10.934	32556335	7720579	1.955	<MDL	#
16) T	DCPA	10.215	10.886	10776307	4215317	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101422\
Data File : PS020796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 08:45
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:13:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

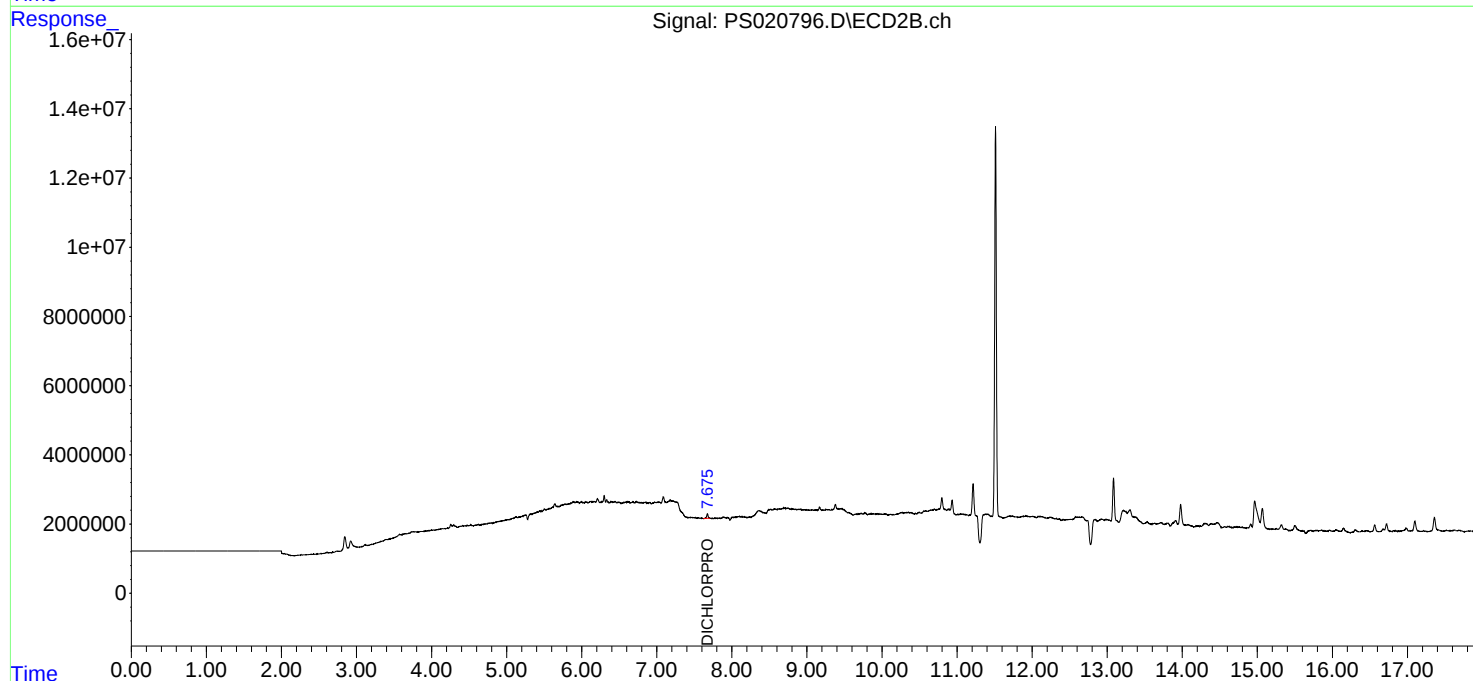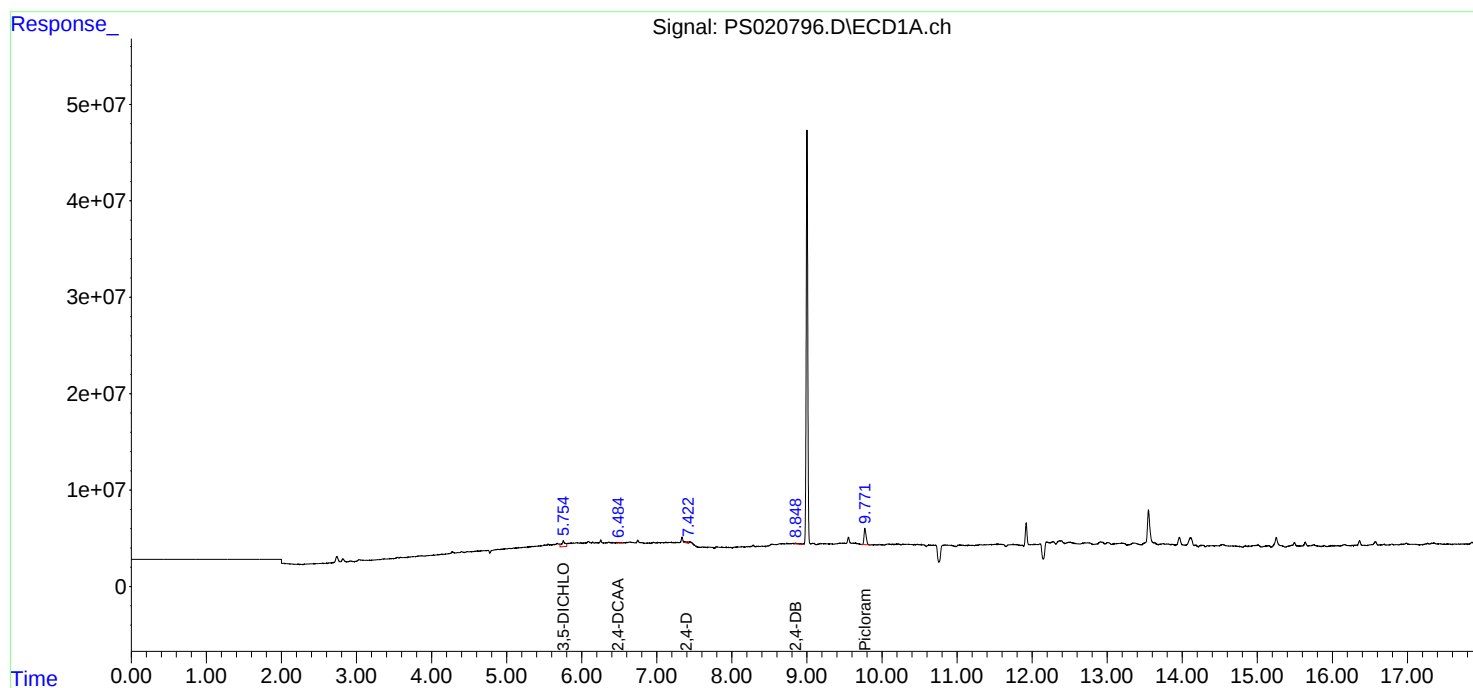


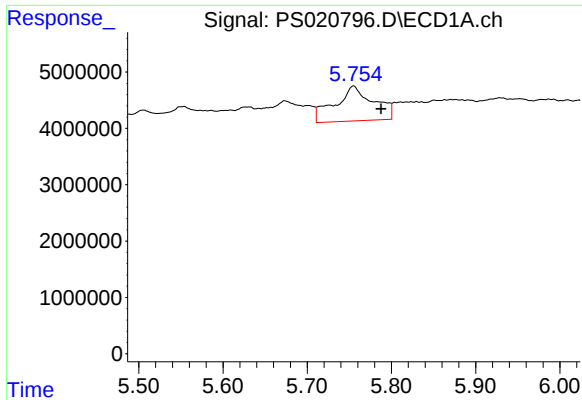

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.755 min
Delta R.T.: -0.033 min
Response: 19755145
Conc: 6.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

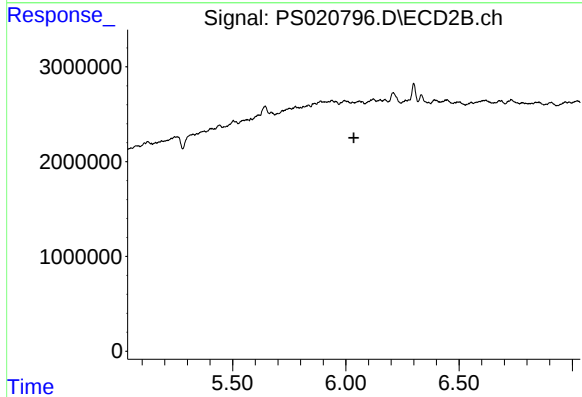


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.035 min
Response: 0
Conc: N.D.

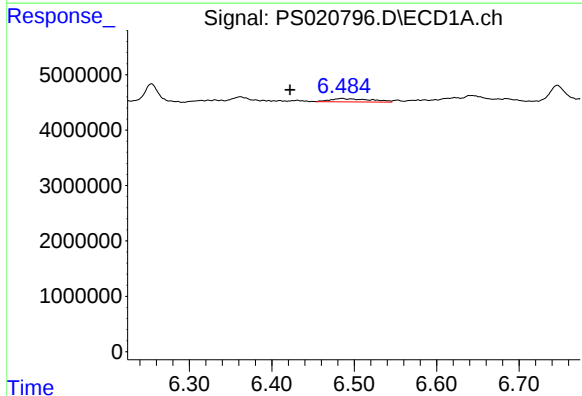


#4 2,4-DCAA

R.T.: 6.485 min
Delta R.T.: 0.063 min
Response: 1972092
Conc: 1.05 ng/ml

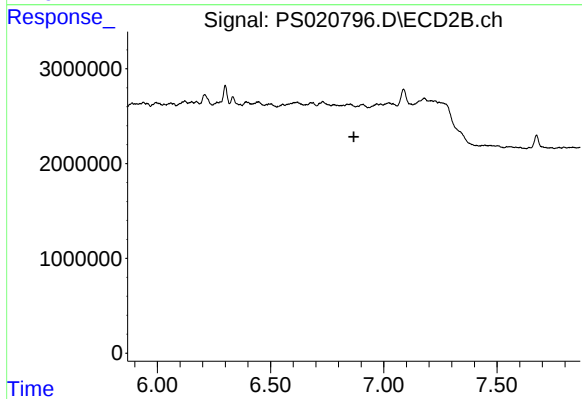

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.868 min
Response: 0
Conc: N.D.

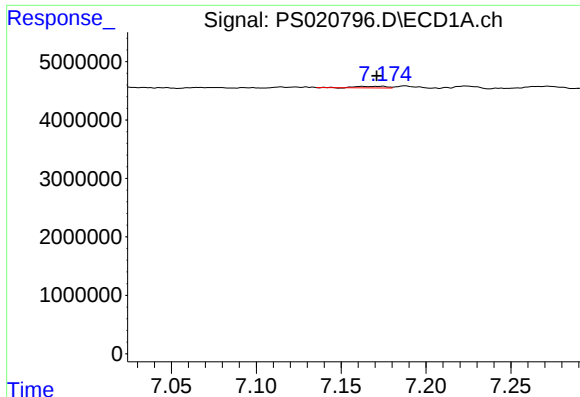

#8 DICHLORPROP


R.T.: 7.172 min
Delta R.T.: 0.001 min
Response: 308727
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

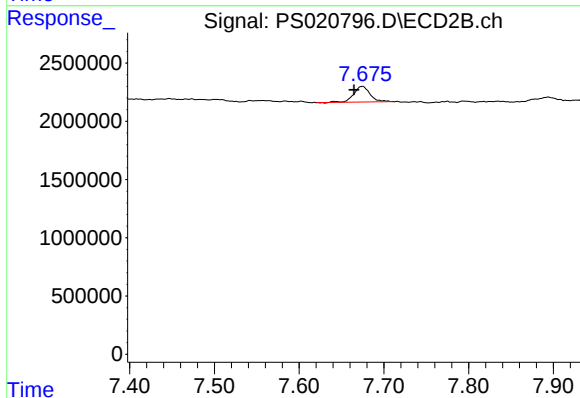


#8 DICHLORPROP

R.T.: 7.674 min
Delta R.T.: 0.009 min
Response: 1790432
Conc: 1.23 ng/ml

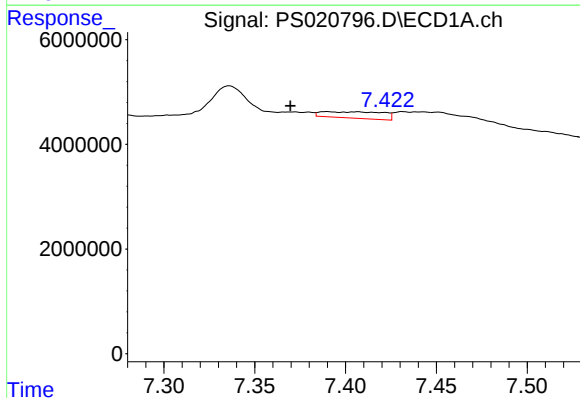


#9 2,4-D

R.T.: 7.390 min
Delta R.T.: 0.021 min
Response: 2848985
Conc: 1.17 ng/ml

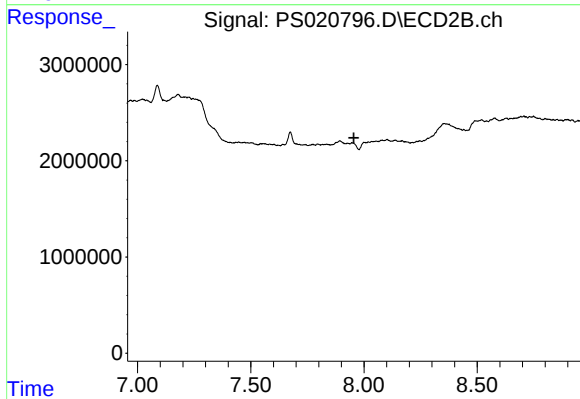

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.956 min
Response: 0
Conc: N.D.

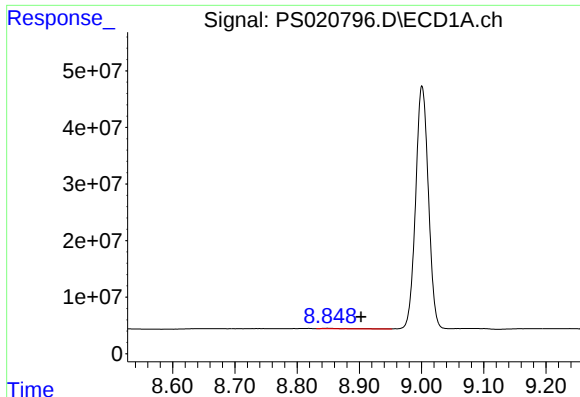

#13 2,4-DB


R.T.: 8.849 min
Delta R.T.: -0.054 min
Response: 2851001
Conc: 1.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

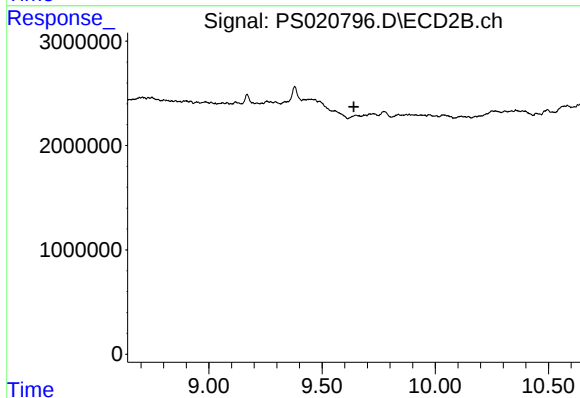


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.641 min
Response: 0
Conc: N.D.

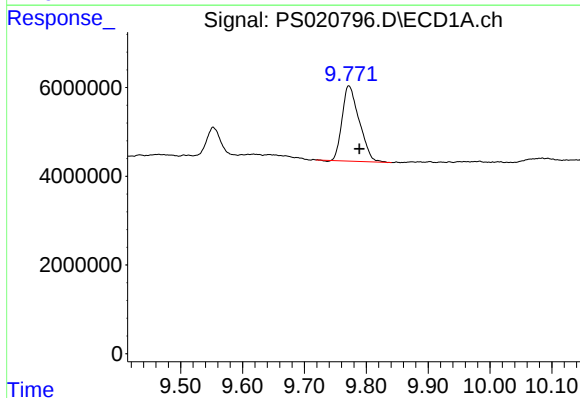

#15 Picloram

R.T.: 9.772 min
Delta R.T.: -0.017 min
Response: 32556335
Conc: 1.95 ng/ml

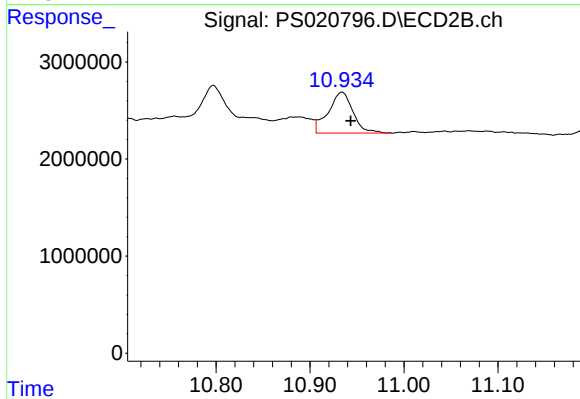

#15 Picloram

R.T.: 10.934 min
Delta R.T.: -0.010 min
Response: 7720579
Conc: N.D.