

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101422\
 Data File : PS020797.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 09:09
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:13:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.419	6.861	937.0E6	668.6E6	496.710	499.325
Target Compounds							
1) T	Dalapon	2.492	0.000	95374	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.771	0.000	2711770	0	<MDL	N.D. #
5) T	DICAMBA	6.616f	0.000	2025943	0	<MDL	N.D. #
6) T	MCP	6.680f	0.000	2056551	0	<MDL	N.D. #
7) T	MCPA	6.787f	0.000	9476872	0	1.113	N.D. #
8) T	DICHLORPROP	7.185	7.676	195524	519189	<MDL	<MDL #
10) T	Pentachlo...	7.648f	0.000	1300361	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.115	0.000	1073533	0	<MDL	N.D. #
12) T	2,4,5-T	8.405	9.166	1309602	1527428	<MDL	<MDL #
13) T	2,4-DB	8.844f	9.573f	3173795	1670230	1.389	1.491
14) T	DINOSEB	9.962	0.000	809241	0	<MDL	N.D. #
15) T	Picloram	9.784	10.933	12293276	8330454	<MDL	<MDL #
16) T	DCPA	10.228	10.933	2019444	8330454	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101422\
Data File : PS020797.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 09:09
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:13:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

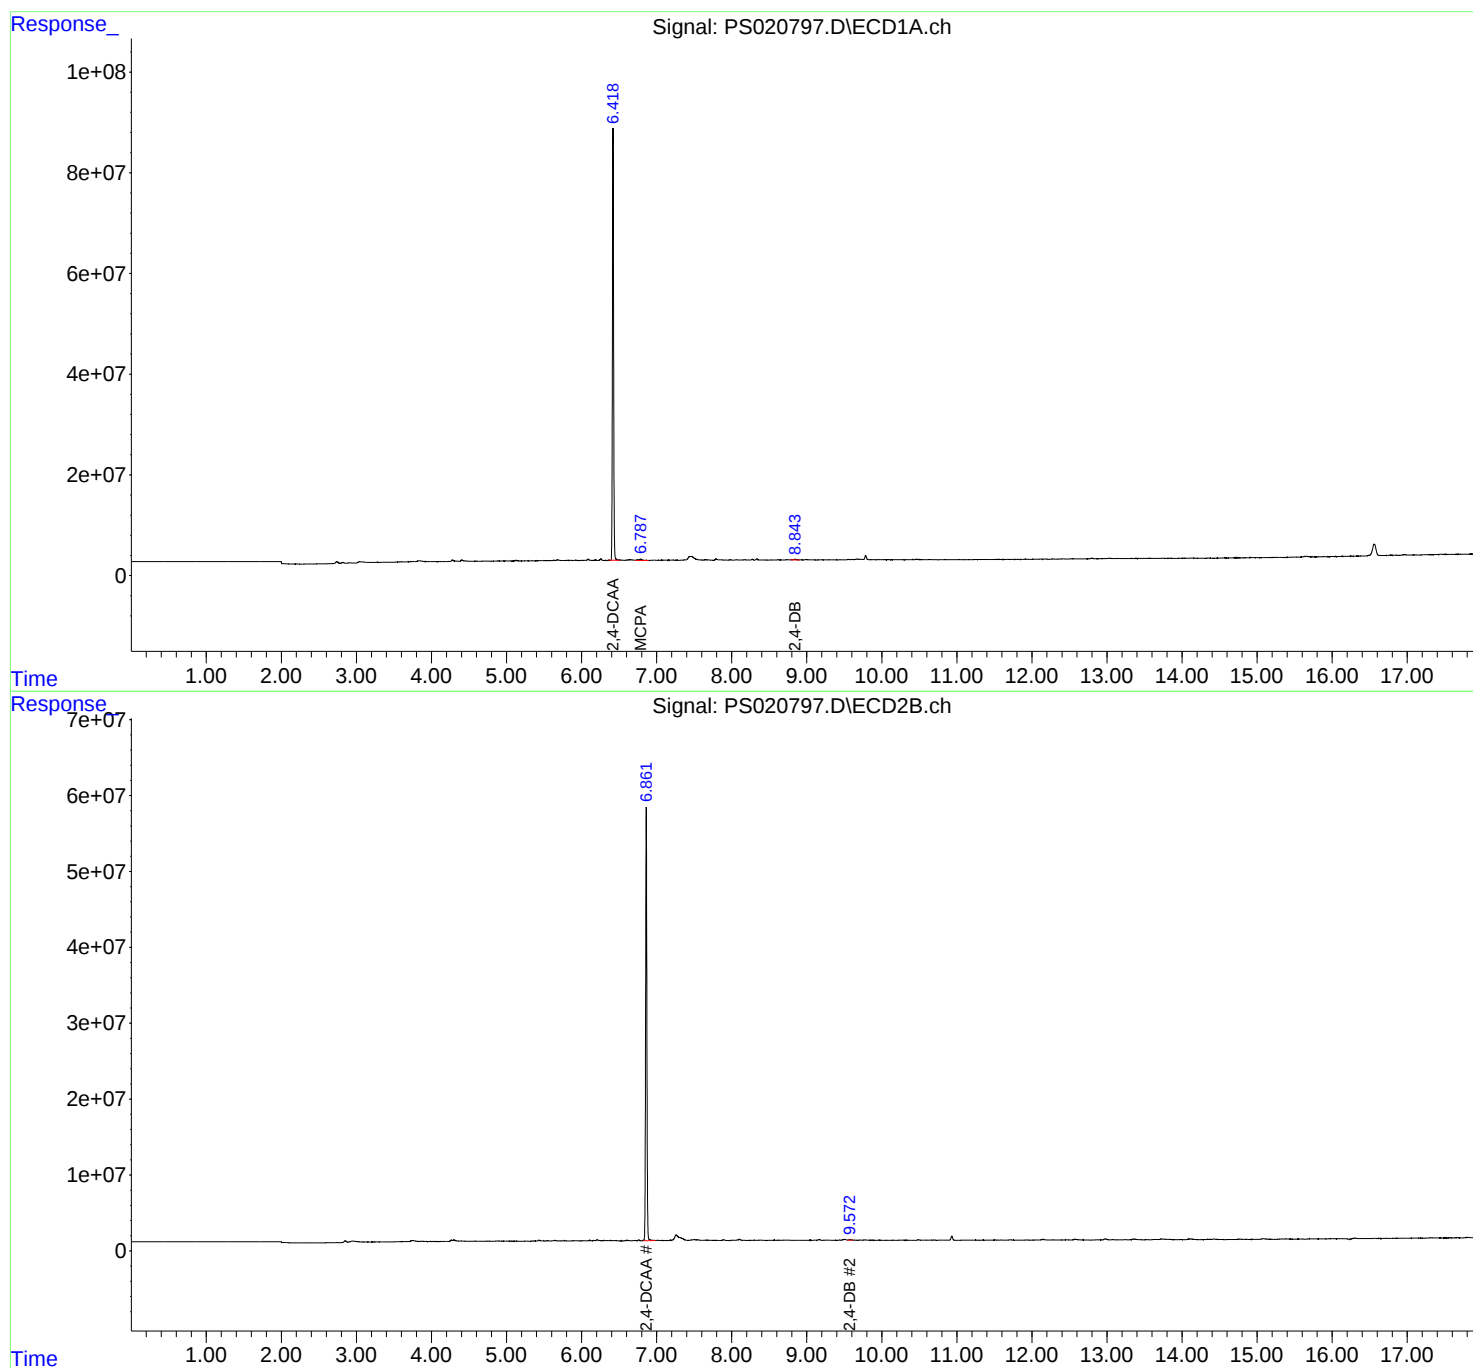


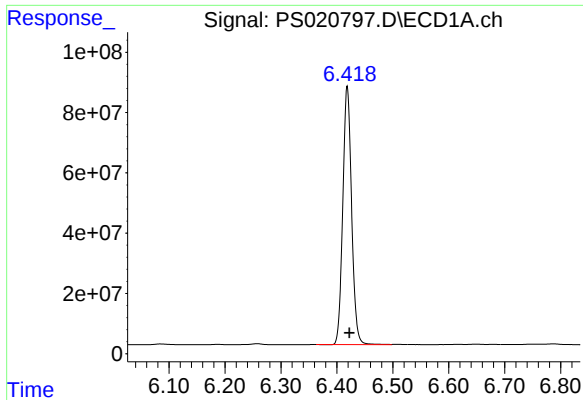

#4 2,4-DCAA


R.T.: 6.419 min
Delta R.T.: -0.004 min
Response: 937018609
Conc: 496.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

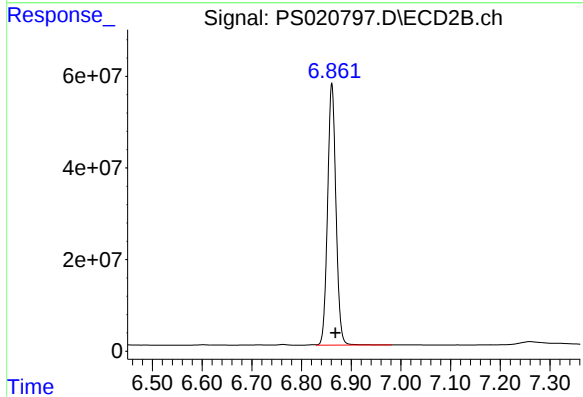


#4 2,4-DCAA

R.T.: 6.861 min
Delta R.T.: -0.007 min
Response: 668586921
Conc: 499.33 ng/ml

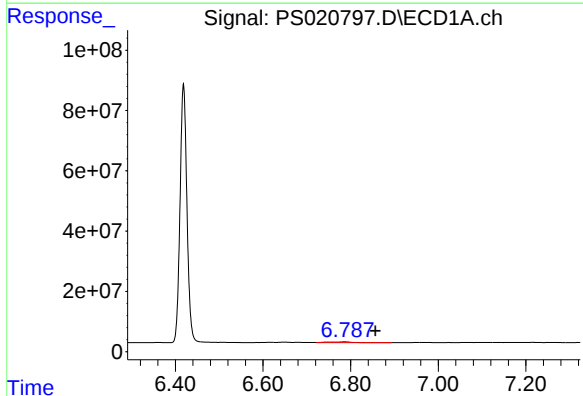


#7 MCPA

R.T.: 6.787 min
Delta R.T.: -0.070 min
Response: 9476872
Conc: 1.11 ug/ml

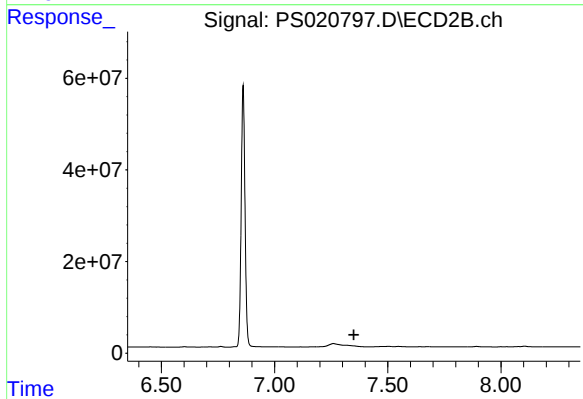

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.351 min
Response: 0
Conc: N.D.

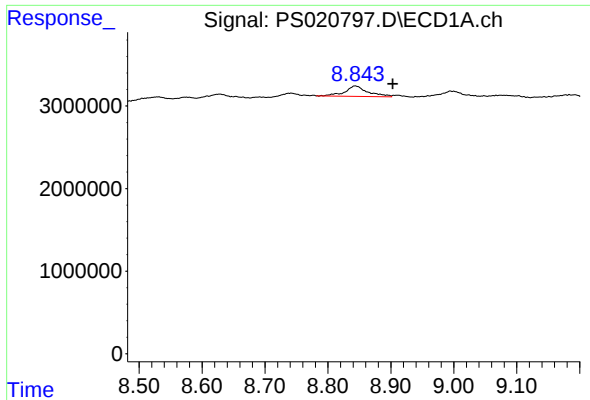

#13 2,4-DB

R.T.: 8.844 min
Delta R.T.: -0.059 min
Response: 3173795
Conc: 1.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

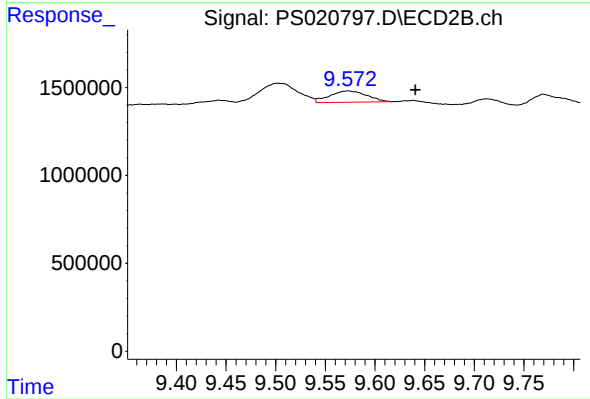

#13 2,4-DB

R.T.: 9.573 min
Delta R.T.: -0.068 min
Response: 1670230
Conc: 1.49 ng/ml