

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101422\
 Data File : PS020804.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2022 18:24
 Operator : AR\AJ
 Sample : N5082-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FLORENCE-COMP-2-FLORENCE-VOC-2

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/17/2022
 Supervised By :Ankita Jodhani 10/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 00:17:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.418	6.862	505.2E6	355.1E6	267.791m	265.174

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101422\
Data File : PS020804.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2022 18:24
Operator : AR\AJ
Sample : N5082-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FLORENCE-COMP-2-FLORENCE-VOC-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/17/2022
Supervised By : Ankita Jodhani 10/17/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 00:17:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

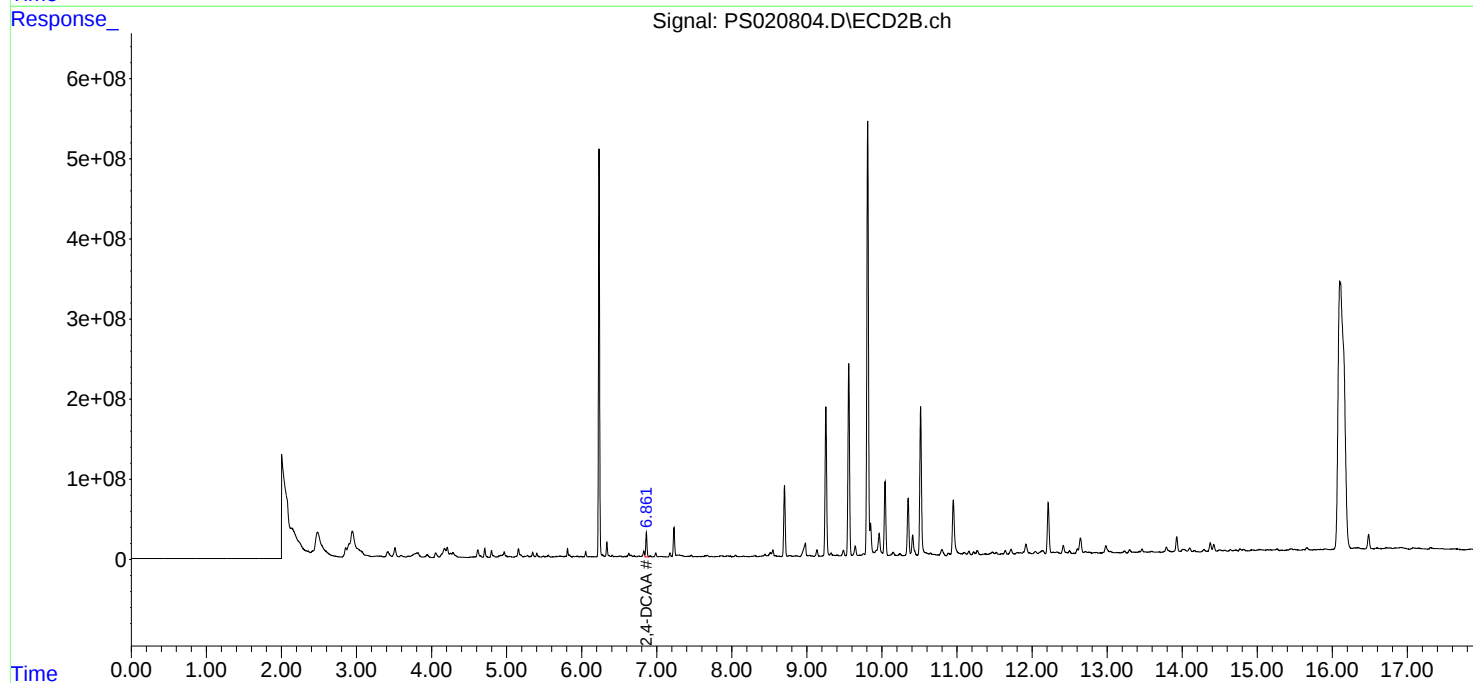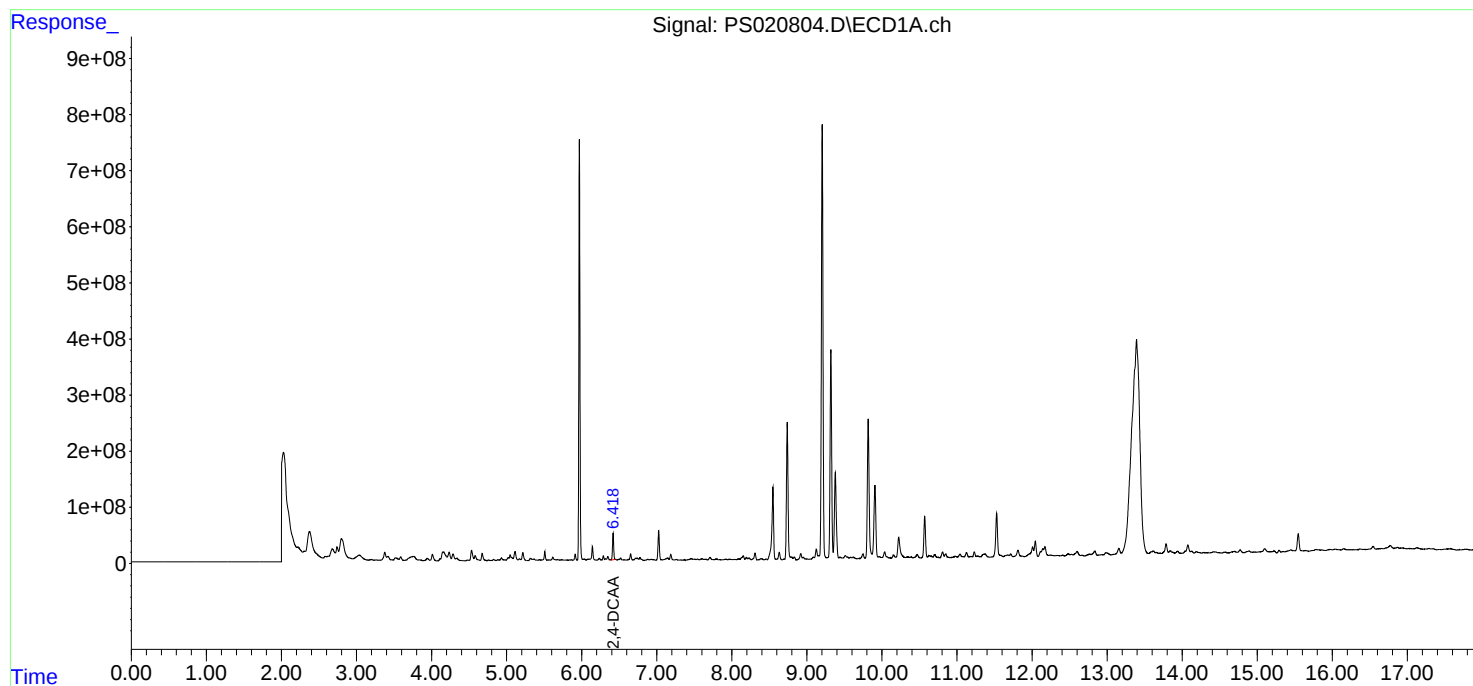

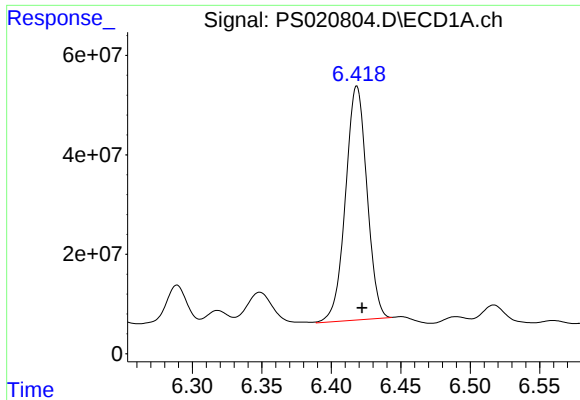


#4 2,4-DCAA

R.T.: 6.418 min
Delta R.T.: -0.004 min
Response: 505174968
Conc: 267.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
FLORENCE-COMP-2-FLORENCE-VOC-2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/17/2022
Supervised By :Ankita Jodhani 10/17/2022

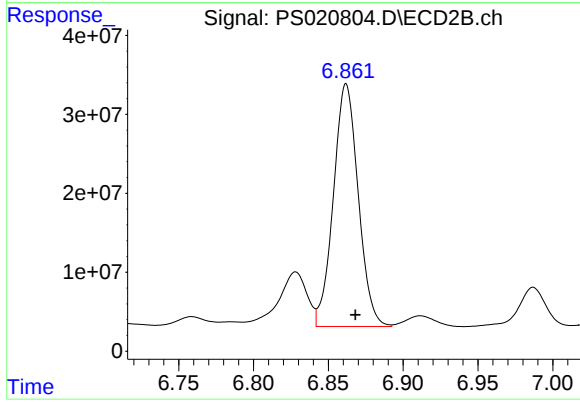

#4 2,4-DCAA

R.T.: 6.862 min
Delta R.T.: -0.006 min
Response: 355062927
Conc: 265.17 ng/ml