

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101424\
 Data File : PS027938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2024 00:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 02:08:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 07 13:46:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.095	7.623	1383.9E6	433.9E6	513.633	436.706
Target Compounds							
1) T	Dalapon	2.526	2.594	25121887	373675	5.598	<MDL #
2) T	3,5-DICHL...	6.296	0.000	1431922	0	<MDL	N.D. #
3) T	4-Nitroph...	6.895	0.000	9613541	0	5.265	N.D. #
5) T	DICAMBA	7.326f	7.812	-1578393	4377631	N.D.	1.259
8) T	DICHLORPROP	0.000	8.563f	0	2367369	N.D.	2.399
10) T	Pentachlo...	8.516f	0.000	986391	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.013f	9.741	10008527	680860	<MDL	<MDL #
12) T	2,4,5-T	0.000	10.168	0	654393	N.D.	<MDL
13) T	2,4-DB	9.843f	0.000	2350116	0	<MDL	N.D. #
14) T	DINOSEB	0.000	11.073	0	229300	N.D.	<MDL
15) T	Picloram	10.869	12.183	12528328	1715024	<MDL	<MDL #
16) T	DCPA	11.356	12.099	2169178	1951276	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101424\
Data File : PS027938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2024 00:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 02:08:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

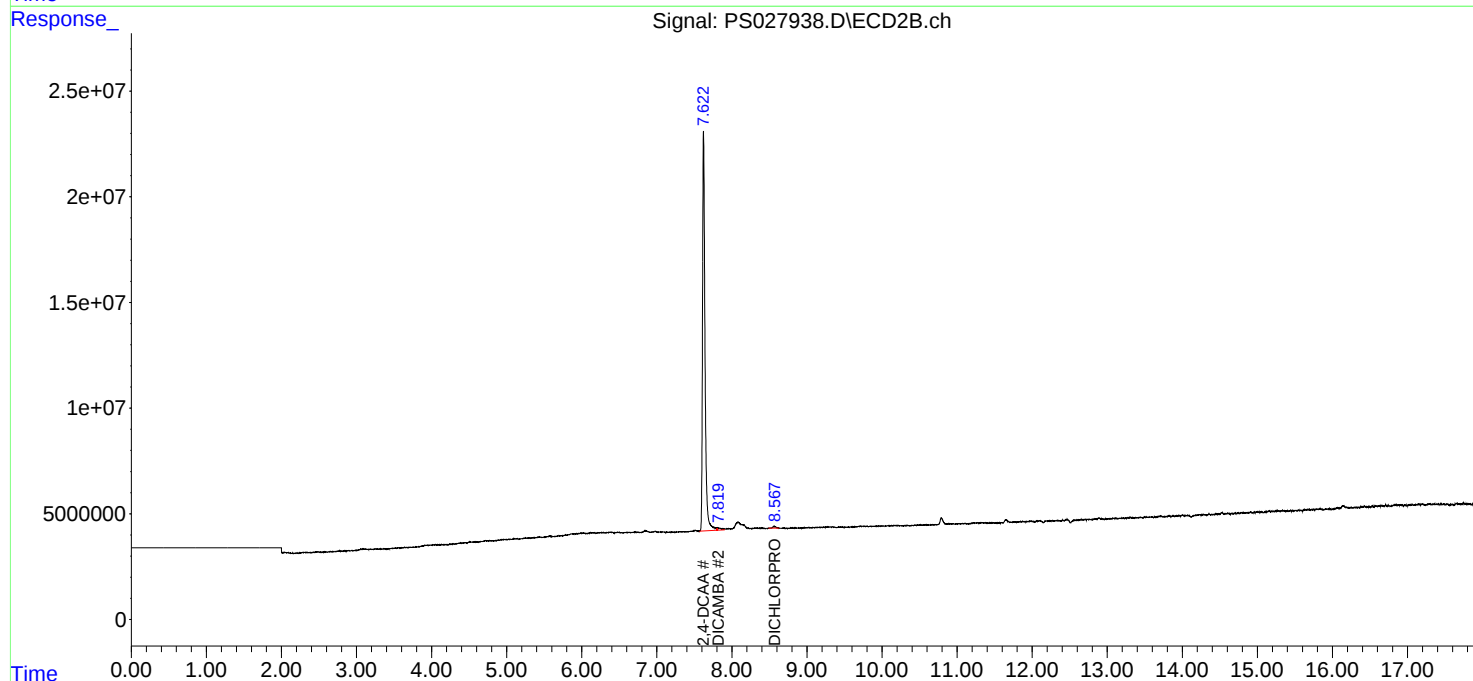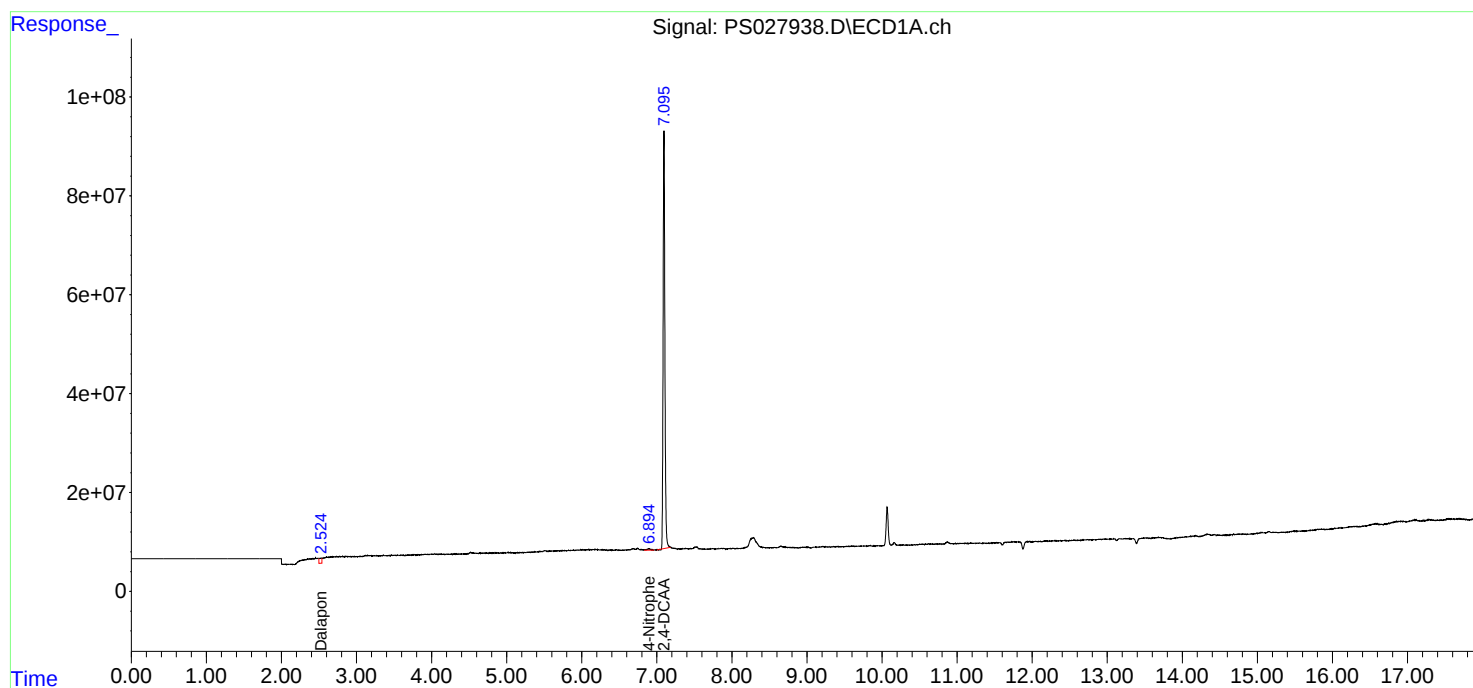


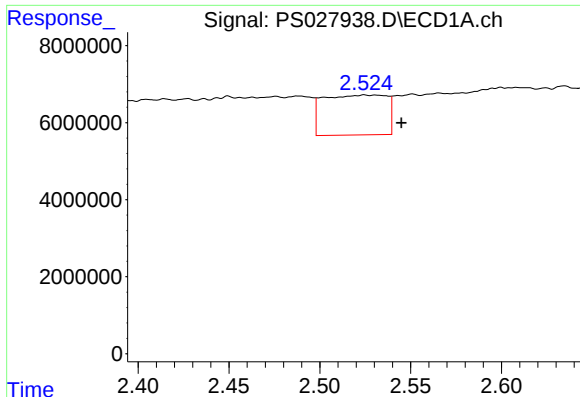

#1 Dalapon


R.T.: 2.526 min
Delta R.T.: -0.019 min
Response: 25121887
Conc: 5.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

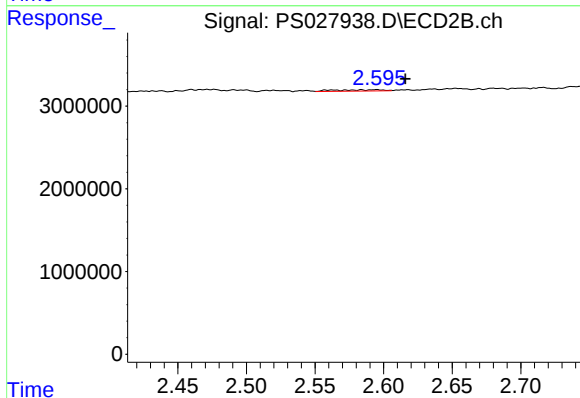


#1 Dalapon

R.T.: 2.594 min
Delta R.T.: -0.022 min
Response: 373675
Conc: N.D.

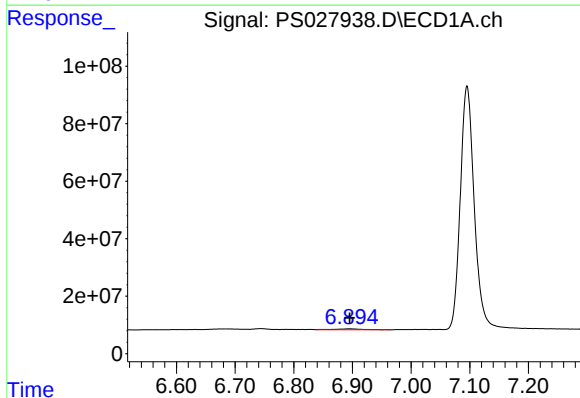


#3 4-Nitrophenol

R.T.: 6.895 min
Delta R.T.: 0.000 min
Response: 9613541
Conc: 5.27 ng/ml

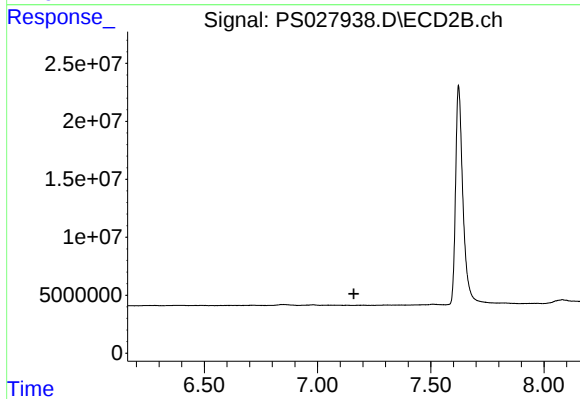

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.160 min
Response: 0
Conc: N.D.

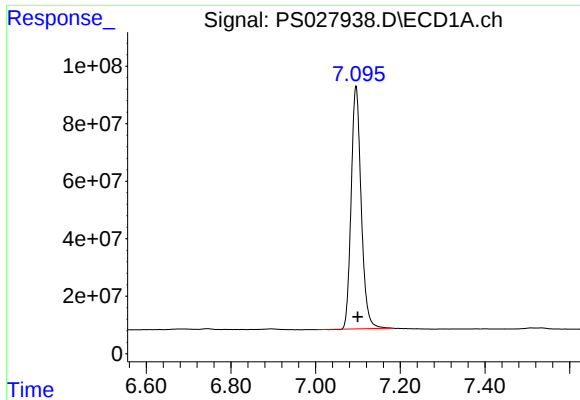

#4 2,4-DCAA


R.T.: 7.095 min
Delta R.T.: -0.005 min
Response: 1383875850
Conc: 513.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

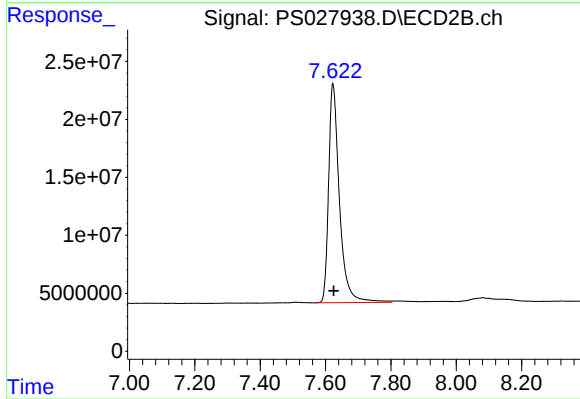


#4 2,4-DCAA

R.T.: 7.623 min
Delta R.T.: -0.002 min
Response: 433948751
Conc: 436.71 ng/ml

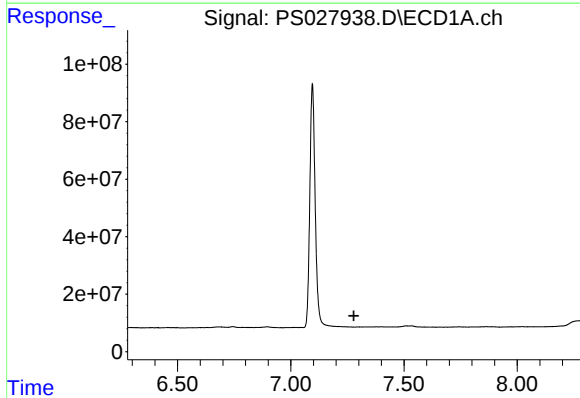


#5 DICAMBA

R.T.: 7.326 min
Delta R.T.: 0.047 min
Response: -1578393
Conc: N.D.

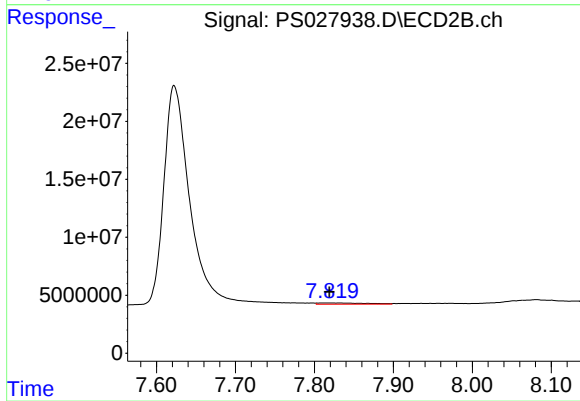

#5 DICAMBA


R.T.: 7.812 min
Delta R.T.: -0.007 min
Response: 4377631
Conc: 1.26 ng/ml

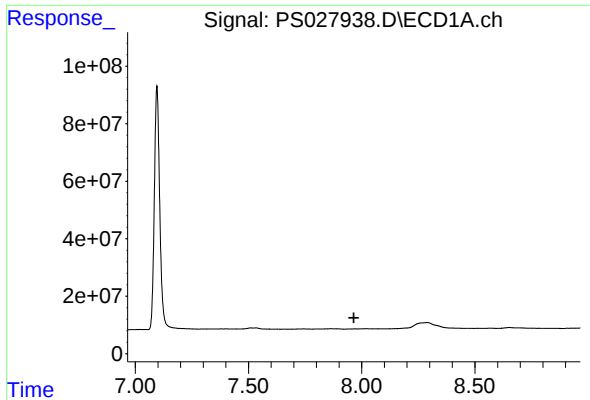

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.965 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

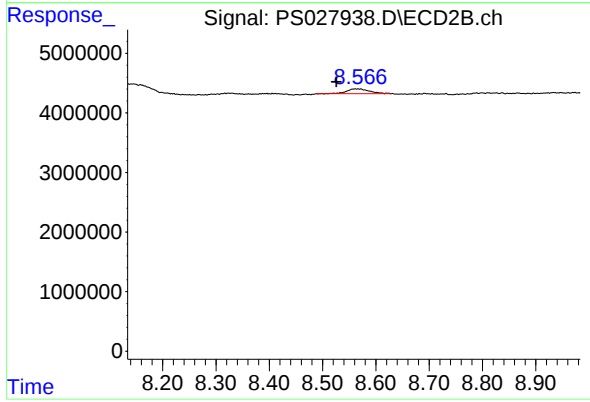

#8 DICHLORPROP

R.T.: 8.563 min
Delta R.T.: 0.037 min
Response: 2367369
Conc: 2.40 ng/ml