Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101424\
Data File : PS027931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2024 21:24
Operator : AR\AJ
Sample : P4395-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
F05308-SOLID

Manual Integrations APPROVED

Reviewed By :Abdul Mirza 10/15/2024
Supervised By :Ankita Jodhani 10/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 02:04:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
4) S	2,4-DCAA	7.095	7.622	796.5E6	241.9E6	295.616m	243.434m
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101424\
Data File : PS027931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2024 21:24
Operator : AR\AJ
Sample : P4395-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
F05308-SOLID

Manual Integrations APPROVED

Reviewed By :Abdul Mirza 10/15/2024
Supervised By :Ankita Jodhani 10/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 02:04:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

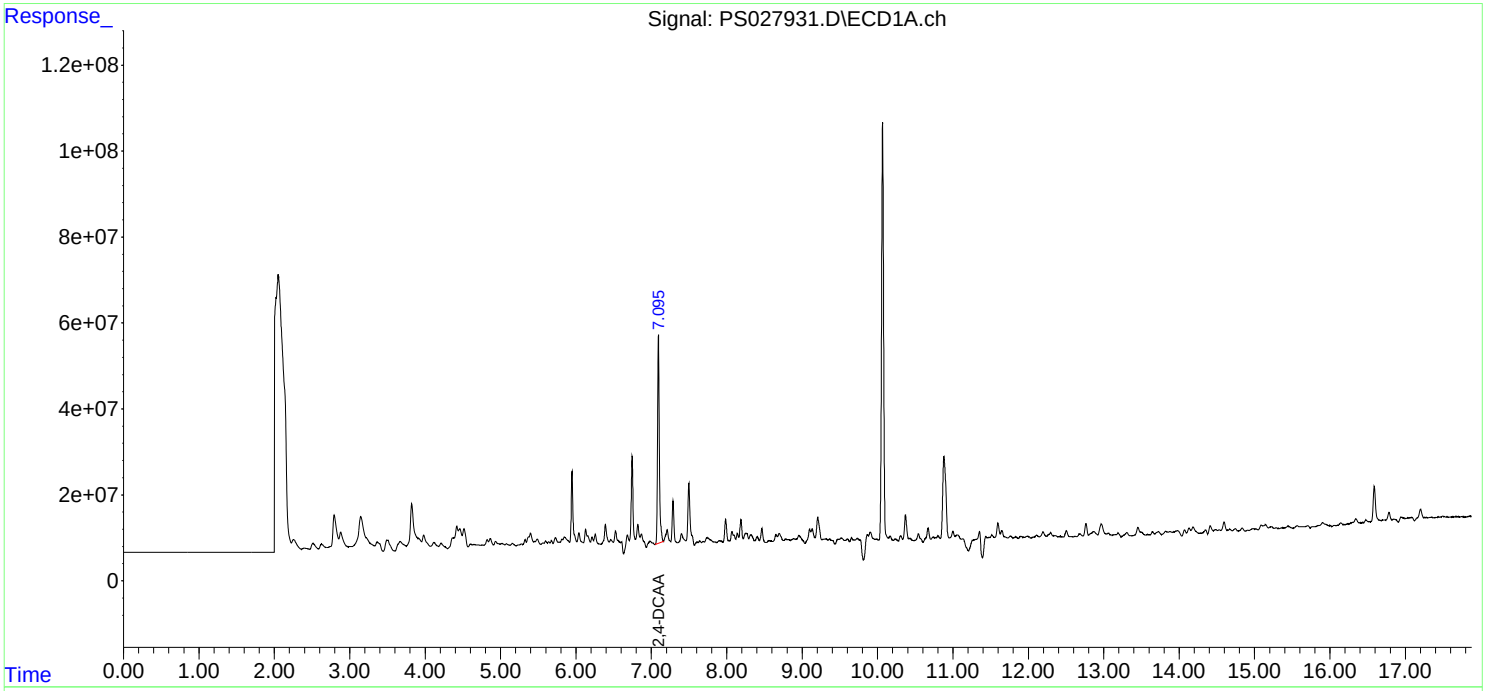

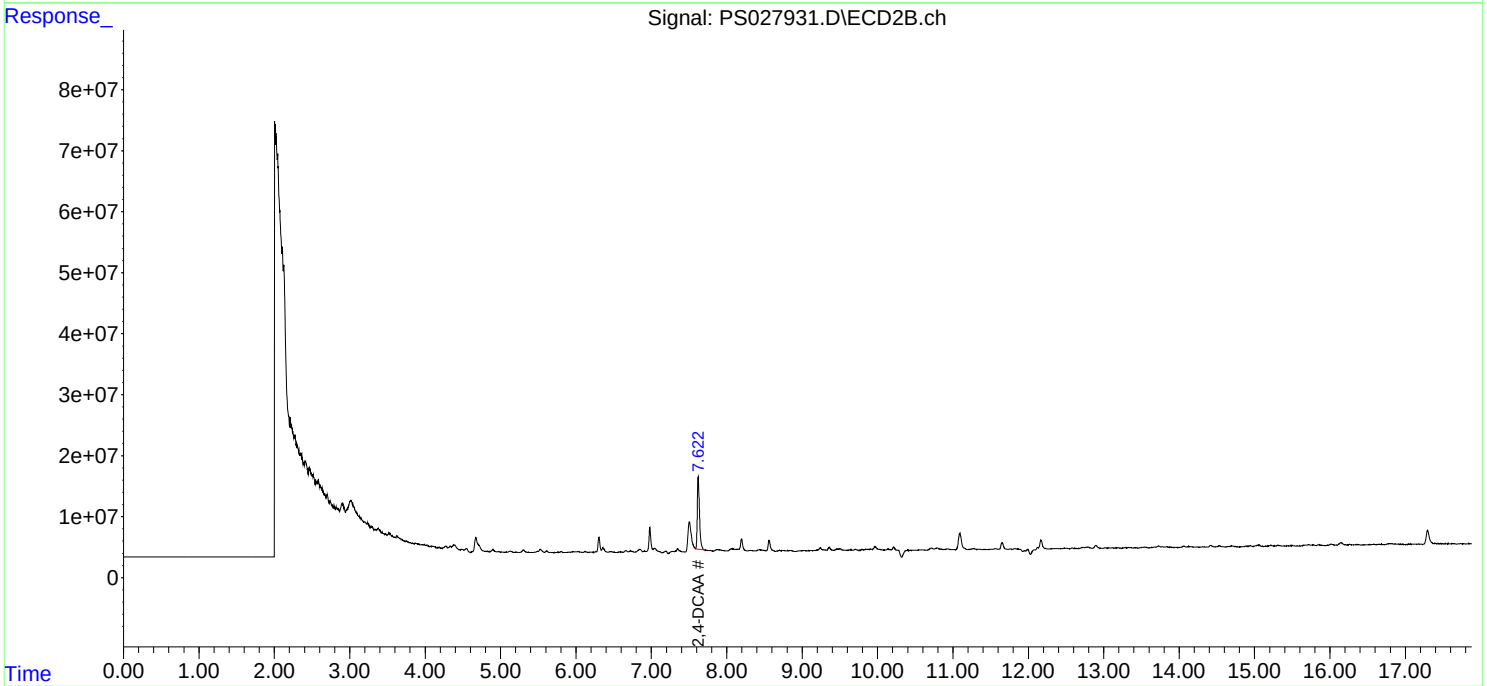

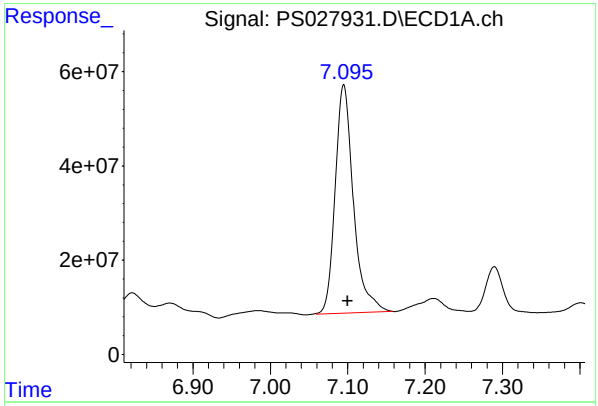

#4 2,4-DCAA

R.T.: 7.095 min
Delta R.T.: -0.005 mi
Response: 796474790
Conc: 295.62 ng/m

Instrument :
ECD_S
ClientSampleId :
F05308-SOLID

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/15/2024
Supervised By :Ankita Jodhani 10/15/2024

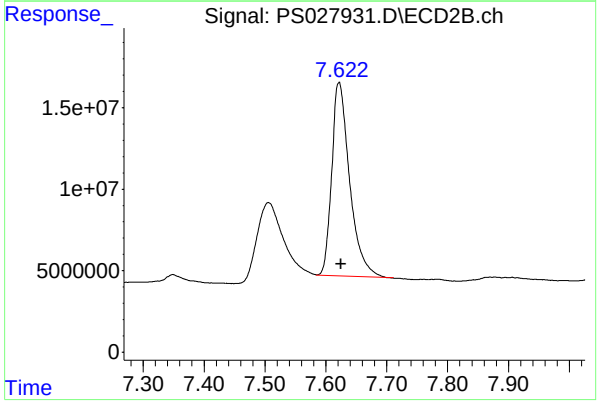

#4 2,4-DCAA

R.T.: 7.622 min
Delta R.T.: -0.003 min
Response: 241897152
Conc: 243.43 ng/ml m