

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS101425\  
 Data File : PS032012.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 Oct 2025 20:44  
 Operator : AR\AJ  
 Sample : Q3337-03  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 15 03:23:36 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS101325.M  
 Quant Title : 8080.M  
 QLast Update : Mon Oct 13 12:51:14 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1    | RT#2    | Resp#1   | Resp#2   | ng/ml   | ng/ml     |
|-----------------------------|--------------|---------|---------|----------|----------|---------|-----------|
| -----                       |              |         |         |          |          |         |           |
| System Monitoring Compounds |              |         |         |          |          |         |           |
| 4) S                        | 2,4-DCAA     | 0.000   | 7.705f  | 0        | 49766250 | N.D.    | 45.228    |
| Target Compounds            |              |         |         |          |          |         |           |
| 1) T                        | Dalapon      | 2.633f  | 2.688   | 2325.1E6 | 2754.4E6 | 300.879 | 732.894 # |
| 3) T                        | 4-Nitroph... | 7.134f  | 0.000   | 10938183 | 0        | 8.195   | N.D. #    |
| 6) T                        | MCP          | 7.665   | 0.000   | 10626481 | 0        | <MDL    | N.D. #    |
| 7) T                        | MCPA         | 0.000   | 8.246f  | 0        | 118.1E6  | N.D.    | 31.297    |
| 8) T                        | DICHLORPROP  | 8.205f  | 8.660   | 10591592 | 18956265 | 2.228   | 9.680 #   |
| 9) T                        | 2,4-D        | 0.000   | 9.042f  | 0        | 18837042 | N.D.    | 9.064     |
| 10) T                       | Pentachlo... | 8.694   | 9.503   | 5380322  | 75688634 | <MDL    | 1.460 #   |
| 11) T                       | 2,4,5-TP ... | 9.328f  | 9.884   | 101.9E6  | 148.2E6  | 3.610   | 7.384 #   |
| 12) T                       | 2,4,5-T      | 9.606f  | 0.000   | 88072376 | 0        | 3.489   | N.D. #    |
| 13) T                       | 2,4-DB       | 10.119f | 10.927f | 37006801 | -2056400 | 11.936  | N.D. #    |
| 14) T                       | DINOSEB      | 11.321  | 11.288  | 20776760 | 9846395  | <MDL    | <MDL #    |
| 15) T                       | Picloram     | 11.164  | 12.413f | 8760289  | 8069527  | <MDL    | <MDL #    |
| 16) T                       | DCPA         | 11.622  | 0.000   | 13279553 | 0        | <MDL    | N.D. #    |
| -----                       |              |         |         |          |          |         |           |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS101425\  
Data File : PS032012.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 Oct 2025 20:44  
Operator : AR\AJ  
Sample : Q3337-03  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 15 03:23:36 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS101325.M  
Quant Title : 8080.M  
QLast Update : Mon Oct 13 12:51:14 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

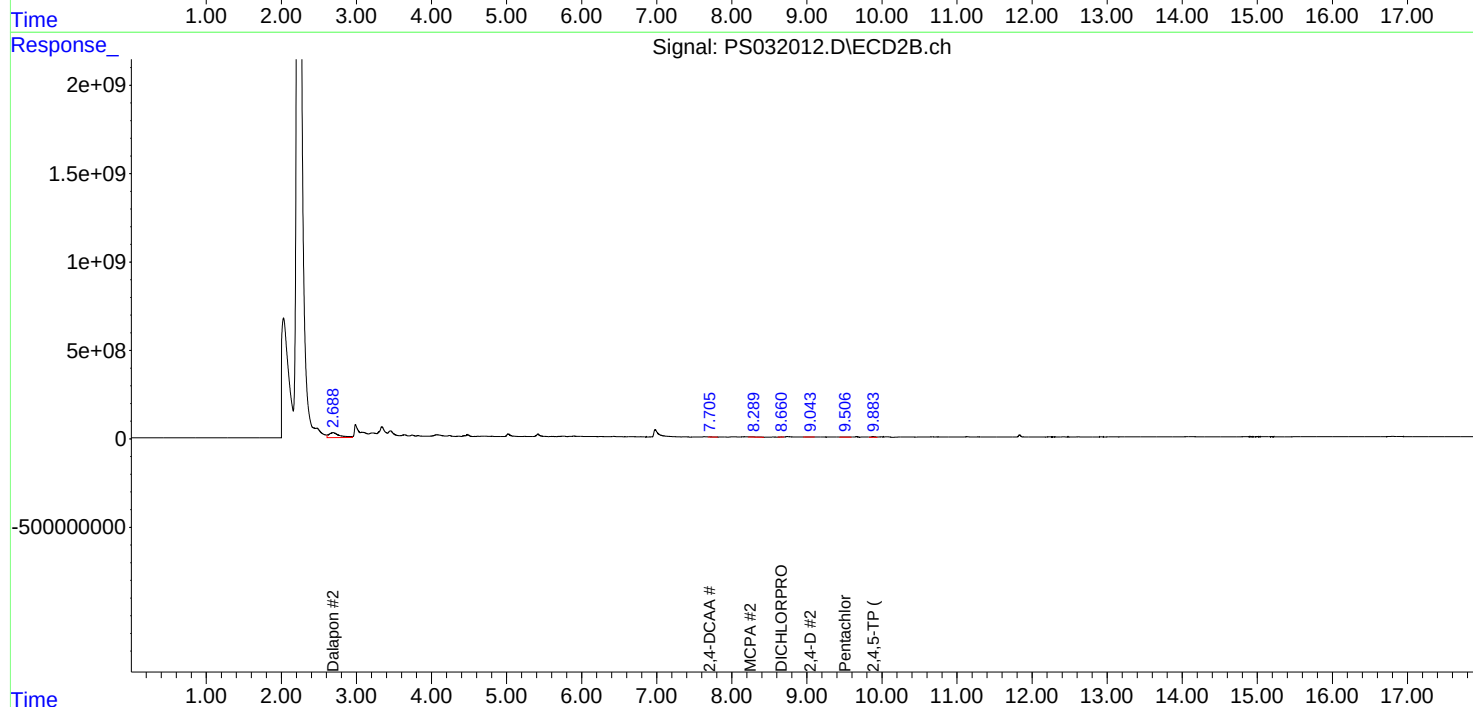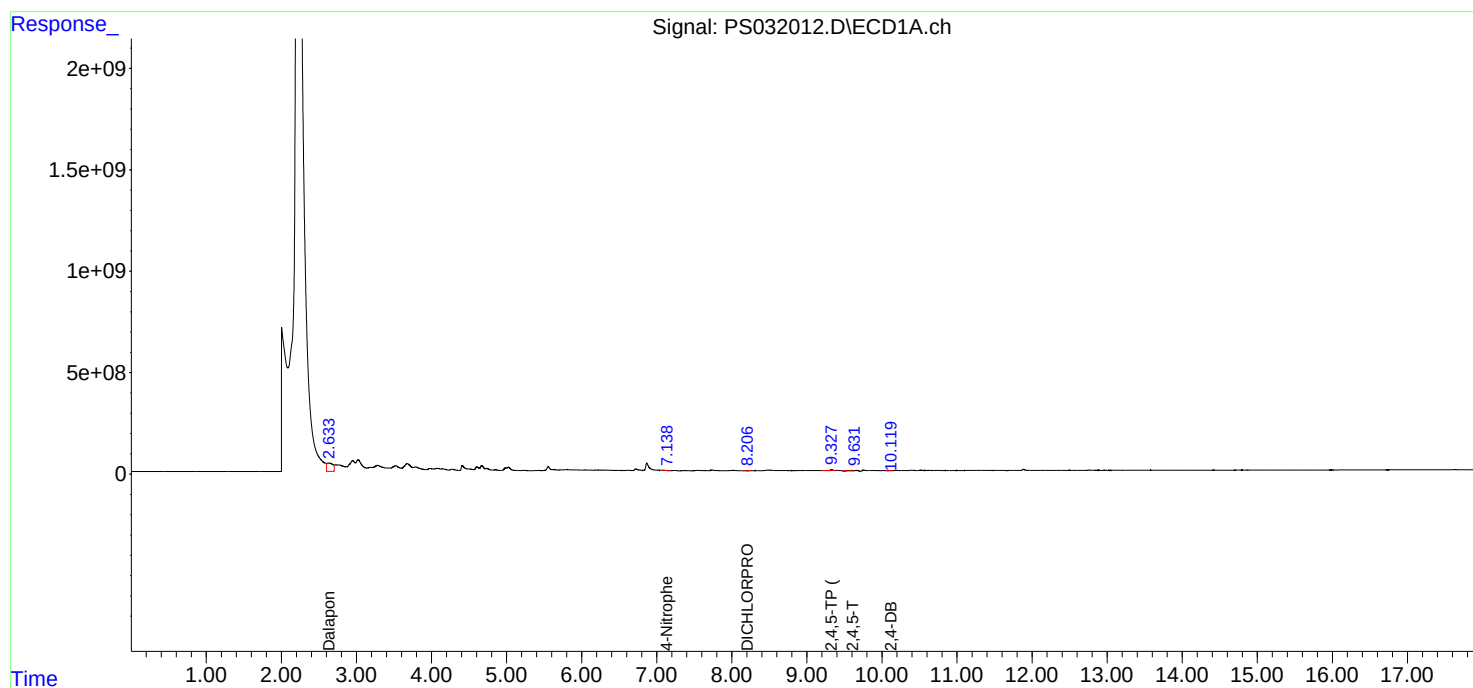


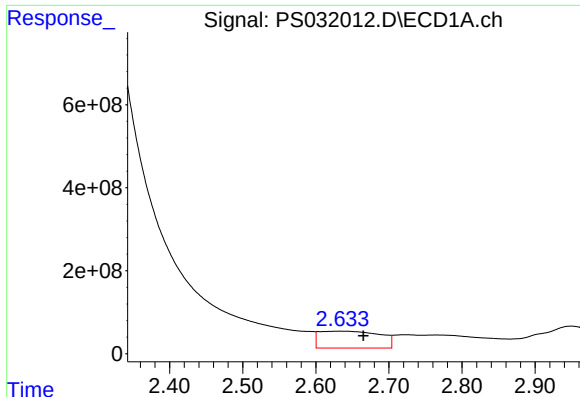

#1 Dalapon


R.T.: 2.633 min  
Delta R.T.: -0.032 min  
Response: 2325050086  
Conc: 300.88 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

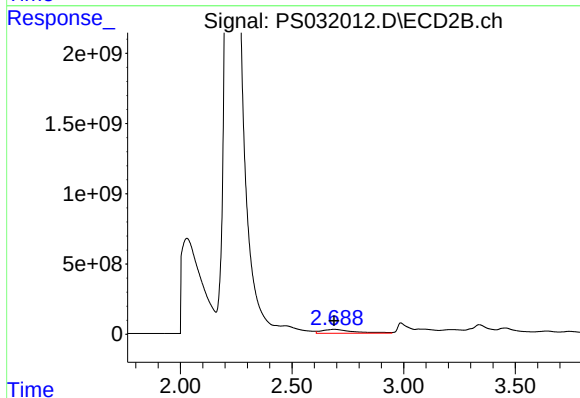


#1 Dalapon

R.T.: 2.688 min  
Delta R.T.: 0.000 min  
Response: 2754413176  
Conc: 732.89 ng/ml

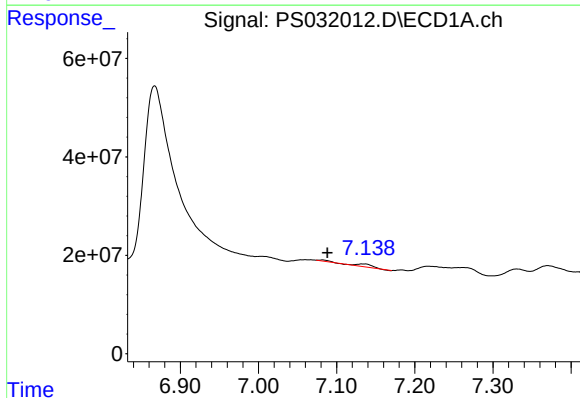


#3 4-Nitrophenol

R.T.: 7.134 min  
Delta R.T.: 0.046 min  
Response: 10938183  
Conc: 8.20 ng/ml

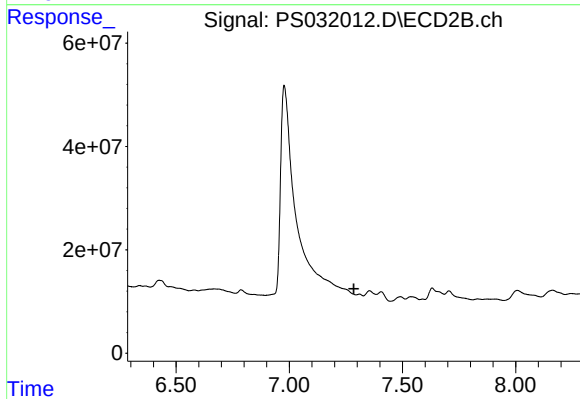

#3 4-Nitrophenol


R.T.: 0.000 min  
Exp R.T. : 7.285 min  
Response: 0  
Conc: N.D.

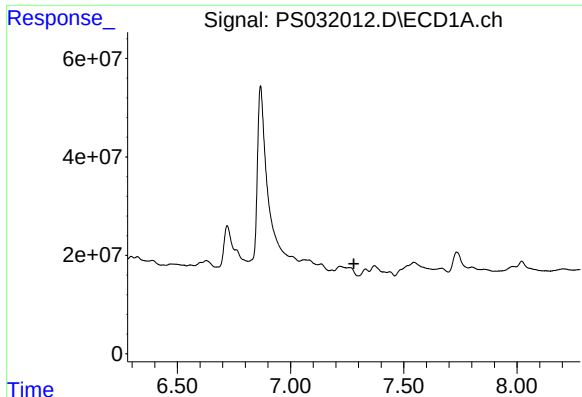

#4 2,4-DCAA


R.T.: 0.000 min  
Exp R.T. : 7.280 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

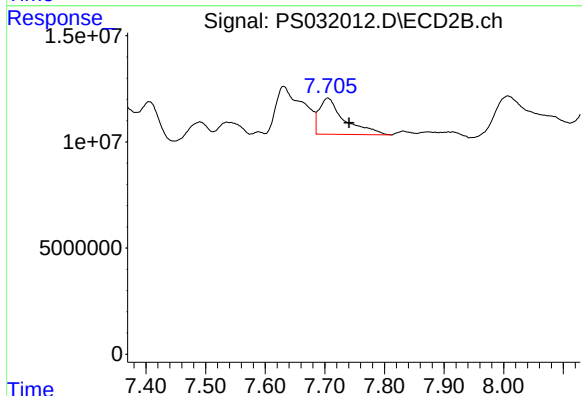


#4 2,4-DCAA

R.T.: 7.705 min  
Delta R.T.: -0.036 min  
Response: 49766250  
Conc: 45.23 ng/ml

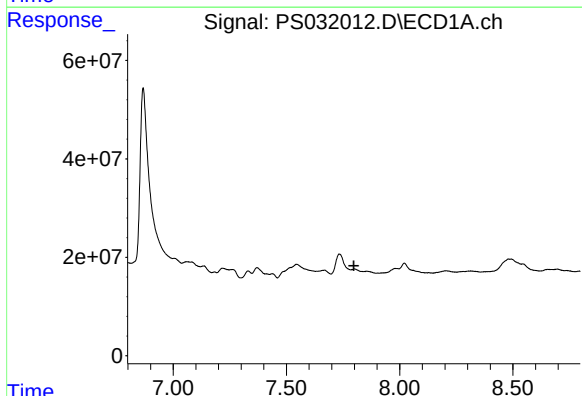


#7 MCPA

R.T.: 0.000 min  
Exp R.T. : 7.798 min  
Response: 0  
Conc: N.D.

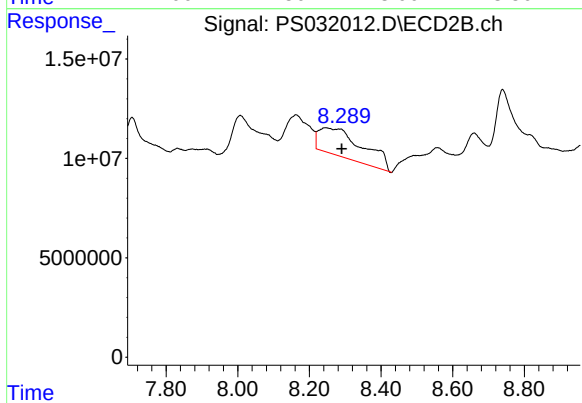

#7 MCPA


R.T.: 8.246 min  
Delta R.T.: -0.044 min  
Response: 118061897  
Conc: 31.30 ug/ml

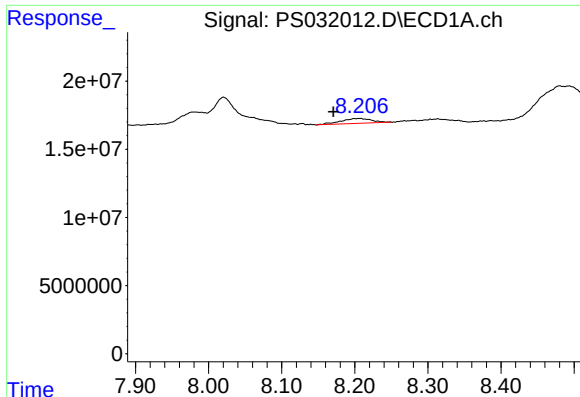

#8 DICHLORPROP


R.T.: 8.205 min  
Delta R.T.: 0.034 min  
Response: 10591592  
Conc: 2.23 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

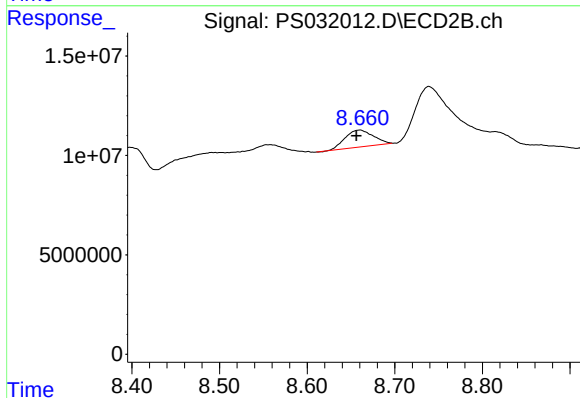


#8 DICHLORPROP

R.T.: 8.660 min  
Delta R.T.: 0.004 min  
Response: 18956265  
Conc: 9.68 ng/ml

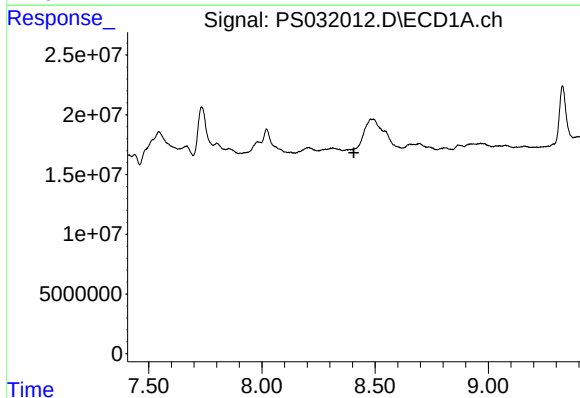


#9 2,4-D

R.T.: 0.000 min  
Exp R.T. : 8.406 min  
Response: 0  
Conc: N.D.

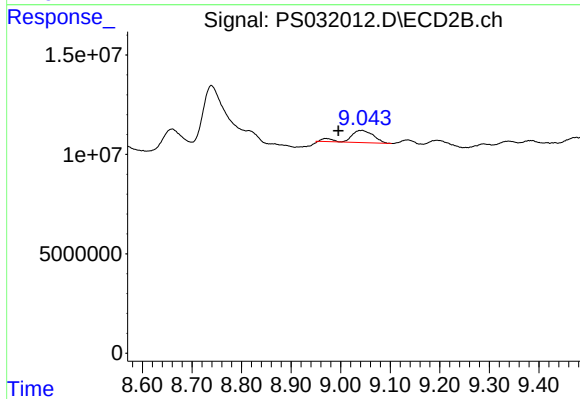

#9 2,4-D


R.T.: 9.042 min  
Delta R.T.: 0.046 min  
Response: 18837042  
Conc: 9.06 ng/ml

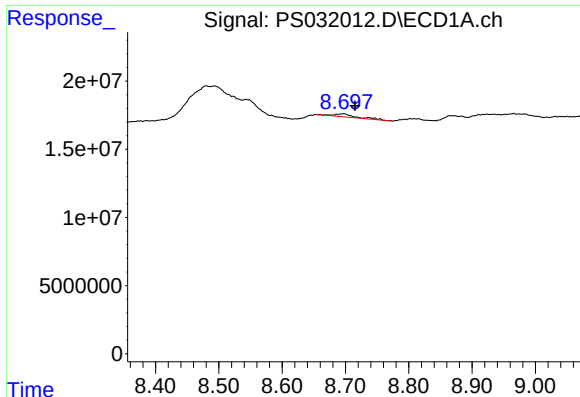

#10 Pentachlorophenol


R.T.: 8.694 min  
Delta R.T.: -0.021 min  
Response: 5380322  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

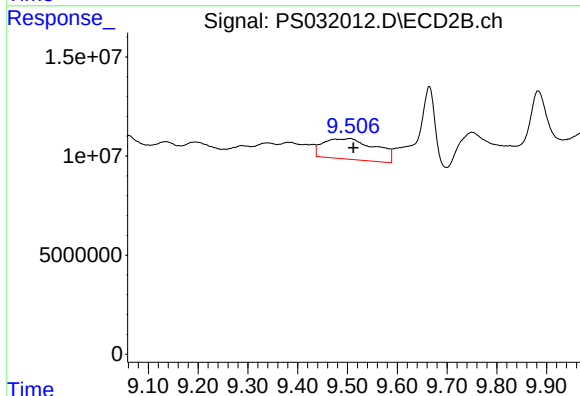


#10 Pentachlorophenol

R.T.: 9.503 min  
Delta R.T.: -0.009 min  
Response: 75688634  
Conc: 1.46 ng/ml

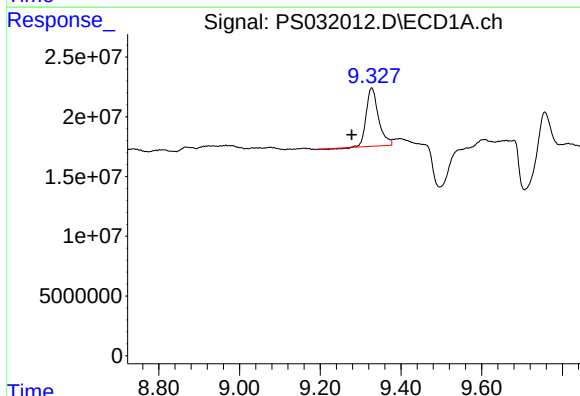


#11 2,4,5-TP (SILVEX)

R.T.: 9.328 min  
Delta R.T.: 0.050 min  
Response: 101944399  
Conc: 3.61 ng/ml

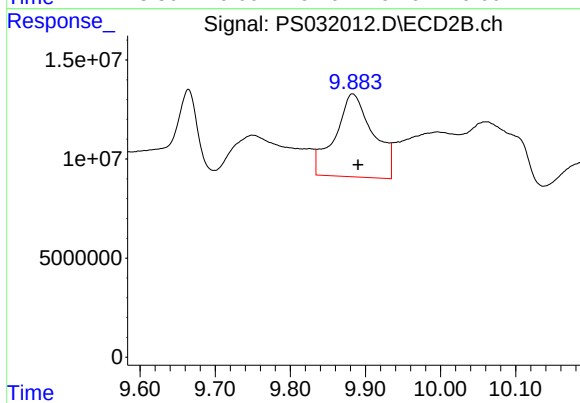

#11 2,4,5-TP (SILVEX)


R.T.: 9.884 min  
Delta R.T.: -0.006 min  
Response: 148222874  
Conc: 7.38 ng/ml

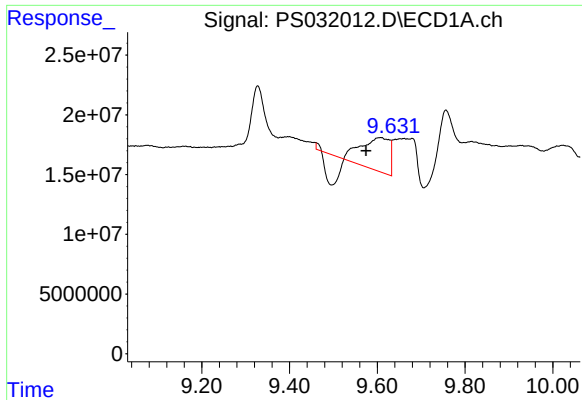

#12 2,4,5-T


R.T.: 9.606 min  
Delta R.T.: 0.032 min  
Response: 88072376  
Conc: 3.49 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

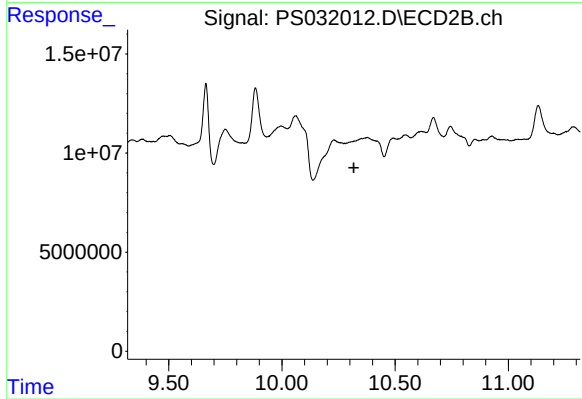


#12 2,4,5-T

R.T.: 0.000 min  
Exp R.T. : 10.318 min  
Response: 0  
Conc: N.D.

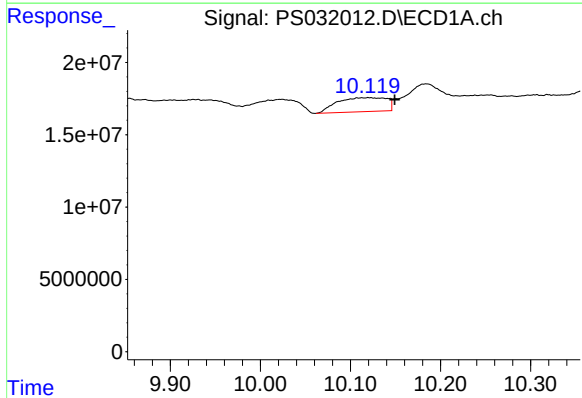

#13 2,4-DB

R.T.: 10.119 min  
Delta R.T.: -0.030 min  
Response: 37006801  
Conc: 11.94 ng/ml

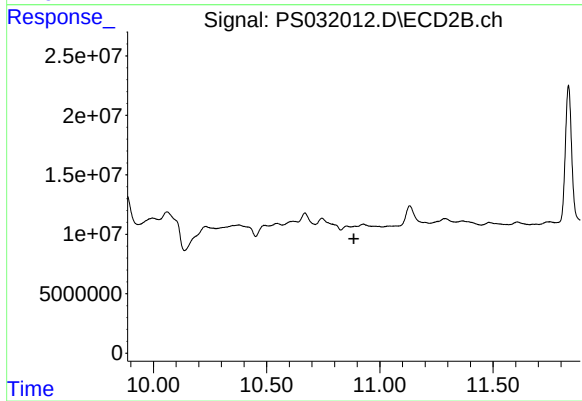

#13 2,4-DB

R.T.: 10.927 min  
Delta R.T.: 0.041 min  
Response: -2056400  
Conc: N.D.