

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101425\
 Data File : PS032017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Oct 2025 23:08
 Operator : AR\AJ
 Sample : PB170062TB
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 03:24:41 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.279	7.788f	1739.3E6	473.3E6	364.869	430.164
Target Compounds							
1) T	Dalapon	2.630f	2.657f	3451.2E6	2484.2E6	446.608	660.985 #
2) T	3,5-DICHL...	6.477f	0.000	308.6E6	0	43.838	N.D. #
3) T	4-Nitroph...	7.135f	0.000	24687570	0	18.497	N.D. #
7) T	MCPA	0.000	8.266	0	2891.3E6	N.D.	766.434
8) T	DICHLORPROP	0.000	8.664	0	71743021	N.D.	36.636
10) T	Pentachlo...	8.734	0.000	41481472	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.247f	9.877	25088267	4918.7E6	<MDL	245.017 #
12) T	2,4,5-T	0.000	10.334	0	6474.6E6	N.D.	377.645
13) T	2,4-DB	10.175f	0.000	1776.9E6	0	573.147	N.D. #
14) T	DINOSEB	11.306f	11.273	175.5E6	150.0E6	7.870	9.866 #
15) T	Picloram	11.148	12.422f	94918386	736.5E6	4.026	22.123 #
16) T	DCPA	11.615f	12.334f	285.6E6	119.8E6	7.772	3.606 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101425\
Data File : PS032017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Oct 2025 23:08
Operator : AR\AJ
Sample : PB170062TB
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 03:24:41 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

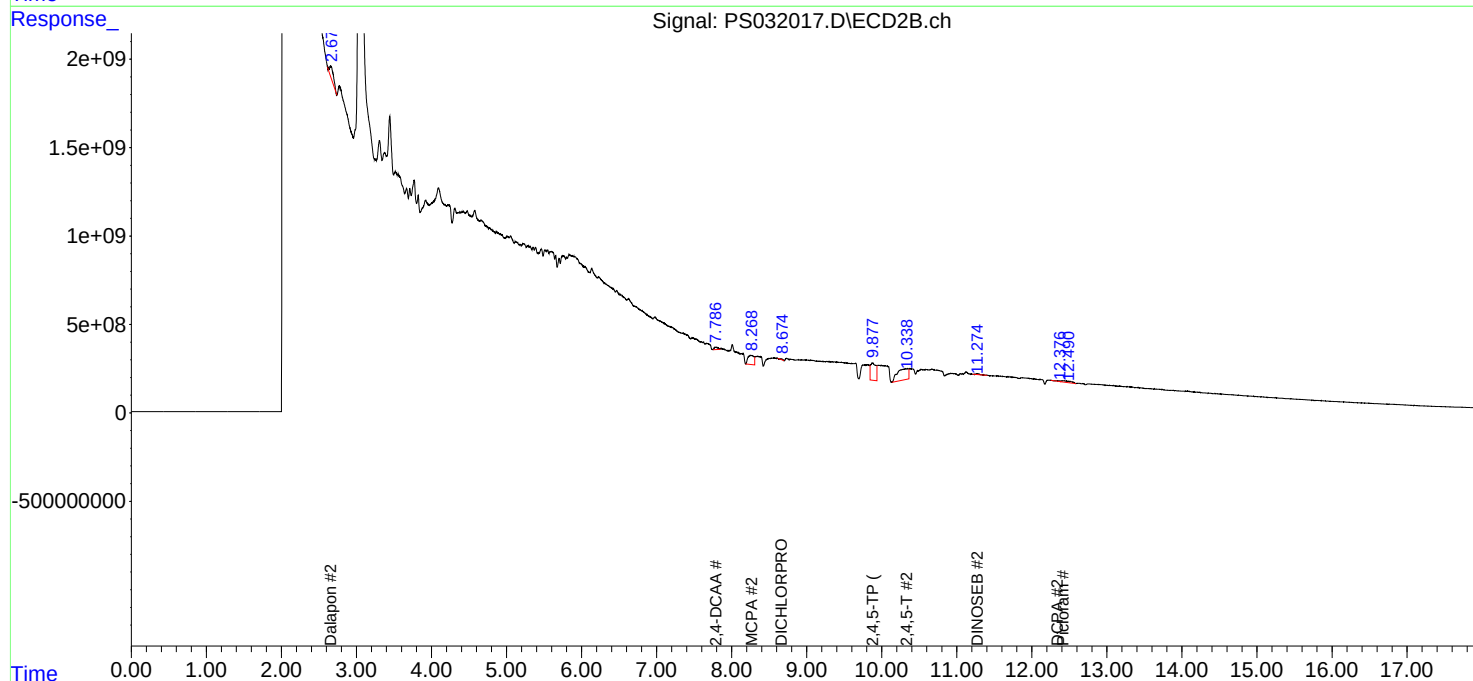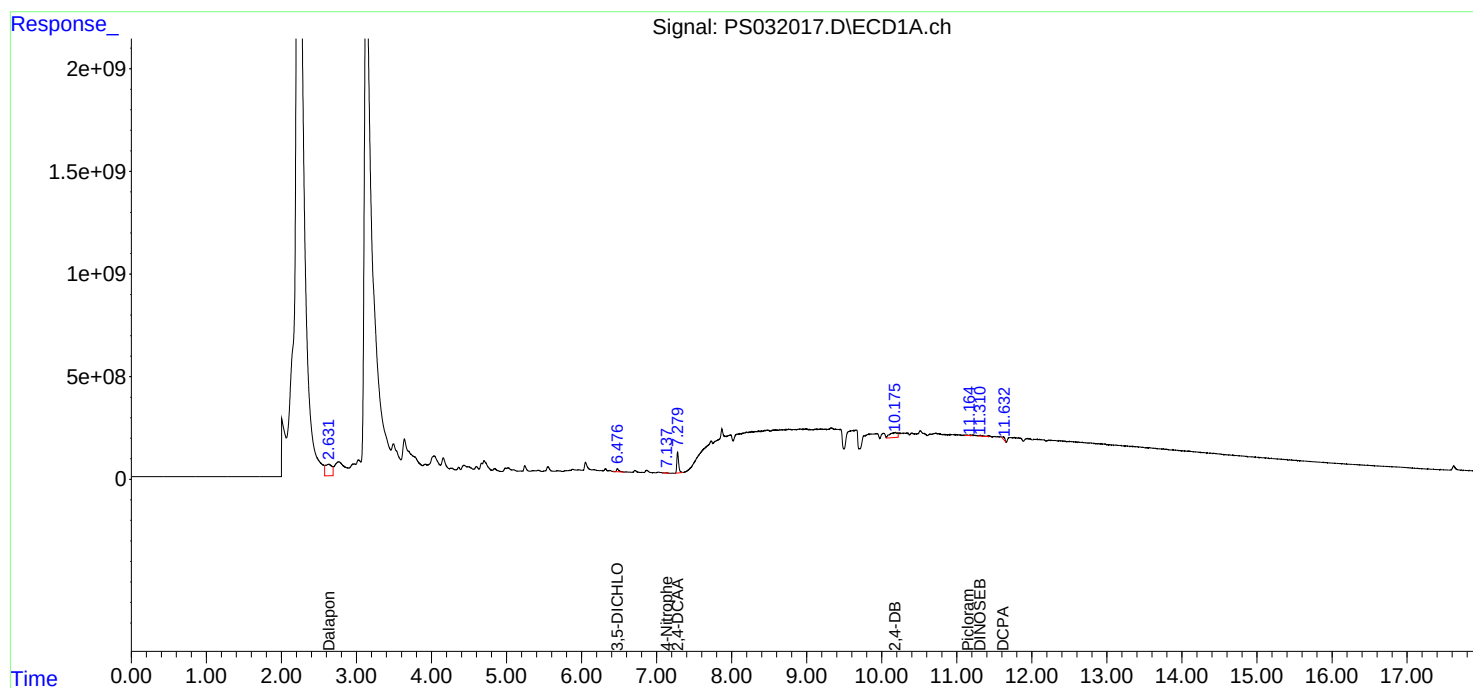


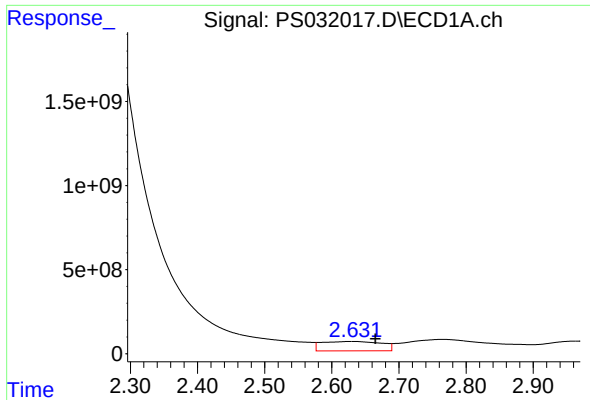

#1 Dalapon


R.T.: 2.630 min
Delta R.T.: -0.035 min
Response: 3451173242
Conc: 446.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

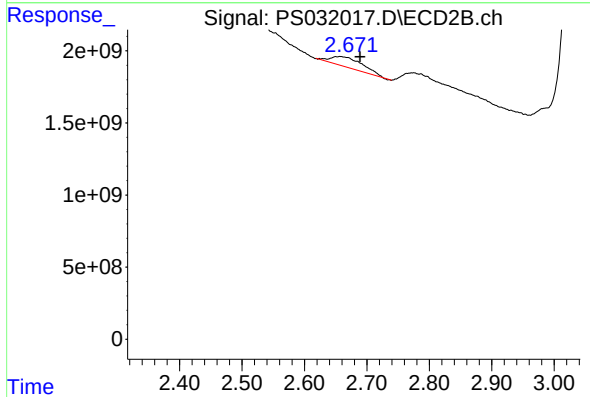


#1 Dalapon

R.T.: 2.657 min
Delta R.T.: -0.032 min
Response: 2484160503
Conc: 660.99 ng/ml

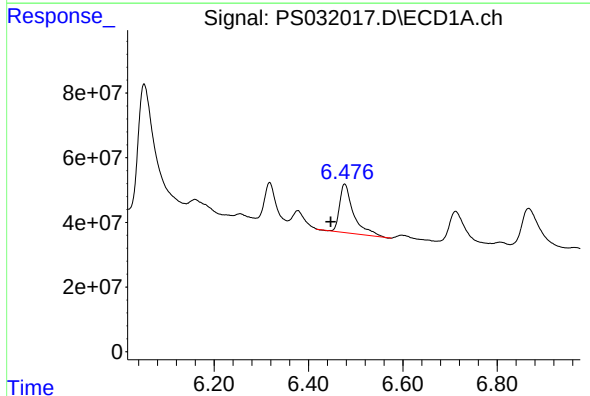


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.477 min
Delta R.T.: 0.029 min
Response: 308568858
Conc: 43.84 ng/ml

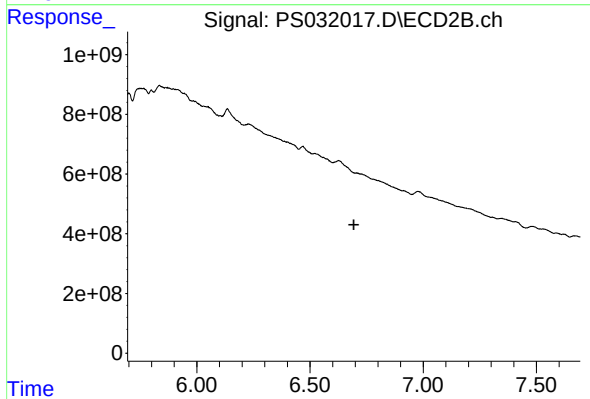

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 6.694 min
Response: 0
Conc: N.D.

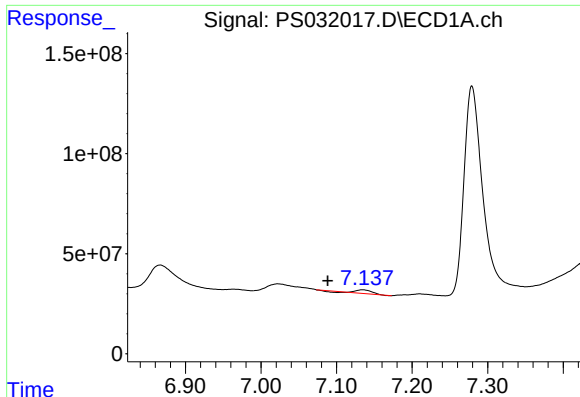

#3 4-Nitrophenol


R.T.: 7.135 min
Delta R.T.: 0.046 min
Response: 24687570
Conc: 18.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

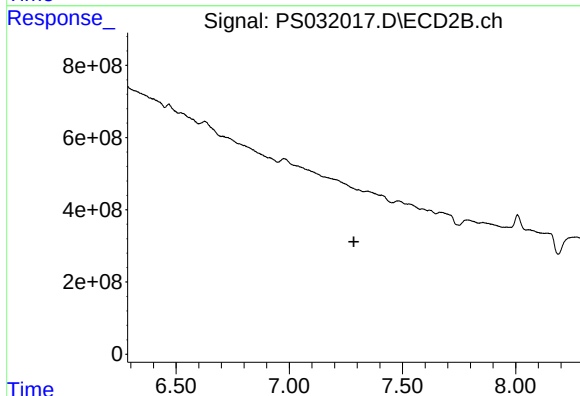


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.285 min
Response: 0
Conc: N.D.

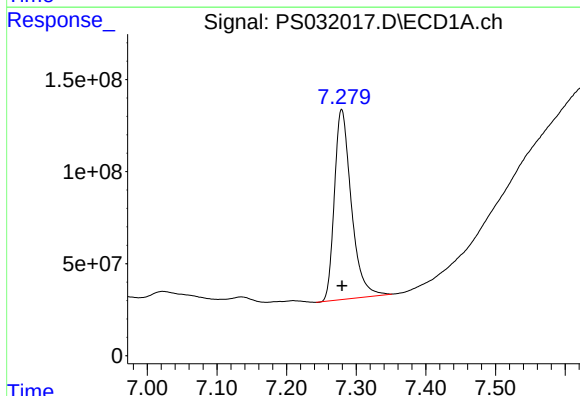


#4 2,4-DCAA

R.T.: 7.279 min
Delta R.T.: 0.000 min
Response: 1739344827
Conc: 364.87 ng/ml

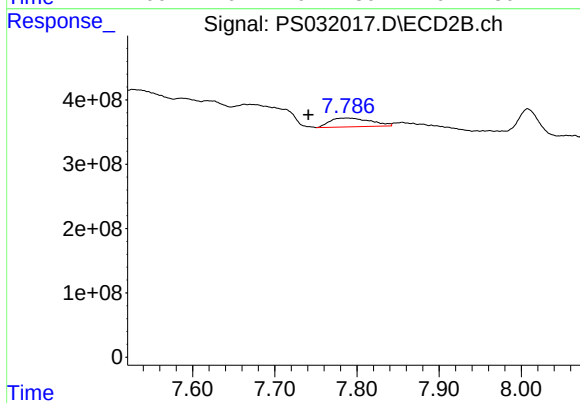

#4 2,4-DCAA


R.T.: 7.788 min
Delta R.T.: 0.047 min
Response: 473327254
Conc: 430.16 ng/ml

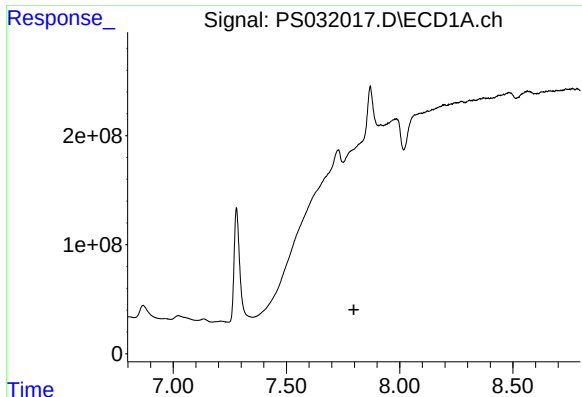

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.798 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

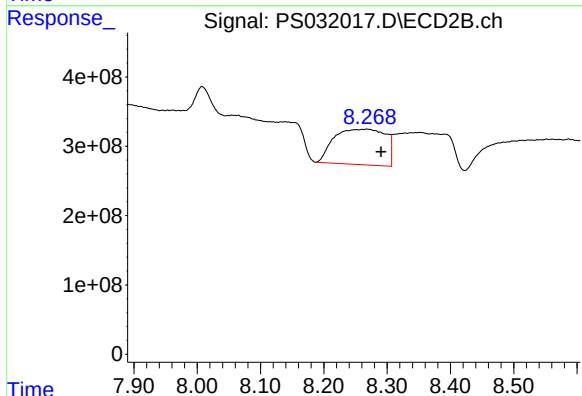


#7 MCPA

R.T.: 8.266 min
Delta R.T.: -0.025 min
Response: 2891259590
Conc: 766.43 ug/ml

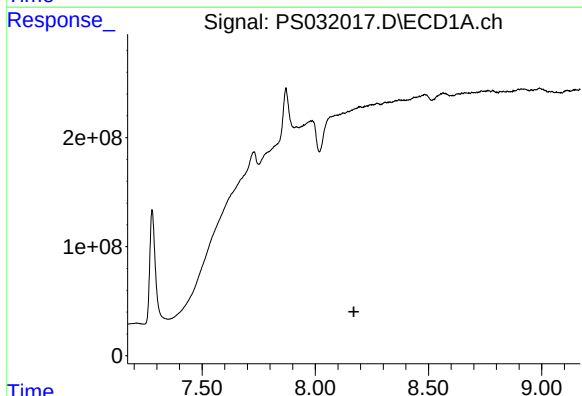


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.171 min
Response: 0
Conc: N.D.

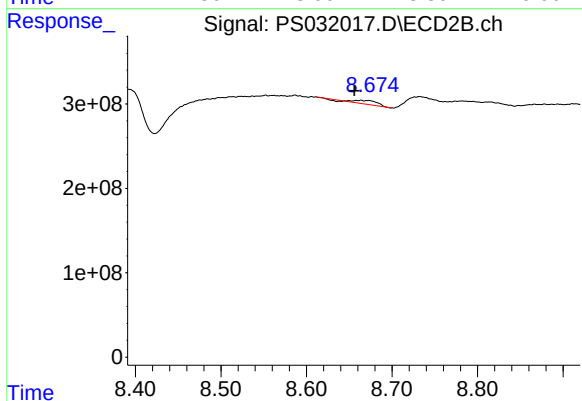

#8 DICHLORPROP


R.T.: 8.664 min
Delta R.T.: 0.008 min
Response: 71743021
Conc: 36.64 ng/ml

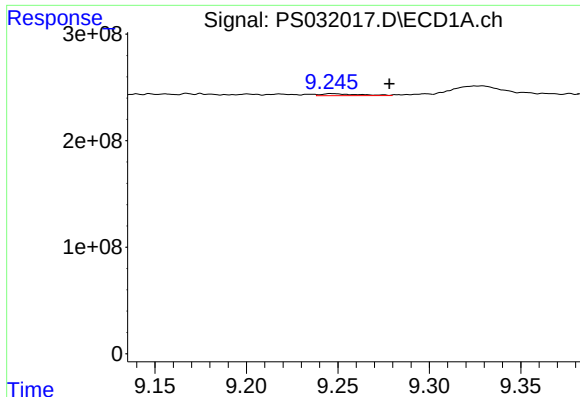

#11 2,4,5-TP (SILVEX)


R.T.: 9.247 min
Delta R.T.: -0.031 min
Response: 25088267
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

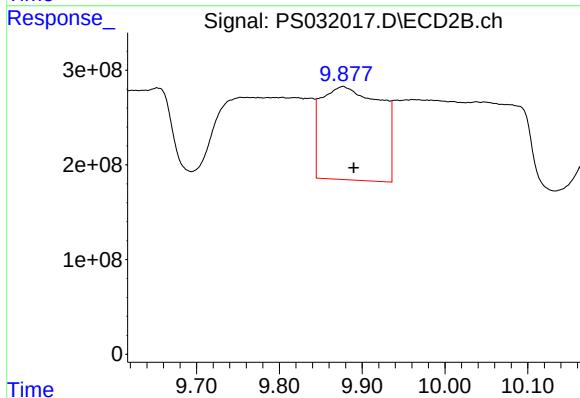


#11 2,4,5-TP (SILVEX)

R.T.: 9.877 min
Delta R.T.: -0.013 min
Response: 4918684490
Conc: 245.02 ng/ml

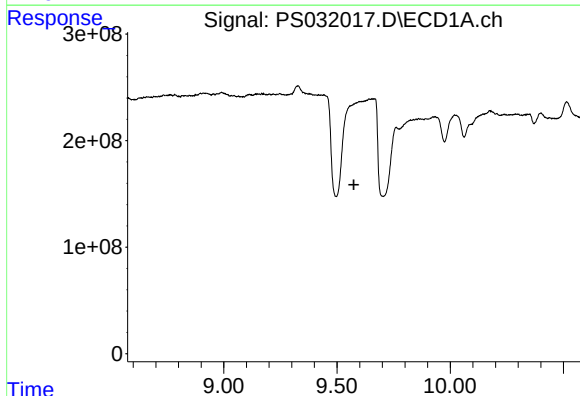


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.574 min
Response: 0
Conc: N.D.

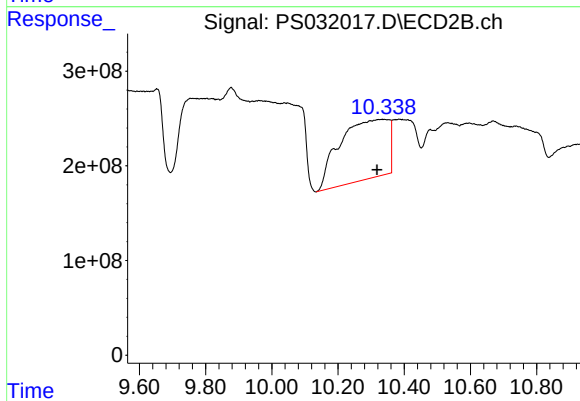

#12 2,4,5-T


R.T.: 10.334 min
Delta R.T.: 0.016 min
Response: 6474603662
Conc: 377.65 ng/ml

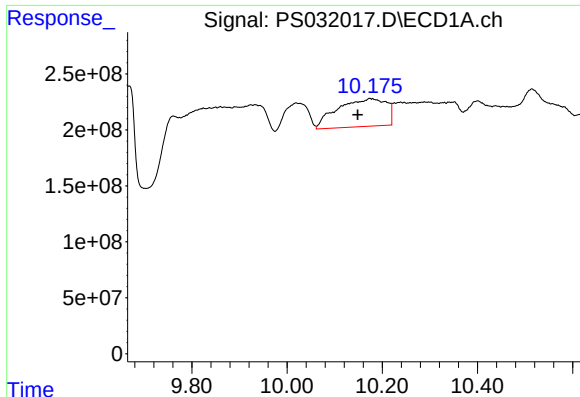

#13 2,4-DB


R.T.: 10.175 min
Delta R.T.: 0.026 min
Response: 1776937792
Conc: 573.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

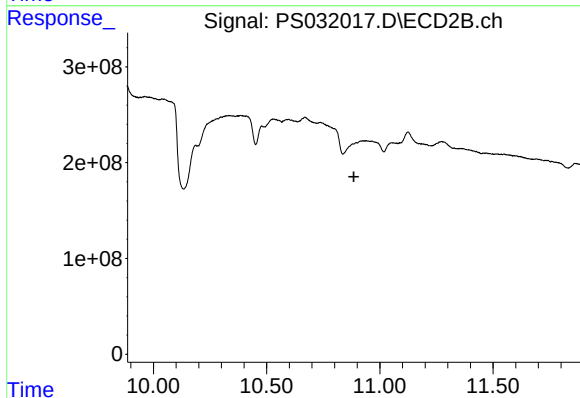


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.885 min
Response: 0
Conc: N.D.

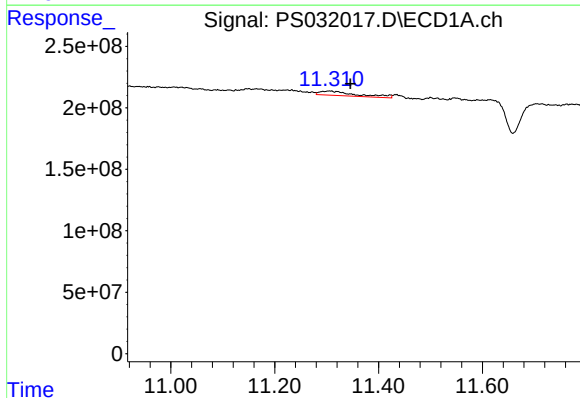


#14 DINOSEB

R.T.: 11.306 min
Delta R.T.: -0.040 min
Response: 175505805
Conc: 7.87 ng/ml

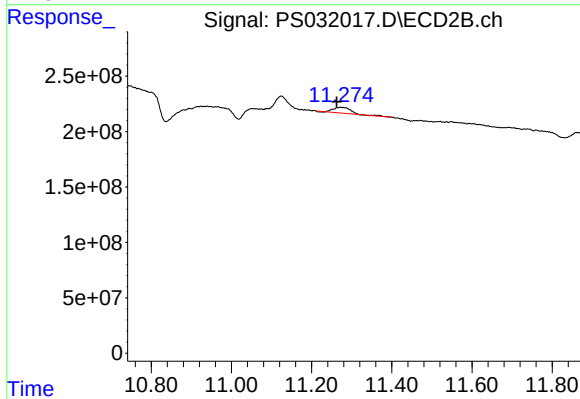

#14 DINOSEB


R.T.: 11.273 min
Delta R.T.: 0.010 min
Response: 149986488
Conc: 9.87 ng/ml

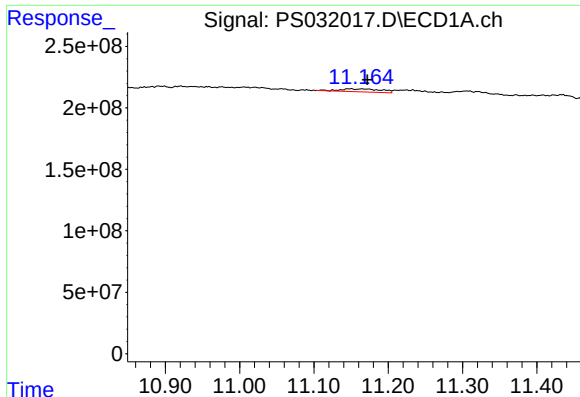

#15 Picloram


R.T.: 11.148 min
Delta R.T.: -0.024 min
Response: 94918386
Conc: 4.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

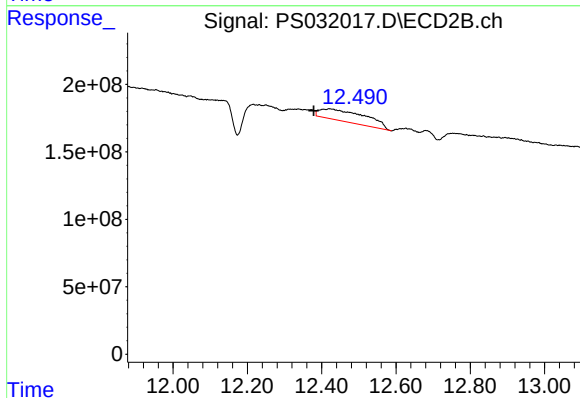


#15 Picloram

R.T.: 12.422 min
Delta R.T.: 0.043 min
Response: 736521751
Conc: 22.12 ng/ml

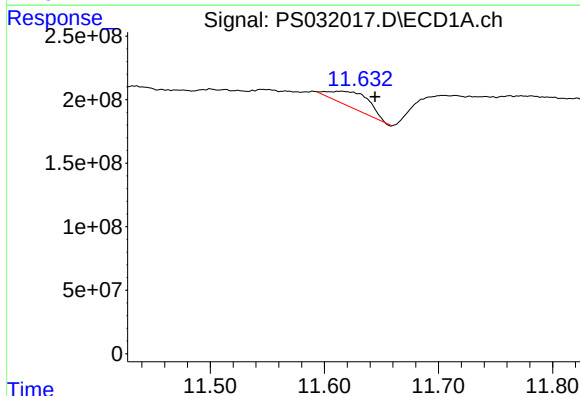

#16 DCPA

R.T.: 11.615 min
Delta R.T.: -0.030 min
Response: 285560667
Conc: 7.77 ng/ml

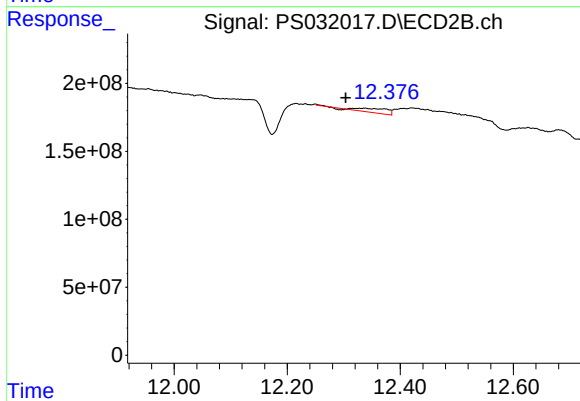

#16 DCPA

R.T.: 12.334 min
Delta R.T.: 0.030 min
Response: 119753695
Conc: 3.61 ng/ml