

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101518\
 Data File : PS002014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2018 19:54
 Operator : EI\SJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 08:48:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:46:20 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.461	10.936	160.0E6	182.2E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.940	2.387	210.1E6	203.3E6	682.500	682.500
2) T	3,5-DICHL...	9.884	9.088	215.1E6	208.2E6	697.500	697.500
3) T	4-Nitroph...	11.051	10.082	94635571	85902812	682.500	682.500
5) T	DICAMBA	11.771	11.221	566.1E6	596.4E6	705.000	705.000
6) T	MCPD	12.111	11.448	41826471	41112000	70.500	70.500
7) T	MCPA	12.361	11.824	66400449	60470231	69.750	69.750
8) T	DICHLORPROP	12.962	12.346	154.5E6	157.7E6	705.000	705.000
9) T	2,4-D	13.321	12.817	194.3E6	213.8E6	705.000	705.000
10) T	Pentachlo...	13.699	13.366	2075.4E6	2337.0E6	712.500	712.500
11) T	2,4,5-TP ...	14.572	13.983	796.5E6	932.2E6	712.500	712.500
12) T	2,4,5-T	14.969	14.550	852.0E6	792.0E6	712.500	712.500
13) T	2,4-DB	15.718	15.199	114.2E6	115.0E6	712.500	712.500
14) T	DINOSEB	17.203	15.628	595.7E6	637.1E6	705.000	705.000
15) T	Picloram	16.968	16.809	1260.3E6	1169.0E6	712.500	712.500
16) T	DCPA	17.546	16.863	1021.4E6	1377.0E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101518\
Data File : PS002014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2018 19:54
Operator : EI\SJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 08:48:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:46:20 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

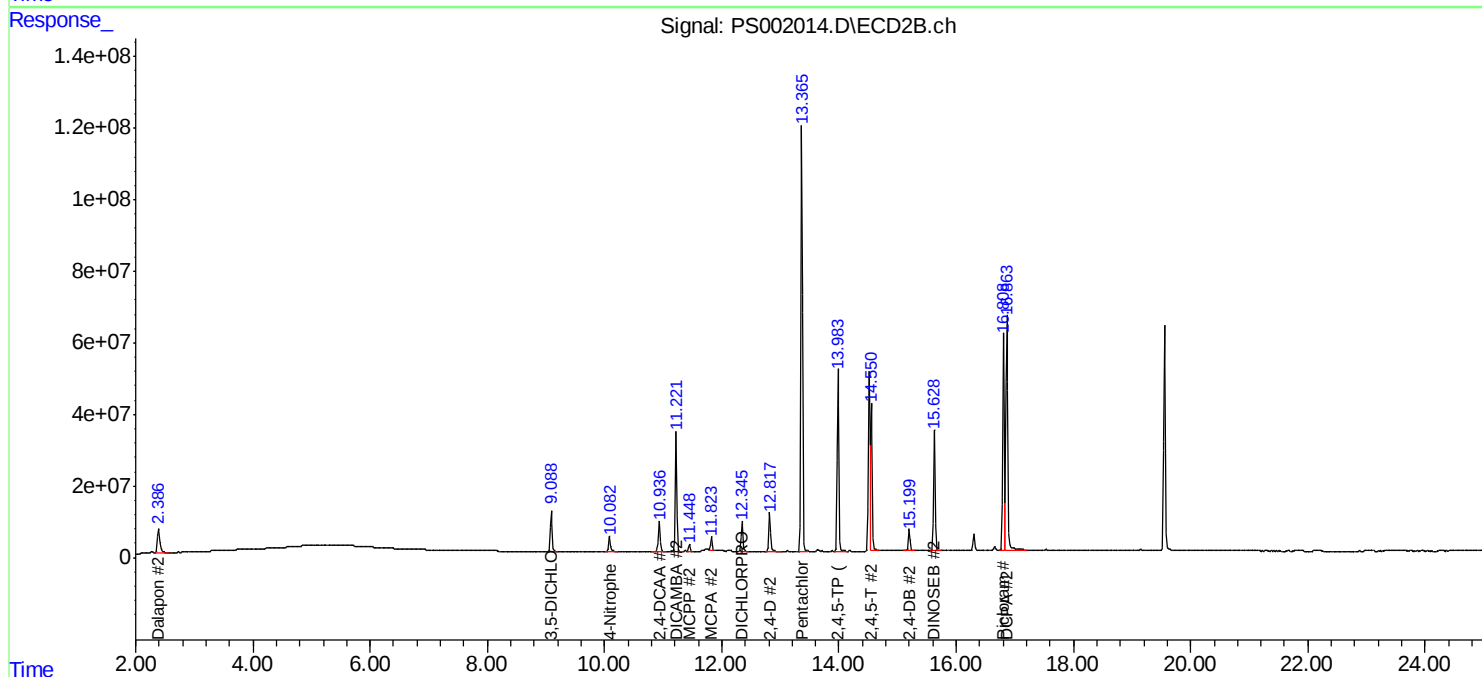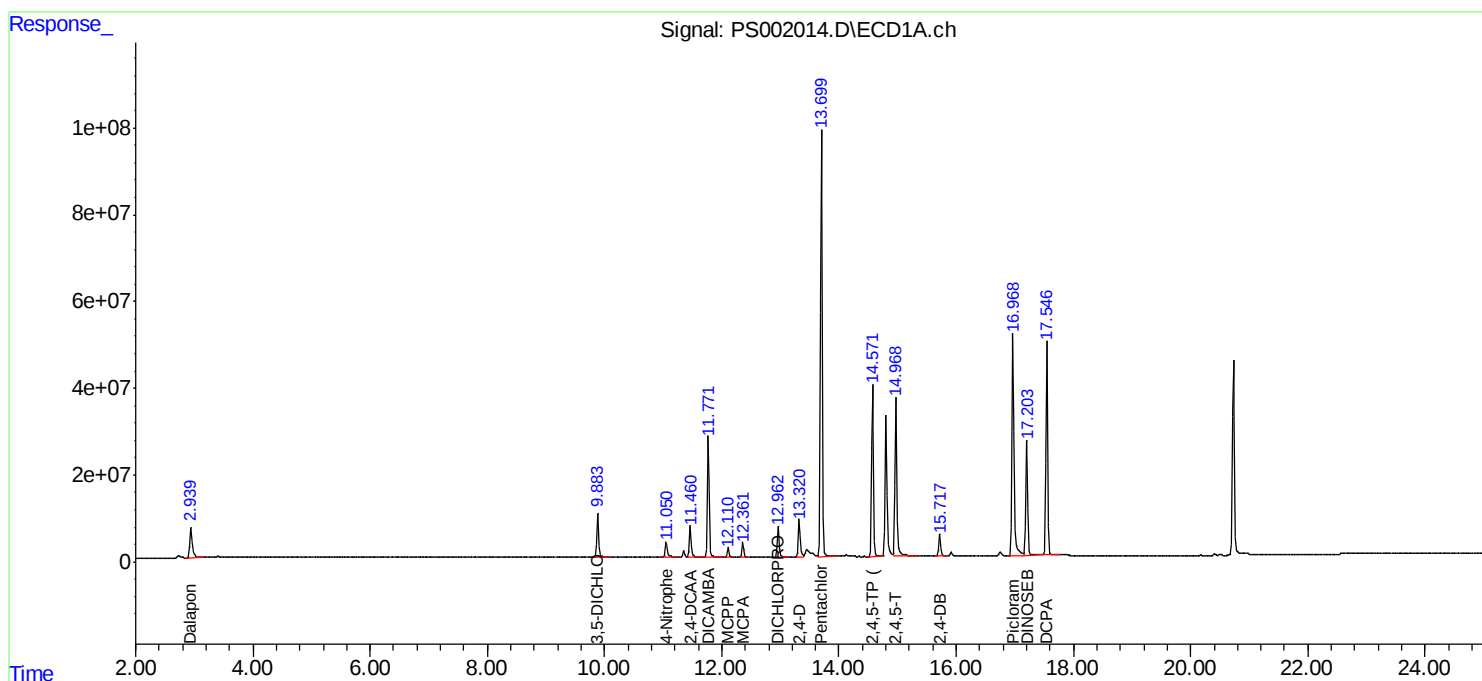


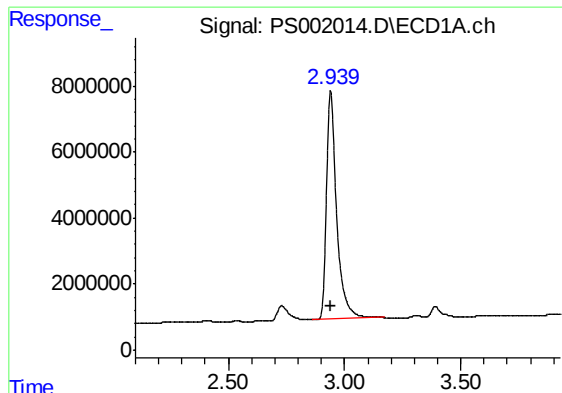

#1 Dalapon


R.T.: 2.940 min
Delta R.T.: 0.000 min
Response: 210080261
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

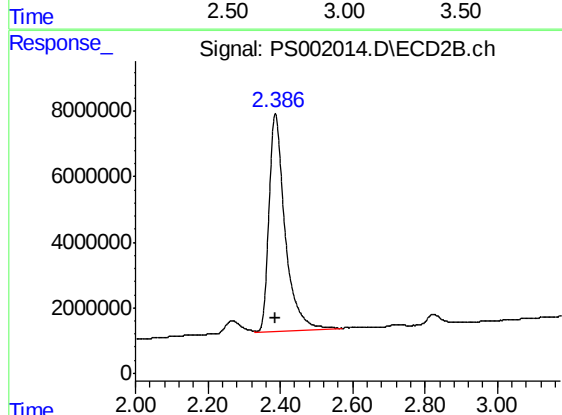


#1 Dalapon

R.T.: 2.387 min
Delta R.T.: 0.000 min
Response: 203308996
Conc: 682.50 ng/ml

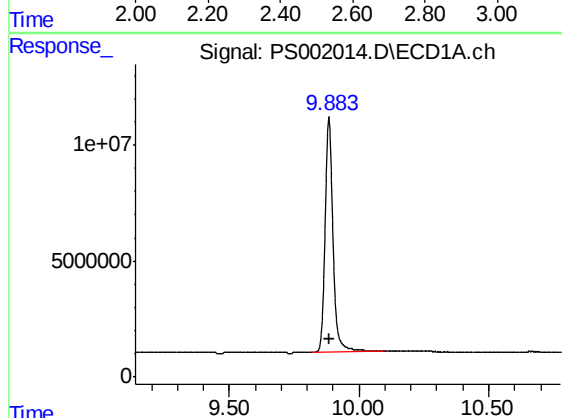


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.884 min
Delta R.T.: 0.000 min
Response: 215114985
Conc: 697.50 ng/ml

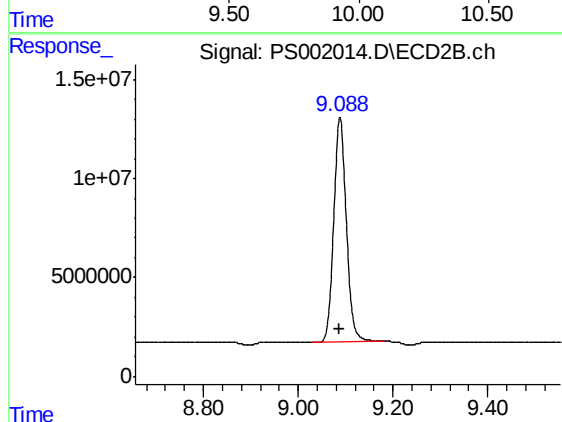

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.088 min
Delta R.T.: 0.000 min
Response: 208212543
Conc: 697.50 ng/ml

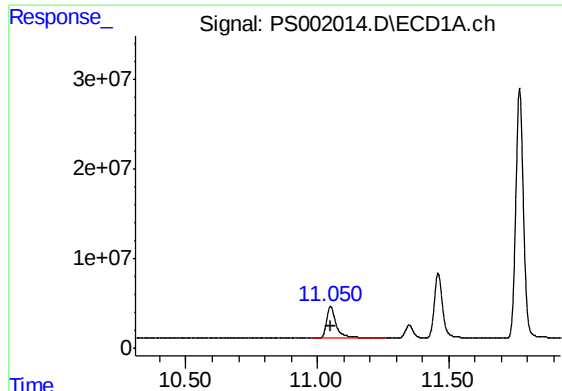

#3 4-Nitrophenol


R.T.: 11.051 min
Delta R.T.: 0.000 min
Response: 94635571
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

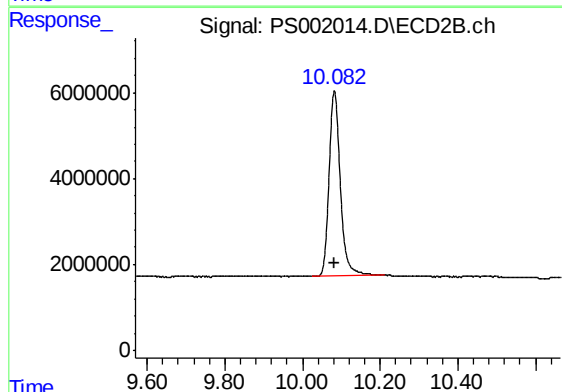


#3 4-Nitrophenol

R.T.: 10.082 min
Delta R.T.: 0.000 min
Response: 85902812
Conc: 682.50 ng/ml

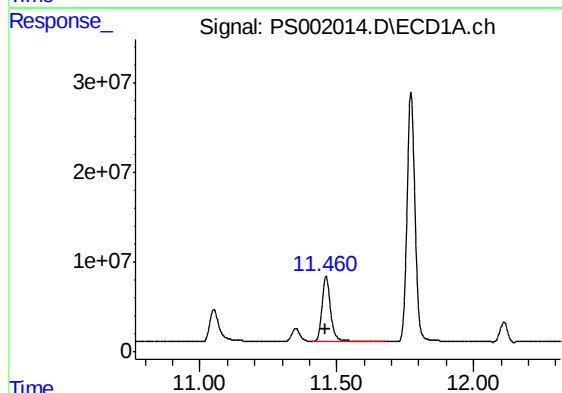


#4 2,4-DCAA

R.T.: 11.461 min
Delta R.T.: 0.000 min
Response: 160025112
Conc: 750.00 ng/ml

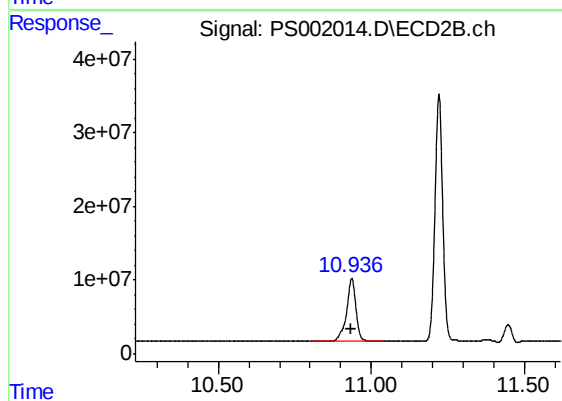

#4 2,4-DCAA


R.T.: 10.936 min
Delta R.T.: 0.000 min
Response: 182161335
Conc: 750.00 ng/ml

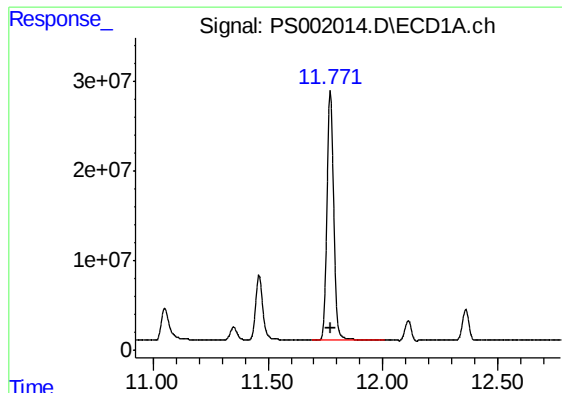

#5 DICAMBA


R.T.: 11.771 min
Delta R.T.: 0.000 min
Response: 566147023
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

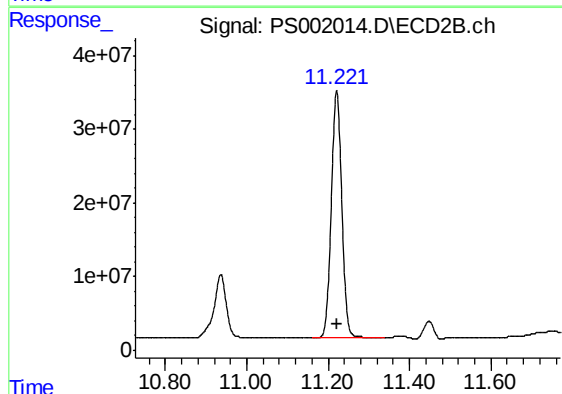


#5 DICAMBA

R.T.: 11.221 min
Delta R.T.: 0.000 min
Response: 596427972
Conc: 705.00 ng/ml

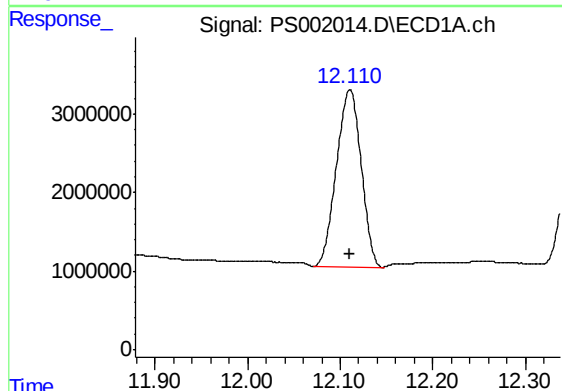


#6 MCPP

R.T.: 12.111 min
Delta R.T.: 0.000 min
Response: 41826471
Conc: 70.50 ug/ml

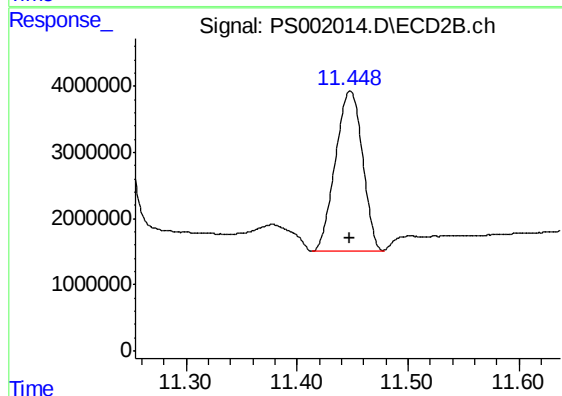

#6 MCPP


R.T.: 11.448 min
Delta R.T.: 0.000 min
Response: 41112000
Conc: 70.50 ug/ml

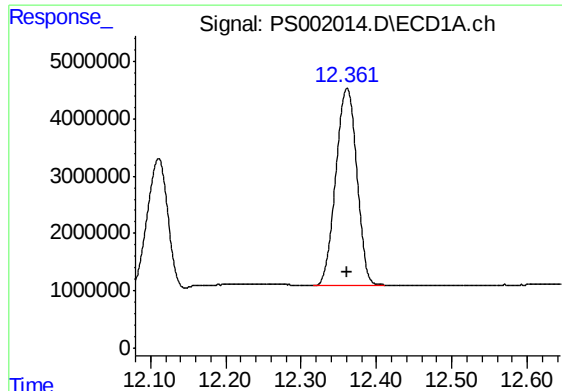

#7 MCPA


R.T.: 12.361 min
Delta R.T.: 0.000 min
Response: 66400449
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

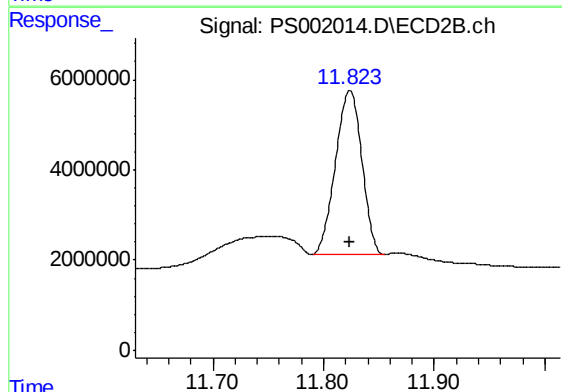


#7 MCPA

R.T.: 11.824 min
Delta R.T.: 0.000 min
Response: 60470231
Conc: 69.75 ug/ml

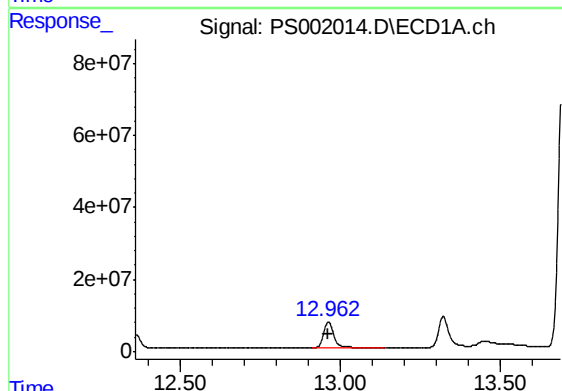


#8 DICHLORPROP

R.T.: 12.962 min
Delta R.T.: 0.000 min
Response: 154541091
Conc: 705.00 ng/ml

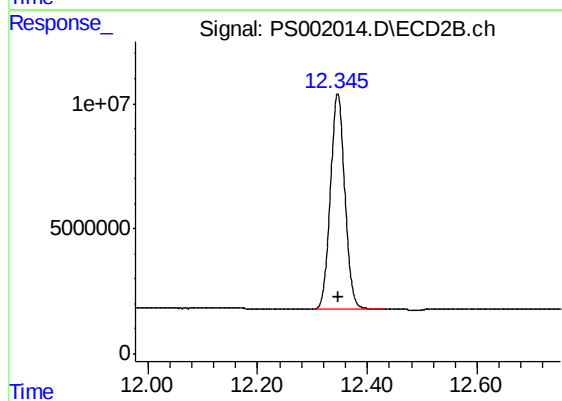

#8 DICHLORPROP


R.T.: 12.346 min
Delta R.T.: 0.000 min
Response: 157650400
Conc: 705.00 ng/ml

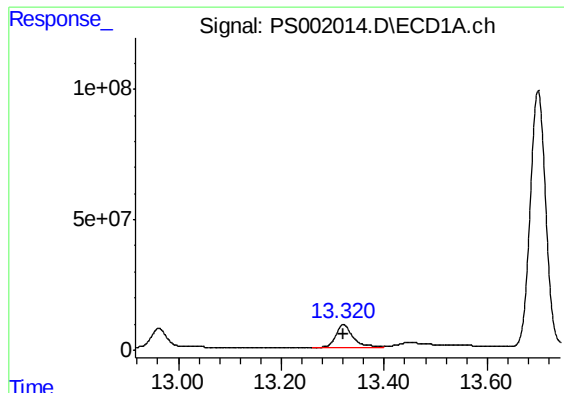

#9 2,4-D


R.T.: 13.321 min
Delta R.T.: 0.000 min
Response: 194309289
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

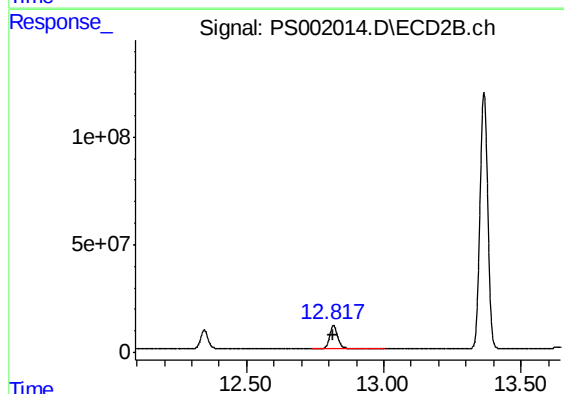


#9 2,4-D

R.T.: 12.817 min
Delta R.T.: 0.000 min
Response: 213783092
Conc: 705.00 ng/ml

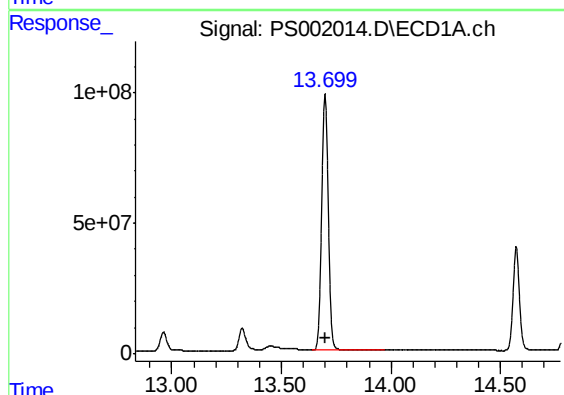


#10 Pentachlorophenol

R.T.: 13.699 min
Delta R.T.: 0.000 min
Response: 2075436344
Conc: 712.50 ng/ml

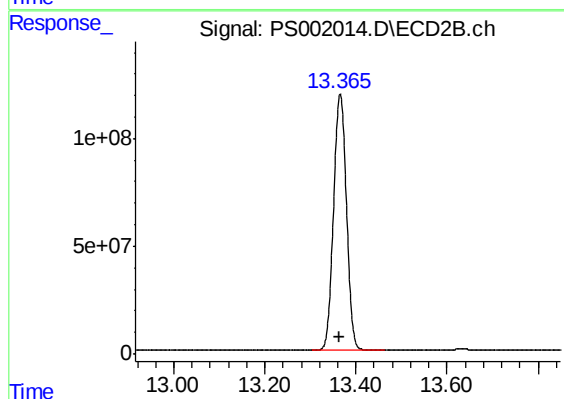

#10 Pentachlorophenol


R.T.: 13.366 min
Delta R.T.: 0.000 min
Response: 2336974598
Conc: 712.50 ng/ml

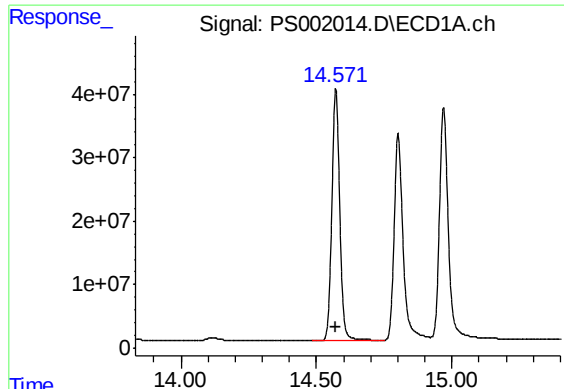

#11 2,4,5-TP (SILVEX)


R.T.: 14.572 min
Delta R.T.: 0.000 min
Response: 796483611
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

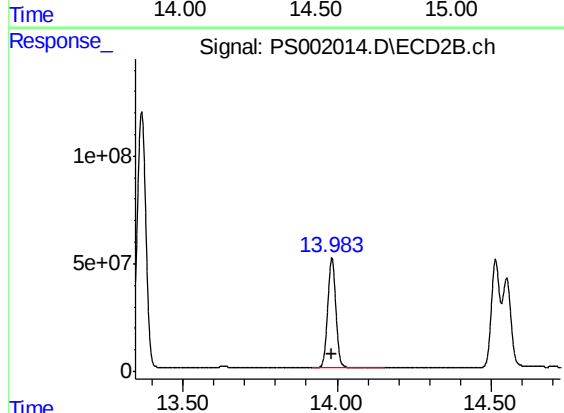


#11 2,4,5-TP (SILVEX)

R.T.: 13.983 min
Delta R.T.: 0.000 min
Response: 932156326
Conc: 712.50 ng/ml

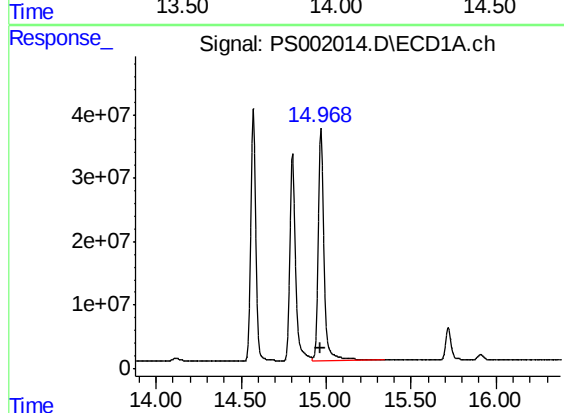


#12 2,4,5-T

R.T.: 14.969 min
Delta R.T.: 0.000 min
Response: 852009511
Conc: 712.50 ng/ml

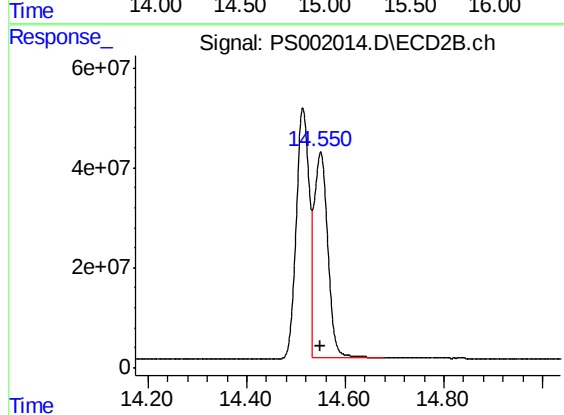

#12 2,4,5-T


R.T.: 14.550 min
Delta R.T.: 0.000 min
Response: 791972123
Conc: 712.50 ng/ml

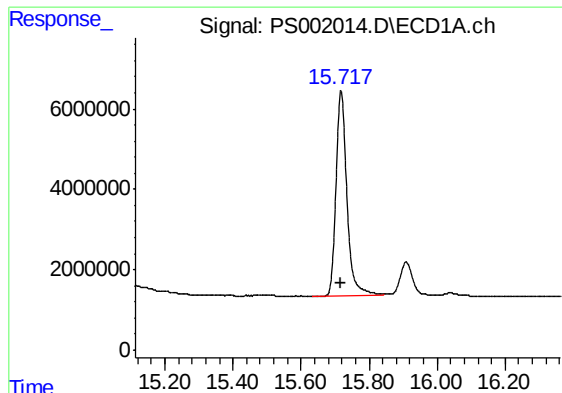

#13 2,4-DB


R.T.: 15.718 min
Delta R.T.: 0.000 min
Response: 114161042
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

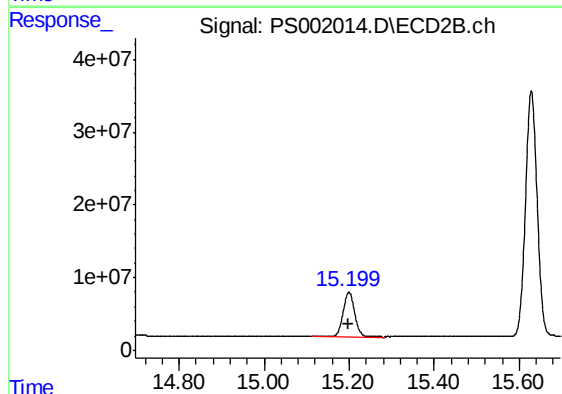


#13 2,4-DB

R.T.: 15.199 min
Delta R.T.: 0.000 min
Response: 115024139
Conc: 712.50 ng/ml

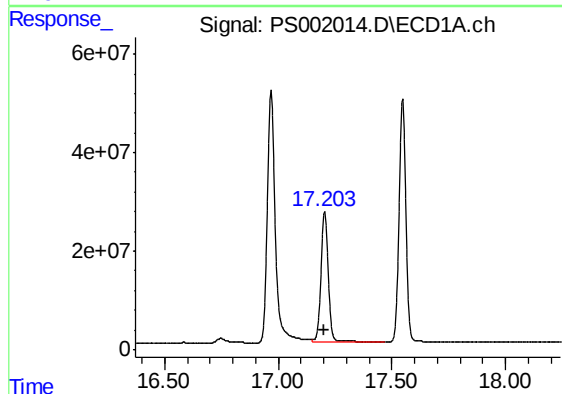


#14 DINOSEB

R.T.: 17.203 min
Delta R.T.: 0.000 min
Response: 595683346
Conc: 705.00 ng/ml

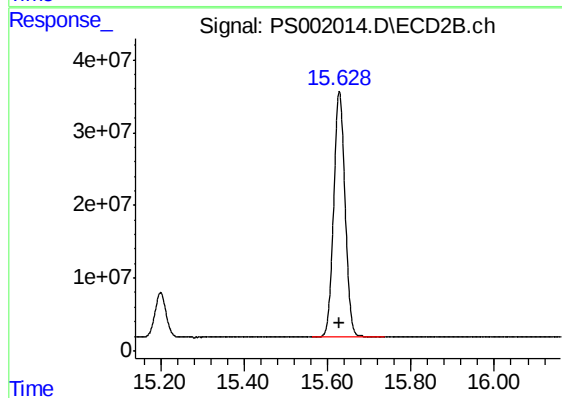

#14 DINOSEB


R.T.: 15.628 min
Delta R.T.: 0.000 min
Response: 637107840
Conc: 705.00 ng/ml

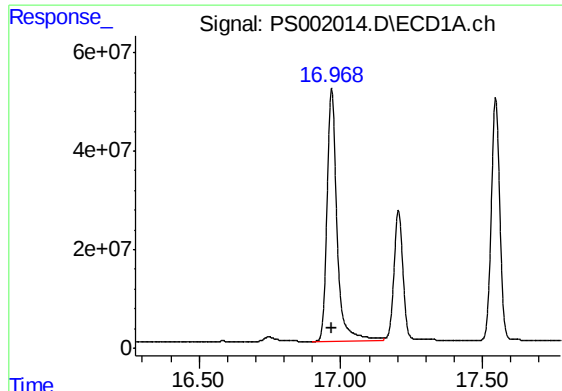

#15 Picloram


R.T.: 16.968 min
Delta R.T.: 0.000 min
Response: 1260284522
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

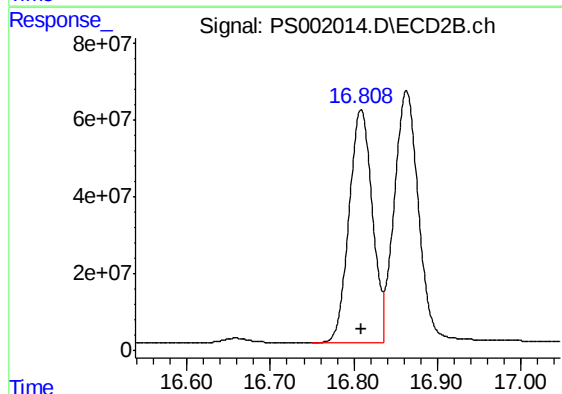


#15 Picloram

R.T.: 16.809 min
Delta R.T.: 0.000 min
Response: 1169021989
Conc: 712.50 ng/ml

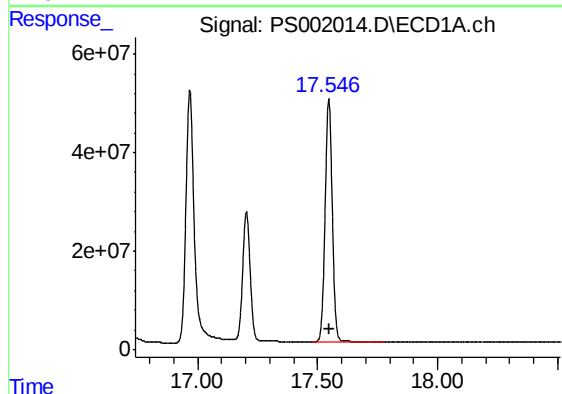

#16 DCPA

R.T.: 17.546 min
Delta R.T.: 0.000 min
Response: 1021383859
Conc: 720.00 ng/ml

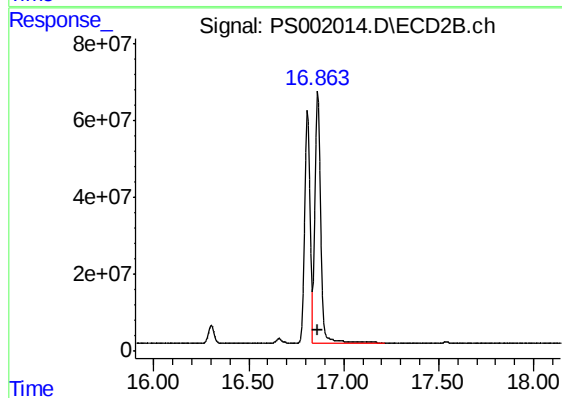

#16 DCPA

R.T.: 16.863 min
Delta R.T.: 0.000 min
Response: 1376975523
Conc: 720.00 ng/ml