

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
 Data File : PS007143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 10:23
 Operator : SM\AJ
 Sample : PB123861BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB123861BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 11:44:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.461	5.189	576.6E6	298.0E6	421.307	423.776
Target Compounds							
7) T	MCPA	0.000	5.511	0	51202830	N.D.	17.613
9) T	2,4-D	6.485	0.000	165.1E6	0	133.981	N.D. #
10) T	Pentachlo...	0.000	6.482	0	9719374	N.D.	1.011
14) T	DINOSEB	9.033	0.000	53149467	0	9.133	N.D. #
15) T	Picloram	0.000	8.955	0	85869684	N.D.	13.985



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
Data File : PS007143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 10:23
Operator : SM\AJ
Sample : PB123861BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB123861BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 11:44:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

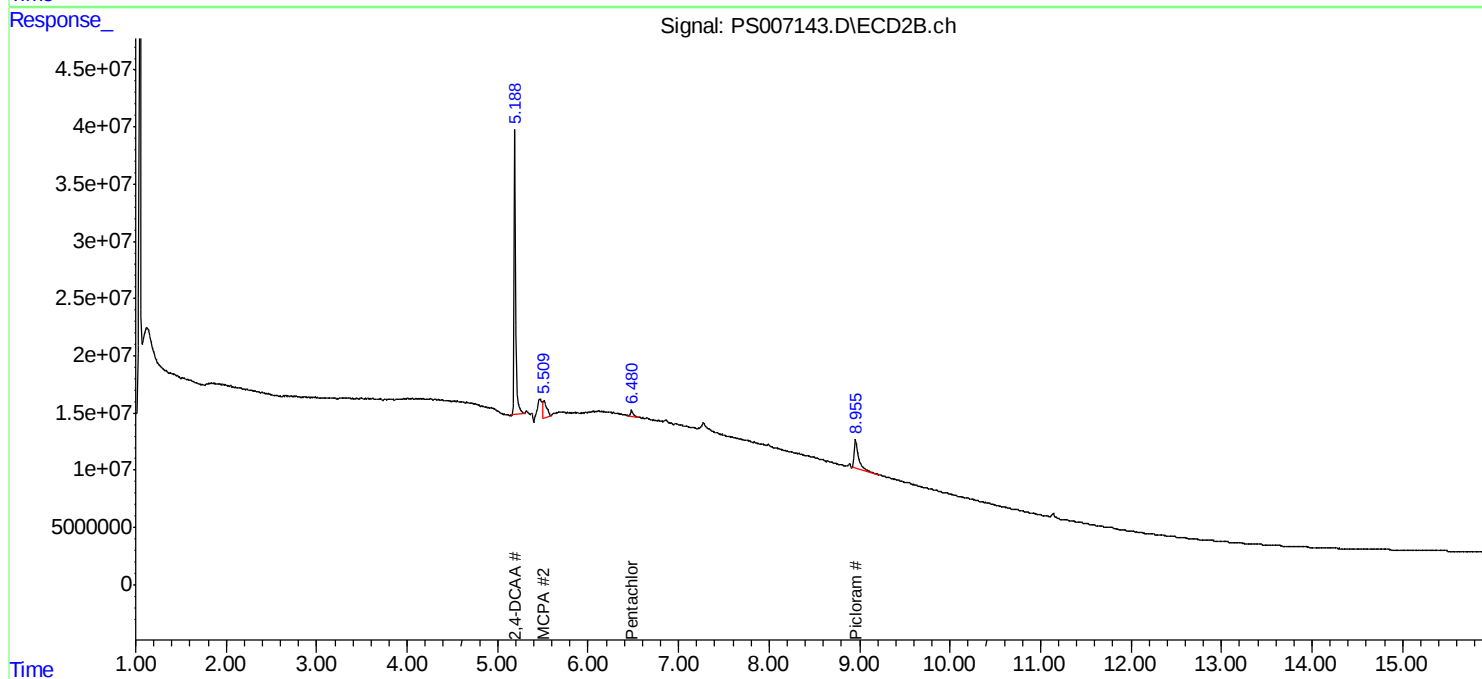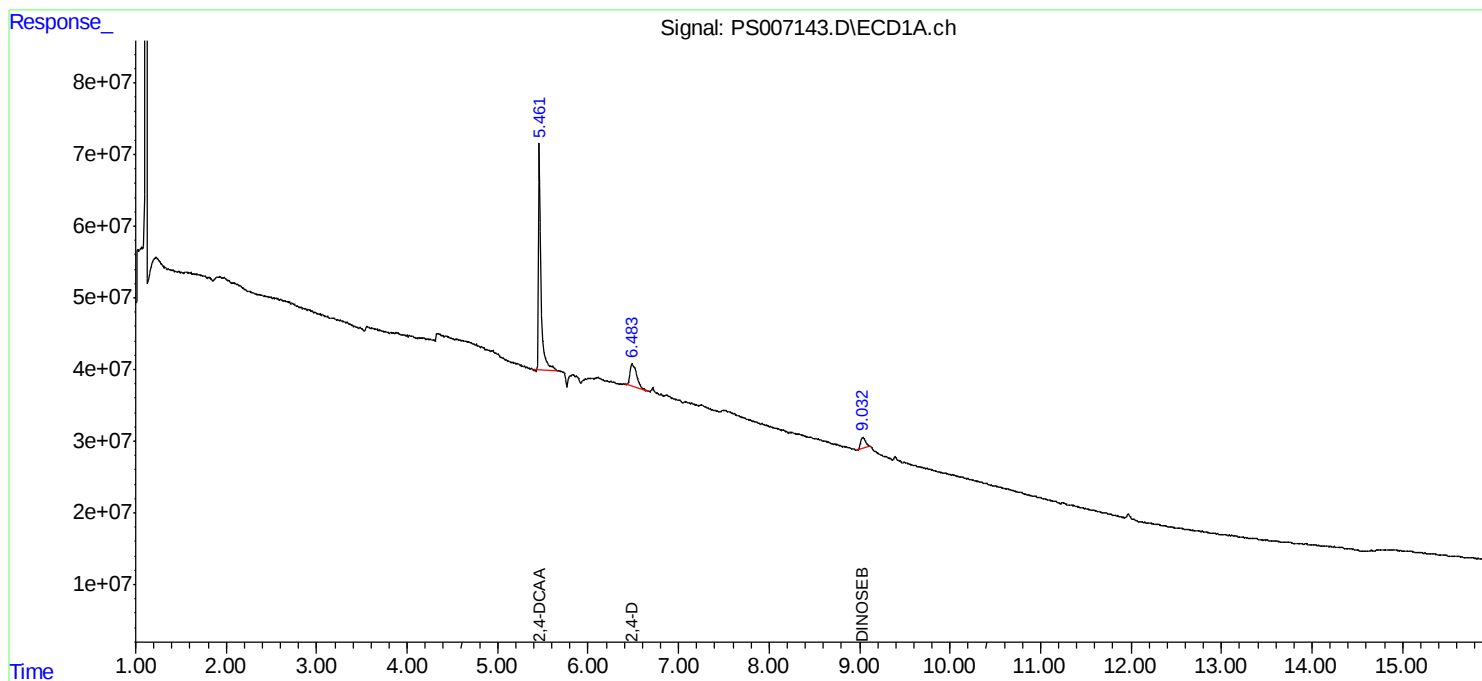


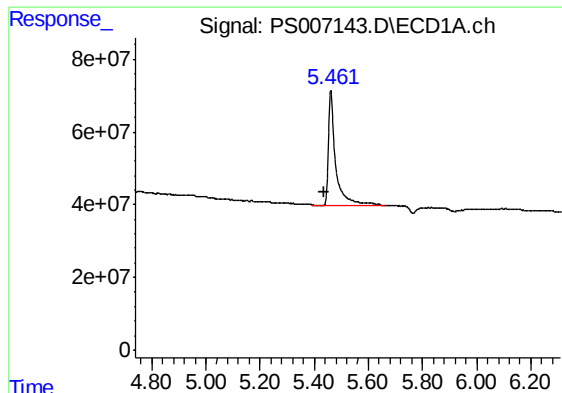

#4 2,4-DCAA


R.T.: 5.461 min
Delta R.T.: 0.026 min
Response: 576630207
Conc: 421.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123861BL

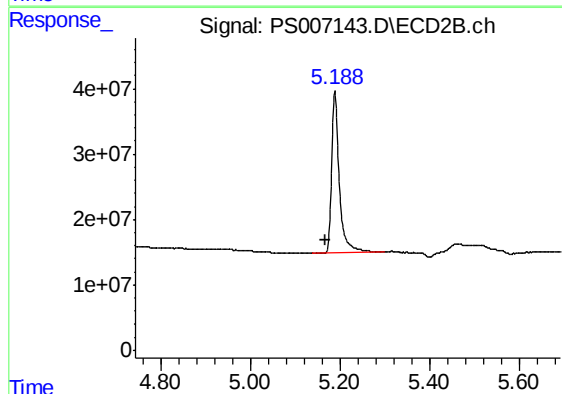


#4 2,4-DCAA

R.T.: 5.189 min
Delta R.T.: 0.020 min
Response: 298044708
Conc: 423.78 ng/ml

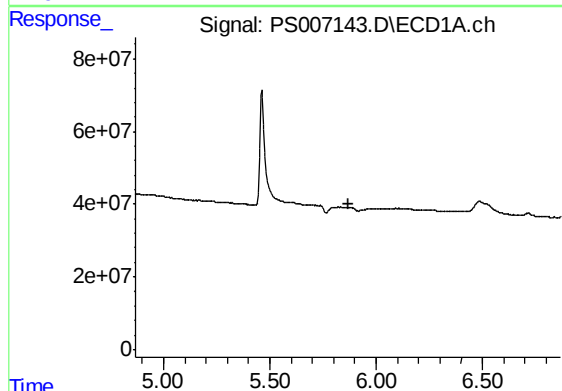


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

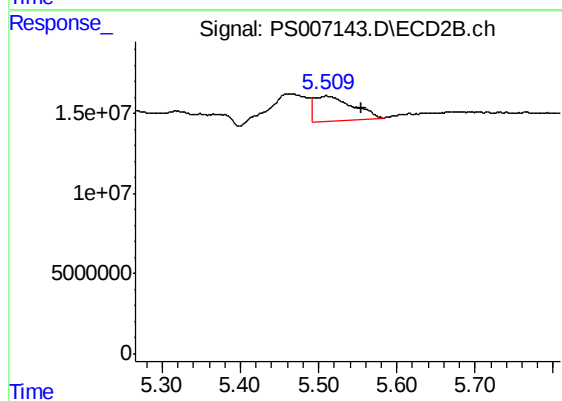

#7 MCPA


R.T.: 5.511 min
Delta R.T.: -0.044 min
Response: 51202830
Conc: 17.61 ug/ml

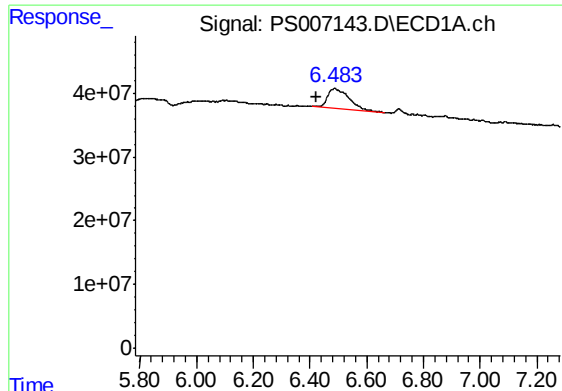

#9 2,4-D


R.T.: 6.485 min
Delta R.T.: 0.061 min
Response: 165110371
Conc: 133.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123861BL

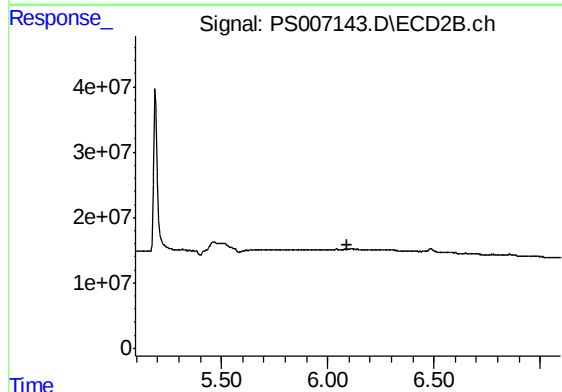


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.095 min
Response: 0
Conc: N.D.

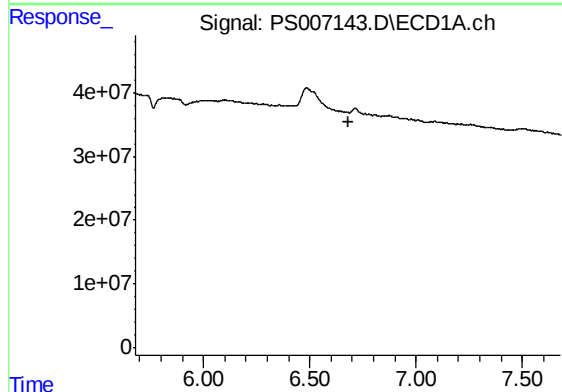


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

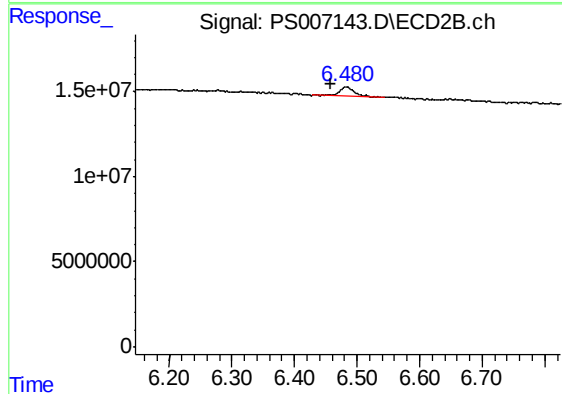

#10 Pentachlorophenol


R.T.: 6.482 min
Delta R.T.: 0.025 min
Response: 9719374
Conc: 1.01 ng/ml

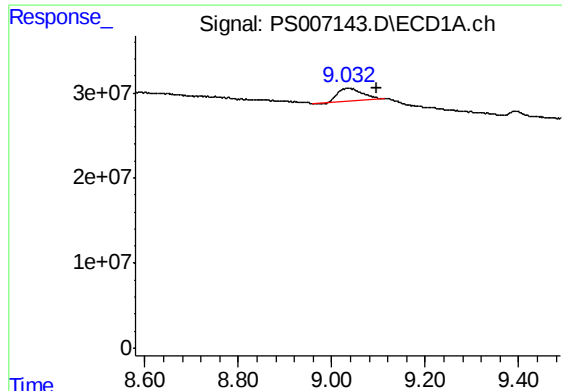

#14 DINOSEB


R.T.: 9.033 min
Delta R.T.: -0.063 min
Response: 53149467
Conc: 9.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB123861BL

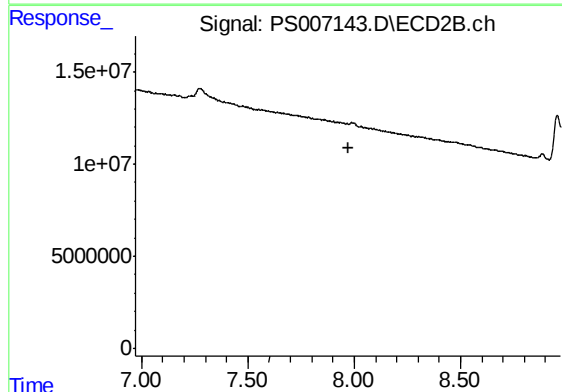


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 7.971 min
Response: 0
Conc: N.D.

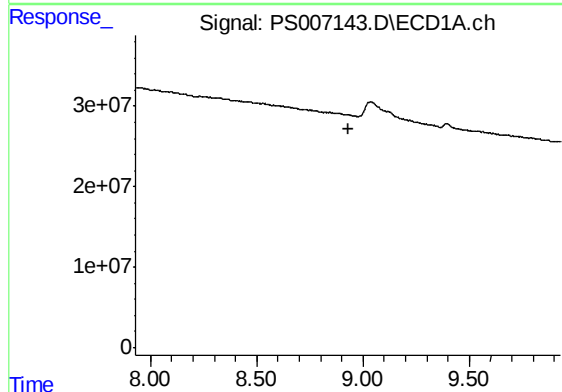

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

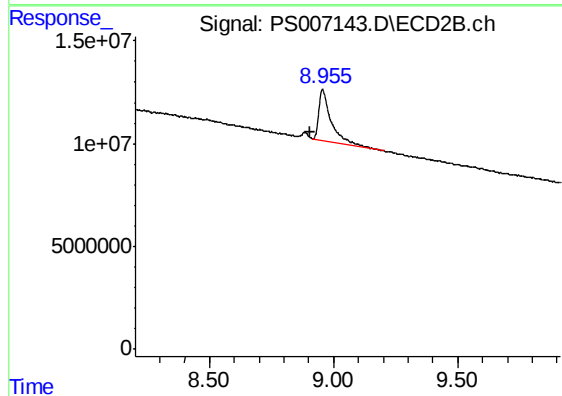

#15 Picloram

R.T.: 8.955 min
Delta R.T.: 0.050 min
Response: 85869684
Conc: 13.98 ng/ml