

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
 Data File : PS007146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 12:12
 Operator : SM\AJ
 Sample : K5325-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 10-10-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 13:15:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.439	5.173	613.7E6	298.3E6	448.364	424.105
Target Compounds							
1) T	Dalapon	1.993	1.703	239.6E6	384.9E6	143.221	422.960 #
2) T	3,5-DICHL...	0.000	4.505	0	75664509	N.D.	87.938
3) T	4-Nitroph...	5.249	0.000	176.0E6	0	293.037	N.D. #
5) T	DICAMBA	5.604	5.296	23808794	15787534	4.846	6.067 #
7) T	MCPA	0.000	5.545	0	18705751	N.D.	6.434
9) T	2,4-D	0.000	6.082	0	20002097	N.D.	25.072
10) T	Pentachlo...	0.000	6.471	0	15903309	N.D.	1.654
11) T	2,4,5-TP ...	0.000	6.776	0	56367564	N.D.	14.819
13) T	2,4-DB	8.020	0.000	25949650	0	27.216	N.D. #
14) T	DINOSEB	0.000	7.969	0	6480643	N.D.	2.308
15) T	Picloram	0.000	8.935	0	48730201	N.D.	7.936



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
Data File : PS007146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 12:12
Operator : SM\AJ
Sample : K5325-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
10-10-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 13:15:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

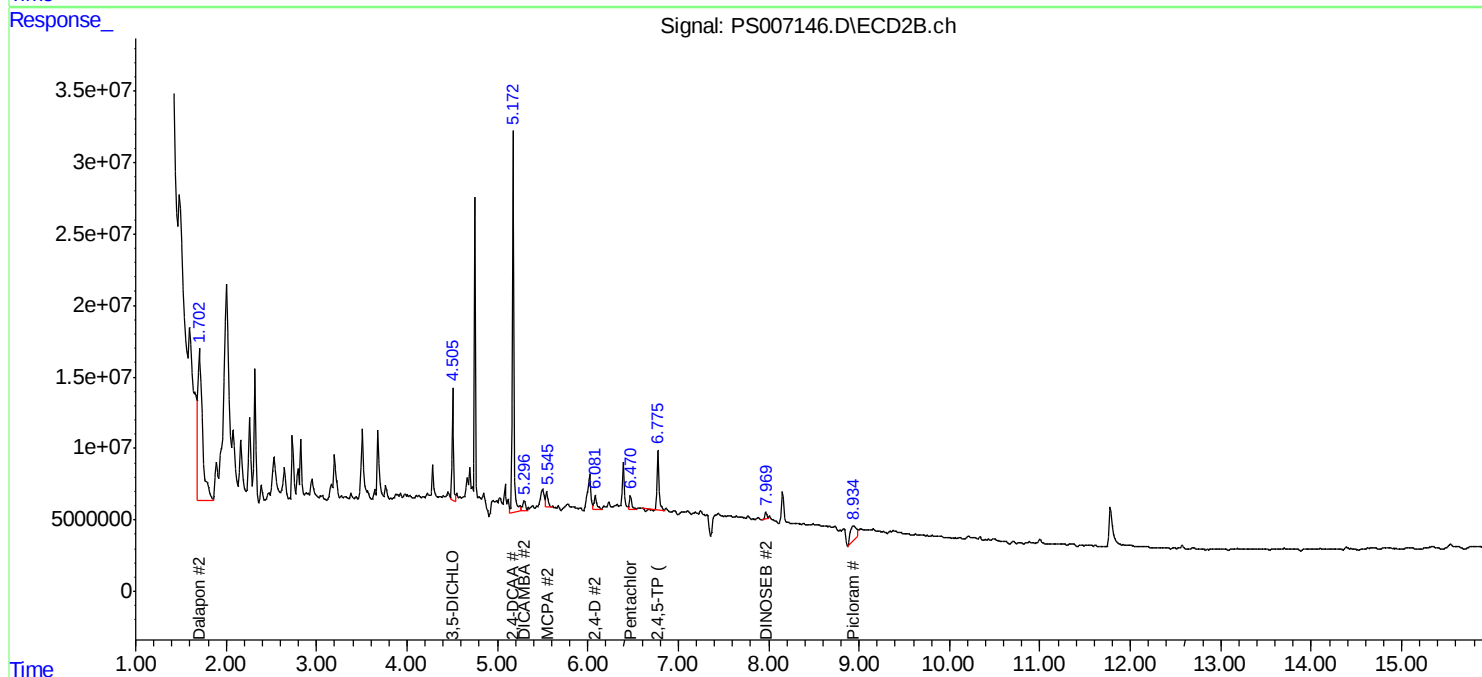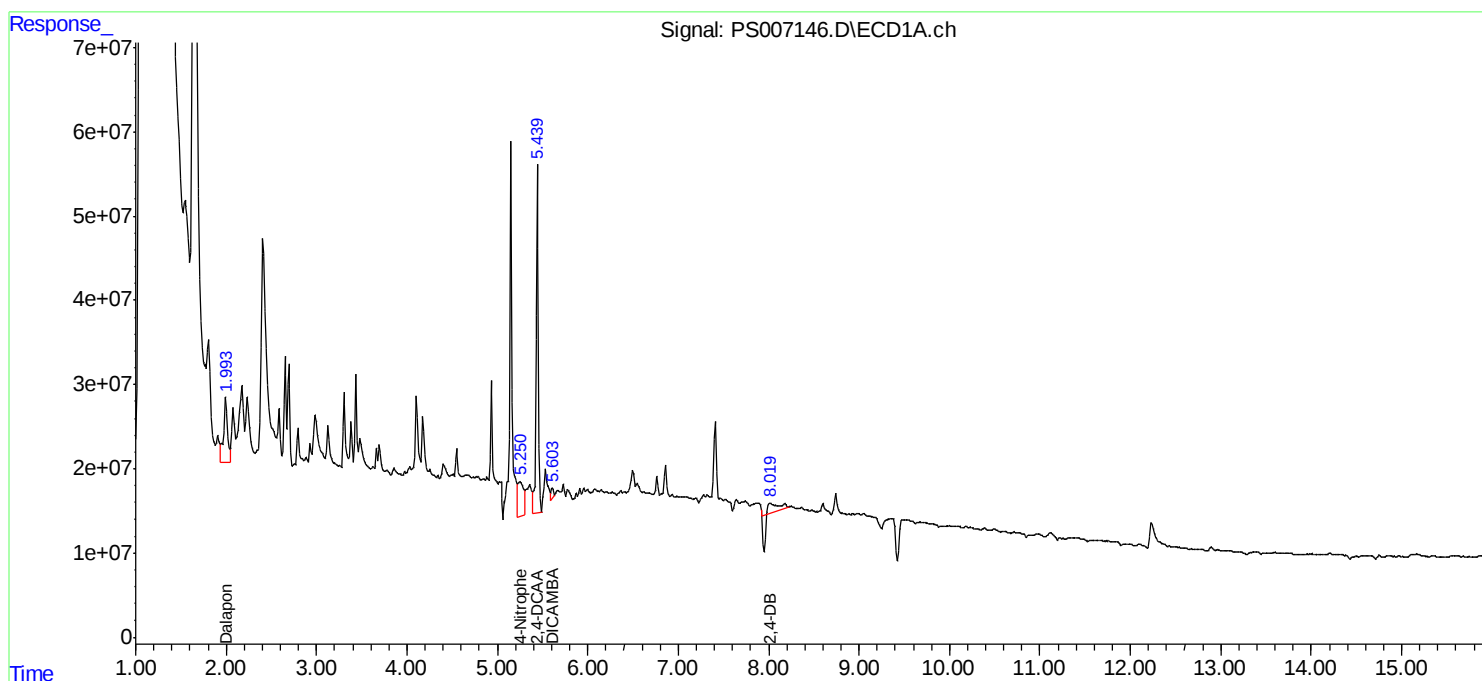


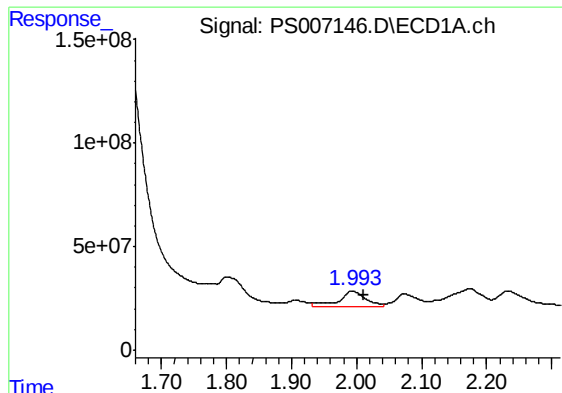

#1 Dalapon


R.T.: 1.993 min
Delta R.T.: -0.018 min
Response: 239648521
Conc: 143.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-A

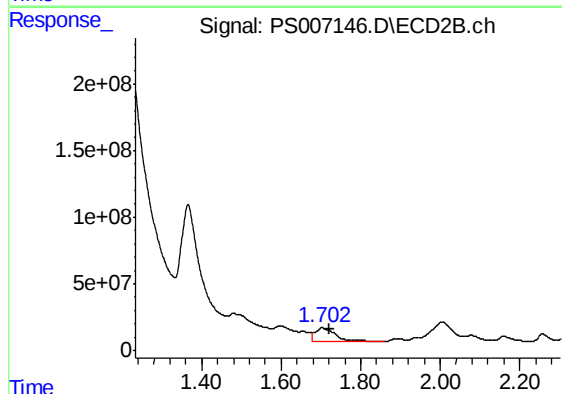


#1 Dalapon

R.T.: 1.703 min
Delta R.T.: -0.018 min
Response: 384894698
Conc: 422.96 ng/ml

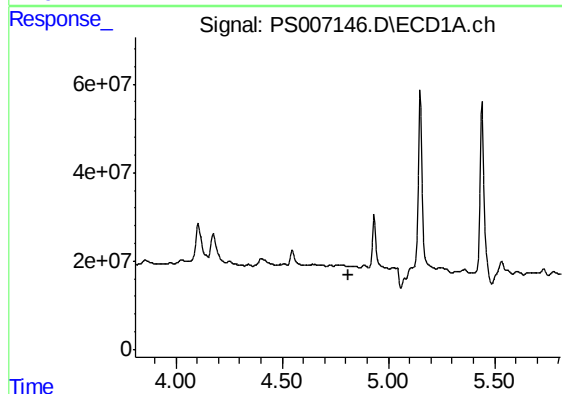


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

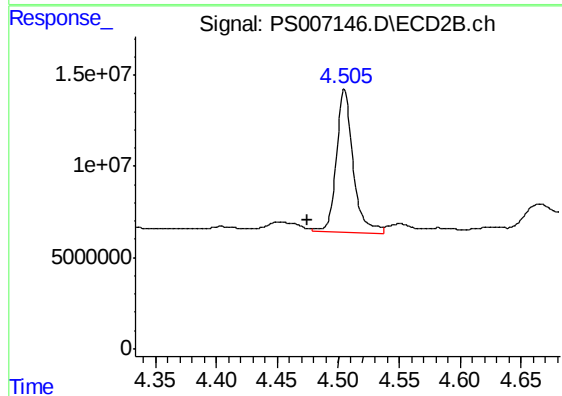

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.505 min
Delta R.T.: 0.030 min
Response: 75664509
Conc: 87.94 ng/ml

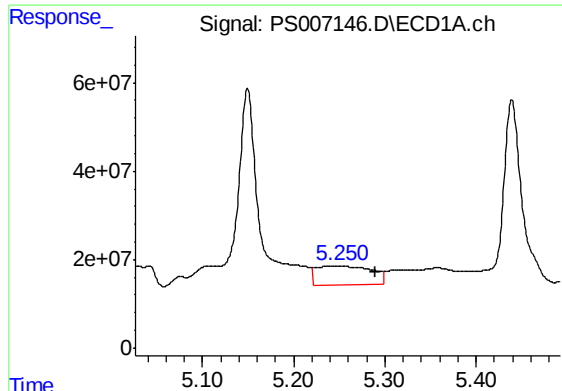

#3 4-Nitrophenol


R.T.: 5.249 min
Delta R.T.: -0.041 min
Response: 175961087
Conc: 293.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-A

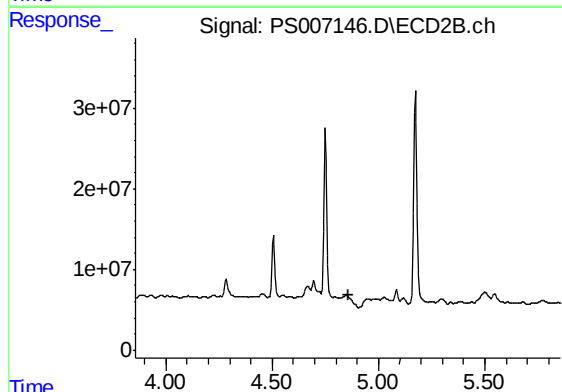


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

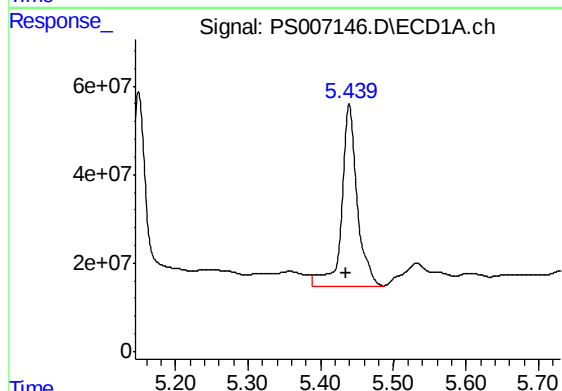


#4 2,4-DCAA

R.T.: 5.439 min
Delta R.T.: 0.004 min
Response: 613662291
Conc: 448.36 ng/ml

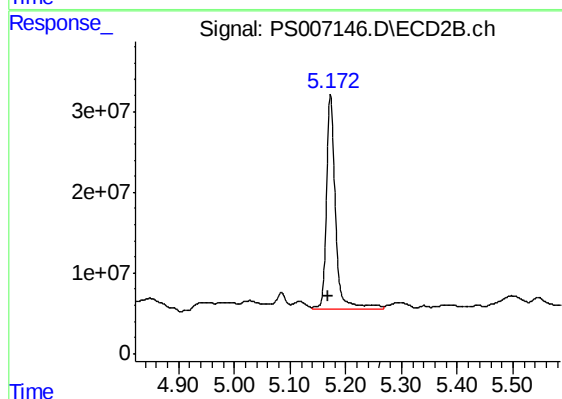

#4 2,4-DCAA


R.T.: 5.173 min
Delta R.T.: 0.004 min
Response: 298275935
Conc: 424.11 ng/ml

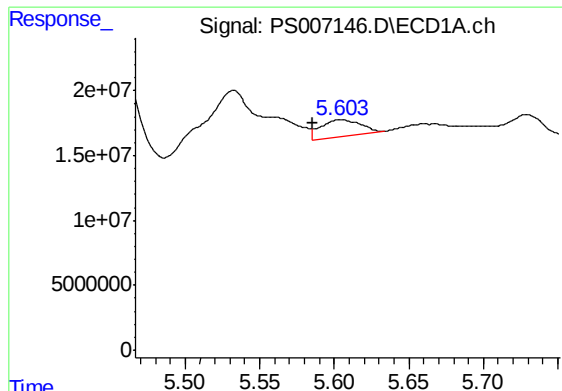

#5 DICAMBA


R.T.: 5.604 min
Delta R.T.: 0.019 min
Response: 23808794
Conc: 4.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-A

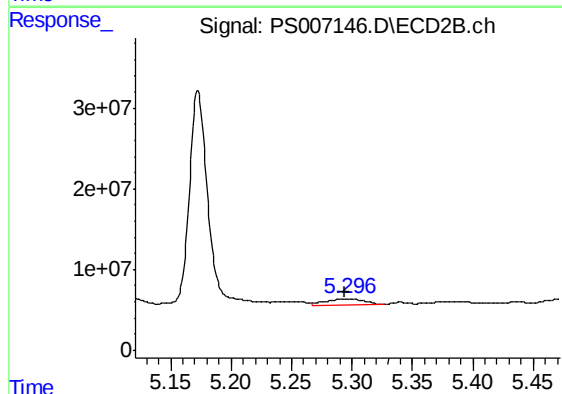


#5 DICAMBA

R.T.: 5.296 min
Delta R.T.: 0.002 min
Response: 15787534
Conc: 6.07 ng/ml

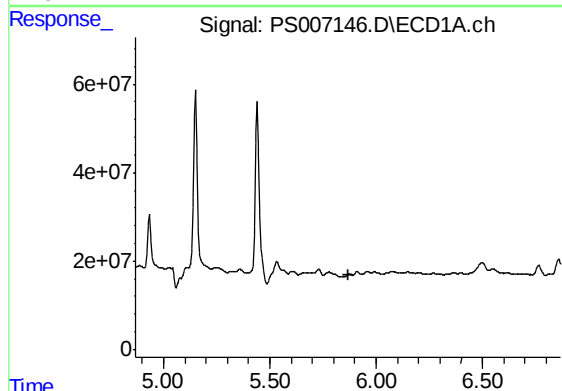


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

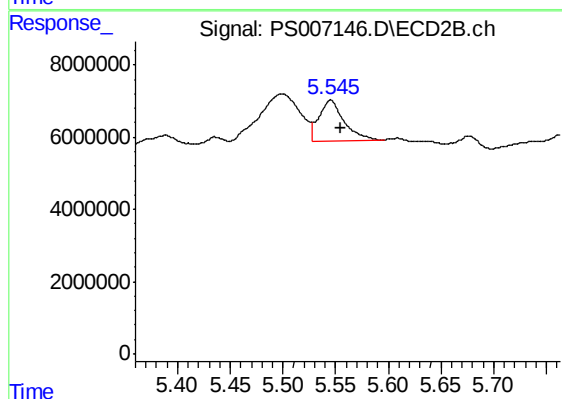

#7 MCPA


R.T.: 5.545 min
Delta R.T.: -0.010 min
Response: 18705751
Conc: 6.43 ug/ml

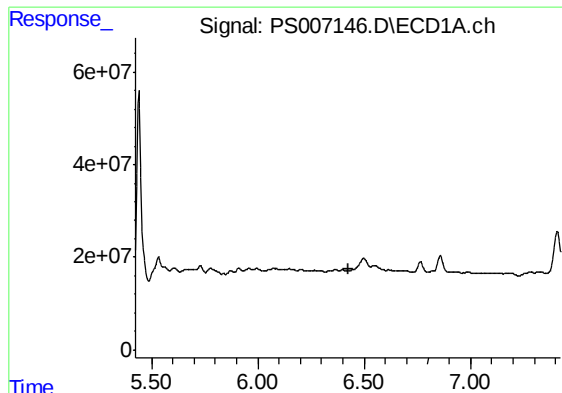

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-A

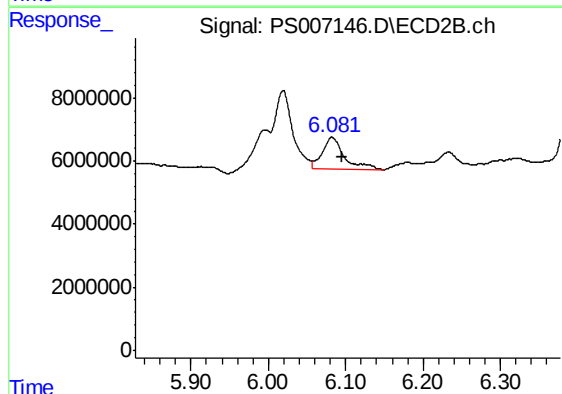


#9 2,4-D

R.T.: 6.082 min
Delta R.T.: -0.013 min
Response: 20002097
Conc: 25.07 ng/ml

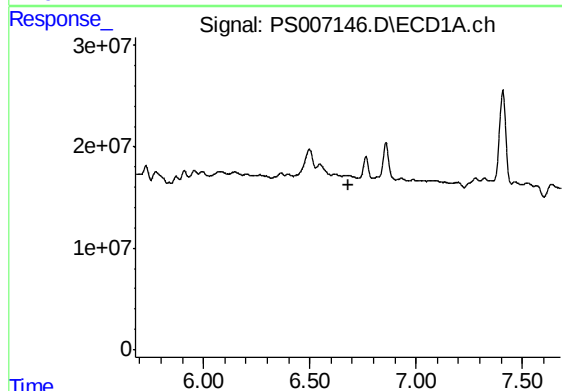


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

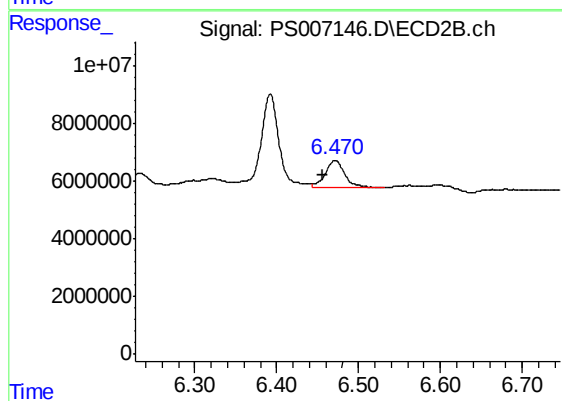

#10 Pentachlorophenol


R.T.: 6.471 min
Delta R.T.: 0.014 min
Response: 15903309
Conc: 1.65 ng/ml

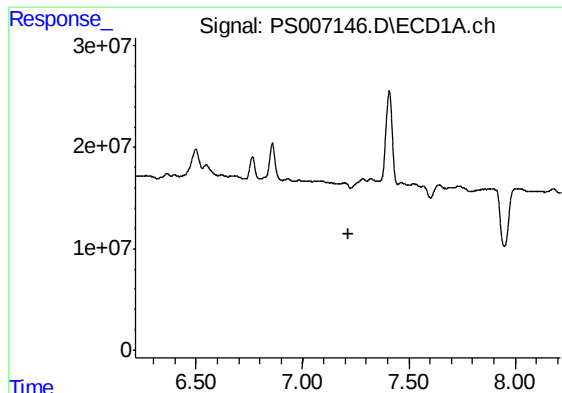

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-A

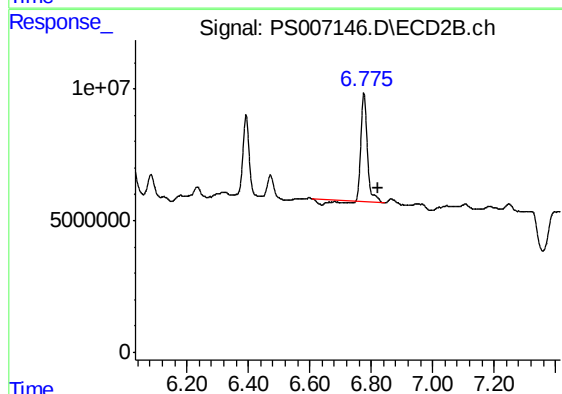


#11 2,4,5-TP (SILVEX)

R.T.: 6.776 min
Delta R.T.: -0.045 min
Response: 56367564
Conc: 14.82 ng/ml

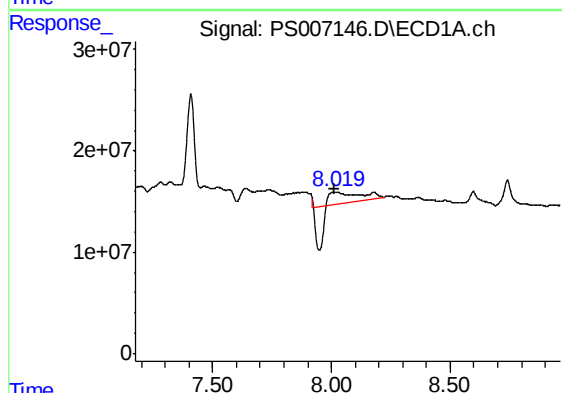


#13 2,4-DB

R.T.: 8.020 min
Delta R.T.: 0.007 min
Response: 25949650
Conc: 27.22 ng/ml

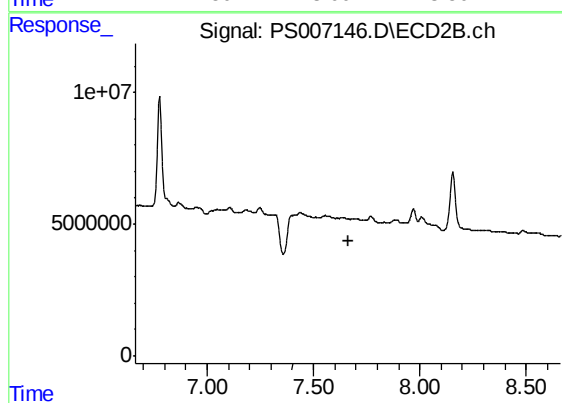

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 7.662 min
Response: 0
Conc: N.D.

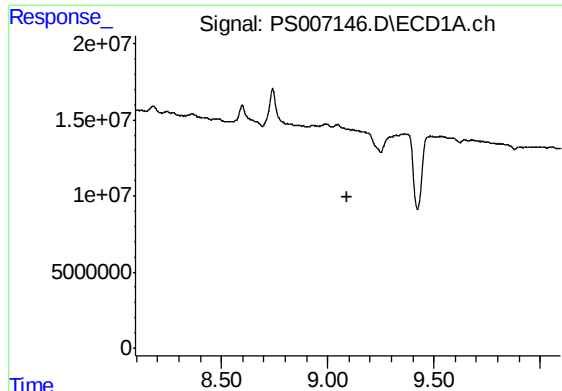

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-A

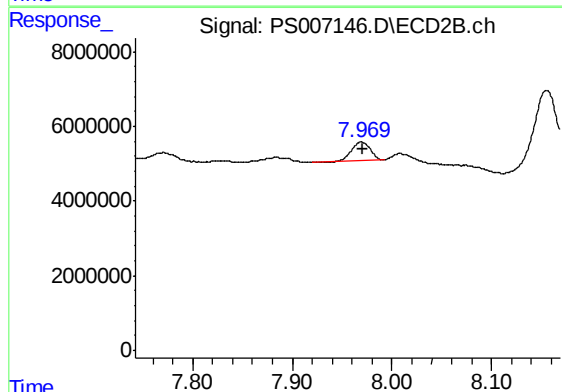


#14 DINOSEB

R.T.: 7.969 min
Delta R.T.: -0.001 min
Response: 6480643
Conc: 2.31 ng/ml

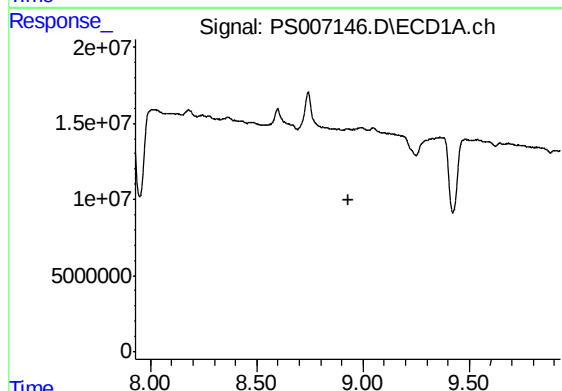

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

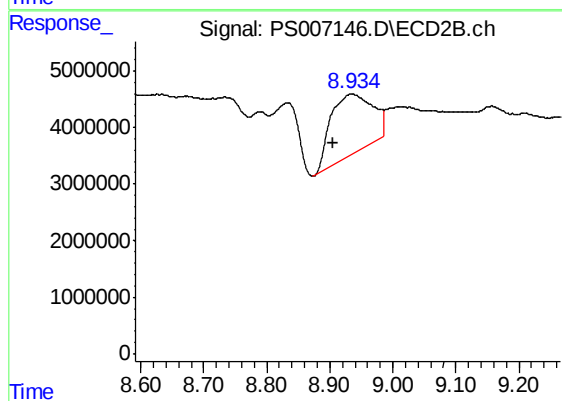

#15 Picloram

R.T.: 8.935 min
Delta R.T.: 0.030 min
Response: 48730201
Conc: 7.94 ng/ml