

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
 Data File : PS007150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 13:40
 Operator : SM\AJ
 Sample : K5325-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 10-10-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 15:32:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.436	5.169	526.9E6	309.1E6	384.940	439.557
Target Compounds							
1) T	Dalapon	1.990	1.699	222.0E6	265.4E6	132.660	291.627 #
2) T	3,5-DICHL...	0.000	4.502	0	44250742	N.D.	51.429
5) T	DICAMBA	5.599	5.294	23087260	21458551	4.699	8.247 #
7) T	MCPA	0.000	5.541	0	20198547	N.D.	6.948
9) T	2,4-D	6.492	6.079	73308761	22586645	59.487	28.311 #
10) T	Pentachlo...	0.000	6.466	0	17359166	N.D.	1.805
11) T	2,4,5-TP ...	0.000	6.860	0	6079716	N.D.	1.598
15) T	Picloram	0.000	8.932	0	38866097	N.D.	6.330
16) T	DCPA	9.366	8.830	212.0E6	28124888	23.679	5.609 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
Data File : PS007150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 13:40
Operator : SM\AJ
Sample : K5325-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
10-10-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 15:32:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

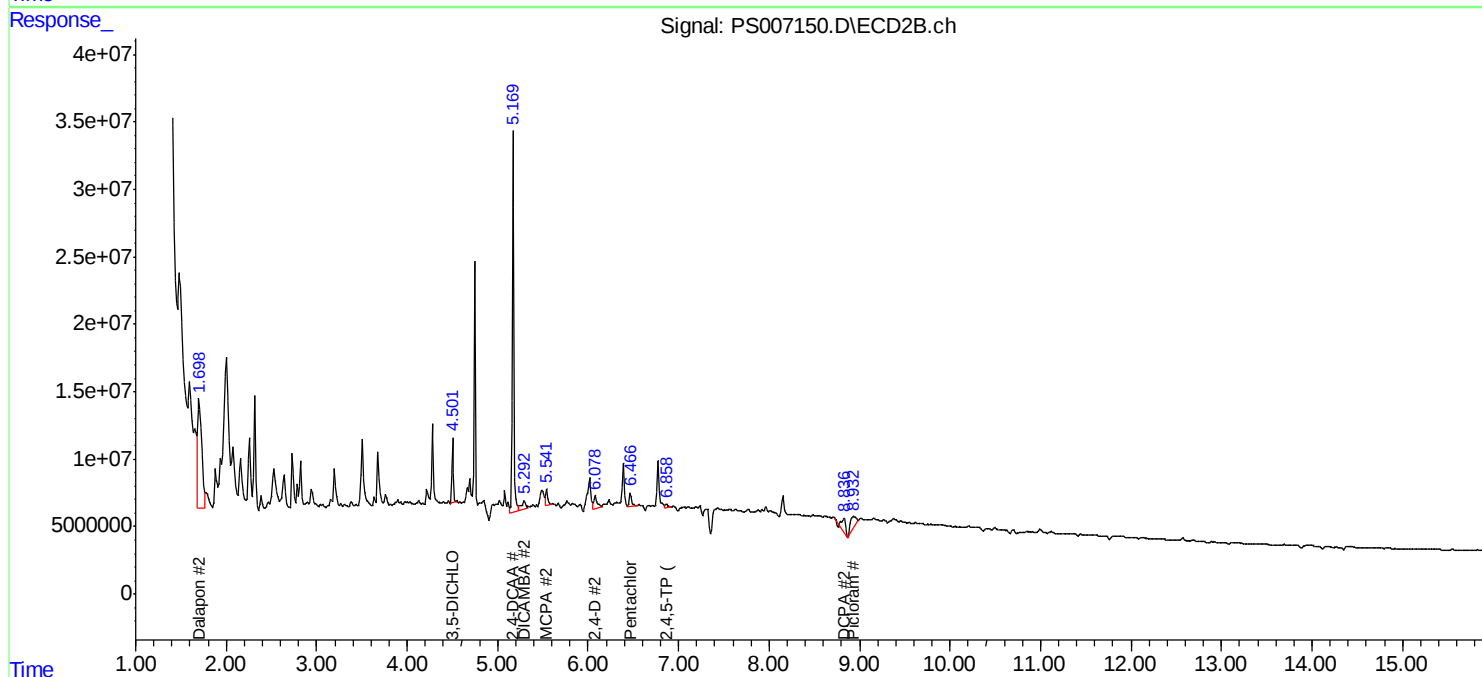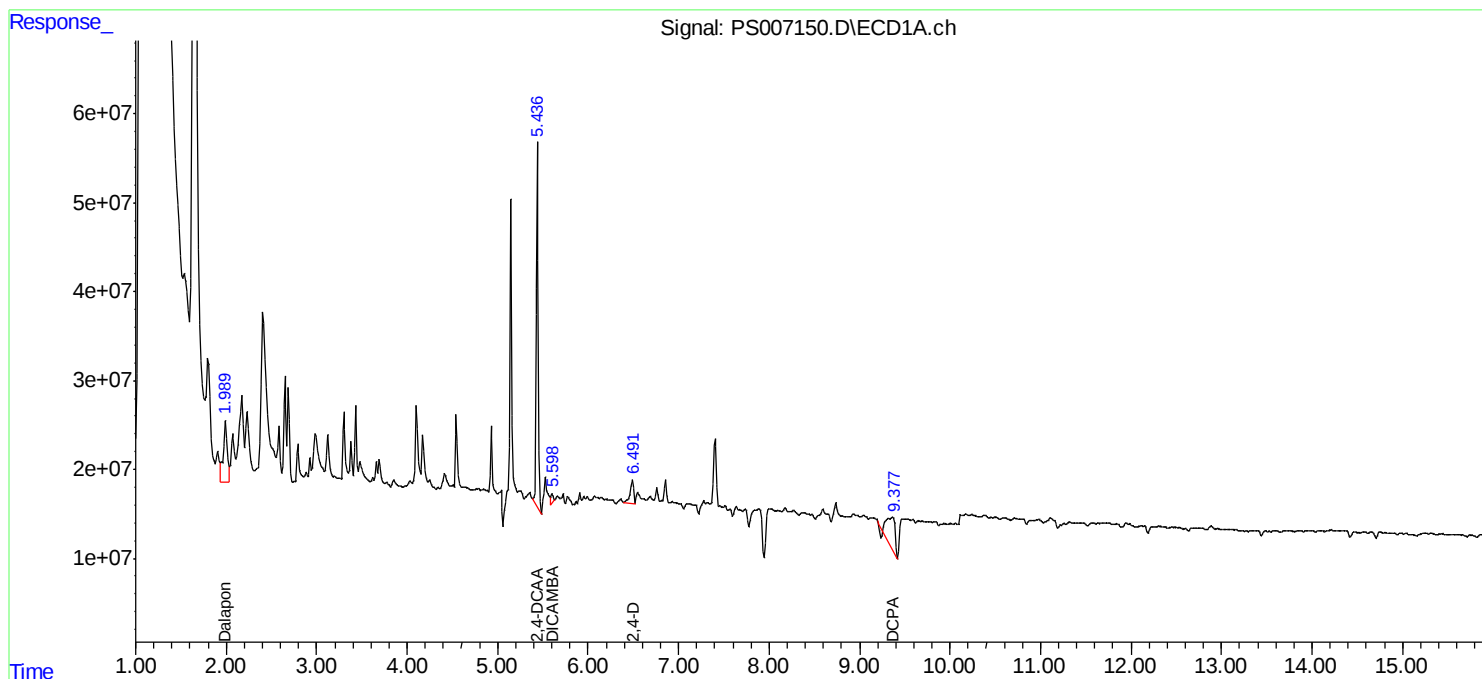


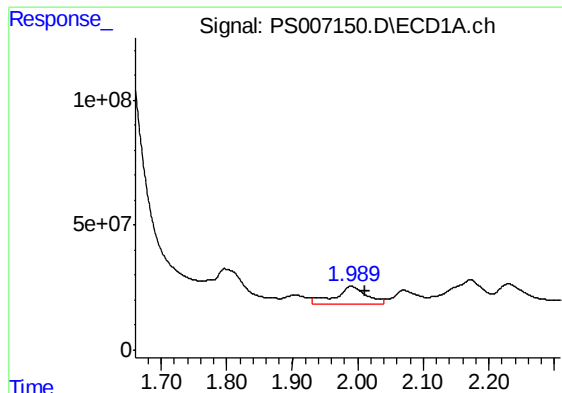

#1 Dalapon


R.T.: 1.990 min
Delta R.T.: -0.021 min
Response: 221977471
Conc: 132.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-C

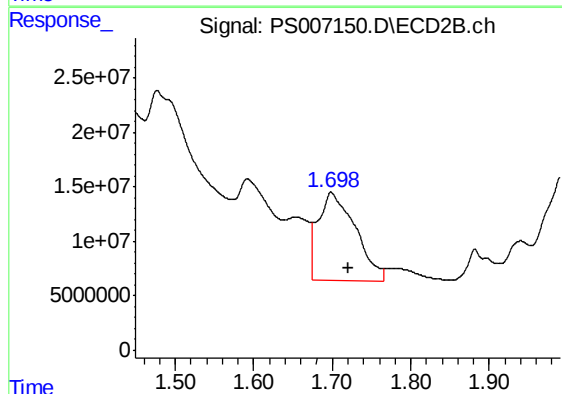


#1 Dalapon

R.T.: 1.699 min
Delta R.T.: -0.021 min
Response: 265381159
Conc: 291.63 ng/ml

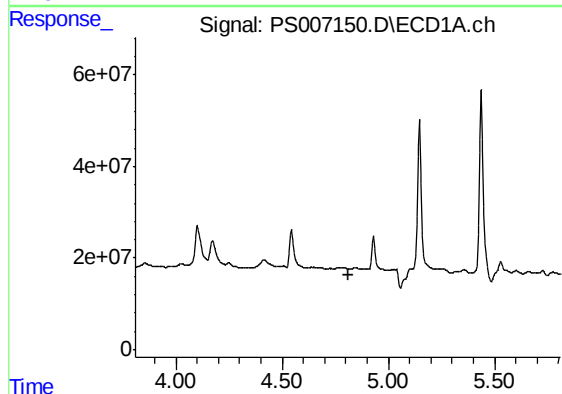


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

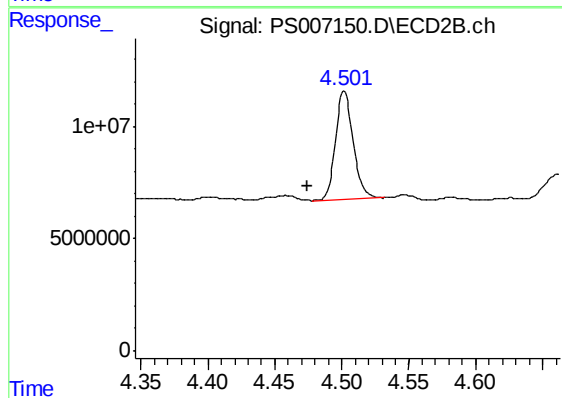

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.502 min
Delta R.T.: 0.027 min
Response: 44250742
Conc: 51.43 ng/ml

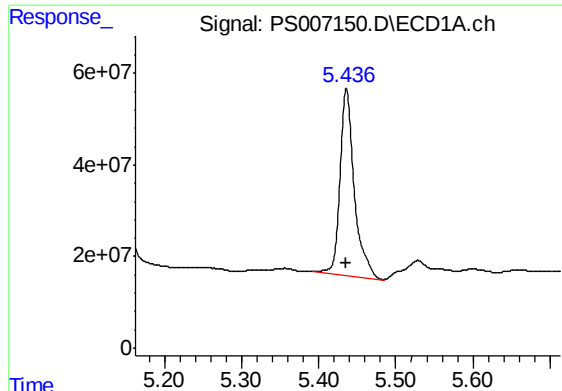

#4 2,4-DCAA


R.T.: 5.436 min
Delta R.T.: 0.000 min
Response: 526854758
Conc: 384.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-C

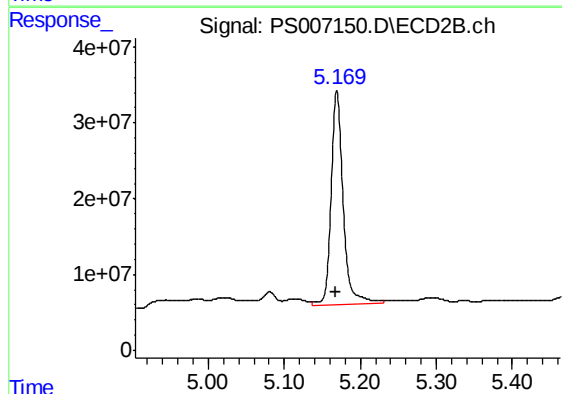


#4 2,4-DCAA

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 309143236
Conc: 439.56 ng/ml

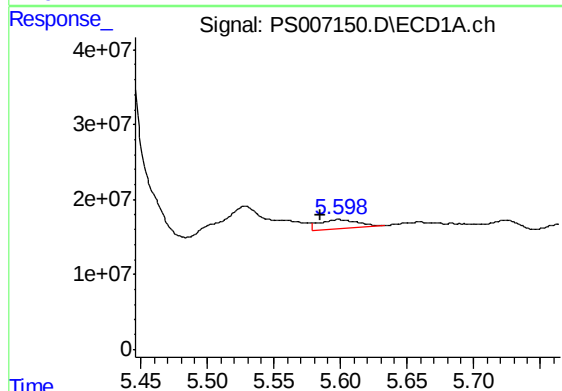


#5 DICAMBA

R.T.: 5.599 min
Delta R.T.: 0.013 min
Response: 23087260
Conc: 4.70 ng/ml

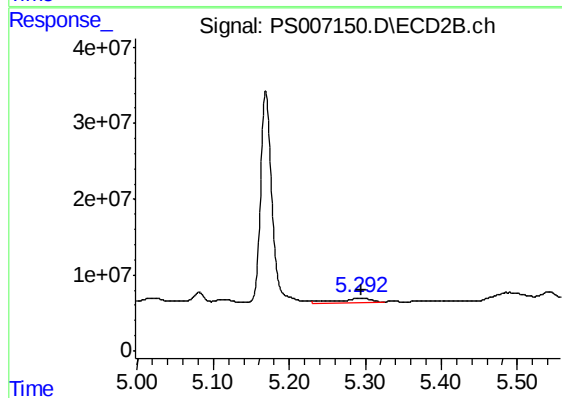

#5 DICAMBA


R.T.: 5.294 min
Delta R.T.: 0.000 min
Response: 21458551
Conc: 8.25 ng/ml

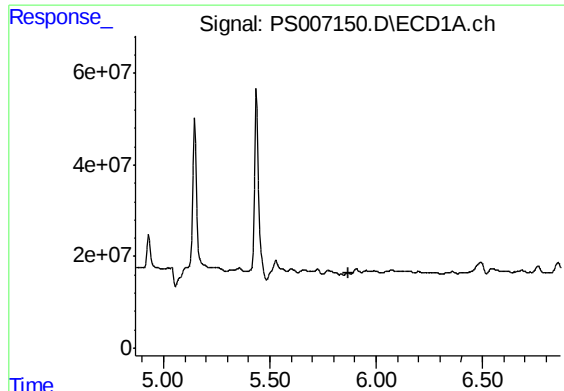

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-C

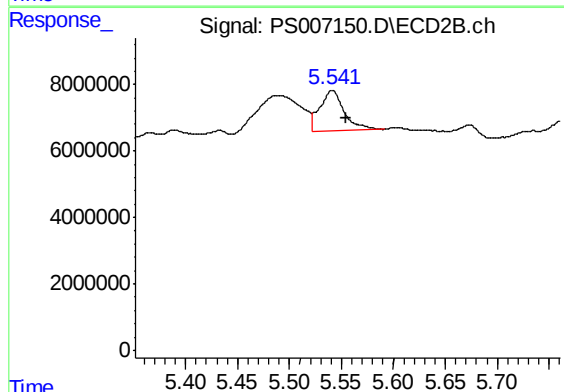


#7 MCPA

R.T.: 5.541 min
Delta R.T.: -0.014 min
Response: 20198547
Conc: 6.95 ug/ml

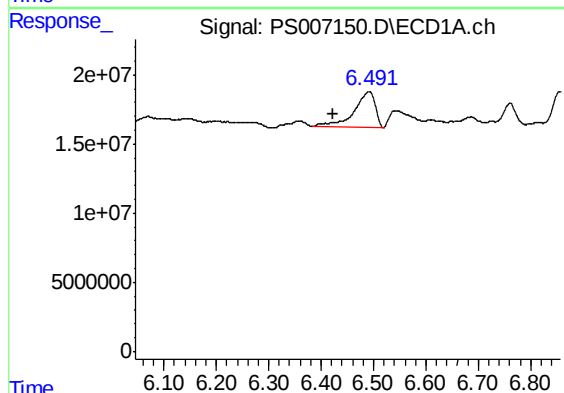


#9 2,4-D

R.T.: 6.492 min
Delta R.T.: 0.068 min
Response: 73308761
Conc: 59.49 ng/ml

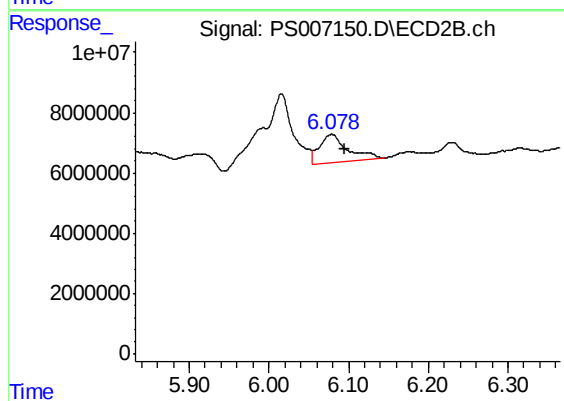

#9 2,4-D


R.T.: 6.079 min
Delta R.T.: -0.017 min
Response: 22586645
Conc: 28.31 ng/ml

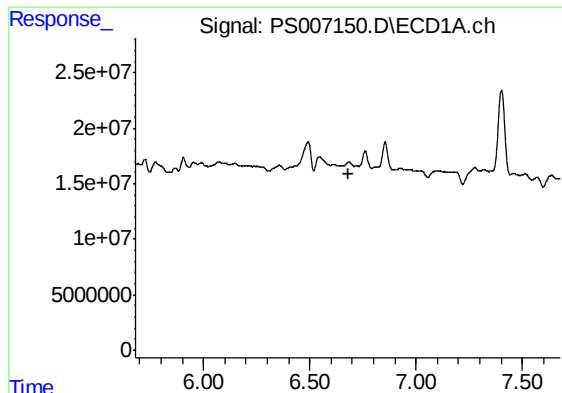

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-C

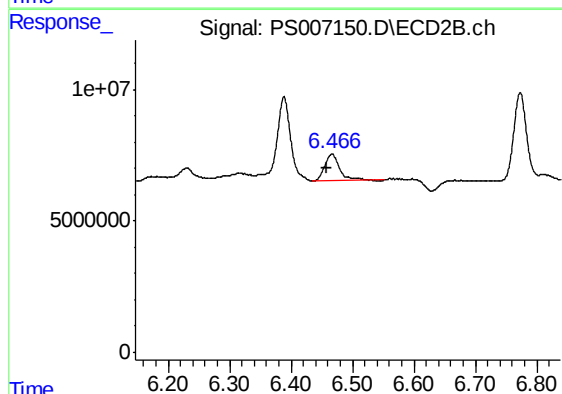


#10 Pentachlorophenol

R.T.: 6.466 min
Delta R.T.: 0.009 min
Response: 17359166
Conc: 1.81 ng/ml

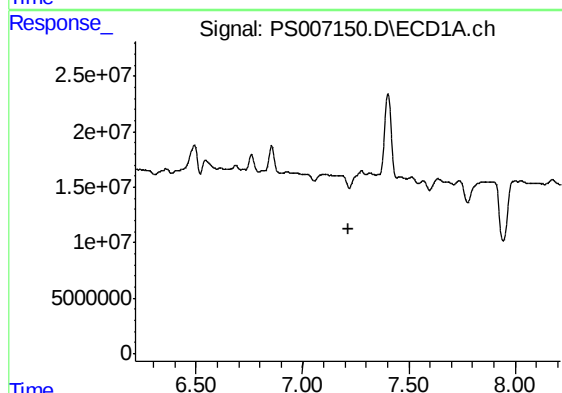


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.214 min
Response: 0
Conc: N.D.

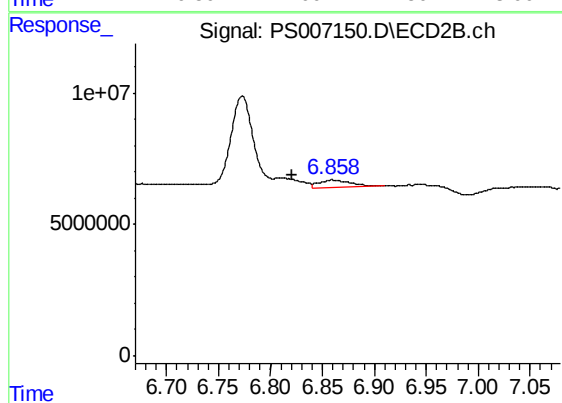

#11 2,4,5-TP (SILVEX)


R.T.: 6.860 min
Delta R.T.: 0.039 min
Response: 6079716
Conc: 1.60 ng/ml

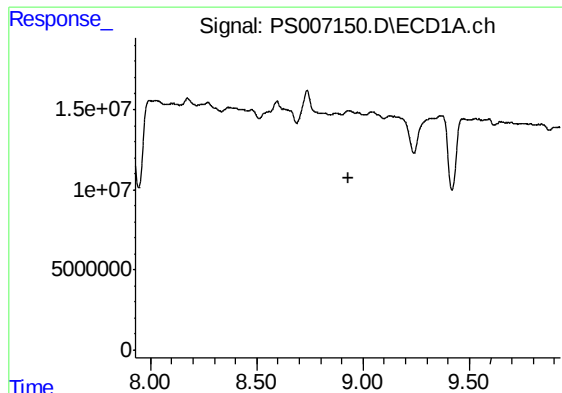

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-C

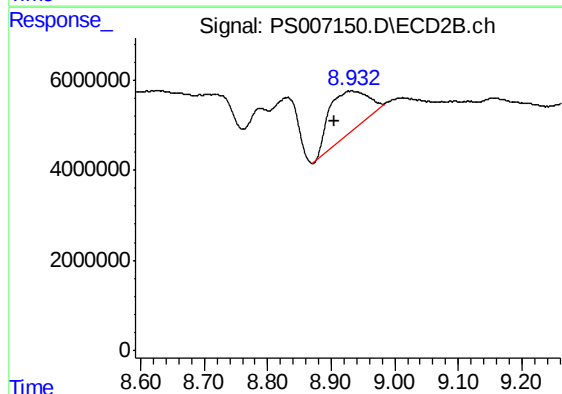


#15 Picloram

R.T.: 8.932 min
Delta R.T.: 0.027 min
Response: 38866097
Conc: 6.33 ng/ml

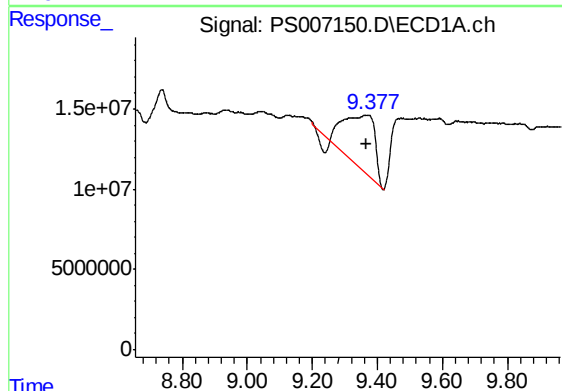

#16 DCPA

R.T.: 9.366 min
Delta R.T.: -0.001 min
Response: 212033126
Conc: 23.68 ng/ml

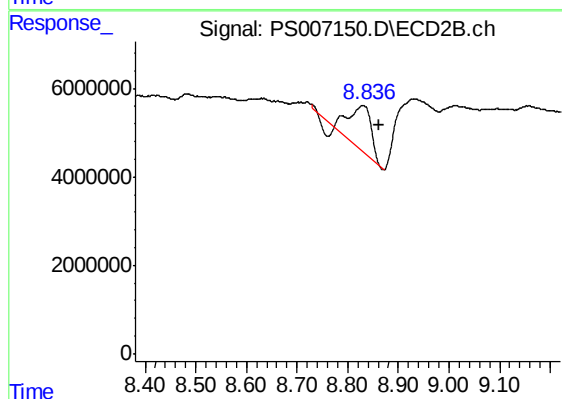

#16 DCPA

R.T.: 8.830 min
Delta R.T.: -0.033 min
Response: 28124888
Conc: 5.61 ng/ml