

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
 Data File : PS007151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 14:02
 Operator : SM\AJ
 Sample : K5325-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 10-10-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 15:32:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.441	5.174	481.9E6	285.2E6	352.117	405.548
Target Compounds							
1) T	Dalapon	1.994	1.704	121.6E6	195.8E6	72.694	215.178 #
2) T	3,5-DICHL...	0.000	4.507	0	36649766	N.D.	42.595
5) T	DICAMBA	5.532	0.000	93189593	0	18.966	N.D. #
7) T	MCPA	0.000	5.546	0	19672249	N.D.	6.767
9) T	2,4-D	0.000	6.082	0	24016768	N.D.	30.104
10) T	Pentachlo...	0.000	6.473	0	13751462	N.D.	1.430
11) T	2,4,5-TP ...	0.000	6.777	0	39107324	N.D.	10.282
15) T	Picloram	0.000	8.941	0	37617330	N.D.	6.126



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
Data File : PS007151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 14:02
Operator : SM\AJ
Sample : K5325-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
10-10-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 15:32:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

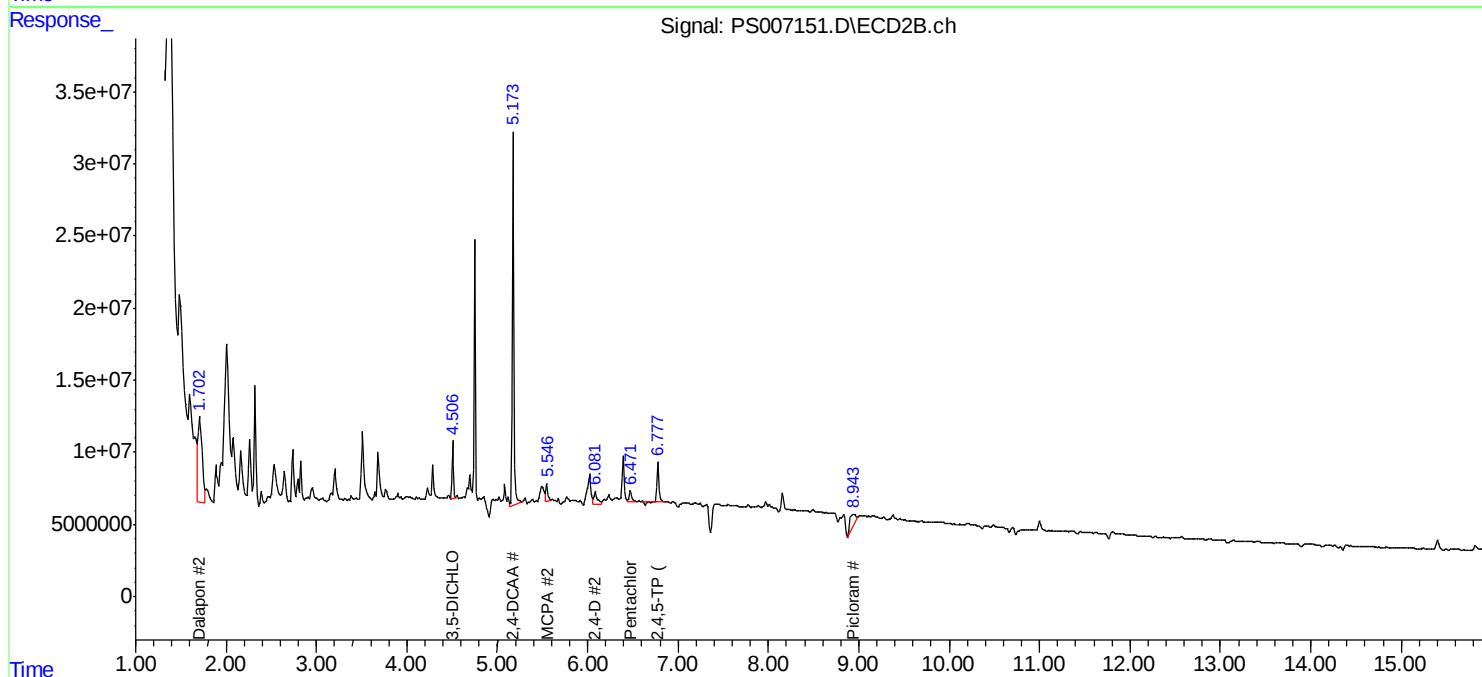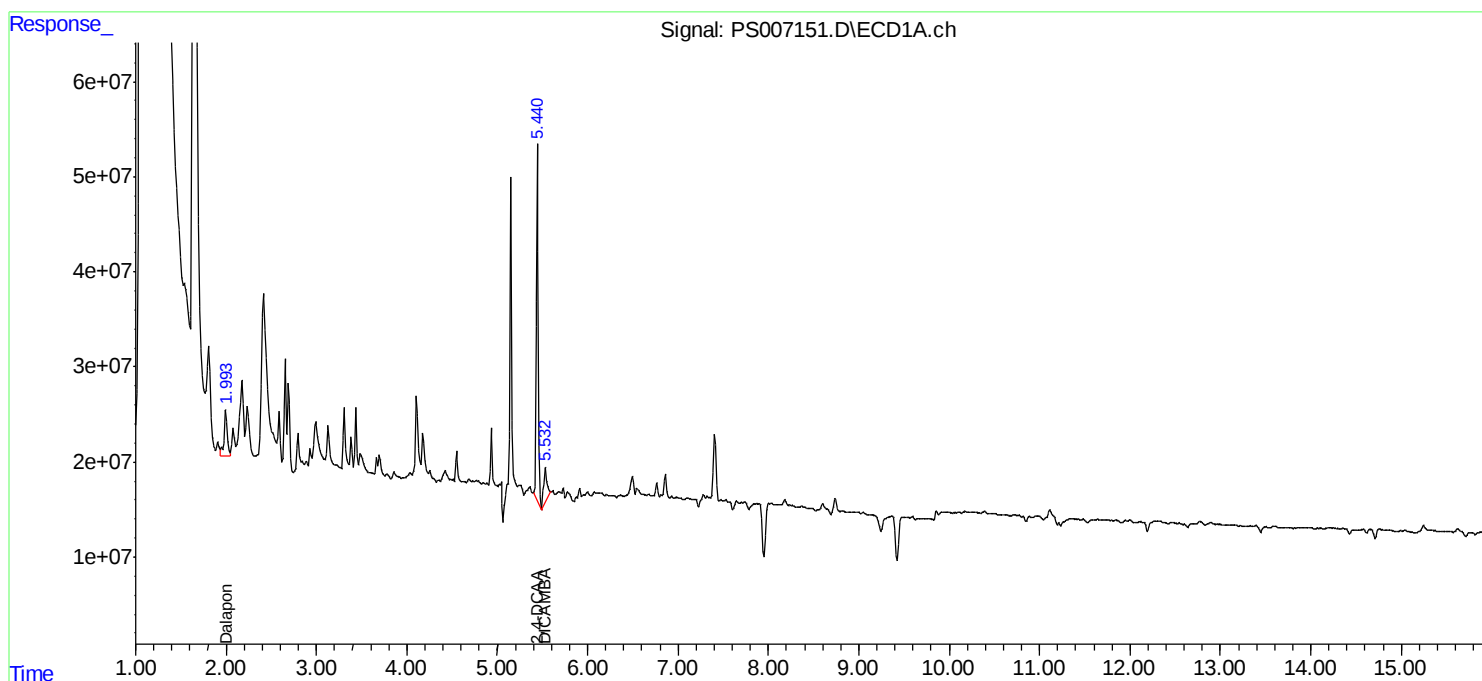


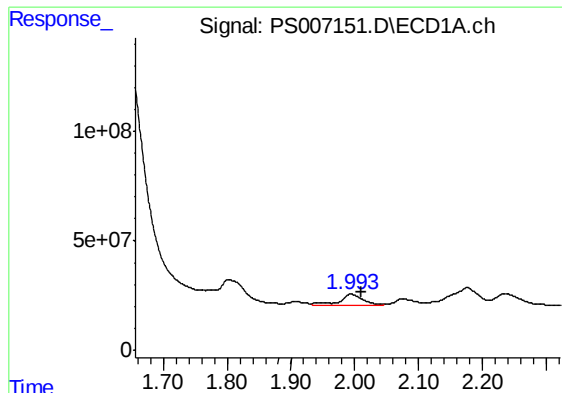

#1 Dalapon


R.T.: 1.994 min
Delta R.T.: -0.017 min
Response: 121637129
Conc: 72.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-D

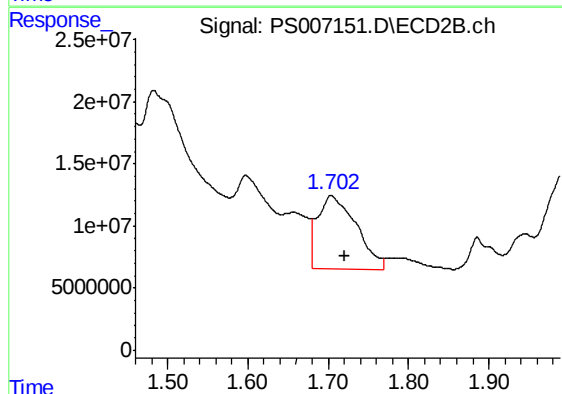


#1 Dalapon

R.T.: 1.704 min
Delta R.T.: -0.017 min
Response: 195812503
Conc: 215.18 ng/ml

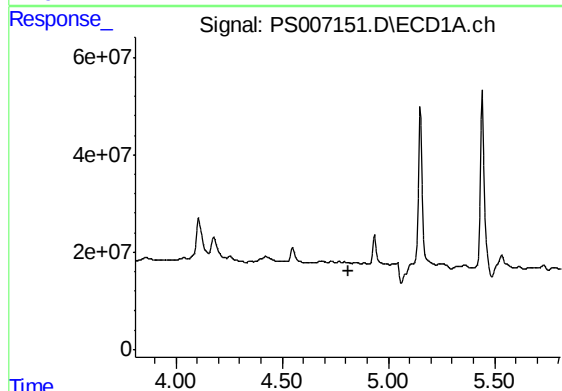


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

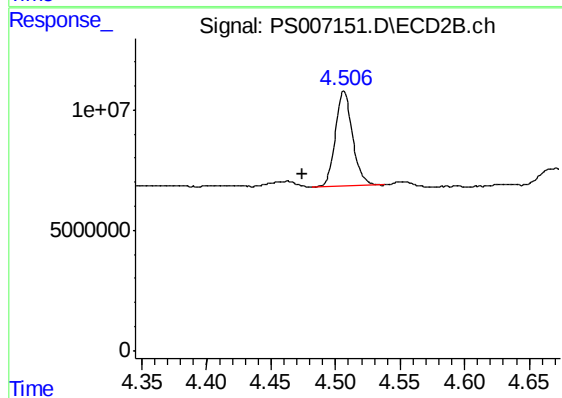

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.507 min
Delta R.T.: 0.032 min
Response: 36649766
Conc: 42.59 ng/ml

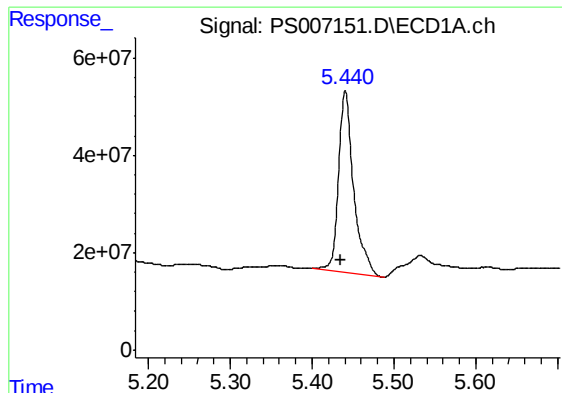

#4 2,4-DCAA


R.T.: 5.441 min
Delta R.T.: 0.005 min
Response: 481931979
Conc: 352.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-D

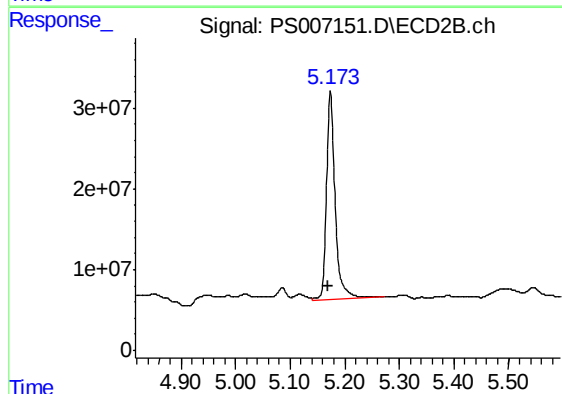


#4 2,4-DCAA

R.T.: 5.174 min
Delta R.T.: 0.005 min
Response: 285224443
Conc: 405.55 ng/ml

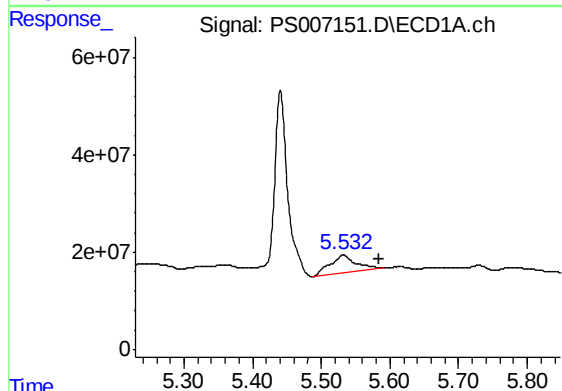


#5 DICAMBA

R.T.: 5.532 min
Delta R.T.: -0.053 min
Response: 93189593
Conc: 18.97 ng/ml

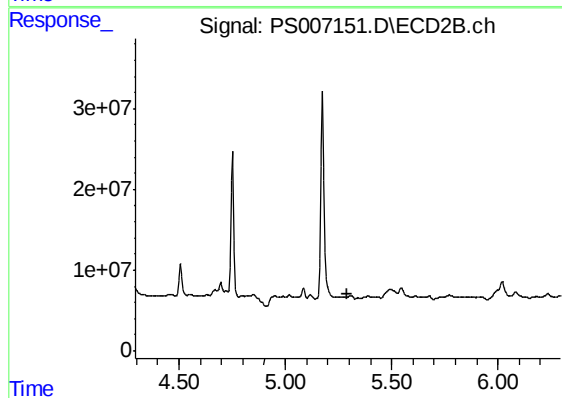

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

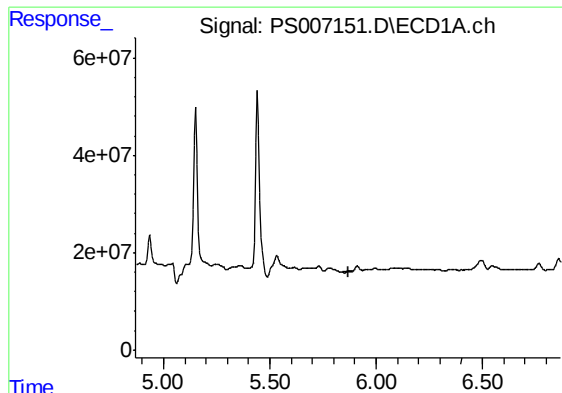

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-D

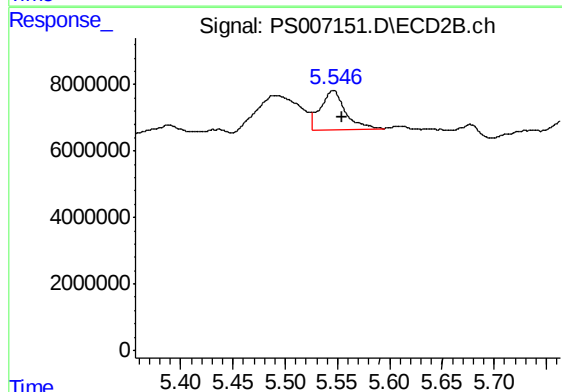


#7 MCPA

R.T.: 5.546 min
Delta R.T.: -0.009 min
Response: 19672249
Conc: 6.77 ug/ml

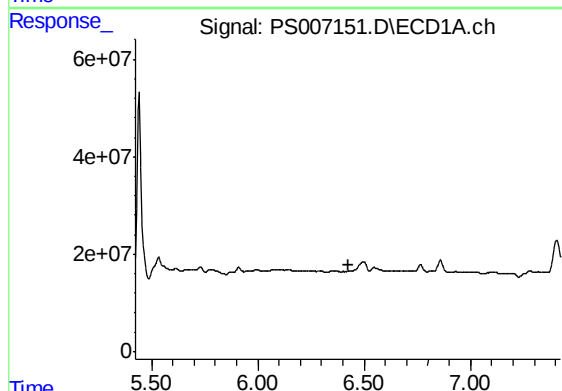


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

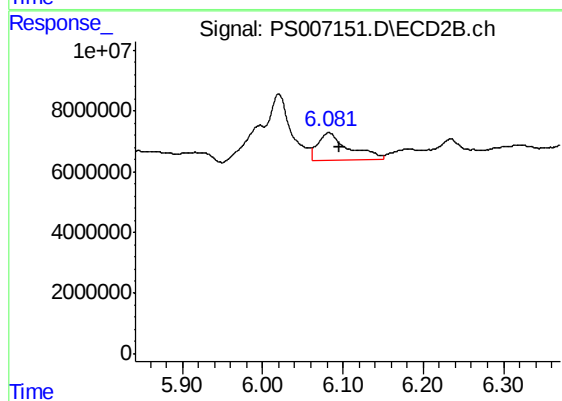

#9 2,4-D


R.T.: 6.082 min
Delta R.T.: -0.013 min
Response: 24016768
Conc: 30.10 ng/ml

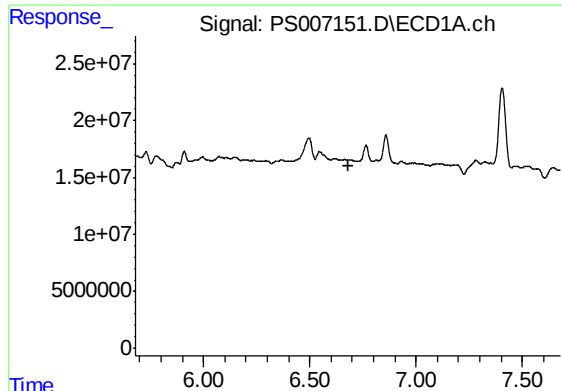

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-D

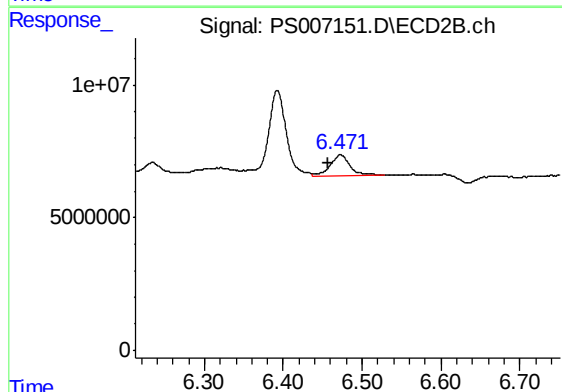


#10 Pentachlorophenol

R.T.: 6.473 min
Delta R.T.: 0.015 min
Response: 13751462
Conc: 1.43 ng/ml

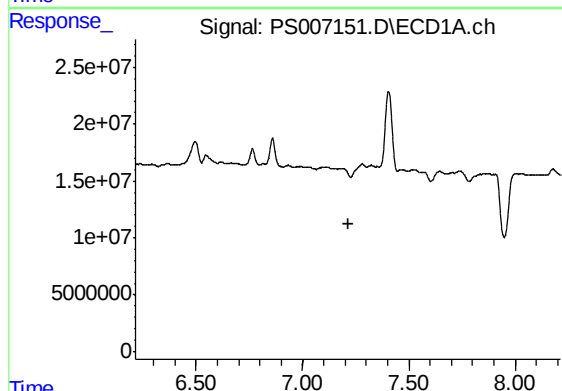


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

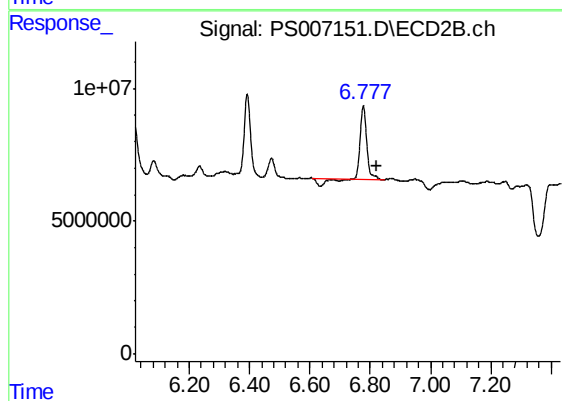

#11 2,4,5-TP (SILVEX)


R.T.: 6.777 min
Delta R.T.: -0.043 min
Response: 39107324
Conc: 10.28 ng/ml

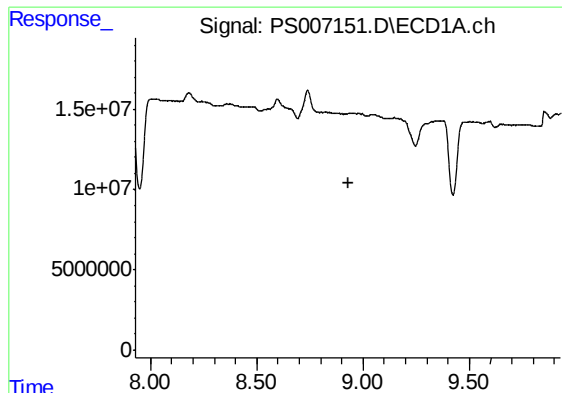

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-D

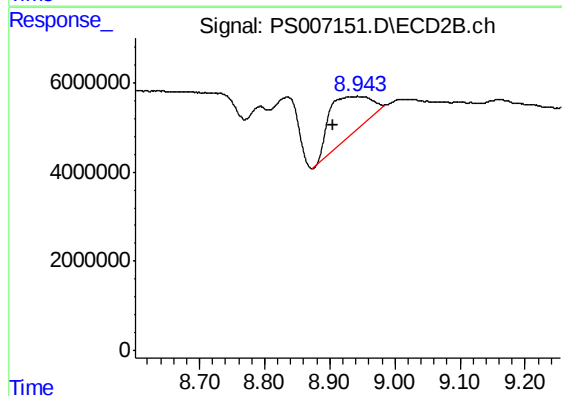

#15 Picloram

R.T.: 8.941 min
Delta R.T.: 0.037 min
Response: 37617330
Conc: 6.13 ng/ml