

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
 Data File : PS007152.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 14:24
 Operator : SM\AJ
 Sample : K5325-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 10-10-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 15:33:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.443	5.170	699.1E6	329.6E6	510.772	468.636
Target Compounds							
1) T	Dalapon	1.996	1.700	119.8E6	317.9E6	71.617	349.325 #
2) T	3,5-DICHL...	0.000	4.502	0	73861159	N.D.	85.842
3) T	4-Nitroph...	5.254	0.000	171.7E6	0	286.015	N.D. #
5) T	DICAMBA	5.616	5.305	19536545	11108060	3.976	4.269
7) T	MCPA	5.912	5.543	23294880	20145695	4.516	6.930 #
9) T	2,4-D	0.000	6.079	0	20943927	N.D.	26.252
10) T	Pentachlo...	0.000	6.468	0	12508824	N.D.	1.301
11) T	2,4,5-TP ...	0.000	6.773	0	69815958	N.D.	18.355
14) T	DINOSEB	0.000	7.966	0	11583119	N.D.	4.126
15) T	Picloram	0.000	8.935	0	60215550	N.D.	9.807
16) T	DCPA	9.373	0.000	287.9E6	0	32.154	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
Data File : PS007152.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 14:24
Operator : SM\AJ
Sample : K5325-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
10-10-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 15:33:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

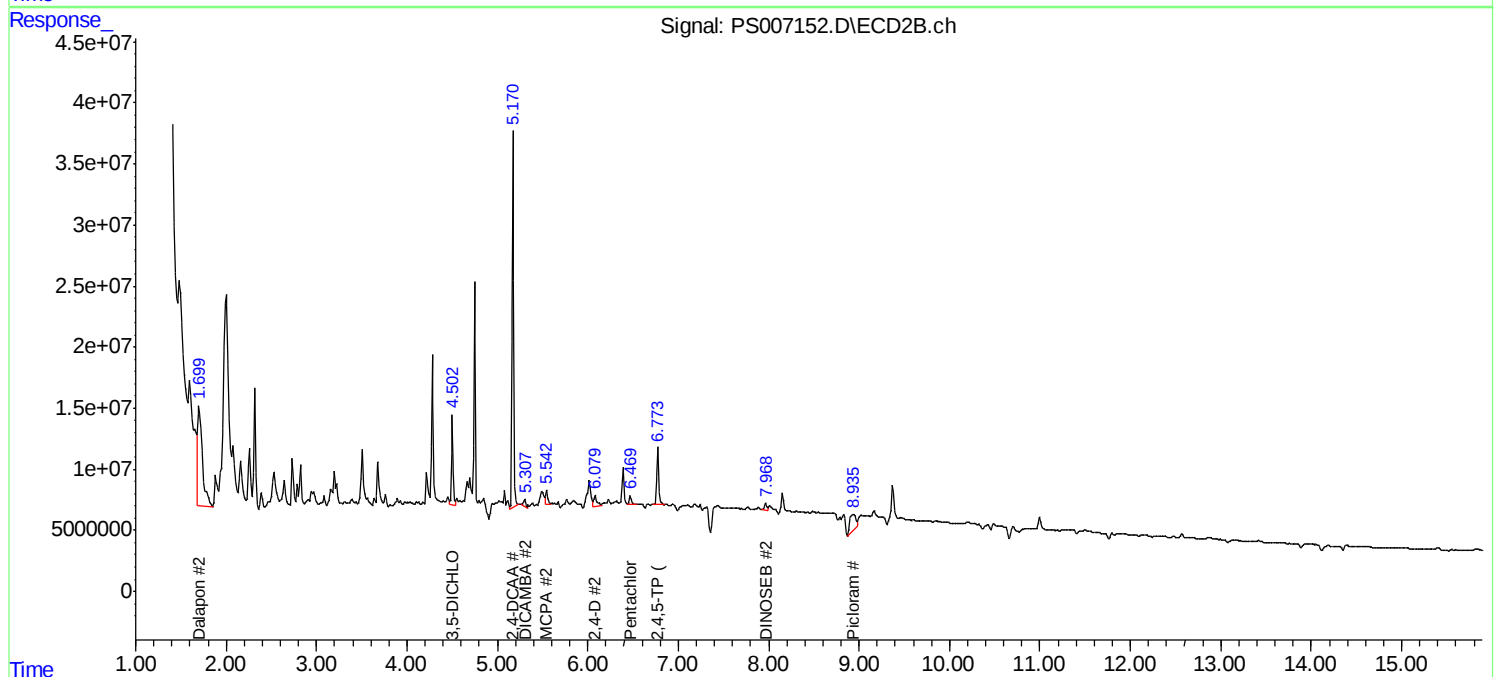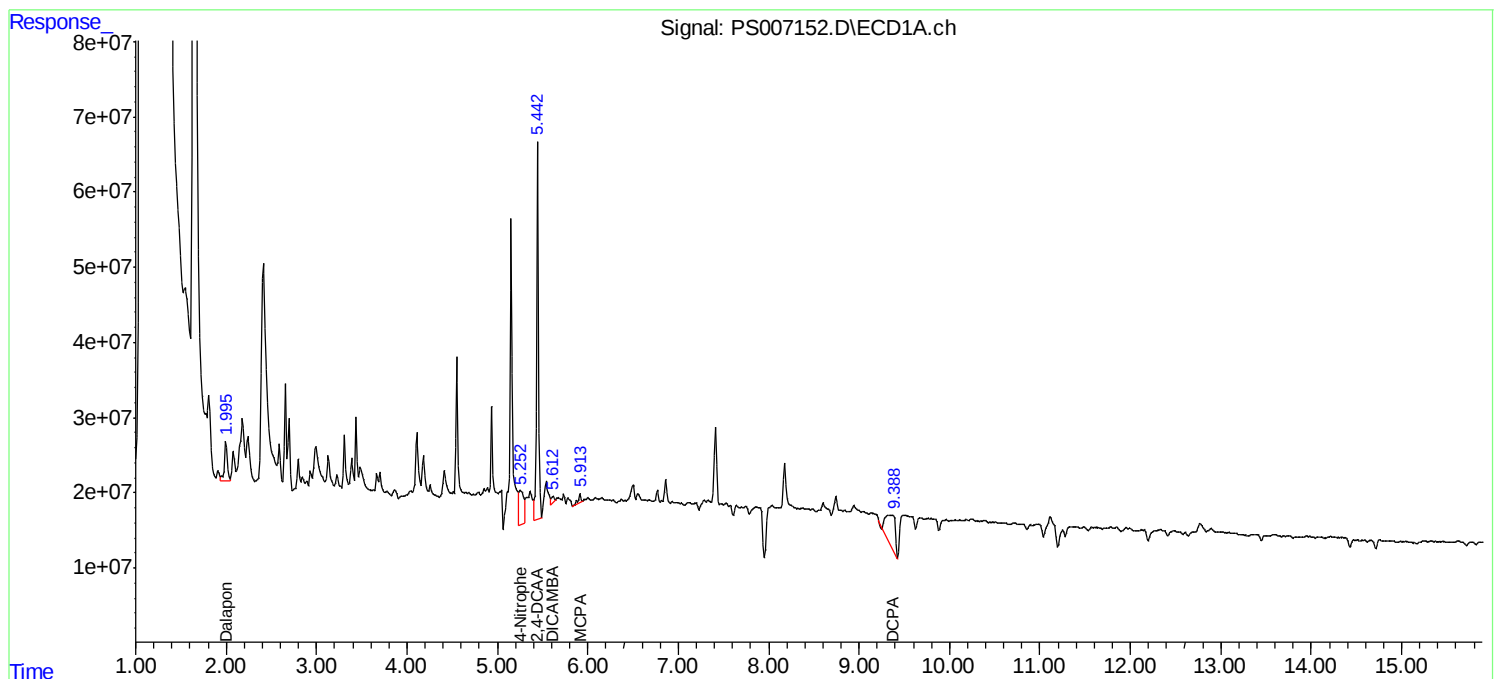


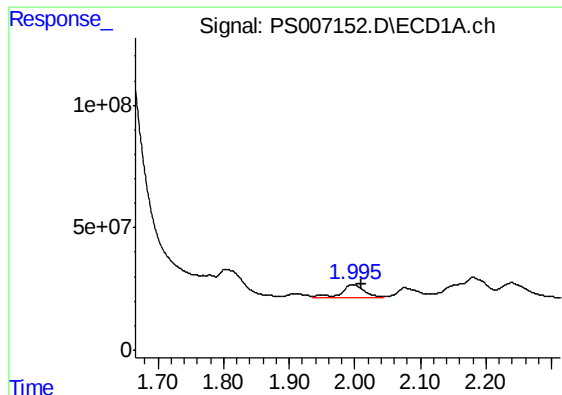

#1 Dalapon


R.T.: 1.996 min
Delta R.T.: -0.015 min
Response: 119834842
Conc: 71.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-E

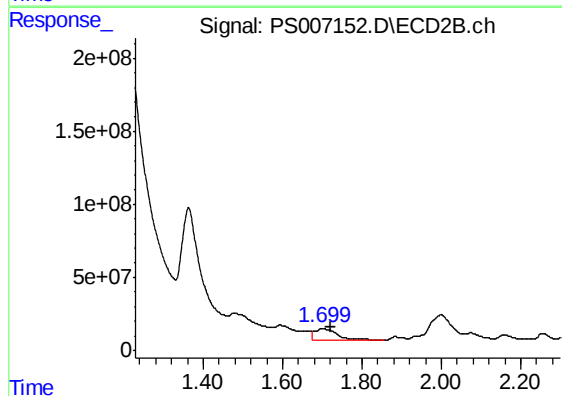


#1 Dalapon

R.T.: 1.700 min
Delta R.T.: -0.021 min
Response: 317887389
Conc: 349.33 ng/ml

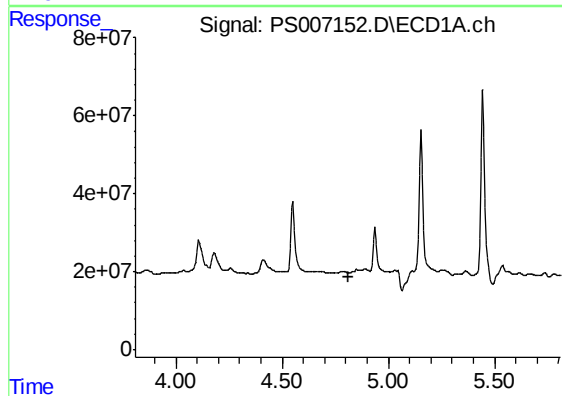


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

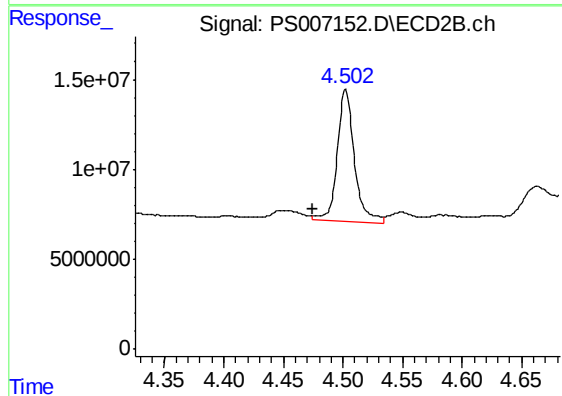

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.502 min
Delta R.T.: 0.028 min
Response: 73861159
Conc: 85.84 ng/ml

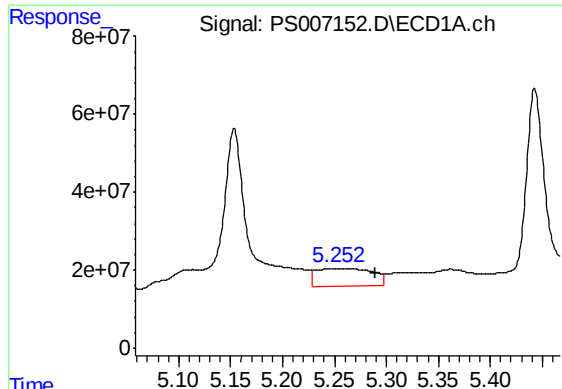

#3 4-Nitrophenol


R.T.: 5.254 min
Delta R.T.: -0.036 min
Response: 171744571
Conc: 286.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-E

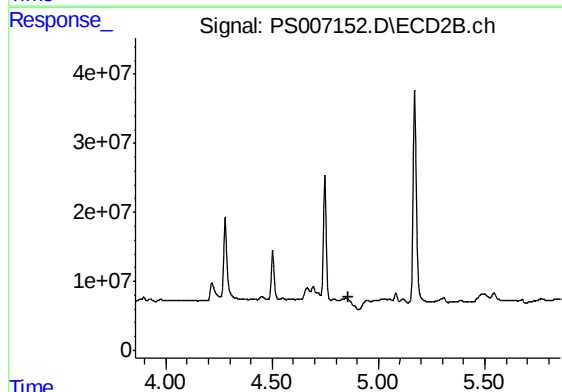


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

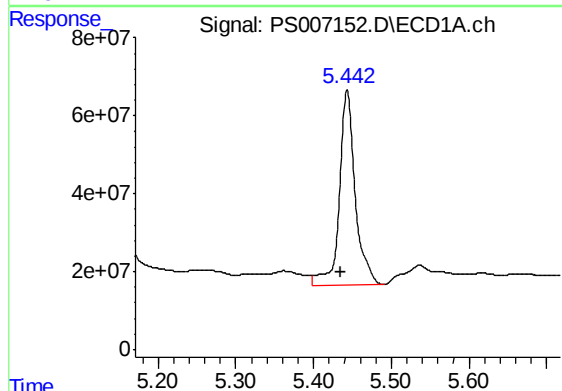


#4 2,4-DCAA

R.T.: 5.443 min
Delta R.T.: 0.007 min
Response: 699077059
Conc: 510.77 ng/ml

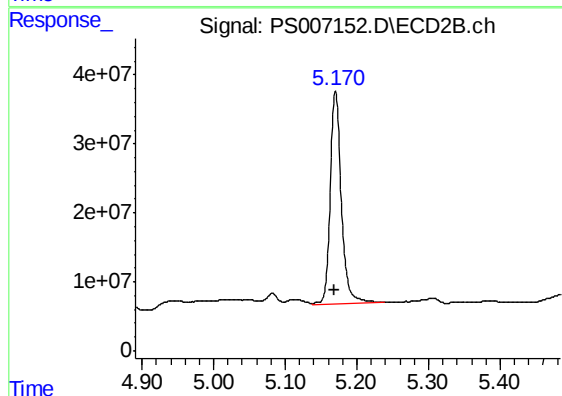

#4 2,4-DCAA


R.T.: 5.170 min
Delta R.T.: 0.002 min
Response: 329595001
Conc: 468.64 ng/ml

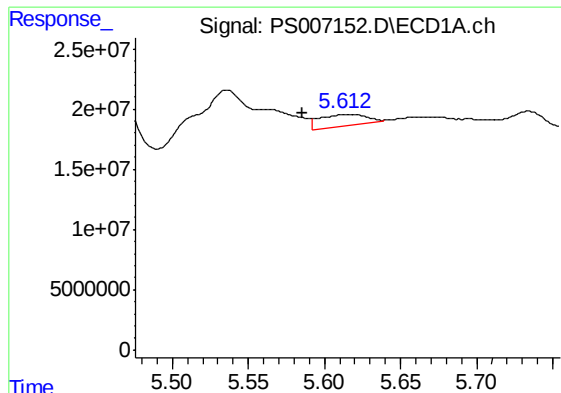

#5 DICAMBA


R.T.: 5.616 min
Delta R.T.: 0.031 min
Response: 19536545
Conc: 3.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-E

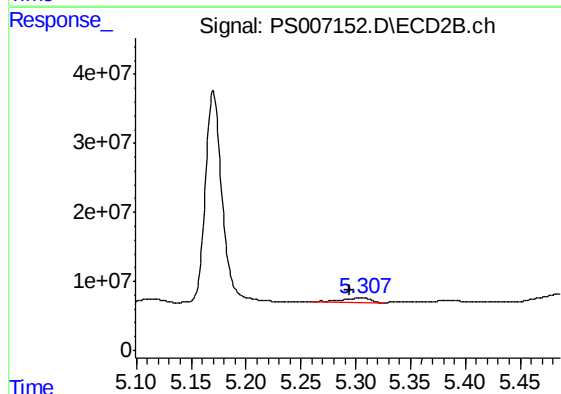


#5 DICAMBA

R.T.: 5.305 min
Delta R.T.: 0.011 min
Response: 11108060
Conc: 4.27 ng/ml

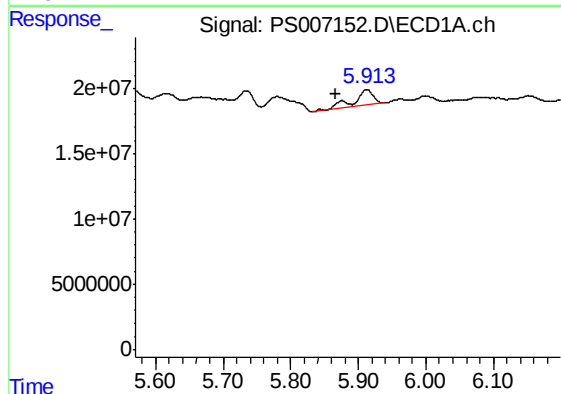


#7 MCPA

R.T.: 5.912 min
Delta R.T.: 0.045 min
Response: 23294880
Conc: 4.52 ug/ml

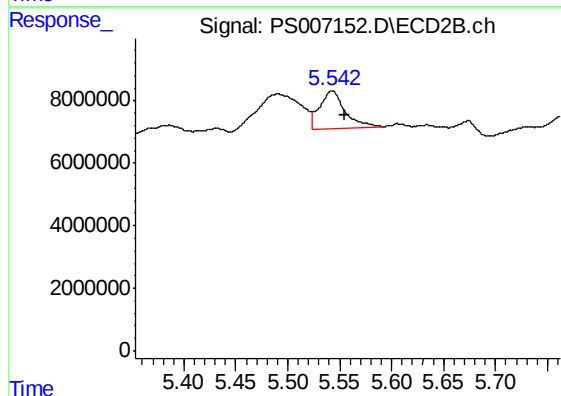

#7 MCPA


R.T.: 5.543 min
Delta R.T.: -0.012 min
Response: 20145695
Conc: 6.93 ug/ml

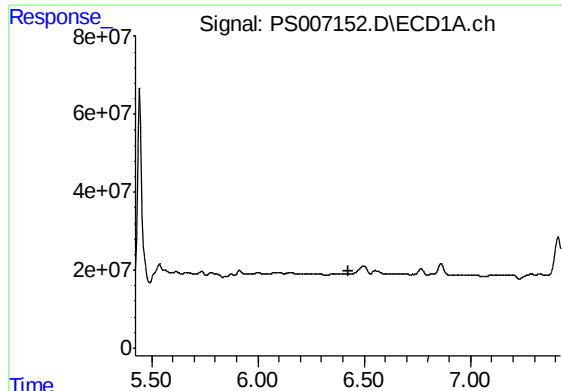

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-E

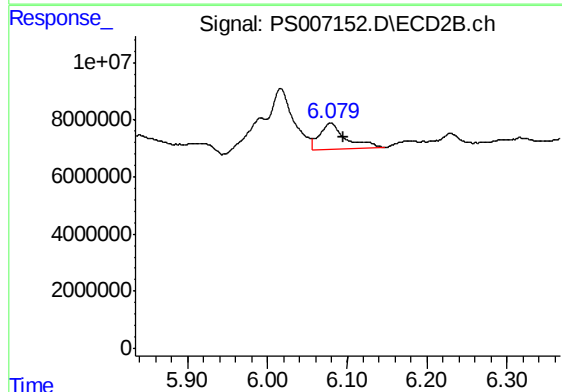


#9 2,4-D

R.T.: 6.079 min
Delta R.T.: -0.016 min
Response: 20943927
Conc: 26.25 ng/ml

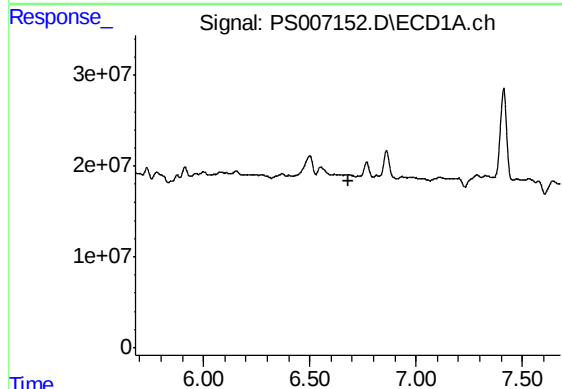


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

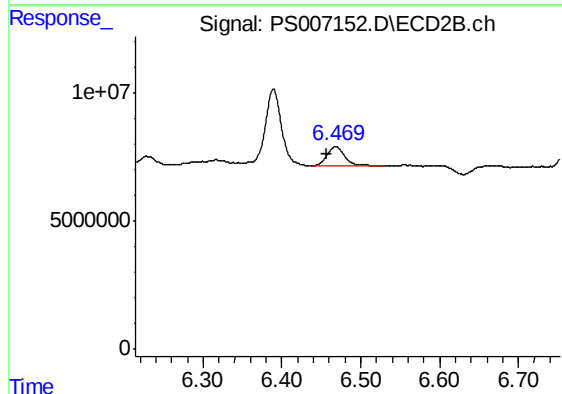

#10 Pentachlorophenol


R.T.: 6.468 min
Delta R.T.: 0.011 min
Response: 12508824
Conc: 1.30 ng/ml

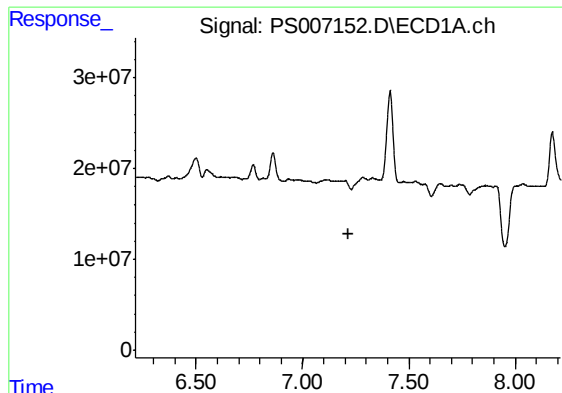

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-E

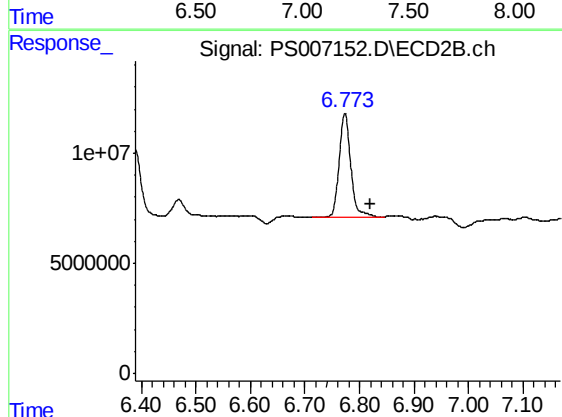


#11 2,4,5-TP (SILVEX)

R.T.: 6.773 min
Delta R.T.: -0.047 min
Response: 69815958
Conc: 18.36 ng/ml

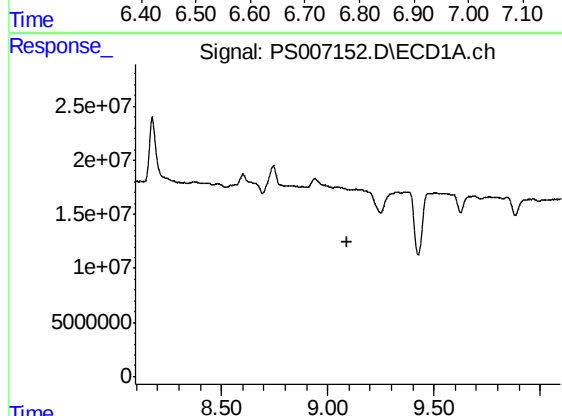


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

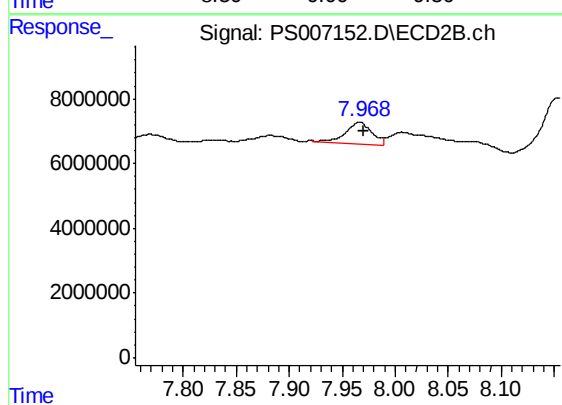

#14 DINOSEB


R.T.: 7.966 min
Delta R.T.: -0.004 min
Response: 11583119
Conc: 4.13 ng/ml

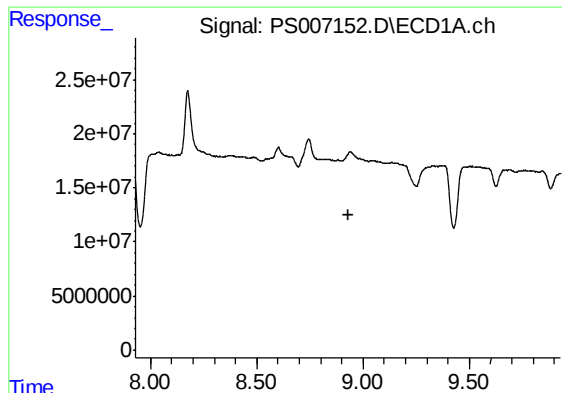

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-E

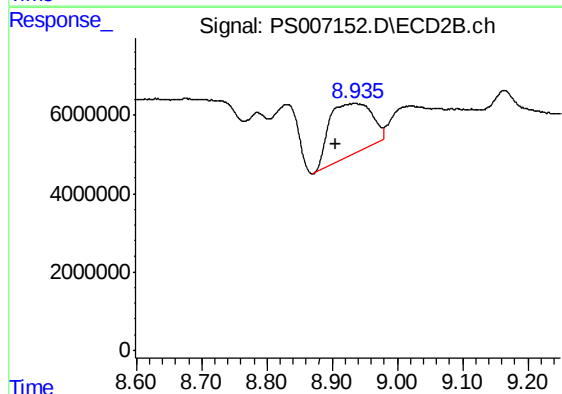


#15 Picloram

R.T.: 8.935 min
Delta R.T.: 0.031 min
Response: 60215550
Conc: 9.81 ng/ml

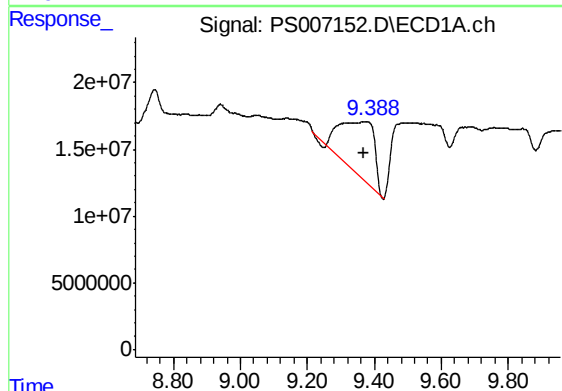

#16 DCPA

R.T.: 9.373 min
Delta R.T.: 0.006 min
Response: 287918565
Conc: 32.15 ng/ml

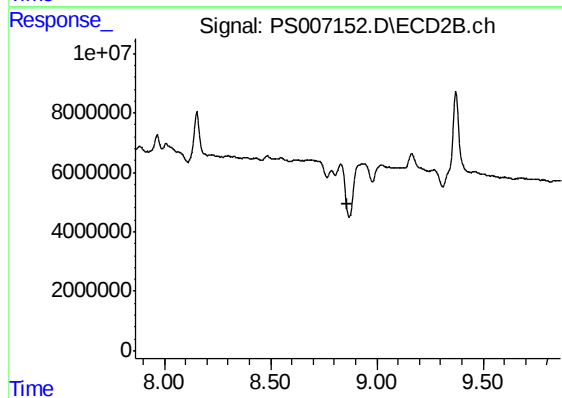

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 8.863 min
Response: 0
Conc: N.D.