

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
 Data File : PS007156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 15:52
 Operator : SM\AJ
 Sample : K5325-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 10-10-G

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 16:35:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.439	5.172	554.6E6	272.3E6	405.196	387.240
Target Compounds							
1) T	Dalapon	1.992	1.702	247.3E6	386.3E6	147.787	424.543 #
2) T	3,5-DICHL...	0.000	4.504	0	45759015	N.D.	53.181
3) T	4-Nitroph...	5.356	0.000	154.6E6	0	257.416	N.D. #
5) T	DICAMBA	5.612	0.000	19503547	0	3.969	N.D. #
7) T	MCPA	0.000	5.543	0	19670439	N.D.	6.766
9) T	2,4-D	0.000	6.081	0	17203882	N.D.	21.564
10) T	Pentachlo...	0.000	6.470	0	9690209	N.D.	1.008
11) T	2,4,5-TP ...	0.000	6.775	0	63402819	N.D.	16.669
14) T	DINOSEB	0.000	7.968	0	5447410	N.D.	1.940
15) T	Picloram	0.000	8.940	0	48352417	N.D.	7.875



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
Data File : PS007156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 15:52
Operator : SM\AJ
Sample : K5325-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
10-10-G

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 16:35:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

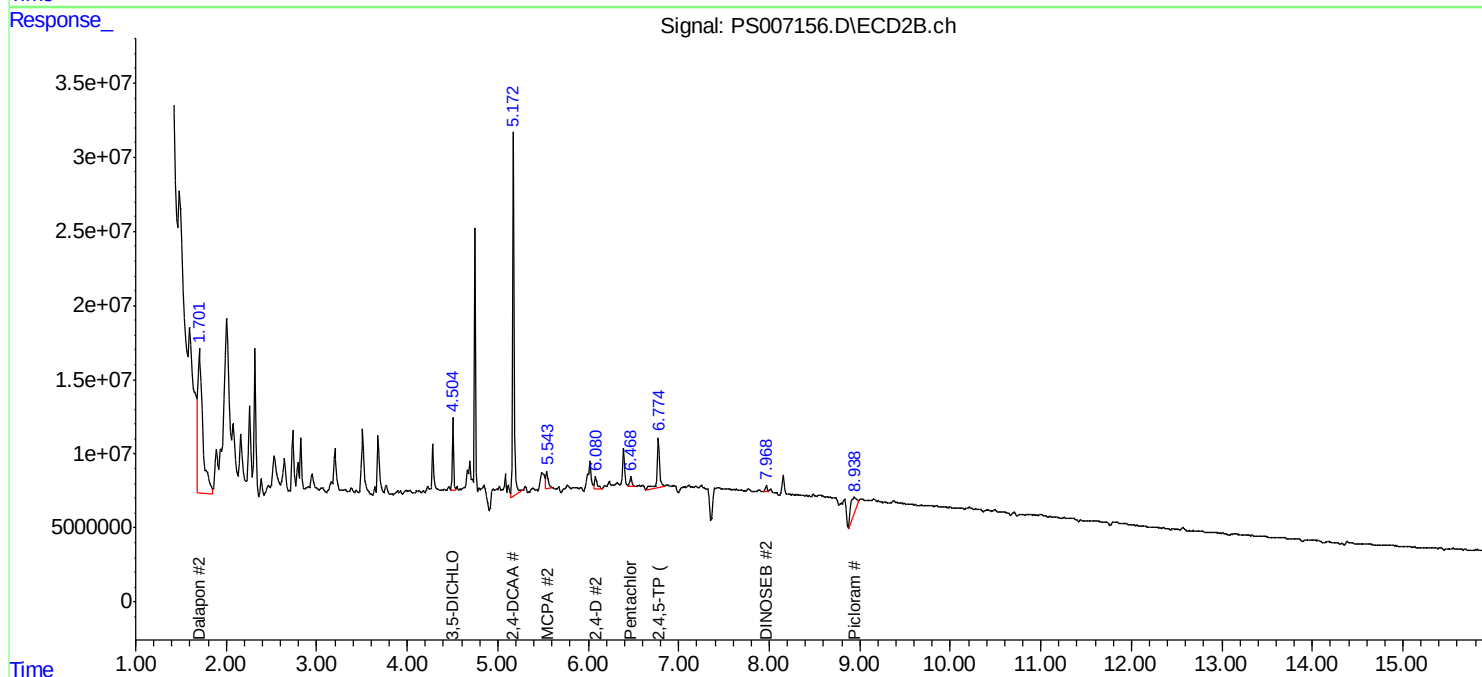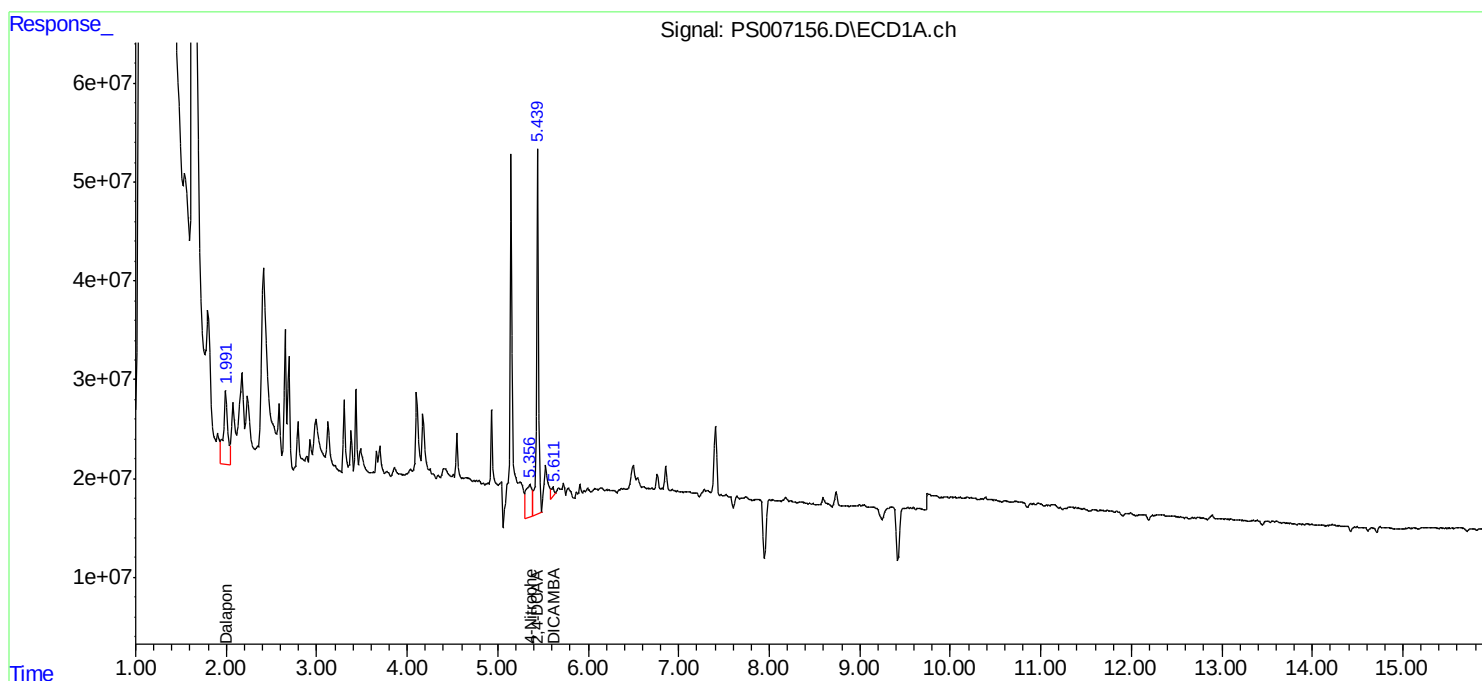


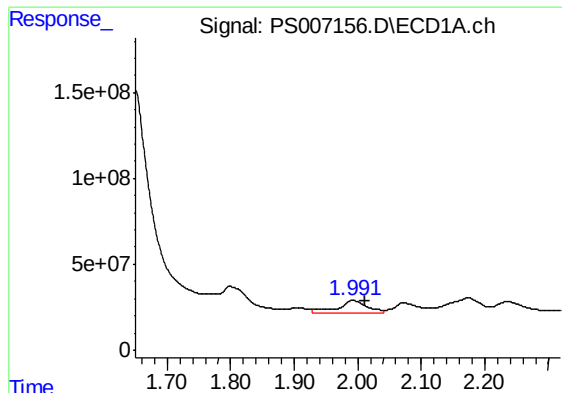

#1 Dalapon


R.T.: 1.992 min
Delta R.T.: -0.019 min
Response: 247289142
Conc: 147.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-G

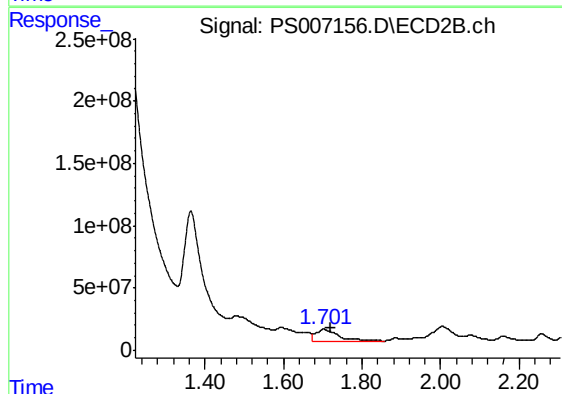


#1 Dalapon

R.T.: 1.702 min
Delta R.T.: -0.019 min
Response: 386335425
Conc: 424.54 ng/ml

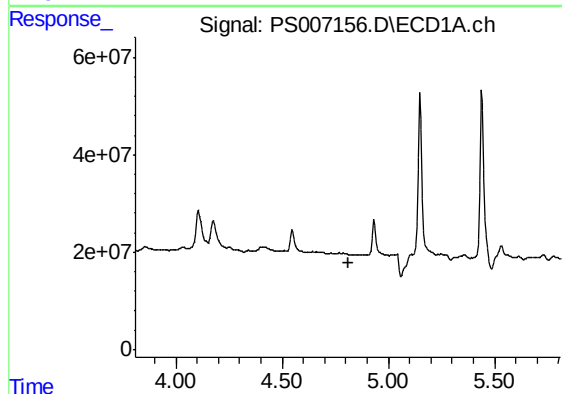


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

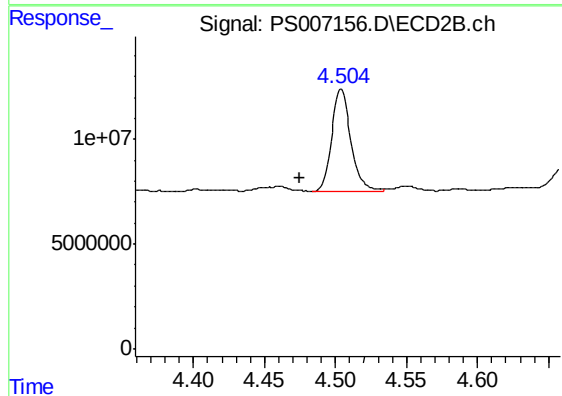

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.504 min
Delta R.T.: 0.029 min
Response: 45759015
Conc: 53.18 ng/ml

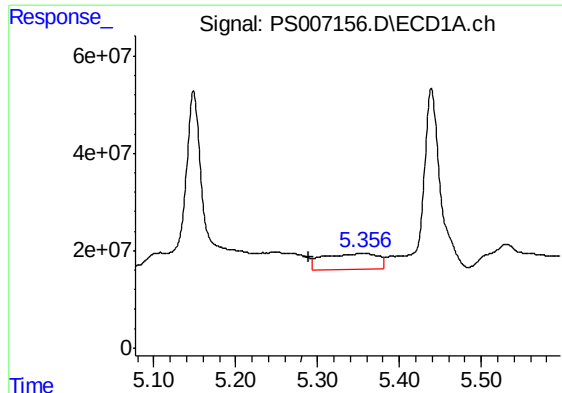

#3 4-Nitrophenol


R.T.: 5.356 min
Delta R.T.: 0.067 min
Response: 154571414
Conc: 257.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-G

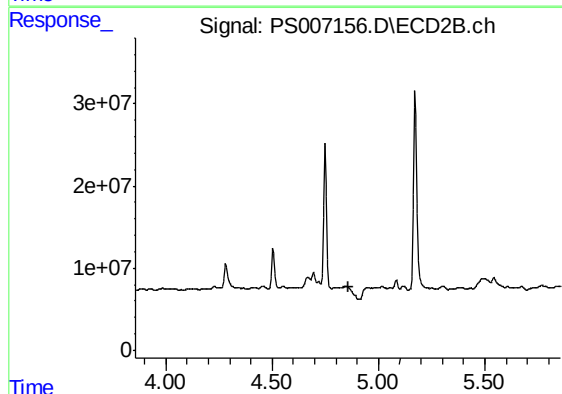


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

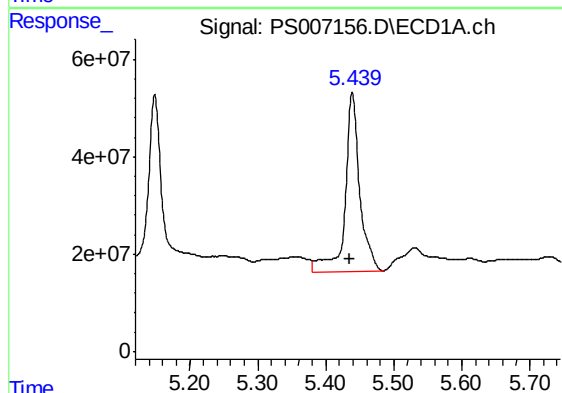


#4 2,4-DCAA

R.T.: 5.439 min
Delta R.T.: 0.003 min
Response: 554579121
Conc: 405.20 ng/ml

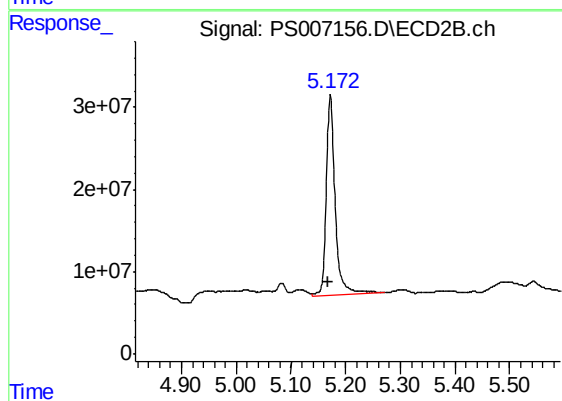

#4 2,4-DCAA


R.T.: 5.172 min
Delta R.T.: 0.004 min
Response: 272348311
Conc: 387.24 ng/ml

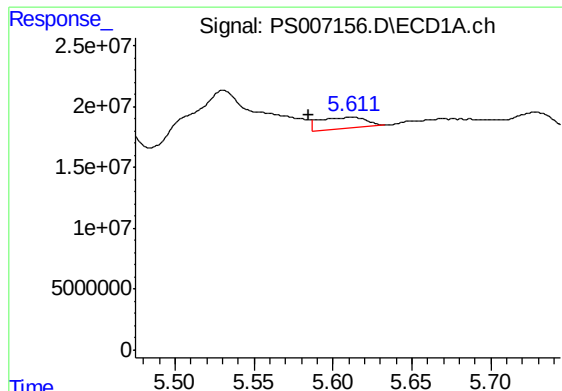

#5 DICAMBA


R.T.: 5.612 min
Delta R.T.: 0.027 min
Response: 19503547
Conc: 3.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-G

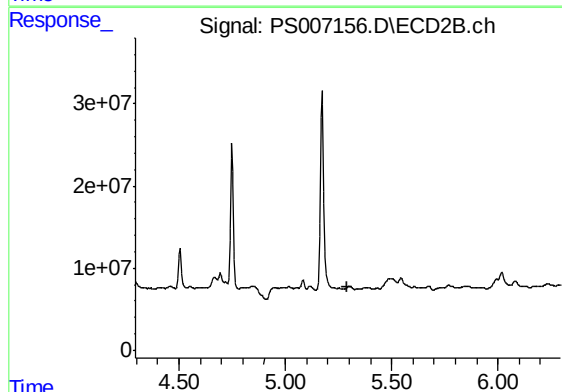


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

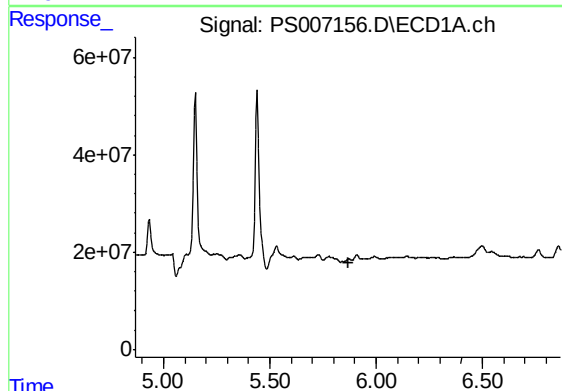


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

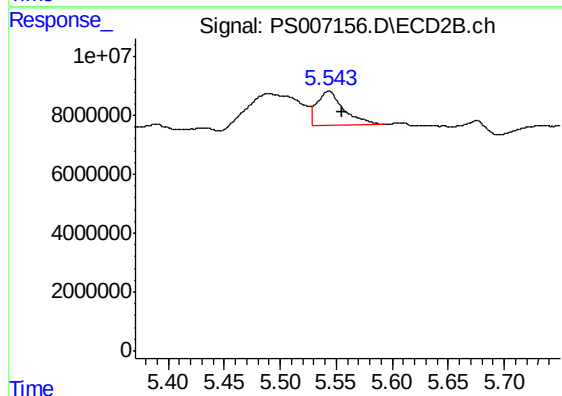

#7 MCPA


R.T.: 5.543 min
Delta R.T.: -0.012 min
Response: 19670439
Conc: 6.77 ug/ml

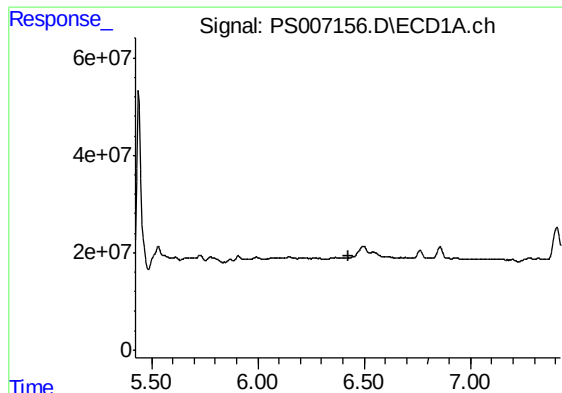

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-G

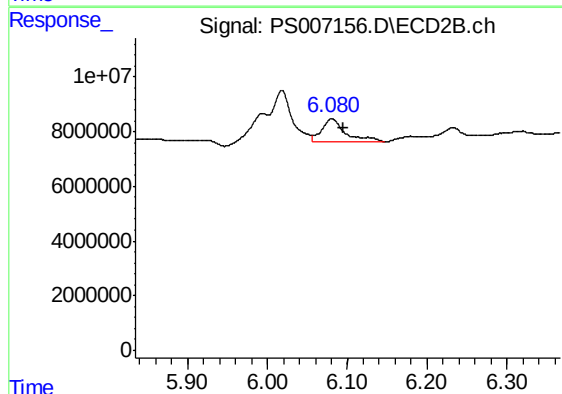


#9 2,4-D

R.T.: 6.081 min
Delta R.T.: -0.015 min
Response: 17203882
Conc: 21.56 ng/ml

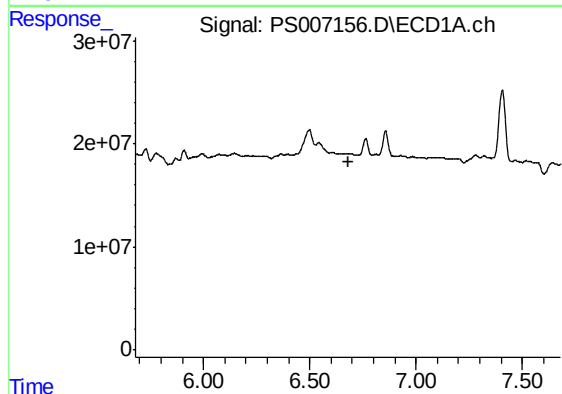


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

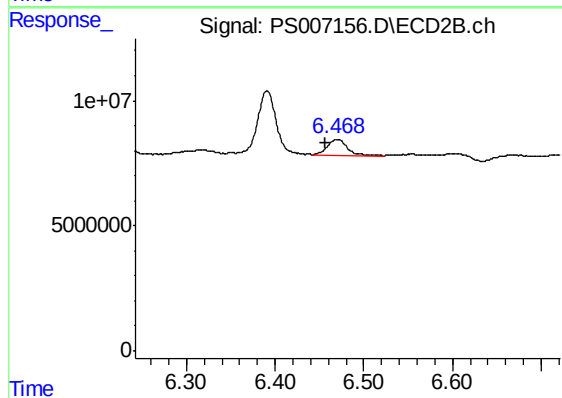

#10 Pentachlorophenol


R.T.: 6.470 min
Delta R.T.: 0.013 min
Response: 9690209
Conc: 1.01 ng/ml

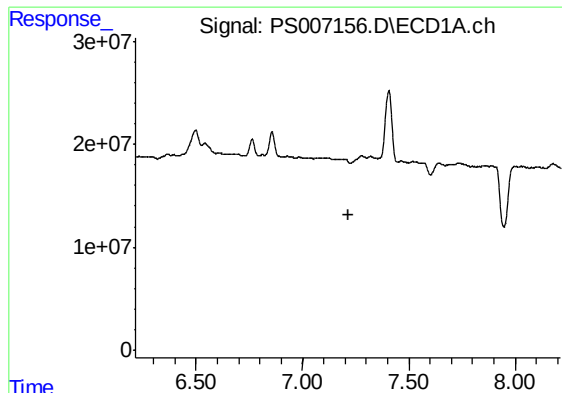

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-G

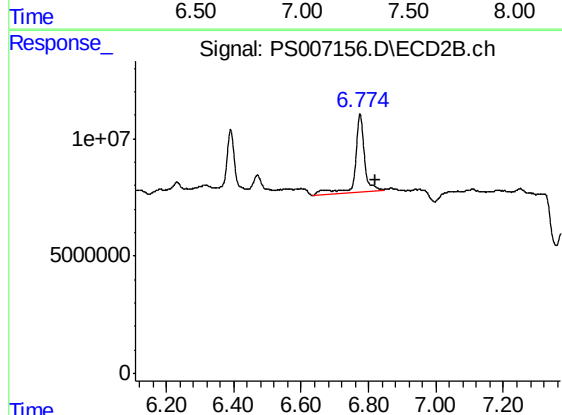


#11 2,4,5-TP (SILVEX)

R.T.: 6.775 min
Delta R.T.: -0.046 min
Response: 63402819
Conc: 16.67 ng/ml

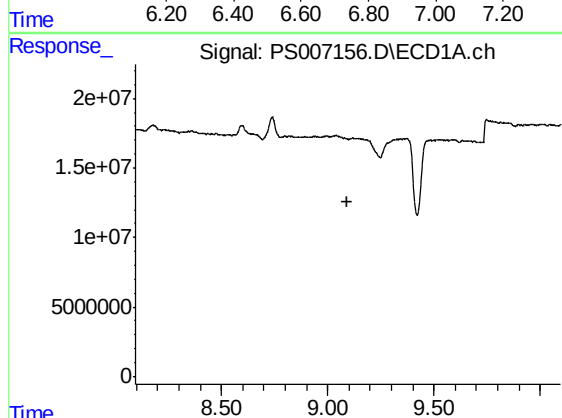


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

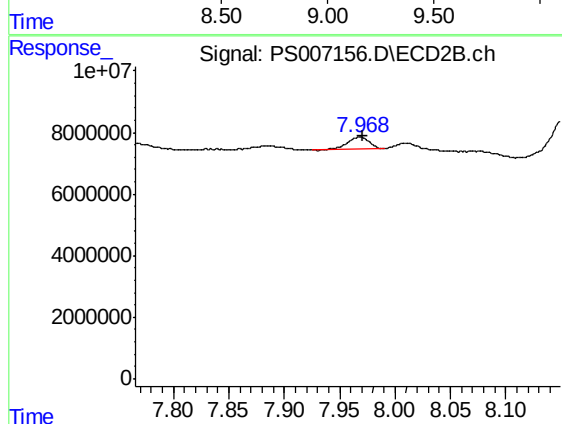

#14 DINOSEB


R.T.: 7.968 min
Delta R.T.: -0.003 min
Response: 5447410
Conc: 1.94 ng/ml

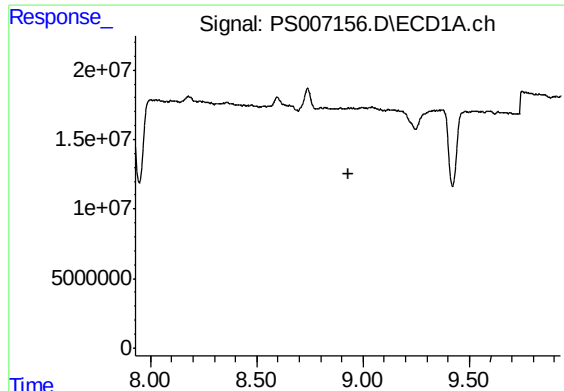

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-G

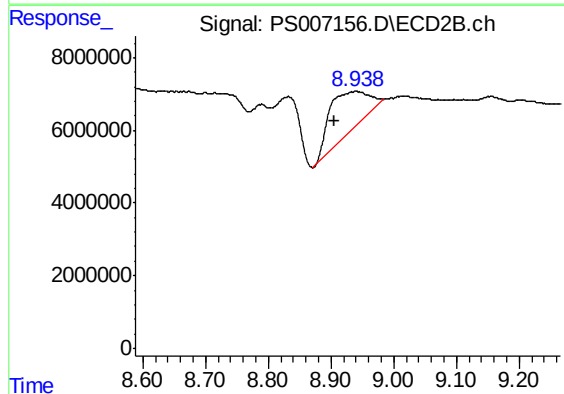

#15 Picloram

R.T.: 8.940 min
Delta R.T.: 0.036 min
Response: 48352417
Conc: 7.87 ng/ml