

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
 Data File : PS007158.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 16:36
 Operator : SM\AJ
 Sample : K5325-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 10-10-I

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 17:35:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.471	5.149	551.2E6	14335509	402.695	20.383 #
Target Compounds							
1) T	Dalapon	2.024	1.735	131.0E6	404.7E6	78.278	444.675 #
2) T	3,5-DICHL...	0.000	4.537	0	41848836	N.D.	48.637
5) T	DICAMBA	5.563	0.000	154.1E6	0	31.363	N.D. #
7) T	MCPA	0.000	5.576	0	22159938	N.D.	7.623
9) T	2,4-D	0.000	6.113	0	17892274	N.D.	22.427
10) T	Pentachlo...	0.000	6.423	0	48279140	N.D.	5.021
11) T	2,4,5-TP ...	0.000	6.807	0	50886154	N.D.	13.378
12) T	2,4,5-T	7.436	7.136	177.1E6	15961331	23.161	4.556 #
14) T	DINOSEB	0.000	8.000	0	6490466	N.D.	2.312
15) T	Picloram	0.000	8.864	0	35643217	N.D.	5.805
16) T	DCPA	9.400	8.864	336.8E6	35643217	37.617	7.108 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
Data File : PS007158.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 16:36
Operator : SM\AJ
Sample : K5325-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
10-10-I

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 17:35:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

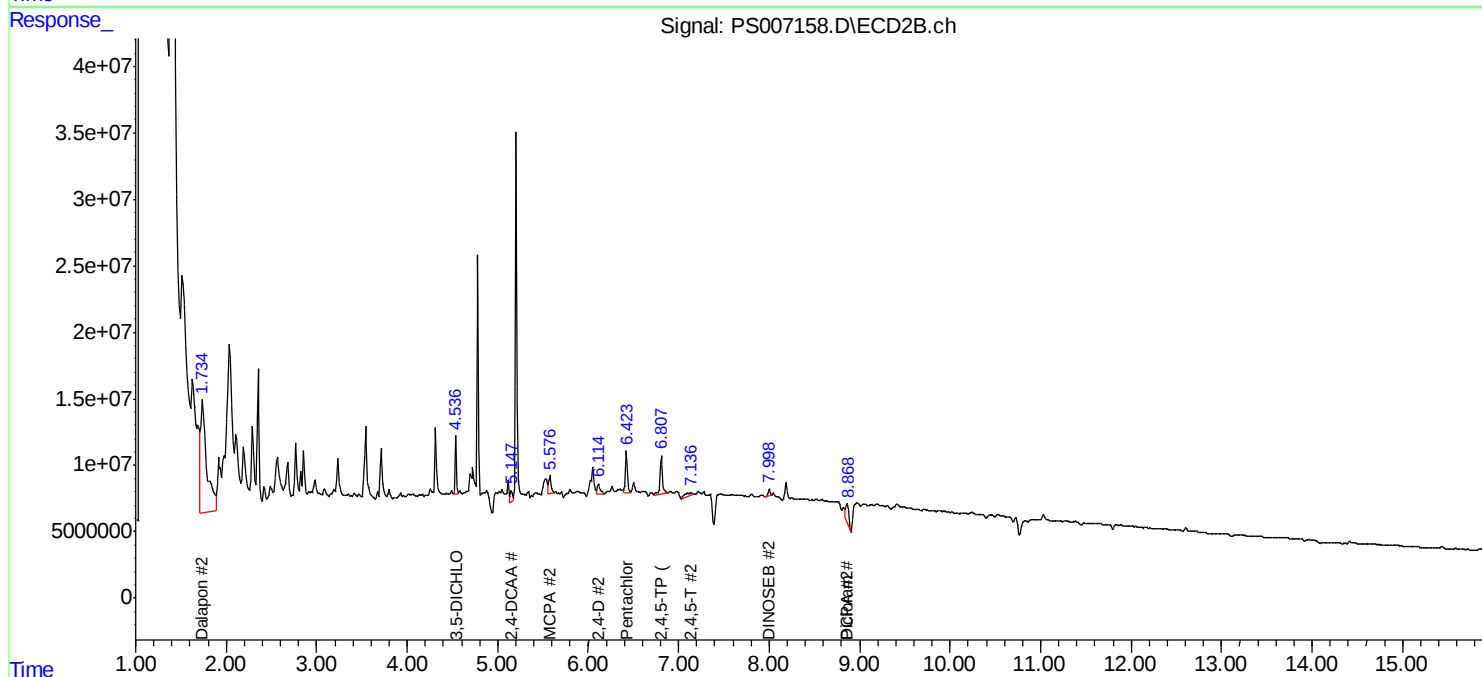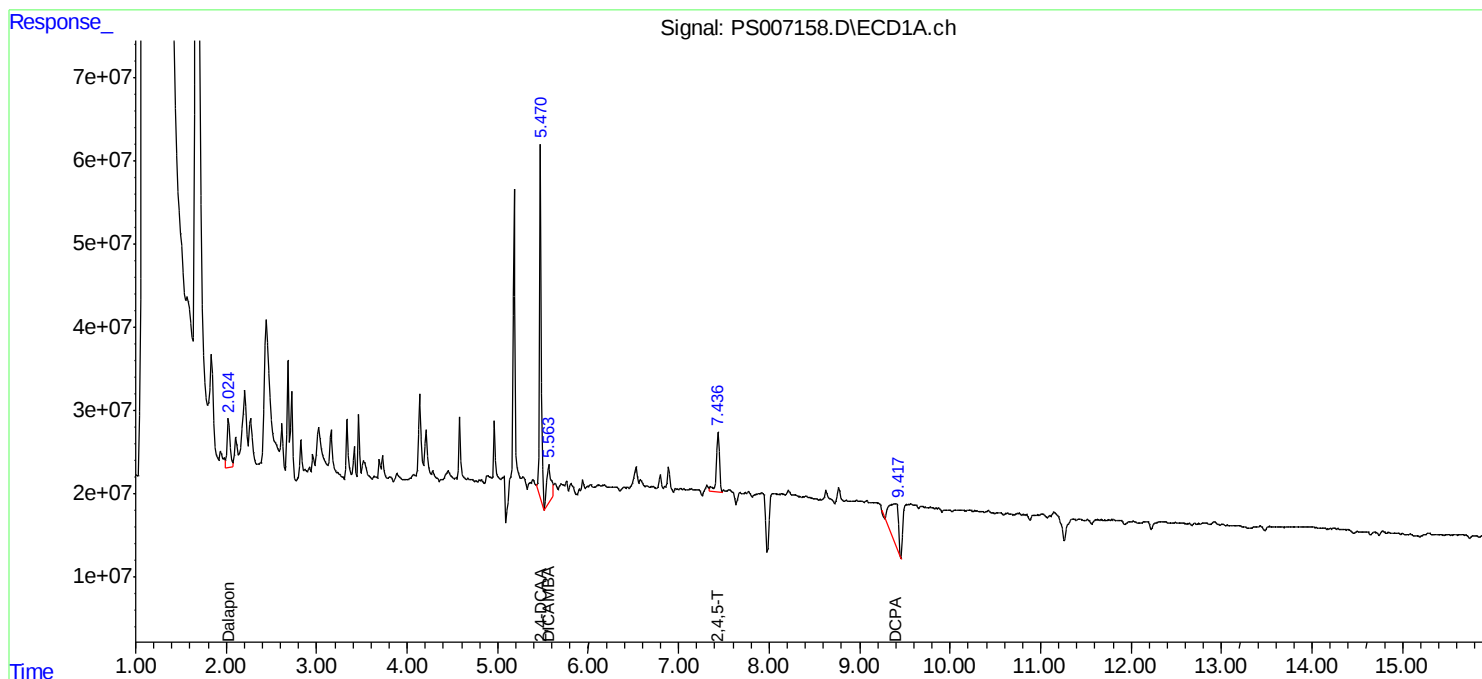


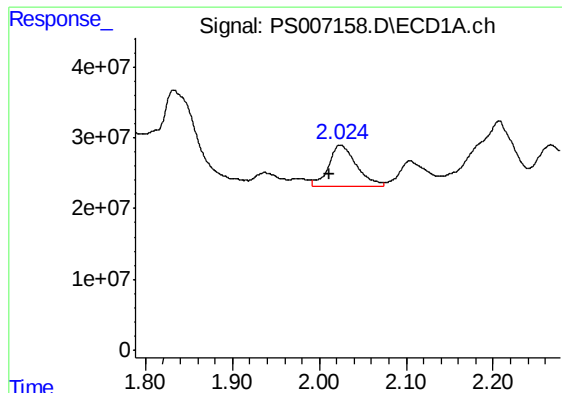

#1 Dalapon


R.T.: 2.024 min
Delta R.T.: 0.013 min
Response: 130980711
Conc: 78.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-I

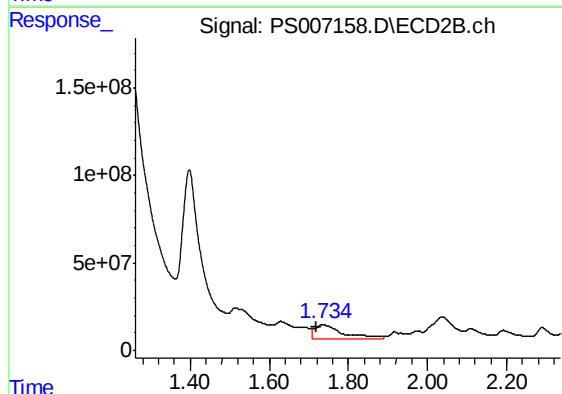


#1 Dalapon

R.T.: 1.735 min
Delta R.T.: 0.014 min
Response: 404655885
Conc: 444.68 ng/ml

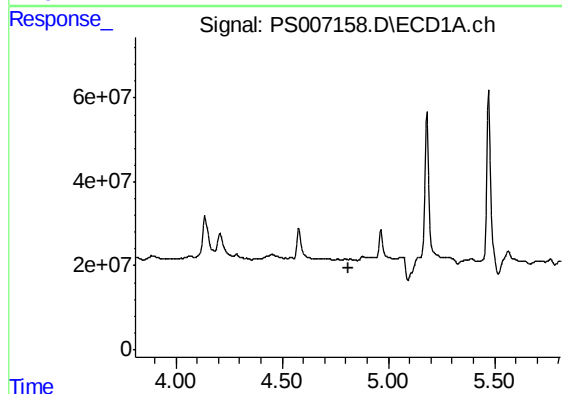


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

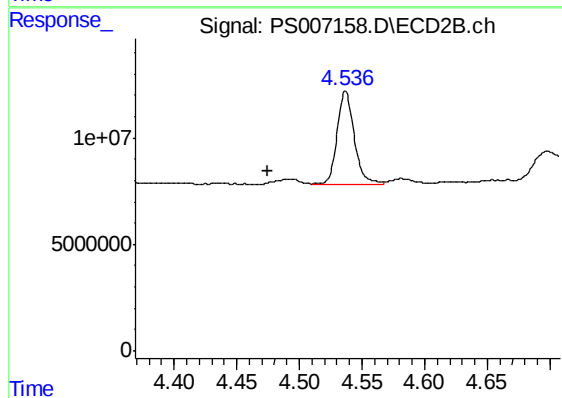

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.537 min
Delta R.T.: 0.062 min
Response: 41848836
Conc: 48.64 ng/ml

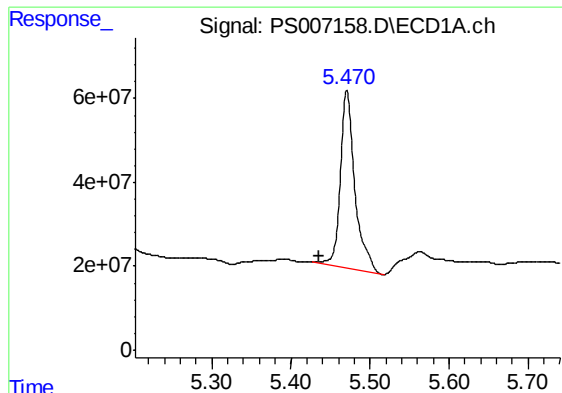

#4 2,4-DCAA


R.T.: 5.471 min
Delta R.T.: 0.035 min
Response: 551156395
Conc: 402.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-I

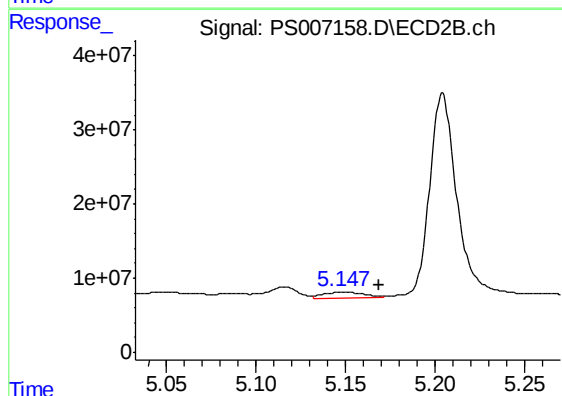


#4 2,4-DCAA

R.T.: 5.149 min
Delta R.T.: -0.020 min
Response: 14335509
Conc: 20.38 ng/ml

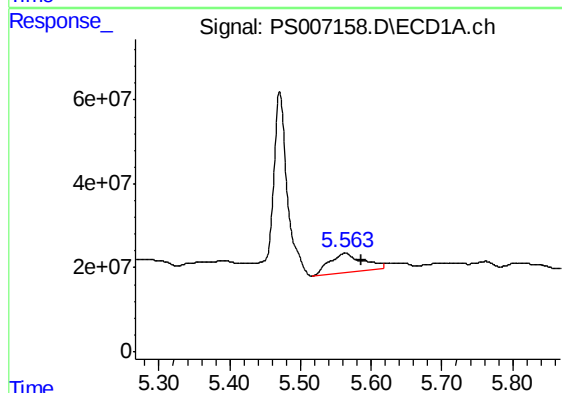


#5 DICAMBA

R.T.: 5.563 min
Delta R.T.: -0.022 min
Response: 154099857
Conc: 31.36 ng/ml

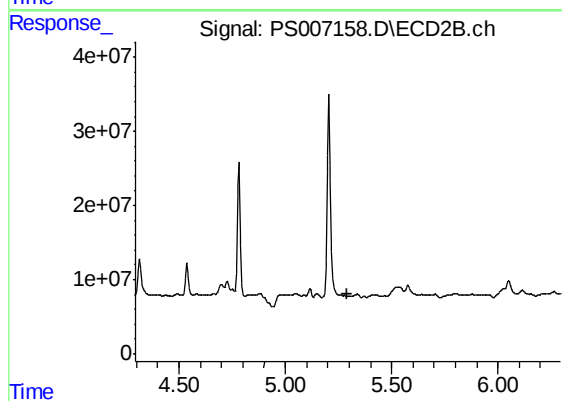

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

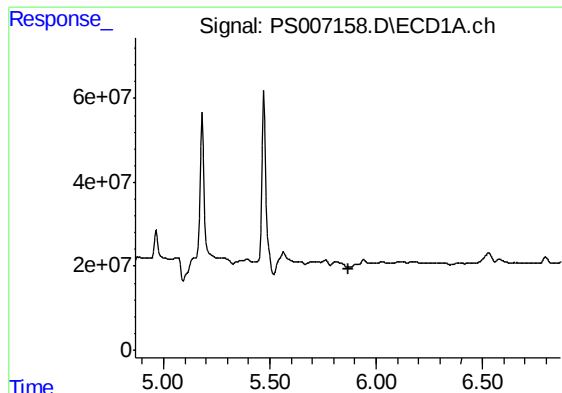

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-I

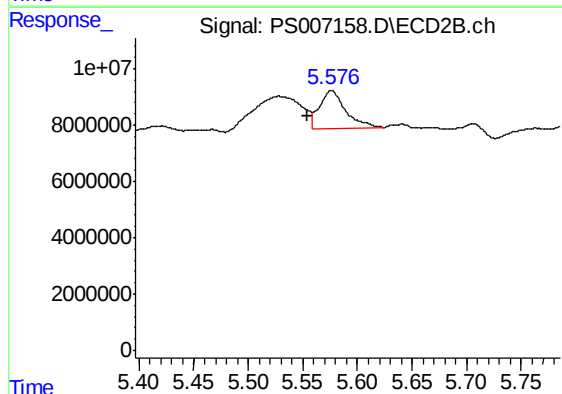


#7 MCPA

R.T.: 5.576 min
Delta R.T.: 0.022 min
Response: 22159938
Conc: 7.62 ug/ml

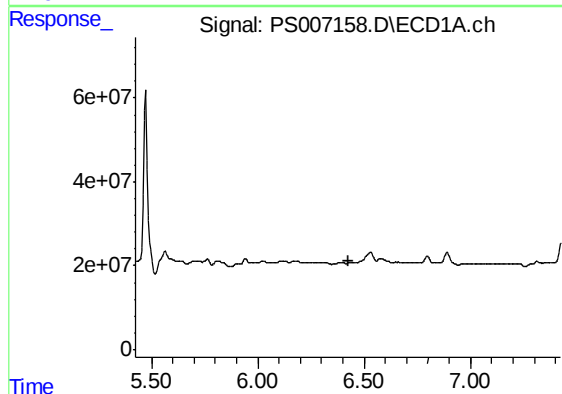


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

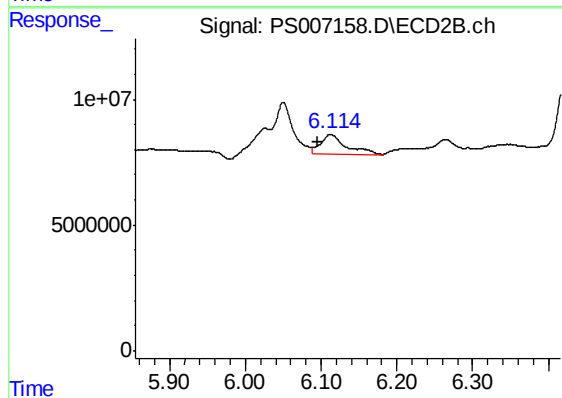

#9 2,4-D


R.T.: 6.113 min
Delta R.T.: 0.018 min
Response: 17892274
Conc: 22.43 ng/ml

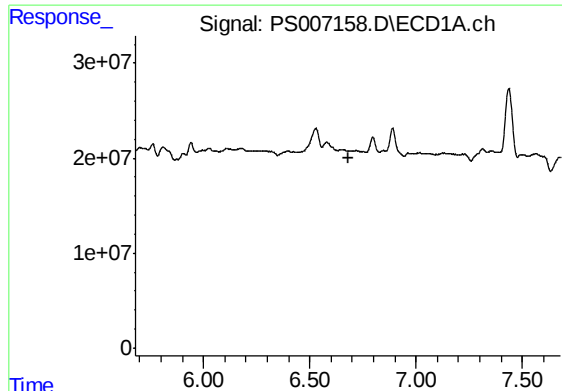

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-I

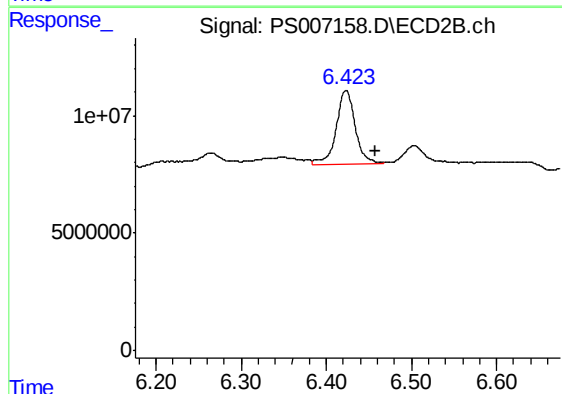


#10 Pentachlorophenol

R.T.: 6.423 min
Delta R.T.: -0.034 min
Response: 48279140
Conc: 5.02 ng/ml

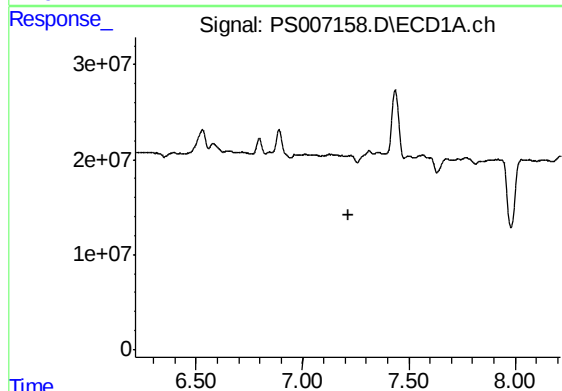


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

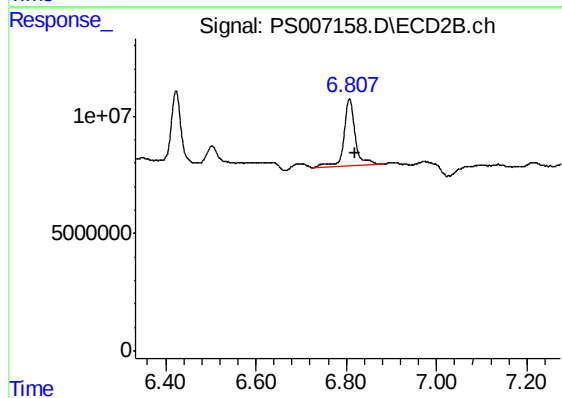

#11 2,4,5-TP (SILVEX)


R.T.: 6.807 min
Delta R.T.: -0.013 min
Response: 50886154
Conc: 13.38 ng/ml

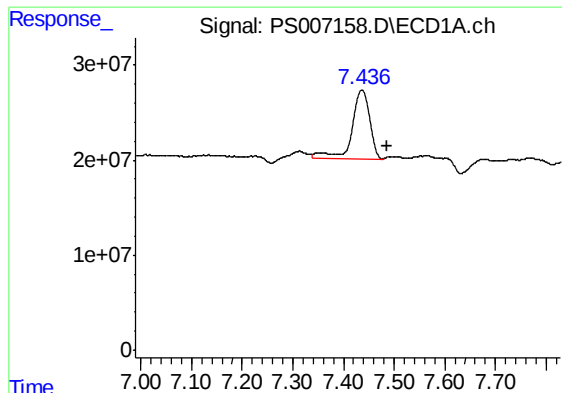

#12 2,4,5-T


R.T.: 7.436 min
Delta R.T.: -0.050 min
Response: 177063492
Conc: 23.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
10-10-I

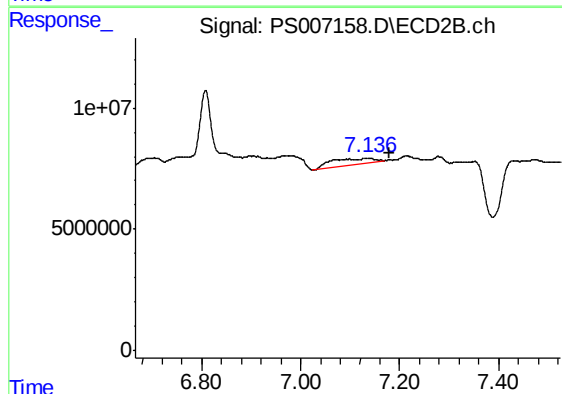


#12 2,4,5-T

R.T.: 7.136 min
Delta R.T.: -0.042 min
Response: 15961331
Conc: 4.56 ng/ml

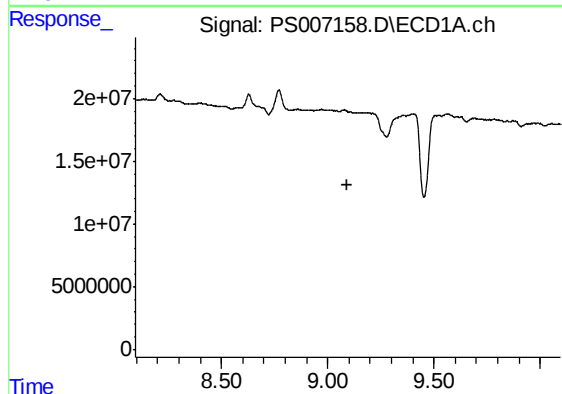


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.095 min
Response: 0
Conc: N.D.

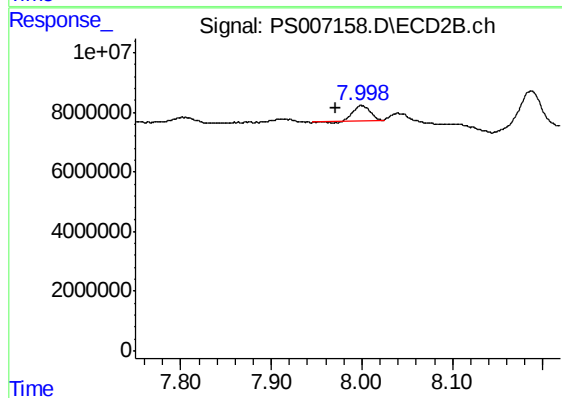

#14 DINOSEB


R.T.: 8.000 min
Delta R.T.: 0.029 min
Response: 6490466
Conc: 2.31 ng/ml

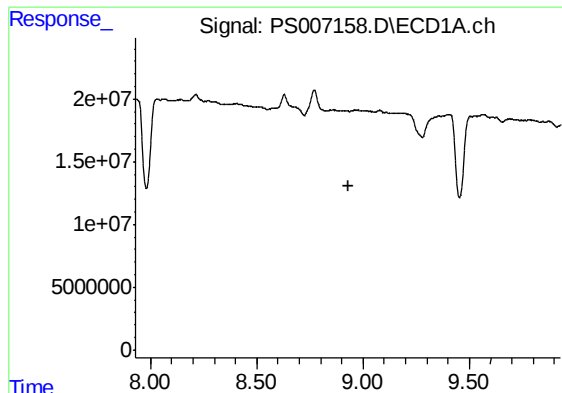

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
10-10-I

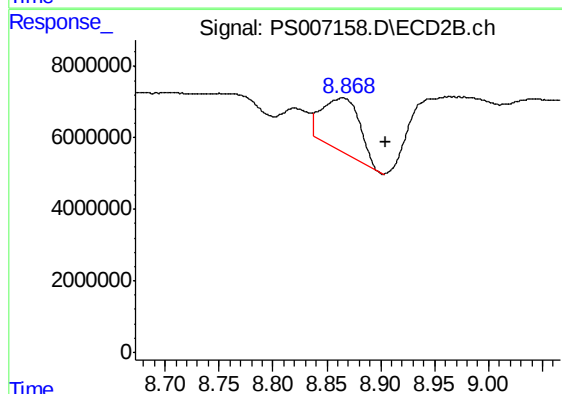


#15 Picloram

R.T.: 8.864 min
Delta R.T.: -0.040 min
Response: 35643217
Conc: 5.80 ng/ml

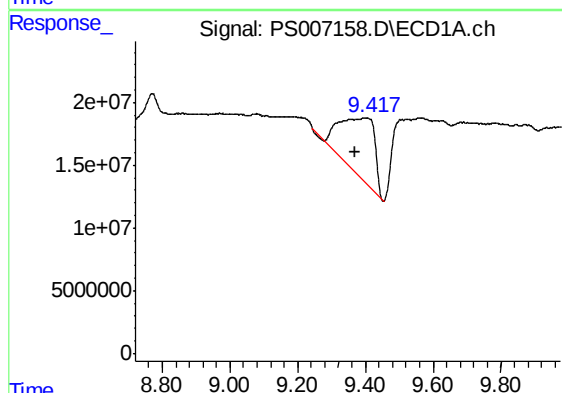

#16 DCPA

R.T.: 9.400 min
Delta R.T.: 0.033 min
Response: 336832003
Conc: 37.62 ng/ml

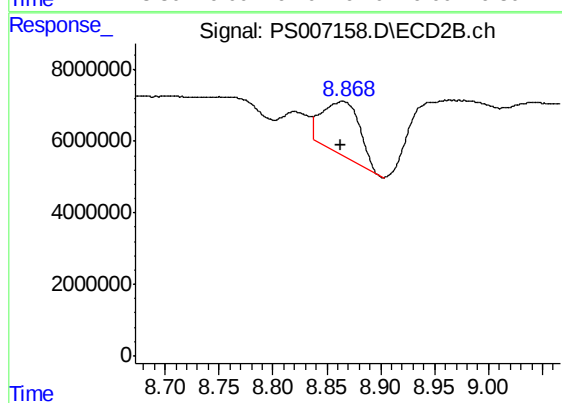

#16 DCPA

R.T.: 8.864 min
Delta R.T.: 0.001 min
Response: 35643217
Conc: 7.11 ng/ml