

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
 Data File : PS007174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2019 22:27
 Operator : SM\AJ
 Sample : K5355-07
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 01:01:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.444	5.175	406.8E6	165.5E6	297.216	235.282
Target Compounds							
1) T	Dalapon	1.996	1.708	132.5E6	132.3E6	79.211	145.425 #
2) T	3,5-DICHL...	0.000	4.465	0	5900326	N.D.	6.857
3) T	4-Nitroph...	5.271	0.000	134.5E6	0	224.013	N.D. #
5) T	DICAMBA	5.620	5.304	31498564	14018351	6.411	5.387
7) T	MCPA	0.000	5.593	0	11284243	N.D.	3.882
8) T	DICHLORPROP	6.155	5.835	-3036921	61161595	N.D.	93.919
10) T	Pentachlo...	0.000	6.468	0	17370003	N.D.	1.806
11) T	2,4,5-TP ...	0.000	6.802	0	99612333	N.D.	26.189
15) T	Picloram	0.000	8.928	0	6926235	N.D.	1.128
16) T	DCPA	0.000	8.928	0	6926235	N.D.	1.381



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101519\
Data File : PS007174.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2019 22:27
Operator : SM\AJ
Sample : K5355-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 01:01:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

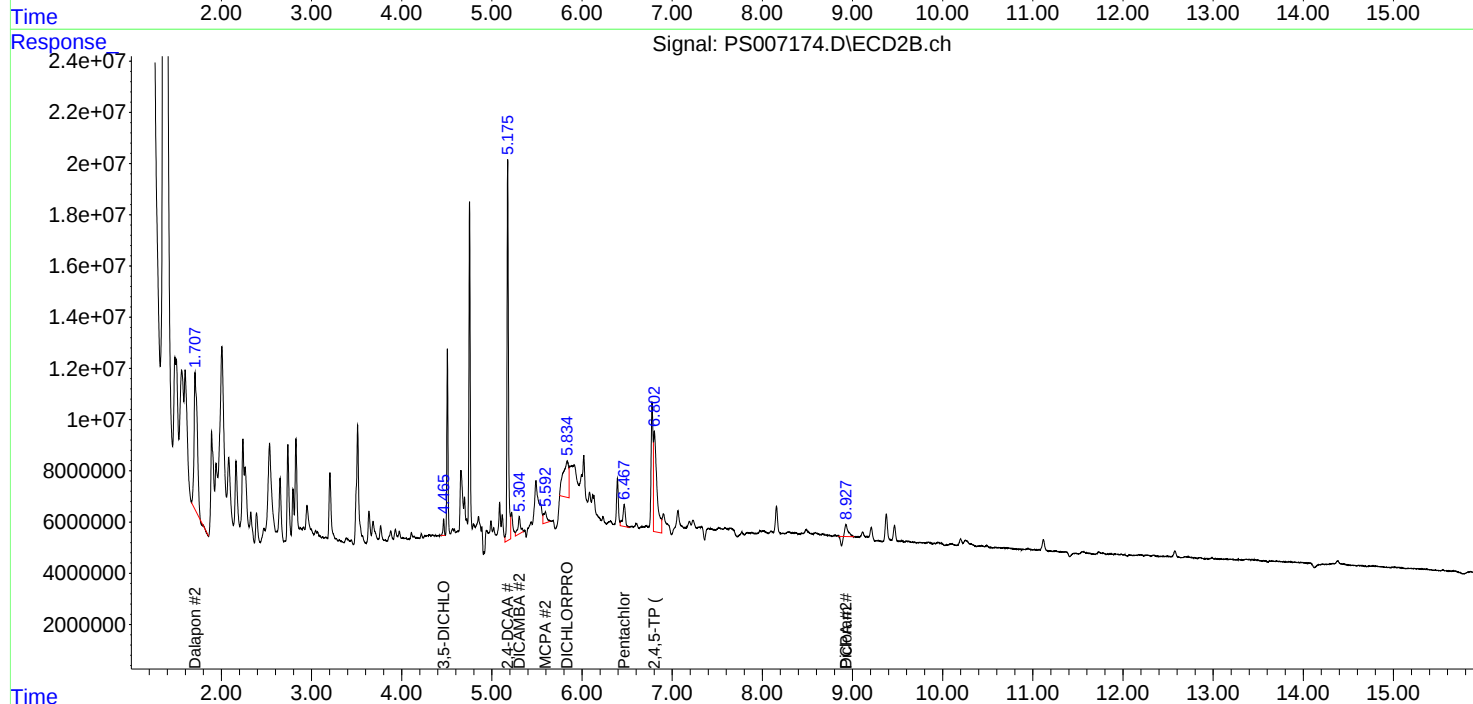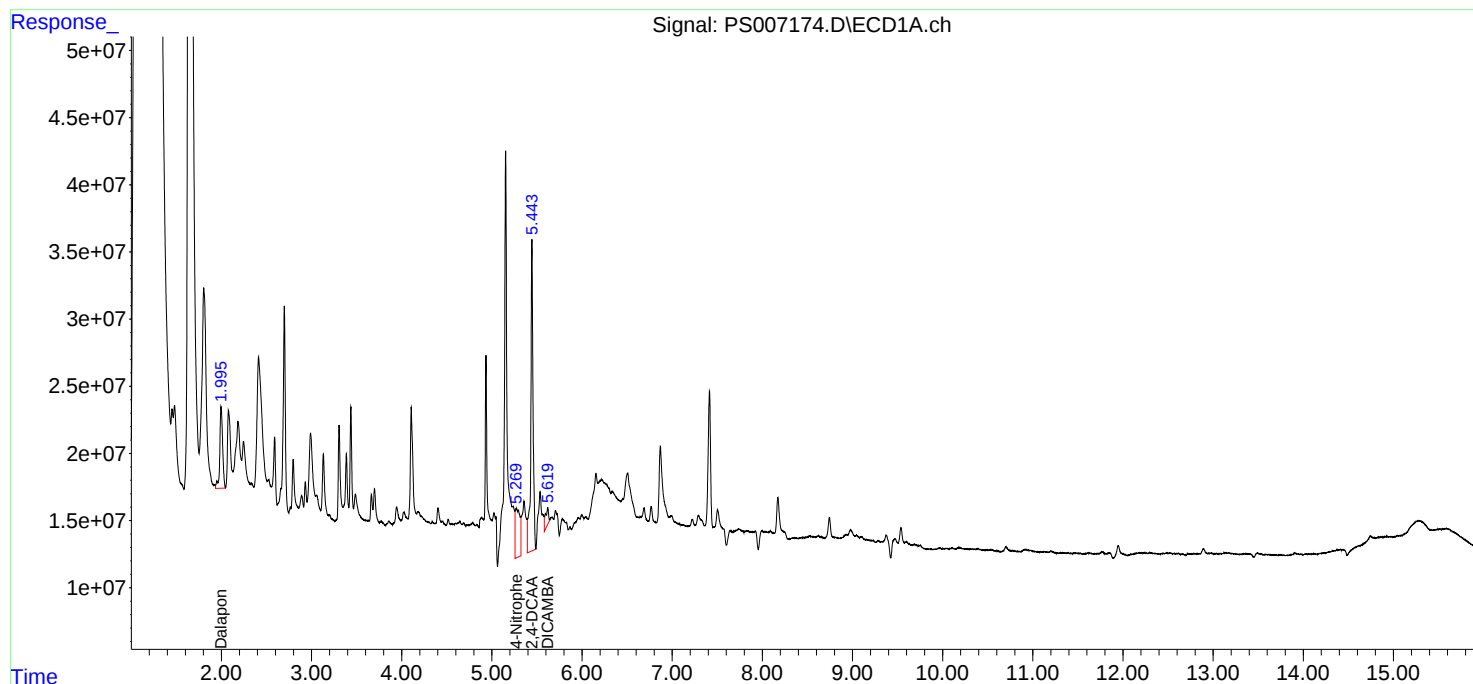


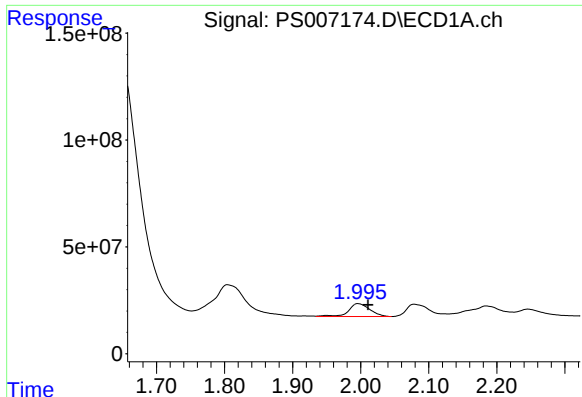

#1 Dalapon


R.T.: 1.996 min
Delta R.T.: -0.015 min
Response: 132541531
Conc: 79.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

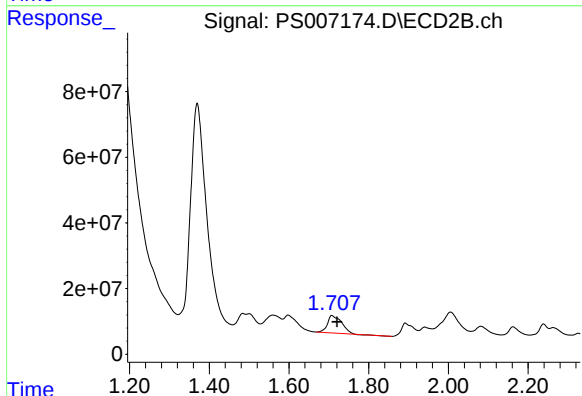


#1 Dalapon

R.T.: 1.708 min
Delta R.T.: -0.013 min
Response: 132336934
Conc: 145.42 ng/ml

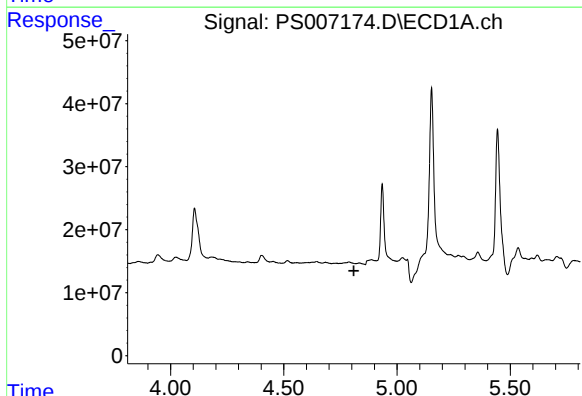


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

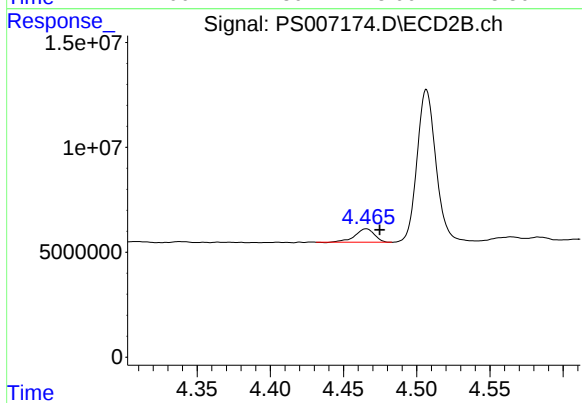

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.465 min
Delta R.T.: -0.009 min
Response: 5900326
Conc: 6.86 ng/ml

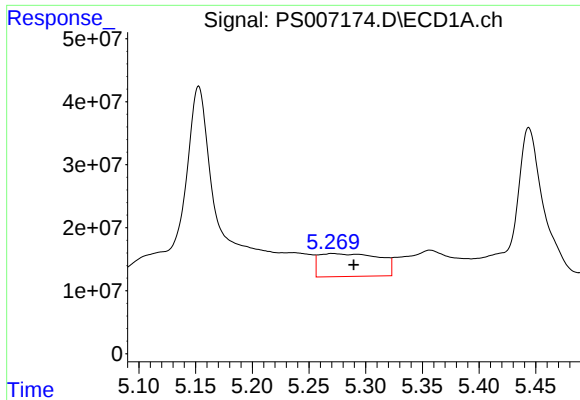

#3 4-Nitrophenol


R.T.: 5.271 min
Delta R.T.: -0.019 min
Response: 134513725
Conc: 224.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

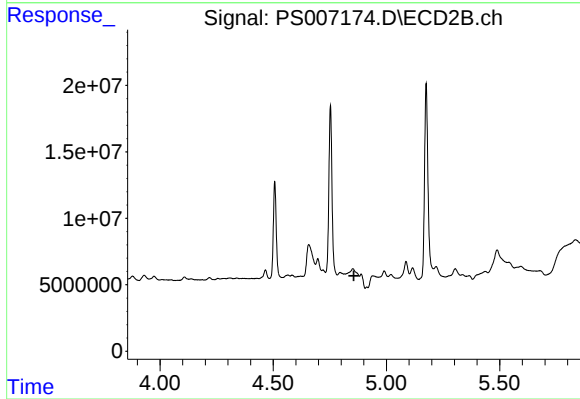


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.856 min
Response: 0
Conc: N.D.

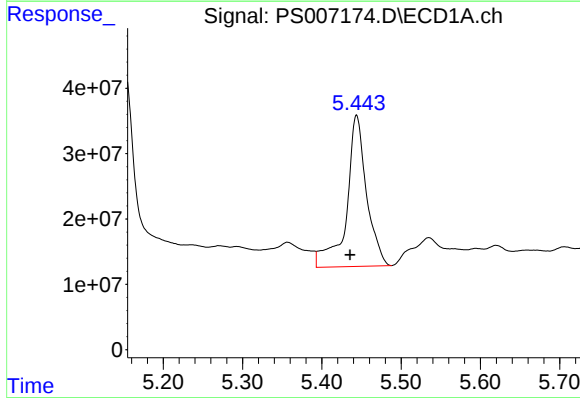


#4 2,4-DCAA

R.T.: 5.444 min
Delta R.T.: 0.008 min
Response: 406789712
Conc: 297.22 ng/ml

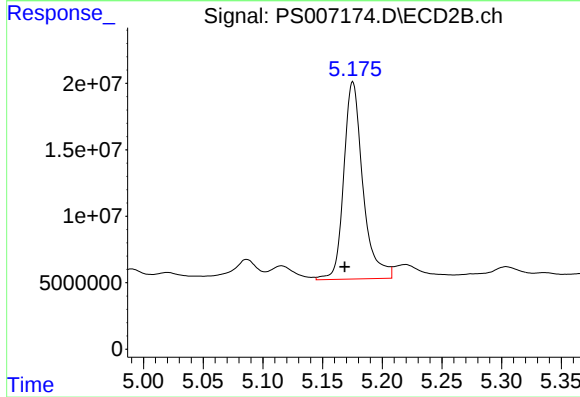

#4 2,4-DCAA


R.T.: 5.175 min
Delta R.T.: 0.007 min
Response: 165475679
Conc: 235.28 ng/ml

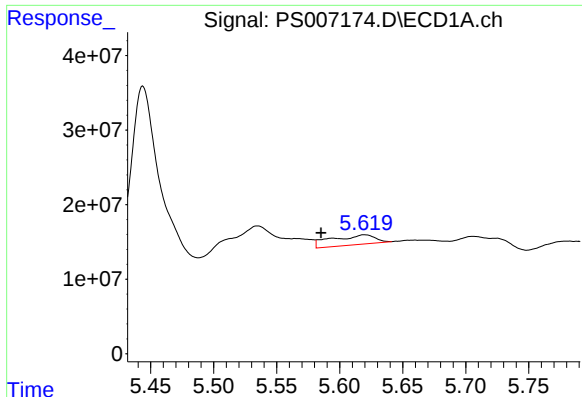

#5 DICAMBA


R.T.: 5.620 min
Delta R.T.: 0.035 min
Response: 31498564
Conc: 6.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

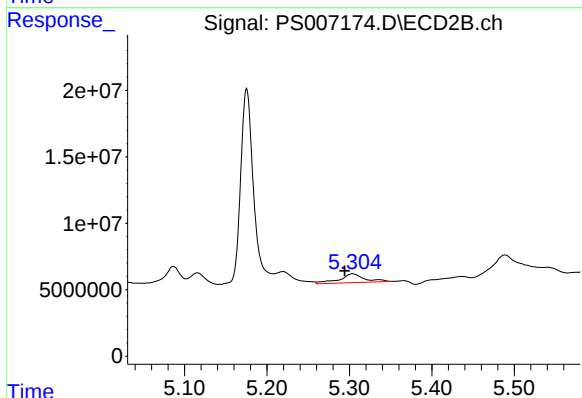


#5 DICAMBA

R.T.: 5.304 min
Delta R.T.: 0.010 min
Response: 14018351
Conc: 5.39 ng/ml

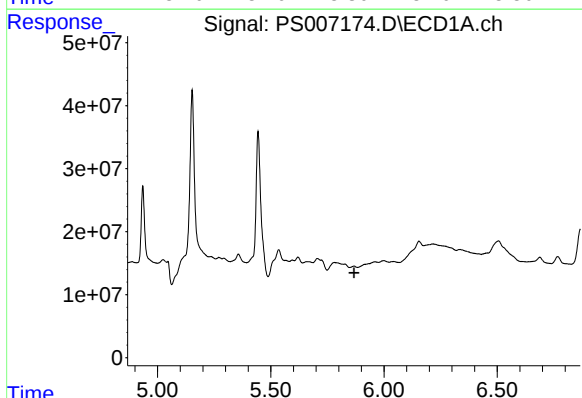


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

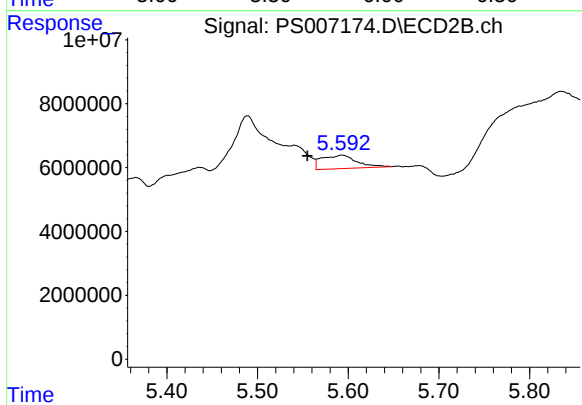

#7 MCPA


R.T.: 5.593 min
Delta R.T.: 0.038 min
Response: 11284243
Conc: 3.88 ug/ml

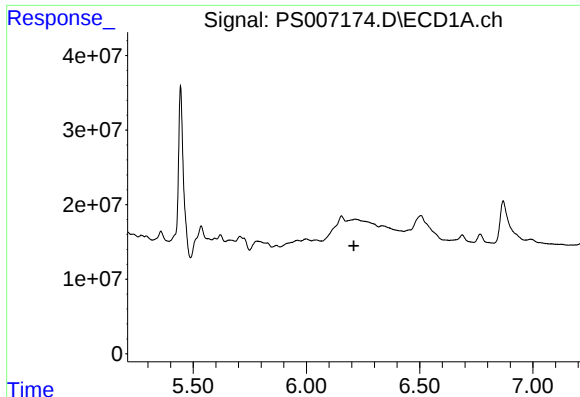

#8 DICHLORPROP


R.T.: 6.155 min
Delta R.T.: -0.055 min
Response: -3036921
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

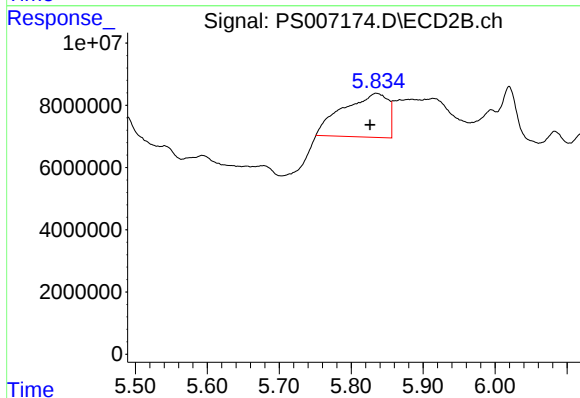


#8 DICHLORPROP

R.T.: 5.835 min
Delta R.T.: 0.009 min
Response: 61161595
Conc: 93.92 ng/ml

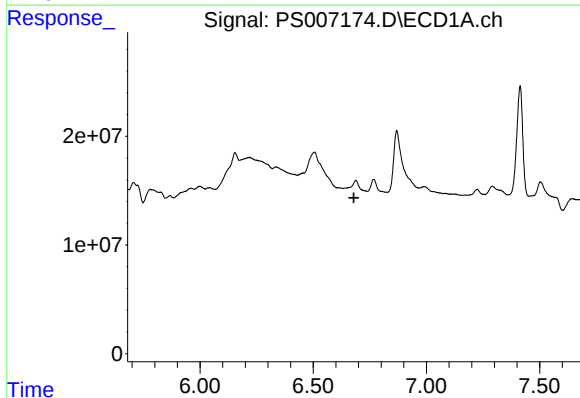


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.680 min
Response: 0
Conc: N.D.

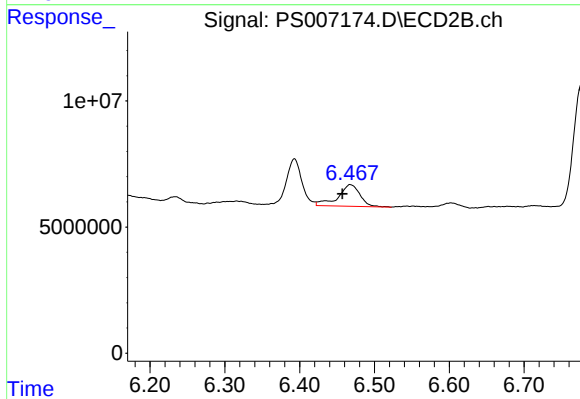

#10 Pentachlorophenol


R.T.: 6.468 min
Delta R.T.: 0.011 min
Response: 17370003
Conc: 1.81 ng/ml

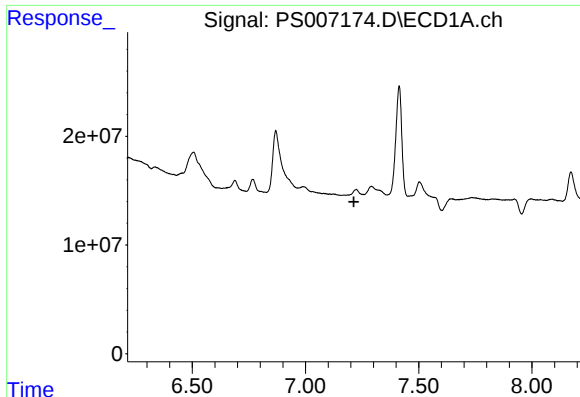

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

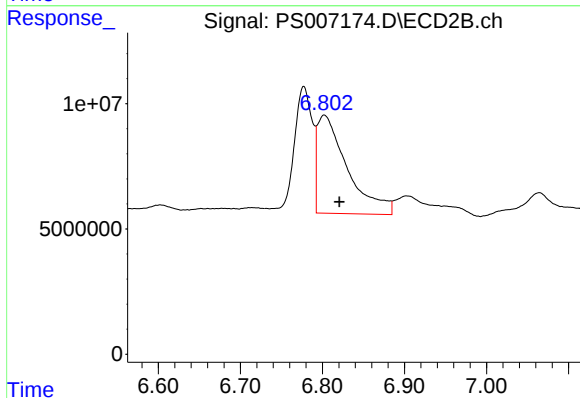


#11 2,4,5-TP (SILVEX)

R.T.: 6.802 min
Delta R.T.: -0.018 min
Response: 99612333
Conc: 26.19 ng/ml

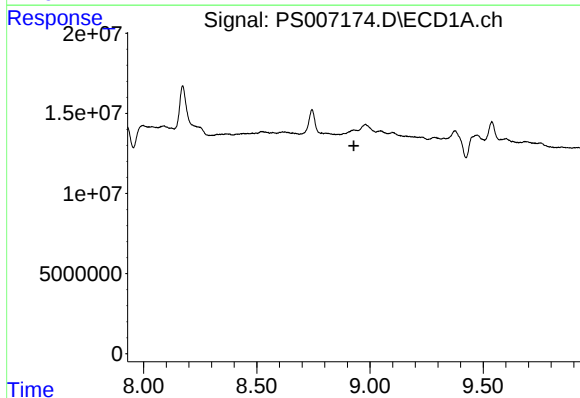


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

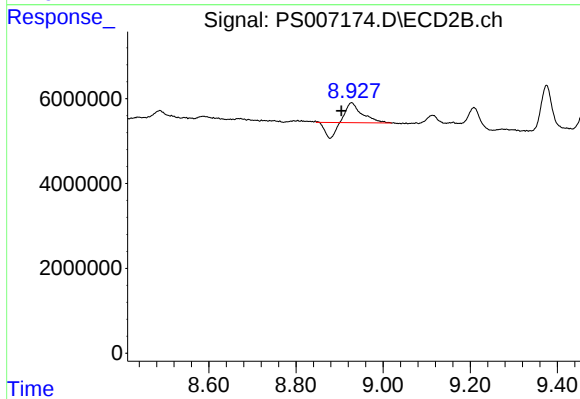

#15 Picloram


R.T.: 8.928 min
Delta R.T.: 0.023 min
Response: 6926235
Conc: 1.13 ng/ml

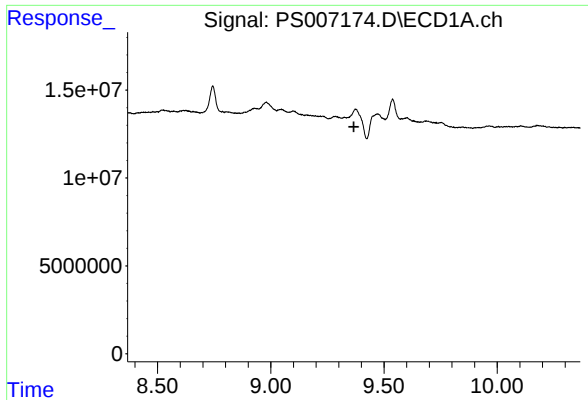

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.367 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

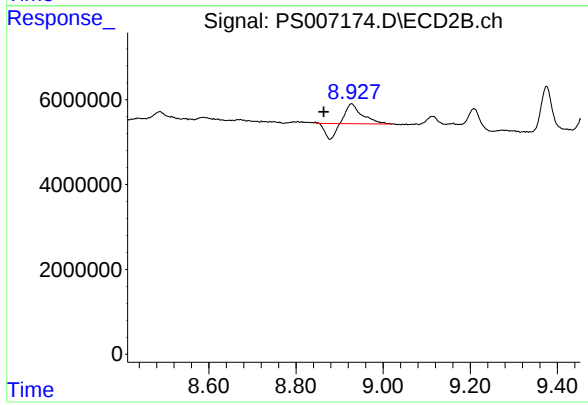

#16 DCPA

R.T.: 8.928 min
Delta R.T.: 0.064 min
Response: 6926235
Conc: 1.38 ng/ml