

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101521\
 Data File : PS017089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2021 15:17
 Operator : DD\AJ
 Sample : PB139927BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 23:58:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.745	686.1E6	298.2E6	450.315	508.643
Target Compounds							
2) T	3,5-DICHL...	0.000	5.965	0	24426661	N.D.	27.706
11) T	2,4,5-TP ...	0.000	8.557f	0	60880985	N.D.	17.389
14) T	DINOSEB	11.072f	0.000	250.2E6	0	41.071	N.D. #
15) T	Picloram	10.939	10.789	274.1E6	90887482	23.033	21.187
16) T	DCPA	0.000	10.789	0	90887482	N.D.	20.851



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101521\
Data File : PS017089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2021 15:17
Operator : DD\AJ
Sample : PB139927BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 23:58:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

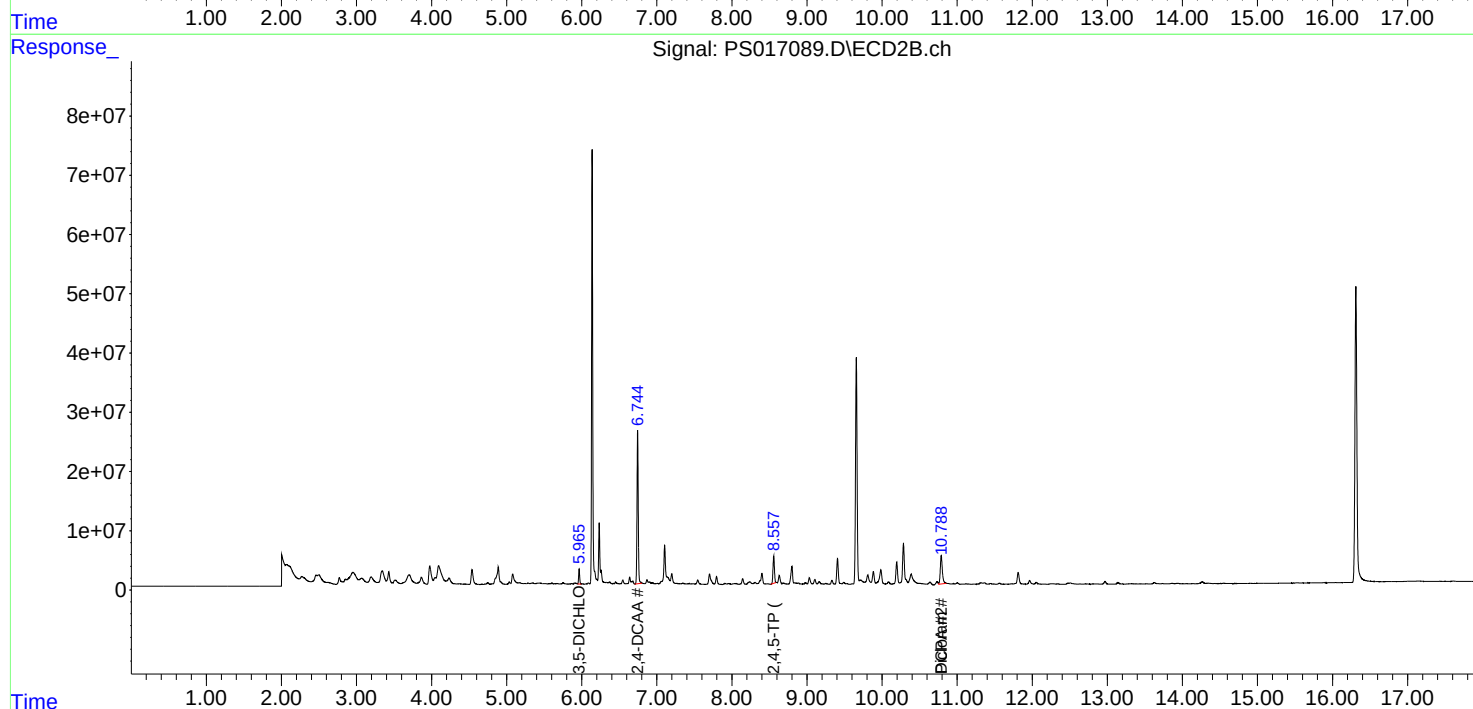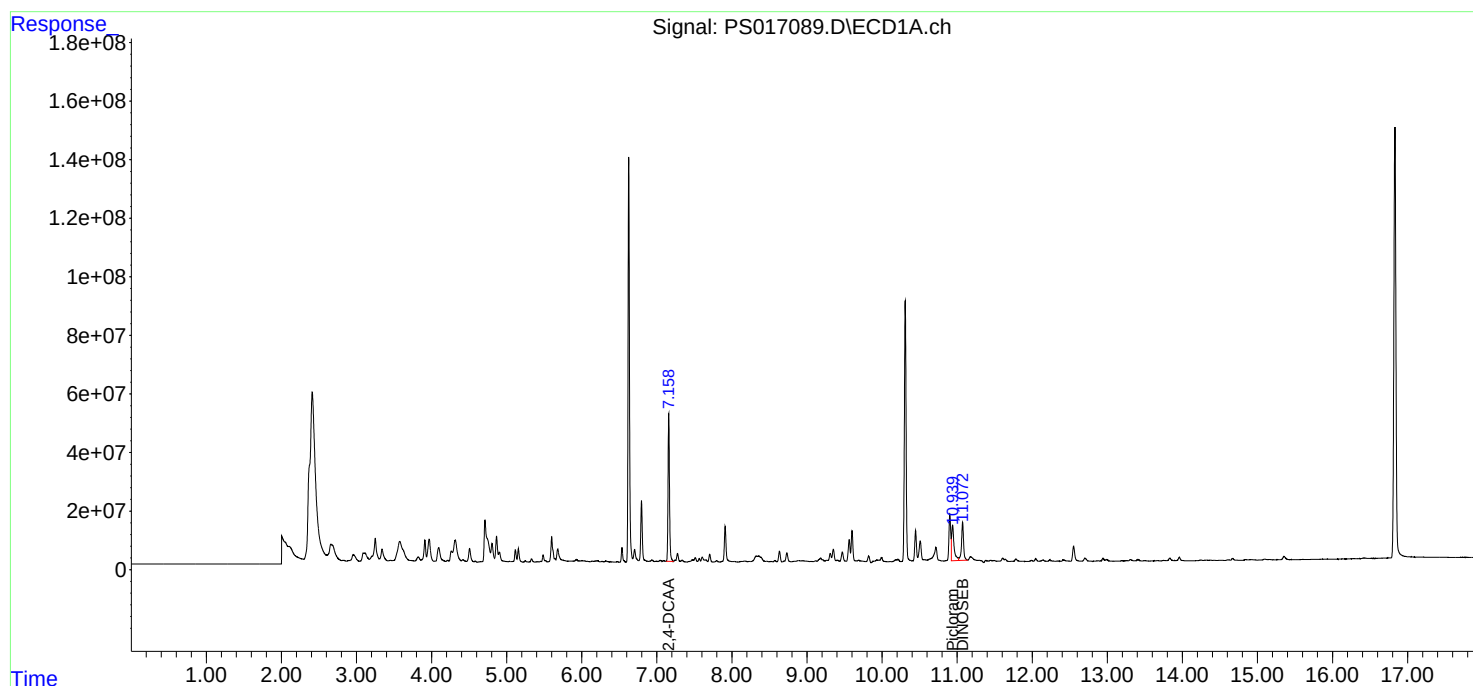


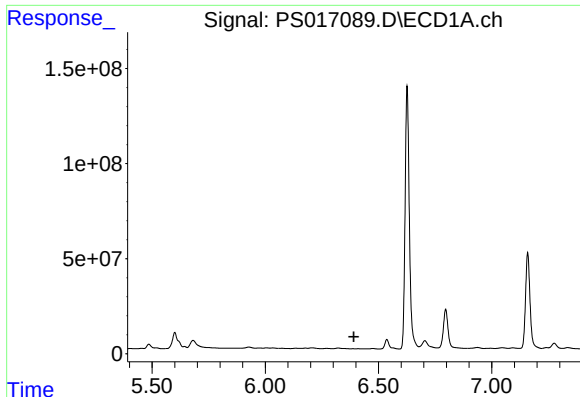

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

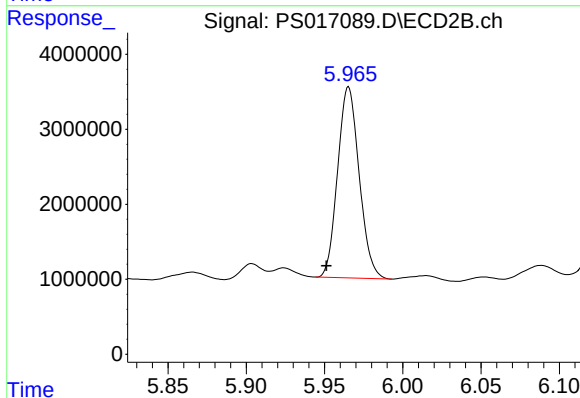


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.965 min
Delta R.T.: 0.014 min
Response: 24426661
Conc: 27.71 ng/ml

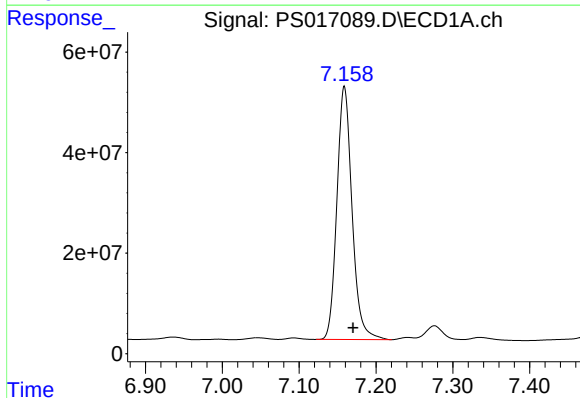


#4 2,4-DCAA

R.T.: 7.159 min
Delta R.T.: -0.012 min
Response: 686077125
Conc: 450.31 ng/ml

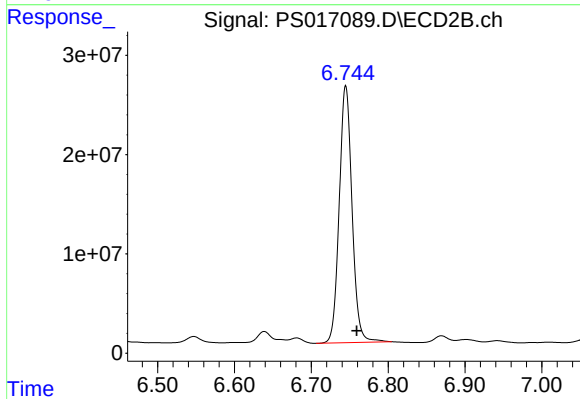

#4 2,4-DCAA


R.T.: 6.745 min
Delta R.T.: -0.014 min
Response: 298249174
Conc: 508.64 ng/ml

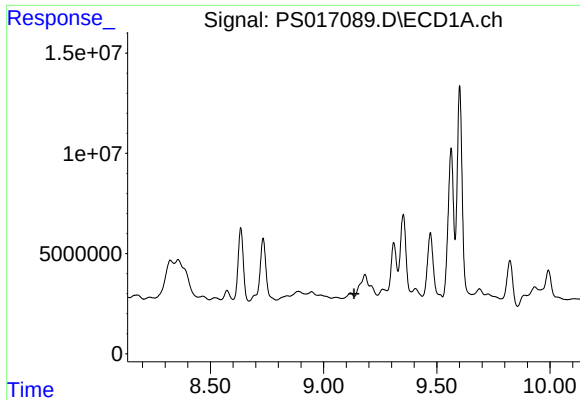

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.134 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

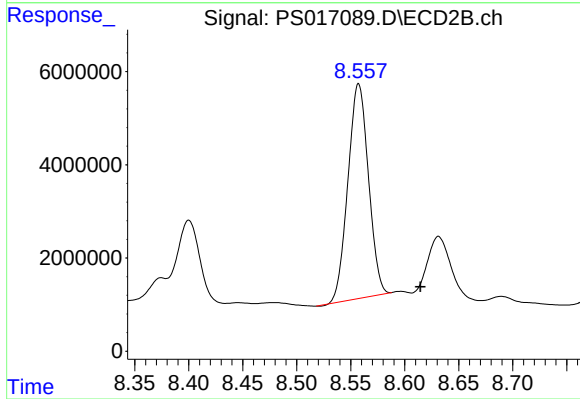


#11 2,4,5-TP (SILVEX)

R.T.: 8.557 min
Delta R.T.: -0.057 min
Response: 60880985
Conc: 17.39 ng/ml

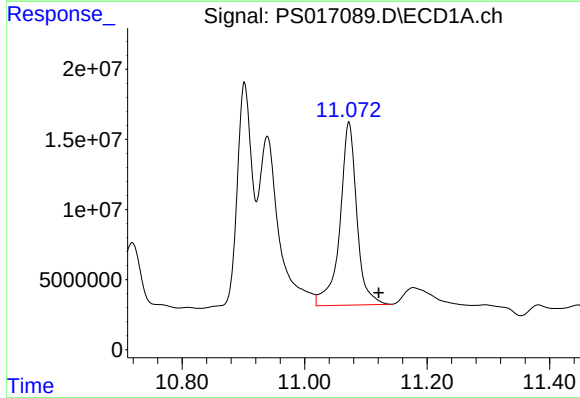


#14 DINOSEB

R.T.: 11.072 min
Delta R.T.: -0.049 min
Response: 250229435
Conc: 41.07 ng/ml

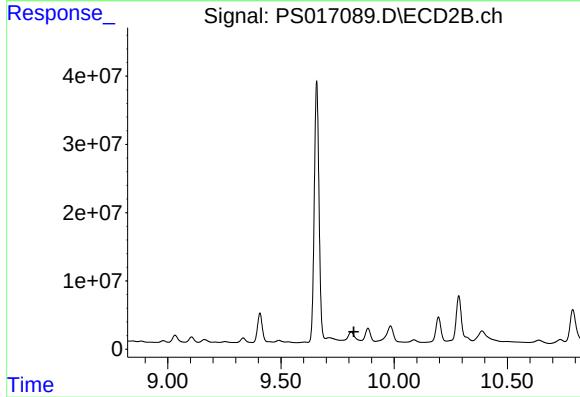

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.822 min
Response: 0
Conc: N.D.

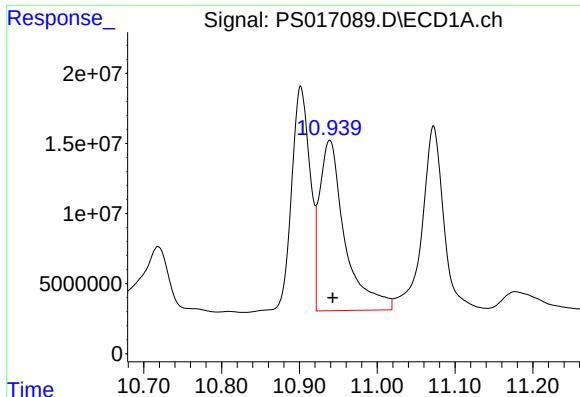

#15 Picloram


R.T.: 10.939 min
Delta R.T.: -0.004 min
Response: 274129155
Conc: 23.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

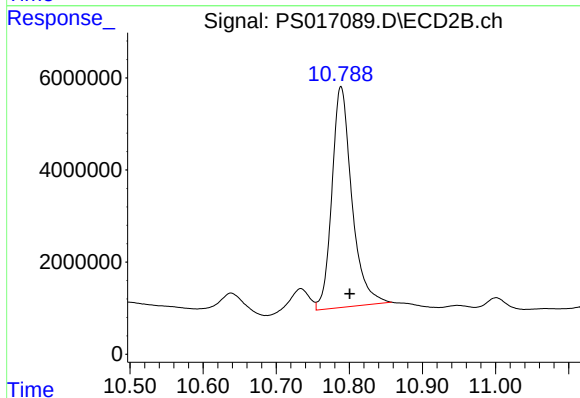


#15 Picloram

R.T.: 10.789 min
Delta R.T.: -0.012 min
Response: 90887482
Conc: 21.19 ng/ml

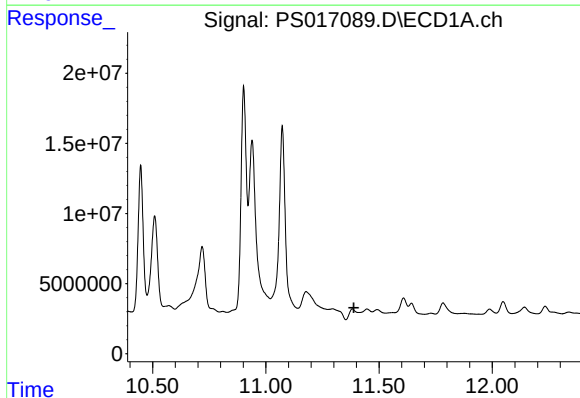

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.389 min
Response: 0
Conc: N.D.

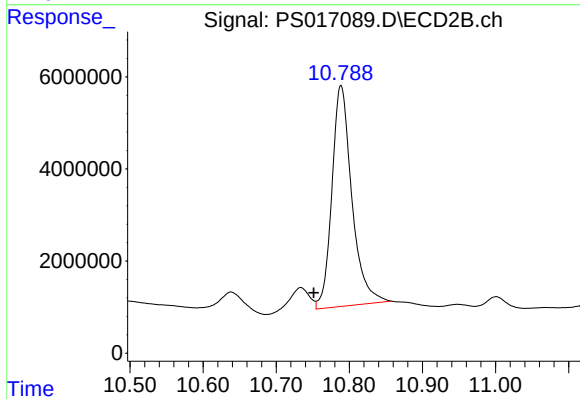

#16 DCPA

R.T.: 10.789 min
Delta R.T.: 0.037 min
Response: 90887482
Conc: 20.85 ng/ml