

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101521\
 Data File : PS017092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2021 16:29
 Operator : DD\AJ
 Sample : M4195-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 15 23:59:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.158	6.746	605.4E6	239.2E6	397.342	407.977
Target Compounds							
2) T	3,5-DICHL...	6.395	5.950	232.4E6	67360742	109.223	76.404 #
7) T	MCPA	7.625f	7.274f	272.4E6	56421474	44.038	18.529 #
11) T	2,4,5-TP ...	0.000	8.558f	0	29041250	N.D.	8.295
12) T	2,4,5-T	9.350f	0.000	139.0E6	0	16.838	N.D. #
13) T	2,4-DB	9.999	0.000	87412951	0	52.881	N.D. #
14) T	DINOSEB	11.070f	9.845	324.5E6	153.1E6	53.269	62.485
15) T	Picloram	10.898f	0.000	510.5E6	0	42.895	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101521\
Data File : PS017092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2021 16:29
Operator : DD\AJ
Sample : M4195-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 15 23:59:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

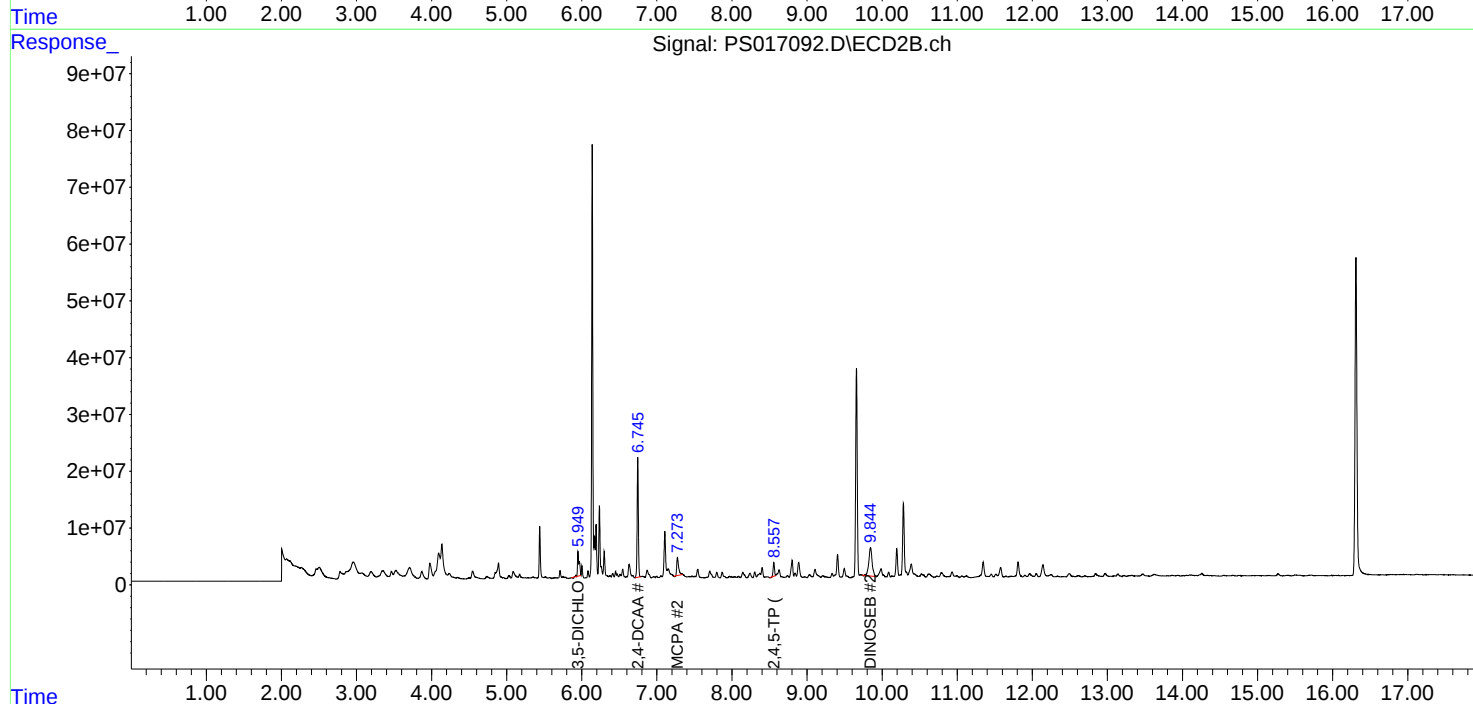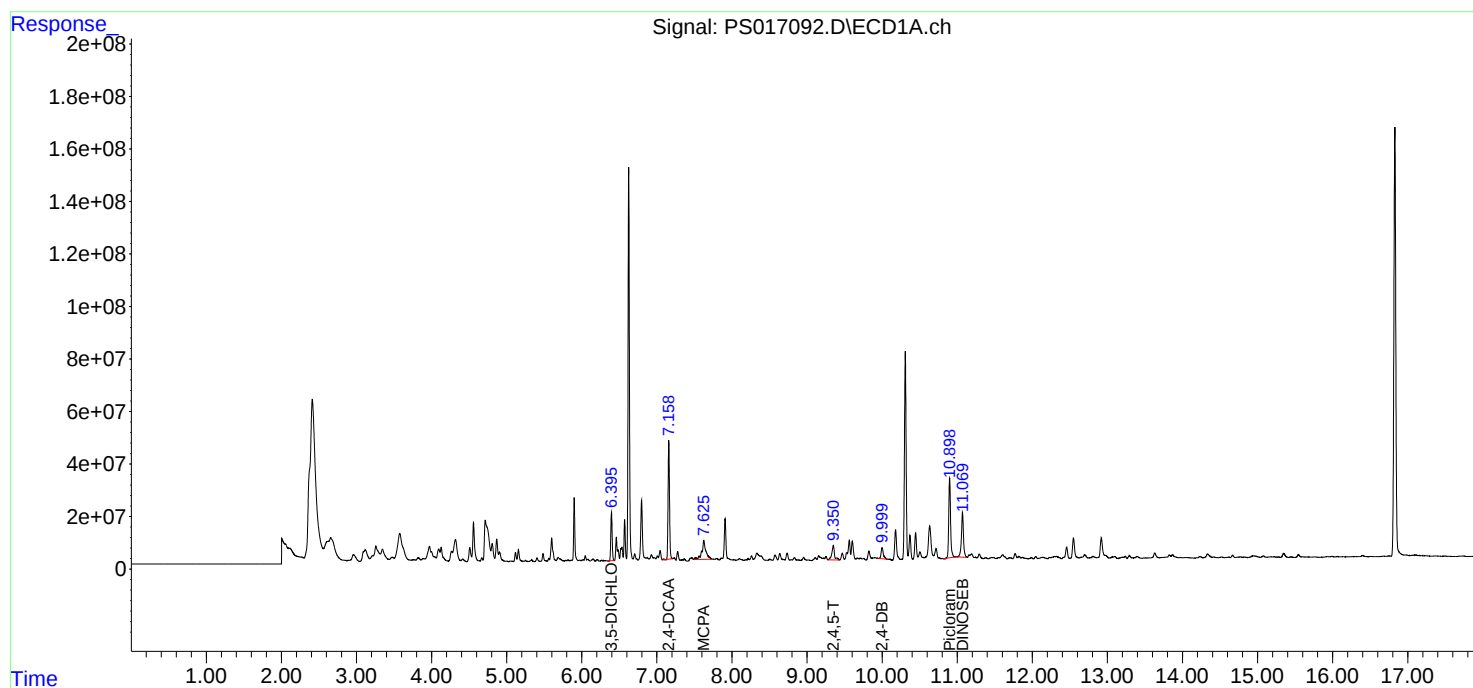


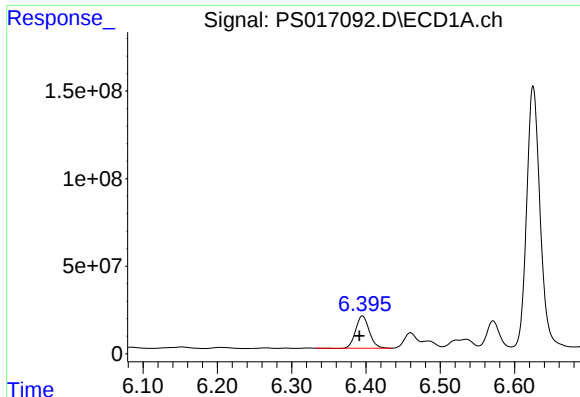

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.395 min
Delta R.T.: 0.004 min
Response: 232436903
Conc: 109.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

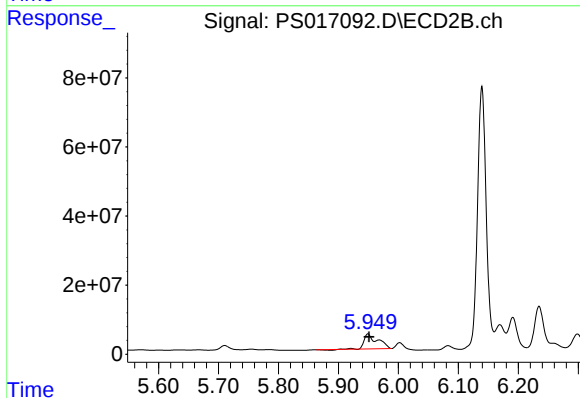


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.950 min
Delta R.T.: -0.002 min
Response: 67360742
Conc: 76.40 ng/ml

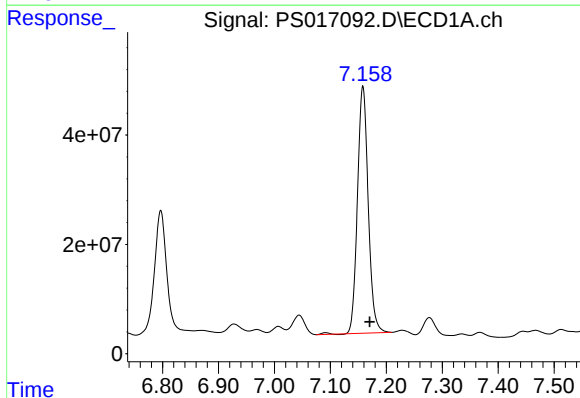


#4 2,4-DCAA

R.T.: 7.158 min
Delta R.T.: -0.012 min
Response: 605369474
Conc: 397.34 ng/ml

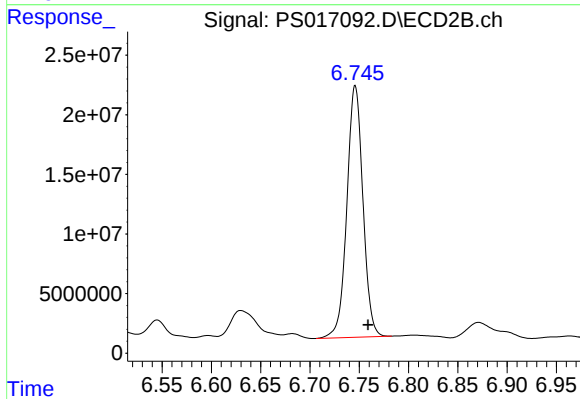

#4 2,4-DCAA


R.T.: 6.746 min
Delta R.T.: -0.013 min
Response: 239222770
Conc: 407.98 ng/ml

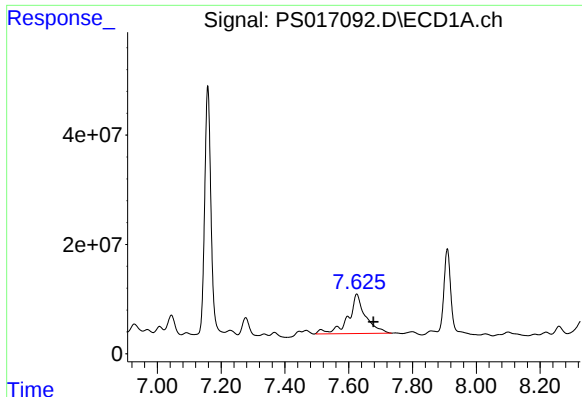

#7 MCPA


R.T.: 7.625 min
Delta R.T.: -0.052 min
Response: 272358183
Conc: 44.04 ug/ml

Instrument :
ECD_S
ClientSampleId :

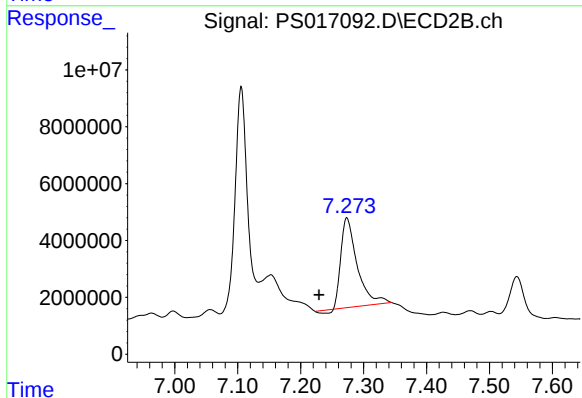


#7 MCPA

R.T.: 7.274 min
Delta R.T.: 0.044 min
Response: 56421474
Conc: 18.53 ug/ml

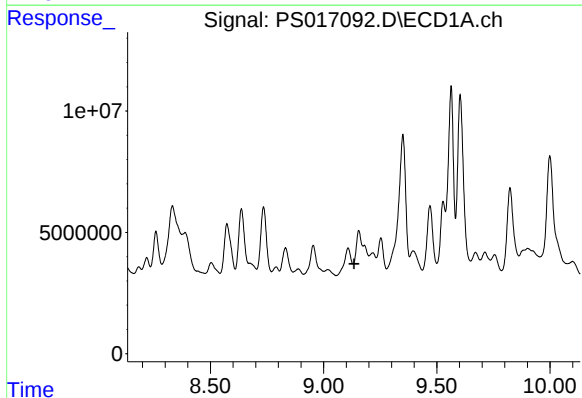


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.134 min
Response: 0
Conc: N.D.

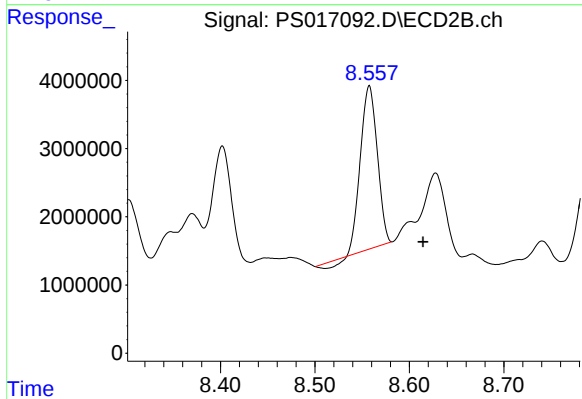

#11 2,4,5-TP (SILVEX)


R.T.: 8.558 min
Delta R.T.: -0.057 min
Response: 29041250
Conc: 8.29 ng/ml

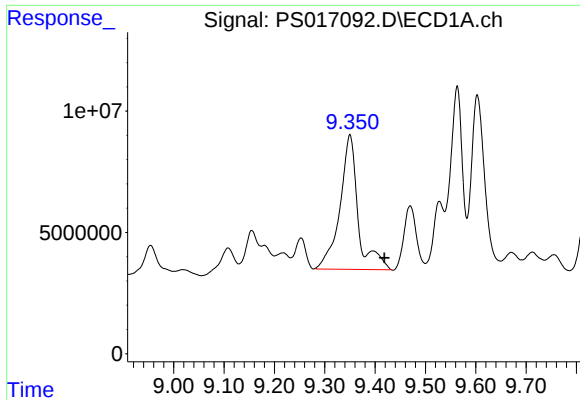

#12 2,4,5-T


R.T.: 9.350 min
Delta R.T.: -0.068 min
Response: 138976278
Conc: 16.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

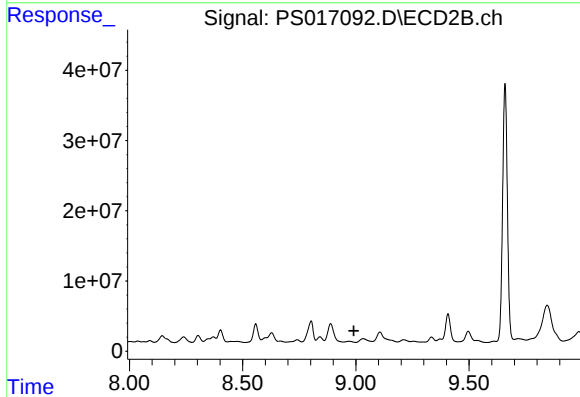


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.

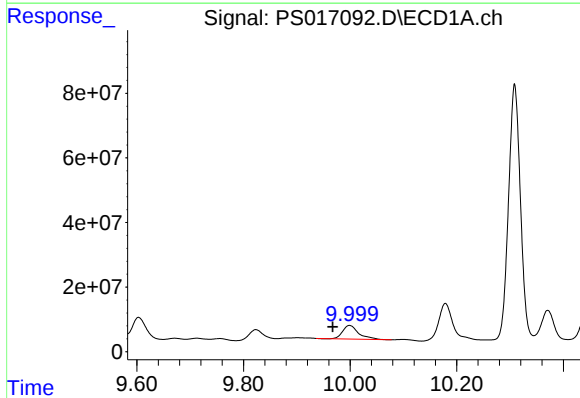


#13 2,4-DB

R.T.: 9.999 min
Delta R.T.: 0.031 min
Response: 87412951
Conc: 52.88 ng/ml

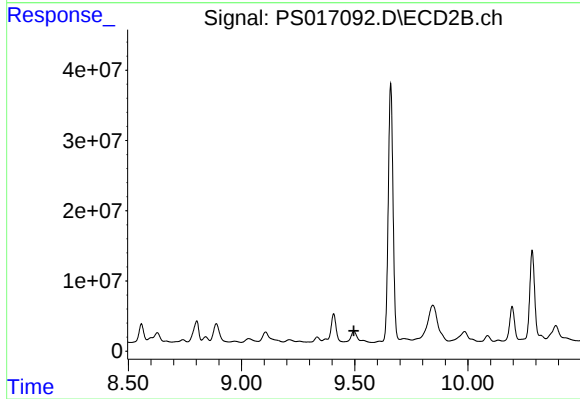

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.496 min
Response: 0
Conc: N.D.

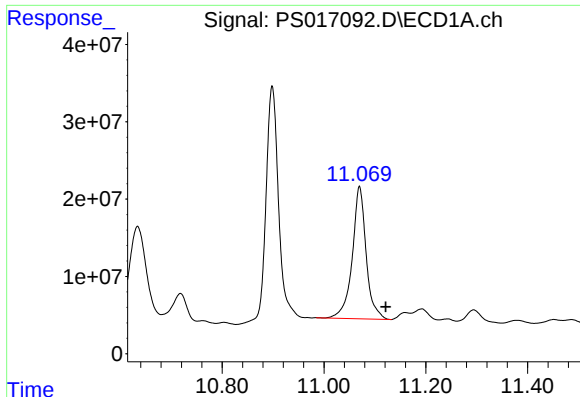

#14 DINOSEB


R.T.: 11.070 min
Delta R.T.: -0.051 min
Response: 324546793
Conc: 53.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

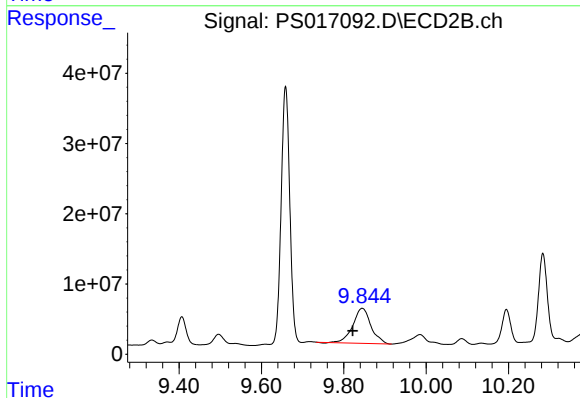


#14 DINOSEB

R.T.: 9.845 min
Delta R.T.: 0.023 min
Response: 153058637
Conc: 62.48 ng/ml

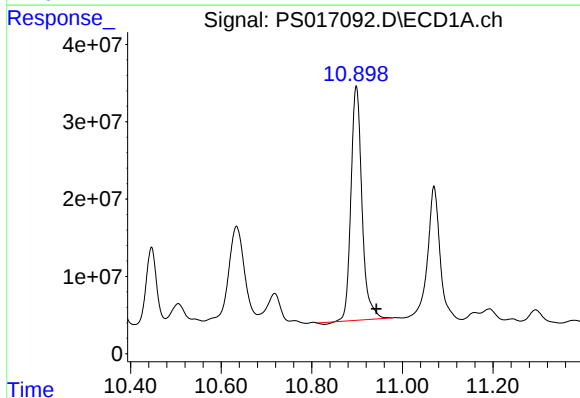

#15 Picloram

R.T.: 10.898 min
Delta R.T.: -0.044 min
Response: 510531567
Conc: 42.90 ng/ml

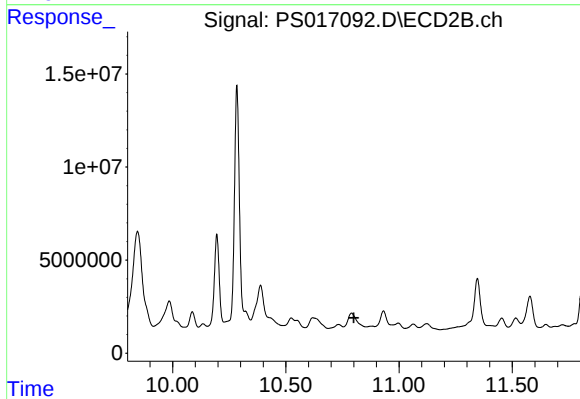

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.801 min
Response: 0
Conc: N.D.