

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101521\
 Data File : PS017095.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2021 17:42
 Operator : DD\AJ
 Sample : M4202-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 00:00:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
 Quant Title : 8080.M
 QLast Update : Tue Sep 21 01:52:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.158	6.746	610.2E6	240.7E6	400.505	410.510
Target Compounds							
2) T	3,5-DICHL...	0.000	5.966	0	25059169	N.D.	28.423
7) T	MCPA	7.629f	7.275f	218.0E6	54531335	35.248	17.908 #
11) T	2,4,5-TP ...	0.000	8.558f	0	20427215	N.D.	5.834
12) T	2,4,5-T	9.352f	0.000	109.9E6	0	13.315	N.D. #
14) T	DINOSEB	11.071f	9.843	308.6E6	142.0E6	50.647	57.965
15) T	Picloram	10.900f	0.000	529.8E6	0	44.516	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101521\
Data File : PS017095.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2021 17:42
Operator : DD\AJ
Sample : M4202-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 00:00:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092021.M
Quant Title : 8080.M
QLast Update : Tue Sep 21 01:52:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

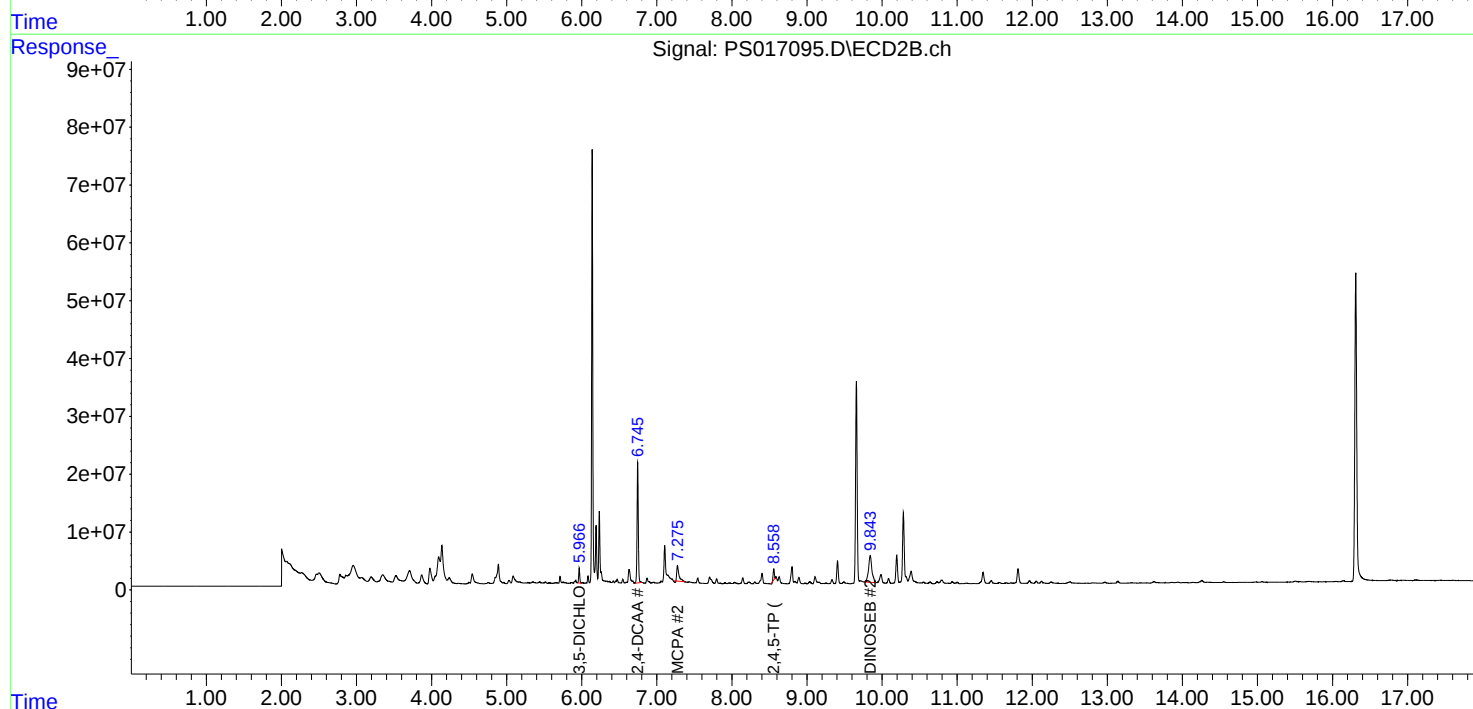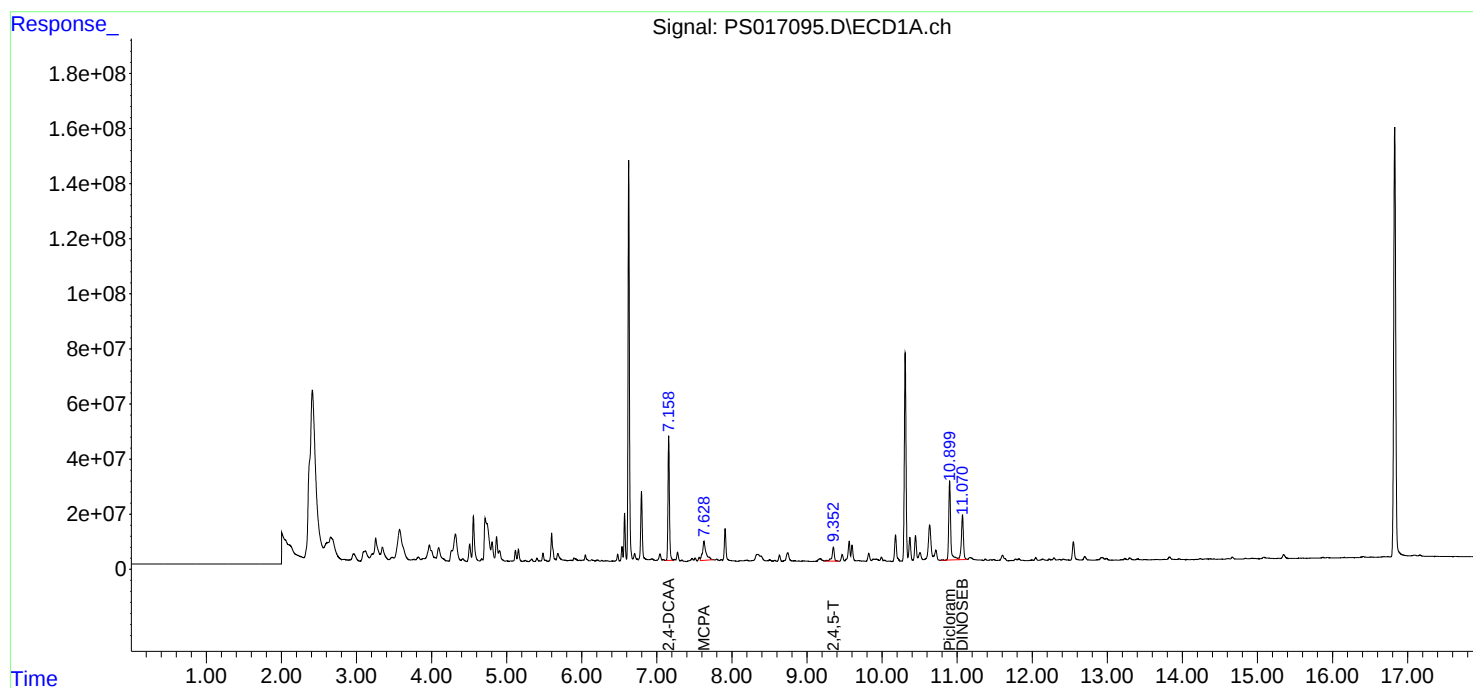


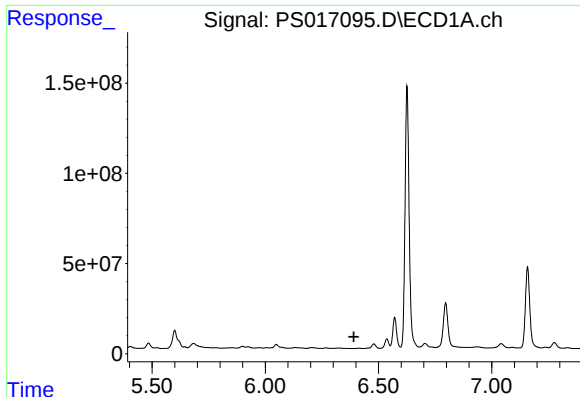

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

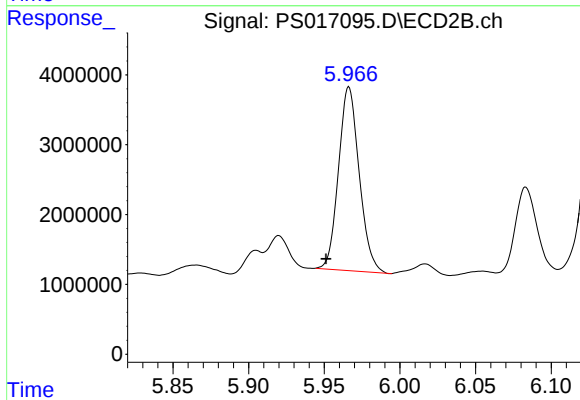


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.966 min
Delta R.T.: 0.015 min
Response: 25059169
Conc: 28.42 ng/ml

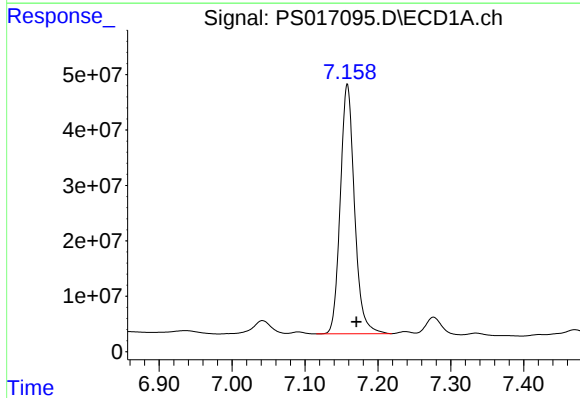


#4 2,4-DCAA

R.T.: 7.158 min
Delta R.T.: -0.012 min
Response: 610188578
Conc: 400.50 ng/ml

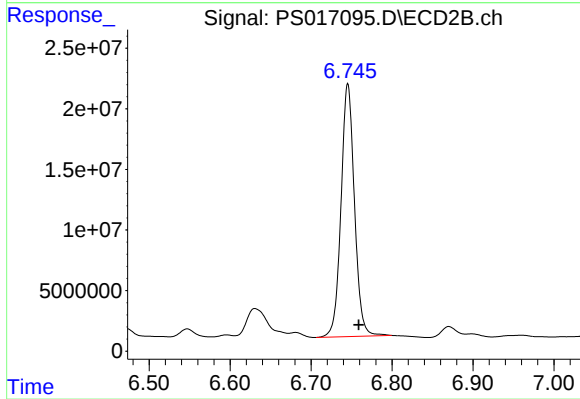

#4 2,4-DCAA


R.T.: 6.746 min
Delta R.T.: -0.013 min
Response: 240707776
Conc: 410.51 ng/ml

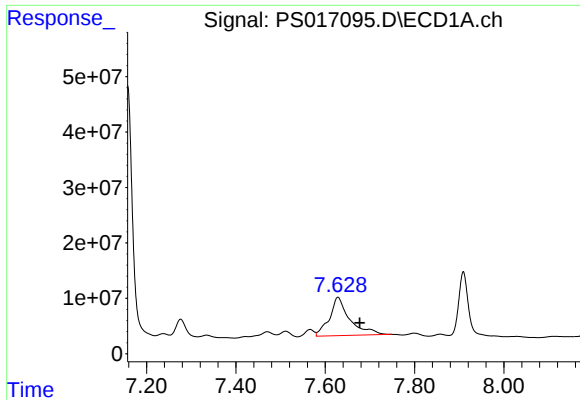

#7 MCPA


R.T.: 7.629 min
Delta R.T.: -0.049 min
Response: 217995467
Conc: 35.25 ug/ml

Instrument :
ECD_S
ClientSampleId :

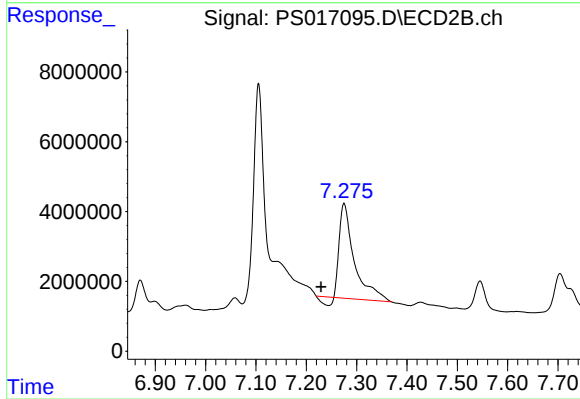


#7 MCPA

R.T.: 7.275 min
Delta R.T.: 0.046 min
Response: 54531335
Conc: 17.91 ug/ml

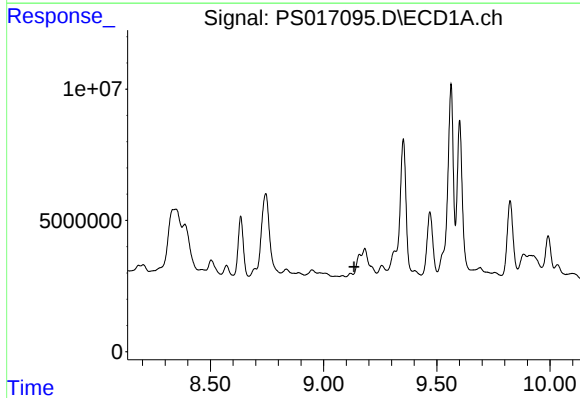


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.134 min
Response: 0
Conc: N.D.

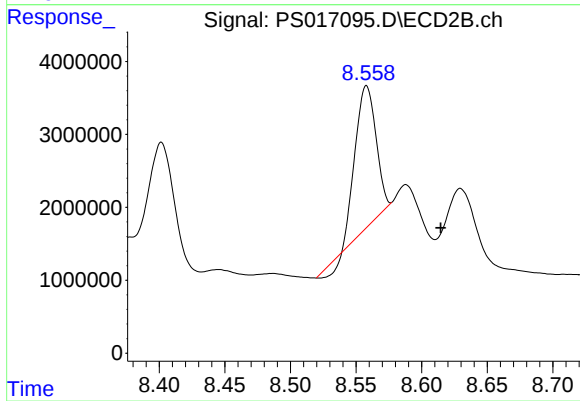

#11 2,4,5-TP (SILVEX)


R.T.: 8.558 min
Delta R.T.: -0.056 min
Response: 20427215
Conc: 5.83 ng/ml

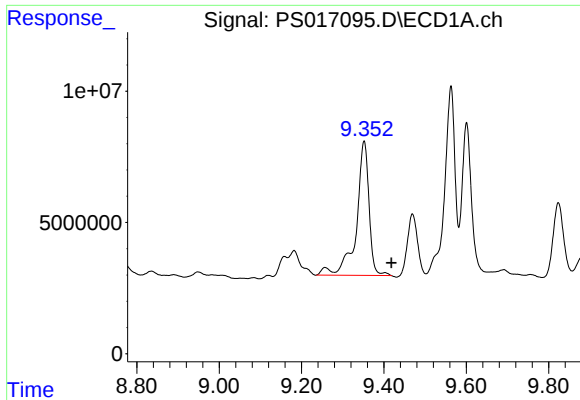

#12 2,4,5-T


R.T.: 9.352 min
Delta R.T.: -0.067 min
Response: 109899032
Conc: 13.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

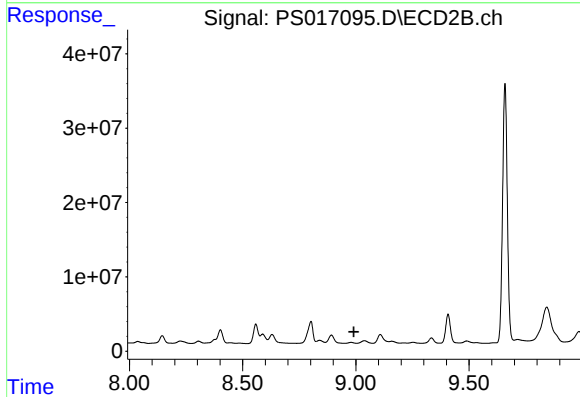


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.991 min
Response: 0
Conc: N.D.

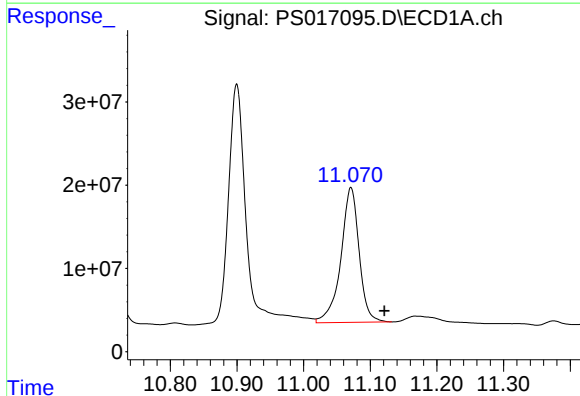


#14 DINOSEB

R.T.: 11.071 min
Delta R.T.: -0.050 min
Response: 308568150
Conc: 50.65 ng/ml

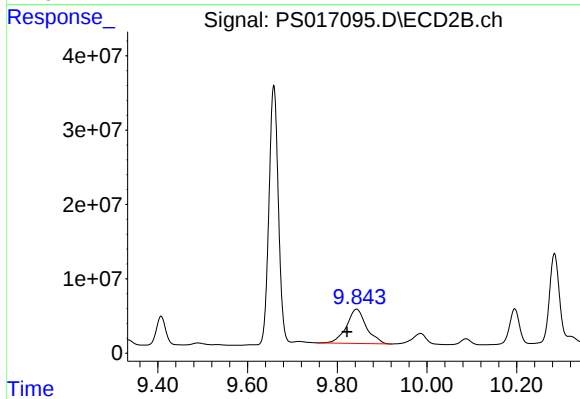

#14 DINOSEB

R.T.: 9.843 min
Delta R.T.: 0.021 min
Response: 141986995
Conc: 57.96 ng/ml

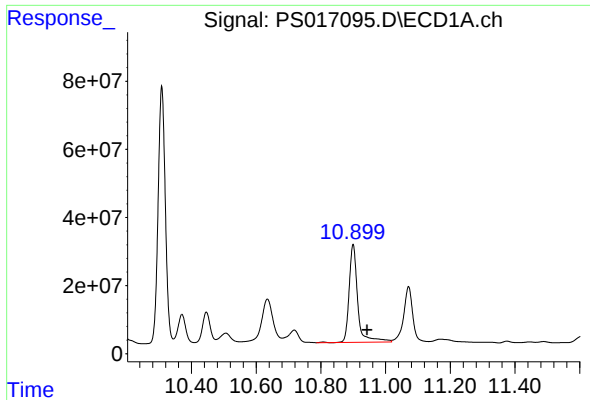

#15 Picloram


R.T.: 10.900 min

Delta R.T.: -0.043 min

Response: 529817278

Conc: 44.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

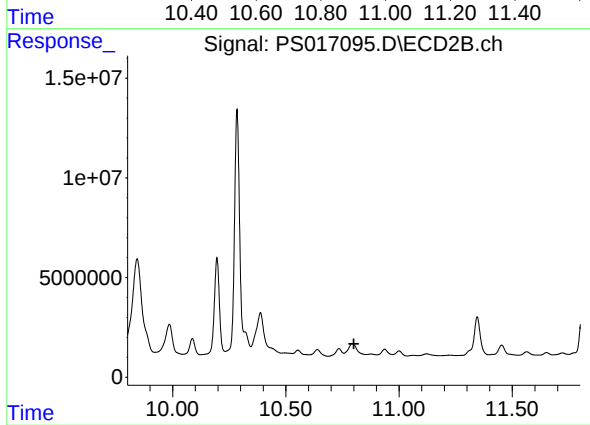

#15 Picloram

R.T.: 0.000 min

Exp R.T. : 10.801 min

Response: 0

Conc: N.D.