

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101525\
 Data File : PS032040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Oct 2025 20:16
 Operator : AR\AJ
 Sample : Q3345-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TANK-FARM-WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 03:06:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.283	7.745	1687.4E6	527.2E6	353.972	479.138 #
Target Compounds							
1) T	Dalapon	2.637f	2.684	1792.1E6	3241.6E6	231.915	862.529 #
2) T	3,5-DICHL...	6.466	0.000	1825471	0	<MDL	N.D. #
5) T	DICAMBA	7.499f	0.000	2238485	0	<MDL	N.D. #
6) T	MCP	0.000	8.043	0	9488727	N.D.	3.823
7) T	MCPA	0.000	8.243f	0	77347805	N.D.	20.504
8) T	DICHLORPROP	8.196	8.677	10301759	1176895	2.167	<MDL #
9) T	2,4-D	8.408	8.974	847735	5479957	<MDL	2.637 #
10) T	Pentachlo...	8.705	9.519	11487547	87047290	<MDL	1.680 #
11) T	2,4,5-TP ...	9.255	9.888	12685956	233.4E6	<MDL	11.626 #
12) T	2,4,5-T	9.614f	10.354f	305.1E6	93759517	12.086	5.469 #
13) T	2,4-DB	10.190f	10.866	57999105	-6746948	18.707	N.D. #
14) T	DINOSEB	0.000	11.294f	0	16255601	N.D.	1.069
16) T	DCPA	11.630	0.000	33585191	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101525\
Data File : PS032040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Oct 2025 20:16
Operator : AR\AJ
Sample : Q3345-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TANK-FARM-WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 03:06:22 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

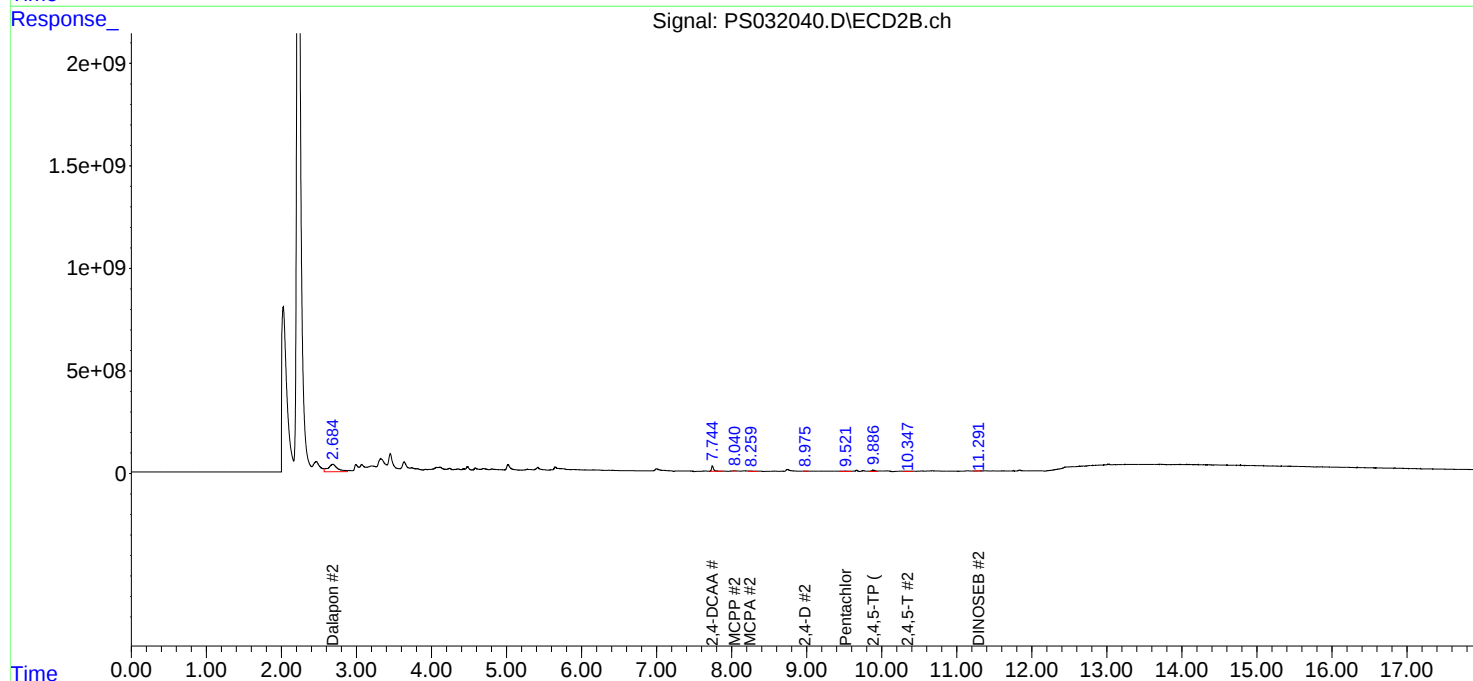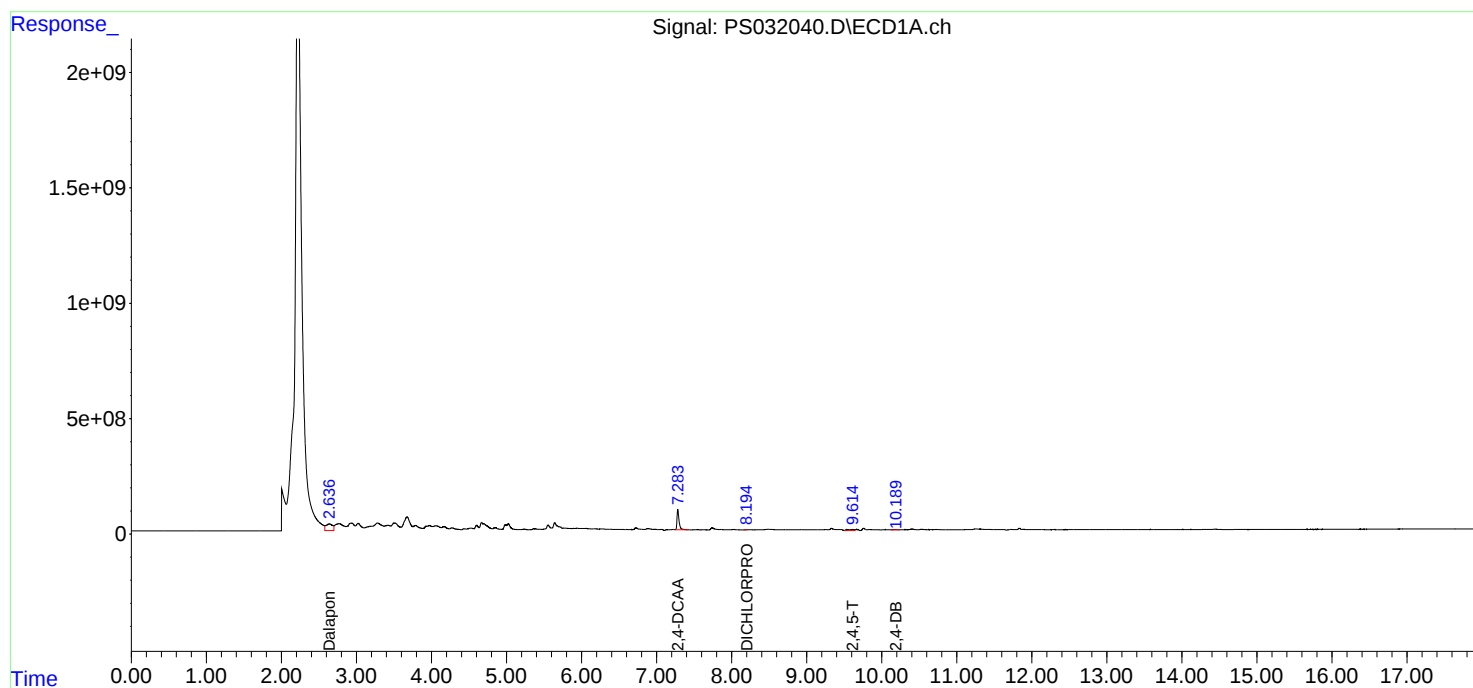


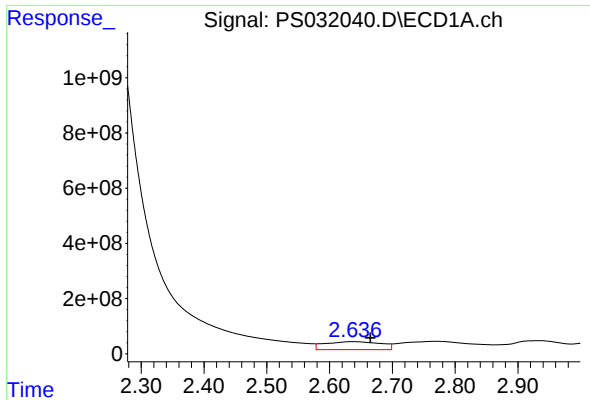

#1 Dalapon


R.T.: 2.637 min
Delta R.T.: -0.028 min
Response: 1792130473
Conc: 231.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
TANK-FARM-WATER

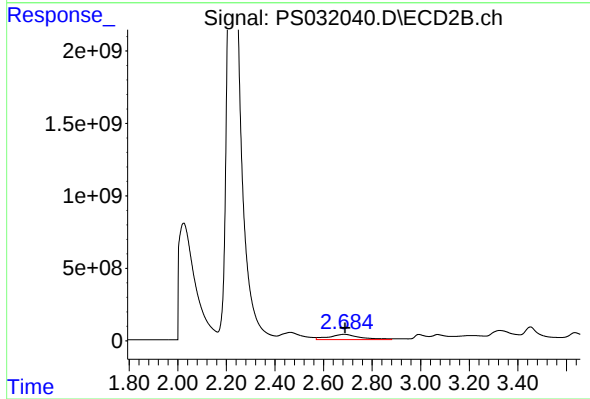


#1 Dalapon

R.T.: 2.684 min
Delta R.T.: -0.005 min
Response: 3241618401
Conc: 862.53 ng/ml

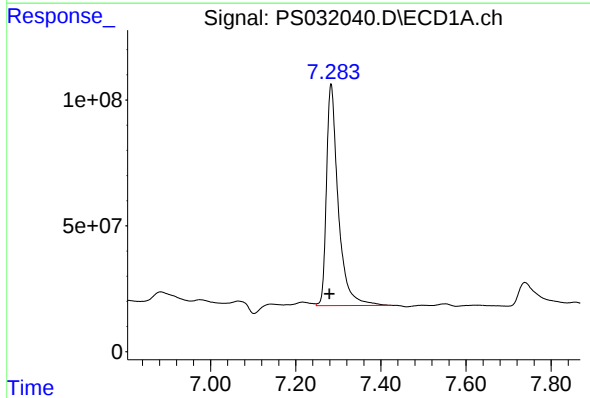


#4 2,4-DCAA

R.T.: 7.283 min
Delta R.T.: 0.003 min
Response: 1687397008
Conc: 353.97 ng/ml

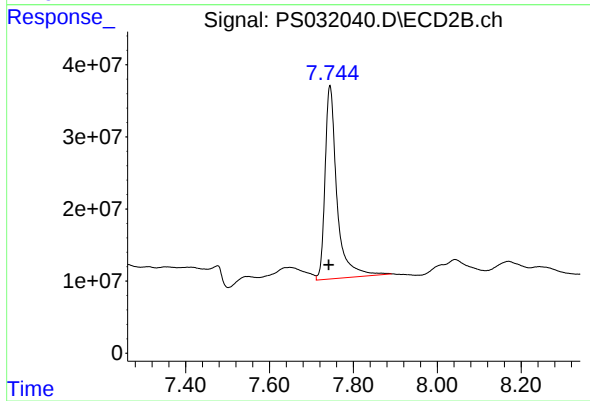

#4 2,4-DCAA


R.T.: 7.745 min
Delta R.T.: 0.004 min
Response: 527214744
Conc: 479.14 ng/ml

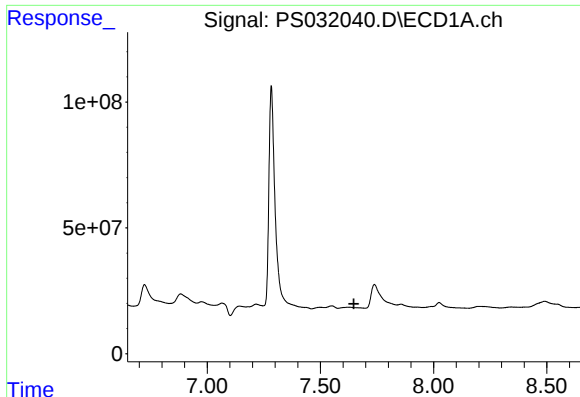

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TANK-FARM-WATER

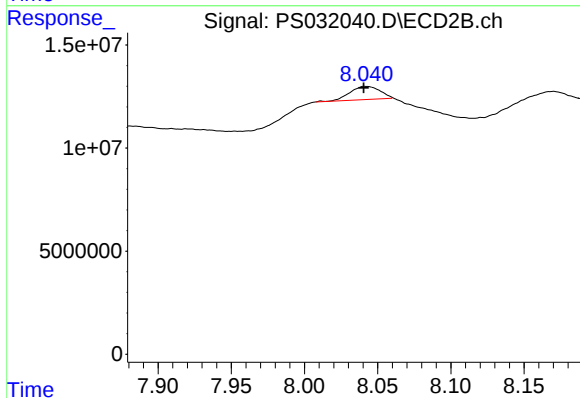


#6 MCPP

R.T.: 8.043 min
Delta R.T.: 0.002 min
Response: 9488727
Conc: 3.82 ug/ml

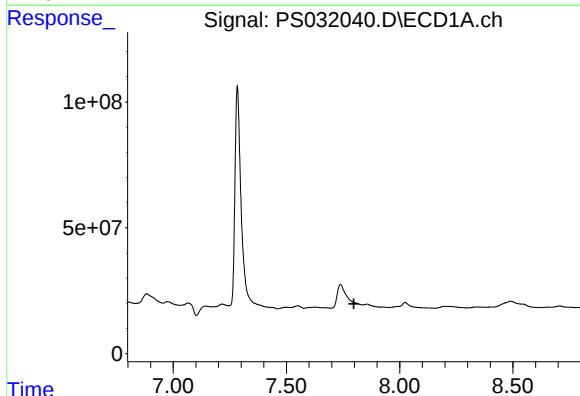


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.798 min
Response: 0
Conc: N.D.

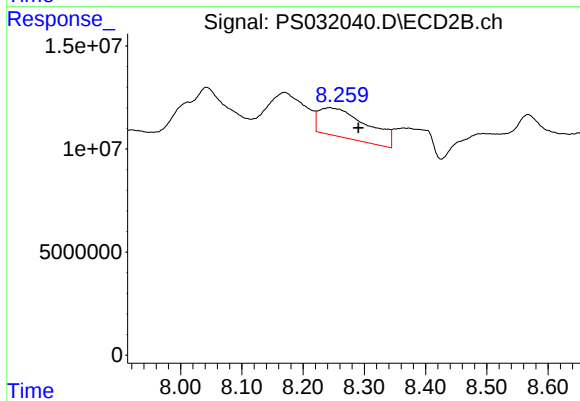

#7 MCPA


R.T.: 8.243 min
Delta R.T.: -0.047 min
Response: 77347805
Conc: 20.50 ug/ml

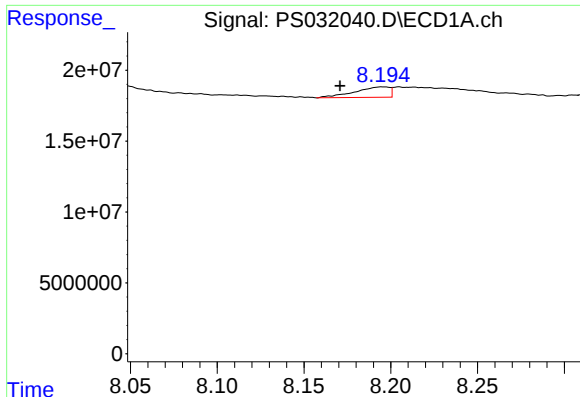

#8 DICHLORPROP


R.T.: 8.196 min
Delta R.T.: 0.025 min
Response: 10301759
Conc: 2.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
TANK-FARM-WATER

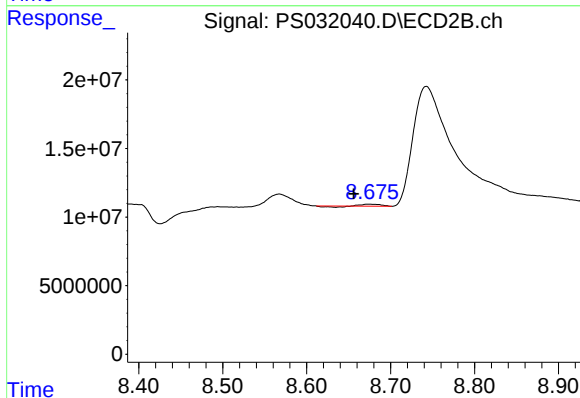


#8 DICHLORPROP

R.T.: 8.677 min
Delta R.T.: 0.021 min
Response: 1176895
Conc: N.D.

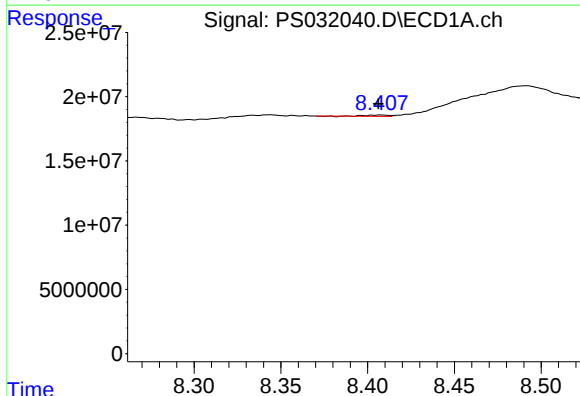


#9 2,4-D

R.T.: 8.408 min
Delta R.T.: 0.001 min
Response: 847735
Conc: N.D.

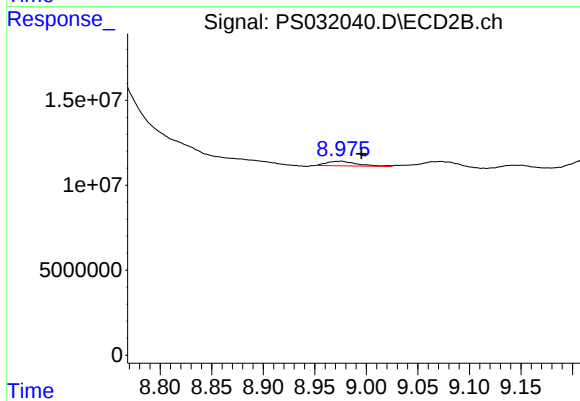

#9 2,4-D


R.T.: 8.974 min
Delta R.T.: -0.022 min
Response: 5479957
Conc: 2.64 ng/ml

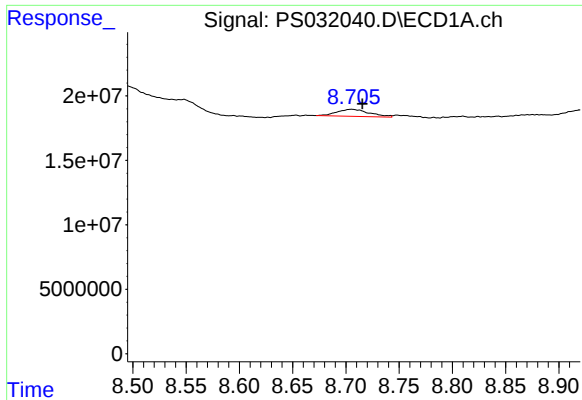

#10 Pentachlorophenol


R.T.: 8.705 min
Delta R.T.: -0.010 min
Response: 11487547
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TANK-FARM-WATER

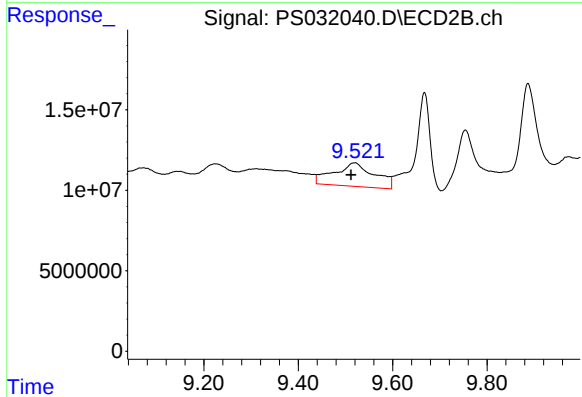


#10 Pentachlorophenol

R.T.: 9.519 min
Delta R.T.: 0.007 min
Response: 87047290
Conc: 1.68 ng/ml

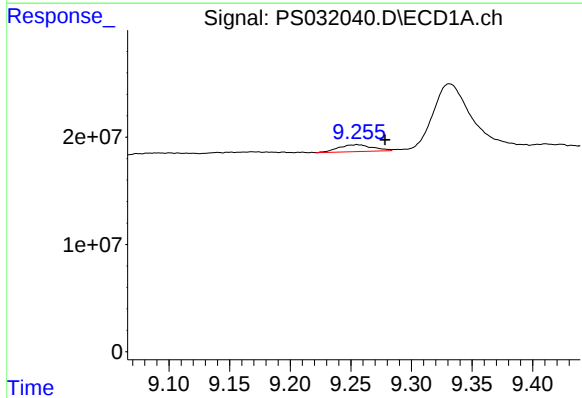


#11 2,4,5-TP (SILVEX)

R.T.: 9.255 min
Delta R.T.: -0.023 min
Response: 12685956
Conc: N.D.

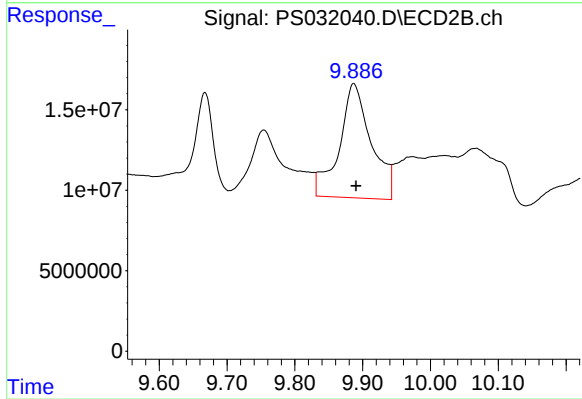

#11 2,4,5-TP (SILVEX)


R.T.: 9.888 min
Delta R.T.: -0.003 min
Response: 233398791
Conc: 11.63 ng/ml

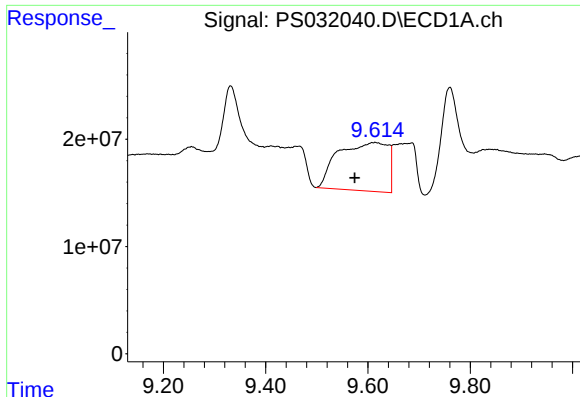

#12 2,4,5-T


R.T.: 9.614 min
Delta R.T.: 0.040 min
Response: 305108011
Conc: 12.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
TANK-FARM-WATER

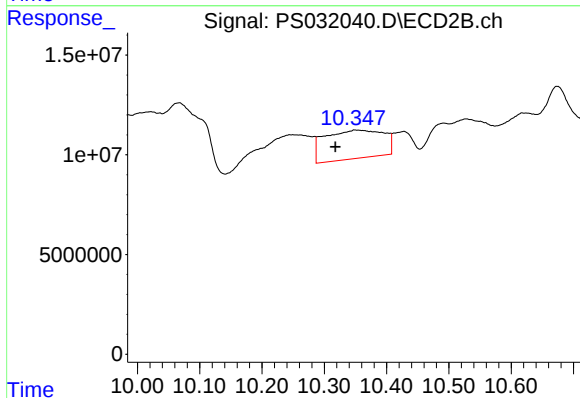


#12 2,4,5-T

R.T.: 10.354 min
Delta R.T.: 0.036 min
Response: 93759517
Conc: 5.47 ng/ml

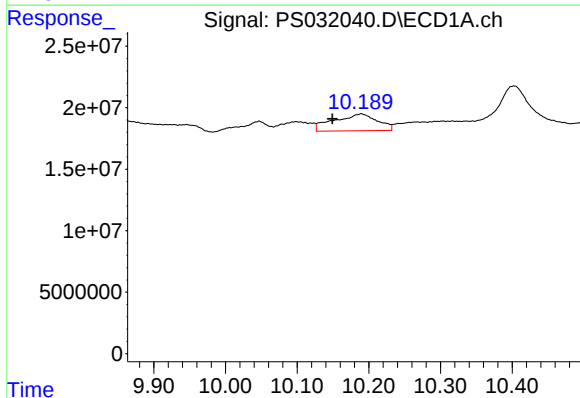


#13 2,4-DB

R.T.: 10.190 min
Delta R.T.: 0.041 min
Response: 57999105
Conc: 18.71 ng/ml

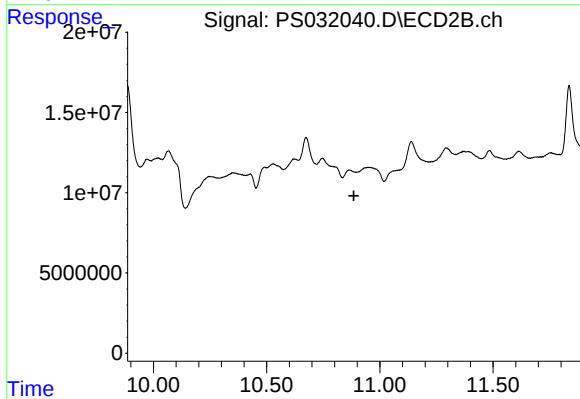

#13 2,4-DB


R.T.: 10.866 min
Delta R.T.: -0.019 min
Response: -6746948
Conc: N.D.

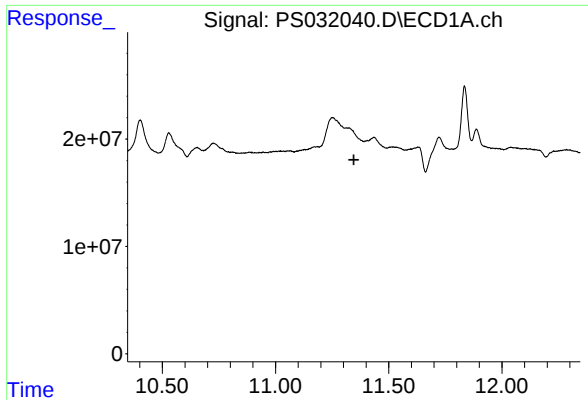

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TANK-FARM-WATER

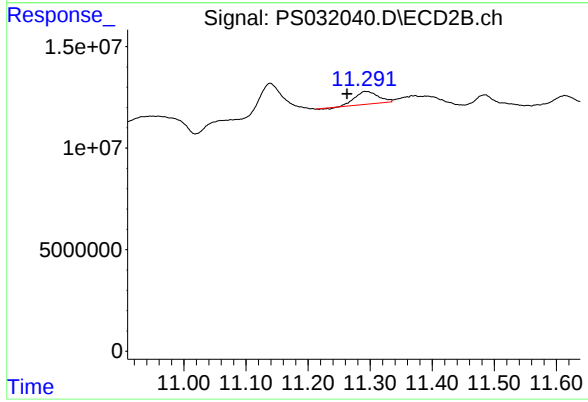

#14 DINOSEB

R.T.: 11.294 min
Delta R.T.: 0.032 min
Response: 16255601
Conc: 1.07 ng/ml