

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101525\
 Data File : PS032051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2025 01:32
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 03:12:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.281	7.747	1726.2E6	474.3E6	362.120	431.062
Target Compounds							
1) T	Dalapon	2.699f	2.646f	9343502	59610688	1.209	15.861 #
2) T	3,5-DICHL...	6.440	0.000	15410369	0	2.189	N.D. #
3) T	4-Nitroph...	7.067	0.000	2582182	0	1.935	N.D. #
7) T	MCPA	7.749f	8.244f	21723901	25564302	1.476	6.777 #
8) T	DICHLORPROP	8.183	0.000	5683297	0	1.195	N.D. #
10) T	Pentachlo...	8.701	9.510	11396148	10266257	<MDL	<MDL #
11) T	2,4,5-TP ...	9.285	9.862f	22802082	2145435	<MDL	<MDL #
12) T	2,4,5-T	9.608f	0.000	5573531	0	<MDL	N.D. #
14) T	DINOSEB	11.350	0.000	12510203	0	<MDL	N.D. #
15) T	Picloram	11.166	12.356	27672826	15125201	1.174	<MDL #
16) T	DCPA	11.647	0.000	8760927	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101525\
Data File : PS032051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2025 01:32
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 03:12:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

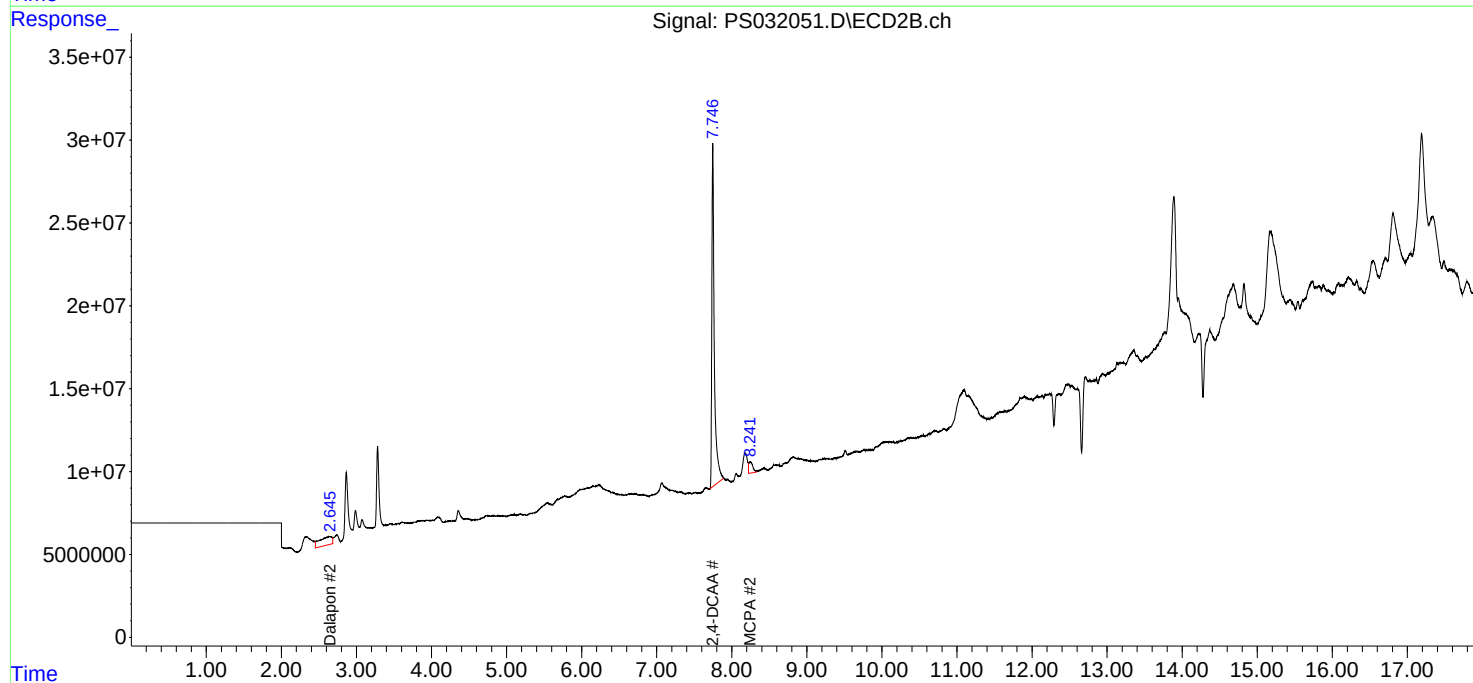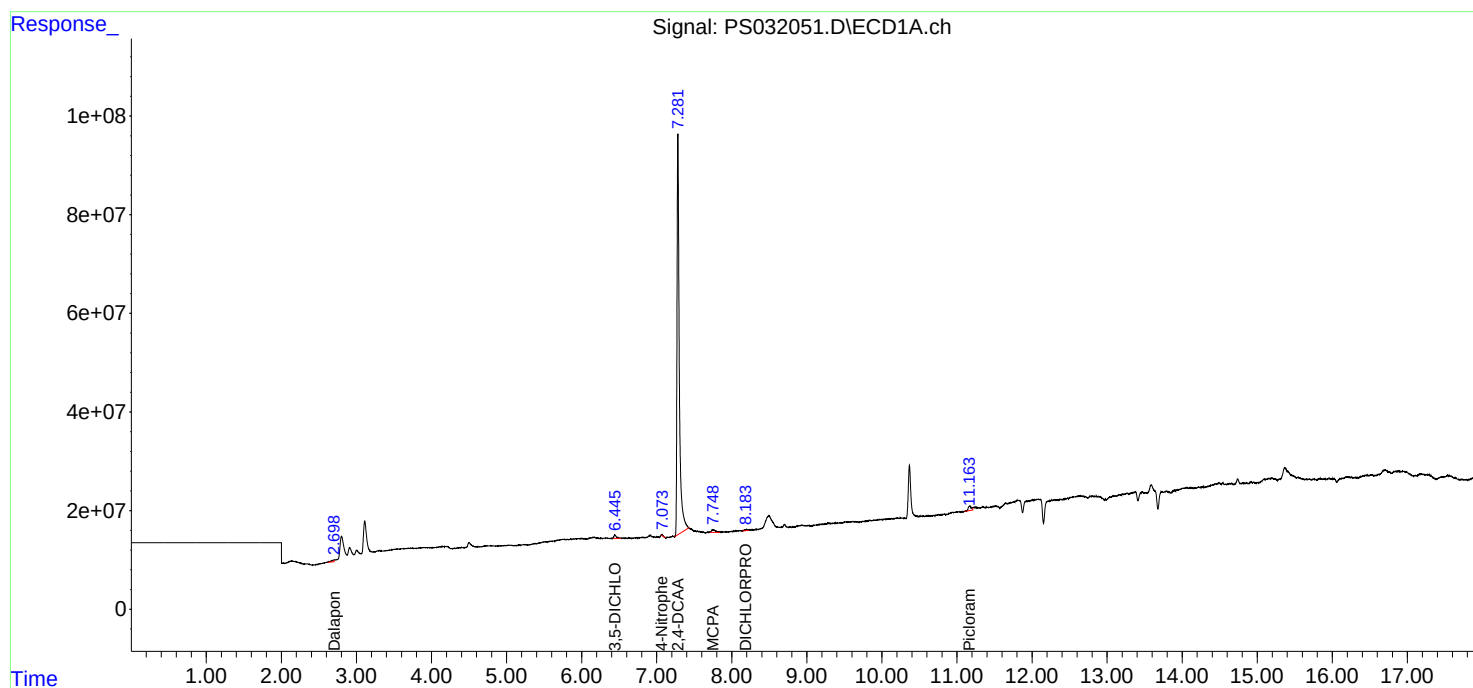


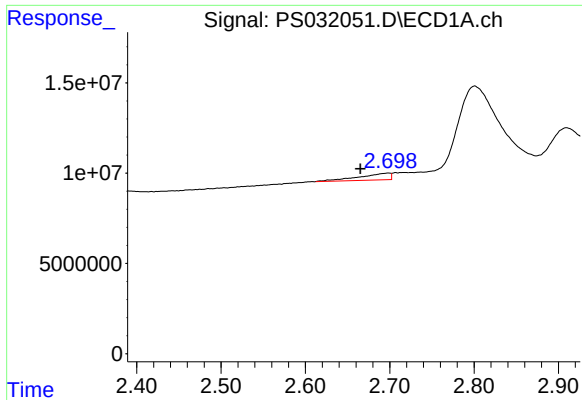

#1 Dalapon


R.T.: 2.699 min
Delta R.T.: 0.034 min
Response: 9343502
Conc: 1.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

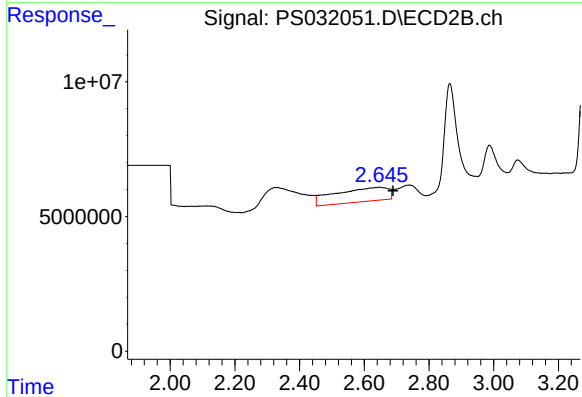


#1 Dalapon

R.T.: 2.646 min
Delta R.T.: -0.043 min
Response: 59610688
Conc: 15.86 ng/ml

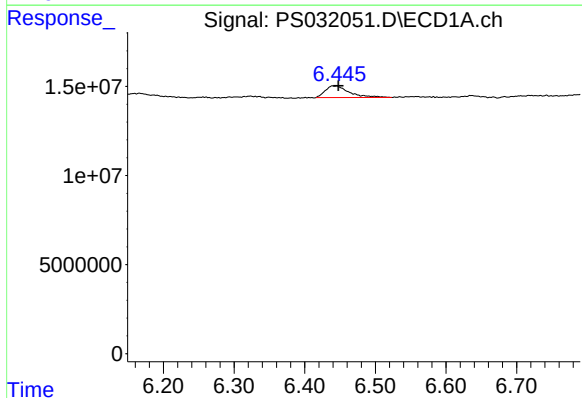


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.440 min
Delta R.T.: -0.008 min
Response: 15410369
Conc: 2.19 ng/ml

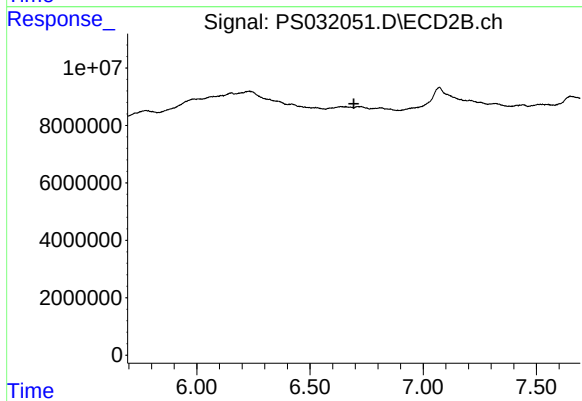

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.694 min
Response: 0
Conc: N.D.

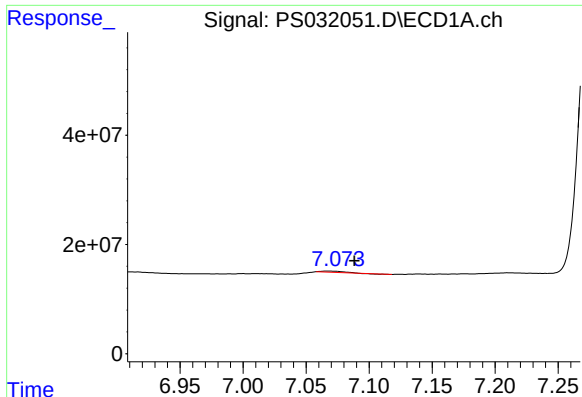

#3 4-Nitrophenol


R.T.: 7.067 min
Delta R.T.: -0.021 min
Response: 2582182
Conc: 1.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

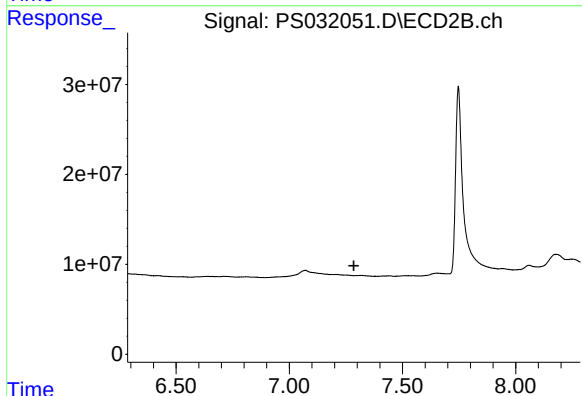


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.285 min
Response: 0
Conc: N.D.

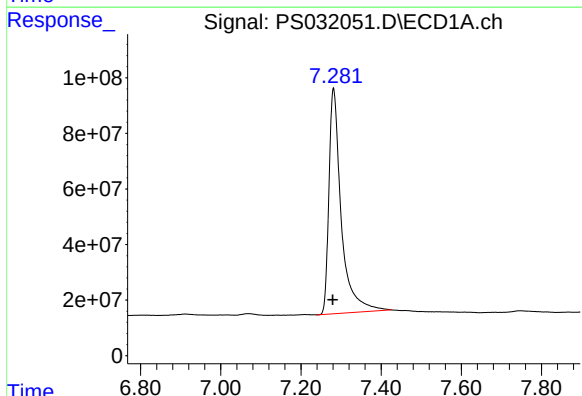


#4 2,4-DCAA

R.T.: 7.281 min
Delta R.T.: 0.002 min
Response: 1726236645
Conc: 362.12 ng/ml

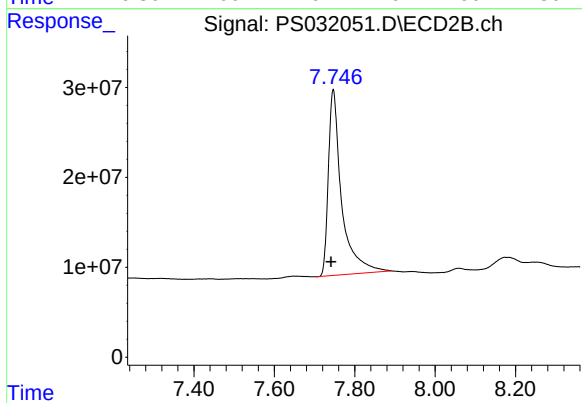

#4 2,4-DCAA


R.T.: 7.747 min
Delta R.T.: 0.006 min
Response: 474314516
Conc: 431.06 ng/ml

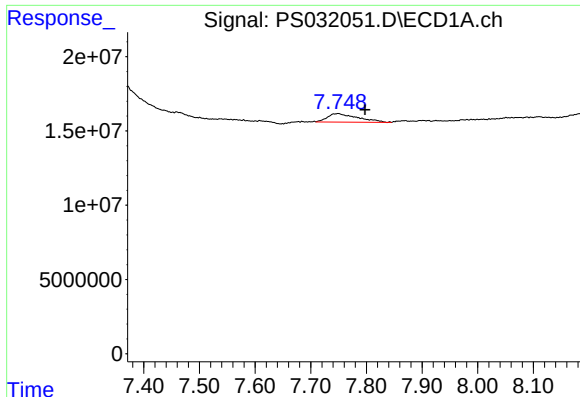

#7 MCPA


R.T.: 7.749 min
Delta R.T.: -0.048 min
Response: 21723901
Conc: 1.48 ug/ml

Instrument :
ECD_S
ClientSampleId :

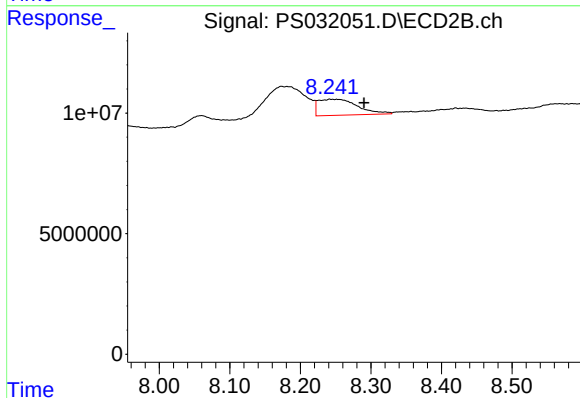


#7 MCPA

R.T.: 8.244 min
Delta R.T.: -0.047 min
Response: 25564302
Conc: 6.78 ug/ml

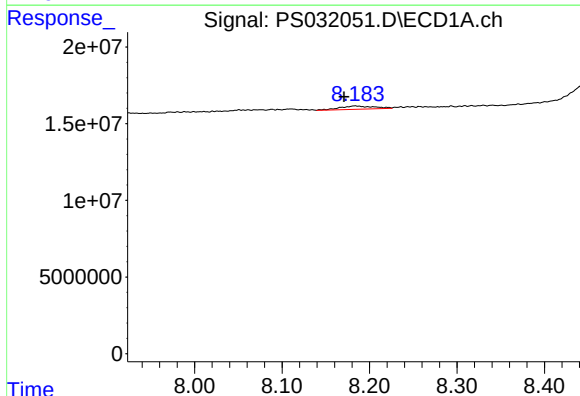


#8 DICHLORPROP

R.T.: 8.183 min
Delta R.T.: 0.013 min
Response: 5683297
Conc: 1.20 ng/ml

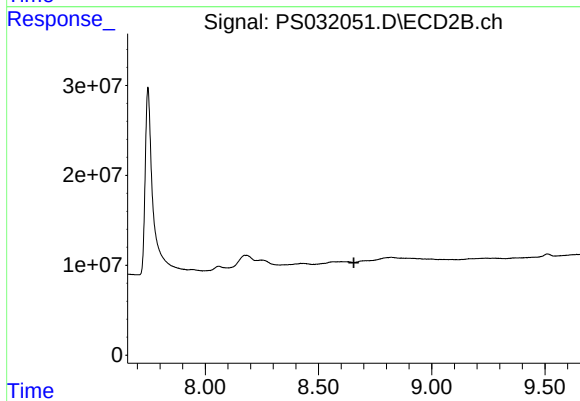

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.656 min
Response: 0
Conc: N.D.

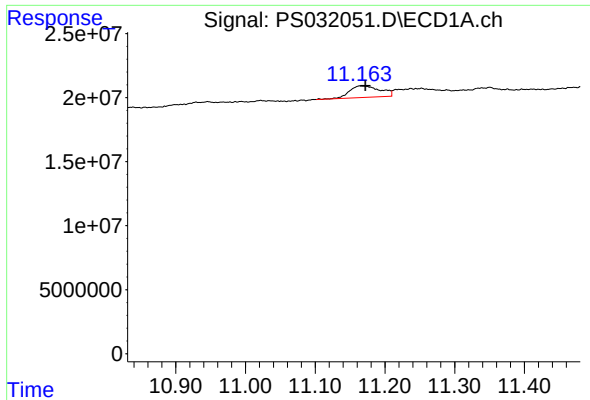

#15 Picloram

R.T.: 11.166 min
Delta R.T.: -0.005 min
Response: 27672826
Conc: 1.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

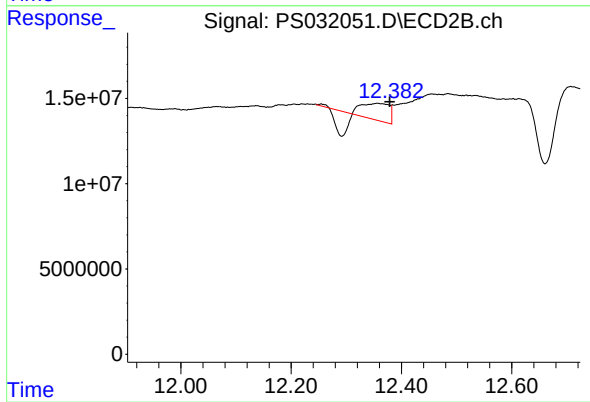

#15 Picloram

R.T.: 12.356 min
Delta R.T.: -0.023 min
Response: 15125201
Conc: N.D.