

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101619\
 Data File : PS007180.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2019 08:54
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 11:31:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.461	5.191	580.8E6	319.7E6	424.377	454.616
Target Compounds							
7) T	MCPA	0.000	5.502	0 37410808		N.D.	12.869
15) T	Picloram	0.000	8.957	0 55023705		N.D.	8.961



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101619\
Data File : PS007180.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2019 08:54
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 11:31:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

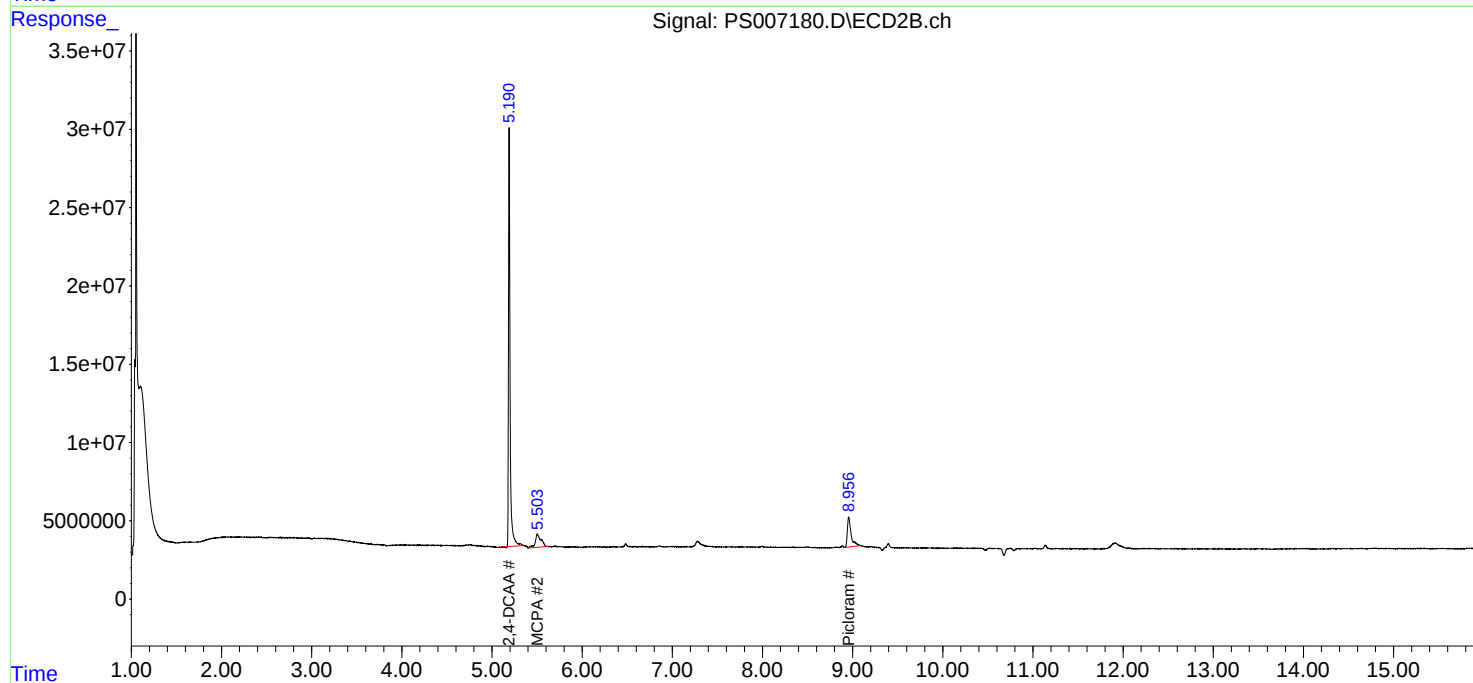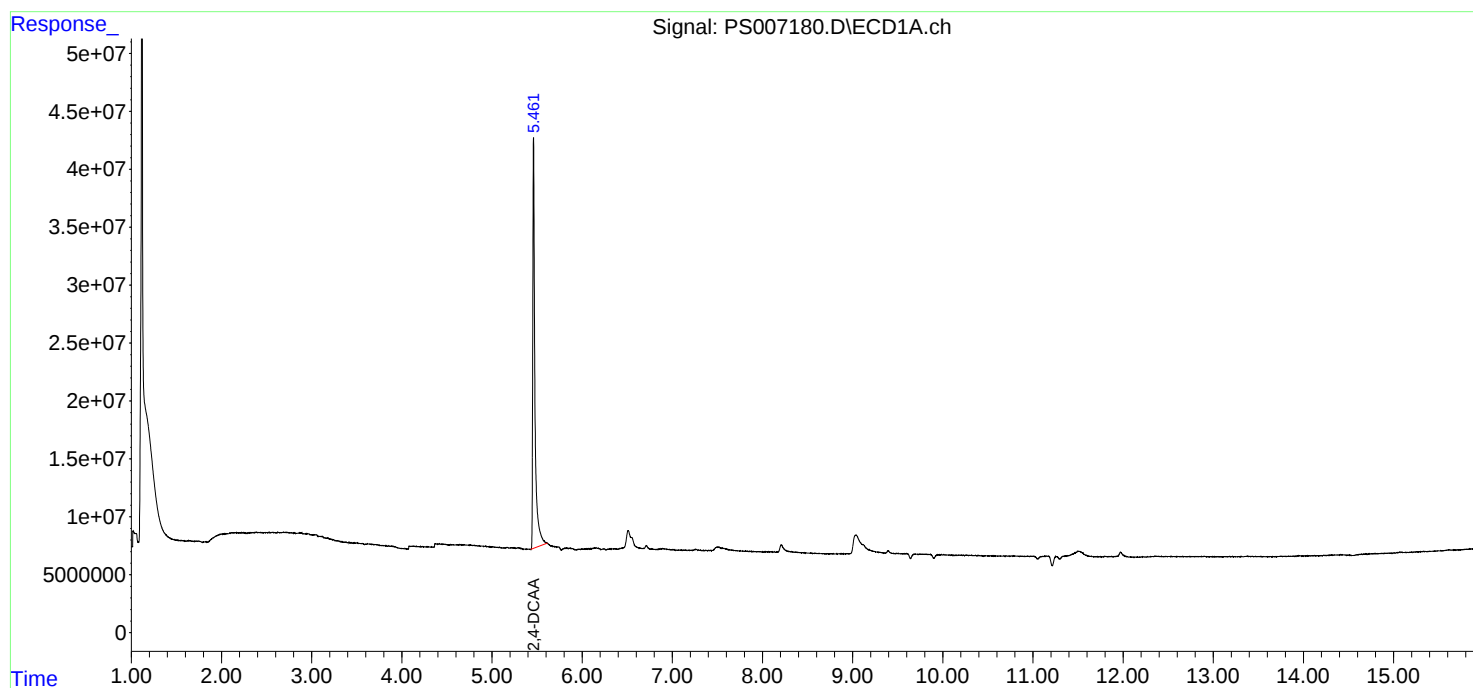


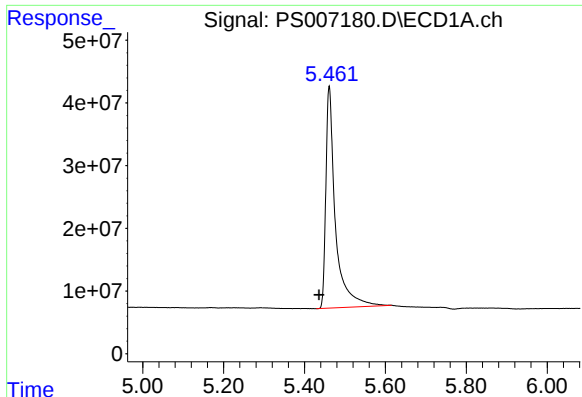

#4 2,4-DCAA


R.T.: 5.461 min
Delta R.T.: 0.026 min
Response: 580832021
Conc: 424.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

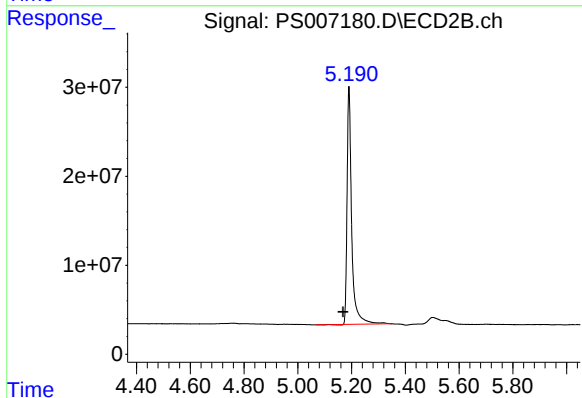


#4 2,4-DCAA

R.T.: 5.191 min
Delta R.T.: 0.022 min
Response: 319734199
Conc: 454.62 ng/ml

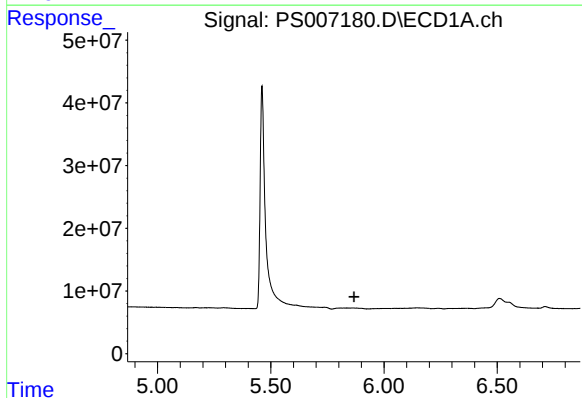


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.867 min
Response: 0
Conc: N.D.

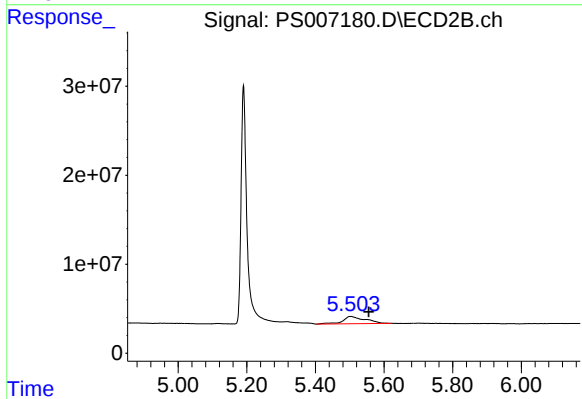

#7 MCPA


R.T.: 5.502 min
Delta R.T.: -0.053 min
Response: 37410808
Conc: 12.87 ug/ml

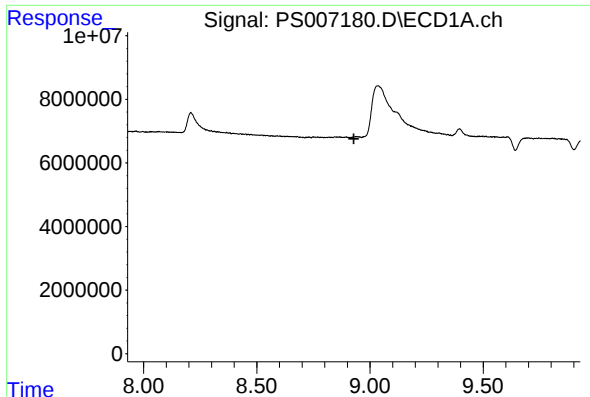

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

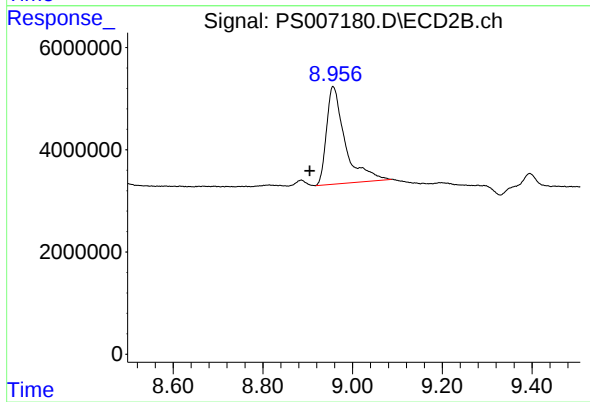

#15 Picloram

R.T.: 8.957 min
Delta R.T.: 0.052 min
Response: 55023705
Conc: 8.96 ng/ml