

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101619\
 Data File : PS007186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2019 11:13
 Operator : SM\AJ
 Sample : K5148-08
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 16 12:59:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.458	5.188	488.9E6	286.1E6	357.238	406.785
Target Compounds							
1) T	Dalapon	2.010	1.722	90745647	154.7E6	54.232	169.975 #
2) T	3,5-DICHL...	0.000	4.478	0	6366412	N.D.	7.399
5) T	DICAMBA	5.549	5.322	51326158	3237383	10.446	1.244 #
6) T	MCP	0.000	5.322	0	3237383	N.D.	1.707
7) T	MCPA	0.000	5.503	0	43772610	N.D.	15.057
9) T	2,4-D	0.000	6.034	0	27661629	N.D.	34.673
10) T	Pentachlo...	0.000	6.486	0	10354491	N.D.	1.077
11) T	2,4,5-TP ...	0.000	6.789	0	60513118	N.D.	15.909
12) T	2,4,5-T	7.427	7.247	181.5E6	10978808	23.736	3.134 #
15) T	Picloram	8.993	8.940	74217543	60397302	6.724	9.836 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101619\
Data File : PS007186.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2019 11:13
Operator : SM\AJ
Sample : K5148-08
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 16 12:59:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

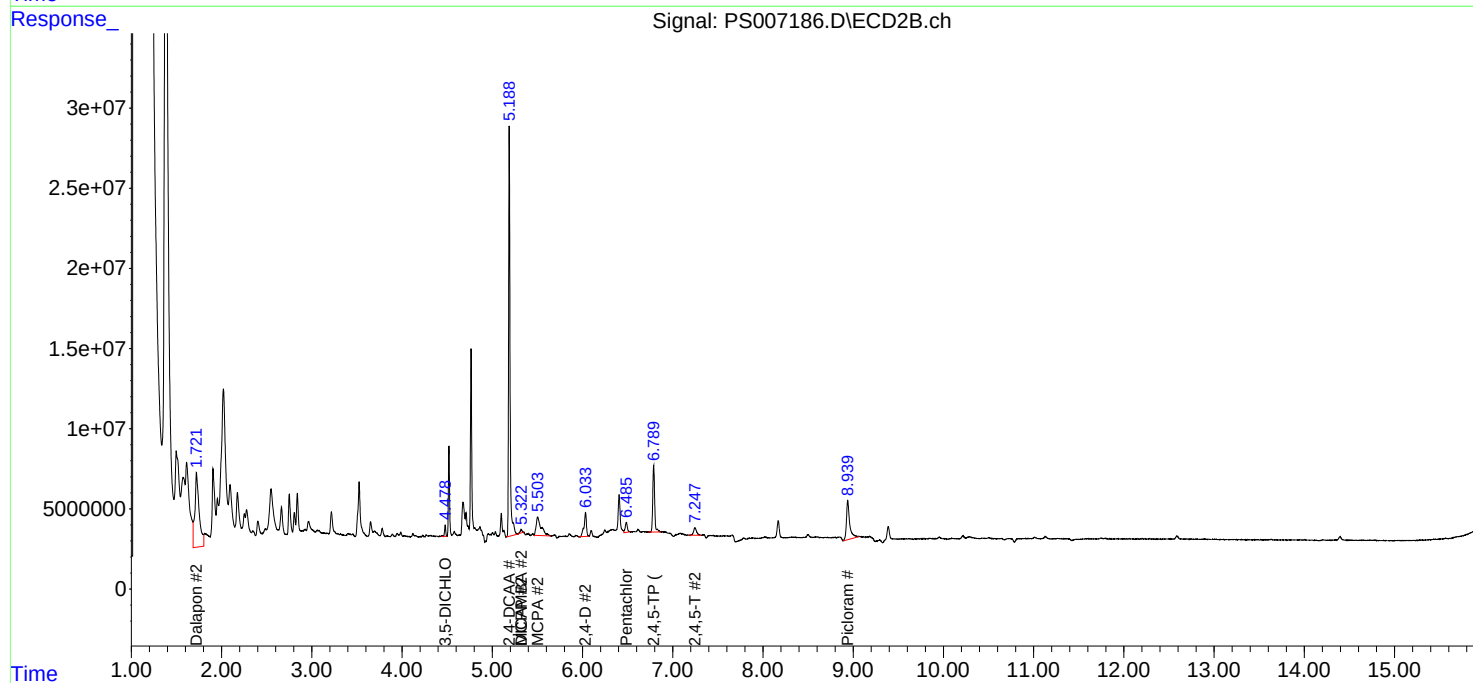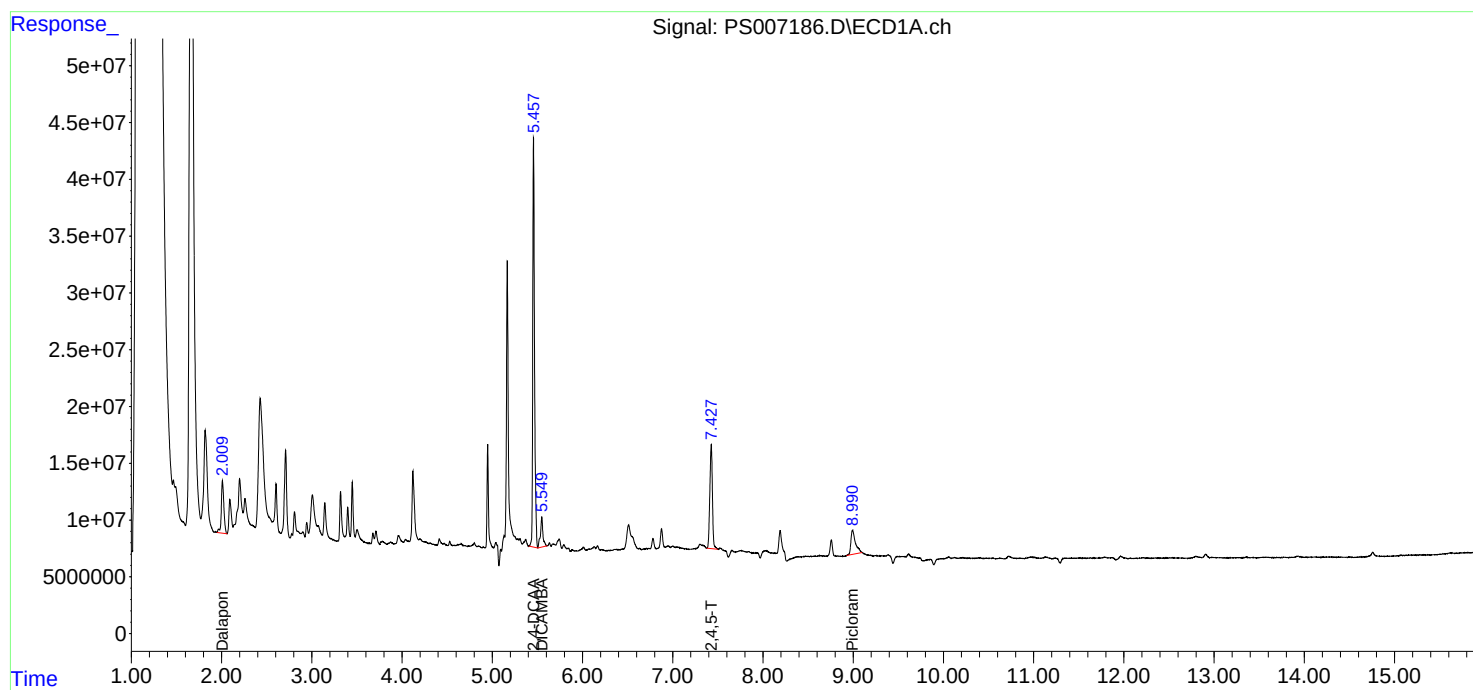


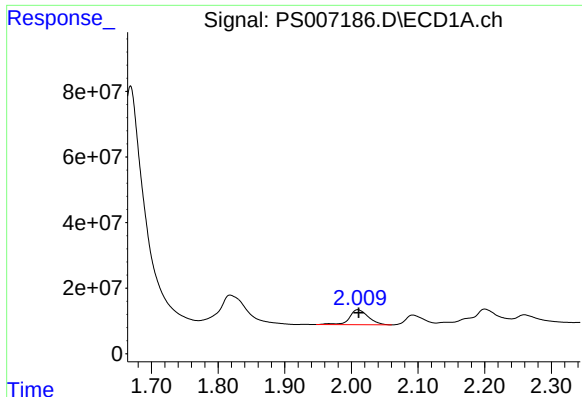

#1 Dalapon


R.T.: 2.010 min
Delta R.T.: -0.001 min
Response: 90745647
Conc: 54.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

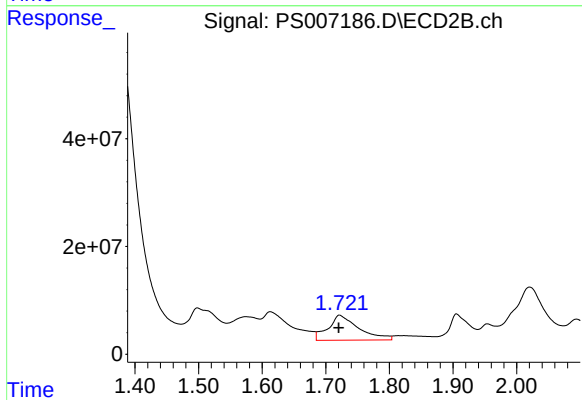


#1 Dalapon

R.T.: 1.722 min
Delta R.T.: 0.001 min
Response: 154677473
Conc: 169.97 ng/ml

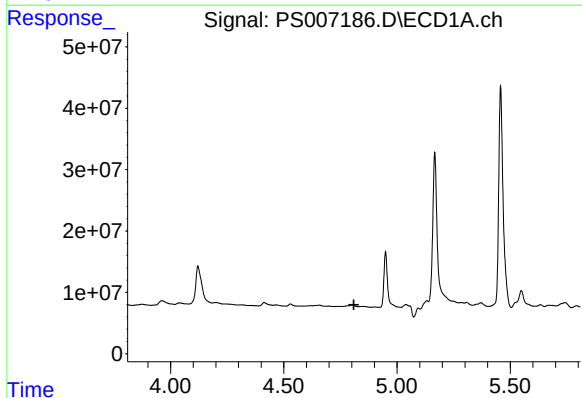


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

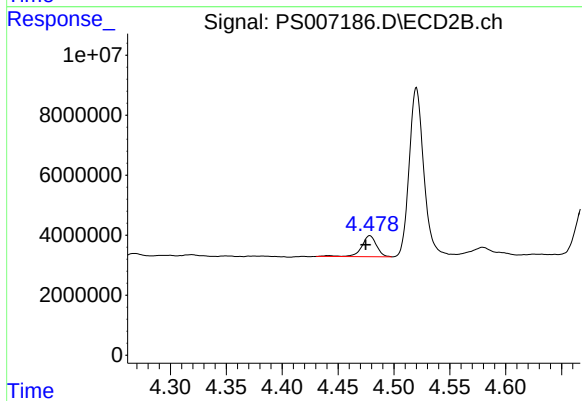

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.478 min
Delta R.T.: 0.004 min
Response: 6366412
Conc: 7.40 ng/ml

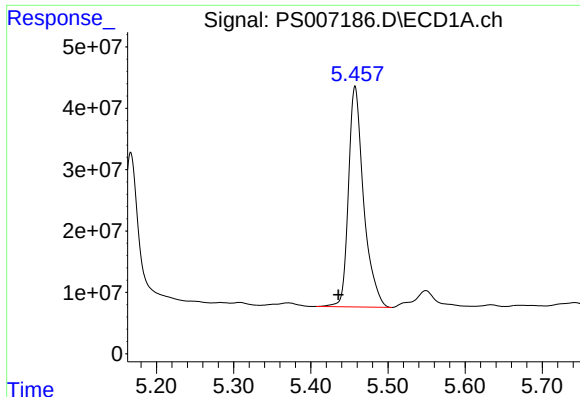

#4 2,4-DCAA


R.T.: 5.458 min
Delta R.T.: 0.022 min
Response: 488940388
Conc: 357.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

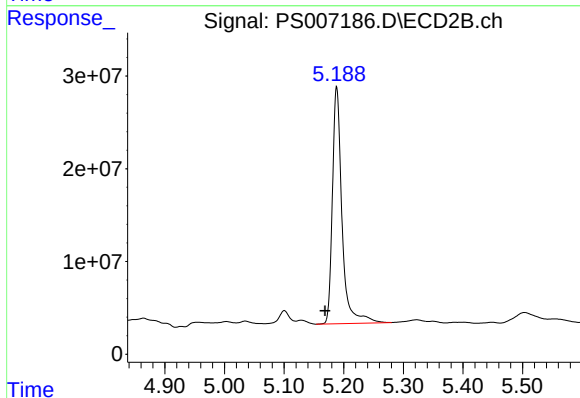


#4 2,4-DCAA

R.T.: 5.188 min
Delta R.T.: 0.020 min
Response: 286094711
Conc: 406.79 ng/ml

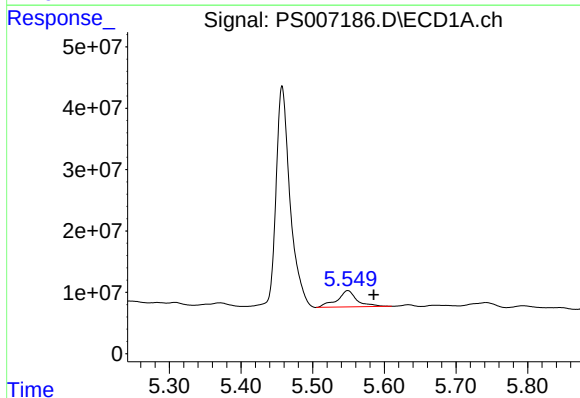


#5 DICAMBA

R.T.: 5.549 min
Delta R.T.: -0.036 min
Response: 51326158
Conc: 10.45 ng/ml

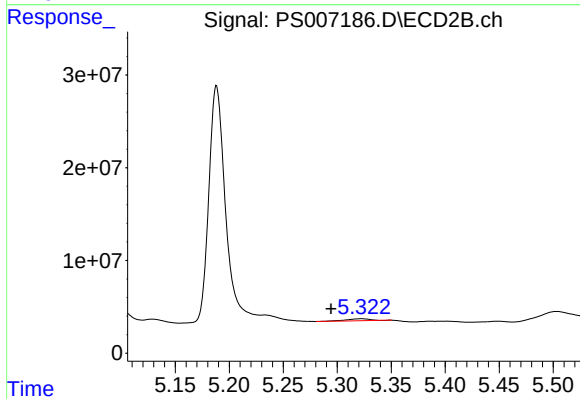

#5 DICAMBA


R.T.: 5.322 min
Delta R.T.: 0.028 min
Response: 3237383
Conc: 1.24 ng/ml

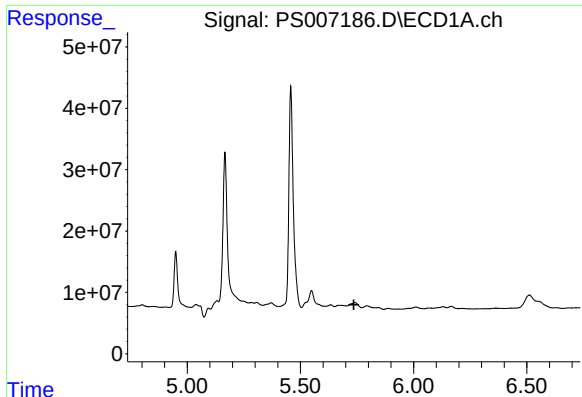

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.736 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

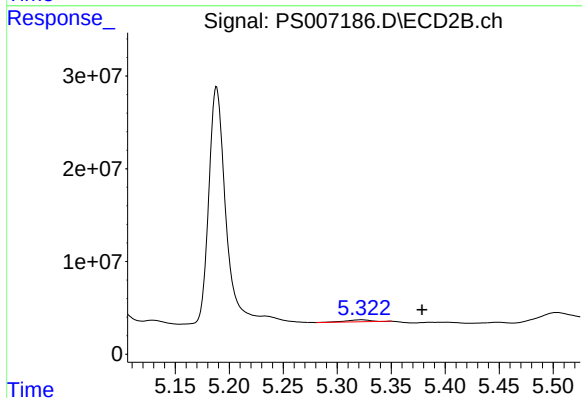


#6 MCPP

R.T.: 5.322 min
Delta R.T.: -0.057 min
Response: 3237383
Conc: 1.71 ug/ml

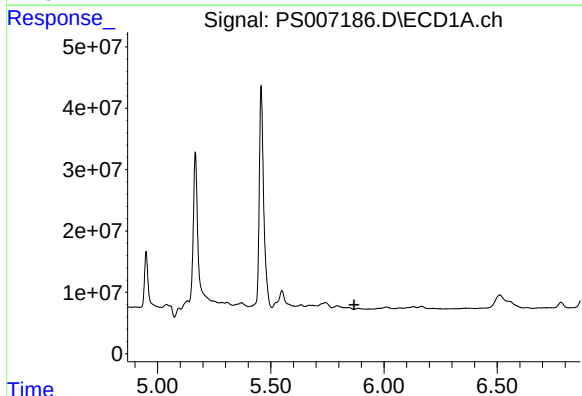


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

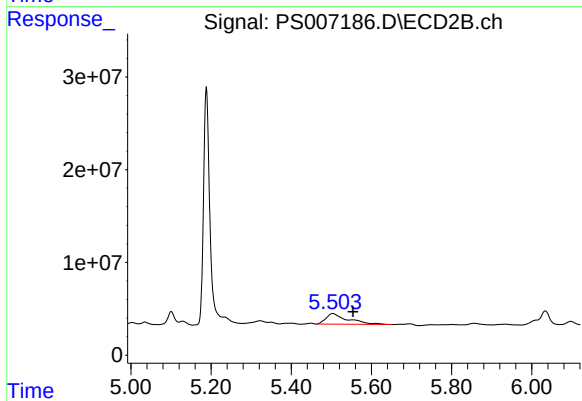

#7 MCPA


R.T.: 5.503 min
Delta R.T.: -0.052 min
Response: 43772610
Conc: 15.06 ug/ml

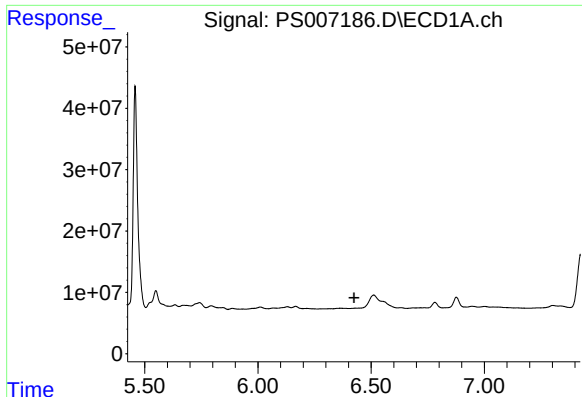

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

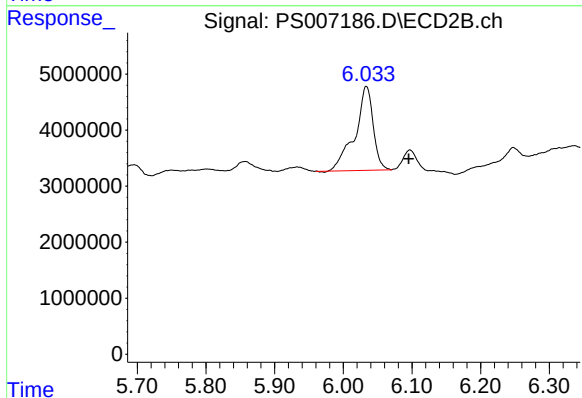


#9 2,4-D

R.T.: 6.034 min
Delta R.T.: -0.062 min
Response: 27661629
Conc: 34.67 ng/ml

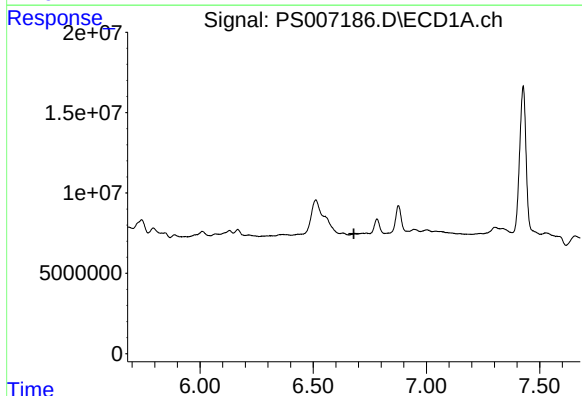


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

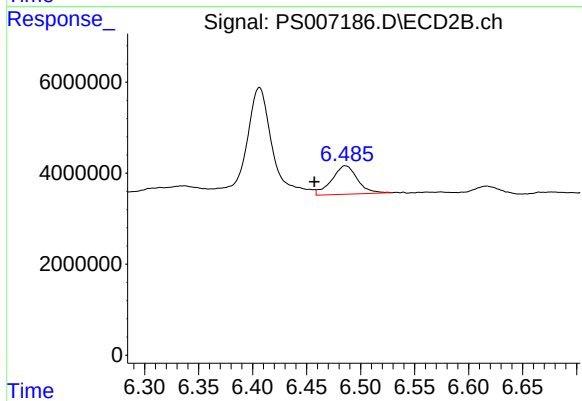

#10 Pentachlorophenol


R.T.: 6.486 min
Delta R.T.: 0.029 min
Response: 10354491
Conc: 1.08 ng/ml

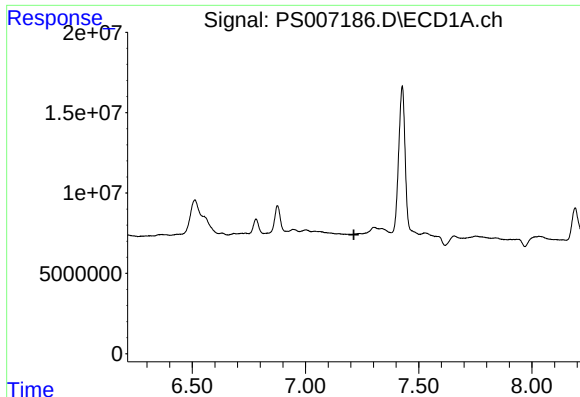

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

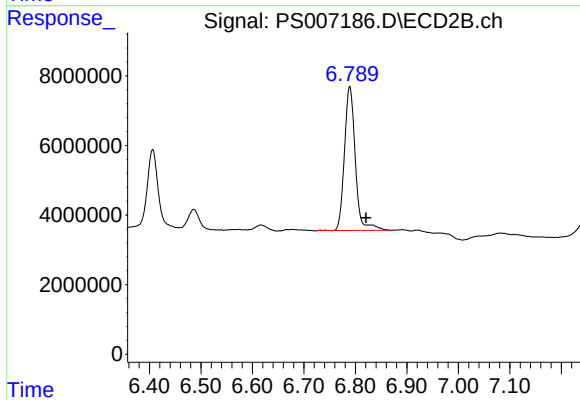


#11 2,4,5-TP (SILVEX)

R.T.: 6.789 min
Delta R.T.: -0.031 min
Response: 60513118
Conc: 15.91 ng/ml

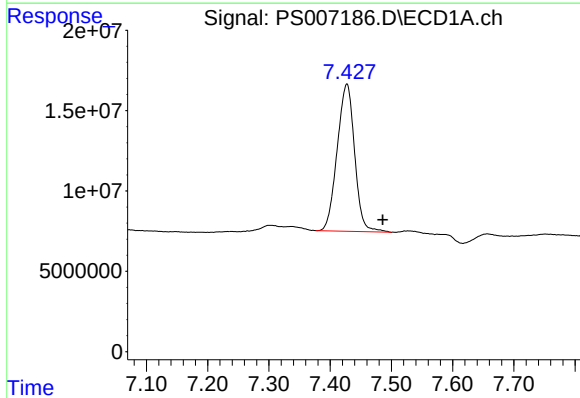


#12 2,4,5-T

R.T.: 7.427 min
Delta R.T.: -0.059 min
Response: 181457734
Conc: 23.74 ng/ml

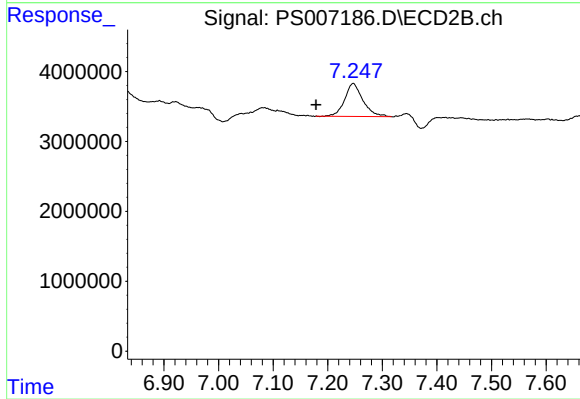

#12 2,4,5-T


R.T.: 7.247 min
Delta R.T.: 0.068 min
Response: 10978808
Conc: 3.13 ng/ml

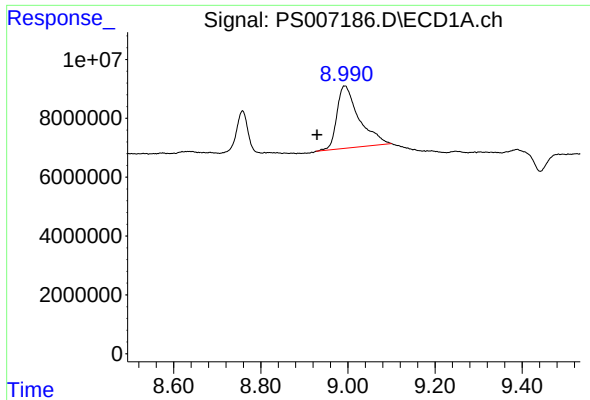

#15 Picloram

R.T.: 8.993 min
Delta R.T.: 0.064 min
Response: 74217543
Conc: 6.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

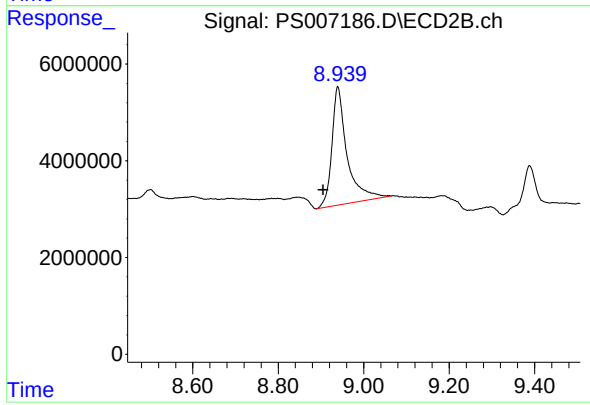

#15 Picloram

R.T.: 8.940 min
Delta R.T.: 0.035 min
Response: 60397302
Conc: 9.84 ng/ml