

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101620\
 Data File : PS012878.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2020 18:53
 Operator : DD\AJ
 Sample : L4223-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 01:53:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.913	314.9E6	169.6E6	321.477	368.625
Target Compounds							
1) T	Dalapon	2.994	2.589	57736416	108.0E6	50.808	180.561 #
2) T	3,5-DICHL...	0.000	6.094	0	34741828	N.D.	48.729
5) T	DICAMBA	7.392	7.046	8944386	15404275	2.319	8.078 #
6) T	MCP	7.626	0.000	18724301	0	6.418	N.D. #
7) T	MCPA	7.755	7.351	21429349	9695102	5.138	4.044
8) T	DICHLORPROP	0.000	7.755	0	11781472	N.D.	22.818
9) T	2,4-D	8.397	0.000	80771604	0	71.138	N.D. #
11) T	2,4,5-TP ...	0.000	8.763	0	12478119	N.D.	4.729
12) T	2,4,5-T	9.405	0.000	15172349	0	2.699	N.D. #
14) T	DINOSEB	0.000	10.051	0	14525492	N.D.	7.583
15) T	Picloram	10.990	0.000	16356981	0	2.272	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101620\
Data File : PS012878.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2020 18:53
Operator : DD\AJ
Sample : L4223-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 01:53:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

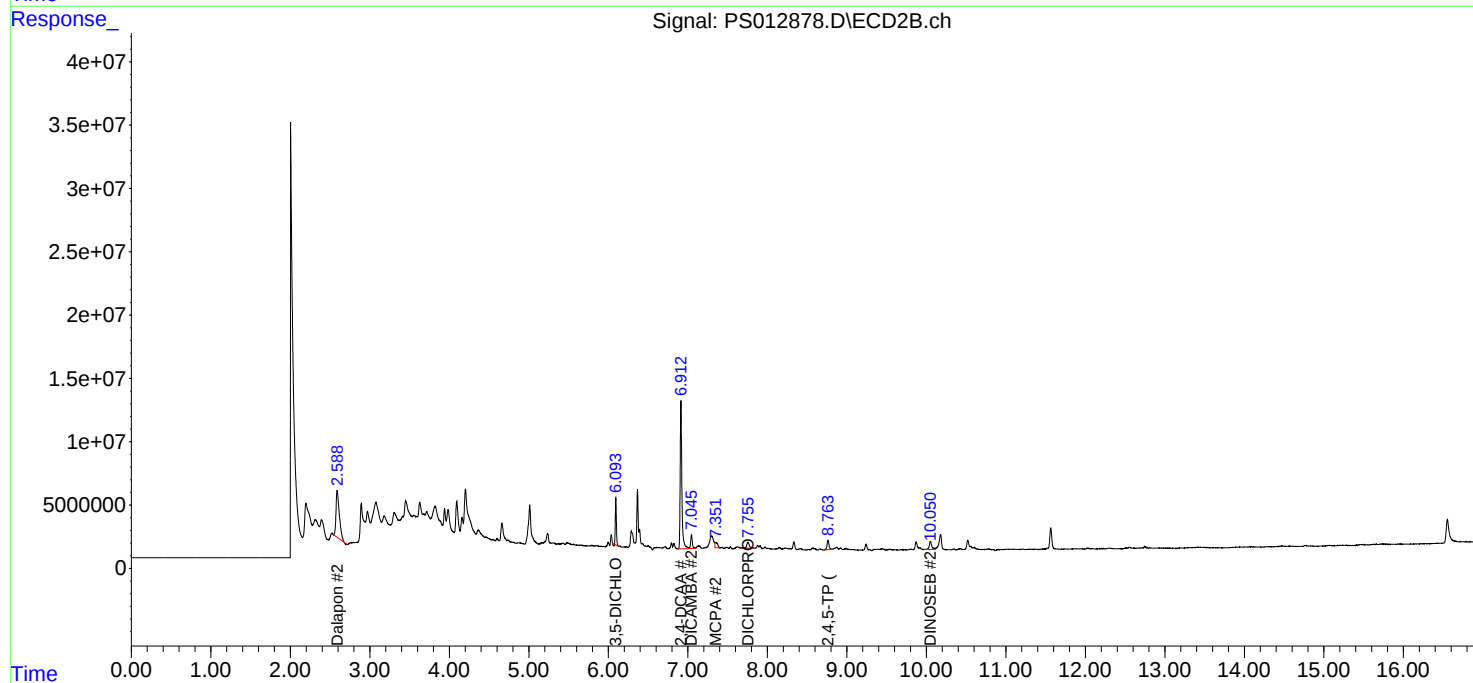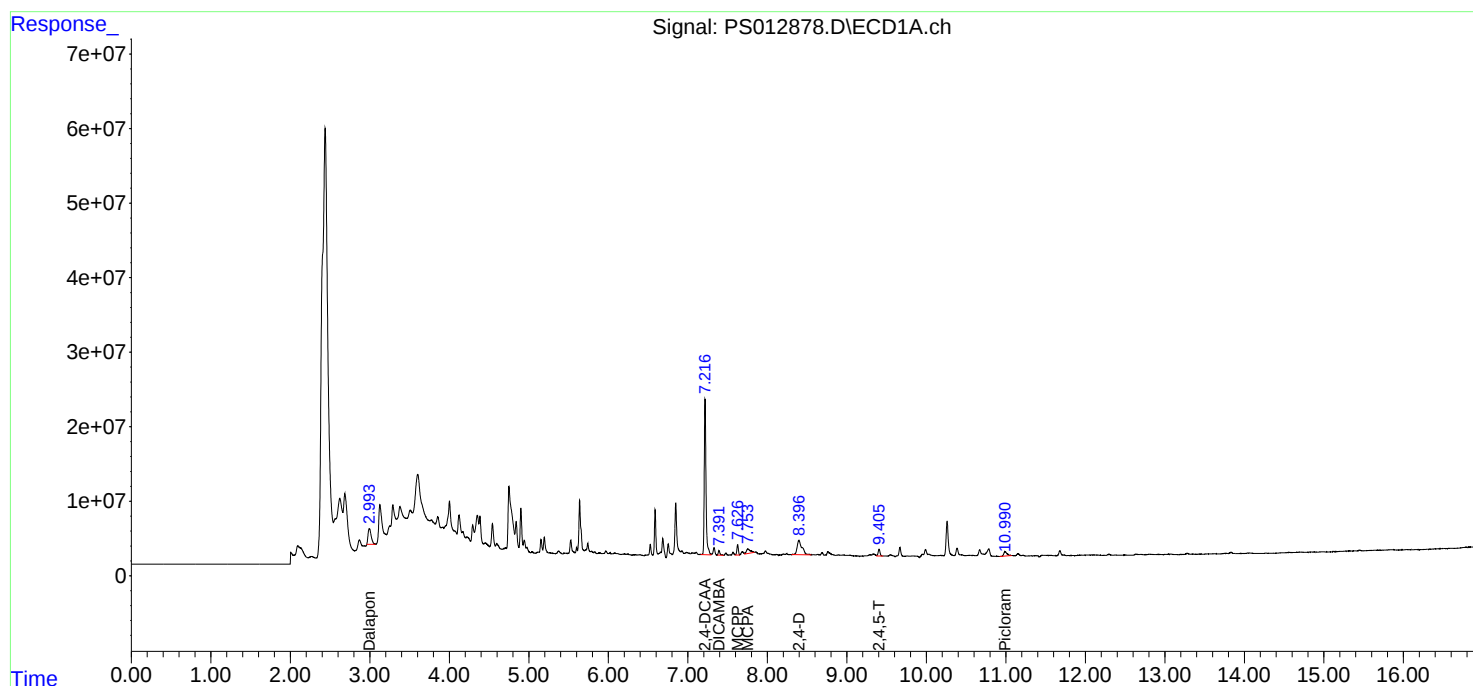


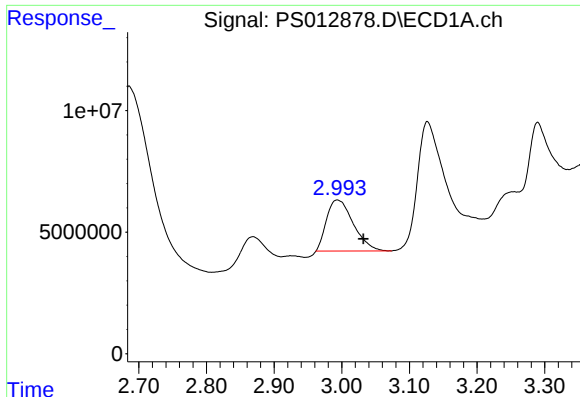

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.038 min
Response: 57736416
Conc: 50.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

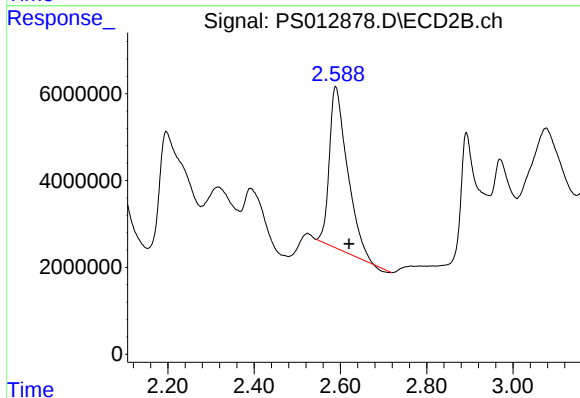


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.032 min
Response: 108009460
Conc: 180.56 ng/ml

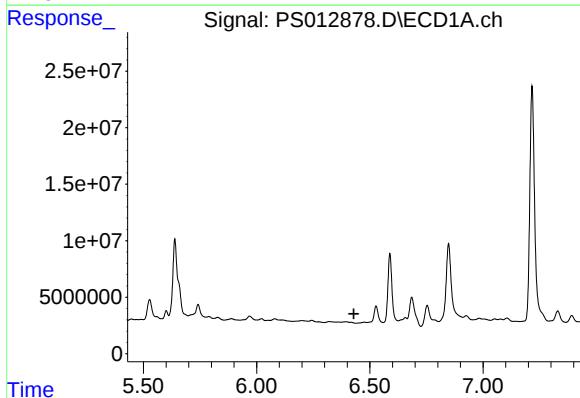


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.430 min
Response: 0
Conc: N.D.

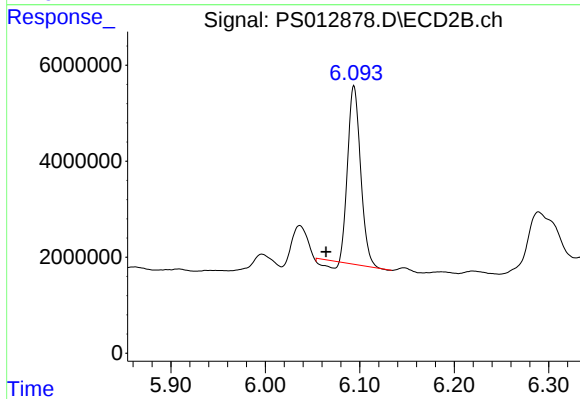

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.094 min
Delta R.T.: 0.029 min
Response: 34741828
Conc: 48.73 ng/ml

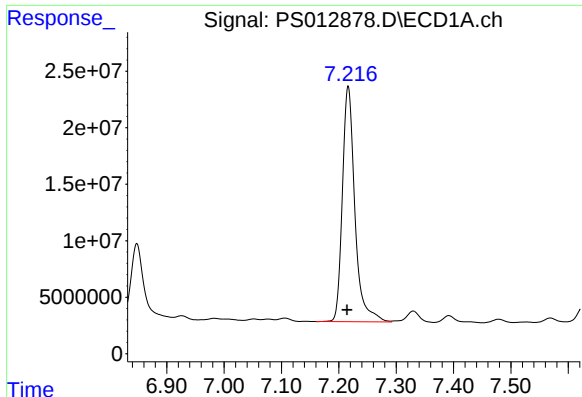

#4 2,4-DCAA


R.T.: 7.216 min
Delta R.T.: 0.002 min
Response: 314870479
Conc: 321.48 ng/ml

Instrument :
ECD_S
ClientSampleId :

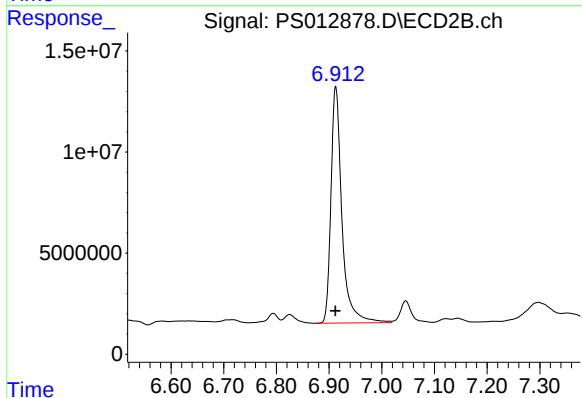


#4 2,4-DCAA

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 169573643
Conc: 368.63 ng/ml

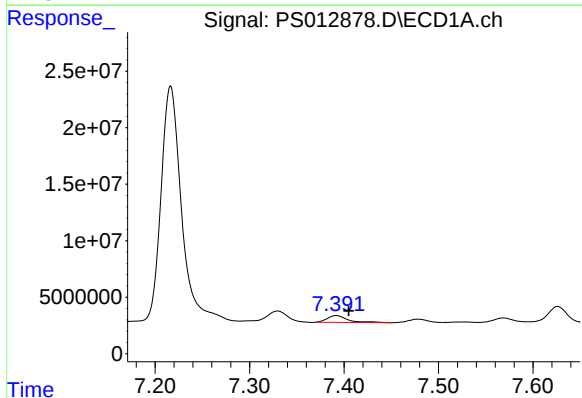


#5 DICAMBA

R.T.: 7.392 min
Delta R.T.: -0.013 min
Response: 8944386
Conc: 2.32 ng/ml

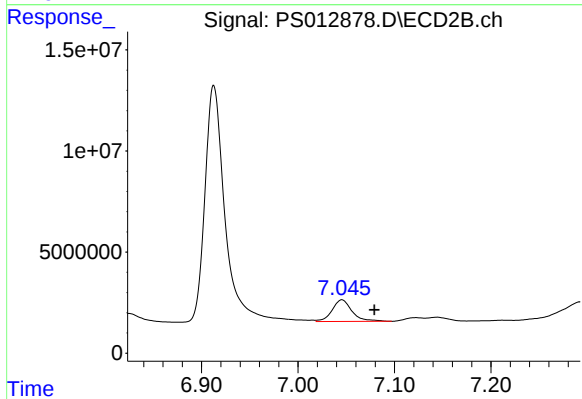

#5 DICAMBA


R.T.: 7.046 min
Delta R.T.: -0.034 min
Response: 15404275
Conc: 8.08 ng/ml

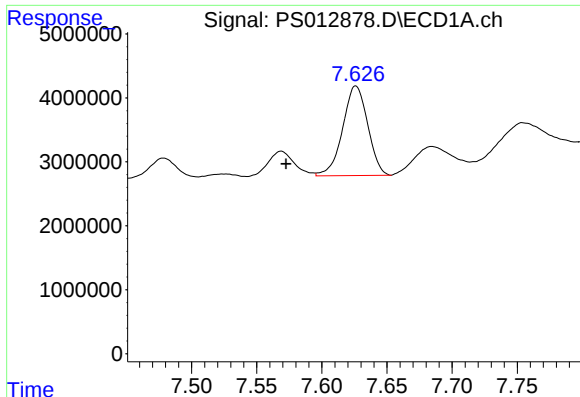

#6 MCPP


R.T.: 7.626 min
Delta R.T.: 0.054 min
Response: 18724301
Conc: 6.42 ug/ml

Instrument :
ECD_S
ClientSampleId :

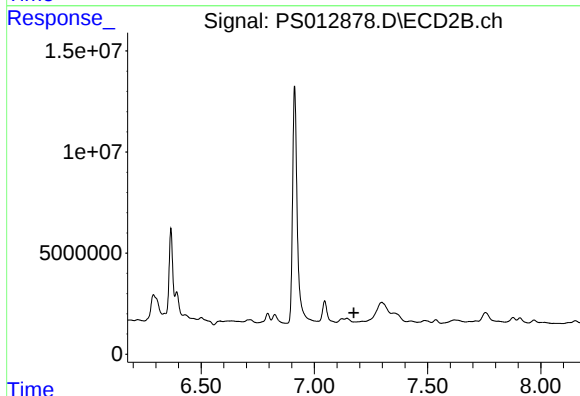


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.175 min
Response: 0
Conc: N.D.

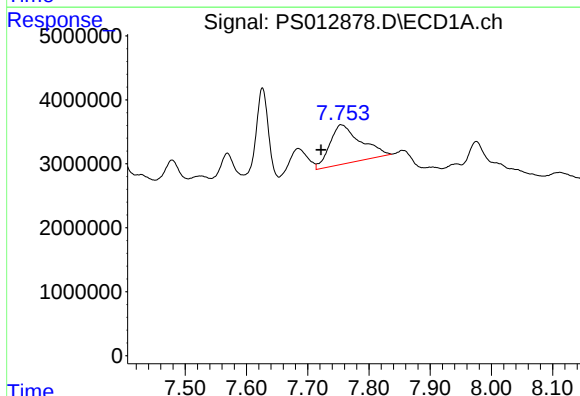


#7 MCPA

R.T.: 7.755 min
Delta R.T.: 0.033 min
Response: 21429349
Conc: 5.14 ug/ml

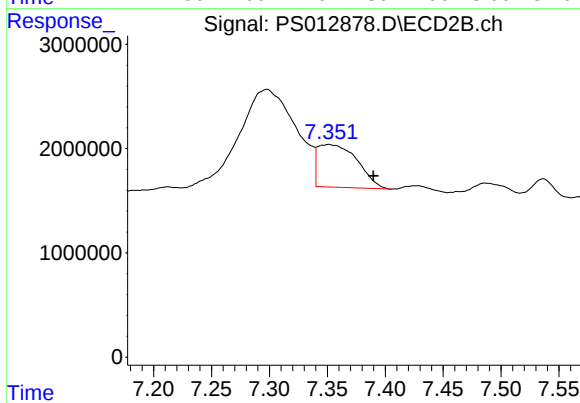

#7 MCPA


R.T.: 7.351 min
Delta R.T.: -0.038 min
Response: 9695102
Conc: 4.04 ug/ml

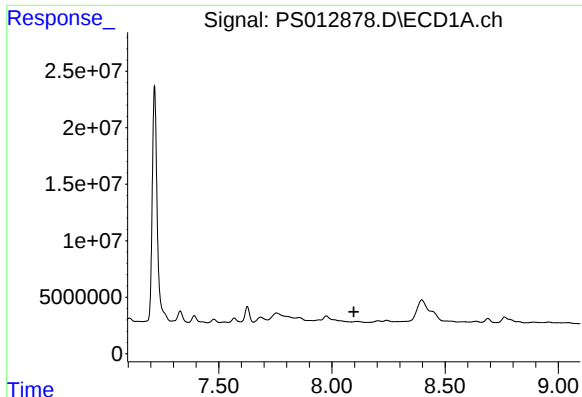

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.097 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

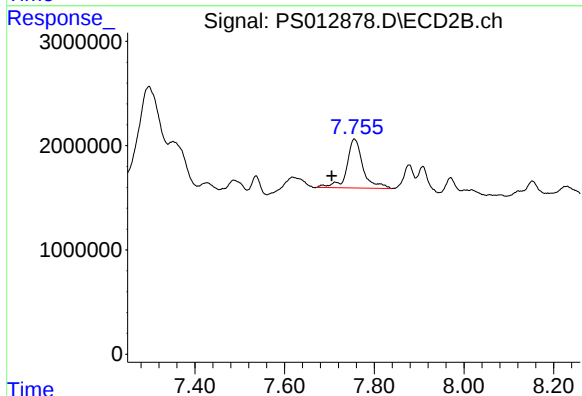


#8 DICHLORPROP

R.T.: 7.755 min
Delta R.T.: 0.050 min
Response: 11781472
Conc: 22.82 ng/ml

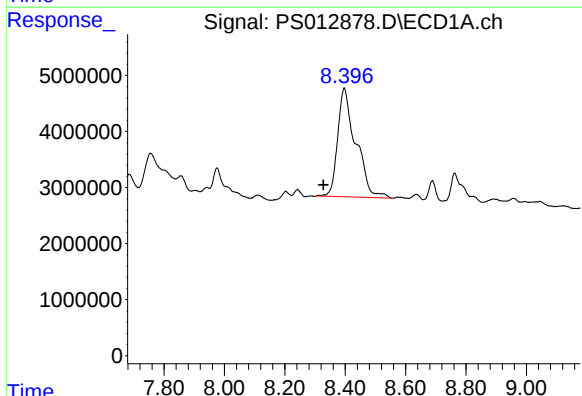


#9 2,4-D

R.T.: 8.397 min
Delta R.T.: 0.069 min
Response: 80771604
Conc: 71.14 ng/ml

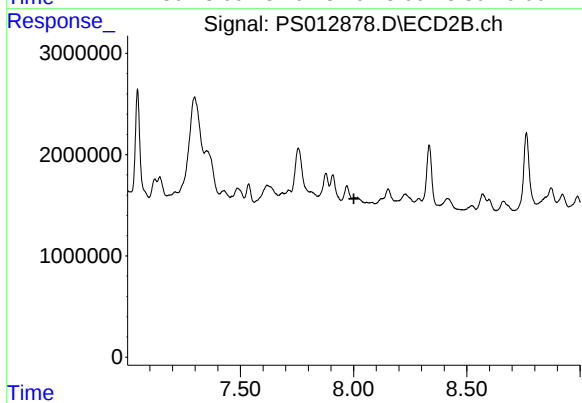

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.001 min
Response: 0
Conc: N.D.

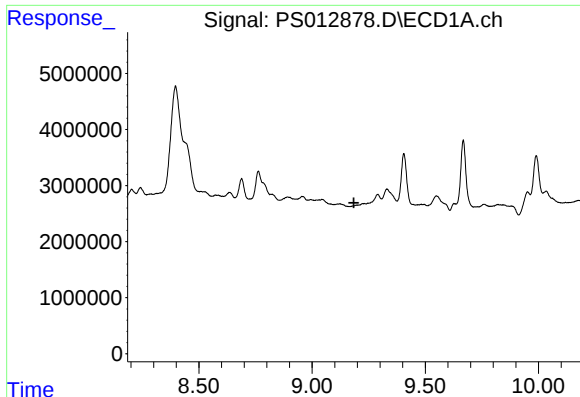

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.185 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

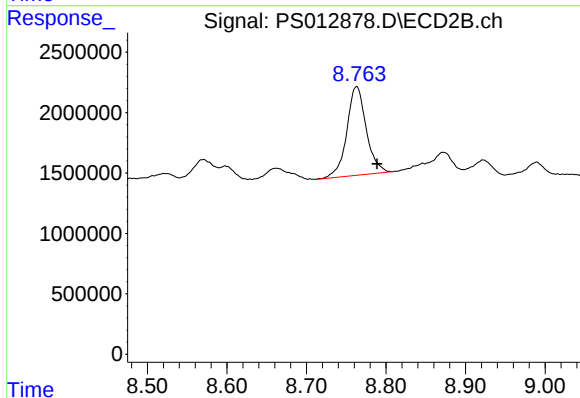


#11 2,4,5-TP (SILVEX)

R.T.: 8.763 min
Delta R.T.: -0.026 min
Response: 12478119
Conc: 4.73 ng/ml

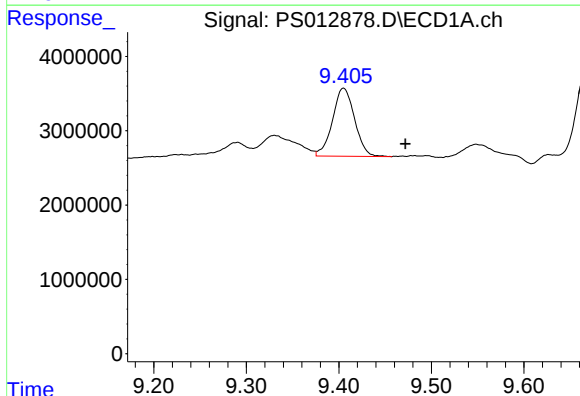


#12 2,4,5-T

R.T.: 9.405 min
Delta R.T.: -0.067 min
Response: 15172349
Conc: 2.70 ng/ml

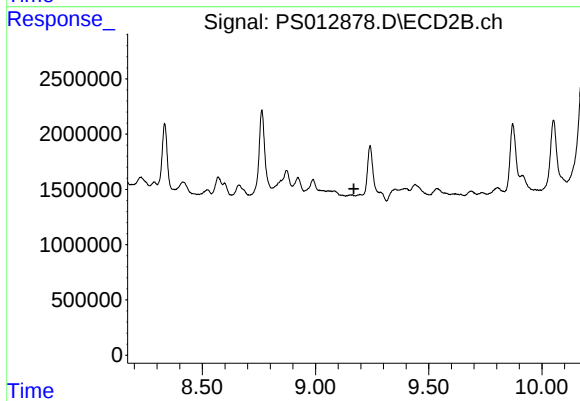

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.169 min
Response: 0
Conc: N.D.

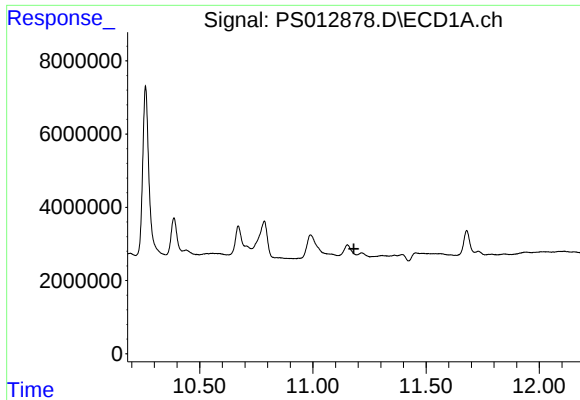

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.181 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

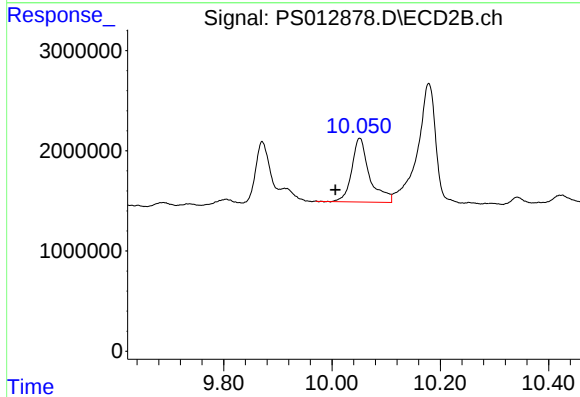


#14 DINOSEB

R.T.: 10.051 min
Delta R.T.: 0.045 min
Response: 14525492
Conc: 7.58 ng/ml

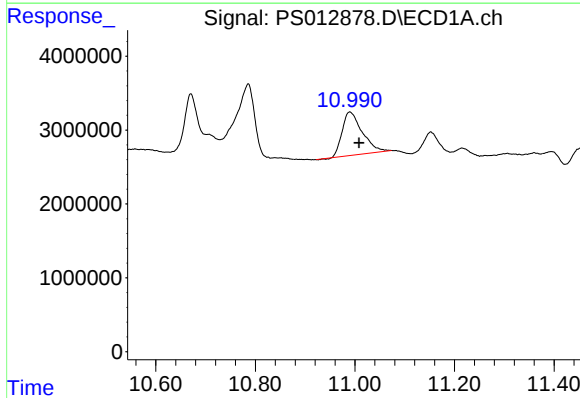

#15 Picloram

R.T.: 10.990 min
Delta R.T.: -0.019 min
Response: 16356981
Conc: 2.27 ng/ml

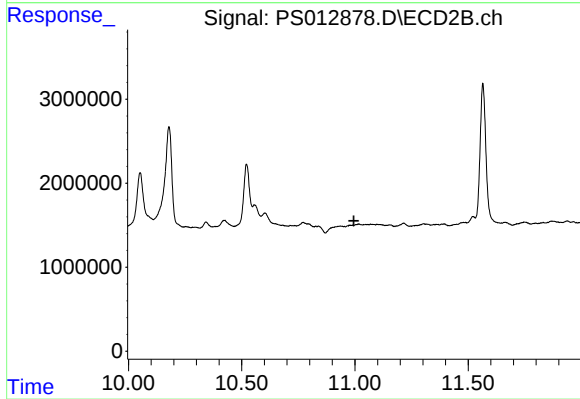

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 10.995 min
Response: 0
Conc: N.D.