

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101620\
 Data File : PS012880.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2020 19:40
 Operator : DD\AJ
 Sample : L4227-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 01:54:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
 Quant Title : 8080.M
 QLast Update : Wed Sep 23 04:57:25 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.216	6.912	338.7E6	185.6E6	345.831	403.392
Target Compounds							
1) T	Dalapon	2.993	2.589	59914016	138.1E6	52.724	230.829 #
2) T	3,5-DICHL...	0.000	6.093	0	70667046	N.D.	99.118
3) T	4-Nitroph...	7.051	0.000	5778563	0	11.884	N.D. #
5) T	DICAMBA	7.391	7.045	10069213	10580330	2.610	5.548 #
6) T	MCPD	7.625	0.000	10191628	0	3.493	N.D. #
7) T	MCPA	7.750	0.000	54941571	0	13.173	N.D. #
8) T	DICHLORPROP	0.000	7.751	0	8141594	N.D.	15.768
9) T	2,4-D	8.394	0.000	64975634	0	57.226	N.D. #
11) T	2,4,5-TP ...	0.000	8.761	0	21257442	N.D.	8.057
12) T	2,4,5-T	9.404	0.000	35917641	0	6.390	N.D. #
14) T	DINOSEB	0.000	10.050	0	20345501	N.D.	10.622
15) T	Picloram	10.985	0.000	18053476	0	2.507	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101620\
Data File : PS012880.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2020 19:40
Operator : DD\AJ
Sample : L4227-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 01:54:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS092220.M
Quant Title : 8080.M
QLast Update : Wed Sep 23 04:57:25 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

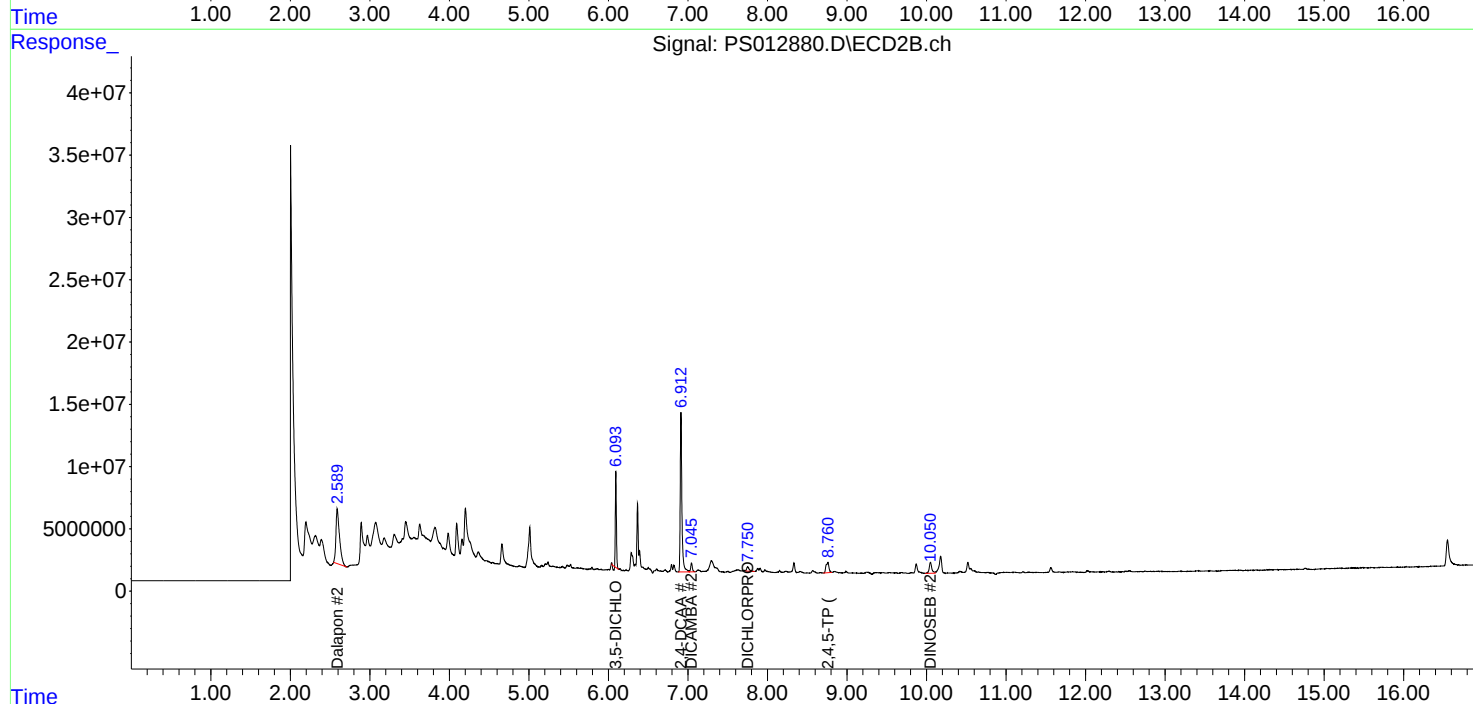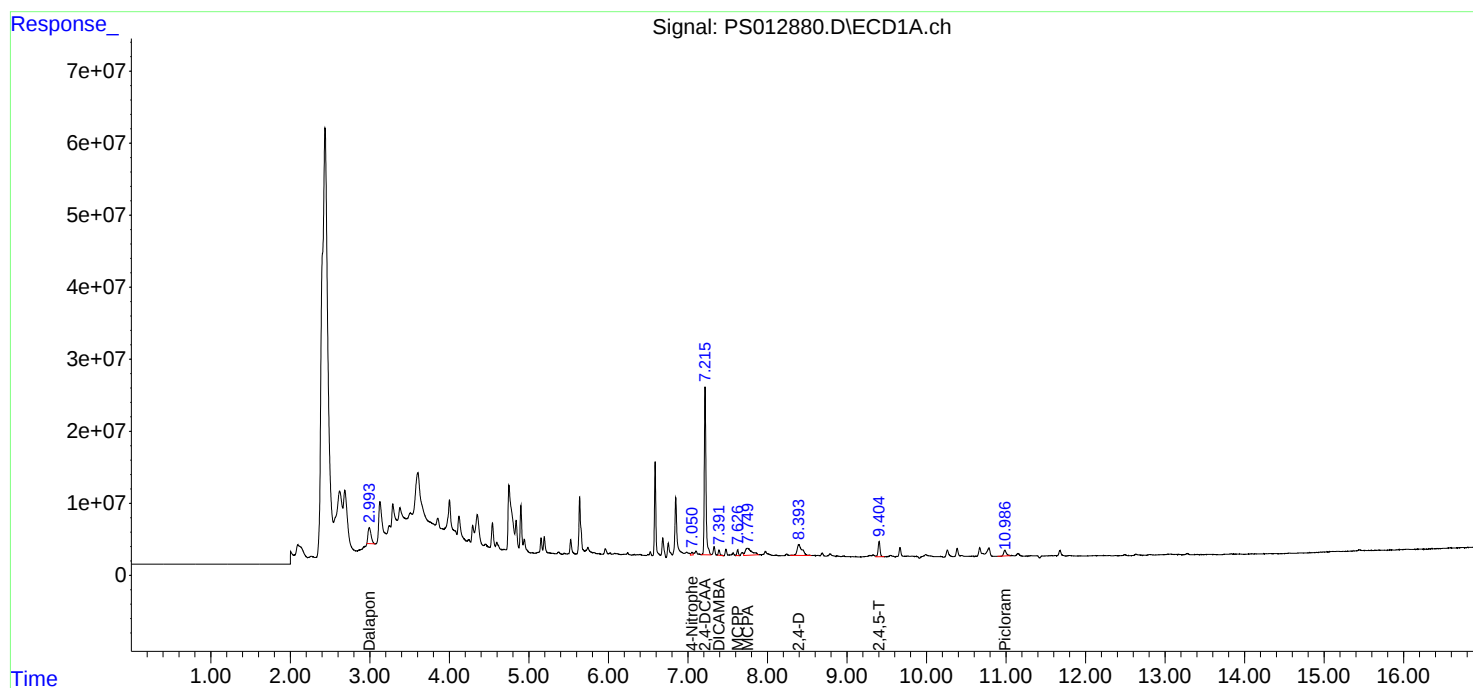


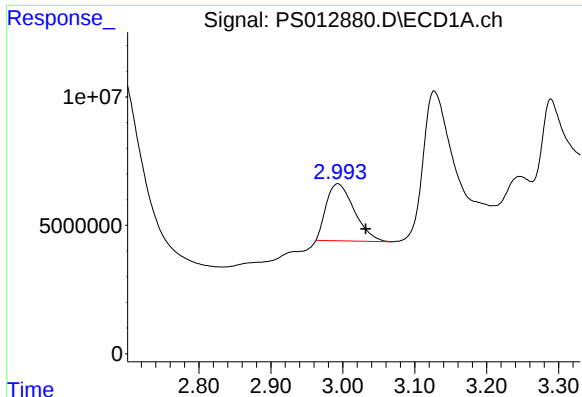

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.039 min
Response: 59914016
Conc: 52.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

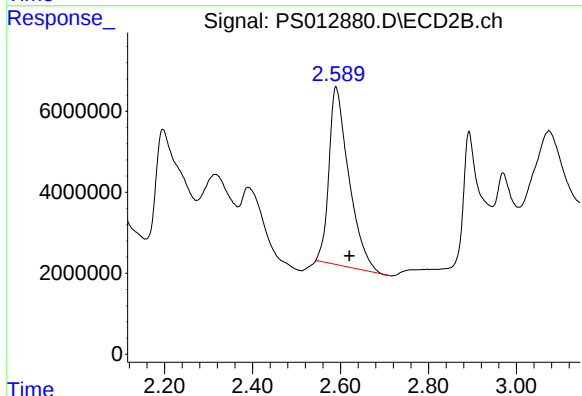


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.031 min
Response: 138079511
Conc: 230.83 ng/ml

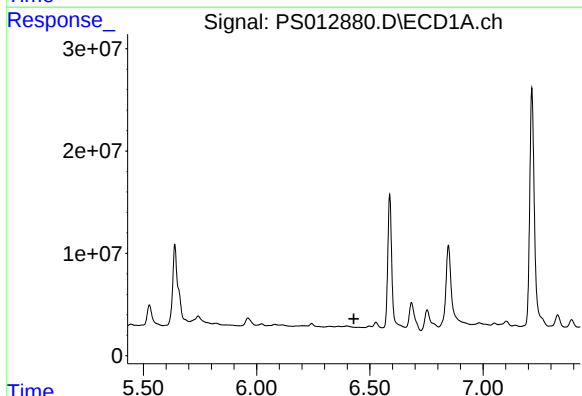


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.430 min
Response: 0
Conc: N.D.

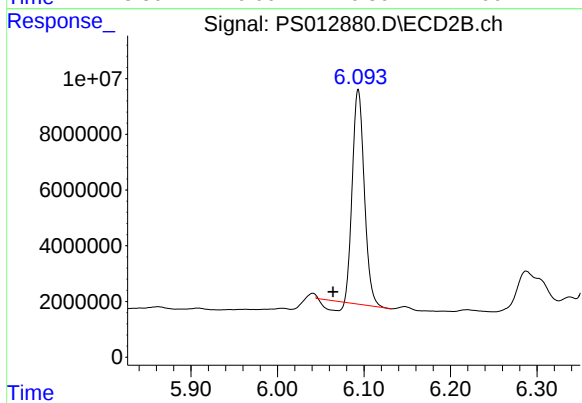

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.093 min
Delta R.T.: 0.029 min
Response: 70667046
Conc: 99.12 ng/ml

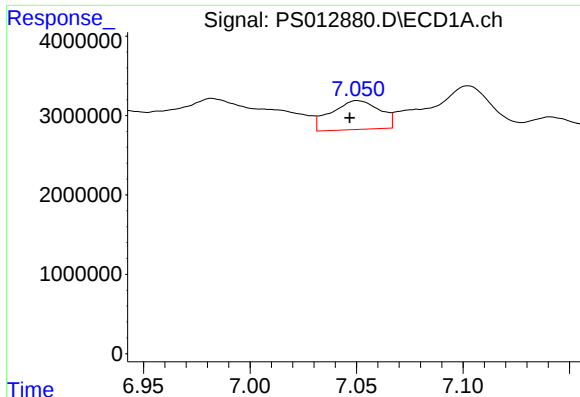

#3 4-Nitrophenol


R.T.: 7.051 min
Delta R.T.: 0.004 min
Response: 5778563
Conc: 11.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

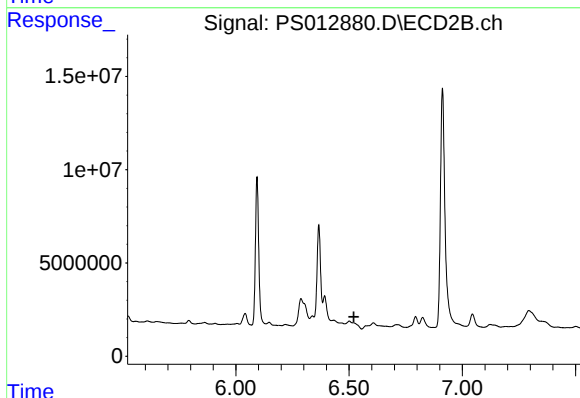


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

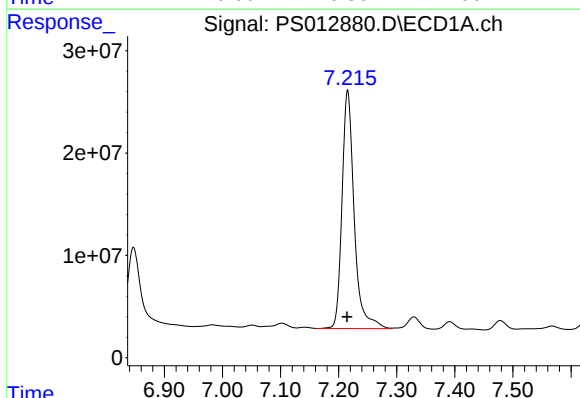


#4 2,4-DCAA

R.T.: 7.216 min
Delta R.T.: 0.001 min
Response: 338723338
Conc: 345.83 ng/ml

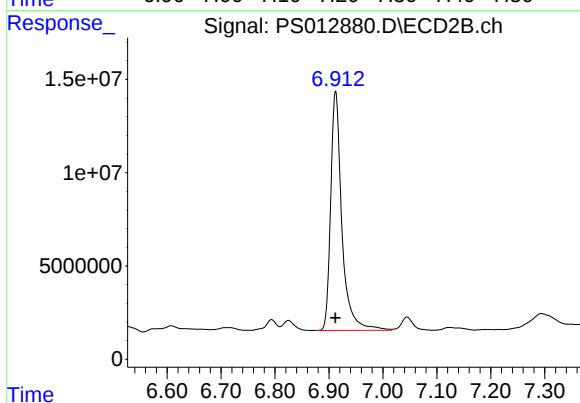

#4 2,4-DCAA


R.T.: 6.912 min
Delta R.T.: 0.000 min
Response: 185566903
Conc: 403.39 ng/ml

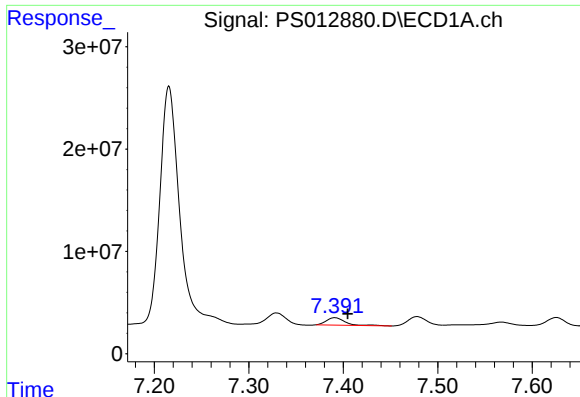

#5 DICAMBA


R.T.: 7.391 min
Delta R.T.: -0.014 min
Response: 10069213
Conc: 2.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

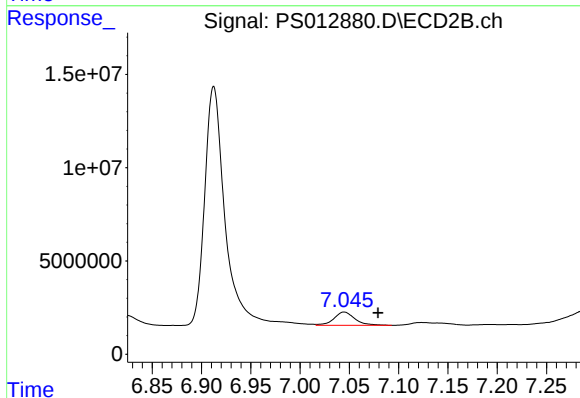


#5 DICAMBA

R.T.: 7.045 min
Delta R.T.: -0.034 min
Response: 10580330
Conc: 5.55 ng/ml

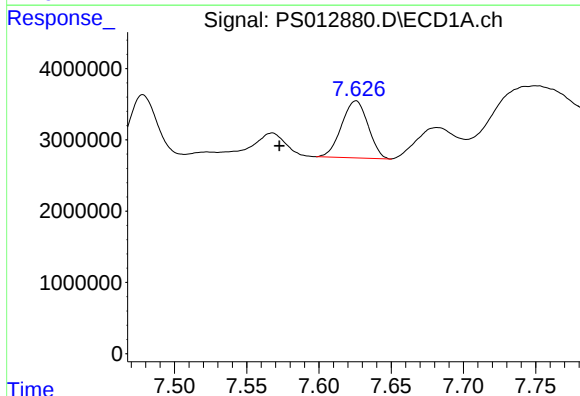


#6 MCP

R.T.: 7.625 min
Delta R.T.: 0.053 min
Response: 10191628
Conc: 3.49 ug/ml

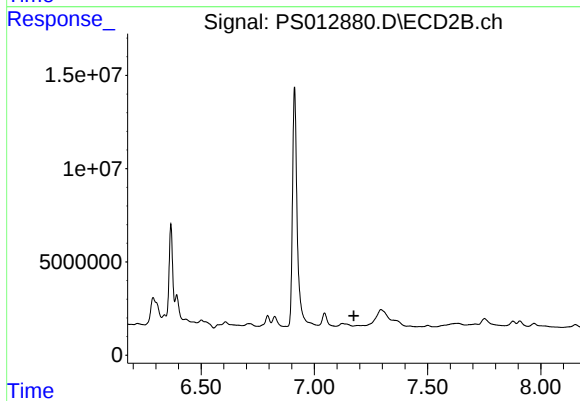

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.175 min
Response: 0
Conc: N.D.

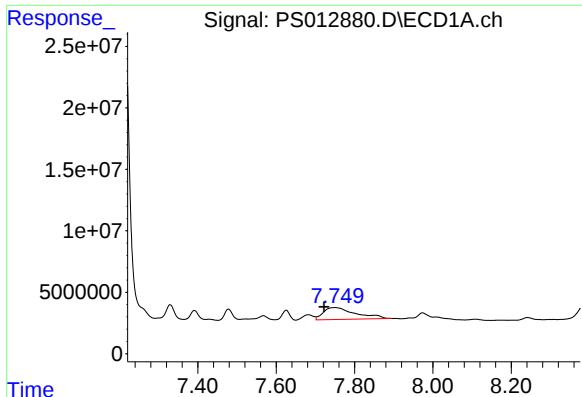

#7 MCPA


R.T.: 7.750 min
Delta R.T.: 0.028 min
Response: 54941571
Conc: 13.17 ug/ml

Instrument :
ECD_S
ClientSampleId :

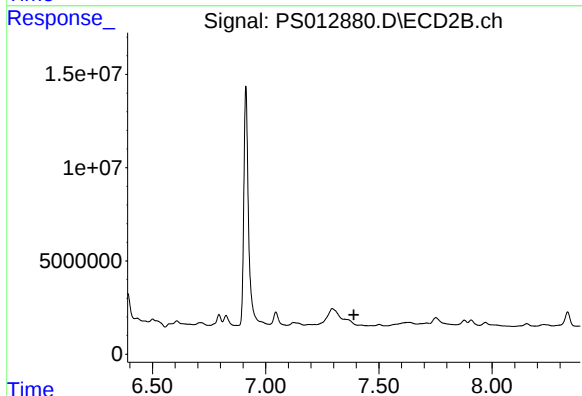


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.390 min
Response: 0
Conc: N.D.

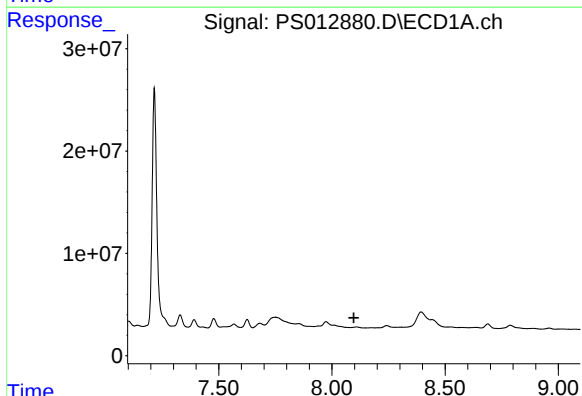


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.097 min
Response: 0
Conc: N.D.

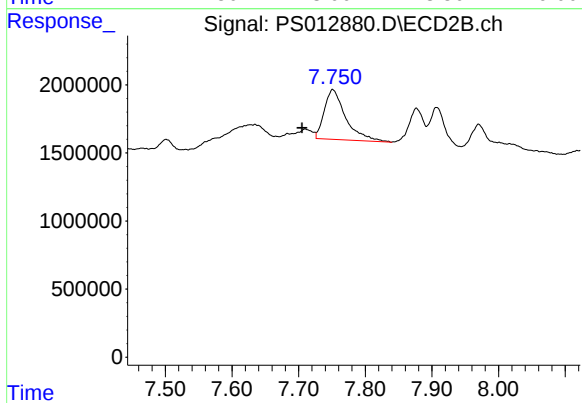

#8 DICHLORPROP


R.T.: 7.751 min
Delta R.T.: 0.046 min
Response: 8141594
Conc: 15.77 ng/ml

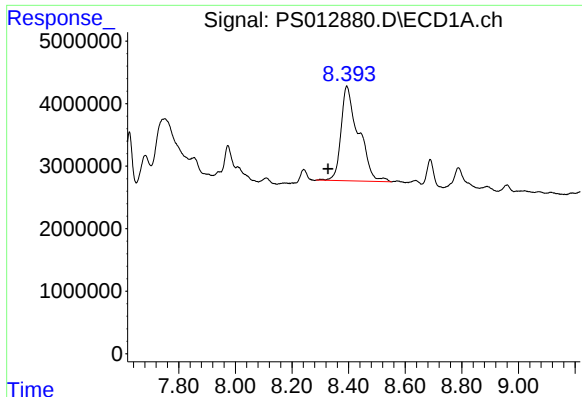

#9 2,4-D


R.T.: 8.394 min
Delta R.T.: 0.066 min
Response: 64975634
Conc: 57.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

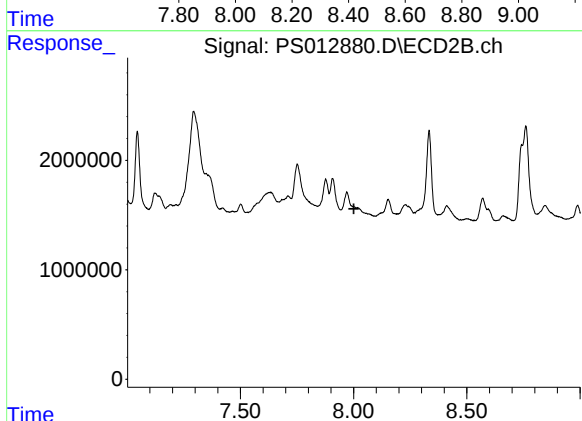


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.001 min
Response: 0
Conc: N.D.

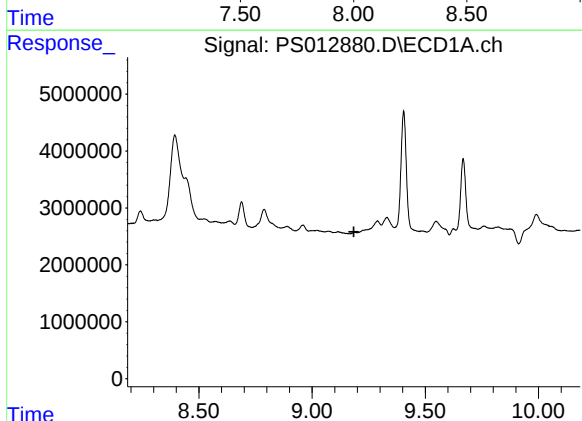


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.185 min
Response: 0
Conc: N.D.

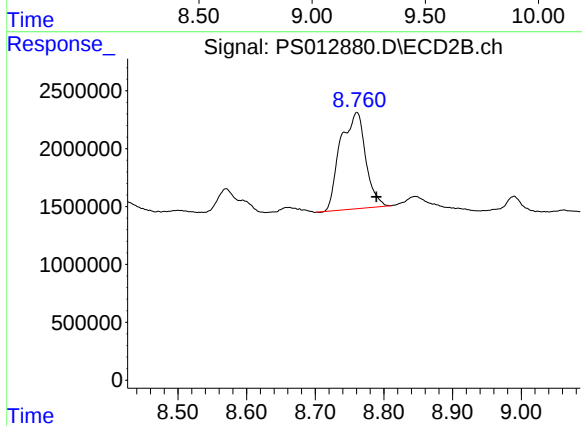

#11 2,4,5-TP (SILVEX)


R.T.: 8.761 min
Delta R.T.: -0.028 min
Response: 21257442
Conc: 8.06 ng/ml

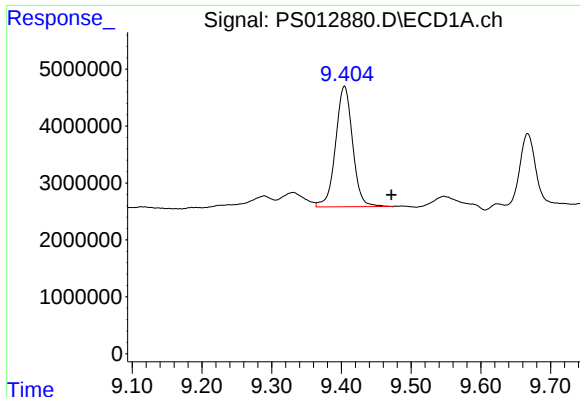

#12 2,4,5-T


R.T.: 9.404 min
Delta R.T.: -0.067 min
Response: 35917641
Conc: 6.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

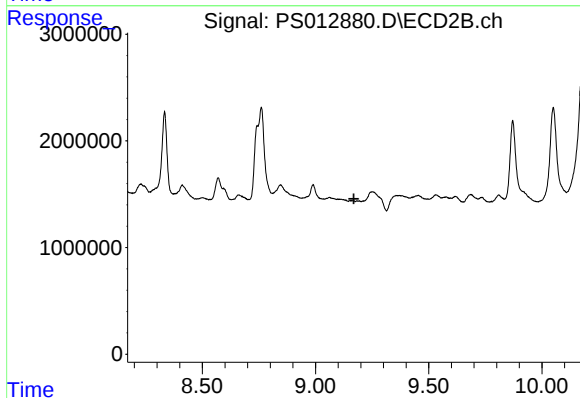


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.169 min
Response: 0
Conc: N.D.

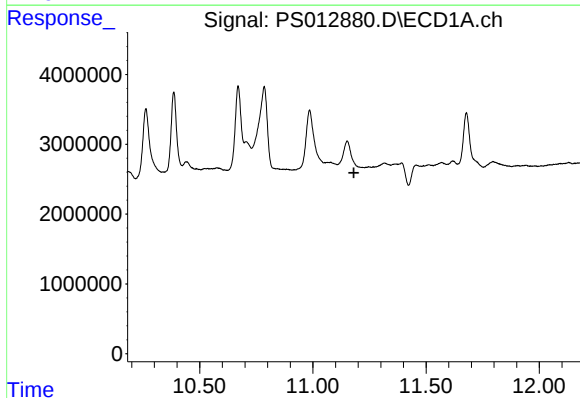


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.181 min
Response: 0
Conc: N.D.

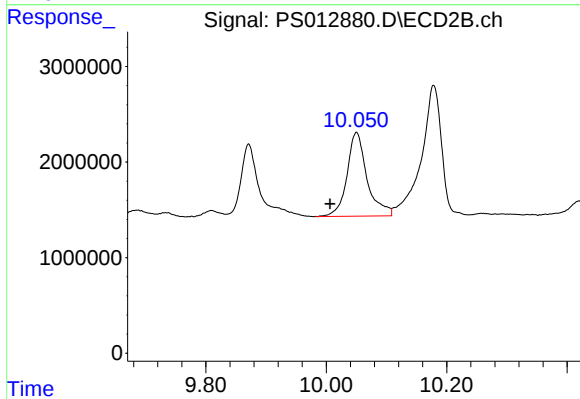

#14 DINOSEB


R.T.: 10.050 min
Delta R.T.: 0.044 min
Response: 20345501
Conc: 10.62 ng/ml

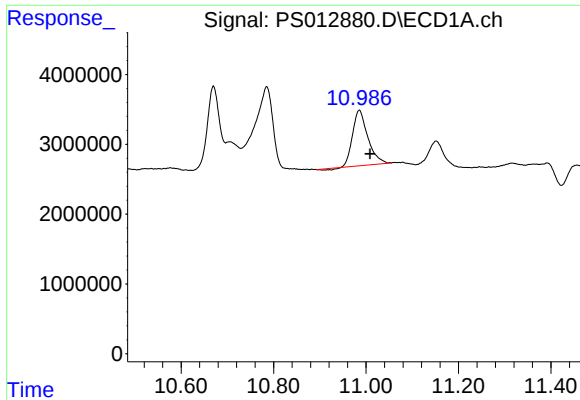

#15 Picloram

R.T.: 10.985 min
Delta R.T.: -0.023 min
Response: 18053476
Conc: 2.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

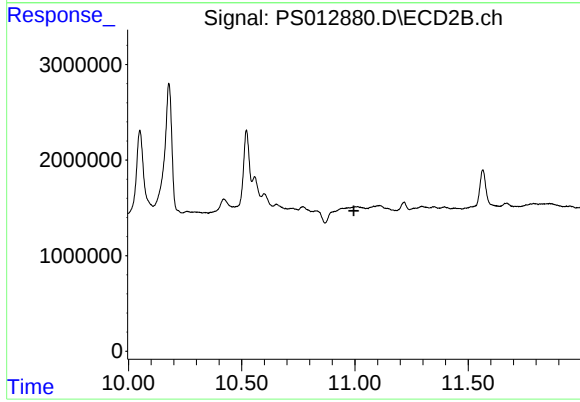

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.