

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101624\
 Data File : PS027960.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 10:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 06:27:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 07 13:46:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.095	7.621	1447.3E6	483.8E6	537.156	486.829
Target Compounds							
1) T	Dalapon	2.526	2.630	756679	1170043	<MDL	<MDL #
3) T	4-Nitroph...	6.892	0.000	10055325	0	5.507	N.D. #
6) T	MCPD	0.000	7.934	0	2224281	N.D.	<MDL
7) T	MCPA	7.631f	8.138	607852	7002862	<MDL	1.400 #
8) T	DICHLORPROP	8.014f	8.560f	4154721	1747744	1.452	1.771
10) T	Pentachlo...	8.471	0.000	3504404	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.728	0	1449213	N.D.	<MDL
12) T	2,4,5-T	9.327	10.160	9503281	2389188	<MDL	<MDL #
13) T	2,4-DB	9.881	0.000	1645885	0	<MDL	N.D. #
14) T	DINOSEB	11.054	0.000	3430685	0	<MDL	N.D. #
15) T	Picloram	10.883	12.177	76949309	6639301	3.574	1.589 #
16) T	DCPA	11.352	12.113	2623788	2776306	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101624\
Data File : PS027960.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 10:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 06:27:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

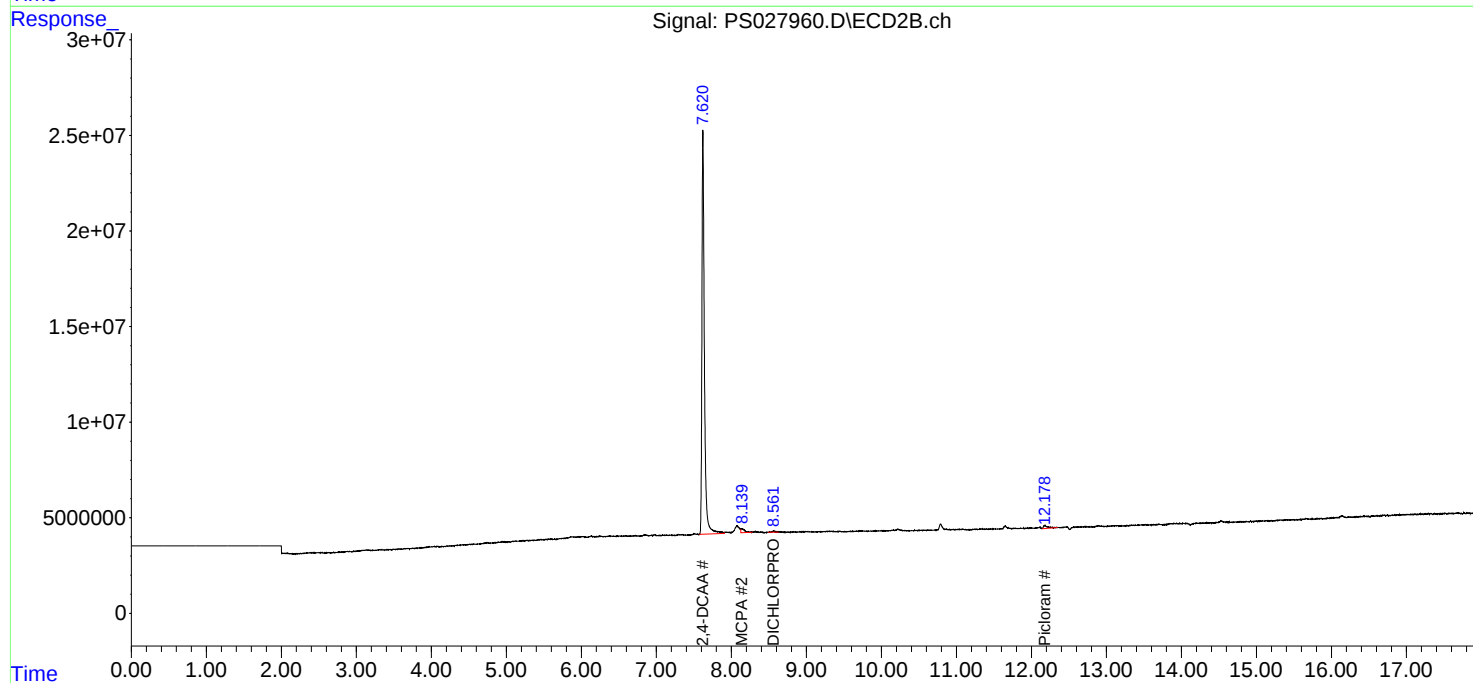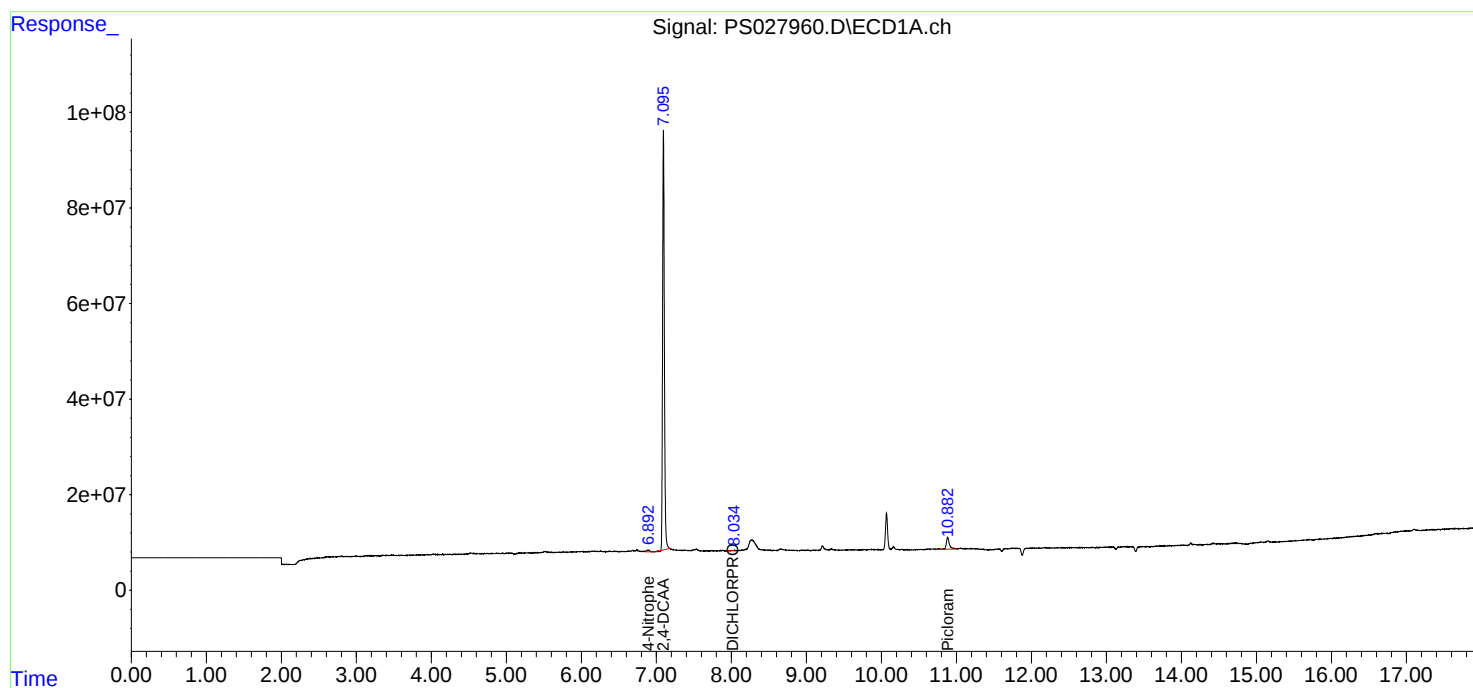


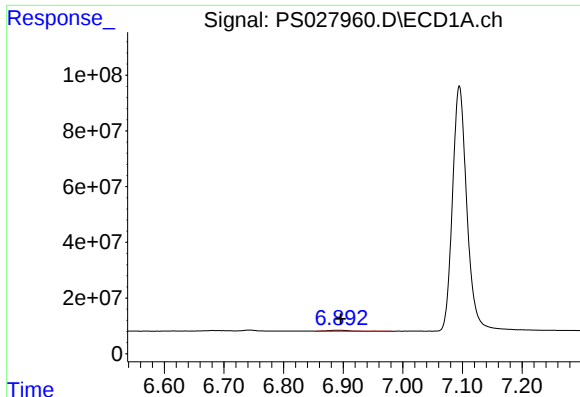

#3 4-Nitrophenol


R.T.: 6.892 min
Delta R.T.: -0.004 min
Response: 10055325
Conc: 5.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

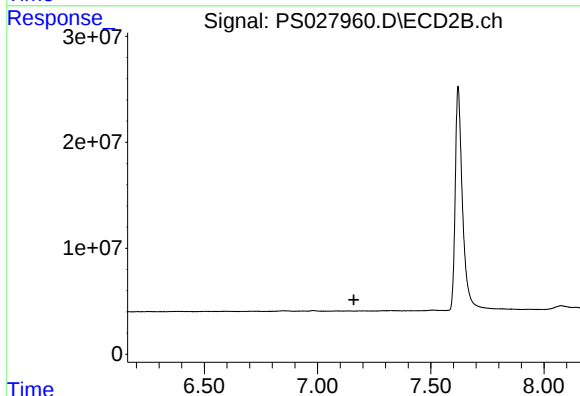


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.160 min
Response: 0
Conc: N.D.

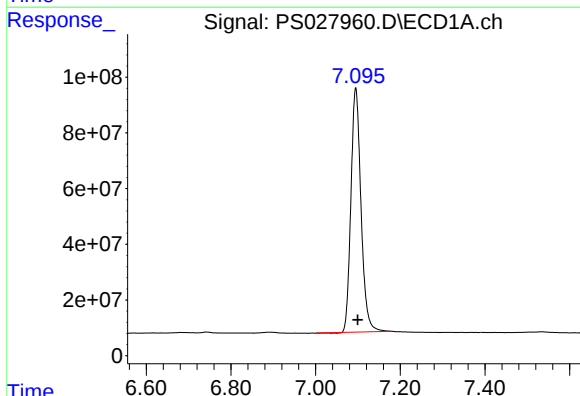


#4 2,4-DCAA

R.T.: 7.095 min
Delta R.T.: -0.005 min
Response: 1447255597
Conc: 537.16 ng/ml

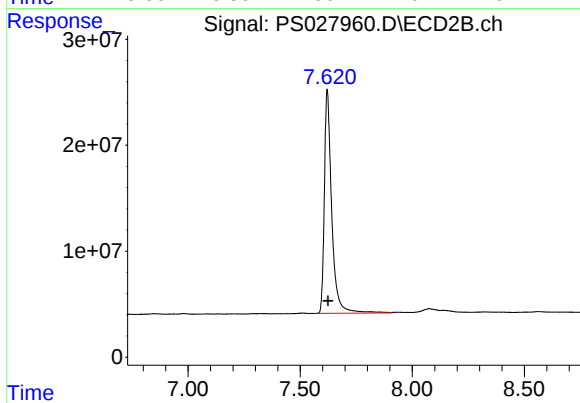

#4 2,4-DCAA


R.T.: 7.621 min
Delta R.T.: -0.004 min
Response: 483754518
Conc: 486.83 ng/ml

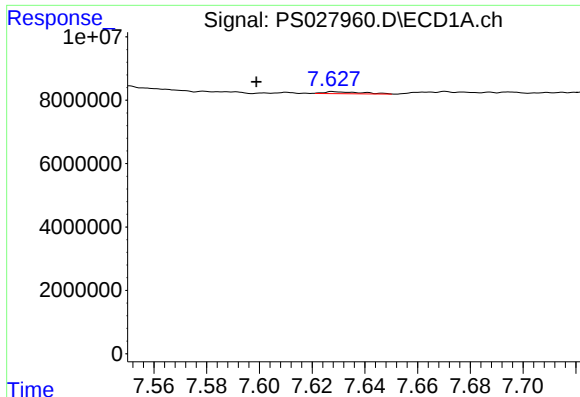

#7 MCPA


R.T.: 7.631 min
Delta R.T.: 0.032 min
Response: 607852
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

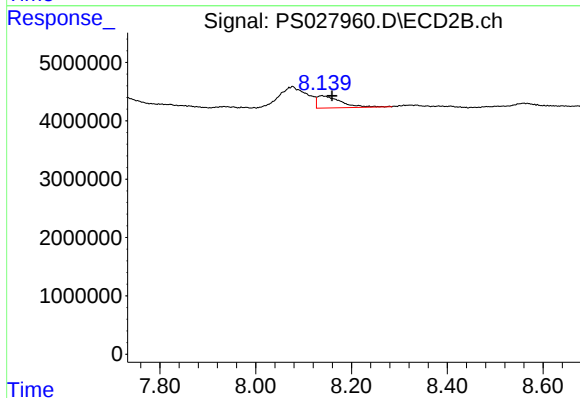


#7 MCPA

R.T.: 8.138 min
Delta R.T.: -0.022 min
Response: 7002862
Conc: 1.40 ug/ml

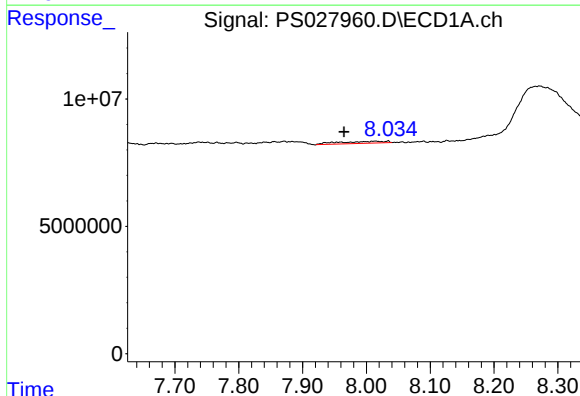


#8 DICHLORPROP

R.T.: 8.014 min
Delta R.T.: 0.049 min
Response: 4154721
Conc: 1.45 ng/ml

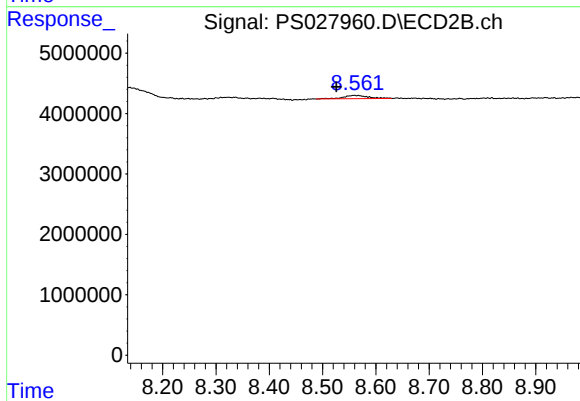

#8 DICHLORPROP


R.T.: 8.560 min
Delta R.T.: 0.034 min
Response: 1747744
Conc: 1.77 ng/ml

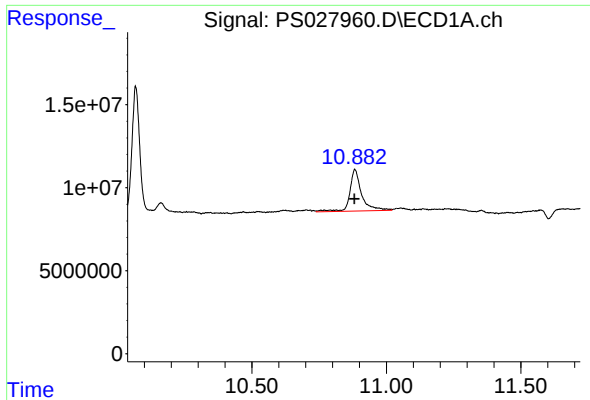

#15 Picloram

R.T.: 10.883 min
Delta R.T.: 0.002 min
Response: 76949309
Conc: 3.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

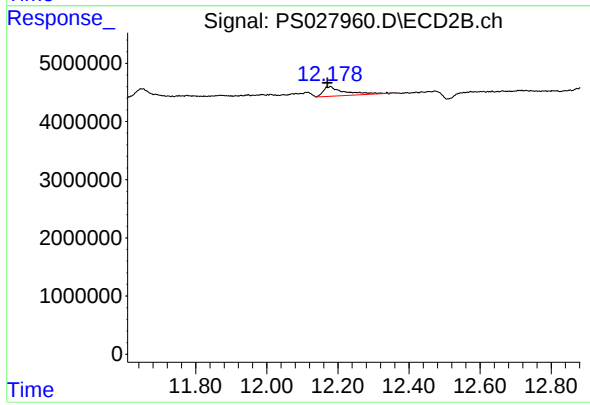

#15 Picloram

R.T.: 12.177 min
Delta R.T.: 0.006 min
Response: 6639301
Conc: 1.59 ng/ml