

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101624\
 Data File : PS027964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Oct 2024 14:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 06:29:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 07 13:46:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.094	7.621	1445.6E6	477.9E6	536.554	480.967
Target Compounds							
1) T	Dalapon	2.549	2.644f	14901389	934493	3.320	<MDL #
3) T	4-Nitroph...	6.890	0.000	9988695	0	5.471	N.D. #
5) T	DICAMBA	0.000	7.802	0	6856276	N.D.	1.972
6) T	MCP	0.000	7.950f	0	1190005	N.D.	<MDL
8) T	DICHLORPROP	7.953	8.564f	1380348	2270927	<MDL	2.301 #
9) T	2,4-D	0.000	8.801f	0	381695	N.D.	<MDL
10) T	Pentachlo...	0.000	9.355	0	2308625	N.D.	<MDL
11) T	2,4,5-TP ...	9.023	9.719	3714834	1268928	<MDL	<MDL #
12) T	2,4,5-T	9.338	0.000	1771404	0	<MDL	N.D. #
14) T	DINOSEB	11.024f	0.000	3461174	0	<MDL	N.D. #
15) T	Picloram	10.879	12.195f	15302123	2624285	<MDL	<MDL #
16) T	DCPA	11.354	12.103	2220796	2871279	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101624\
Data File : PS027964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Oct 2024 14:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 06:29:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

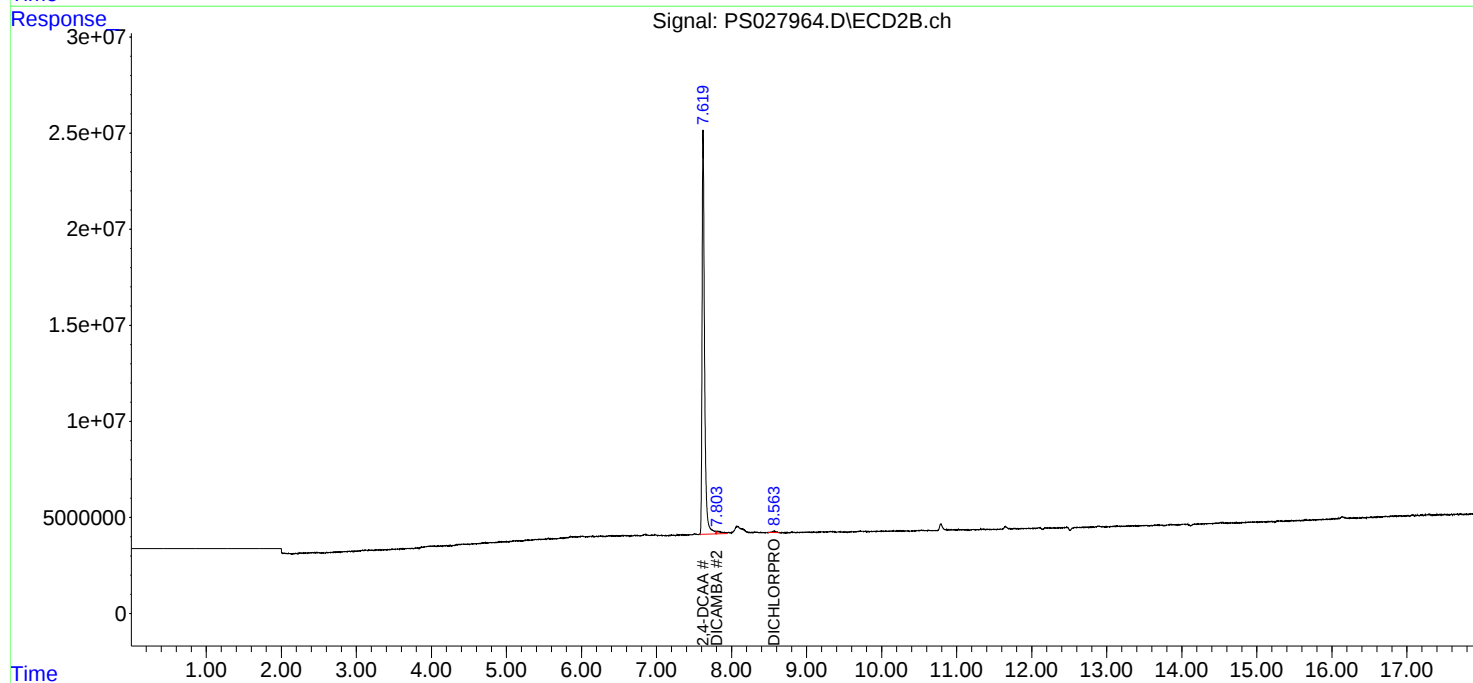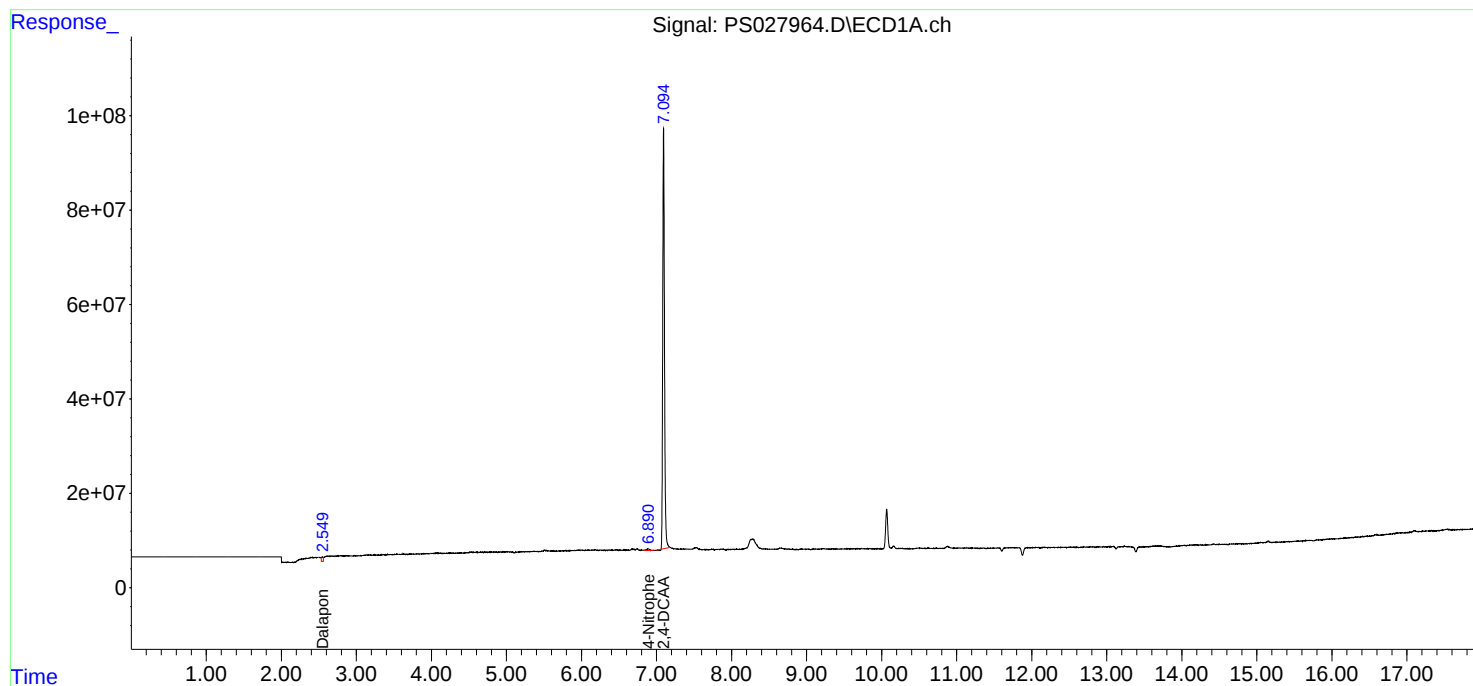


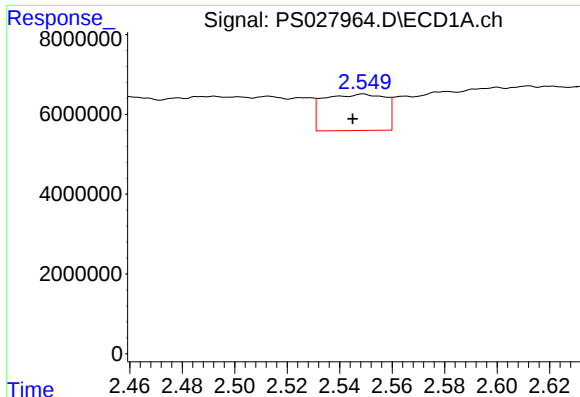

#1 Dalapon


R.T.: 2.549 min
Delta R.T.: 0.004 min
Response: 14901389
Conc: 3.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

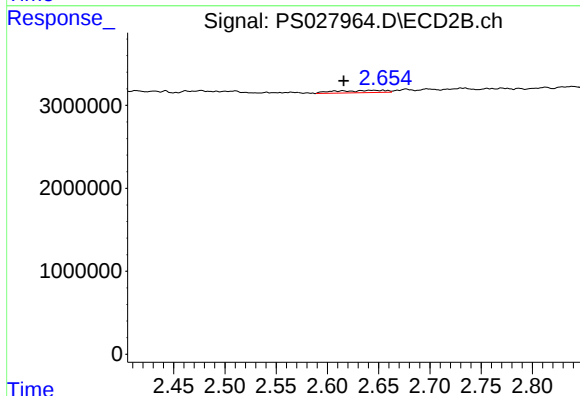


#1 Dalapon

R.T.: 2.644 min
Delta R.T.: 0.028 min
Response: 934493
Conc: N.D.

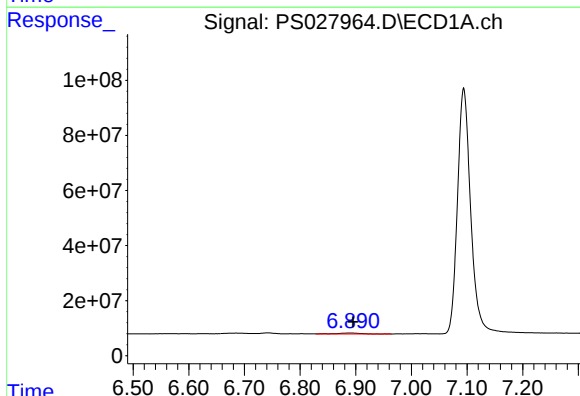


#3 4-Nitrophenol

R.T.: 6.890 min
Delta R.T.: -0.006 min
Response: 9988695
Conc: 5.47 ng/ml

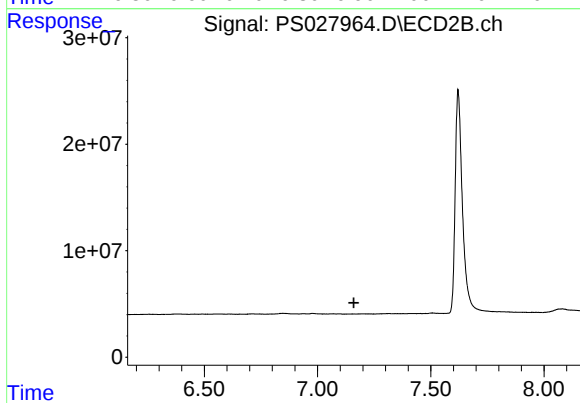

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.160 min
Response: 0
Conc: N.D.

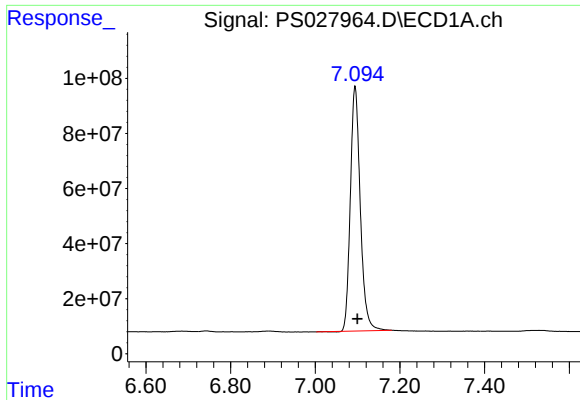

#4 2,4-DCAA


R.T.: 7.094 min
Delta R.T.: -0.006 min
Response: 1445632763
Conc: 536.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

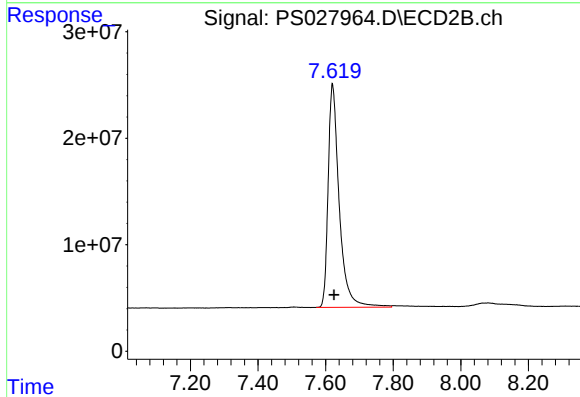


#4 2,4-DCAA

R.T.: 7.621 min
Delta R.T.: -0.004 min
Response: 477930400
Conc: 480.97 ng/ml

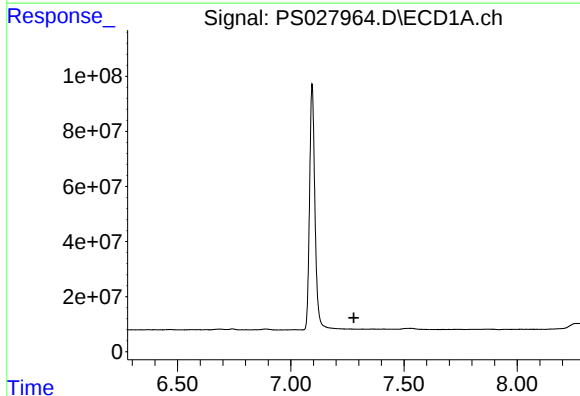


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.279 min
Response: 0
Conc: N.D.

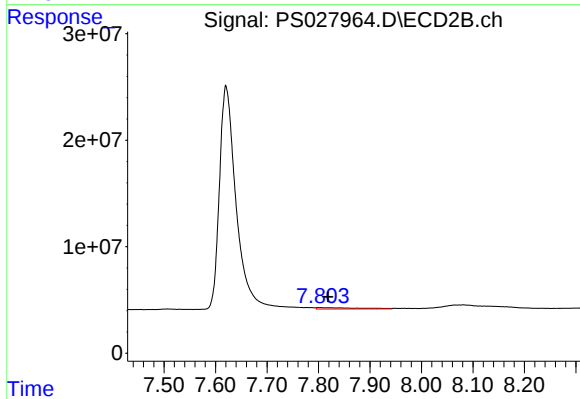

#5 DICAMBA


R.T.: 7.802 min
Delta R.T.: -0.017 min
Response: 6856276
Conc: 1.97 ng/ml

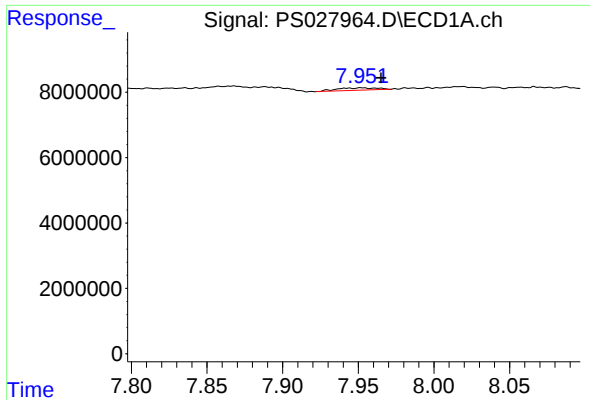

#8 DICHLORPROP

R.T.: 7.953 min
Delta R.T.: -0.012 min
Response: 1380348
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

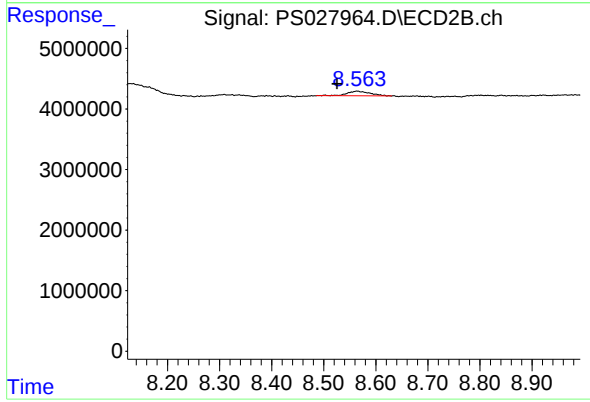

#8 DICHLORPROP

R.T.: 8.564 min
Delta R.T.: 0.038 min
Response: 2270927
Conc: 2.30 ng/ml