

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101719\
 Data File : PS007197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2019 16:34
 Operator : SM\AJ
 Sample : PB124053BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB124053BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 17 18:01:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.442	5.165	559.8E6	350.0E6	409.005	497.718
Target Compounds							
5) T	DICAMBA	0.000	5.295	0 10671811	N.D.		4.101
15) T	Picloram	0.000	8.944	0 15092120	N.D.		2.458



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101719\
Data File : PS007197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 16:34
Operator : SM\AJ
Sample : PB124053BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB124053BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 17 18:01:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

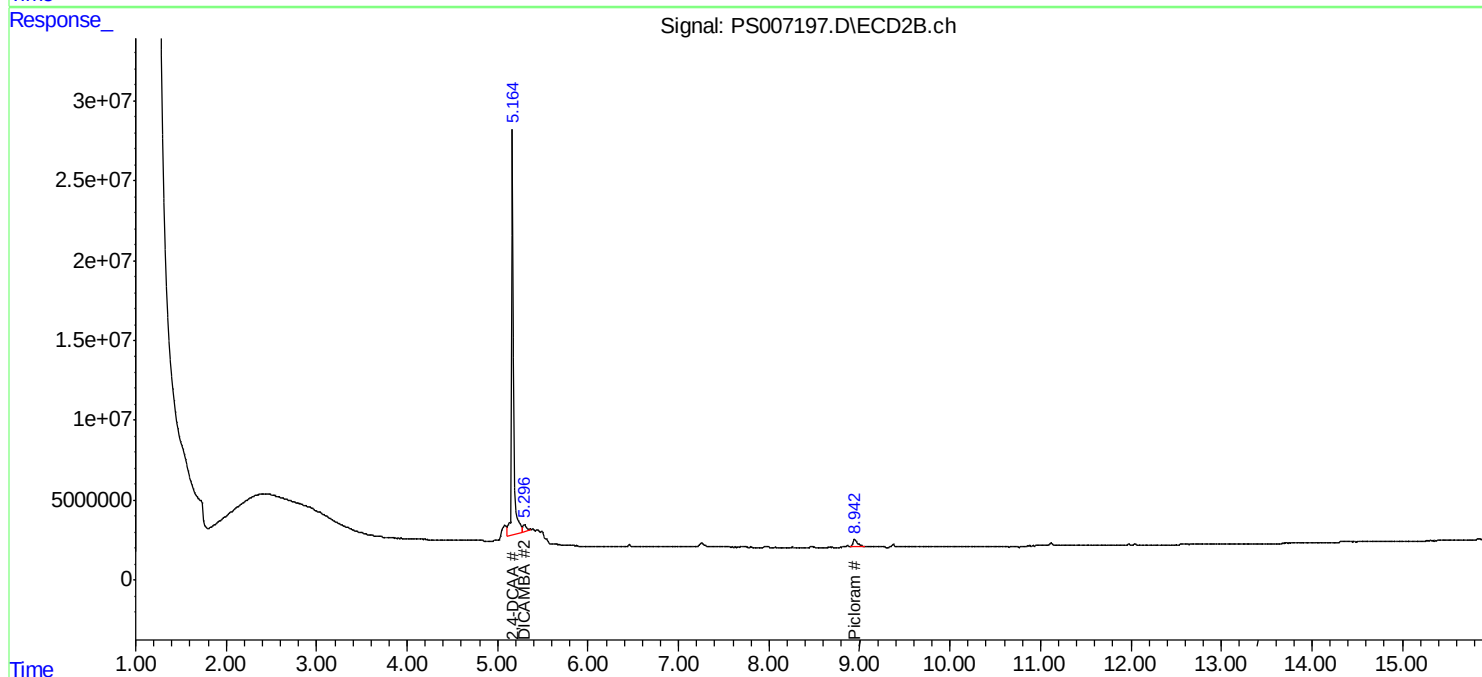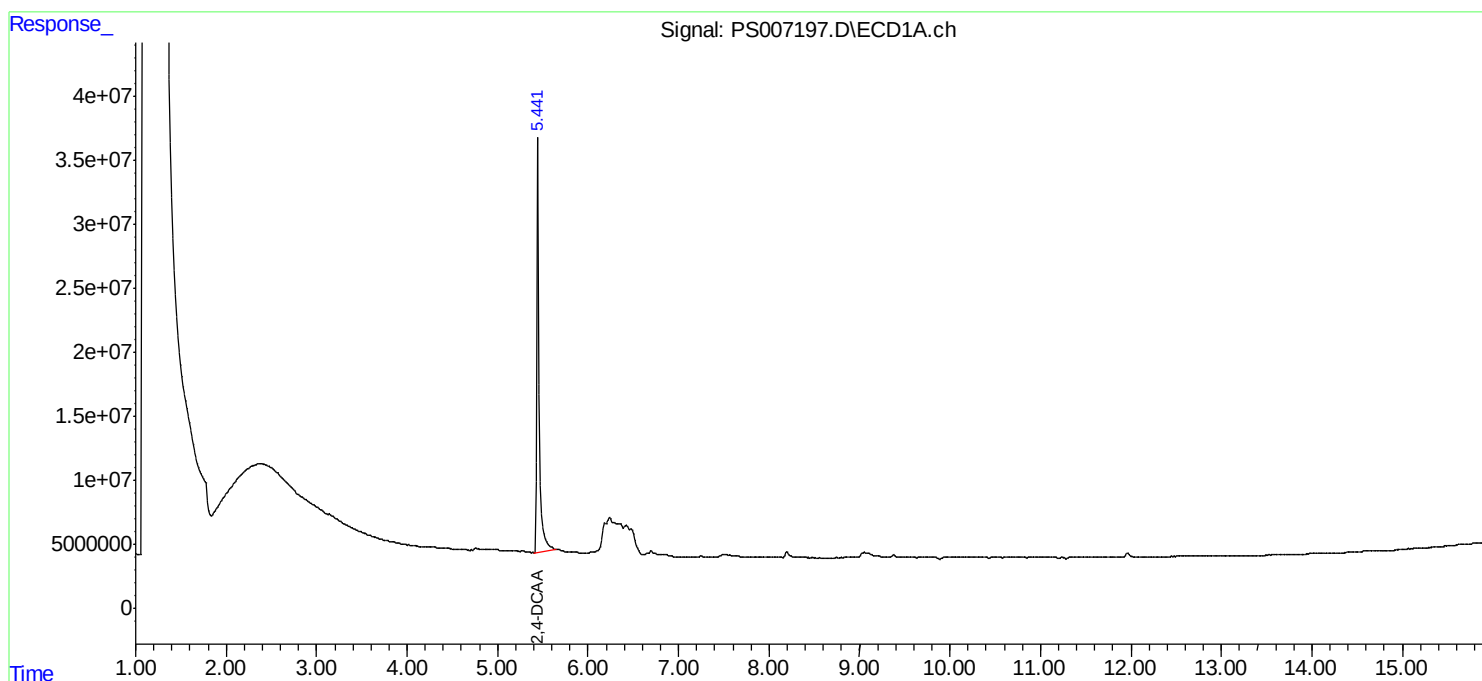


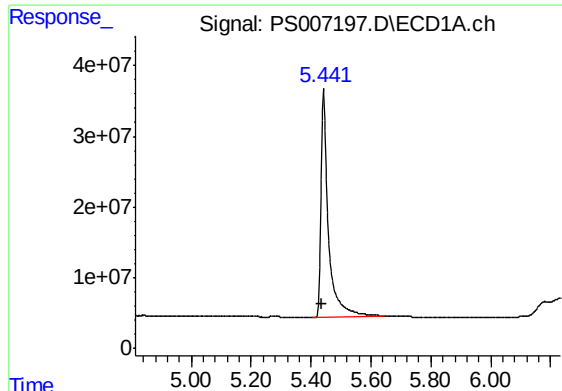

#4 2,4-DCAA


R.T.: 5.442 min
Delta R.T.: 0.007 min
Response: 559792694
Conc: 409.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124053BL

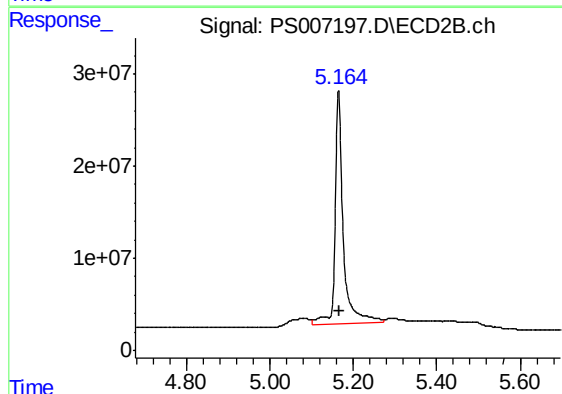


#4 2,4-DCAA

R.T.: 5.165 min
Delta R.T.: -0.004 min
Response: 350048050
Conc: 497.72 ng/ml

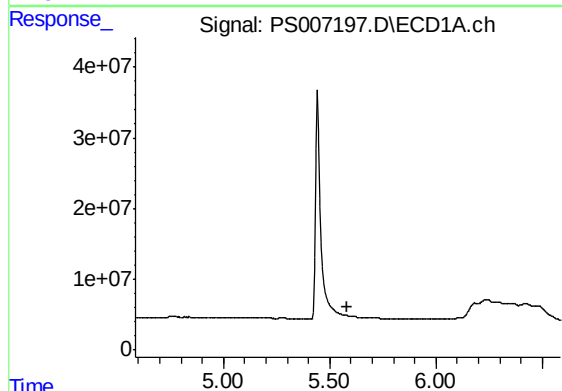


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.585 min
Response: 0
Conc: N.D.

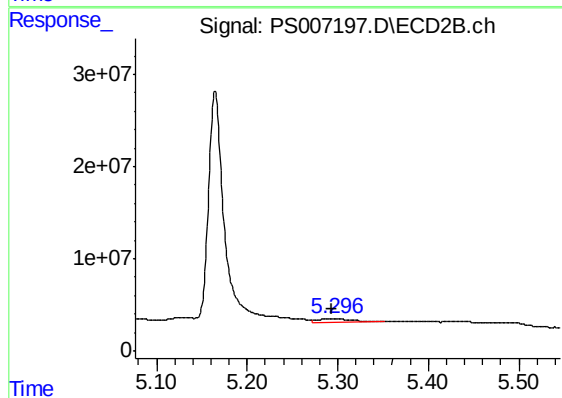

#5 DICAMBA


R.T.: 5.295 min
Delta R.T.: 0.000 min
Response: 10671811
Conc: 4.10 ng/ml

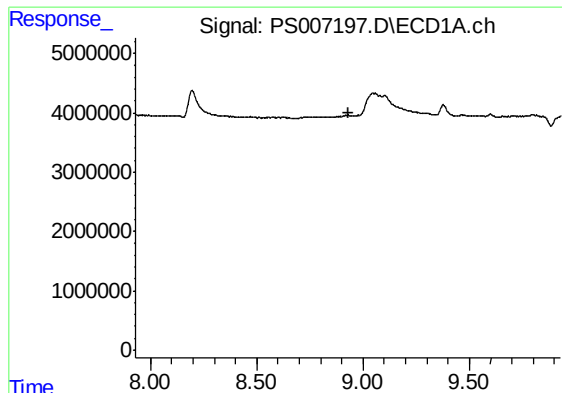

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 8.929 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124053BL

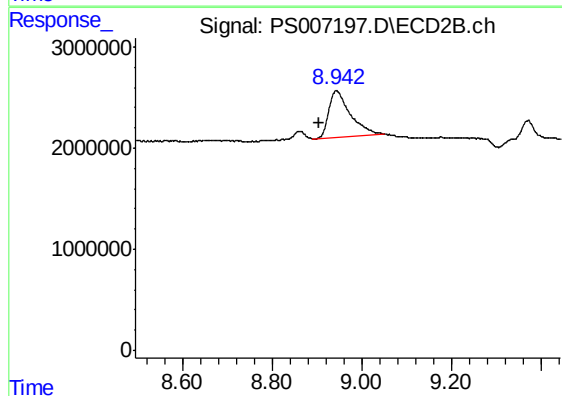

#15 Picloram

R.T.: 8.944 min
Delta R.T.: 0.039 min
Response: 15092120
Conc: 2.46 ng/ml