

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101719\
 Data File : PS007203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2019 18:46
 Operator : SM\AJ
 Sample : K5152-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 00:54:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.454	5.185	615.3E6	346.5E6	449.592	492.625
Target Compounds							
1) T	Dalapon	2.007	1.720	196.4E6	348.9E6	117.369	383.408 #
2) T	3,5-DICHL...	0.000	4.475	0	8787907	N.D.	10.213
3) T	4-Nitroph...	0.000	4.861	0	23003720	N.D.	58.253
5) T	DICAMBA	5.546	5.316	47951413	6168661	9.759	2.371 #
6) T	MCPD	0.000	5.316	0	6168661	N.D.	3.252
7) T	MCPA	0.000	5.502	0	48396528	N.D.	16.648
9) T	2,4-D	0.000	6.030	0	28893044	N.D.	36.216
10) T	Pentachlo...	0.000	6.482	0	9407105	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.786	0	59951486	N.D.	15.762
12) T	2,4,5-T	7.424	0.000	163.2E6	0	21.350	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101719\
Data File : PS007203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 18:46
Operator : SM\AJ
Sample : K5152-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 00:54:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

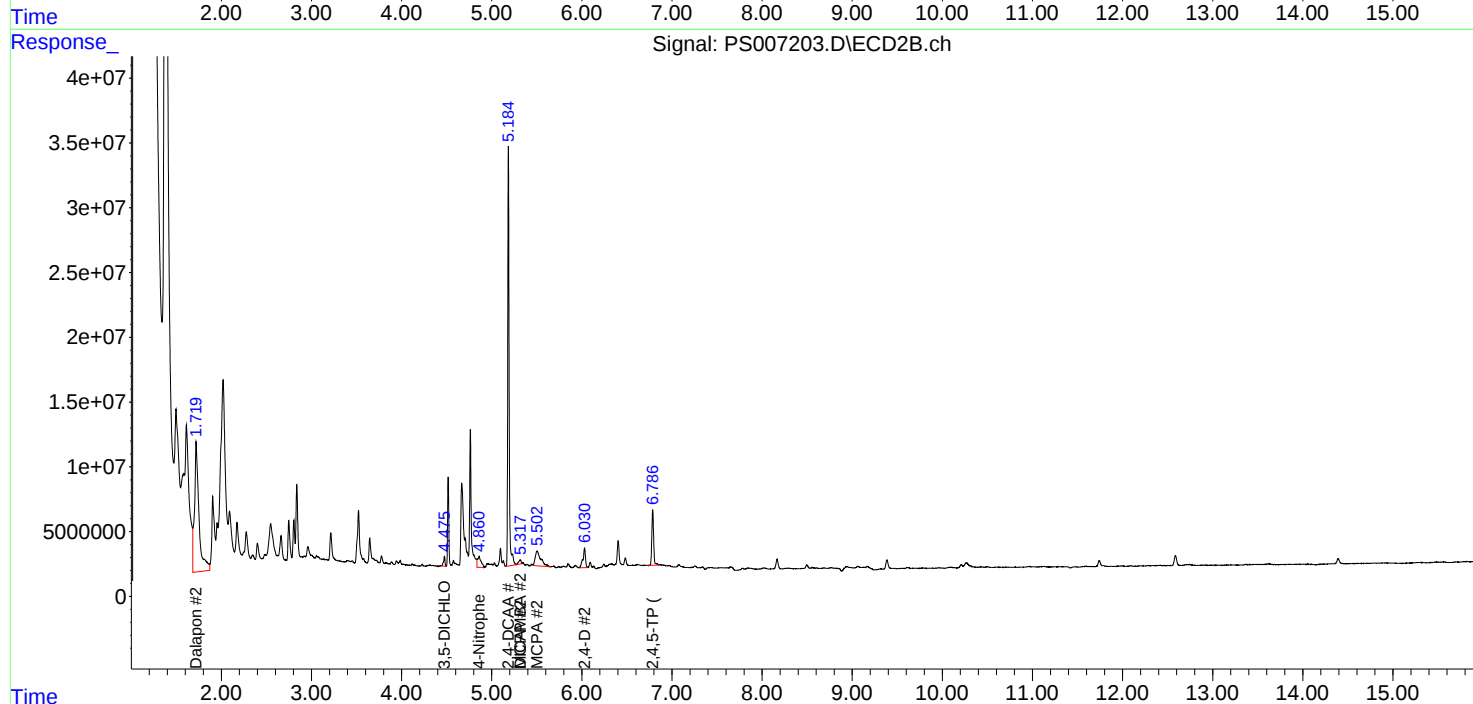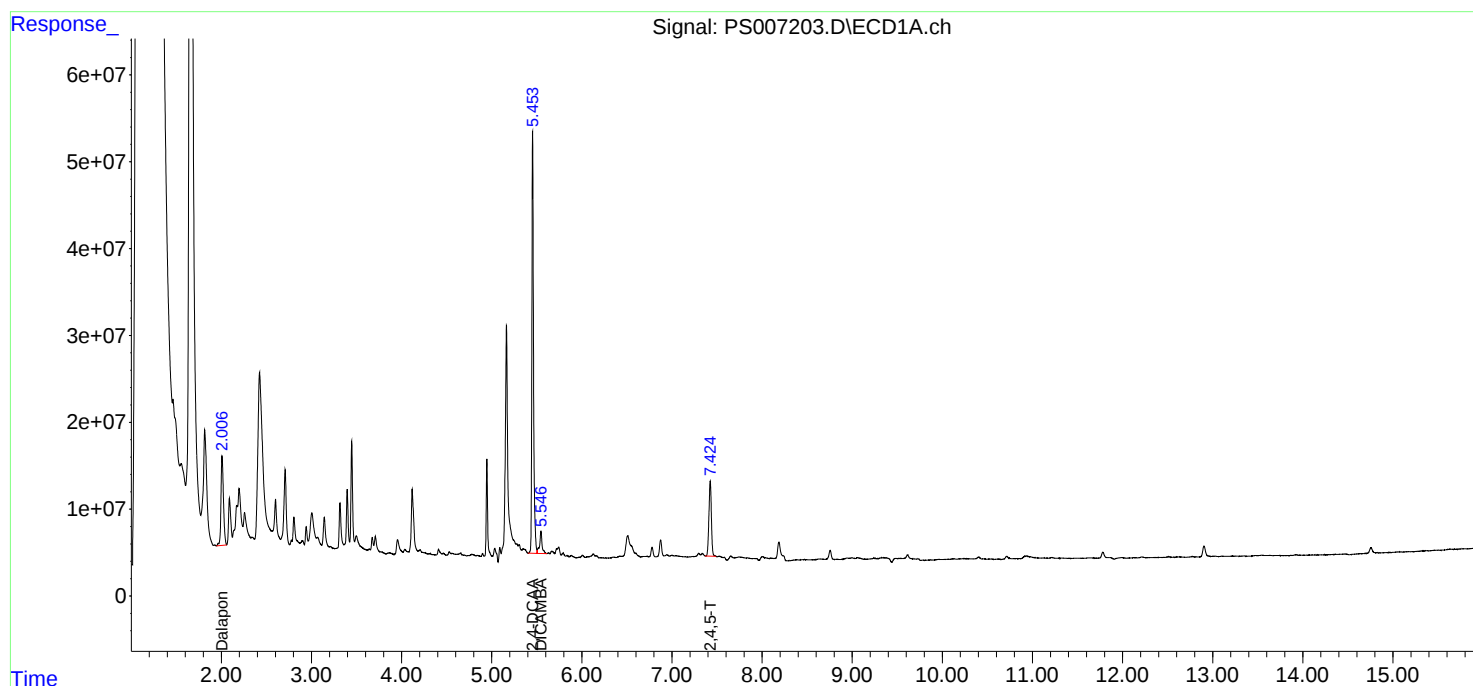


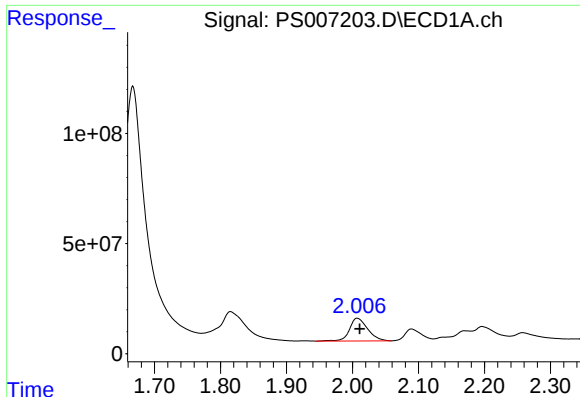

#1 Dalapon


R.T.: 2.007 min
Delta R.T.: -0.004 min
Response: 196390659
Conc: 117.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

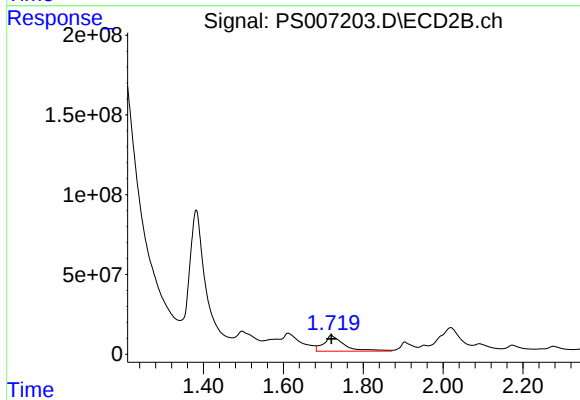


#1 Dalapon

R.T.: 1.720 min
Delta R.T.: 0.000 min
Response: 348902200
Conc: 383.41 ng/ml

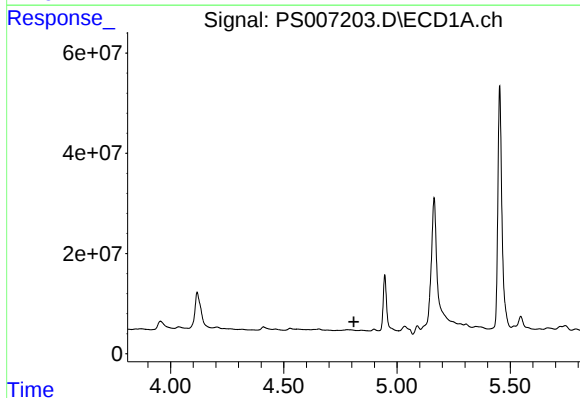


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

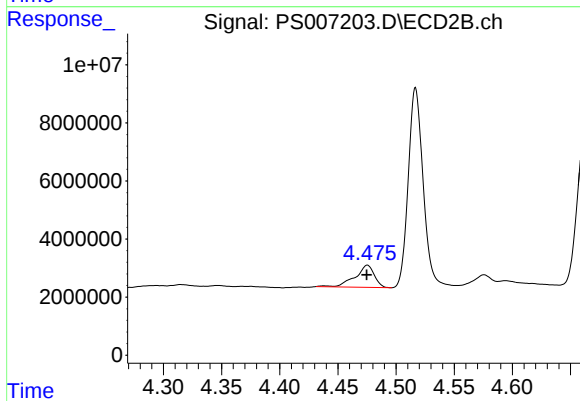

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.475 min
Delta R.T.: 0.000 min
Response: 8787907
Conc: 10.21 ng/ml

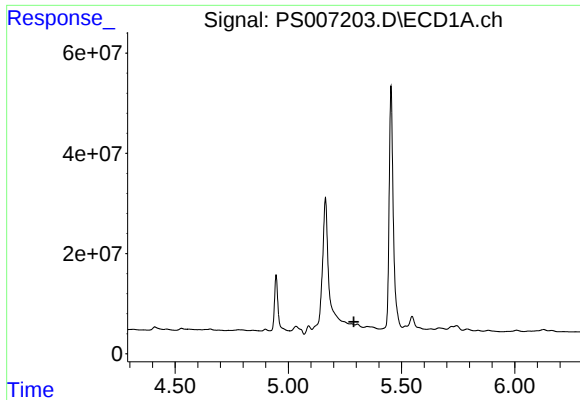

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

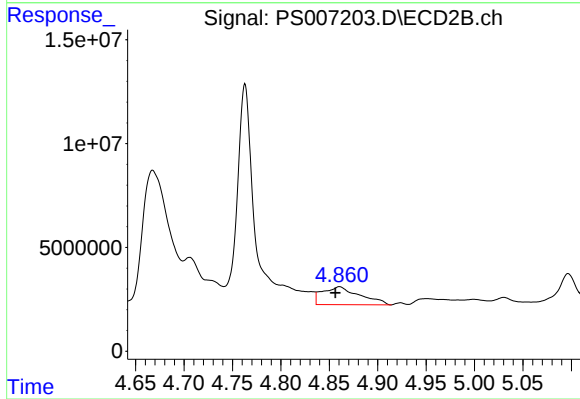


#3 4-Nitrophenol

R.T.: 4.861 min
Delta R.T.: 0.004 min
Response: 23003720
Conc: 58.25 ng/ml

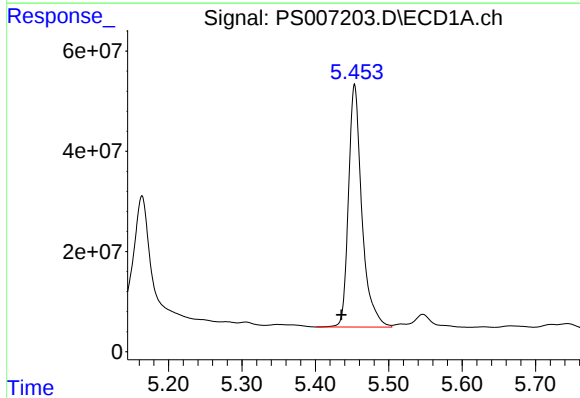


#4 2,4-DCAA

R.T.: 5.454 min
Delta R.T.: 0.018 min
Response: 615341833
Conc: 449.59 ng/ml

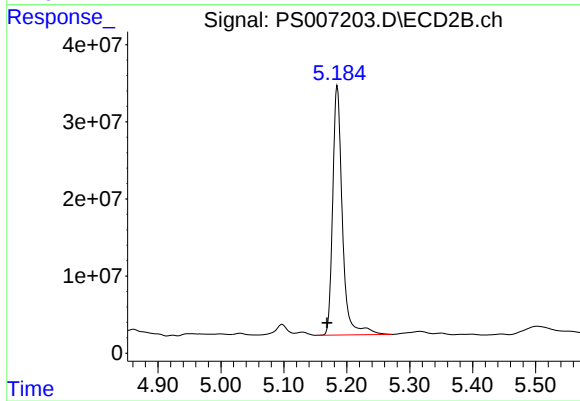

#4 2,4-DCAA


R.T.: 5.185 min
Delta R.T.: 0.016 min
Response: 346466622
Conc: 492.63 ng/ml

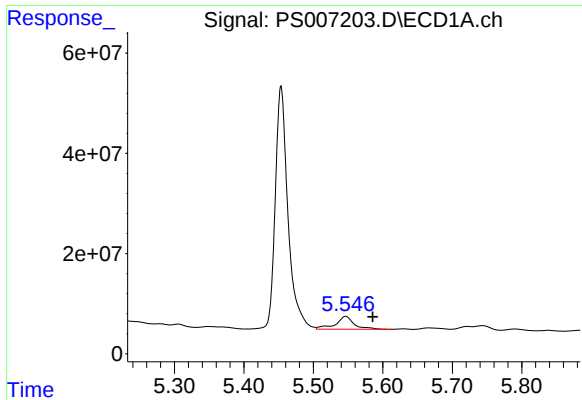

#5 DICAMBA


R.T.: 5.546 min
Delta R.T.: -0.039 min
Response: 47951413
Conc: 9.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

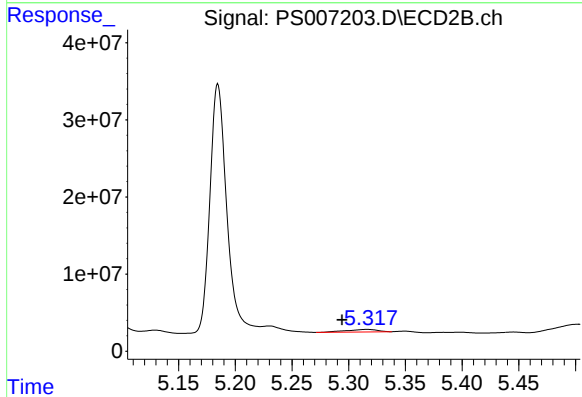


#5 DICAMBA

R.T.: 5.316 min
Delta R.T.: 0.022 min
Response: 6168661
Conc: 2.37 ng/ml

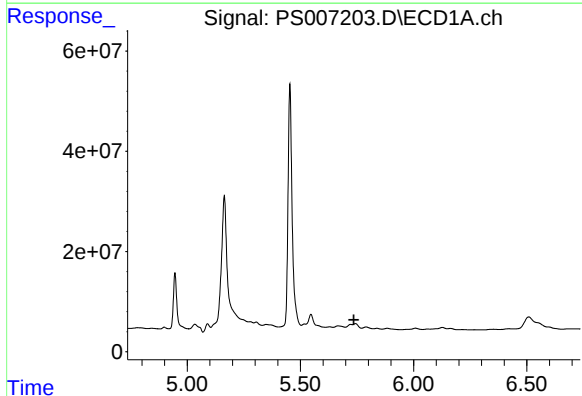


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.736 min
Response: 0
Conc: N.D.

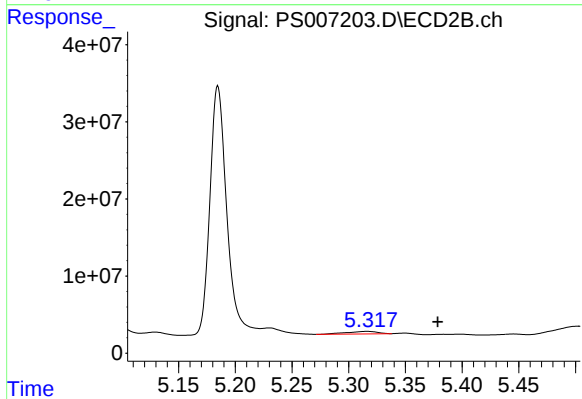

#6 MCP


R.T.: 5.316 min
Delta R.T.: -0.063 min
Response: 6168661
Conc: 3.25 ug/ml

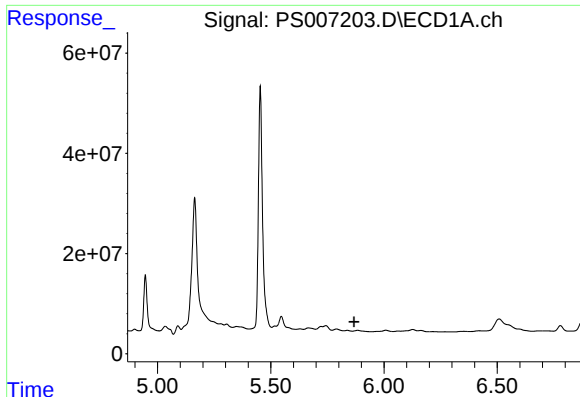

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

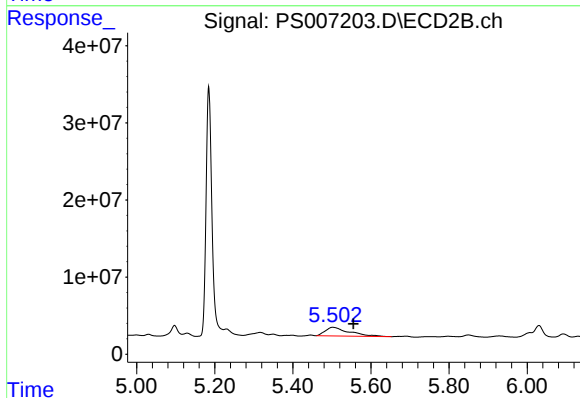


#7 MCPA

R.T.: 5.502 min
Delta R.T.: -0.052 min
Response: 48396528
Conc: 16.65 ug/ml

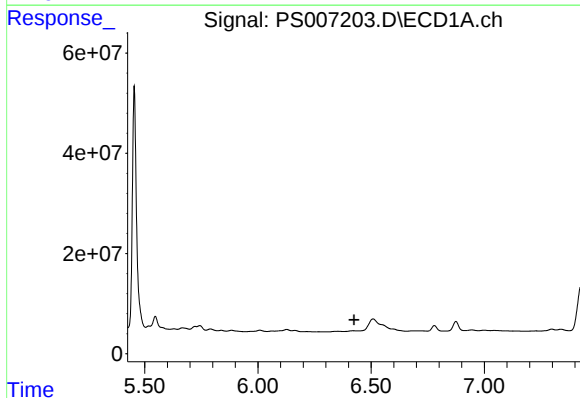


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

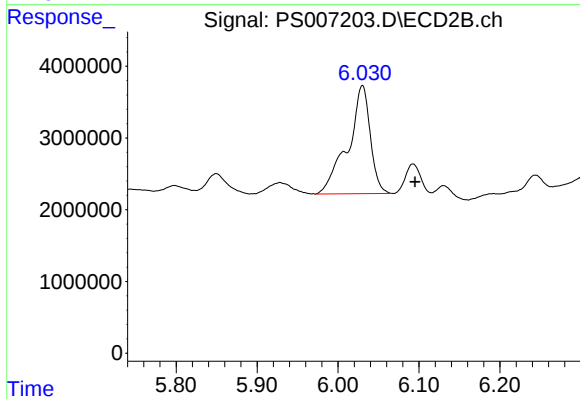

#9 2,4-D


R.T.: 6.030 min
Delta R.T.: -0.065 min
Response: 28893044
Conc: 36.22 ng/ml

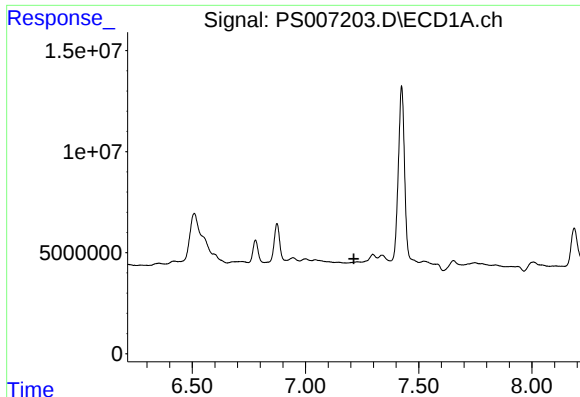

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

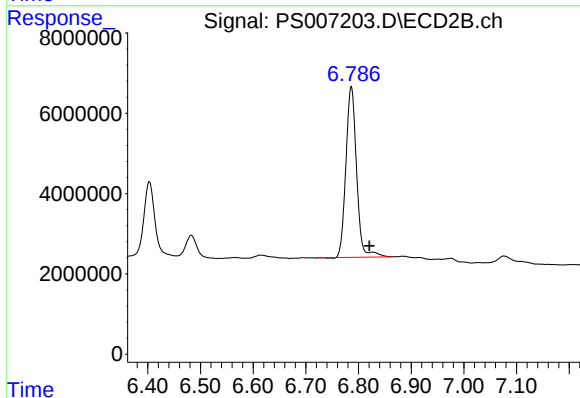


#11 2,4,5-TP (SILVEX)

R.T.: 6.786 min
Delta R.T.: -0.034 min
Response: 59951486
Conc: 15.76 ng/ml

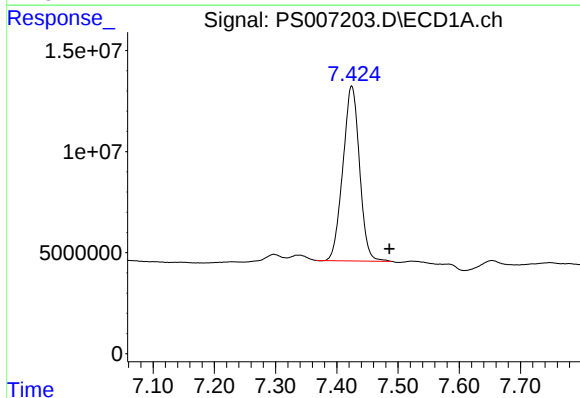

#12 2,4,5-T

R.T.: 7.424 min
Delta R.T.: -0.061 min
Response: 163212665
Conc: 21.35 ng/ml

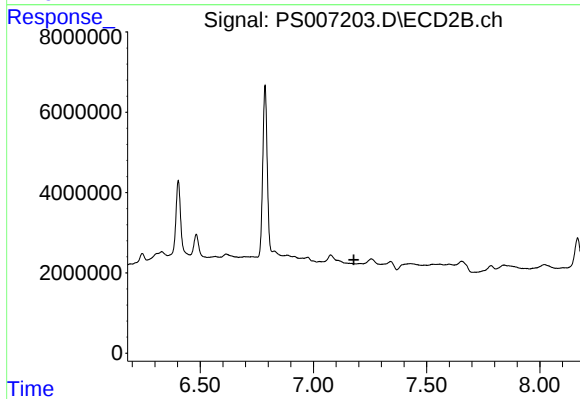

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.178 min
Response: 0
Conc: N.D.