

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101719\
 Data File : PS007206.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2019 19:52
 Operator : SM\AJ
 Sample : K5153-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 00:54:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.454	5.185	594.1E6	337.0E6	434.055	479.102
Target Compounds							
1) T	Dalapon	2.009	1.722	203.9E6	382.6E6	121.828	420.417 #
2) T	3,5-DICHL...	0.000	4.463	0	16688294	N.D.	19.395
5) T	DICAMBA	5.548	0.000	38592732	0	7.855	N.D. #
7) T	MCPA	0.000	5.504	0	75194472	N.D.	25.866
8) T	DICHLORPROP	0.000	5.843	0	71077779	N.D.	109.146
9) T	2,4-D	0.000	6.143	0	18214527	N.D.	22.831
10) T	Pentachlo...	0.000	6.483	0	8012914	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.814	0	116.0E6	N.D.	30.489
12) T	2,4,5-T	7.423	0.000	109.0E6	0	14.264	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101719\
Data File : PS007206.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 19:52
Operator : SM\AJ
Sample : K5153-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 00:54:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

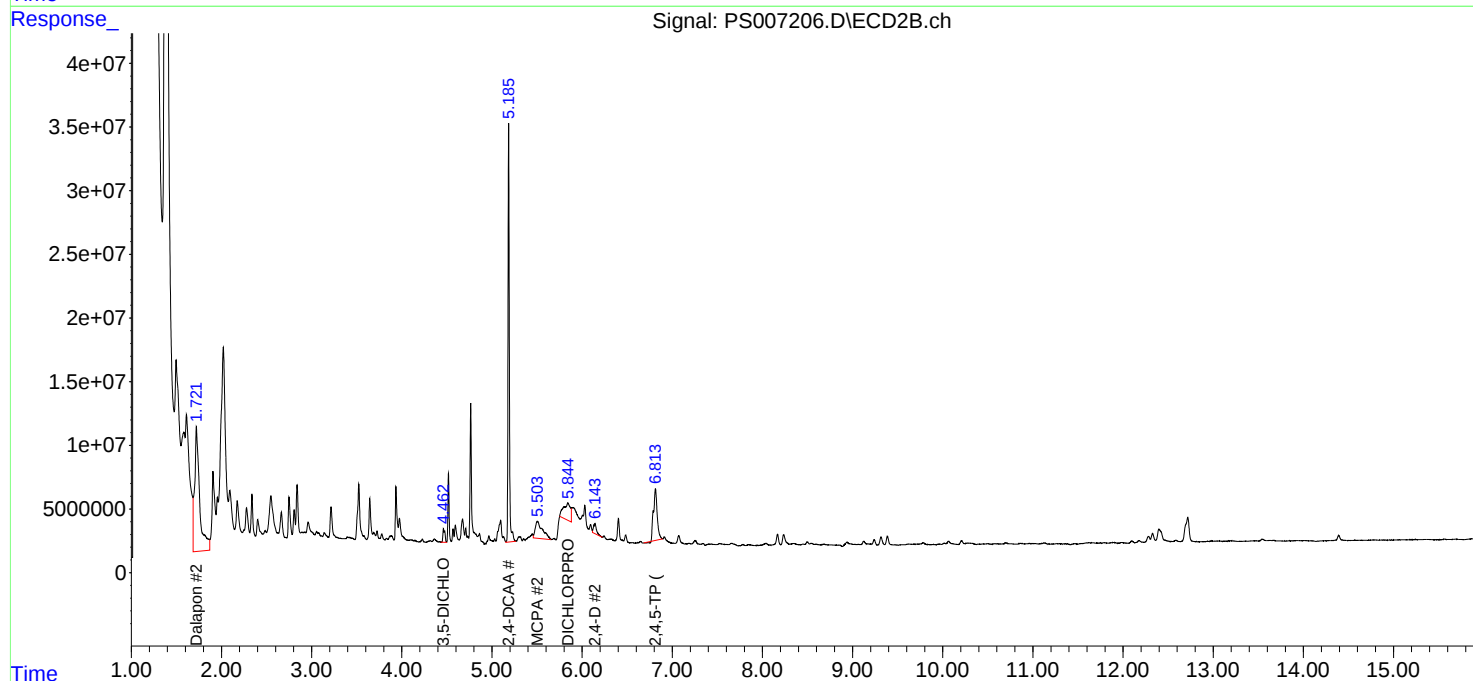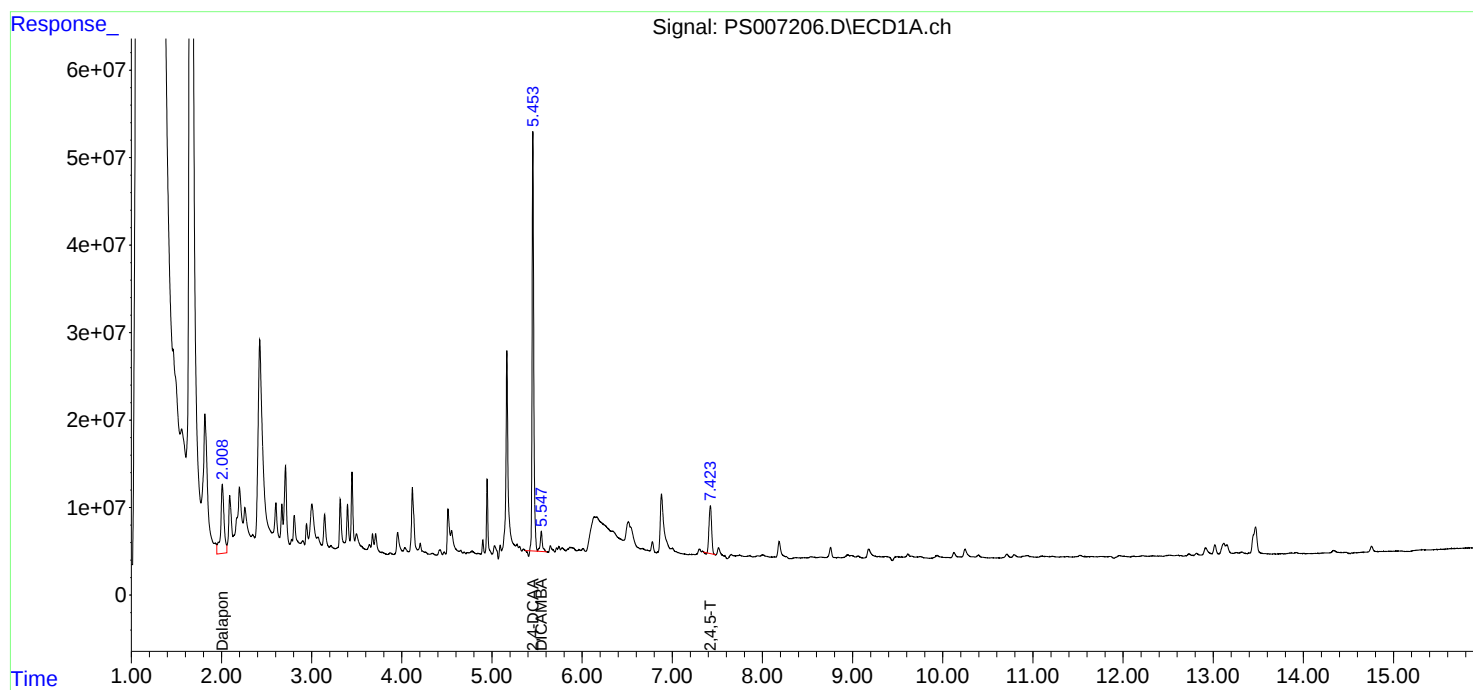


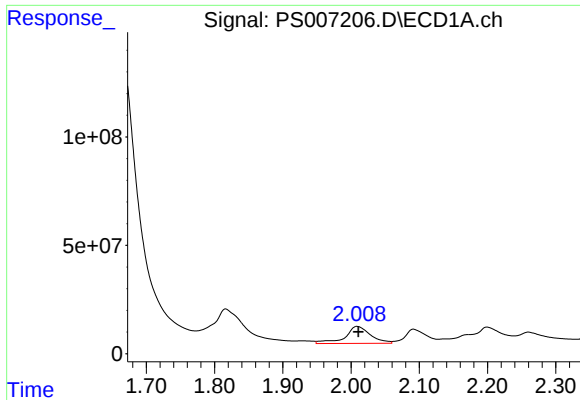

#1 Dalapon


R.T.: 2.009 min
Delta R.T.: -0.002 min
Response: 203851776
Conc: 121.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

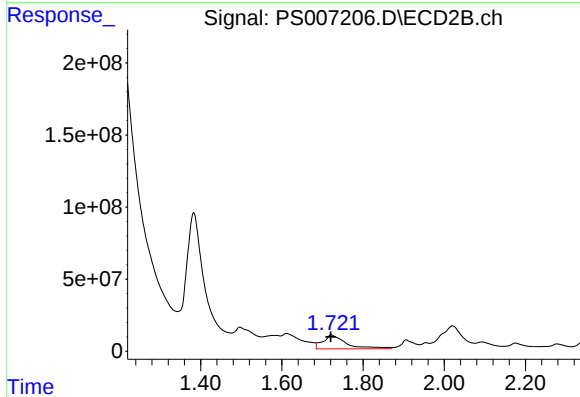


#1 Dalapon

R.T.: 1.722 min
Delta R.T.: 0.001 min
Response: 382580530
Conc: 420.42 ng/ml

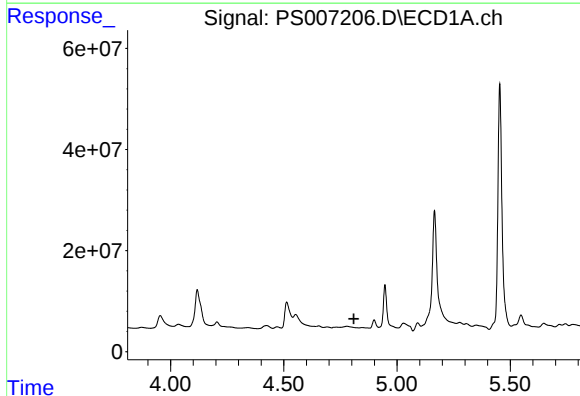


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

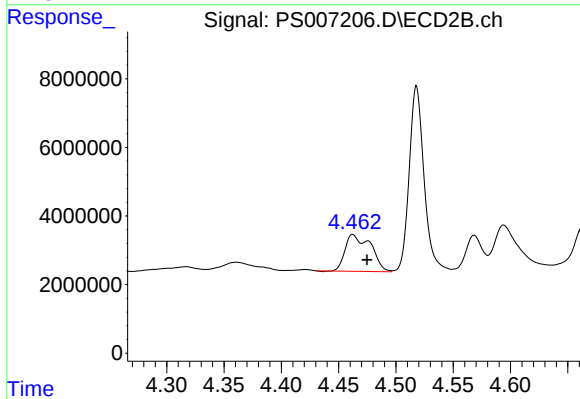

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.463 min
Delta R.T.: -0.012 min
Response: 16688294
Conc: 19.40 ng/ml

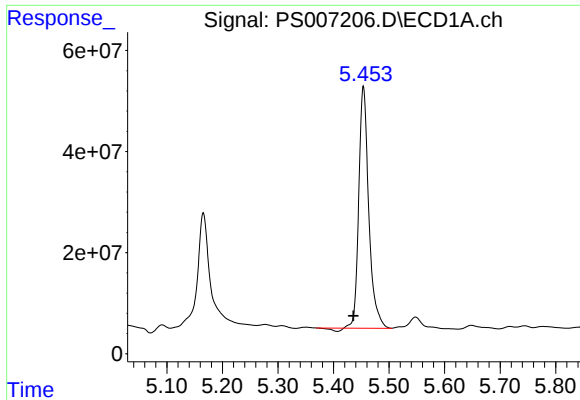

#4 2,4-DCAA


R.T.: 5.454 min
Delta R.T.: 0.018 min
Response: 594077020
Conc: 434.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

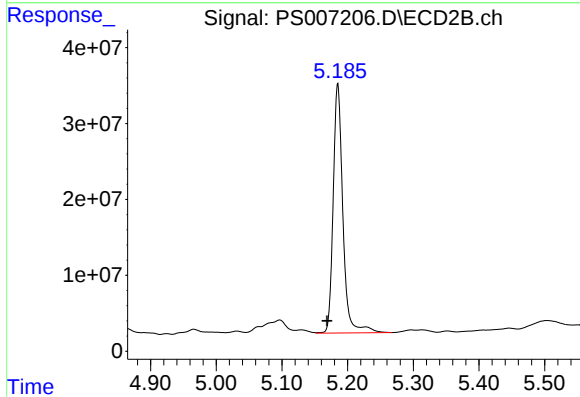


#4 2,4-DCAA

R.T.: 5.185 min
Delta R.T.: 0.017 min
Response: 336955576
Conc: 479.10 ng/ml

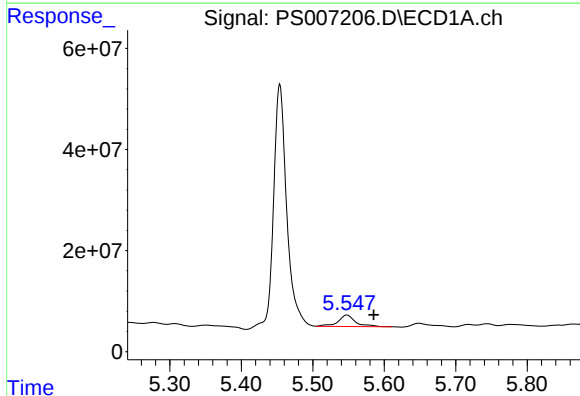


#5 DICAMBA

R.T.: 5.548 min
Delta R.T.: -0.038 min
Response: 38592732
Conc: 7.85 ng/ml

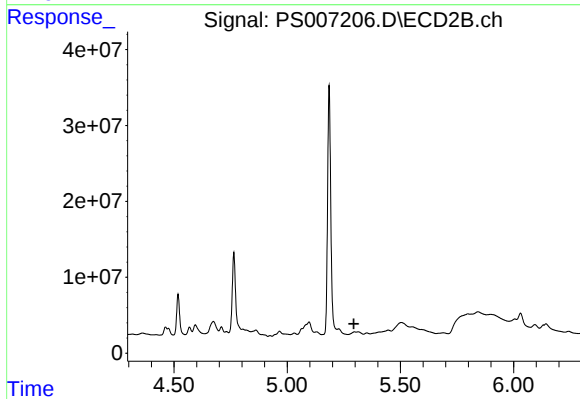

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

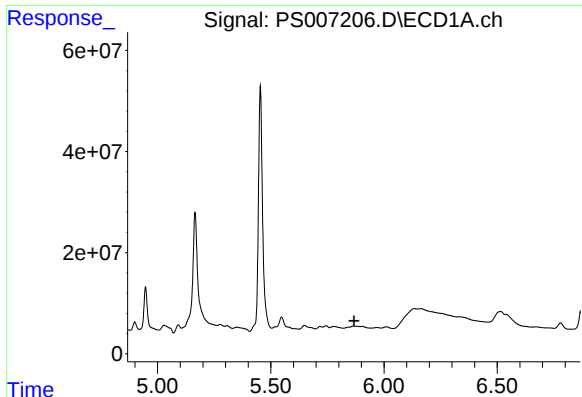

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

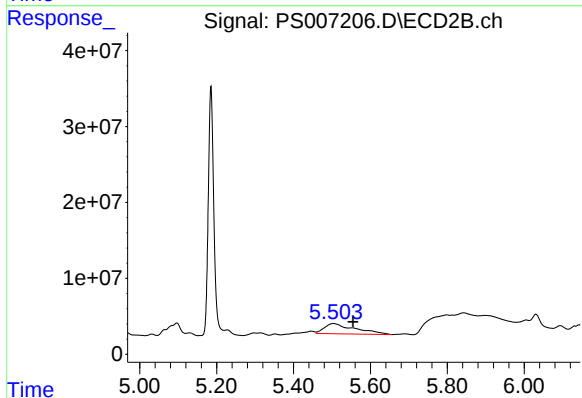


#7 MCPA

R.T.: 5.504 min
Delta R.T.: -0.051 min
Response: 75194472
Conc: 25.87 ug/ml

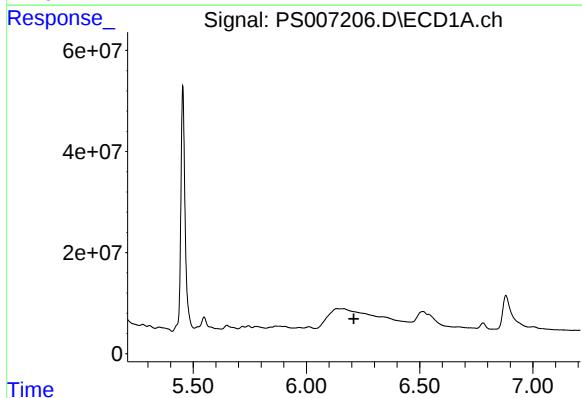


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.209 min
Response: 0
Conc: N.D.

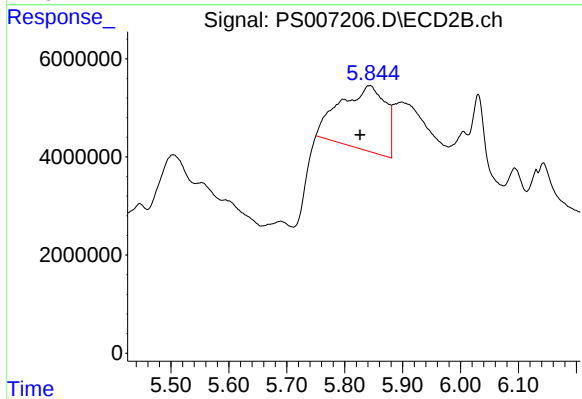

#8 DICHLORPROP


R.T.: 5.843 min
Delta R.T.: 0.017 min
Response: 71077779
Conc: 109.15 ng/ml

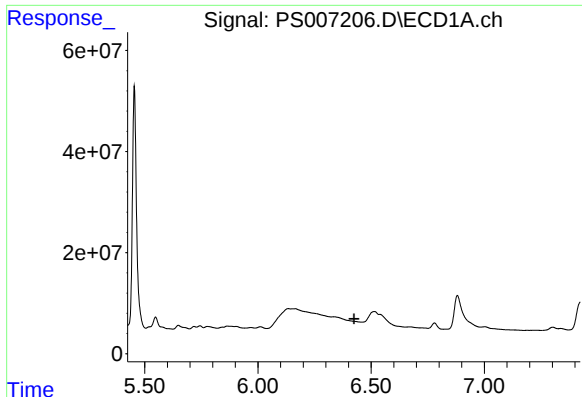

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

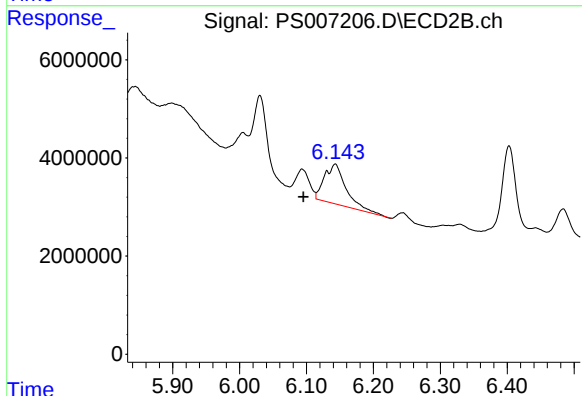


#9 2,4-D

R.T.: 6.143 min
Delta R.T.: 0.048 min
Response: 18214527
Conc: 22.83 ng/ml

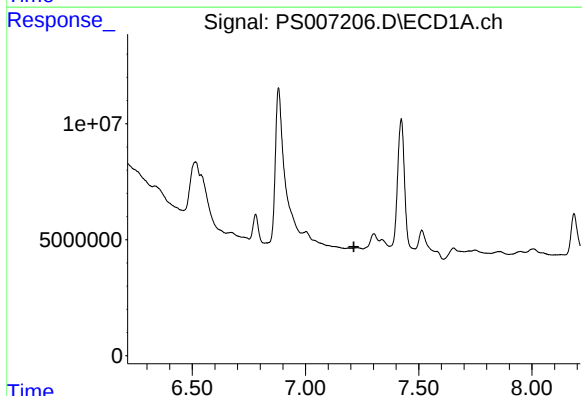


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

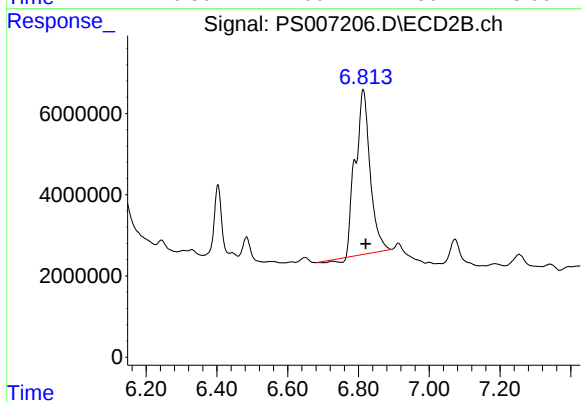

#11 2,4,5-TP (SILVEX)


R.T.: 6.814 min
Delta R.T.: -0.007 min
Response: 115966481
Conc: 30.49 ng/ml

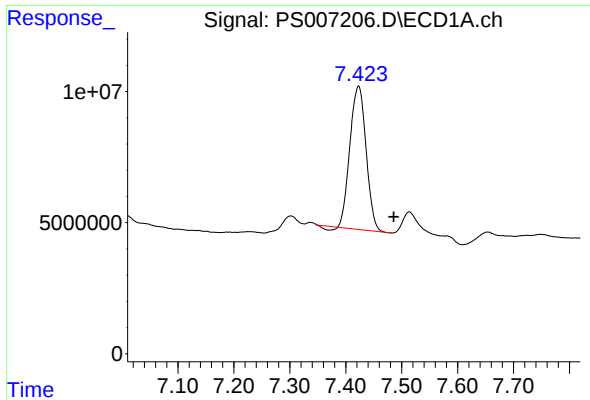

#12 2,4,5-T

R.T.: 7.423 min
Delta R.T.: -0.063 min
Response: 109046133
Conc: 14.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

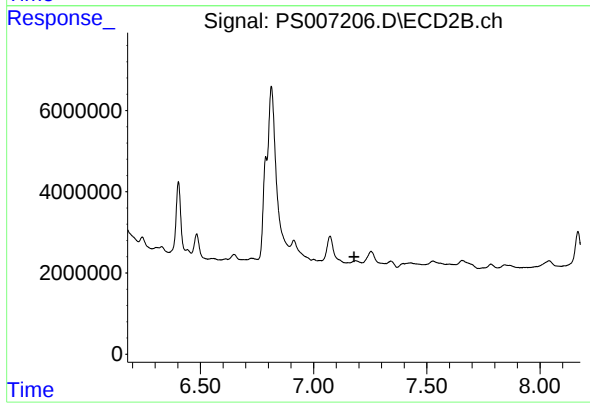

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.178 min
Response: 0
Conc: N.D.