

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101719\
 Data File : PS007214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2019 22:49
 Operator : SM\AJ
 Sample : K5393-20
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 00:56:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.456	5.188	673.1E6	361.5E6	491.761	514.063
Target Compounds							
1) T	Dalapon	2.012	1.725	242.1E6	377.7E6	144.694	415.045 #
2) T	3,5-DICHL...	0.000	4.479	0	15560617	N.D.	18.085
3) T	4-Nitroph...	0.000	4.865	0	21183887	N.D.	53.644
5) T	DICAMBA	5.551	5.324	40711001	10237570	8.286	3.934 #
6) T	MCPD	0.000	5.324	0	10237570	N.D.	5.397
7) T	MCPA	0.000	5.505	0	45955836	N.D.	15.808
9) T	2,4-D	0.000	6.095	0	24129410	N.D.	30.245
10) T	Pentachlo...	0.000	6.485	0	9814914	N.D.	1.021
11) T	2,4,5-TP ...	0.000	6.789	0	74064796	N.D.	19.472
12) T	2,4,5-T	7.428	0.000	169.2E6	0	22.127	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101719\
Data File : PS007214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 22:49
Operator : SM\AJ
Sample : K5393-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 00:56:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

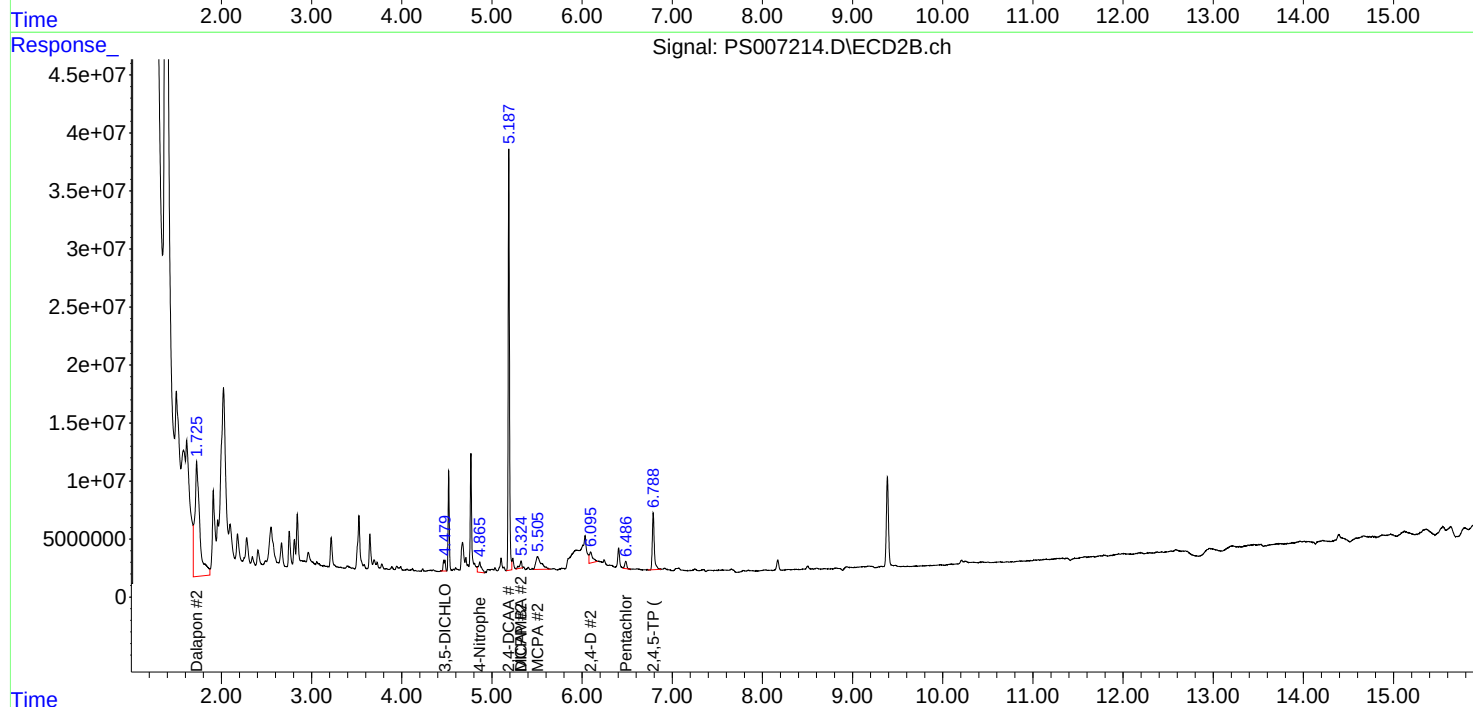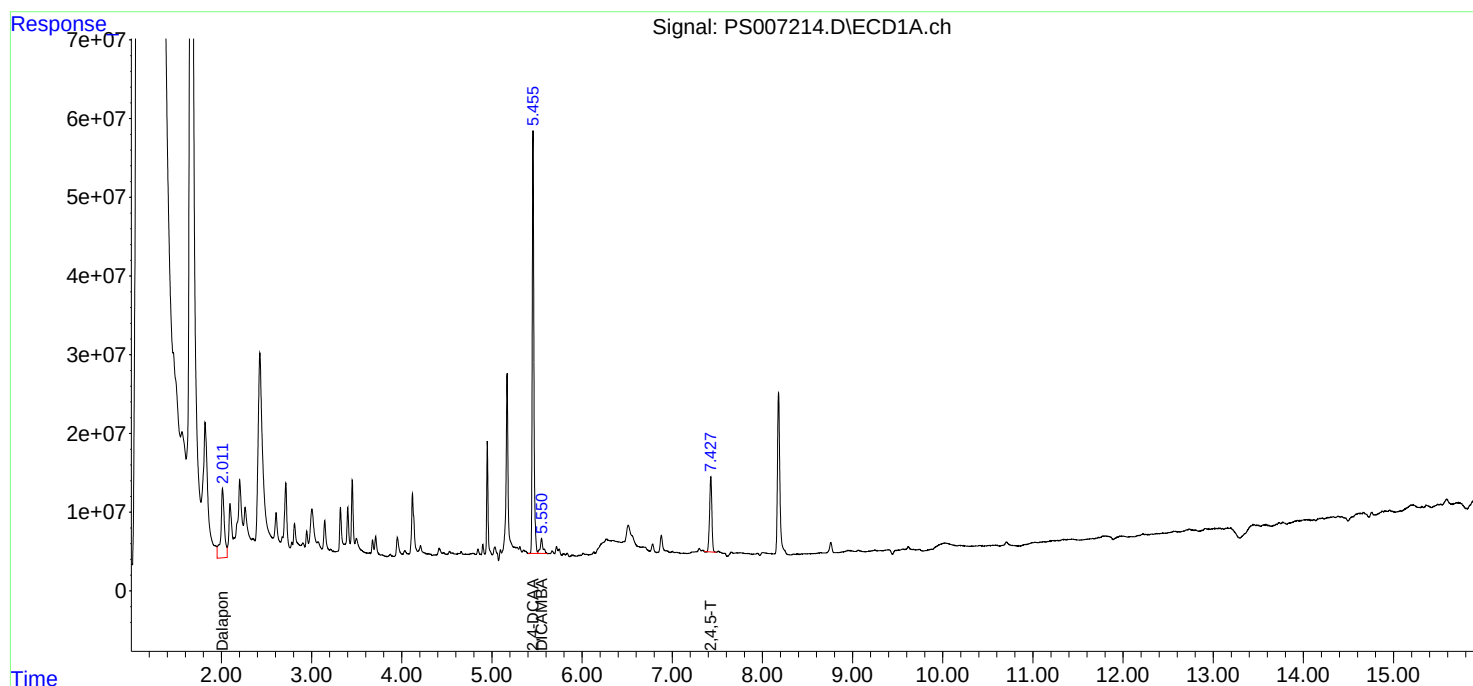


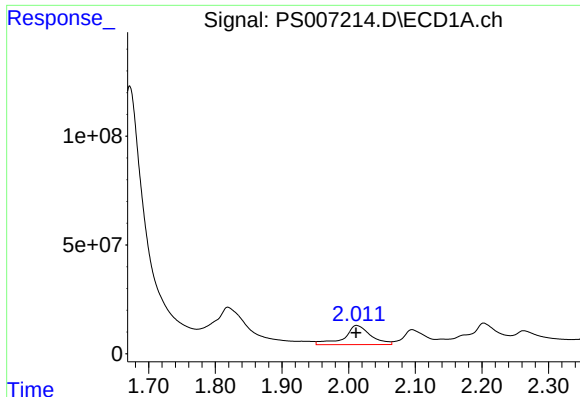

#1 Dalapon


R.T.: 2.012 min
Delta R.T.: 0.001 min
Response: 242114111
Conc: 144.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

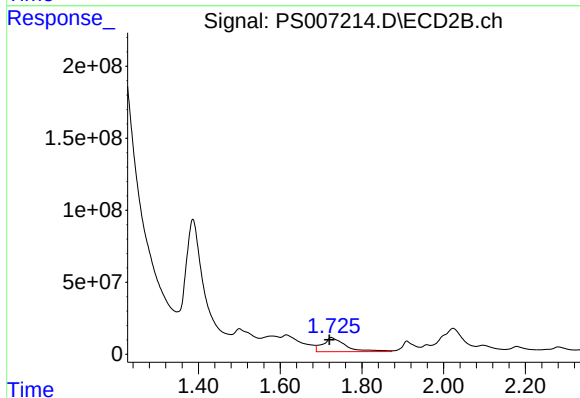


#1 Dalapon

R.T.: 1.725 min
Delta R.T.: 0.005 min
Response: 377692302
Conc: 415.04 ng/ml

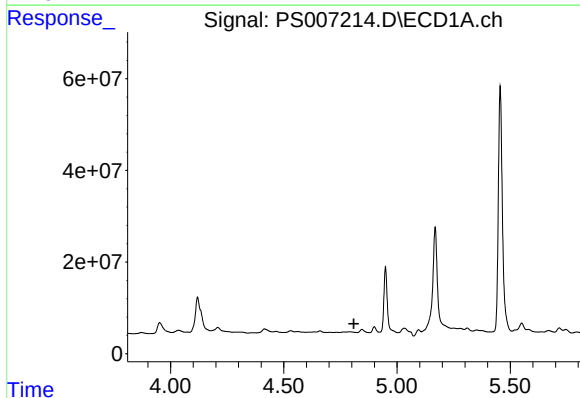


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

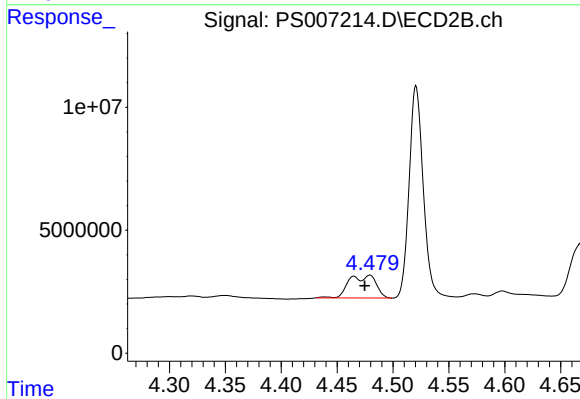

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.479 min
Delta R.T.: 0.004 min
Response: 15560617
Conc: 18.08 ng/ml

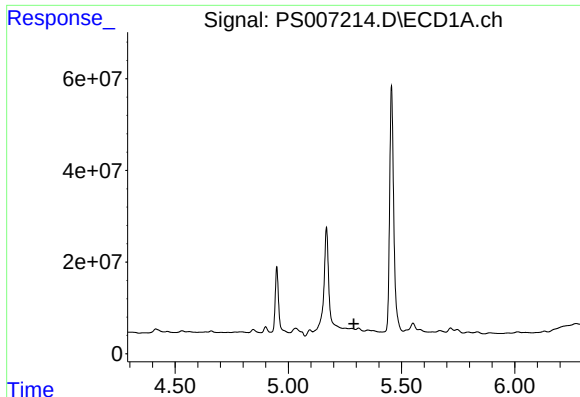

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.290 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

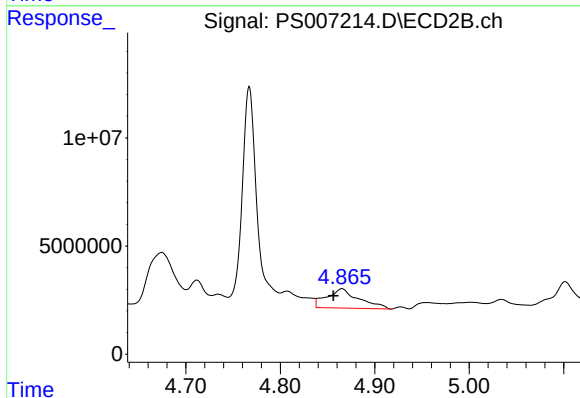


#3 4-Nitrophenol

R.T.: 4.865 min
Delta R.T.: 0.009 min
Response: 21183887
Conc: 53.64 ng/ml

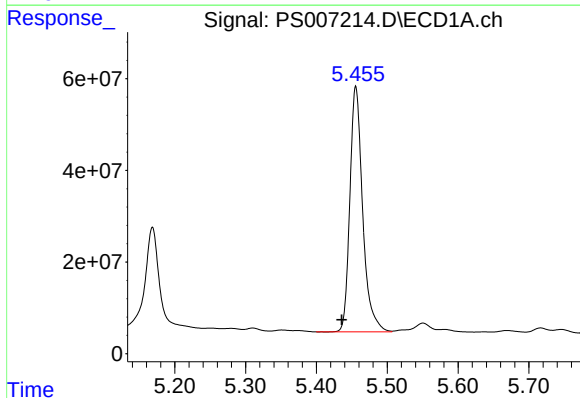


#4 2,4-DCAA

R.T.: 5.456 min
Delta R.T.: 0.020 min
Response: 673058002
Conc: 491.76 ng/ml

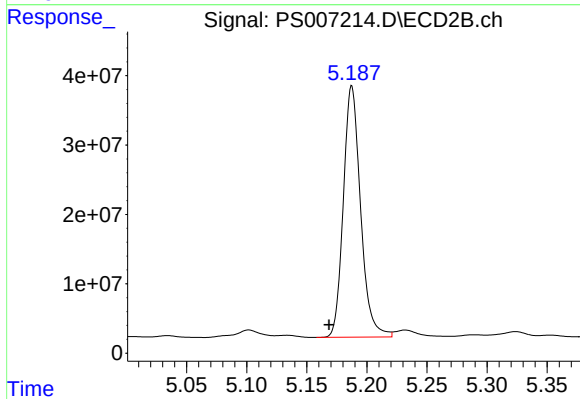

#4 2,4-DCAA


R.T.: 5.188 min
Delta R.T.: 0.019 min
Response: 361544198
Conc: 514.06 ng/ml

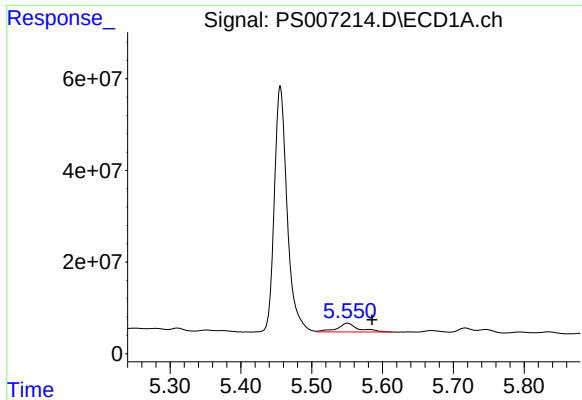

#5 DICAMBA


R.T.: 5.551 min
Delta R.T.: -0.035 min
Response: 40711001
Conc: 8.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

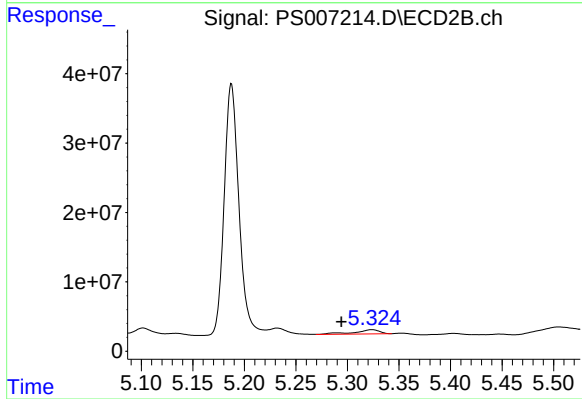


#5 DICAMBA

R.T.: 5.324 min
Delta R.T.: 0.029 min
Response: 10237570
Conc: 3.93 ng/ml

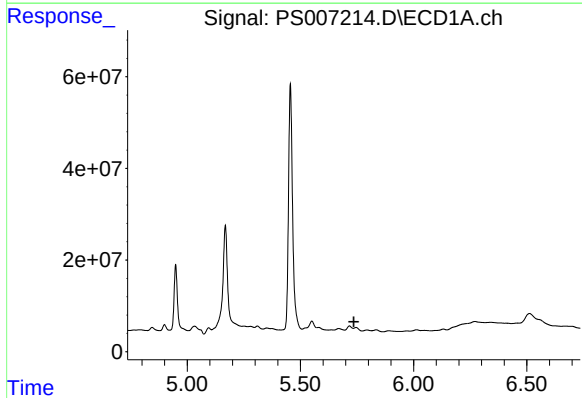


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.736 min
Response: 0
Conc: N.D.

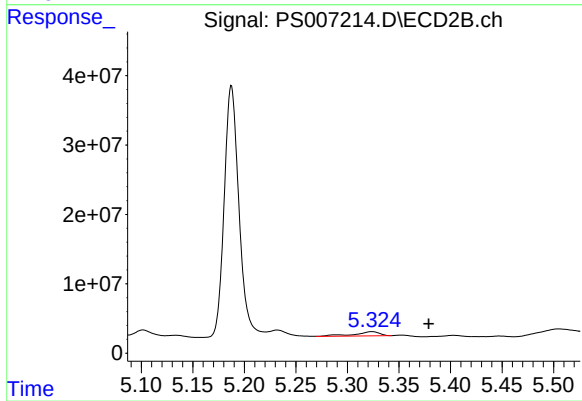

#6 MCP


R.T.: 5.324 min
Delta R.T.: -0.055 min
Response: 10237570
Conc: 5.40 ug/ml

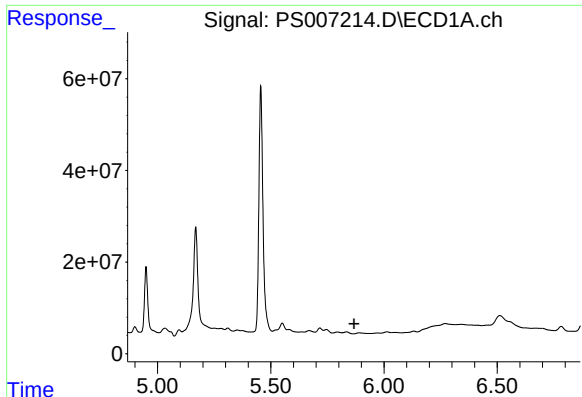

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

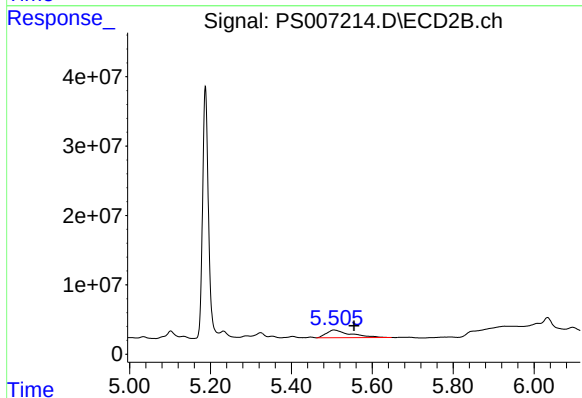


#7 MCPA

R.T.: 5.505 min
Delta R.T.: -0.049 min
Response: 45955836
Conc: 15.81 ug/ml

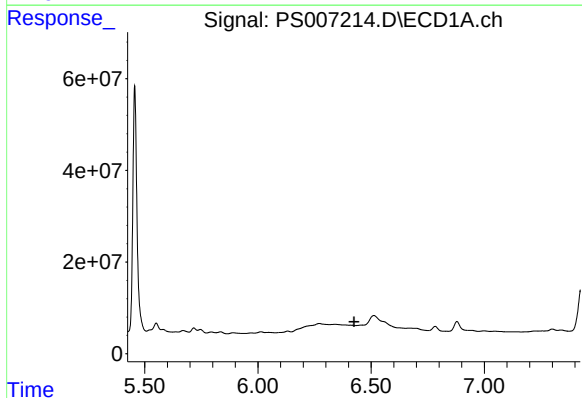


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

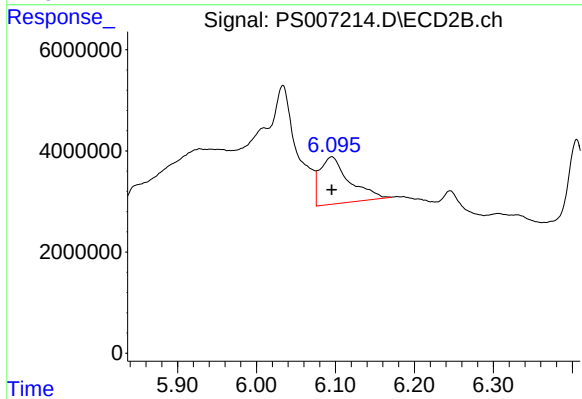

#9 2,4-D


R.T.: 6.095 min
Delta R.T.: 0.000 min
Response: 24129410
Conc: 30.25 ng/ml

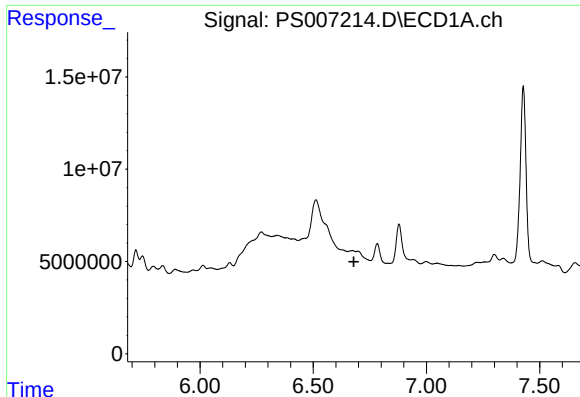

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.680 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

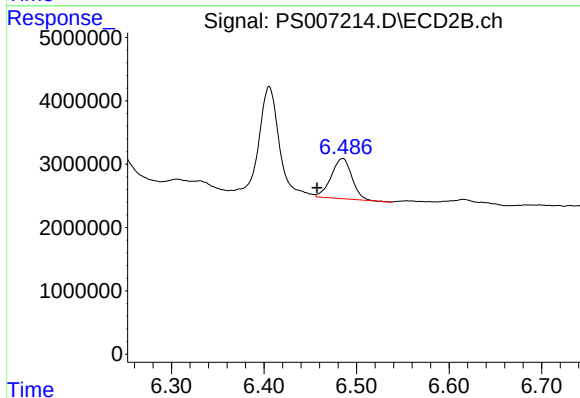


#10 Pentachlorophenol

R.T.: 6.485 min
Delta R.T.: 0.027 min
Response: 9814914
Conc: 1.02 ng/ml

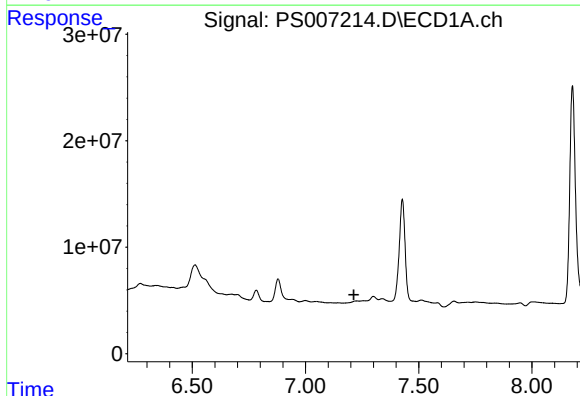


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

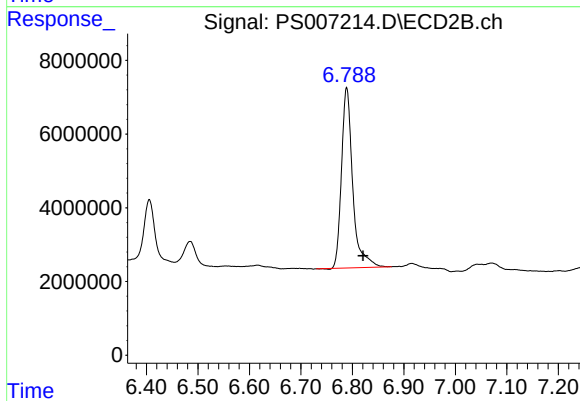

#11 2,4,5-TP (SILVEX)


R.T.: 6.789 min
Delta R.T.: -0.032 min
Response: 74064796
Conc: 19.47 ng/ml

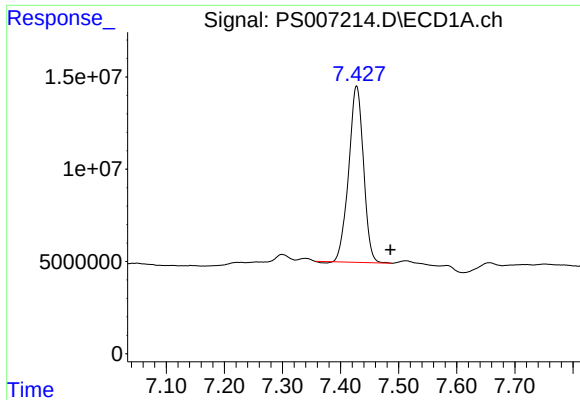

#12 2,4,5-T

R.T.: 7.428 min
Delta R.T.: -0.058 min
Response: 169157165
Conc: 22.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

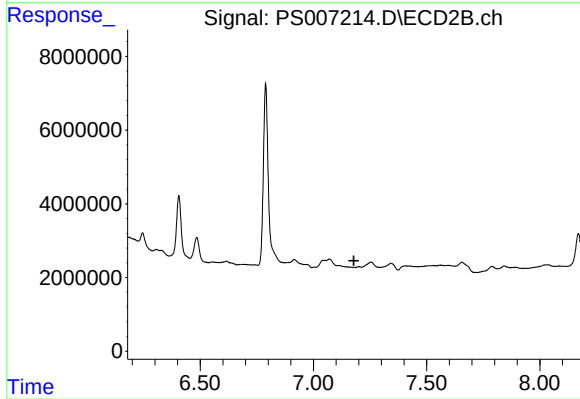

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.178 min
Response: 0
Conc: N.D.