

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101719\
 Data File : PS007215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2019 23:10
 Operator : SM\AJ
 Sample : K5393-22
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 00:57:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 14 13:54:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.466	5.199	539.1E6	301.4E6	393.885	428.540
Target Compounds							
1) T	Dalapon	2.023	1.736	142.5E6	338.2E6	85.173	371.612 #
2) T	3,5-DICHL...	0.000	4.489	0	14835215	N.D.	17.242
5) T	DICAMBA	5.560	5.330	38019094	5787275	7.738	2.224 #
6) T	MCPD	0.000	5.330	0	5787275	N.D.	3.051
7) T	MCPA	0.000	5.520	0	46532640	N.D.	16.006
9) T	2,4-D	0.000	6.107	0	23522325	N.D.	29.484
10) T	Pentachlo...	0.000	6.497	0	5817459	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.799	0	48674303	N.D.	12.797
12) T	2,4,5-T	7.437	0.000	121.5E6	0	15.893	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101719\
Data File : PS007215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2019 23:10
Operator : SM\AJ
Sample : K5393-22
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 00:57:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101419.M
Quant Title : 8080.M
QLast Update : Mon Oct 14 13:54:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

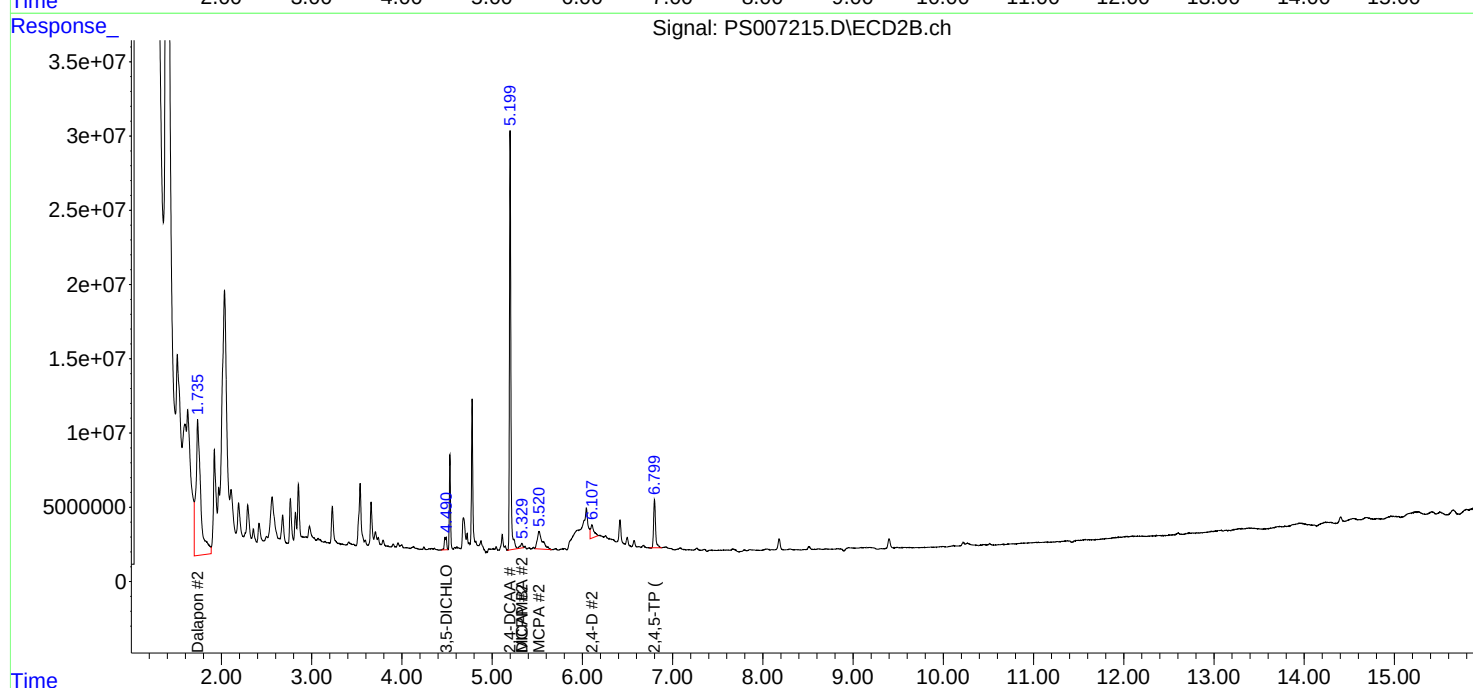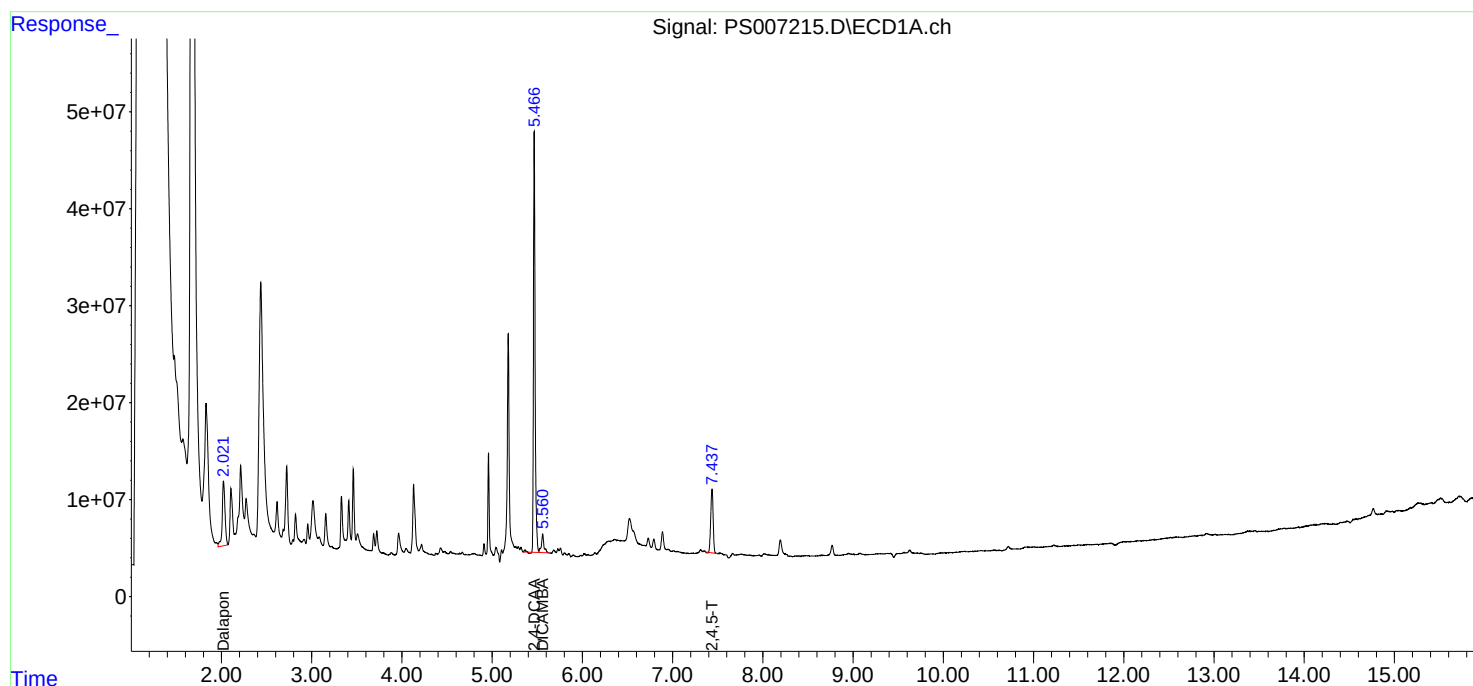


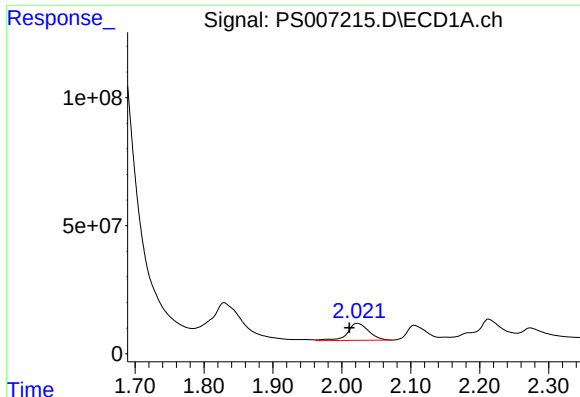

#1 Dalapon


R.T.: 2.023 min
Delta R.T.: 0.012 min
Response: 142518966
Conc: 85.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

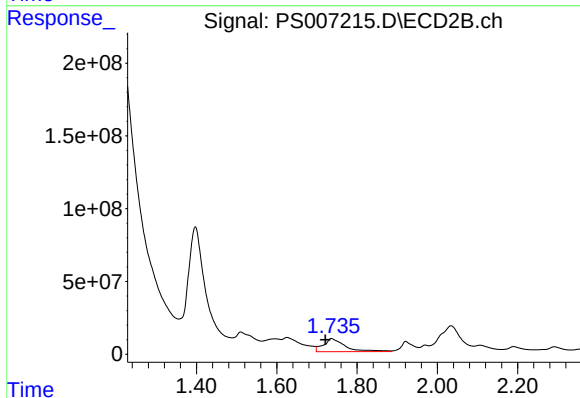


#1 Dalapon

R.T.: 1.736 min
Delta R.T.: 0.016 min
Response: 338168355
Conc: 371.61 ng/ml

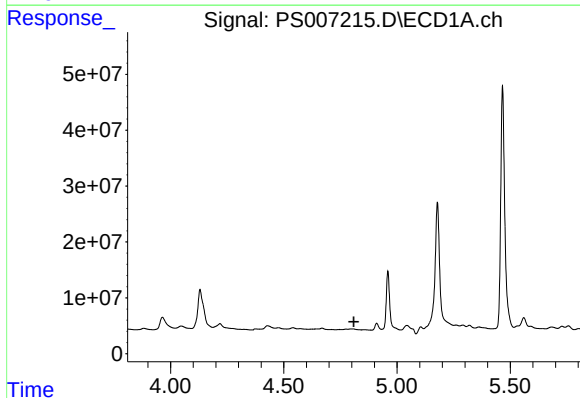


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.810 min
Response: 0
Conc: N.D.

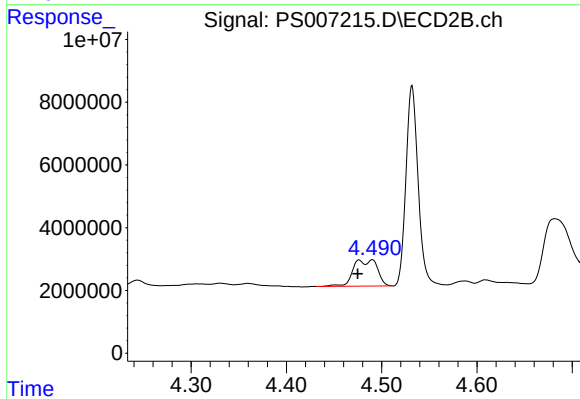

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.489 min
Delta R.T.: 0.015 min
Response: 14835215
Conc: 17.24 ng/ml

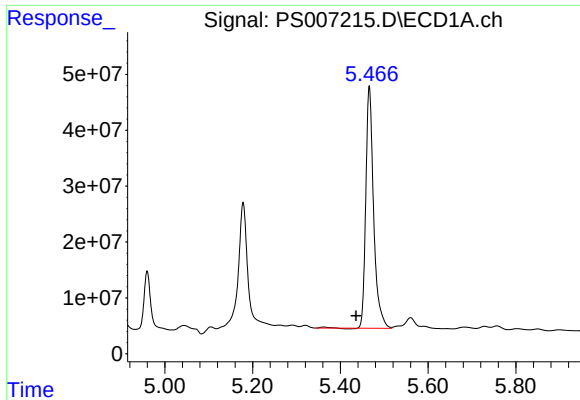

#4 2,4-DCAA


R.T.: 5.466 min
Delta R.T.: 0.030 min
Response: 539097408
Conc: 393.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

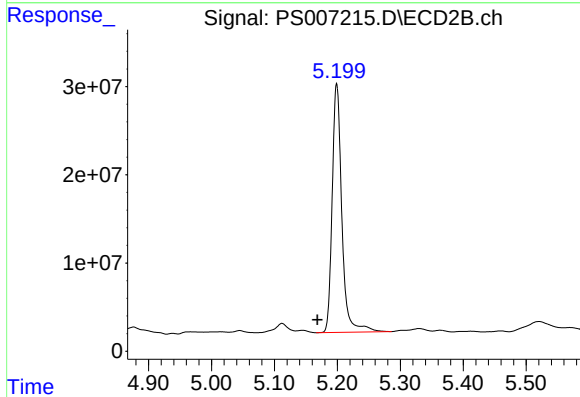


#4 2,4-DCAA

R.T.: 5.199 min
Delta R.T.: 0.031 min
Response: 301395296
Conc: 428.54 ng/ml

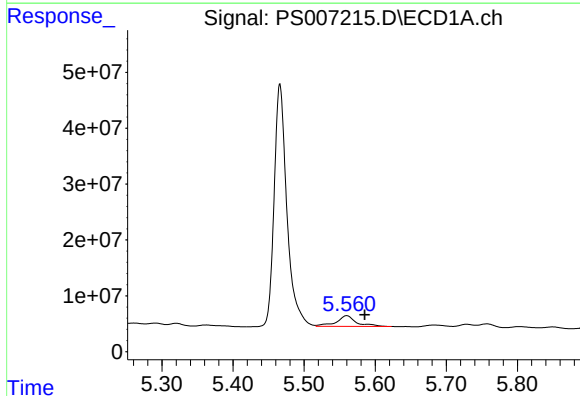


#5 DICAMBA

R.T.: 5.560 min
Delta R.T.: -0.025 min
Response: 38019094
Conc: 7.74 ng/ml

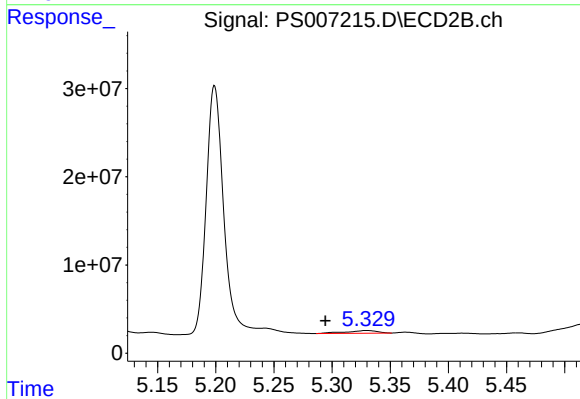

#5 DICAMBA


R.T.: 5.330 min
Delta R.T.: 0.035 min
Response: 5787275
Conc: 2.22 ng/ml

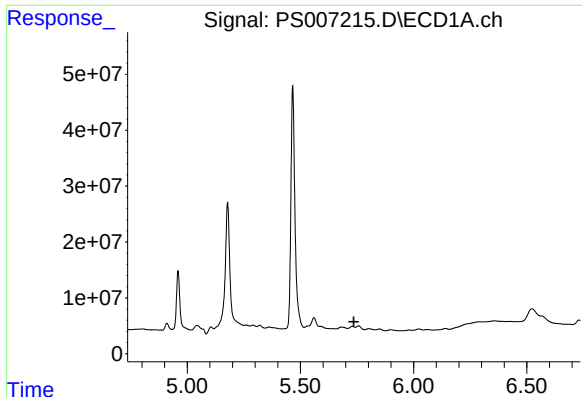

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.736 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

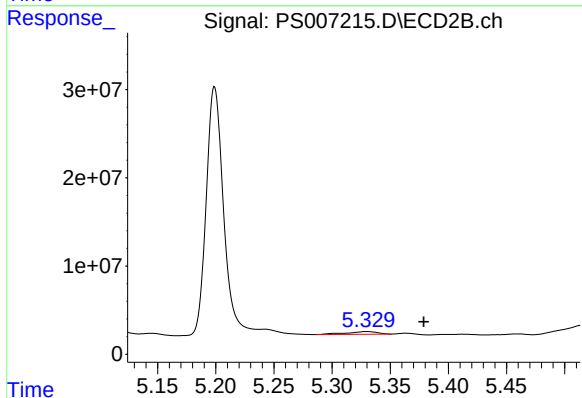


#6 MCPP

R.T.: 5.330 min
Delta R.T.: -0.049 min
Response: 5787275
Conc: 3.05 ug/ml

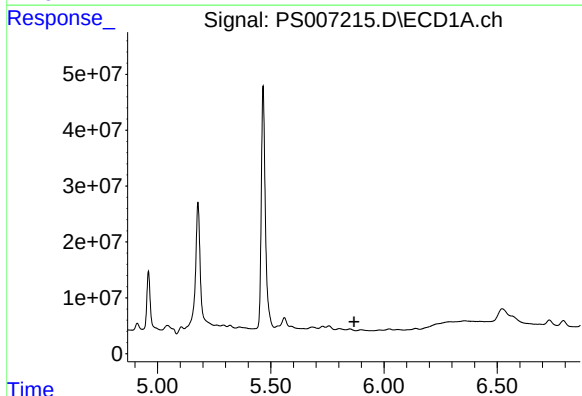


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 5.867 min
Response: 0
Conc: N.D.

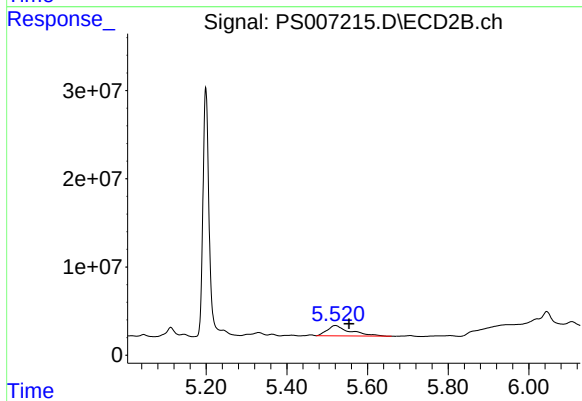

#7 MCPA


R.T.: 5.520 min
Delta R.T.: -0.035 min
Response: 46532640
Conc: 16.01 ug/ml

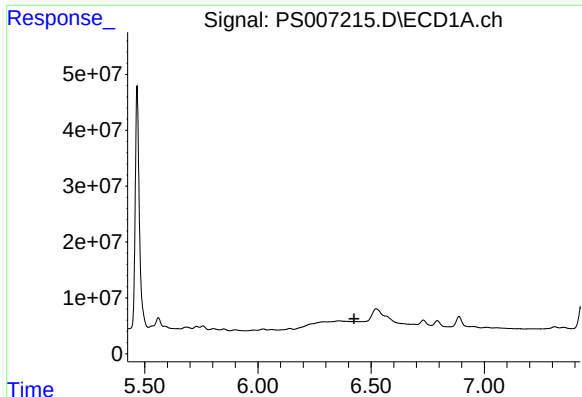

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.424 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

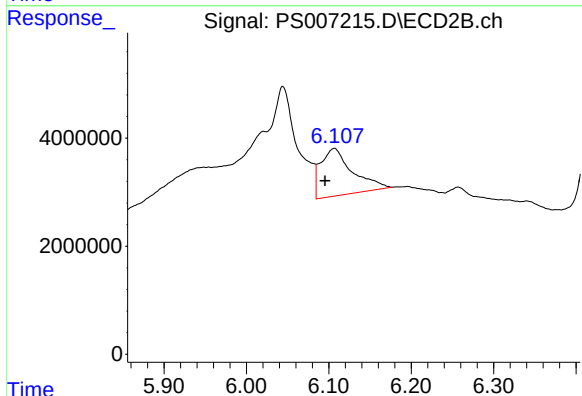


#9 2,4-D

R.T.: 6.107 min
Delta R.T.: 0.011 min
Response: 23522325
Conc: 29.48 ng/ml

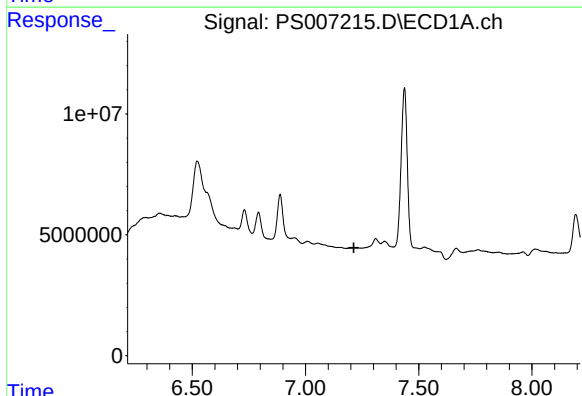


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.214 min
Response: 0
Conc: N.D.

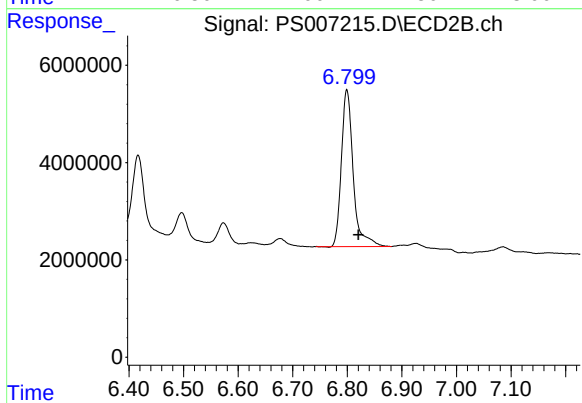

#11 2,4,5-TP (SILVEX)


R.T.: 6.799 min
Delta R.T.: -0.021 min
Response: 48674303
Conc: 12.80 ng/ml

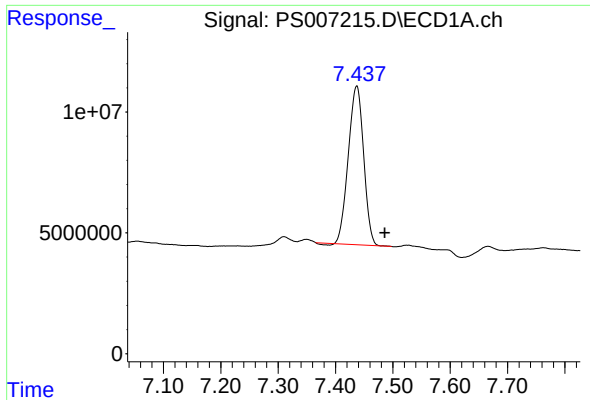

#12 2,4,5-T

R.T.: 7.437 min
Delta R.T.: -0.049 min
Response: 121494210
Conc: 15.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

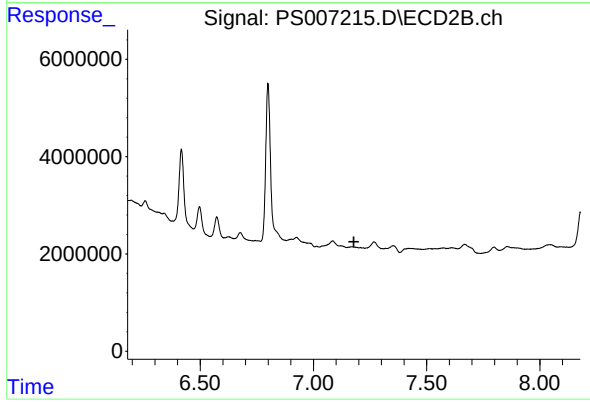

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.178 min
Response: 0
Conc: N.D.