

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101723\
 Data File : PS024633.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 08:21
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 01:26:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	0.000	2.574	0	2359274	N.D.	2.108
5) T	DICAMBA	0.000	6.983	0	1432986	N.D.	<MDL
6) T	MCPD	0.000	6.983f	0	1432986	N.D.	<MDL
7) T	MCPA	0.000	7.246	0	4626397	N.D.	1.444
12) T	2,4,5-T	0.000	9.037	0	3004298	N.D.	<MDL
15) T	Picloram	9.690	10.781	49931568	12543005	2.864	2.018 #
16) T	DCPA	0.000	10.781	0	12543005	N.D.	2.404



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101723\
Data File : PS024633.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 08:21
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 01:26:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

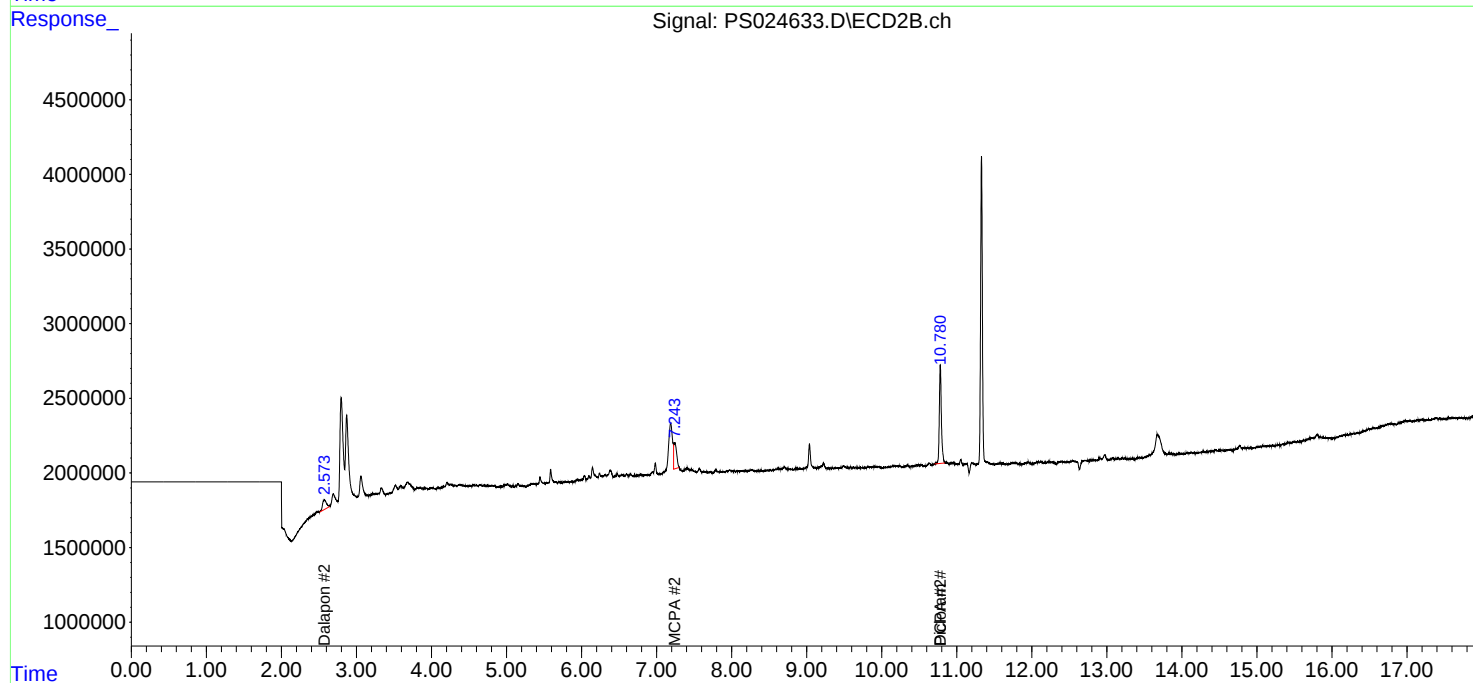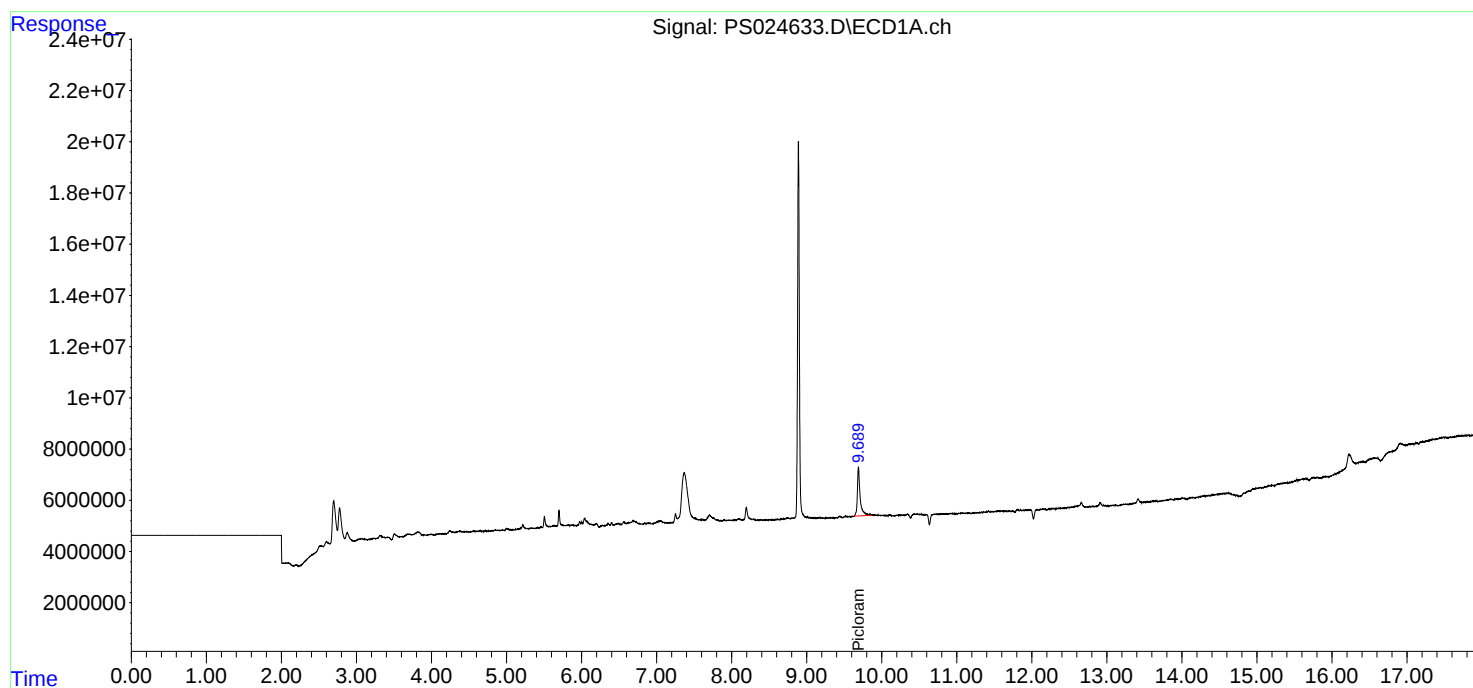


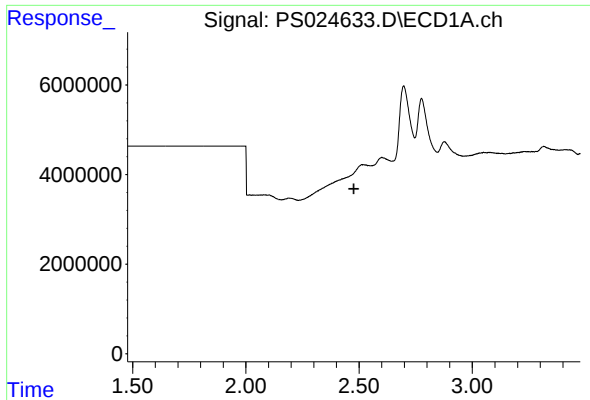

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

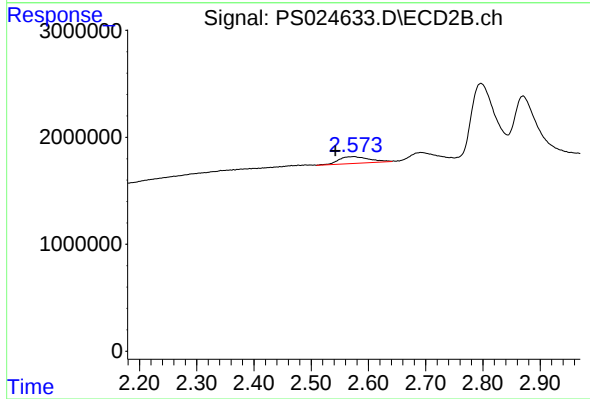


#1 Dalapon

R.T.: 2.574 min
Delta R.T.: 0.031 min
Response: 2359274
Conc: 2.11 ng/ml

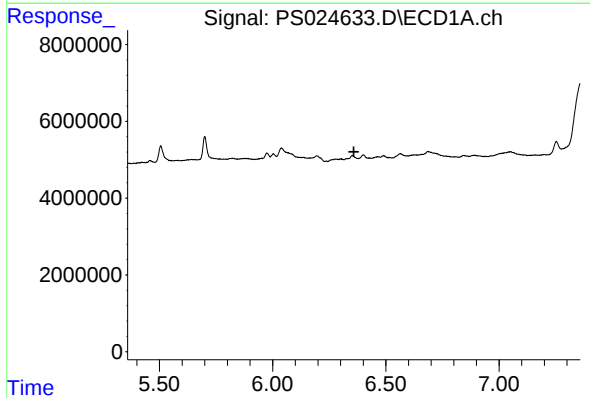


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.359 min
Response: 0
Conc: N.D.

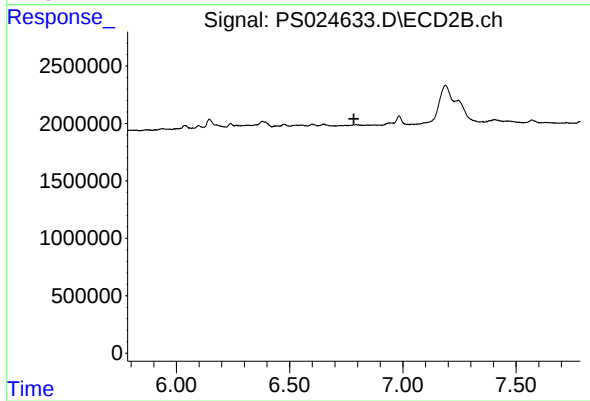

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.784 min
Response: 0
Conc: N.D.

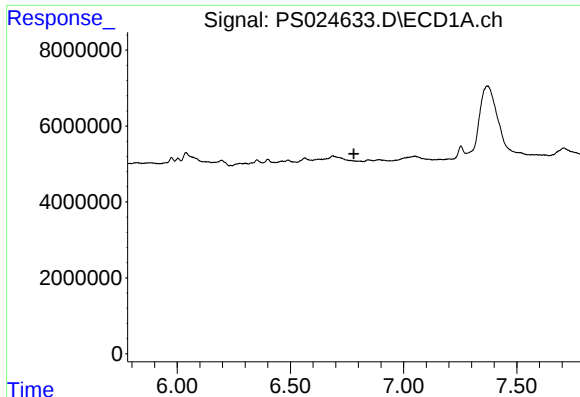

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

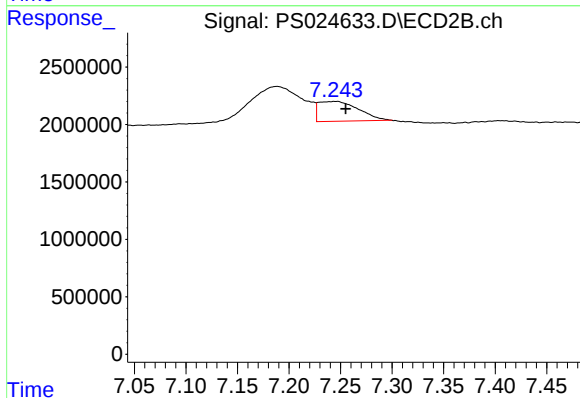


#7 MCPA

R.T.: 7.246 min
Delta R.T.: -0.009 min
Response: 4626397
Conc: 1.44 ug/ml

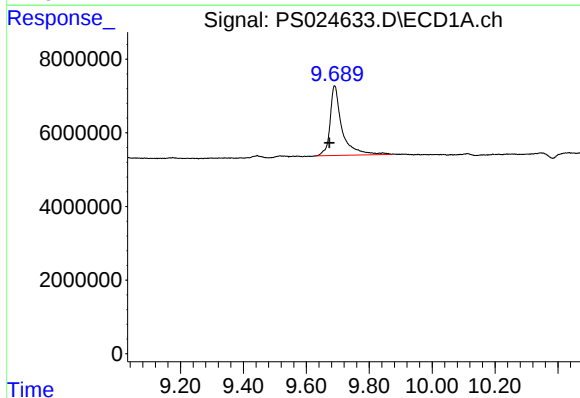


#15 Picloram

R.T.: 9.690 min
Delta R.T.: 0.017 min
Response: 49931568
Conc: 2.86 ng/ml

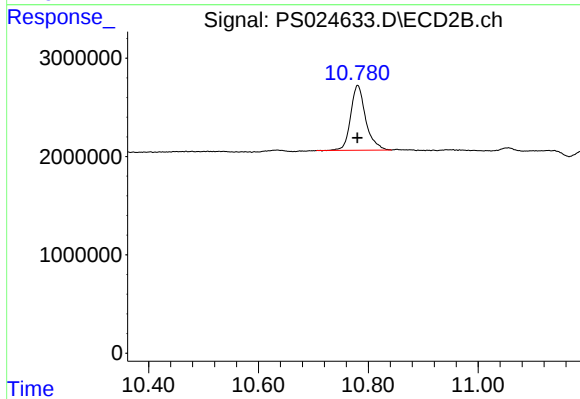

#15 Picloram


R.T.: 10.781 min
Delta R.T.: 0.000 min
Response: 12543005
Conc: 2.02 ng/ml

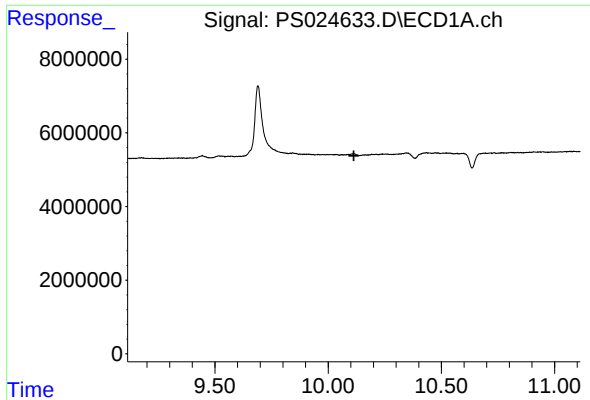

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

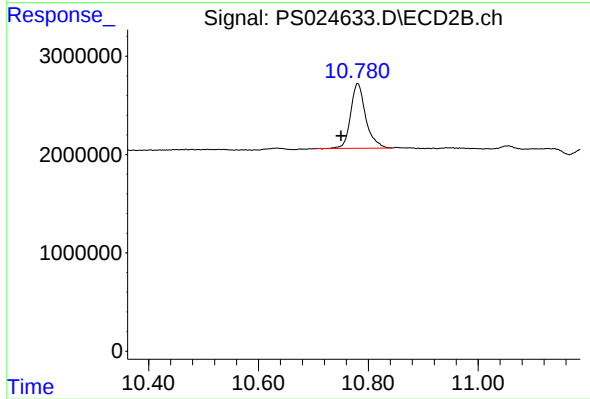

#16 DCPA

R.T.: 10.781 min
Delta R.T.: 0.031 min
Response: 12543005
Conc: 2.40 ng/ml