

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101723\
 Data File : PS024644.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2023 15:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 01:34:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.359	6.780	1047.1E6	344.5E6	508.939	498.367
Target Compounds							
1) T	Dalapon	2.515	2.574	7934517	4167192	3.212	3.724
5) T	DICAMBA	0.000	6.984	0	1592624	N.D.	<MDL
6) T	MCP	0.000	7.094f	0	248600	N.D.	<MDL
7) T	MCPA	0.000	7.236	0	7397881	N.D.	2.309
8) T	DICHLORPROP	0.000	7.572	0	2335654	N.D.	3.106
9) T	2,4-D	7.351f	7.787f	151.7E6	963128	54.894	1.046 #
11) T	2,4,5-TP ...	0.000	8.624	0	667352	N.D.	<MDL
12) T	2,4,5-T	0.000	9.036	0	1837903	N.D.	<MDL
13) T	2,4-DB	0.000	9.490	0	893766	N.D.	1.754
15) T	Picloram	9.690	10.781	27968821	8145020	1.604	1.311
16) T	DCPA	0.000	10.781	0	8145020	N.D.	1.561



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101723\
Data File : PS024644.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2023 15:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 01:34:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

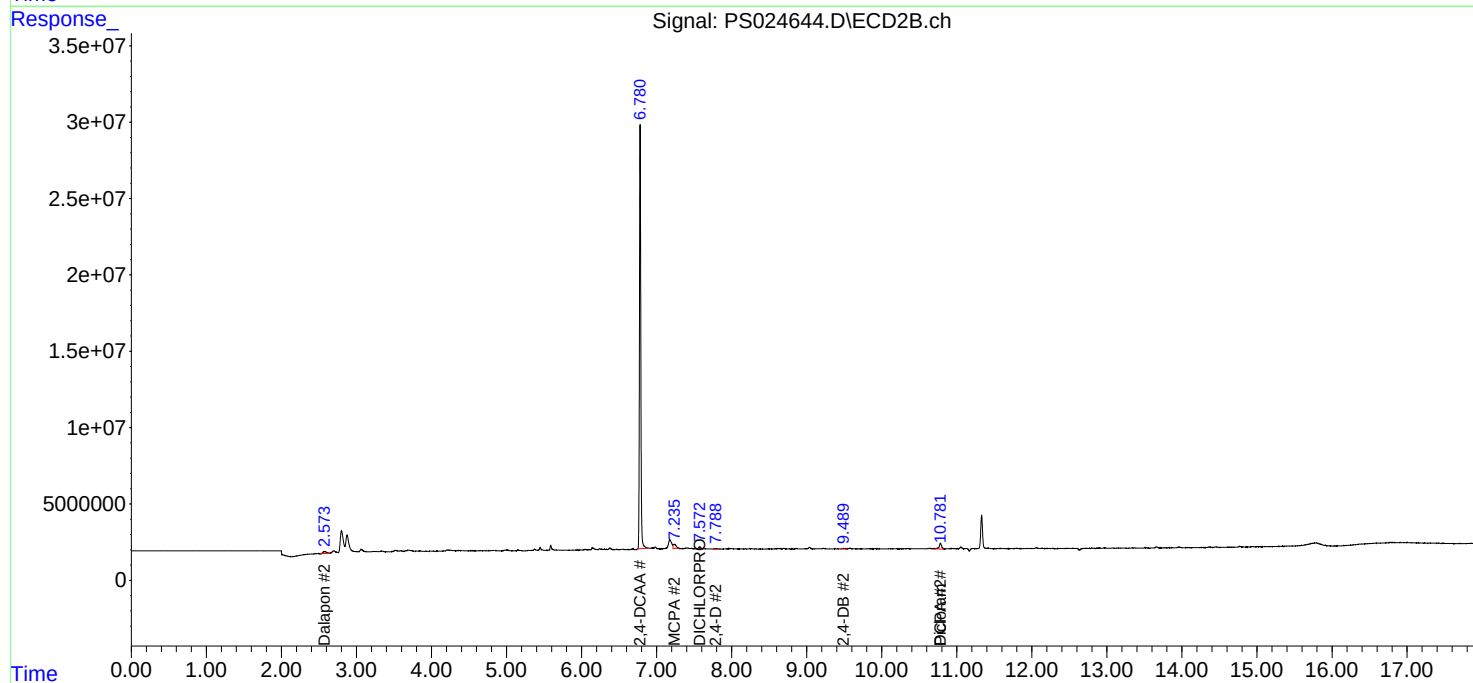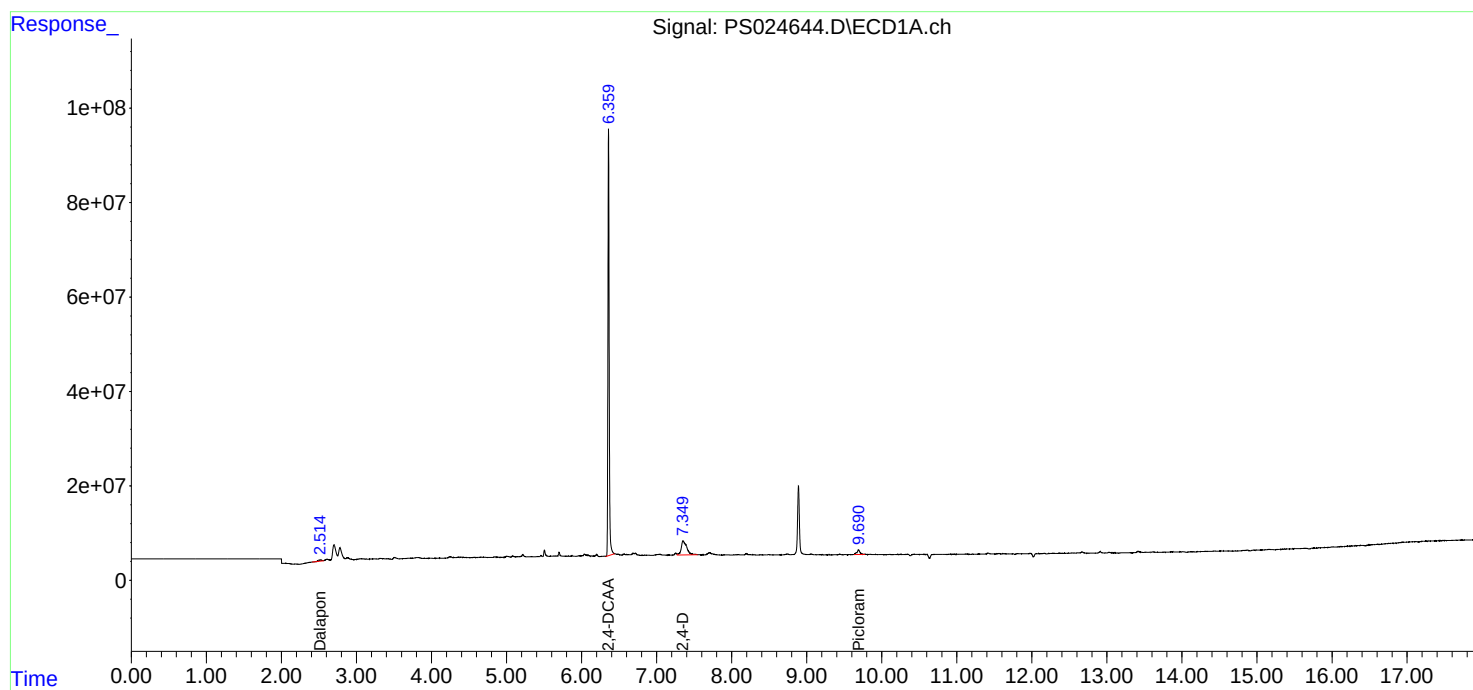


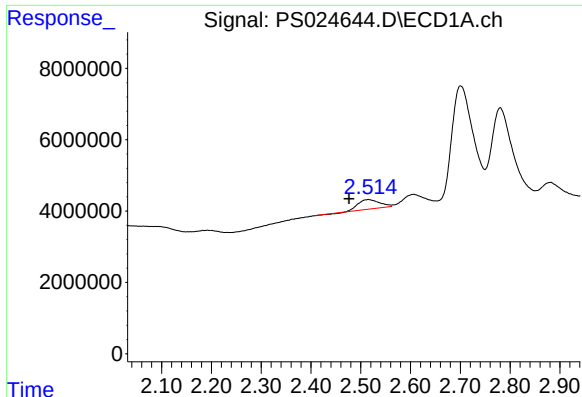

#1 Dalapon


R.T.: 2.515 min
Delta R.T.: 0.038 min
Response: 7934517
Conc: 3.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

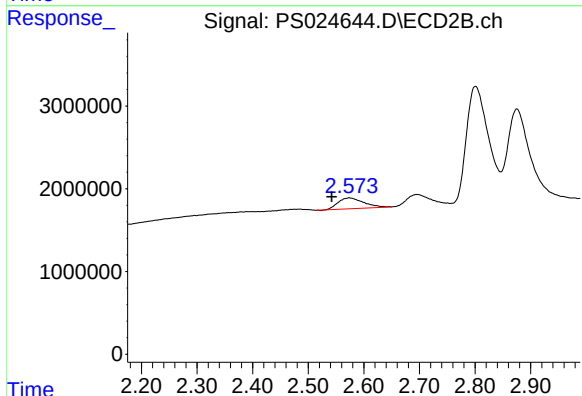


#1 Dalapon

R.T.: 2.574 min
Delta R.T.: 0.032 min
Response: 4167192
Conc: 3.72 ng/ml

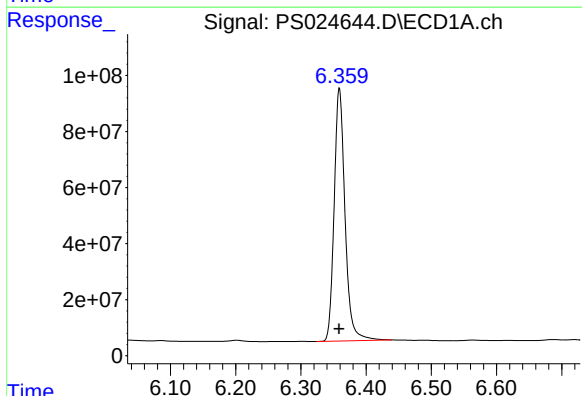


#4 2,4-DCAA

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 1047055309
Conc: 508.94 ng/ml

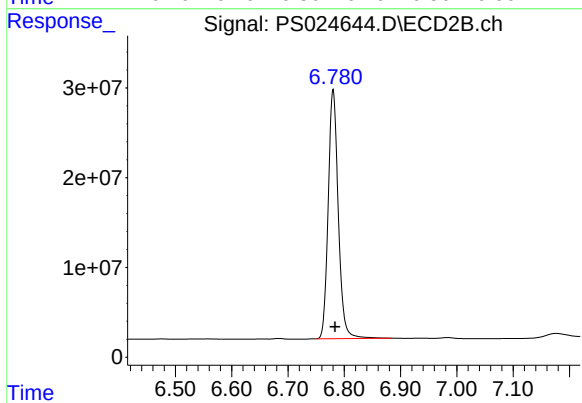

#4 2,4-DCAA


R.T.: 6.780 min
Delta R.T.: -0.003 min
Response: 344516344
Conc: 498.37 ng/ml

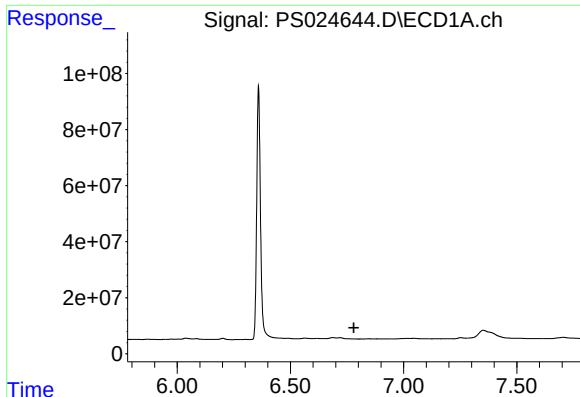

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

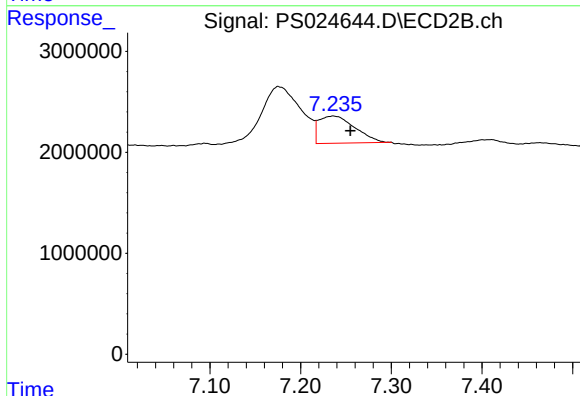


#7 MCPA

R.T.: 7.236 min
Delta R.T.: -0.019 min
Response: 7397881
Conc: 2.31 ug/ml

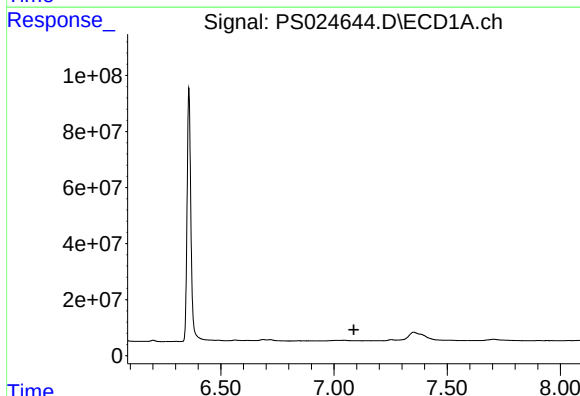


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

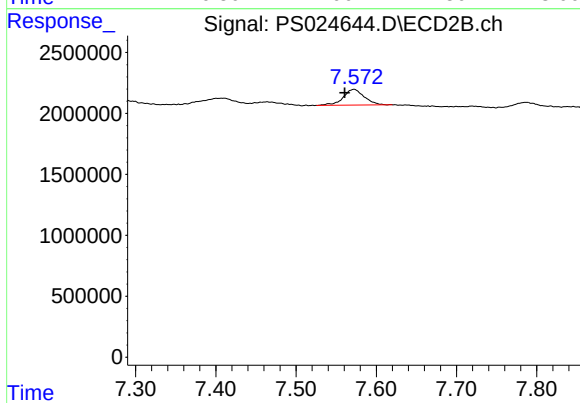

#8 DICHLORPROP


R.T.: 7.572 min
Delta R.T.: 0.011 min
Response: 2335654
Conc: 3.11 ng/ml

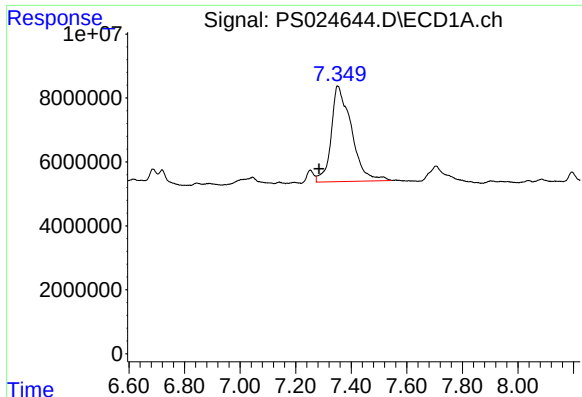

#9 2,4-D


R.T.: 7.351 min
Delta R.T.: 0.067 min
Response: 151671714
Conc: 54.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

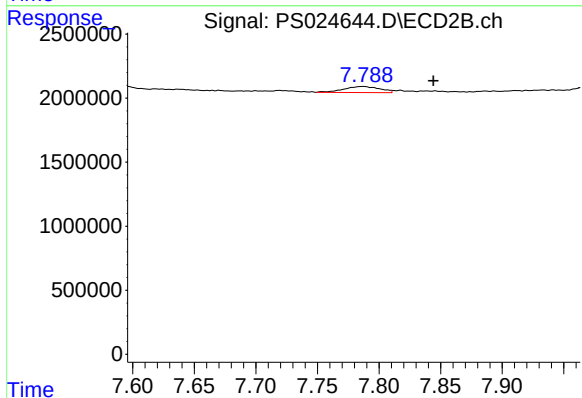


#9 2,4-D

R.T.: 7.787 min
Delta R.T.: -0.057 min
Response: 963128
Conc: 1.05 ng/ml

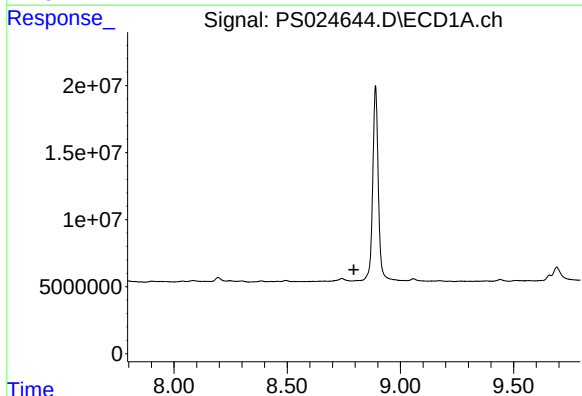


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.795 min
Response: 0
Conc: N.D.

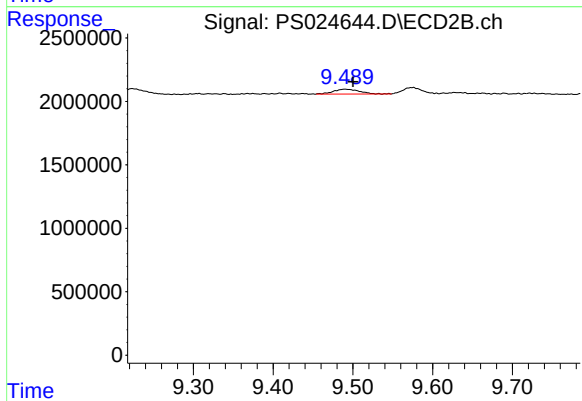

#13 2,4-DB


R.T.: 9.490 min
Delta R.T.: -0.010 min
Response: 893766
Conc: 1.75 ng/ml

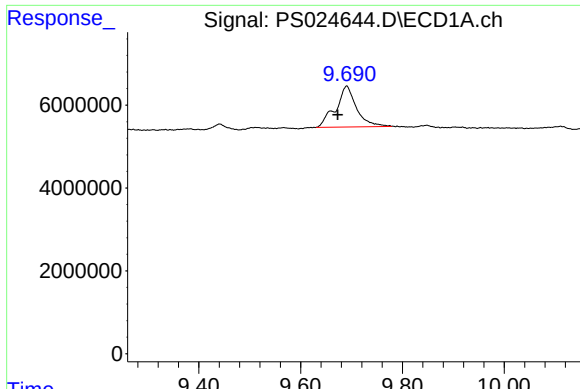

#15 Picloram


R.T.: 9.690 min
Delta R.T.: 0.017 min
Response: 27968821
Conc: 1.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

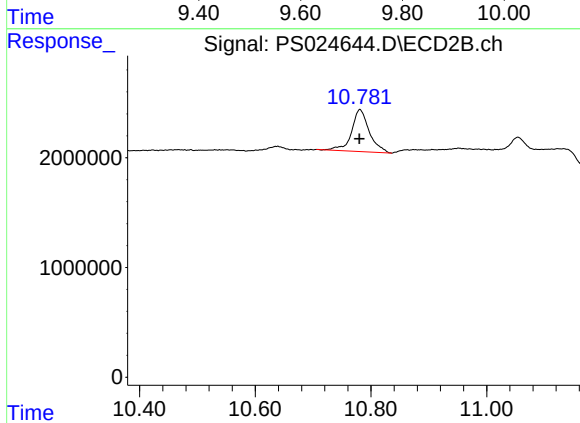


#15 Picloram

R.T.: 10.781 min
Delta R.T.: 0.000 min
Response: 8145020
Conc: 1.31 ng/ml

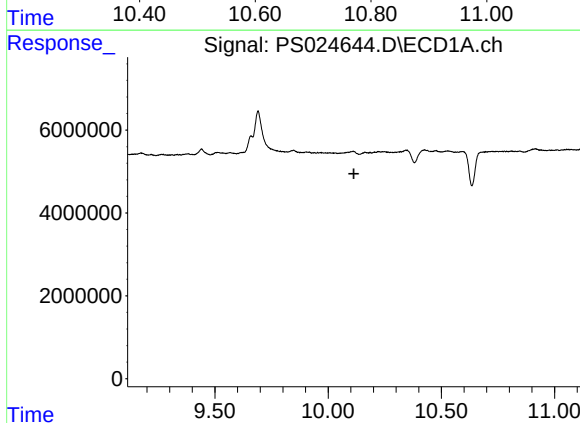

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.114 min
Response: 0
Conc: N.D.

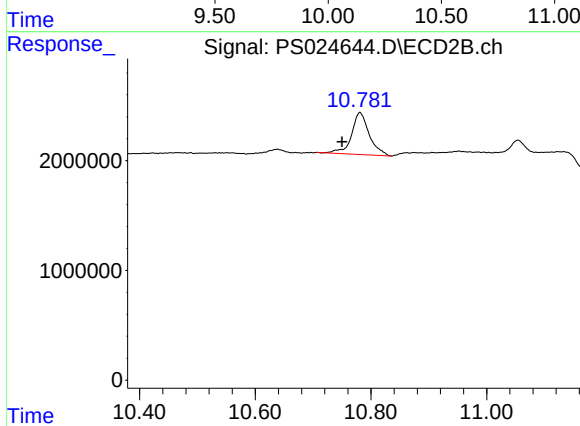

#16 DCPA

R.T.: 10.781 min
Delta R.T.: 0.031 min
Response: 8145020
Conc: 1.56 ng/ml