

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101725\
 Data File : PS032087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2025 21:27
 Operator : AR\AJ
 Sample : Q3352-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 01:45:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.285	7.755	90465821	32745667	18.977	29.760 #
Target Compounds							
1) T	Dalapon	2.637f	2.678	2031.0E6	2021.8E6	262.824	537.973 #
2) T	3,5-DICHL...	6.438	0.000	286284	0	<MDL	N.D. #
3) T	4-Nitroph...	7.079	0.000	3597470	0	2.695	N.D. #
5) T	DICAMBA	7.474	7.979f	3301364	36022170	<MDL	4.159 #
6) T	MCPD	7.671	0.000	14487227	0	1.185	N.D. #
7) T	MCPA	7.792	8.280	20085115	79549842	1.365	21.088 #
8) T	DICHLORPROP	8.132f	8.651	7243212	67811653	1.524	34.629 #
10) T	Pentachlo...	8.750f	9.511	5409114	138.6E6	<MDL	2.674 #
11) T	2,4,5-TP ...	9.243f	9.883	9519541	183.6E6	<MDL	9.147 #
12) T	2,4,5-T	9.563	0.000	114.5E6	0	4.536	N.D. #
13) T	2,4-DB	10.143	0.000	17503251	0	5.646	N.D. #
14) T	DINOSEB	11.363	11.292f	2985994	7213866	<MDL	<MDL #
15) T	Picloram	11.198f	0.000	37812918	0	1.604	N.D. #
16) T	DCPA	11.627	0.000	28289485	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101725\
Data File : PS032087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2025 21:27
Operator : AR\AJ
Sample : Q3352-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 01:45:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

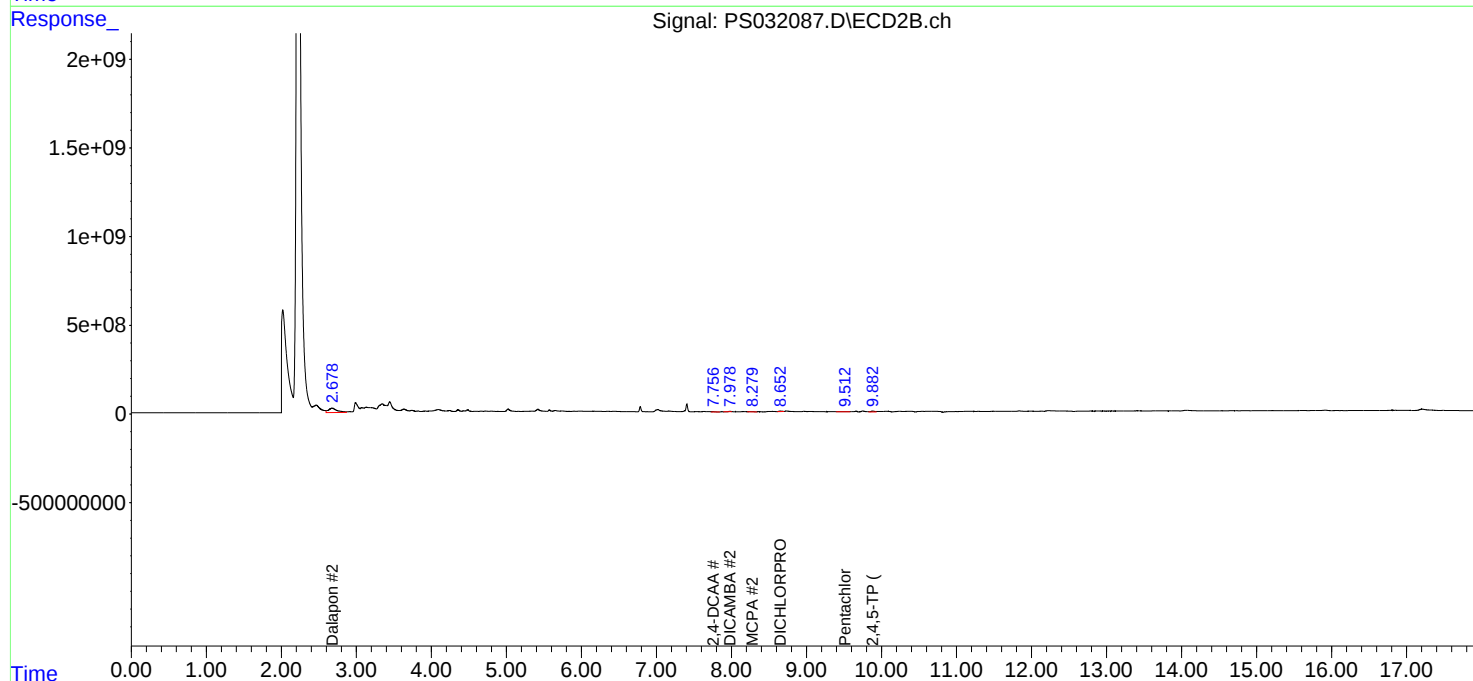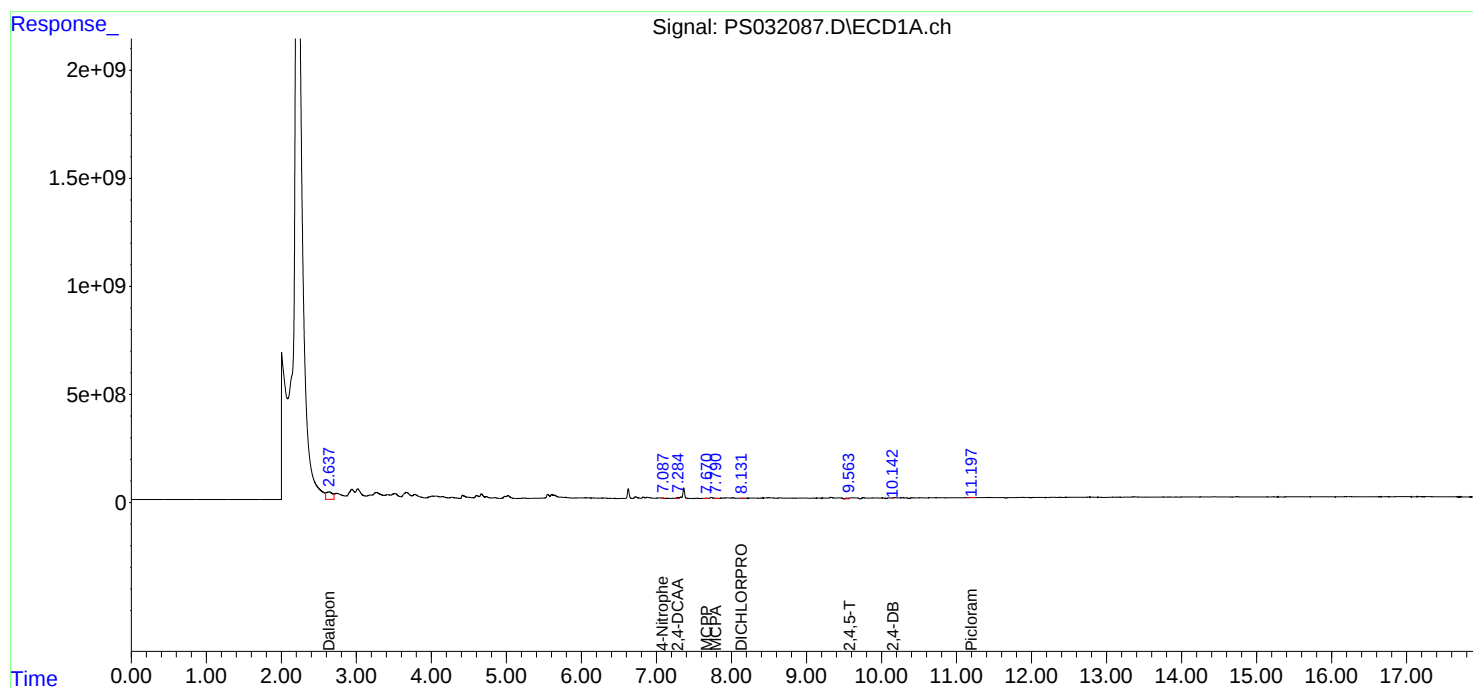


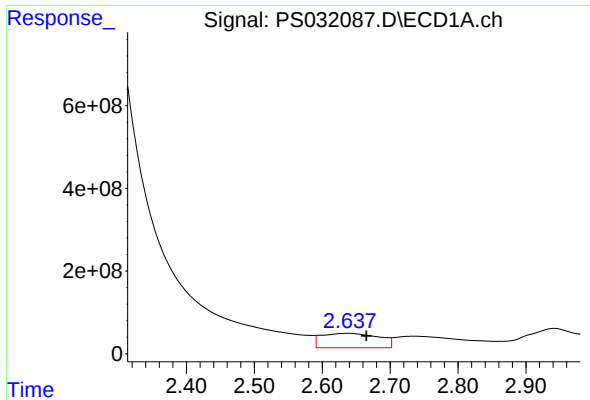

#1 Dalapon


R.T.: 2.637 min
Delta R.T.: -0.028 min
Response: 2030983127
Conc: 262.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

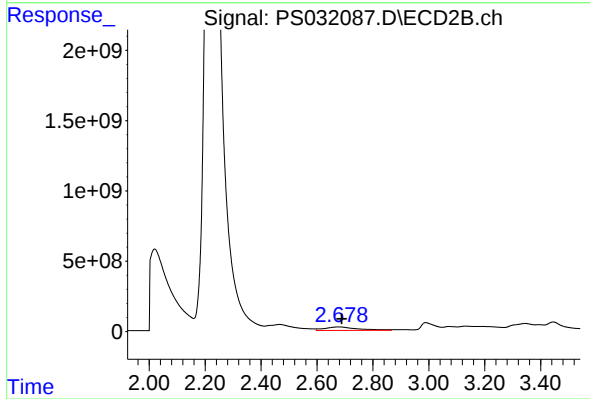


#1 Dalapon

R.T.: 2.678 min
Delta R.T.: -0.011 min
Response: 2021849150
Conc: 537.97 ng/ml

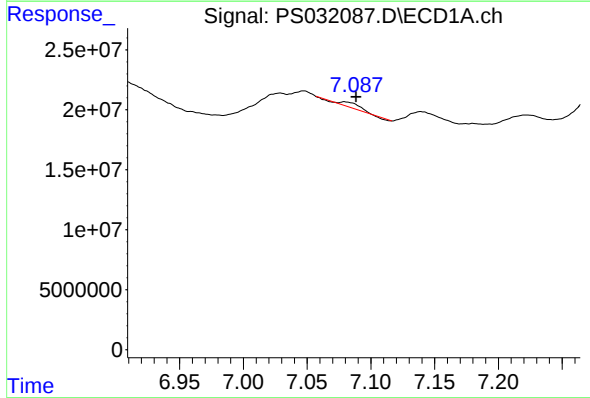


#3 4-Nitrophenol

R.T.: 7.079 min
Delta R.T.: -0.009 min
Response: 3597470
Conc: 2.70 ng/ml

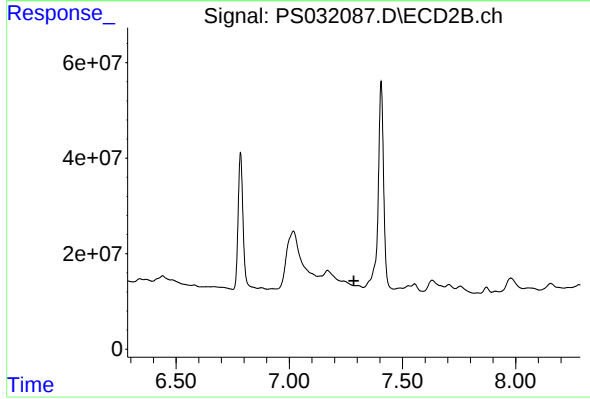

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.285 min
Response: 0
Conc: N.D.

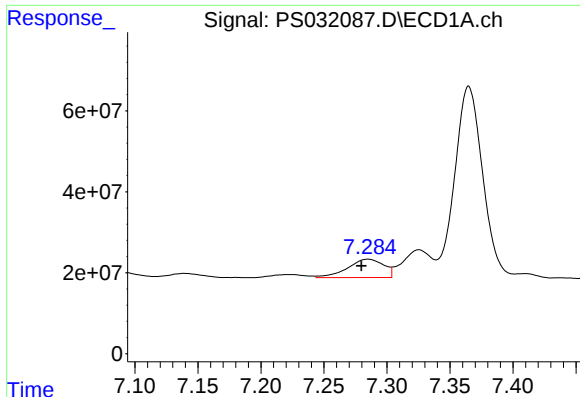

#4 2,4-DCAA


R.T.: 7.285 min
Delta R.T.: 0.005 min
Response: 90465821
Conc: 18.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

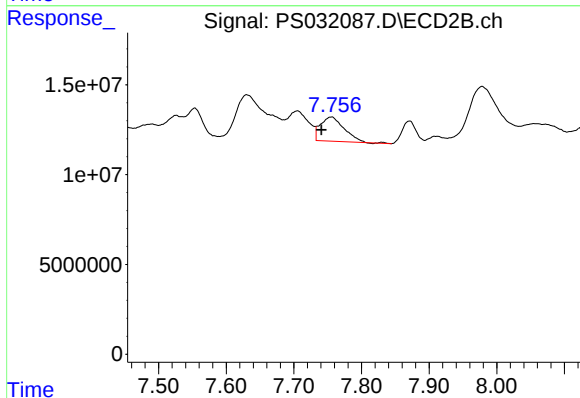


#4 2,4-DCAA

R.T.: 7.755 min
Delta R.T.: 0.014 min
Response: 32745667
Conc: 29.76 ng/ml

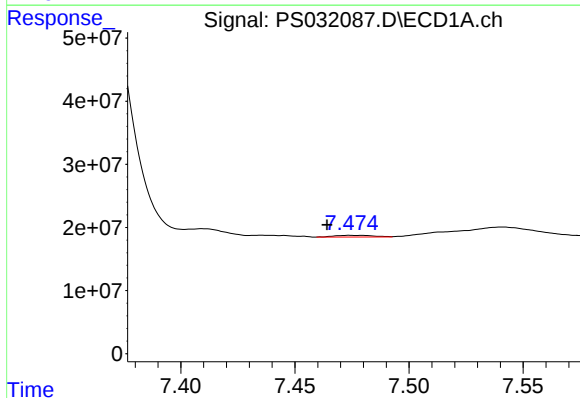


#5 DICAMBA

R.T.: 7.474 min
Delta R.T.: 0.010 min
Response: 3301364
Conc: N.D.

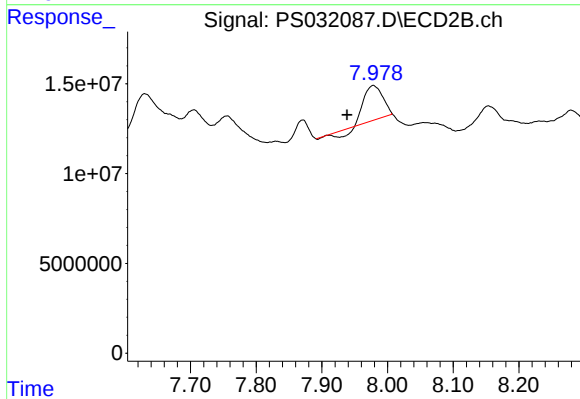

#5 DICAMBA


R.T.: 7.979 min
Delta R.T.: 0.040 min
Response: 36022170
Conc: 4.16 ng/ml

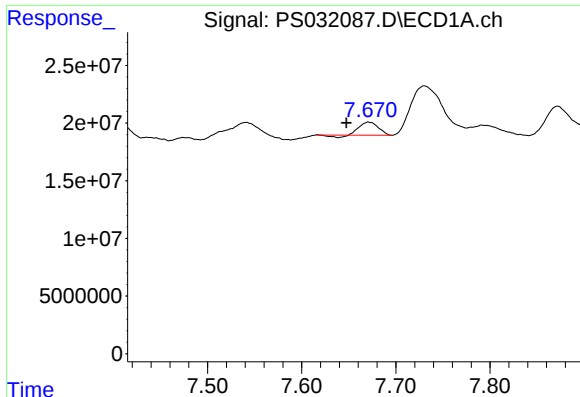

#6 MCPP


R.T.: 7.671 min
Delta R.T.: 0.023 min
Response: 14487227
Conc: 1.18 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

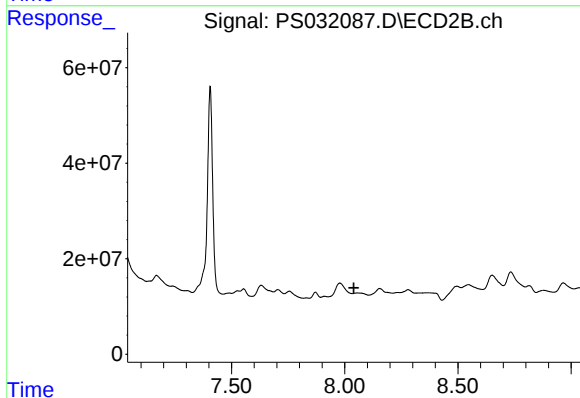


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 8.040 min
Response: 0
Conc: N.D.

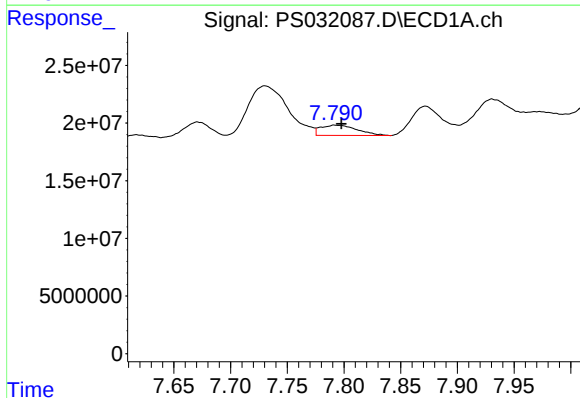


#7 MCPA

R.T.: 7.792 min
Delta R.T.: -0.006 min
Response: 20085115
Conc: 1.36 ug/ml

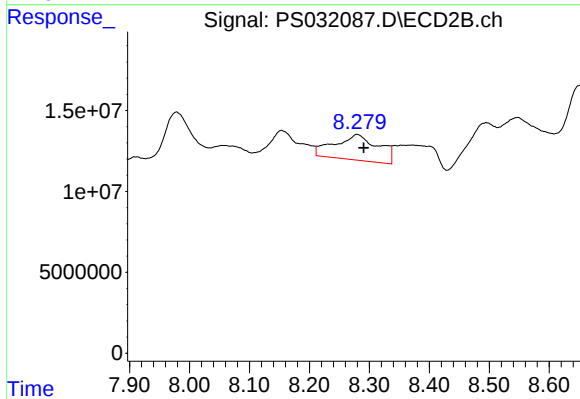

#7 MCPA


R.T.: 8.280 min
Delta R.T.: -0.011 min
Response: 79549842
Conc: 21.09 ug/ml

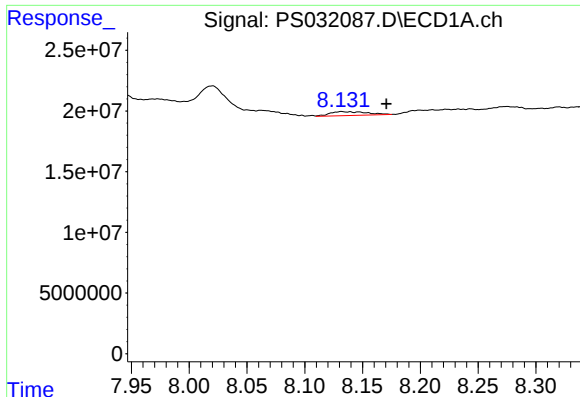

#8 DICHLORPROP


R.T.: 8.132 min
Delta R.T.: -0.039 min
Response: 7243212
Conc: 1.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

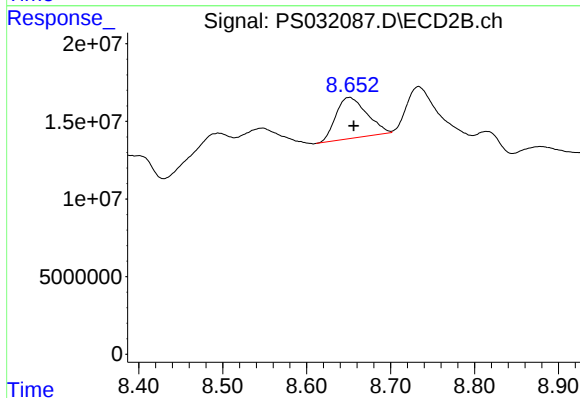


#8 DICHLORPROP

R.T.: 8.651 min
Delta R.T.: -0.005 min
Response: 67811653
Conc: 34.63 ng/ml

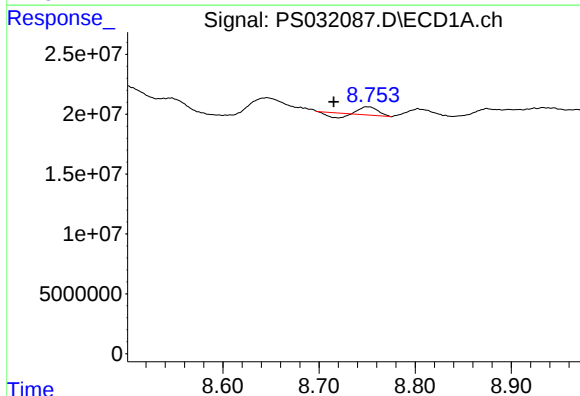


#10 Pentachlorophenol

R.T.: 8.750 min
Delta R.T.: 0.035 min
Response: 5409114
Conc: N.D.

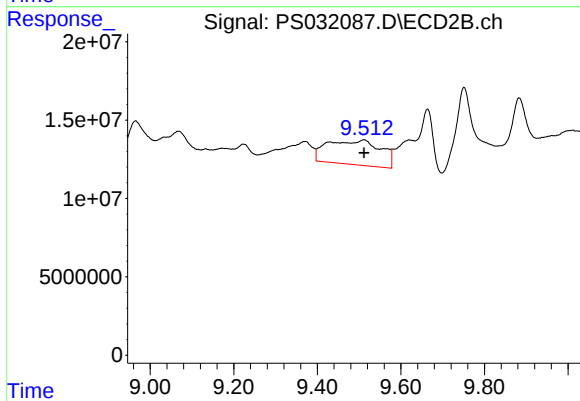

#10 Pentachlorophenol


R.T.: 9.511 min
Delta R.T.: -0.001 min
Response: 138583627
Conc: 2.67 ng/ml

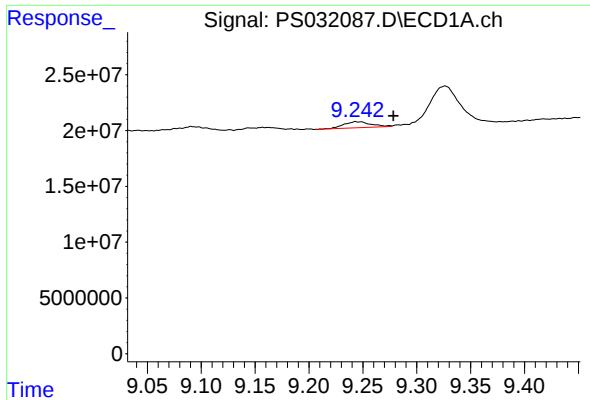

#11 2,4,5-TP (SILVEX)


R.T.: 9.243 min
Delta R.T.: -0.035 min
Response: 9519541
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3

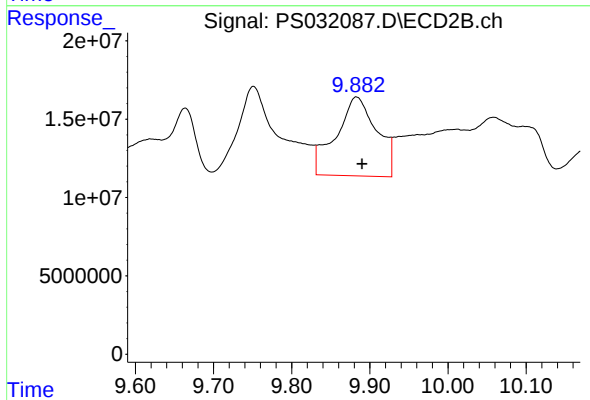


#11 2,4,5-TP (SILVEX)

R.T.: 9.883 min
Delta R.T.: -0.007 min
Response: 183631694
Conc: 9.15 ng/ml

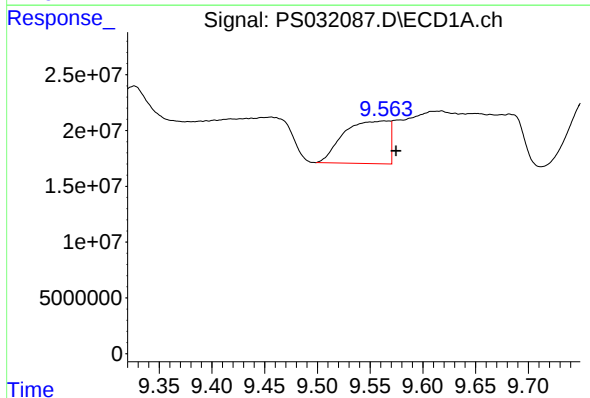


#12 2,4,5-T

R.T.: 9.563 min
Delta R.T.: -0.011 min
Response: 114496720
Conc: 4.54 ng/ml

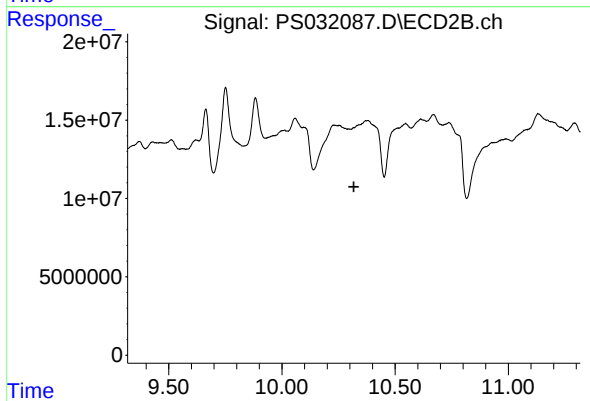

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 10.318 min
Response: 0
Conc: N.D.

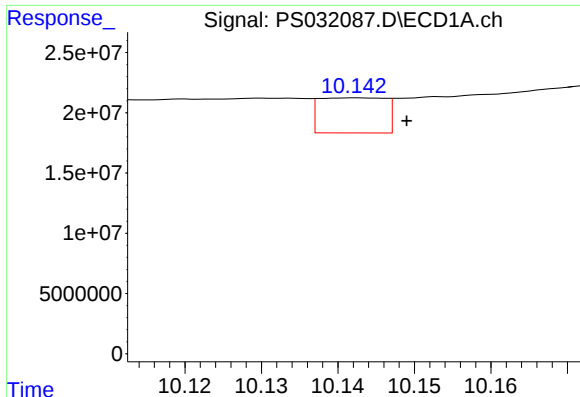

#13 2,4-DB


R.T.: 10.143 min
Delta R.T.: -0.006 min
Response: 17503251
Conc: 5.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

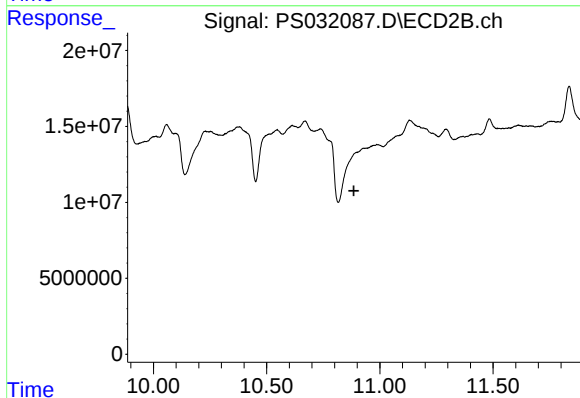


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.885 min
Response: 0
Conc: N.D.

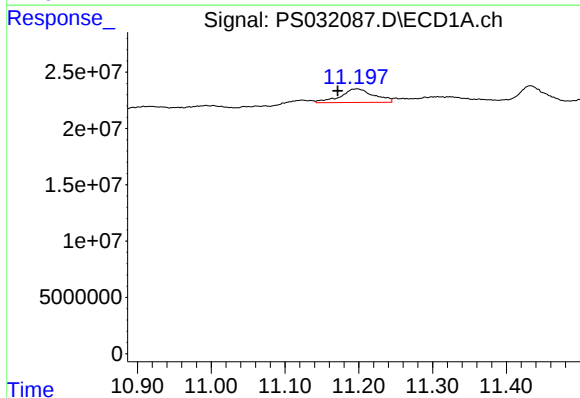

#15 Picloram

R.T.: 11.198 min
Delta R.T.: 0.026 min
Response: 37812918
Conc: 1.60 ng/ml

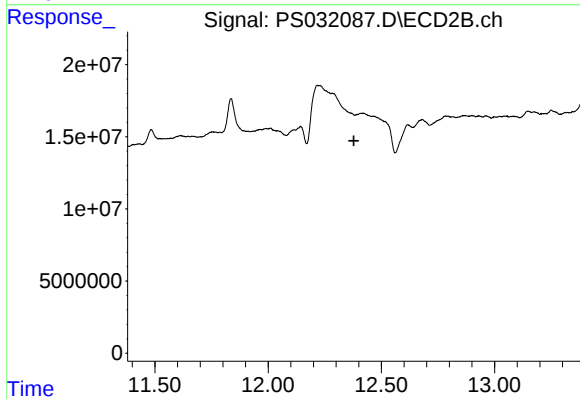

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 12.379 min
Response: 0
Conc: N.D.