

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101725\
 Data File : PS032090.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Oct 2025 22:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 01:46:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 13 12:51:14 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.283	7.751	1752.4E6	434.4E6	367.616	394.770
Target Compounds							
1) T	Dalapon	2.625f	2.693	376535	53658757	<MDL	14.278 #
2) T	3,5-DICHL...	6.450	0.000	3942312	0	<MDL	N.D. #
3) T	4-Nitroph...	7.073	0.000	1965161	0	1.472	N.D. #
7) T	MCPA	7.793	8.242f	283304	22557460	<MDL	5.980 #
8) T	DICHLORPROP	8.162	0.000	1544314	0	<MDL	N.D. #
10) T	Pentachlo...	8.718	9.516	4706969	26799332	<MDL	<MDL #
11) T	2,4,5-TP ...	9.277	9.921f	3002895	3767627	<MDL	<MDL #
12) T	2,4,5-T	9.617f	10.306	3810602	6942147	<MDL	<MDL #
13) T	2,4-DB	10.161	10.921f	743076	7070141	<MDL	5.472 #
14) T	DINOSEB	11.359	0.000	1821757	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101725\
Data File : PS032090.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Oct 2025 22:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 01:46:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101325.M
Quant Title : 8080.M
QLast Update : Mon Oct 13 12:51:14 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

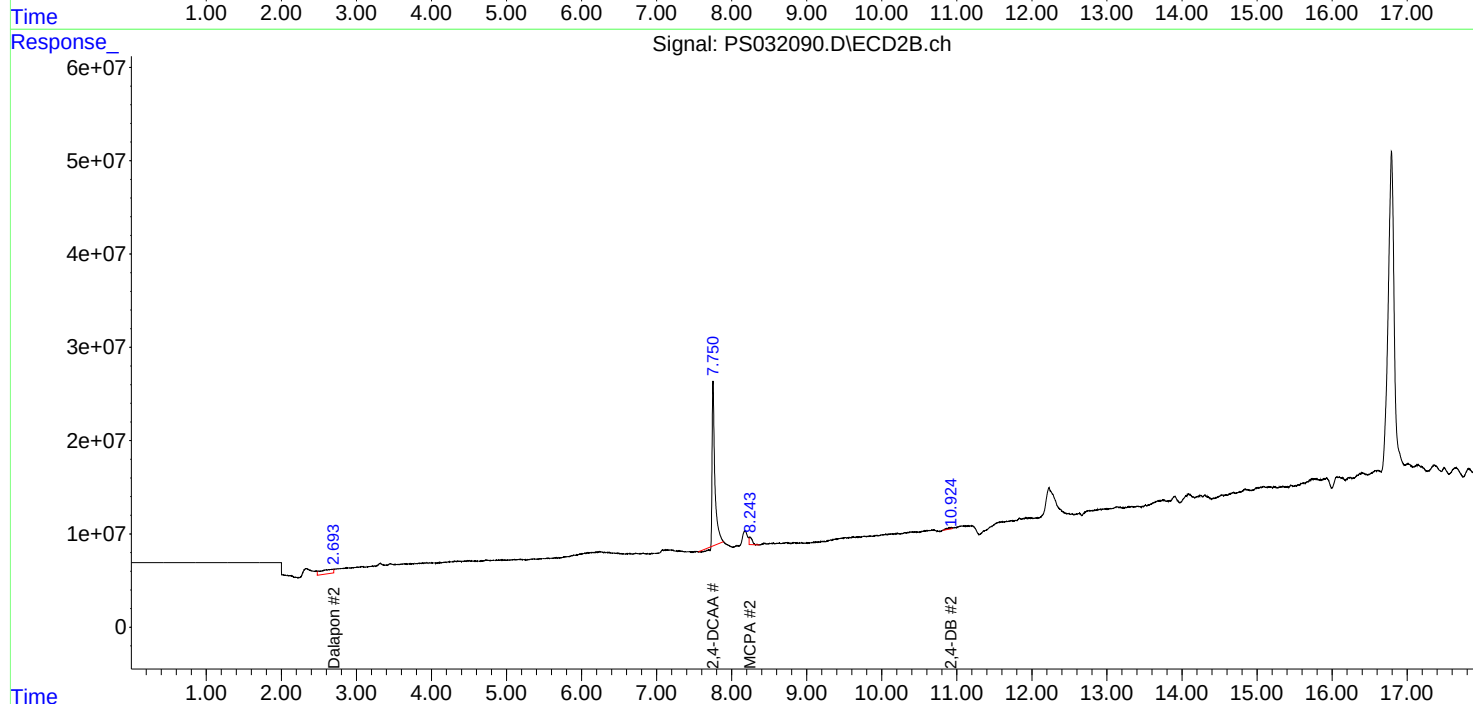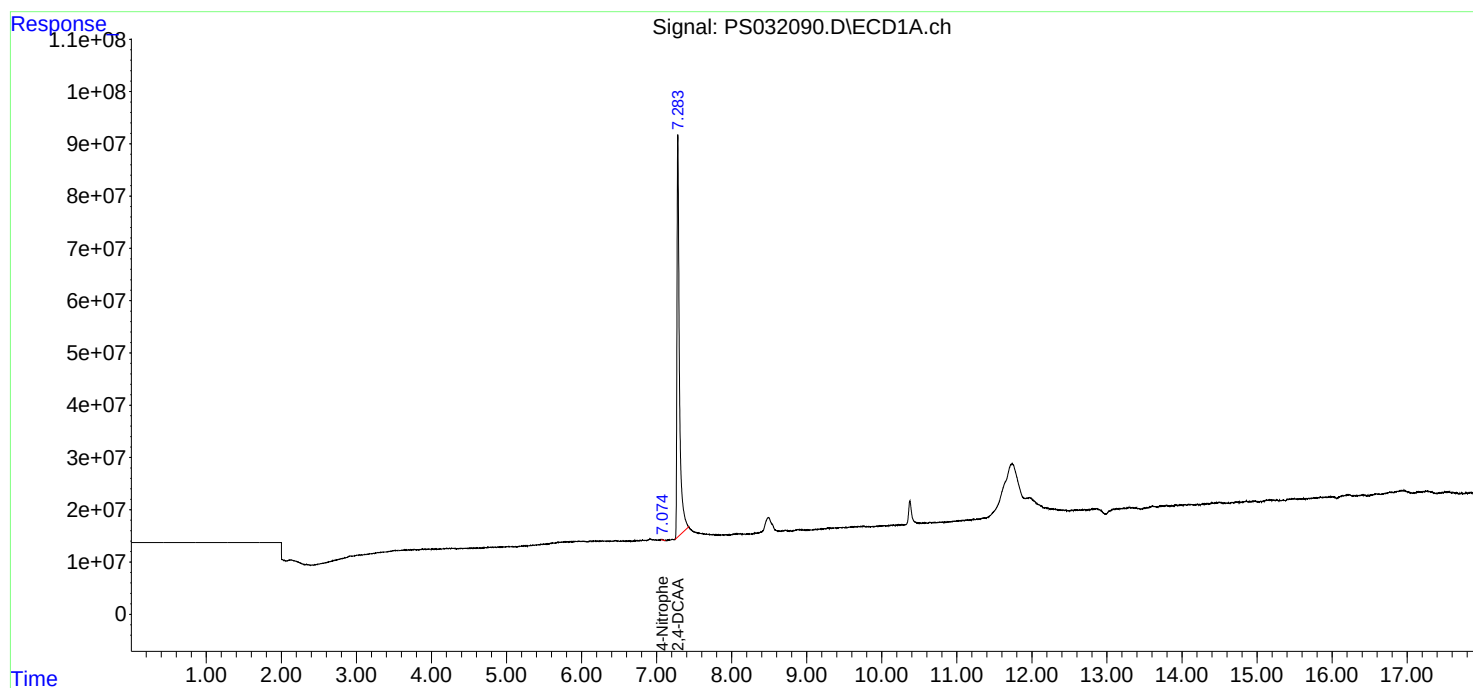


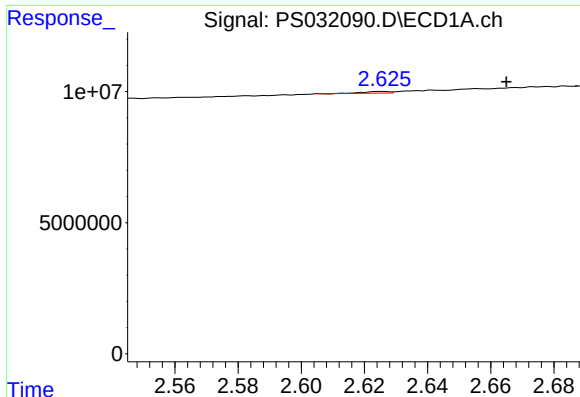

#1 Dalapon


R.T.: 2.625 min
Delta R.T.: -0.040 min
Response: 376535
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

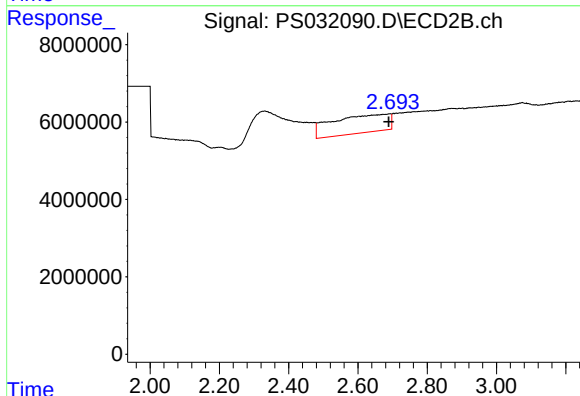


#1 Dalapon

R.T.: 2.693 min
Delta R.T.: 0.004 min
Response: 53658757
Conc: 14.28 ng/ml

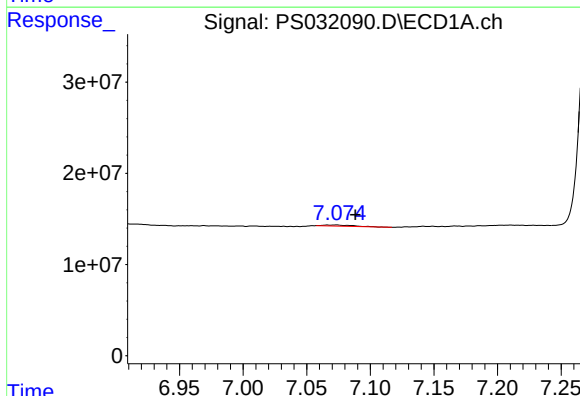


#3 4-Nitrophenol

R.T.: 7.073 min
Delta R.T.: -0.015 min
Response: 1965161
Conc: 1.47 ng/ml

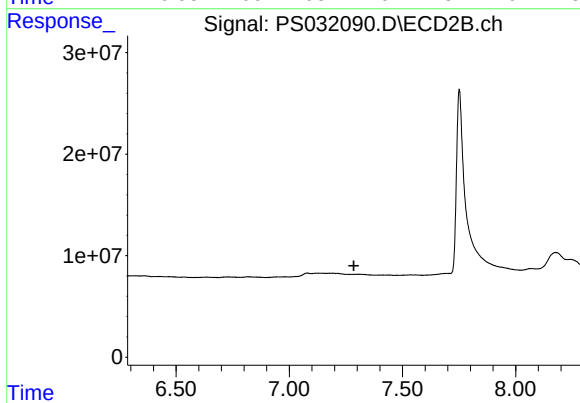

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.285 min
Response: 0
Conc: N.D.

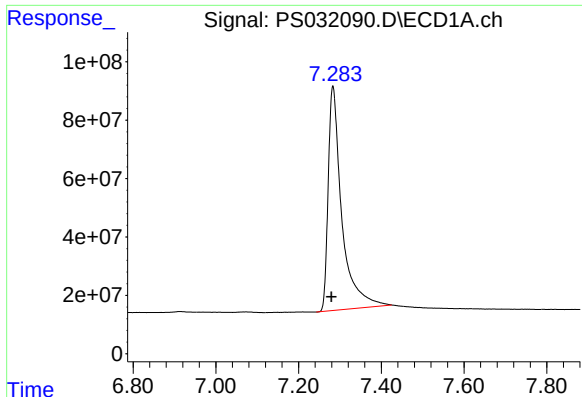

#4 2,4-DCAA


R.T.: 7.283 min
Delta R.T.: 0.003 min
Response: 1752437238
Conc: 367.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

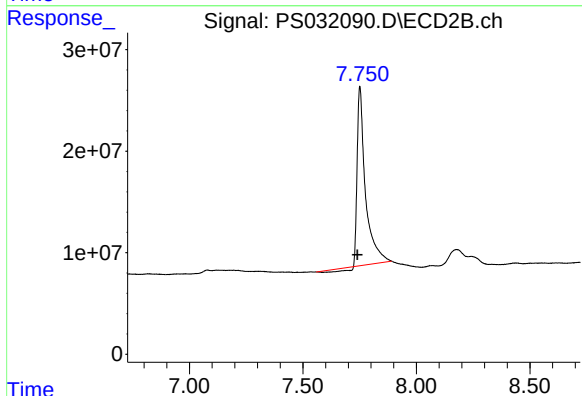


#4 2,4-DCAA

R.T.: 7.751 min
Delta R.T.: 0.010 min
Response: 434381013
Conc: 394.77 ng/ml

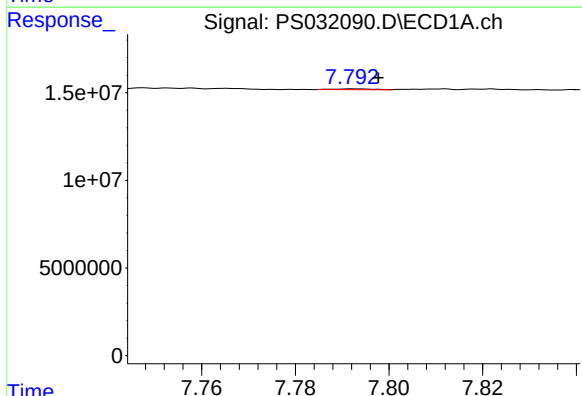


#7 MCPA

R.T.: 7.793 min
Delta R.T.: -0.005 min
Response: 283304
Conc: N.D.

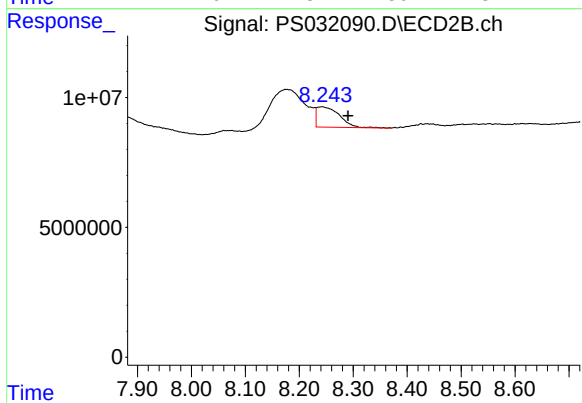

#7 MCPA


R.T.: 8.242 min
Delta R.T.: -0.049 min
Response: 22557460
Conc: 5.98 ug/ml

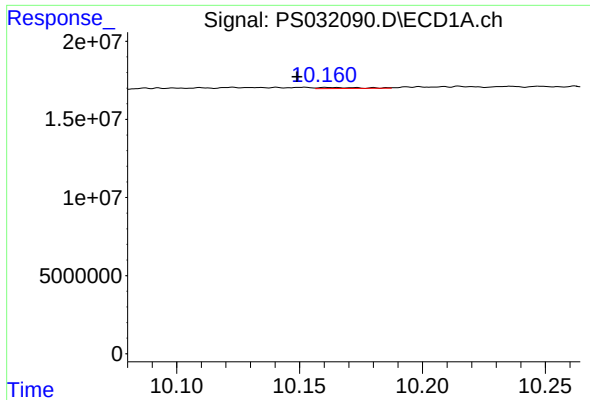

#13 2,4-DB

R.T.: 10.161 min
Delta R.T.: 0.012 min
Response: 743076
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

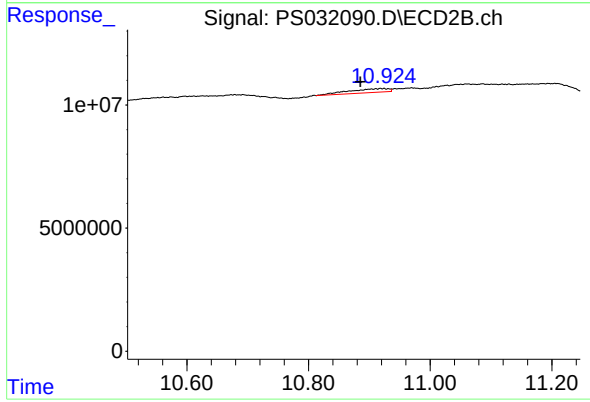

#13 2,4-DB

R.T.: 10.921 min
Delta R.T.: 0.036 min
Response: 7070141
Conc: 5.47 ng/ml