

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101818\
 Data File : PS002024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2018 16:01
 Operator : EI\SJ
 Sample : PB113948BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 04:35:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.444	10.926	105.9E6	149.5E6	500.944	626.799 #
Target Compounds							
1) T	Dalapon	2.879	2.361	46238437	66568600	151.523	228.001 #
5) T	DICAMBA	0.000	11.273	0	9865366	N.D.	12.006 #
6) T	MCPD	12.131	0.000	23502890	0	41.973	N.D. #
7) T	MCPA	0.000	11.786	0	301399	N.D.	0.366 #
8) T	DICHLORPROP	12.930	0.000	41584411	0	191.896	N.D. #
12) T	2,4,5-T	0.000	14.553	0	5828682	N.D.	5.321 #
14) T	DINOSEB	0.000	15.675	0	3546665	N.D.	4.010 #
15) T	Picloram	16.977	16.865	21252837	47896654	12.431	30.195 #
16) T	DCPA	0.000	16.865	0	47896654	N.D.	26.474 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101818\
Data File : PS002024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2018 16:01
Operator : EI\SJ
Sample : PB113948BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 04:35:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

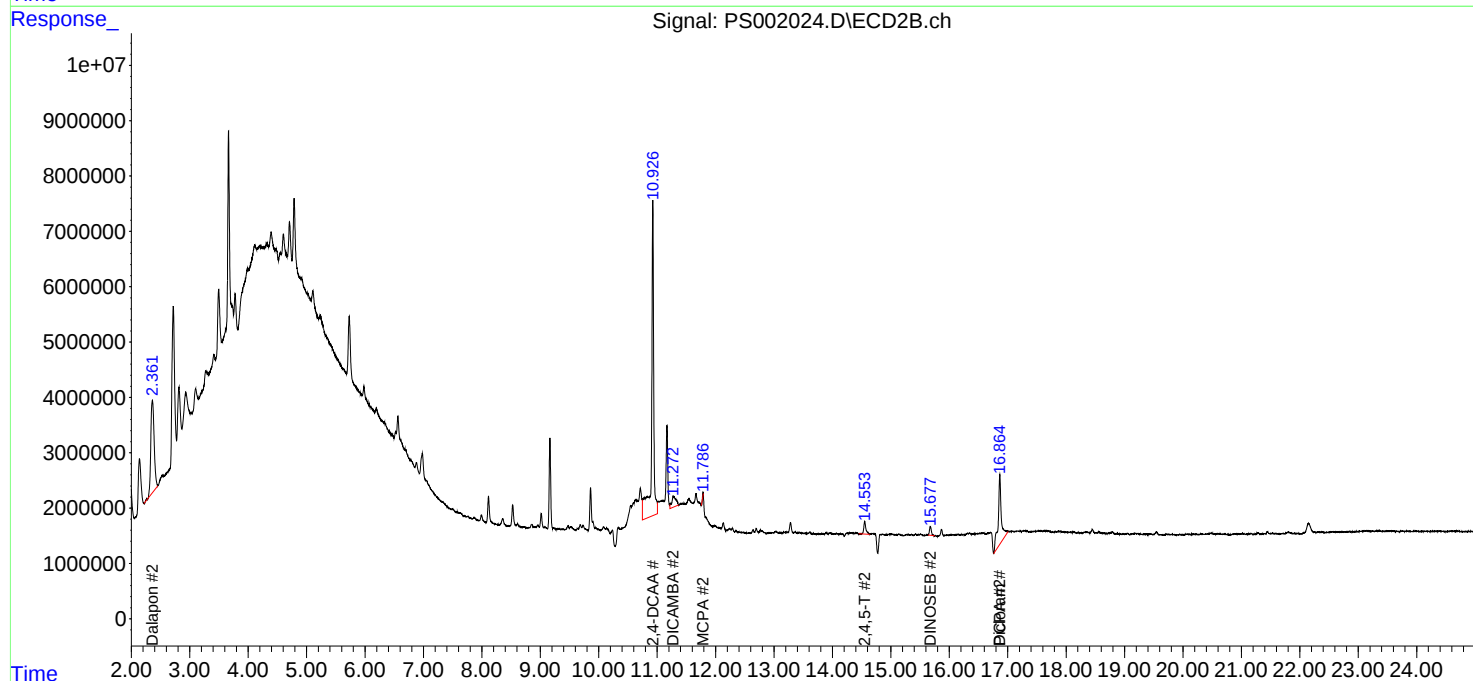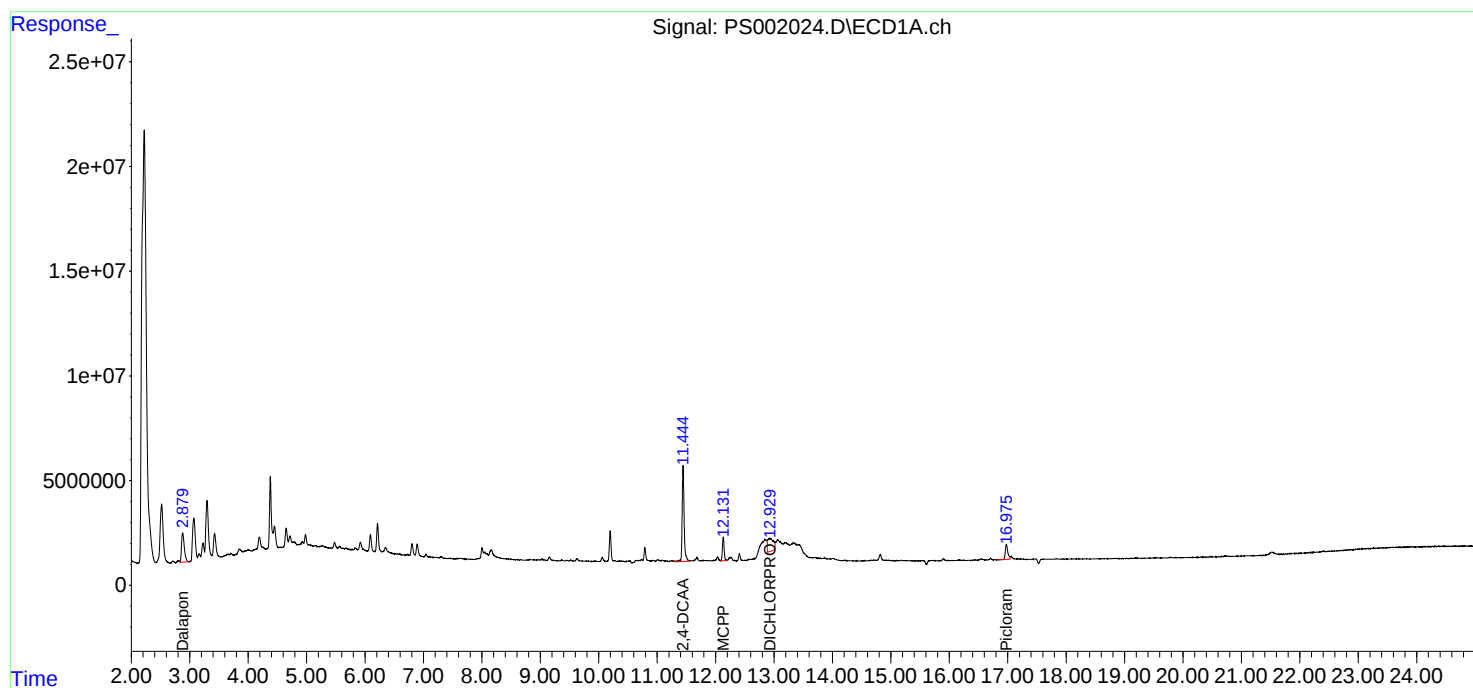


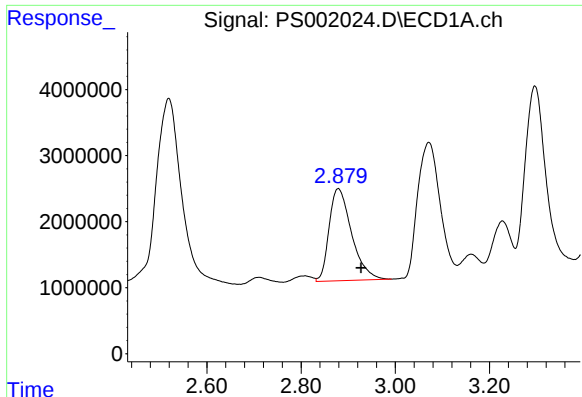

#1 Dalapon


R.T.: 2.879 min
Delta R.T.: -0.048 min
Response: 46238437
Conc: 151.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

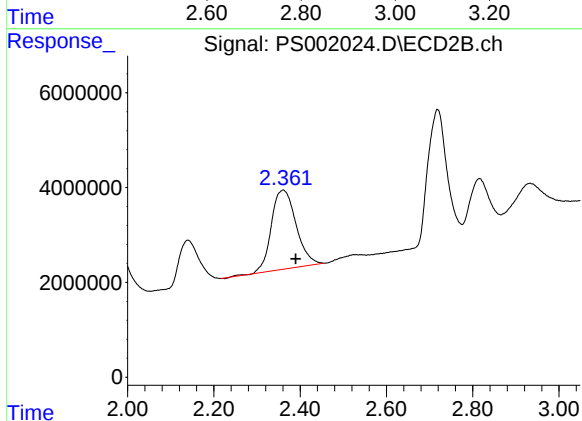


#1 Dalapon

R.T.: 2.361 min
Delta R.T.: -0.029 min
Response: 66568600
Conc: 228.00 ng/ml

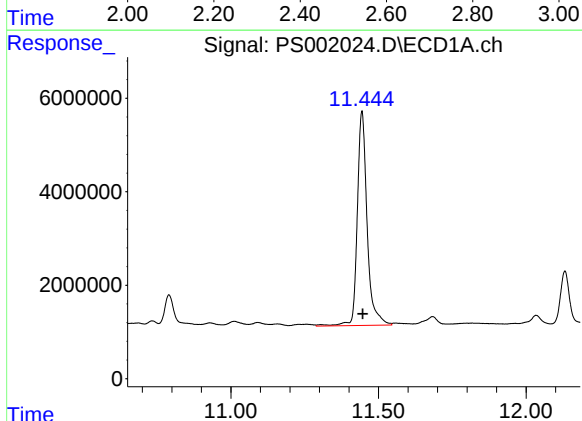


#4 2,4-DCAA

R.T.: 11.444 min
Delta R.T.: -0.003 min
Response: 105900550
Conc: 500.94 ng/ml

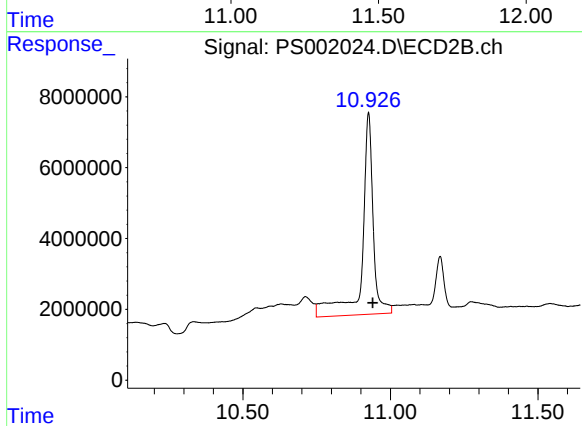

#4 2,4-DCAA


R.T.: 10.926 min
Delta R.T.: -0.014 min
Response: 149495934
Conc: 626.80 ng/ml

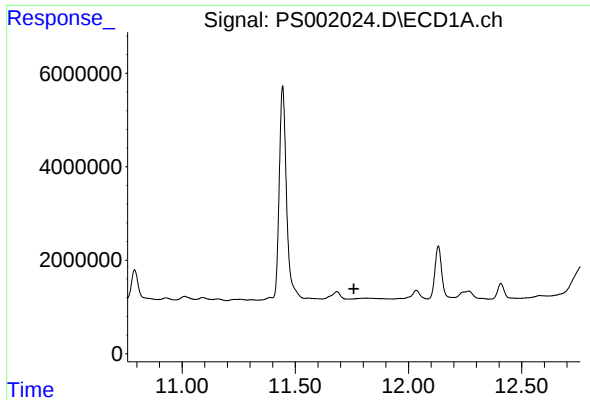

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.759 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

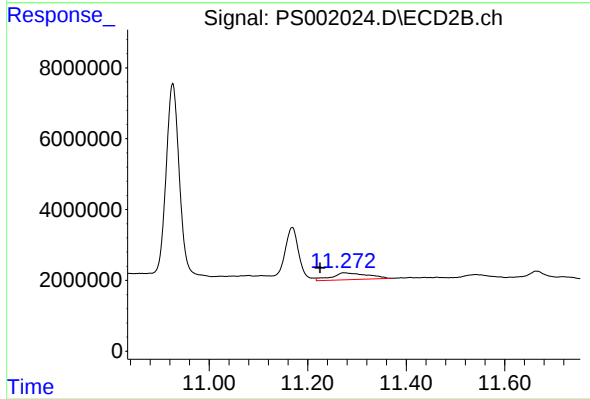


#5 DICAMBA

R.T.: 11.273 min
Delta R.T.: 0.048 min
Response: 9865366
Conc: 12.01 ng/ml

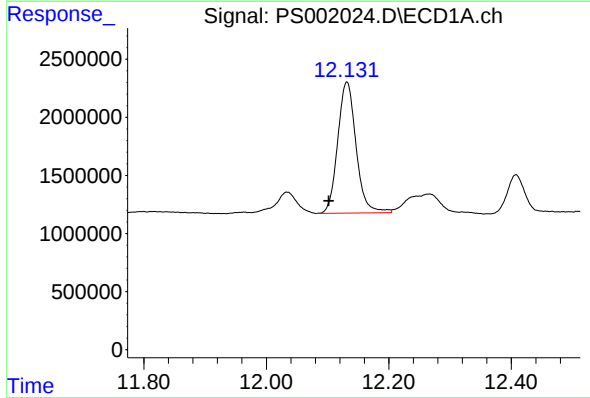


#6 MCP

R.T.: 12.131 min
Delta R.T.: 0.030 min
Response: 23502890
Conc: 41.97 ug/ml

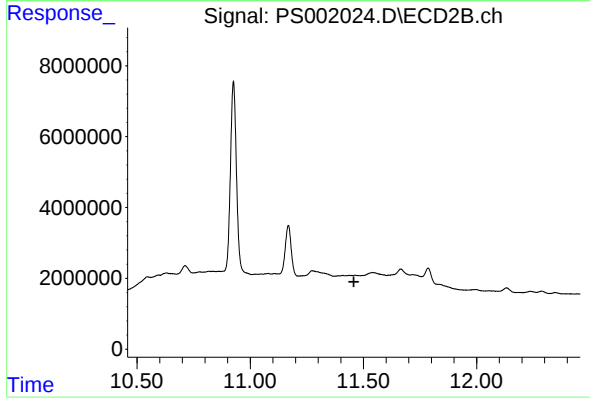

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.458 min
Response: 0
Conc: N.D.

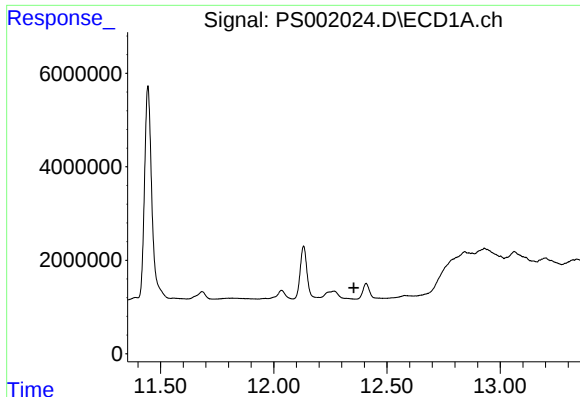

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.354 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

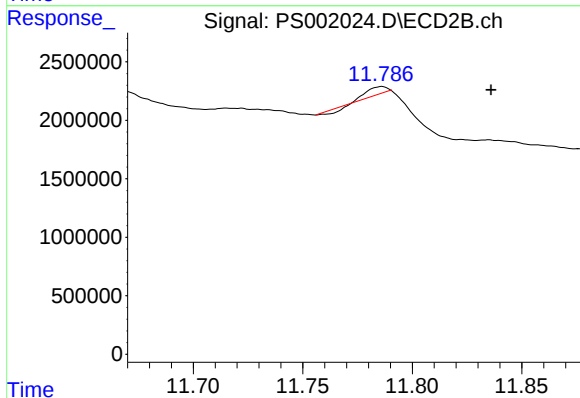


#7 MCPA

R.T.: 11.786 min
Delta R.T.: -0.050 min
Response: 301399
Conc: 0.37 ug/ml

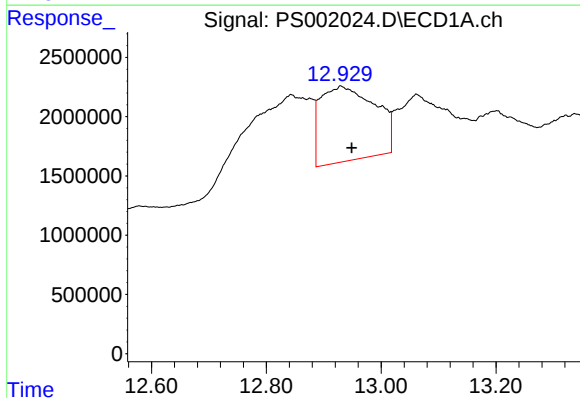


#8 DICHLORPROP

R.T.: 12.930 min
Delta R.T.: -0.019 min
Response: 41584411
Conc: 191.90 ng/ml

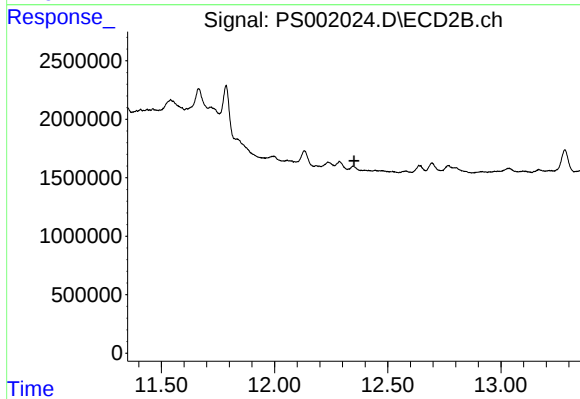

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.351 min
Response: 0
Conc: N.D.

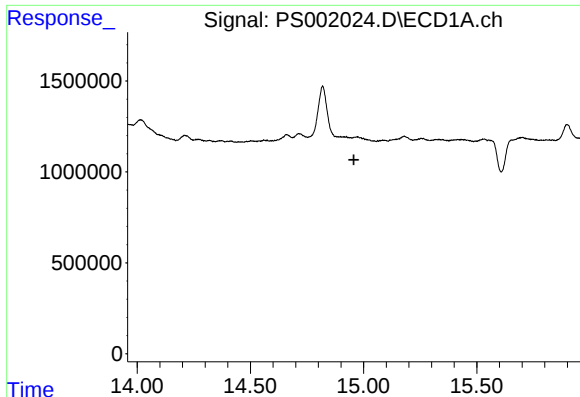

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

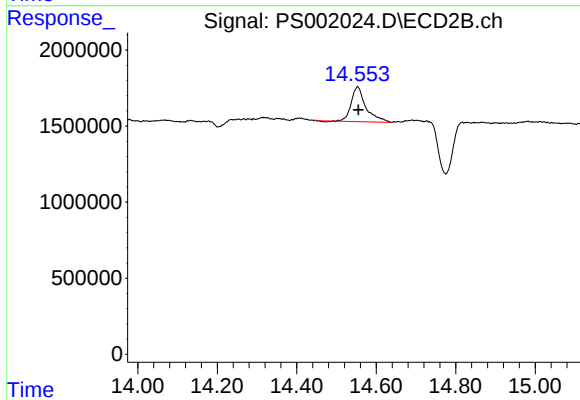


#12 2,4,5-T

R.T.: 14.553 min
Delta R.T.: -0.002 min
Response: 5828682
Conc: 5.32 ng/ml

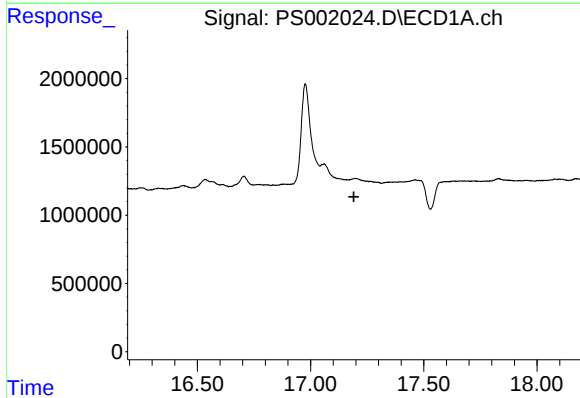


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 17.192 min
Response: 0
Conc: N.D.

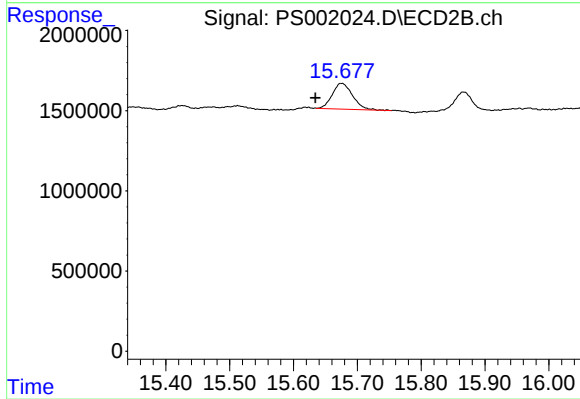

#14 DINOSEB


R.T.: 15.675 min
Delta R.T.: 0.041 min
Response: 3546665
Conc: 4.01 ng/ml

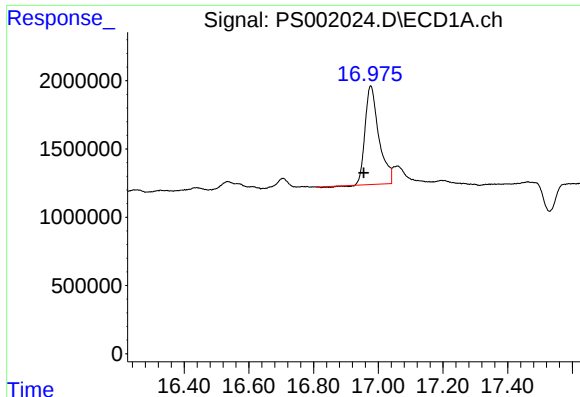

#15 Picloram


R.T.: 16.977 min
Delta R.T.: 0.022 min
Response: 21252837
Conc: 12.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

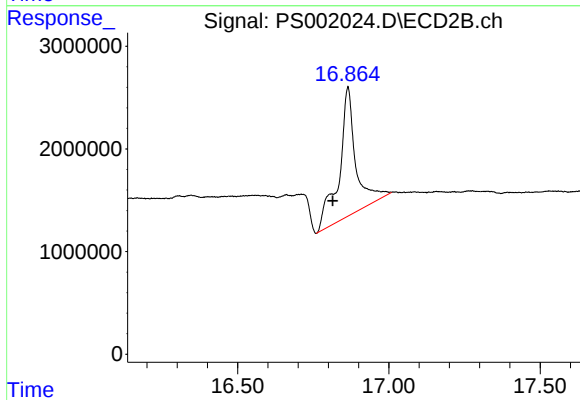


#15 Picloram

R.T.: 16.865 min
Delta R.T.: 0.051 min
Response: 47896654
Conc: 30.19 ng/ml

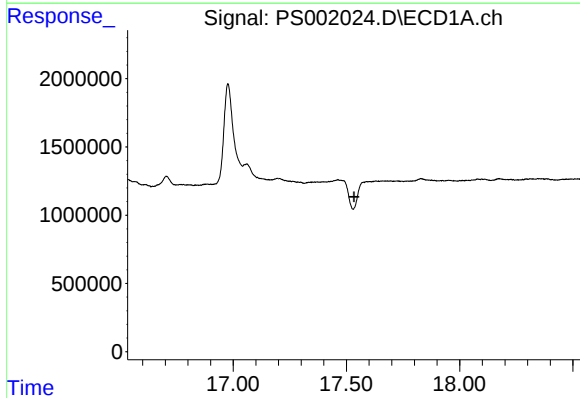

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.533 min
Response: 0
Conc: N.D.

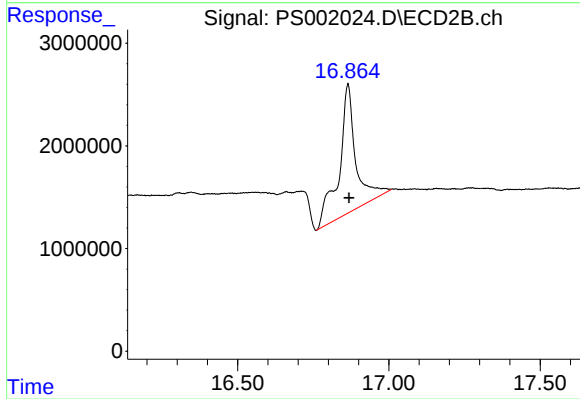

#16 DCPA

R.T.: 16.865 min
Delta R.T.: -0.003 min
Response: 47896654
Conc: 26.47 ng/ml