

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101818\
 Data File : PS002041.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2018 00:47
 Operator : EI\SJ
 Sample : PB113983BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 04:40:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.477	10.972	106.8E6	100.9E6	505.308	423.040
Target Compounds							
1) T	Dalapon	2.916	2.397	50435551	72144692	165.277	247.099 #
2) T	3,5-DICHL...	0.000	9.063	0	6112812	N.D.	20.903 #
5) T	DICAMBA	11.718	11.213	4424639	26972776	5.622	32.826 #
6) T	MCP	12.163	0.000	20444562	0	36.511	N.D. #
7) T	MCPA	0.000	11.829	0	3464694	N.D.	4.208 #
10) T	Pentachlo...	0.000	13.325	0	3854525	N.D.	1.217 #
13) T	2,4-DB	15.724	0.000	4091668	0	26.050	N.D. #
16) T	DCPA	0.000	16.902	0	11270635	N.D.	6.230 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101818\
Data File : PS002041.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2018 00:47
Operator : EI\SJ
Sample : PB113983BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 04:40:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

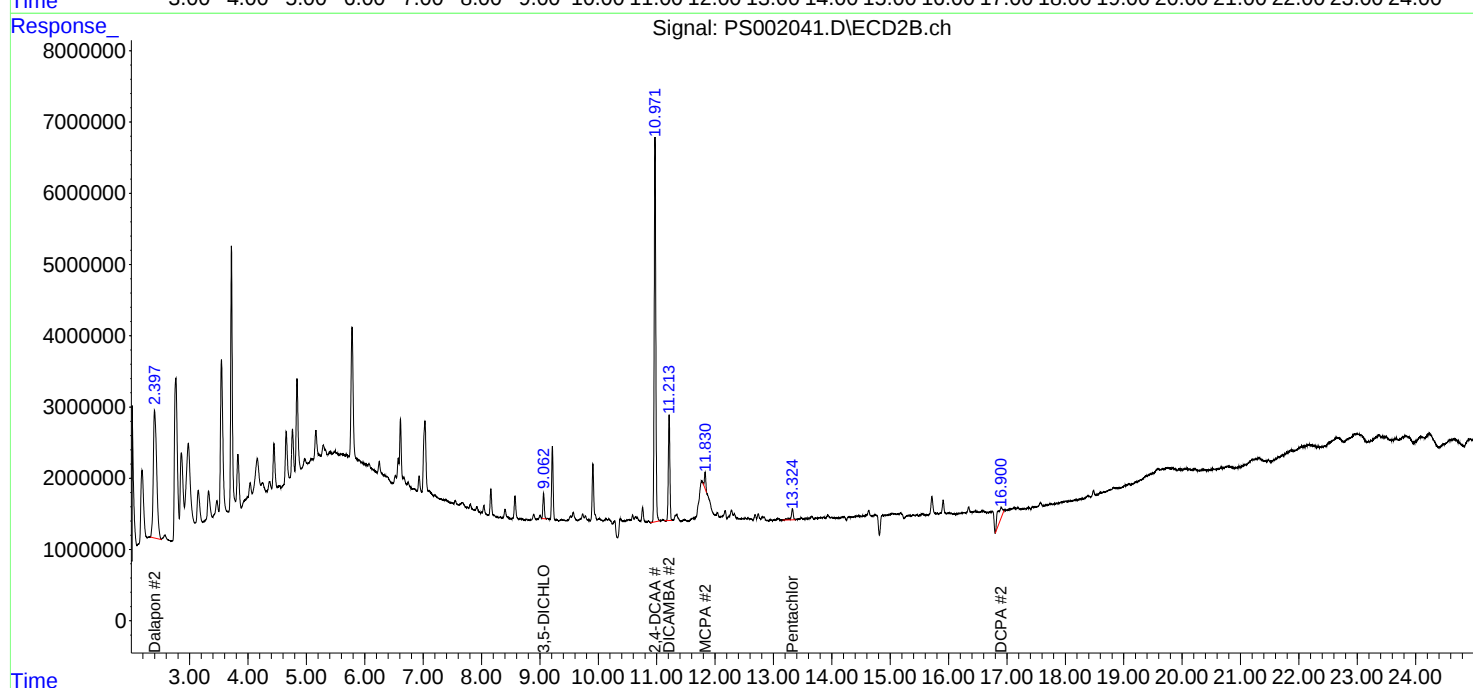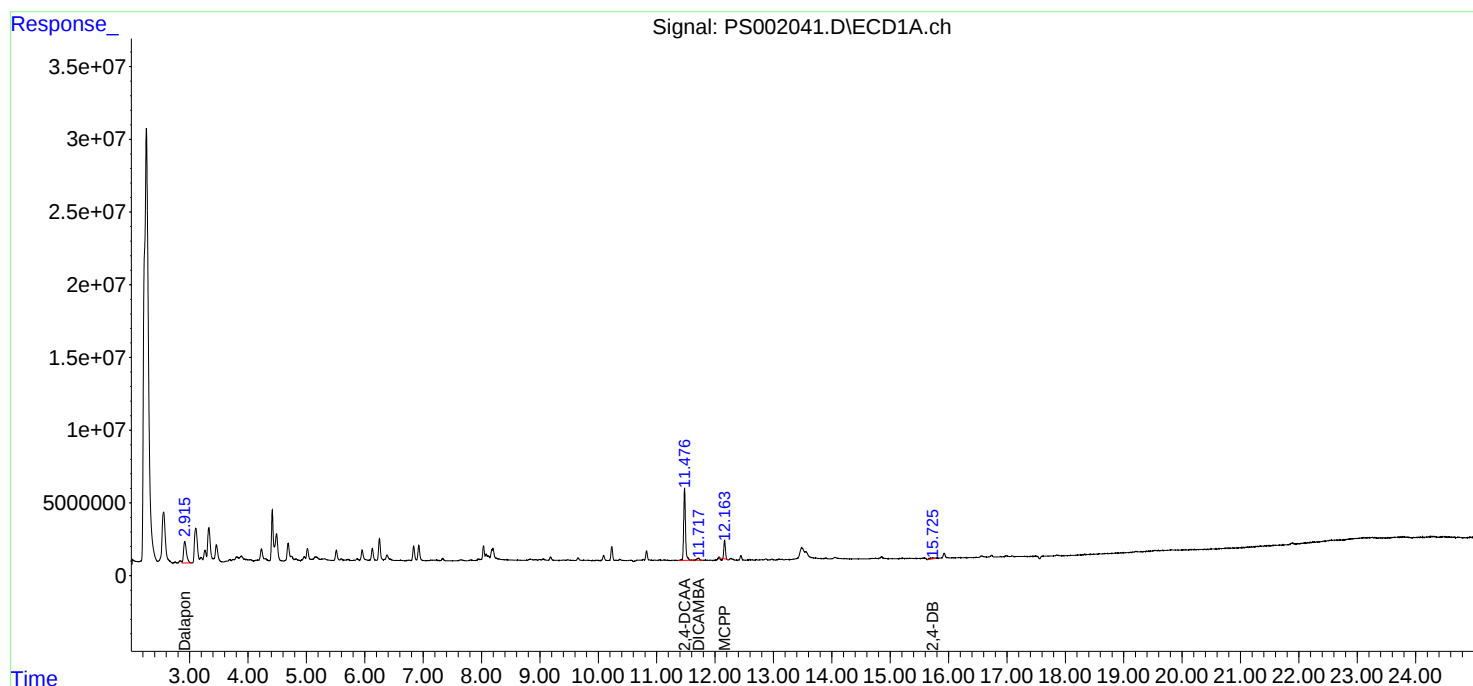


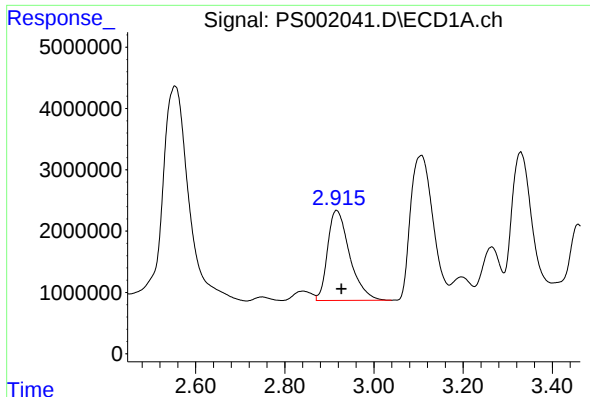

#1 Dalapon


R.T.: 2.916 min
Delta R.T.: -0.011 min
Response: 50435551
Conc: 165.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

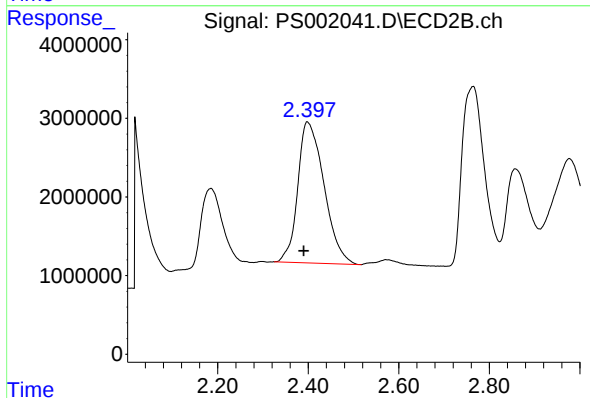


#1 Dalapon

R.T.: 2.397 min
Delta R.T.: 0.007 min
Response: 72144692
Conc: 247.10 ng/ml

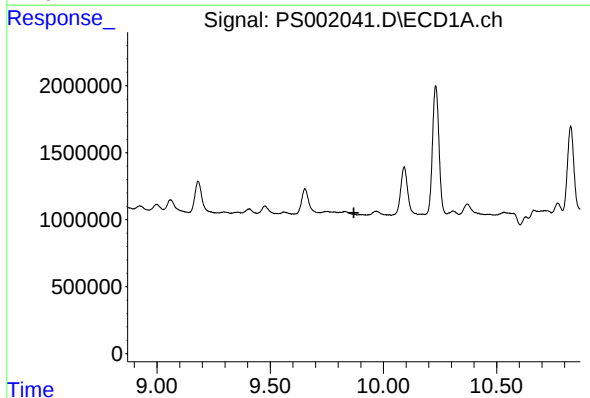


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

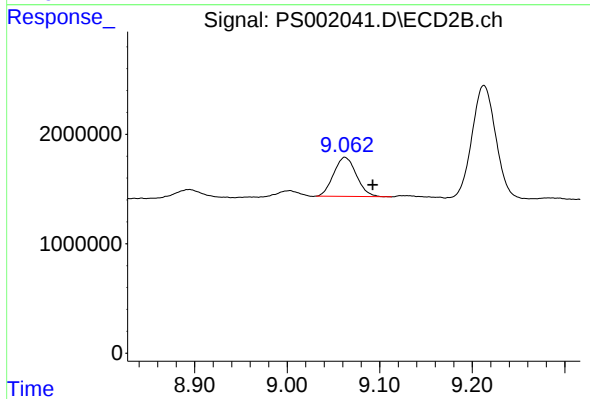

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.063 min
Delta R.T.: -0.030 min
Response: 6112812
Conc: 20.90 ng/ml

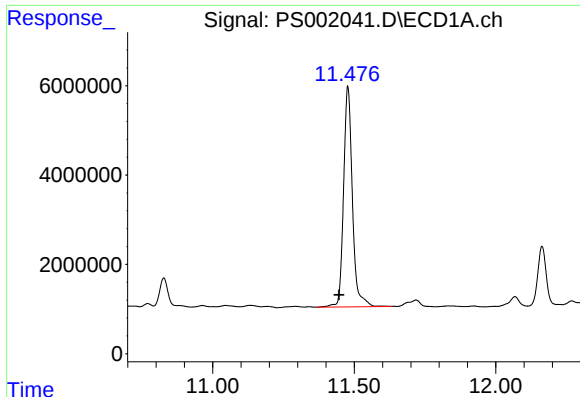

#4 2,4-DCAA


R.T.: 11.477 min
Delta R.T.: 0.030 min
Response: 106823077
Conc: 505.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

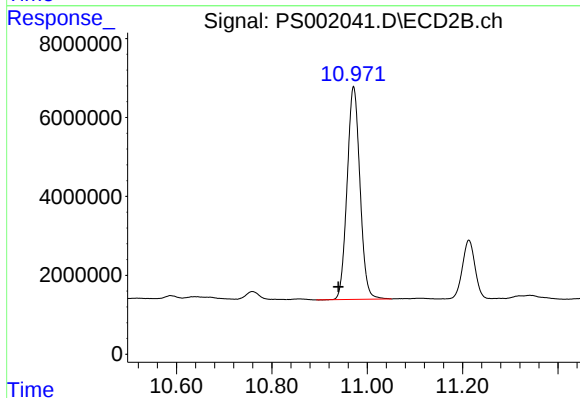


#4 2,4-DCAA

R.T.: 10.972 min
Delta R.T.: 0.032 min
Response: 100897914
Conc: 423.04 ng/ml

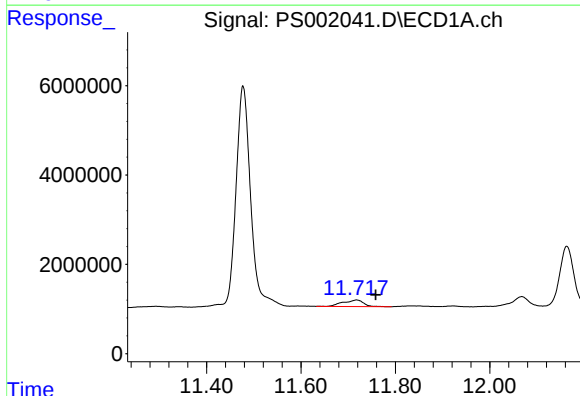


#5 DICAMBA

R.T.: 11.718 min
Delta R.T.: -0.041 min
Response: 4424639
Conc: 5.62 ng/ml

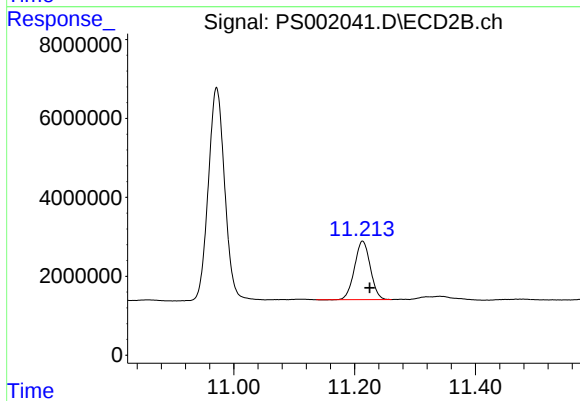

#5 DICAMBA


R.T.: 11.213 min
Delta R.T.: -0.012 min
Response: 26972776
Conc: 32.83 ng/ml

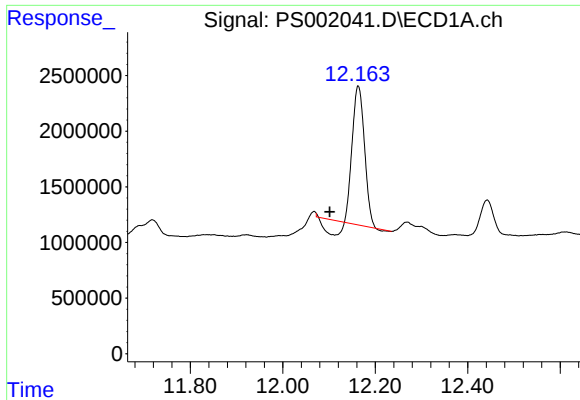

#6 MCPP


R.T.: 12.163 min
Delta R.T.: 0.061 min
Response: 20444562
Conc: 36.51 ug/ml

Instrument :
ECD_S
ClientSampleId :

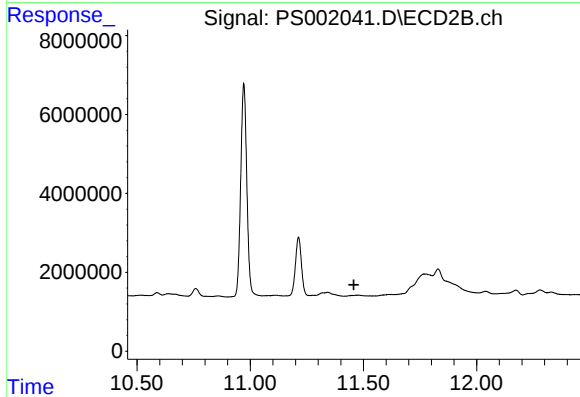


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.458 min
Response: 0
Conc: N.D.

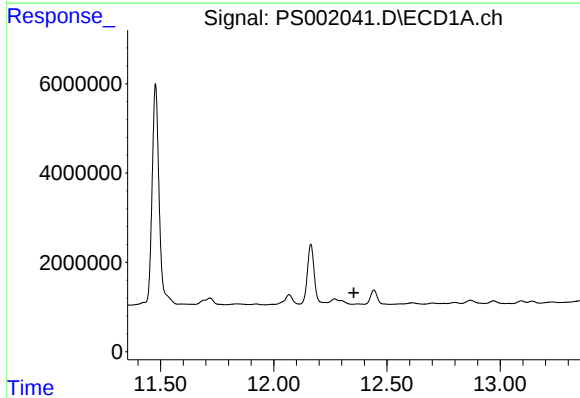


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.354 min
Response: 0
Conc: N.D.

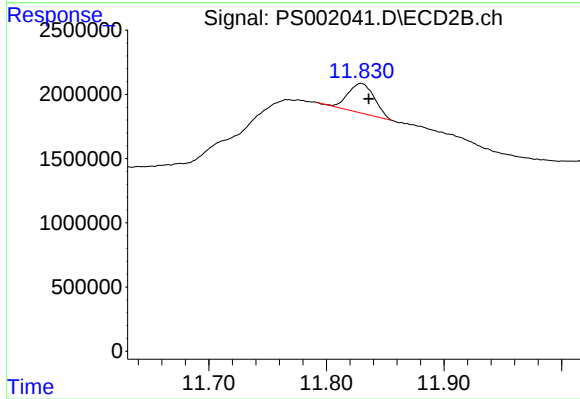

#7 MCPA


R.T.: 11.829 min
Delta R.T.: -0.007 min
Response: 3464694
Conc: 4.21 ug/ml

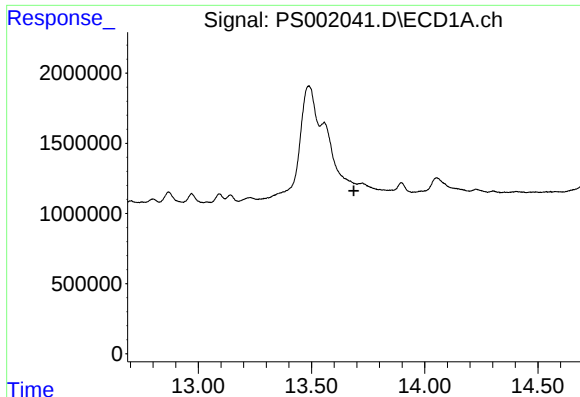

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.687 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

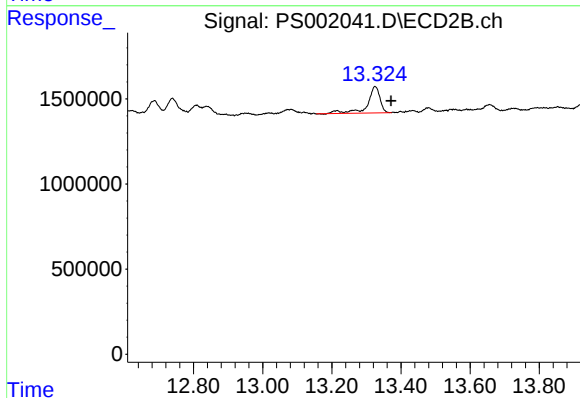


#10 Pentachlorophenol

R.T.: 13.325 min
Delta R.T.: -0.046 min
Response: 3854525
Conc: 1.22 ng/ml

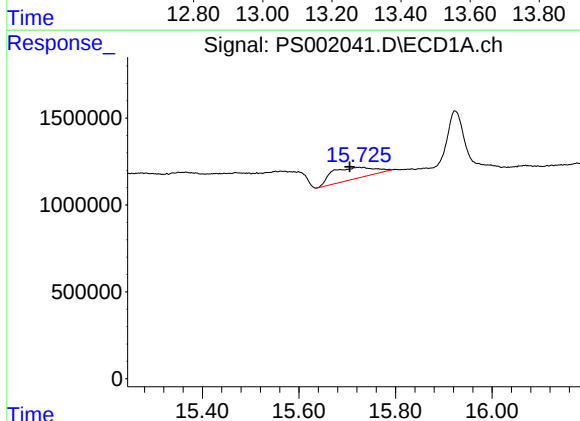


#13 2,4-DB

R.T.: 15.724 min
Delta R.T.: 0.019 min
Response: 4091668
Conc: 26.05 ng/ml

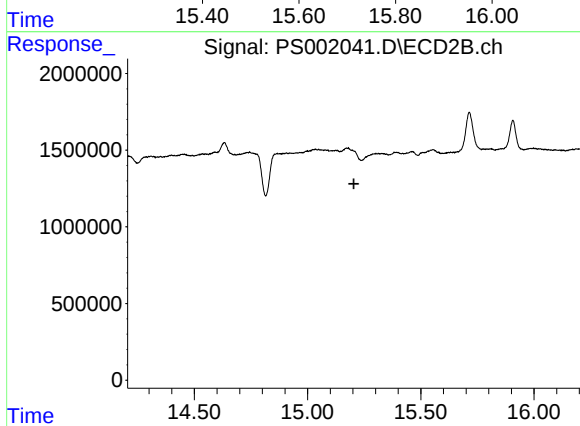

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.205 min
Response: 0
Conc: N.D.

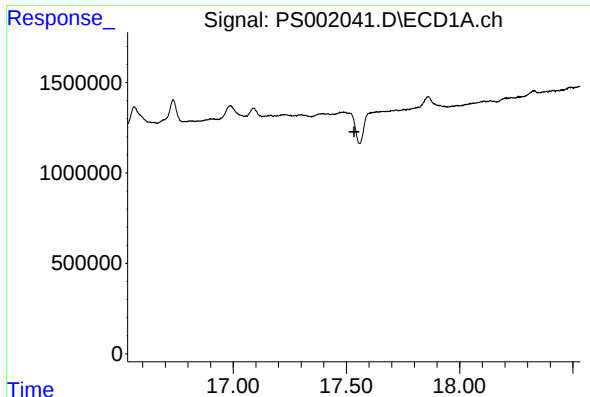

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.533 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

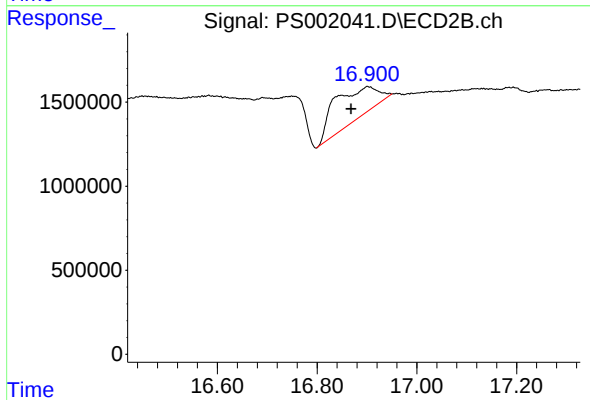

#16 DCPA

R.T.: 16.902 min
Delta R.T.: 0.034 min
Response: 11270635
Conc: 6.23 ng/ml