

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101823\
 Data File : PS024660.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2023 08:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 17:03:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.359	6.779	1057.4E6	349.2E6	513.960	505.139
Target Compounds							
1) T	Dalapon	0.000	2.573	0	2644084	N.D.	2.363
5) T	DICAMBA	0.000	6.982	0	1322167	N.D.	<MDL
6) T	MCPD	0.000	6.982f	0	1322167	N.D.	<MDL
7) T	MCPA	0.000	7.239	0	3766376	N.D.	1.175
8) T	DICHLORPROP	0.000	7.570	0	1246525	N.D.	1.658
9) T	2,4-D	7.251	7.781f	6753791	549499	2.444	<MDL #
11) T	2,4,5-TP ...	0.000	8.619	0	561069	N.D.	<MDL
12) T	2,4,5-T	0.000	8.995	0	361963	N.D.	<MDL
13) T	2,4-DB	0.000	9.496	0	659534	N.D.	1.294
15) T	Picloram	9.687	10.778	81540706	22156968	4.676	3.565
16) T	DCPA	0.000	10.778	0	22156968	N.D.	4.247



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101823\
Data File : PS024660.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2023 08:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 17:03:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

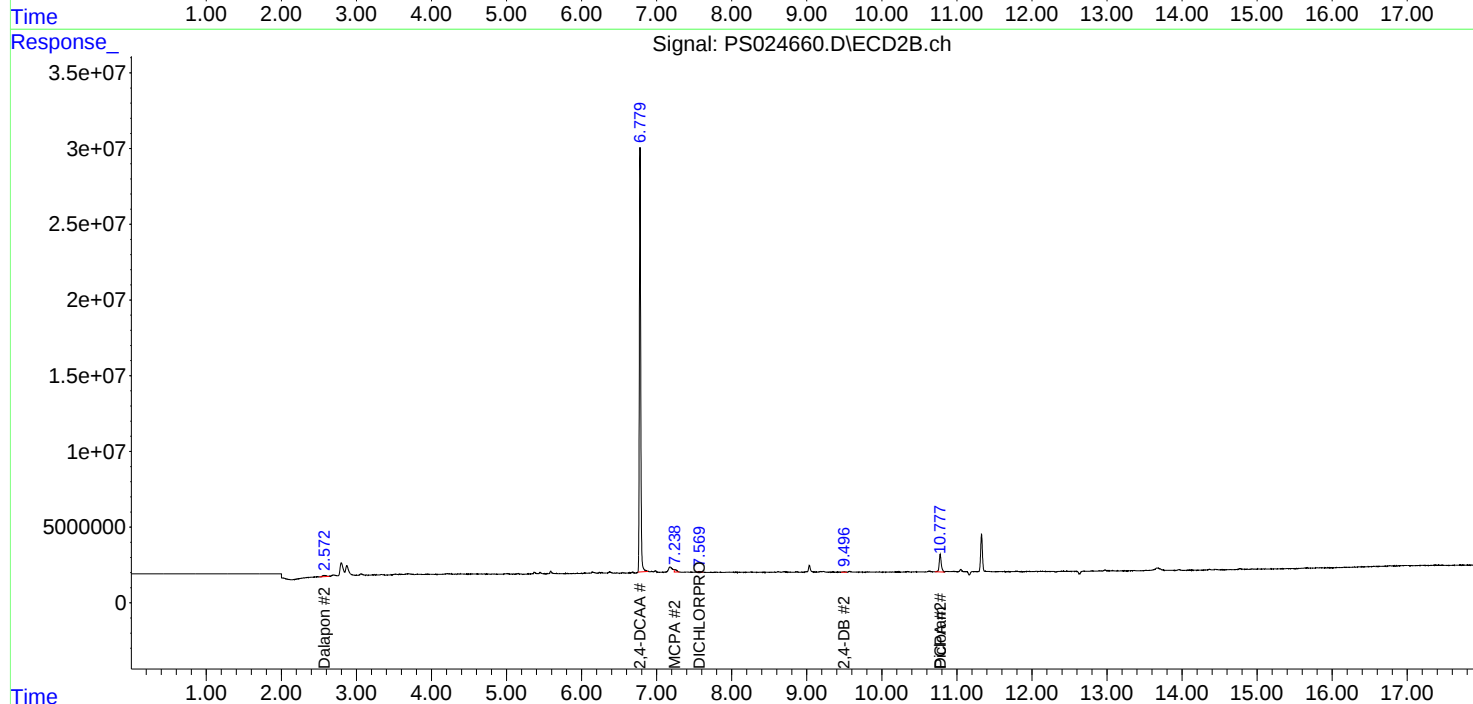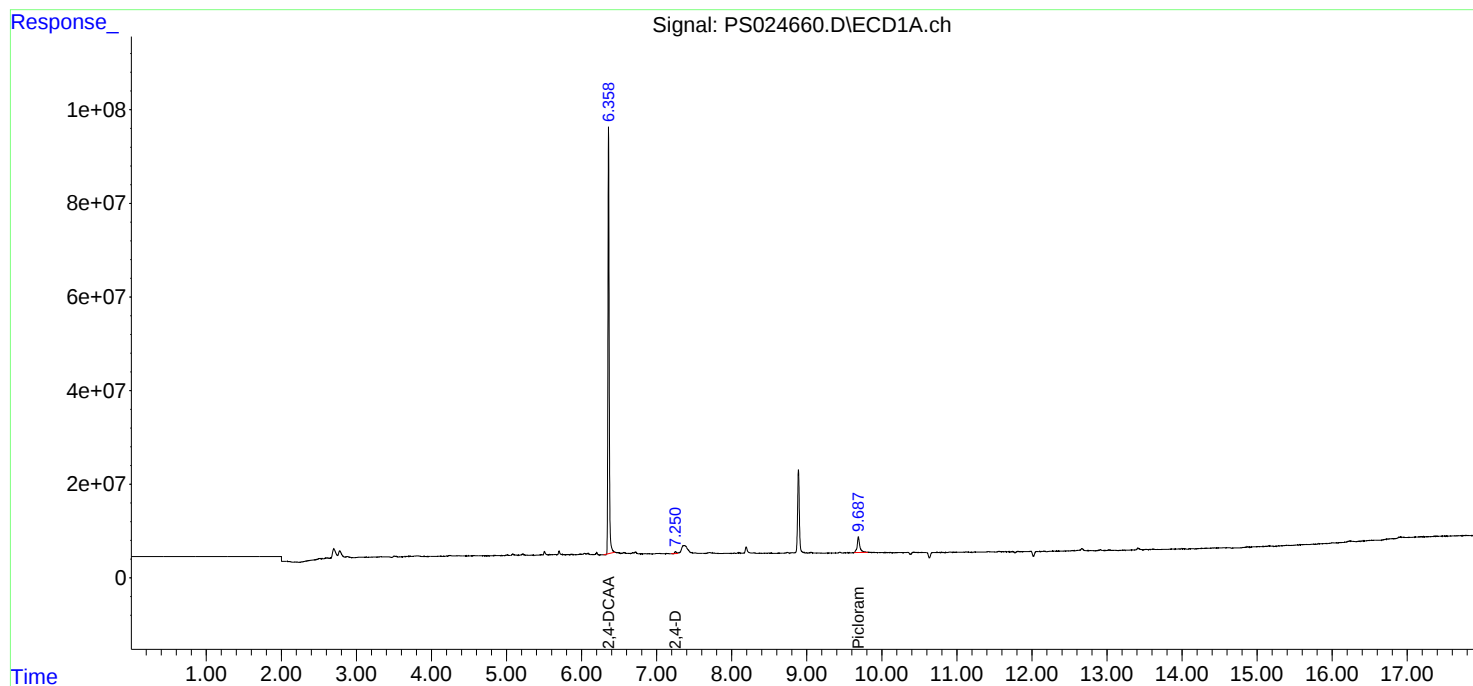


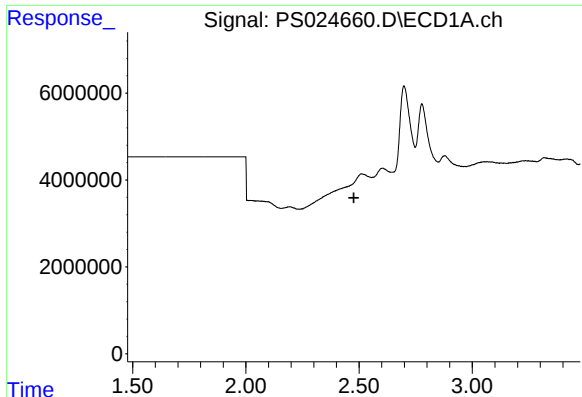

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.477 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

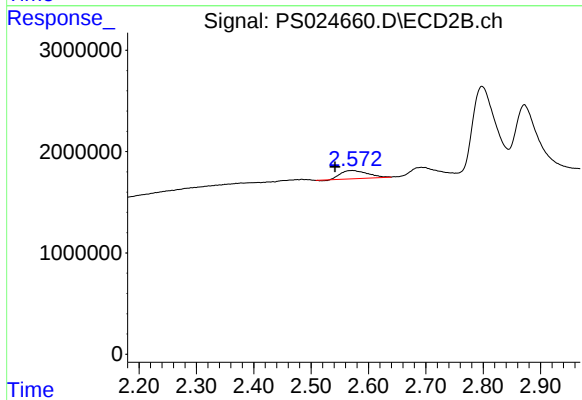


#1 Dalapon

R.T.: 2.573 min
Delta R.T.: 0.030 min
Response: 2644084
Conc: 2.36 ng/ml

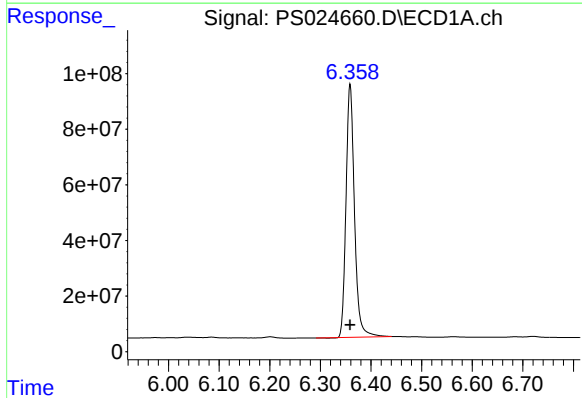


#4 2,4-DCAA

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 1057385081
Conc: 513.96 ng/ml

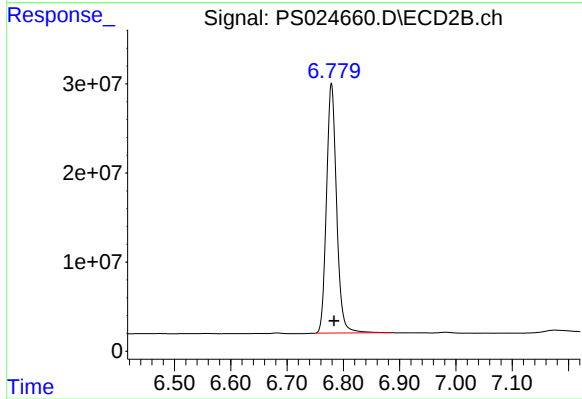

#4 2,4-DCAA


R.T.: 6.779 min
Delta R.T.: -0.005 min
Response: 349198072
Conc: 505.14 ng/ml

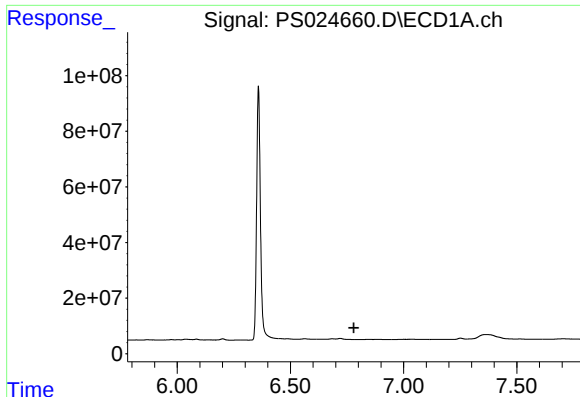

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

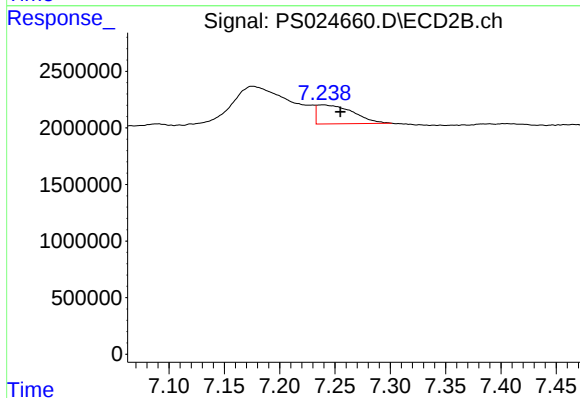


#7 MCPA

R.T.: 7.239 min
Delta R.T.: -0.016 min
Response: 3766376
Conc: 1.18 ug/ml

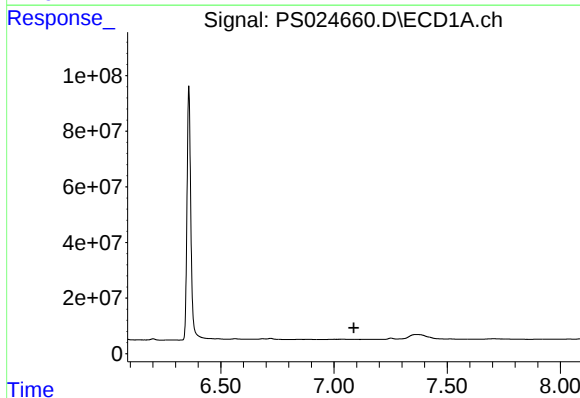


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

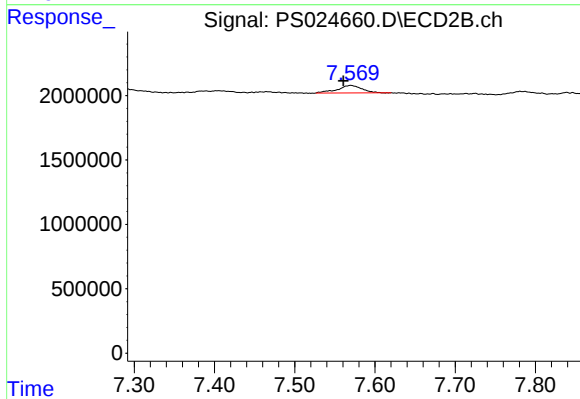

#8 DICHLORPROP


R.T.: 7.570 min
Delta R.T.: 0.009 min
Response: 1246525
Conc: 1.66 ng/ml

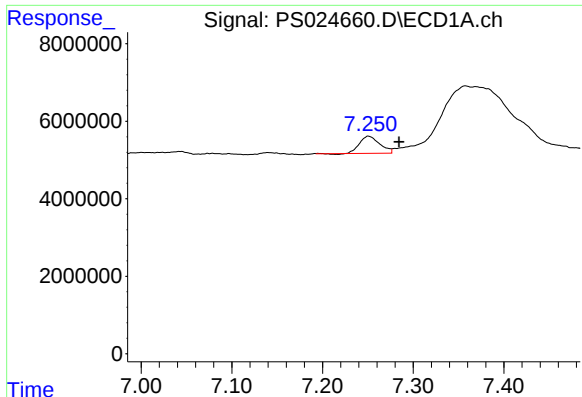

#9 2,4-D


R.T.: 7.251 min
Delta R.T.: -0.033 min
Response: 6753791
Conc: 2.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

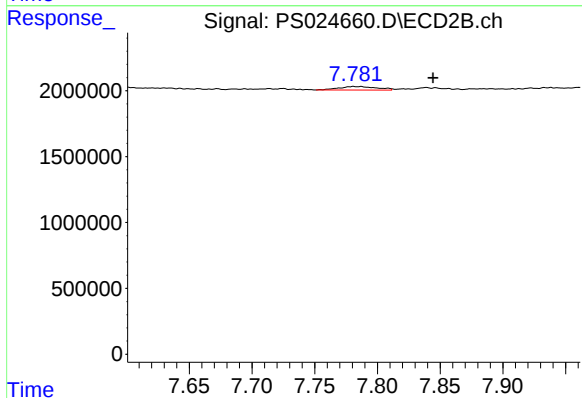


#9 2,4-D

R.T.: 7.781 min
Delta R.T.: -0.063 min
Response: 549499
Conc: N.D.

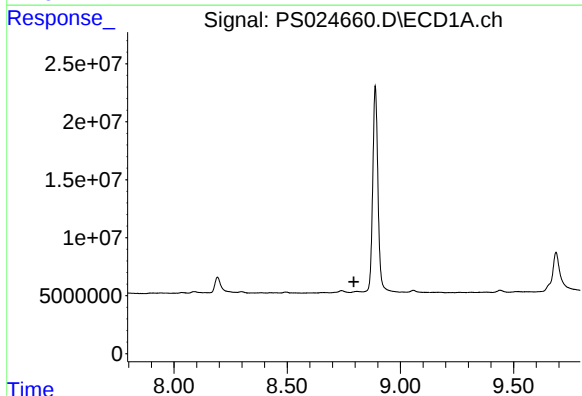


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 8.795 min
Response: 0
Conc: N.D.

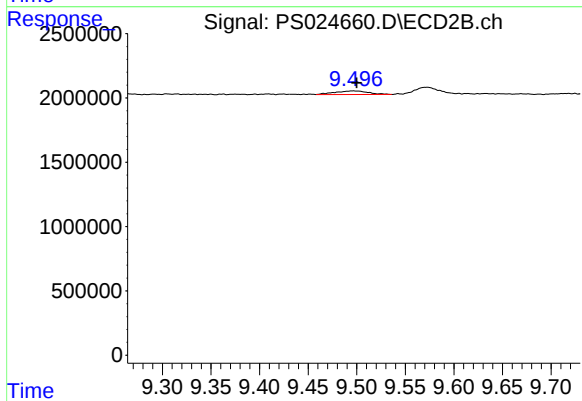

#13 2,4-DB


R.T.: 9.496 min
Delta R.T.: -0.004 min
Response: 659534
Conc: 1.29 ng/ml

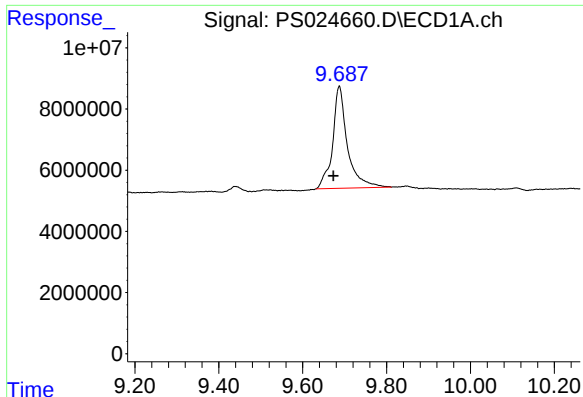

#15 Picloram


R.T.: 9.687 min
Delta R.T.: 0.014 min
Response: 81540706
Conc: 4.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

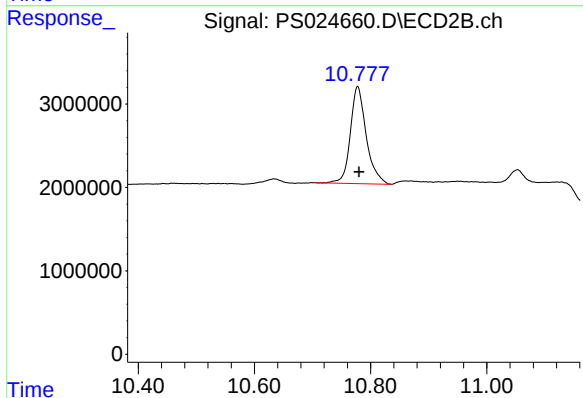


#15 Picloram

R.T.: 10.778 min
Delta R.T.: -0.002 min
Response: 22156968
Conc: 3.57 ng/ml

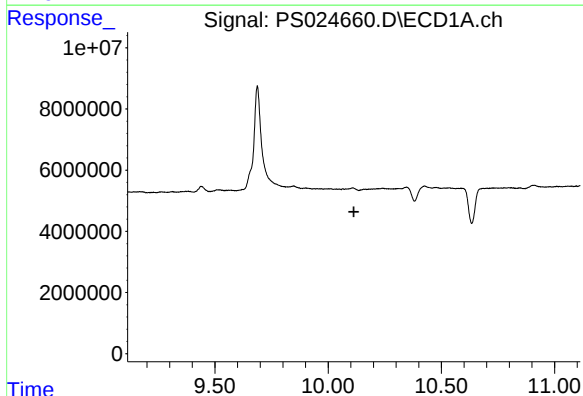

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.114 min
Response: 0
Conc: N.D.

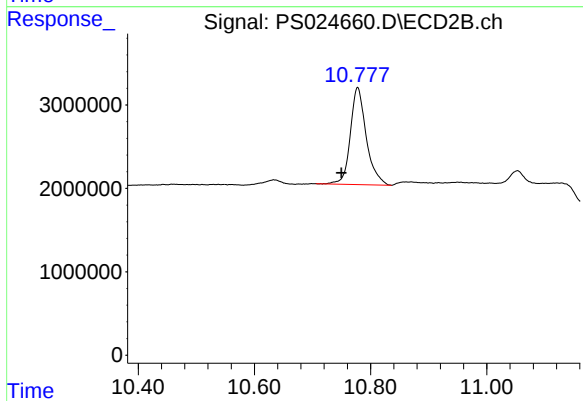

#16 DCPA

R.T.: 10.778 min
Delta R.T.: 0.028 min
Response: 22156968
Conc: 4.25 ng/ml