

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101823\
 Data File : PS024664.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2023 10:38
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 17:05:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 03 14:54:54 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.358	6.779	1064.6E6	353.5E6	517.478	511.298
Target Compounds							
1) T	Dalapon	2.514	2.571	8296889	4073533	3.358	3.640
5) T	DICAMBA	0.000	6.982	0	2304395	N.D.	<MDL
6) T	MCPD	0.000	6.982f	0	2304395	N.D.	1.169
7) T	MCPA	0.000	7.194f	0	18250184	N.D.	5.696
8) T	DICHLORPROP	0.000	7.569	0	1780208	N.D.	2.367
9) T	2,4-D	7.251	7.783f	12615435	443305	4.566	<MDL #
11) T	2,4,5-TP ...	0.000	8.621	0	606749	N.D.	<MDL
12) T	2,4,5-T	0.000	9.037	0	1361119	N.D.	<MDL
13) T	2,4-DB	0.000	9.498	0	744535	N.D.	1.461
15) T	Picloram	9.656	10.781	10324514	6284452	<MDL	1.011 #
16) T	DCPA	0.000	10.781	0	6284452	N.D.	1.205



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101823\
Data File : PS024664.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2023 10:38
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 17:05:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100323.M
Quant Title : 8080.M
QLast Update : Tue Oct 03 14:54:54 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

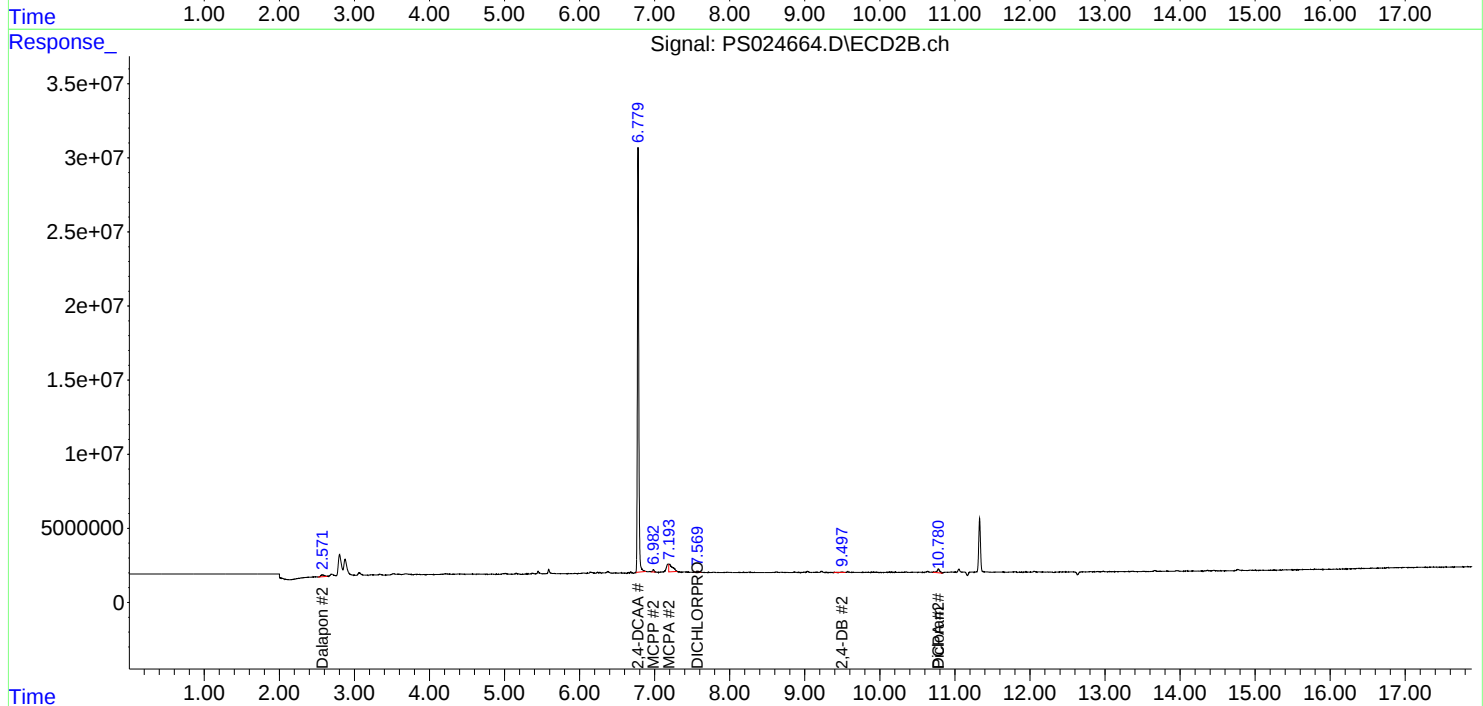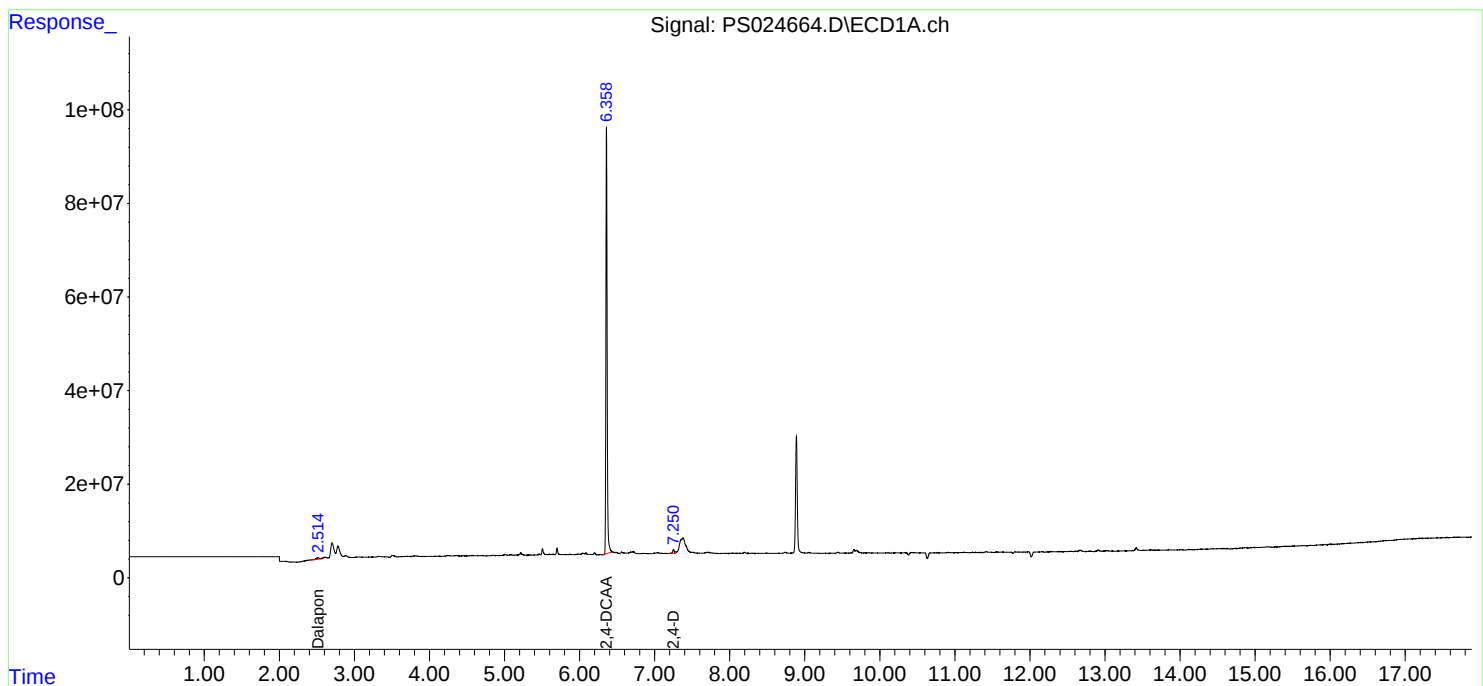


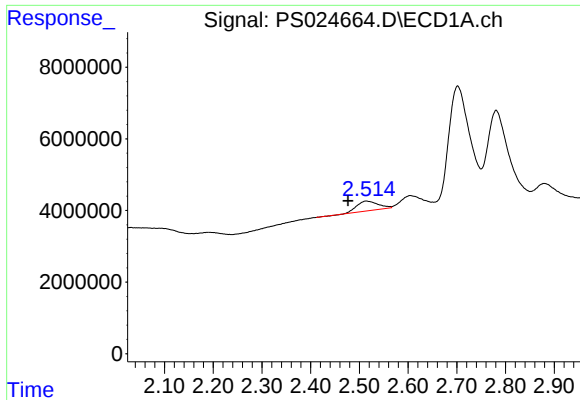

#1 Dalapon


R.T.: 2.514 min
Delta R.T.: 0.037 min
Response: 8296889
Conc: 3.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

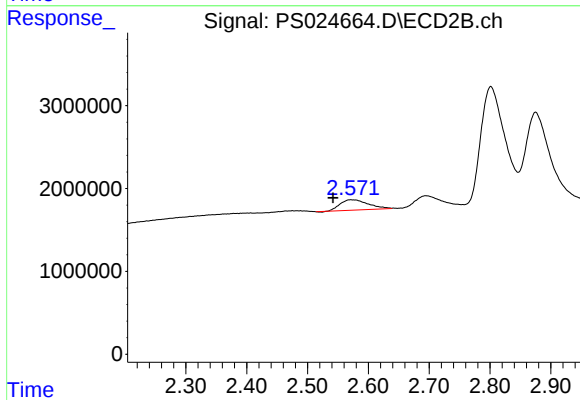


#1 Dalapon

R.T.: 2.571 min
Delta R.T.: 0.029 min
Response: 4073533
Conc: 3.64 ng/ml

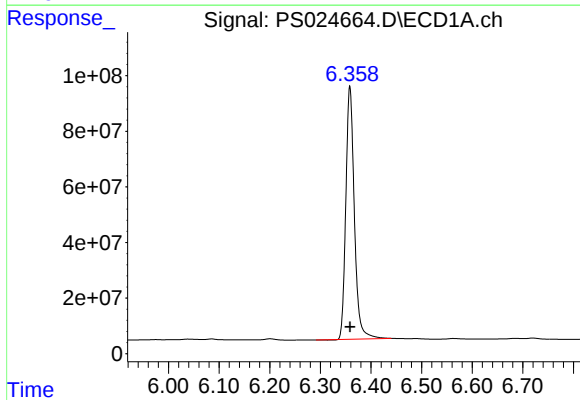


#4 2,4-DCAA

R.T.: 6.358 min
Delta R.T.: 0.000 min
Response: 1064622353
Conc: 517.48 ng/ml

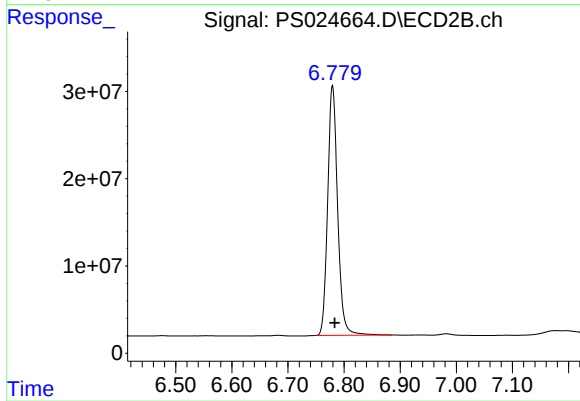

#4 2,4-DCAA


R.T.: 6.779 min
Delta R.T.: -0.004 min
Response: 353455284
Conc: 511.30 ng/ml

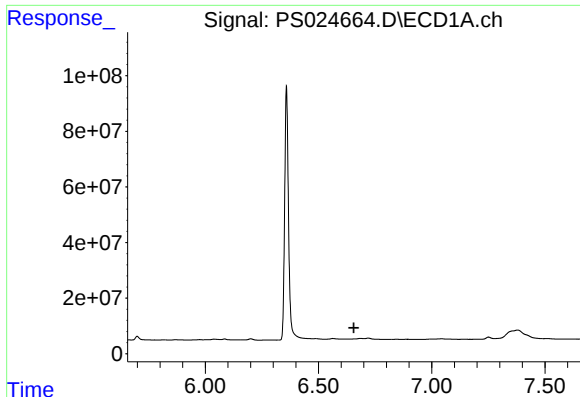

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.656 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

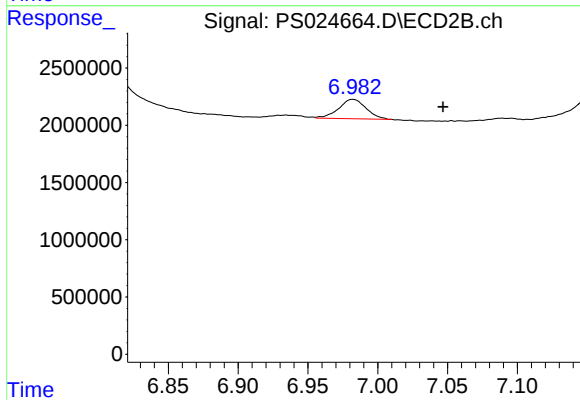


#6 MCPP

R.T.: 6.982 min
Delta R.T.: -0.065 min
Response: 2304395
Conc: 1.17 ug/ml

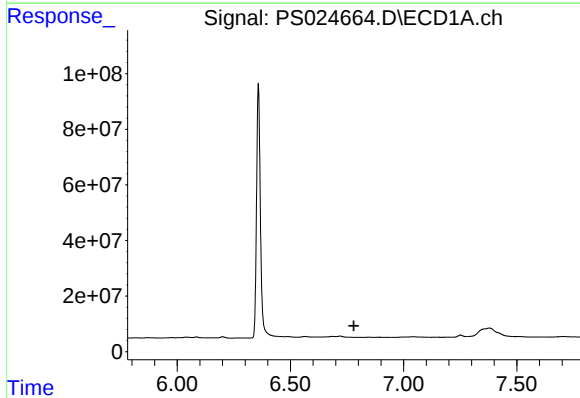


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.780 min
Response: 0
Conc: N.D.

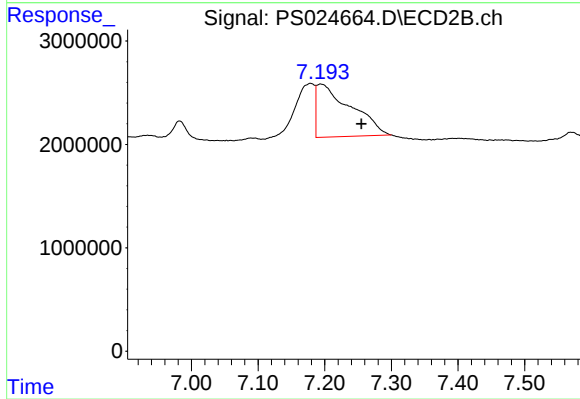

#7 MCPA


R.T.: 7.194 min
Delta R.T.: -0.061 min
Response: 18250184
Conc: 5.70 ug/ml

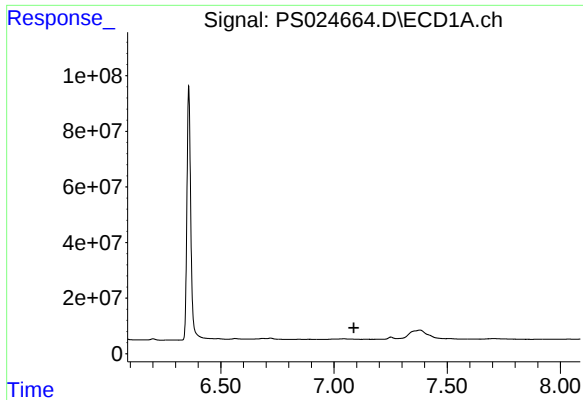

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.088 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

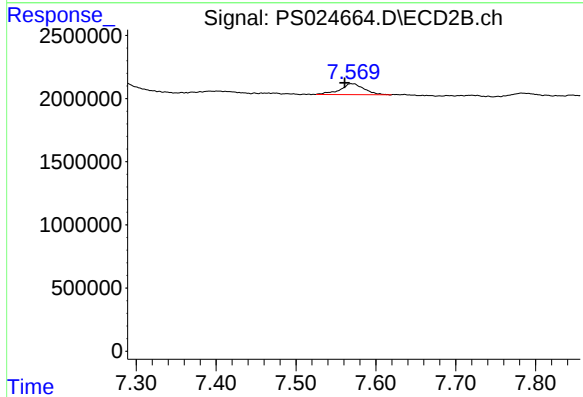


#8 DICHLORPROP

R.T.: 7.569 min
Delta R.T.: 0.008 min
Response: 1780208
Conc: 2.37 ng/ml

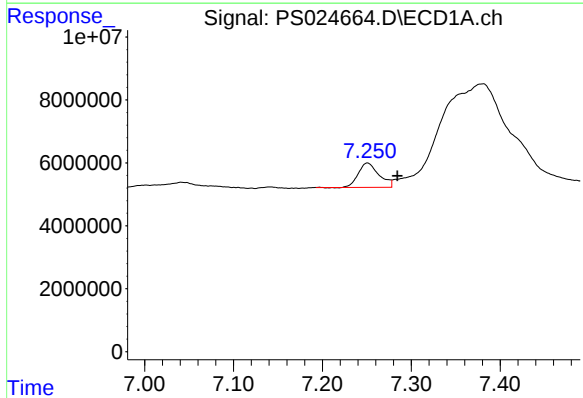


#9 2,4-D

R.T.: 7.251 min
Delta R.T.: -0.034 min
Response: 12615435
Conc: 4.57 ng/ml

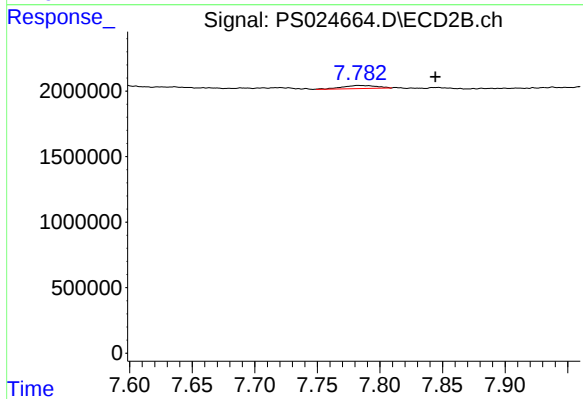

#9 2,4-D


R.T.: 7.783 min
Delta R.T.: -0.062 min
Response: 443305
Conc: N.D.

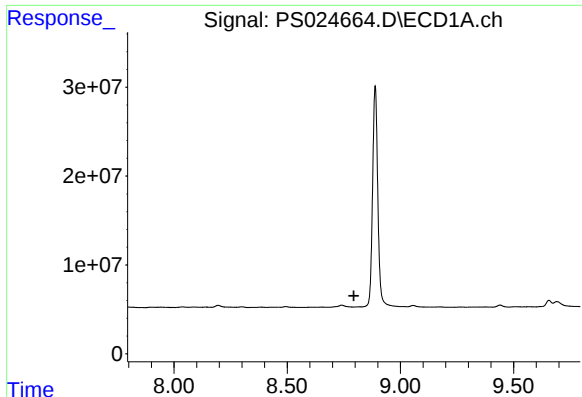

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

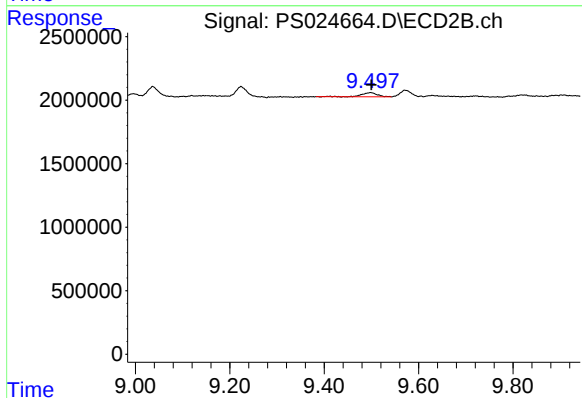


#13 2,4-DB

R.T.: 9.498 min
Delta R.T.: -0.002 min
Response: 744535
Conc: 1.46 ng/ml

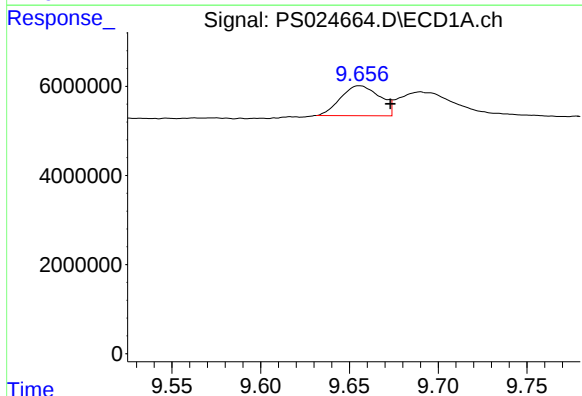


#15 Picloram

R.T.: 9.656 min
Delta R.T.: -0.017 min
Response: 10324514
Conc: N.D.

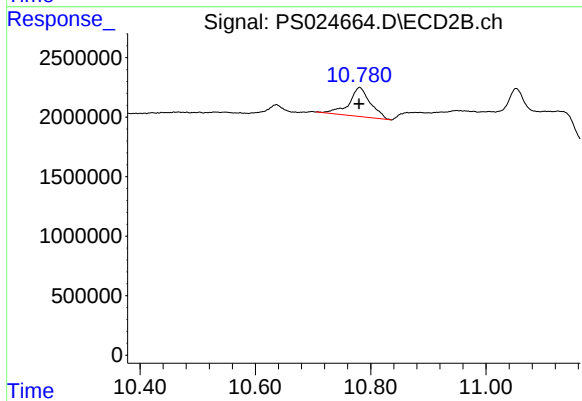

#15 Picloram


R.T.: 10.781 min
Delta R.T.: 0.000 min
Response: 6284452
Conc: 1.01 ng/ml

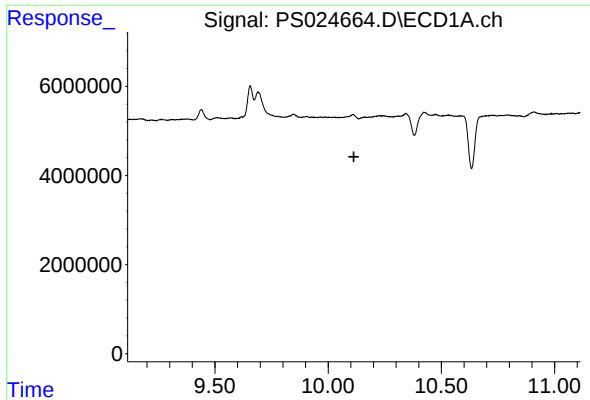

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.114 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

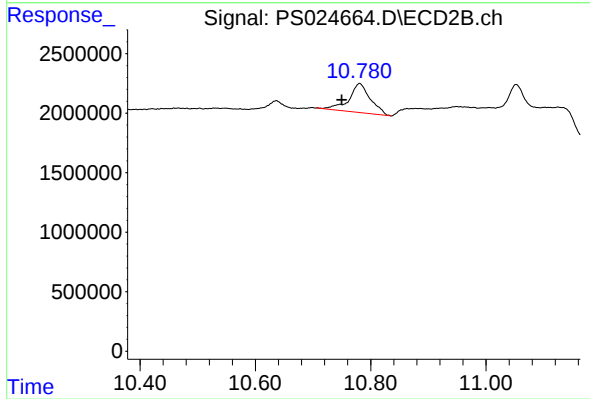

#16 DCPA

R.T.: 10.781 min
Delta R.T.: 0.031 min
Response: 6284452
Conc: 1.20 ng/ml