

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101824\
Data File : PS027992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2024 19:04
Operator : AR\AJ
Sample : P4425-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/21/2024
Supervised By :Ankita Jodhani 10/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 01:07:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	7.089	7.616	366.0E6	85190760	135.844m	85.732 #
------	----------	-------	-------	---------	----------	----------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101824\
Data File : PS027992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2024 19:04
Operator : AR\AJ
Sample : P4425-03
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/21/2024
Supervised By : Ankita Jodhani 10/21/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 01:07:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100724.M
Quant Title : 8080.M
QLast Update : Mon Oct 07 13:46:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

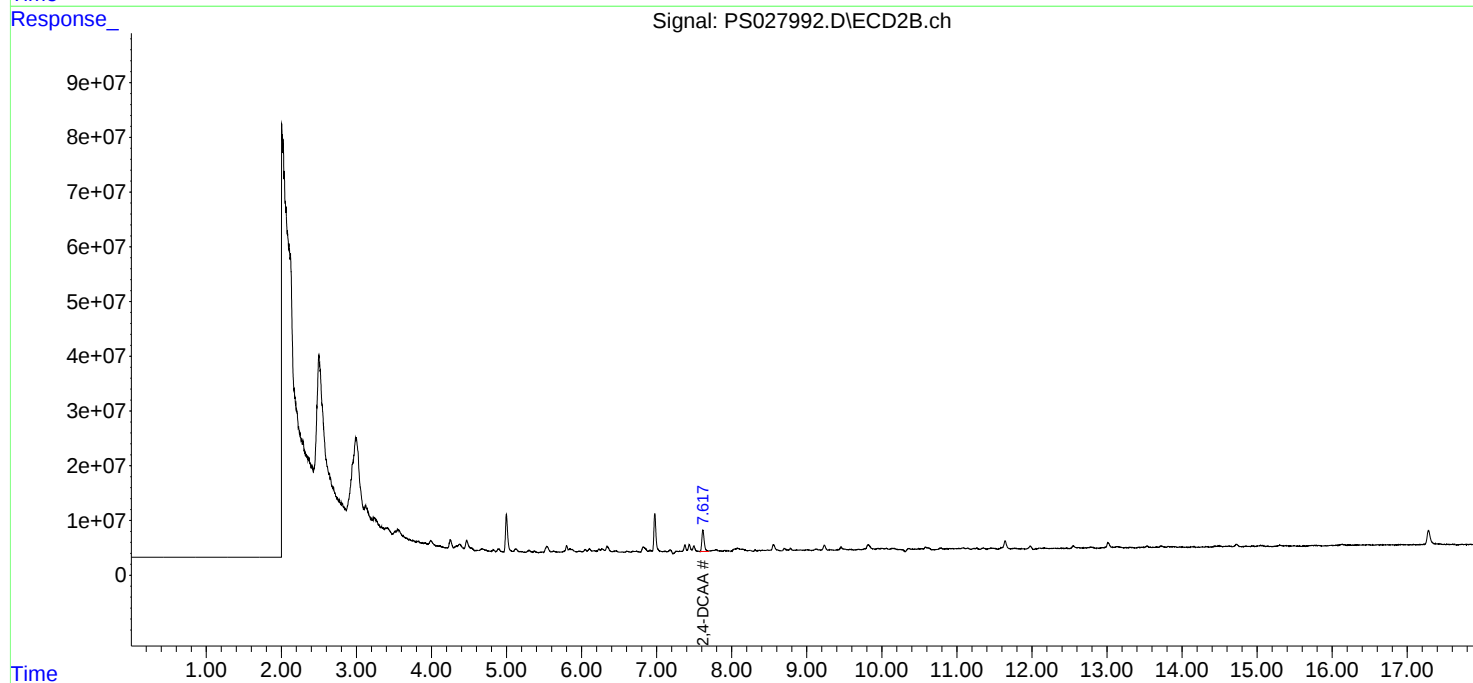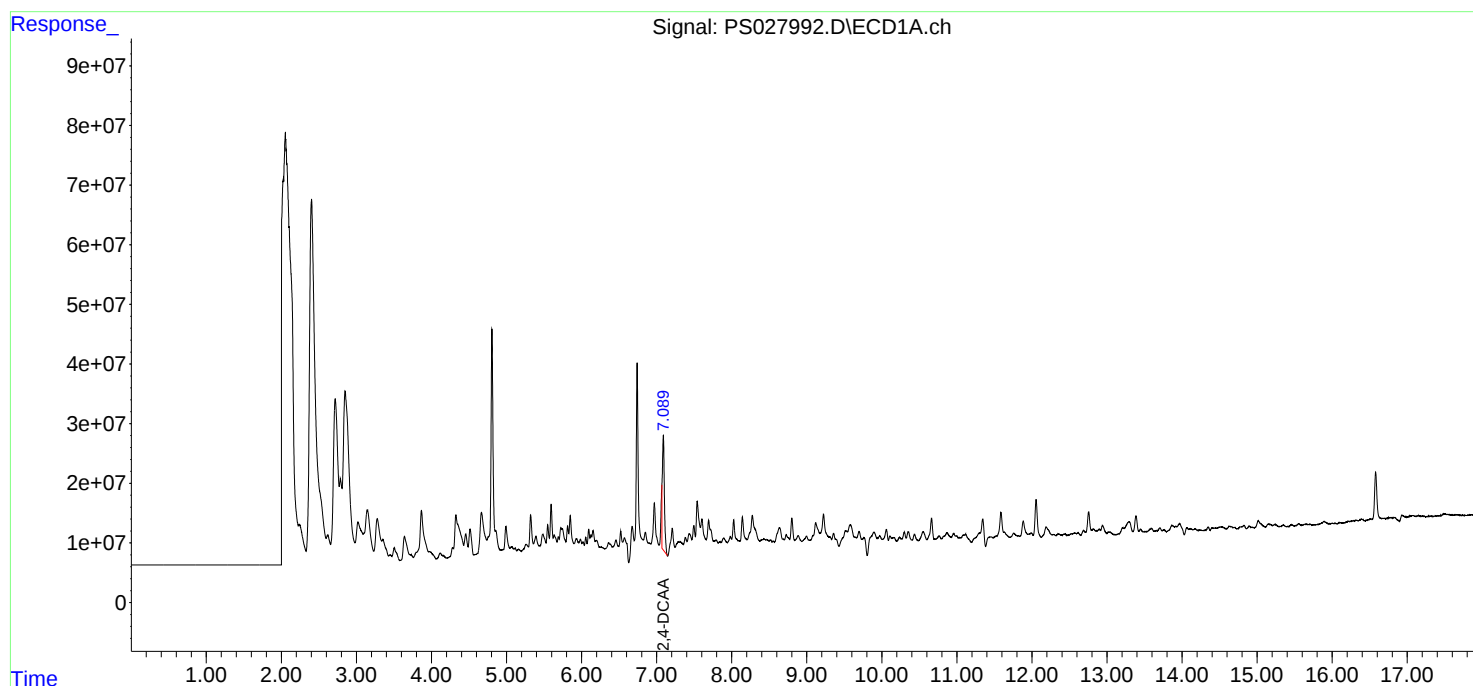

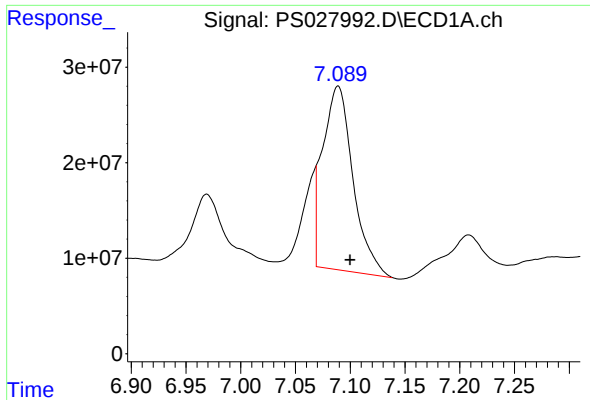


#4 2,4-DCAA

R.T.: 7.089 min
Delta R.T.: -0.011 min
Response: 366002987
Conc: 135.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/21/2024
Supervised By :Ankita Jodhani 10/21/2024

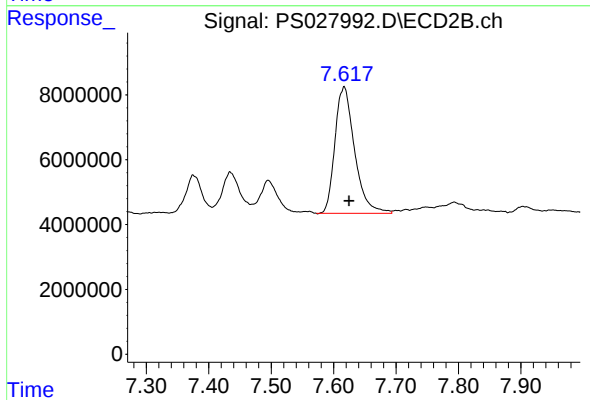

#4 2,4-DCAA

R.T.: 7.616 min
Delta R.T.: -0.008 min
Response: 85190760
Conc: 85.73 ng/ml