

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101918\
 Data File : PS002047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2018 11:56
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 02:15:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.444	10.936	103.7E6	100.3E6	490.540	420.601
Target Compounds							
12) T	2,4,5-T	0.000	14.561	0	2197070	N.D.	2.006 #
15) T	Picloram	16.982	16.871	3710981	4073184	2.171	2.568
16) T	DCPA	0.000	16.871	0	4073184	N.D.	2.251 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101918\
Data File : PS002047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2018 11:56
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 02:15:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

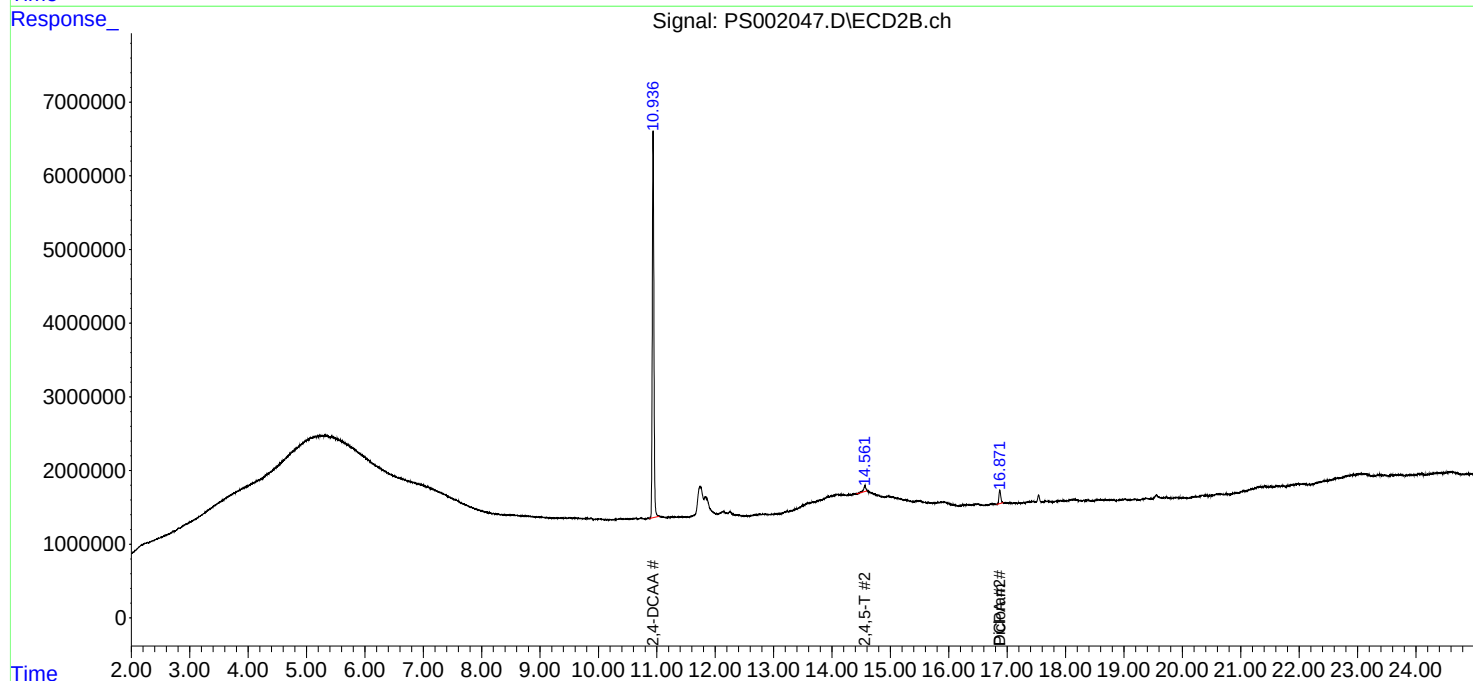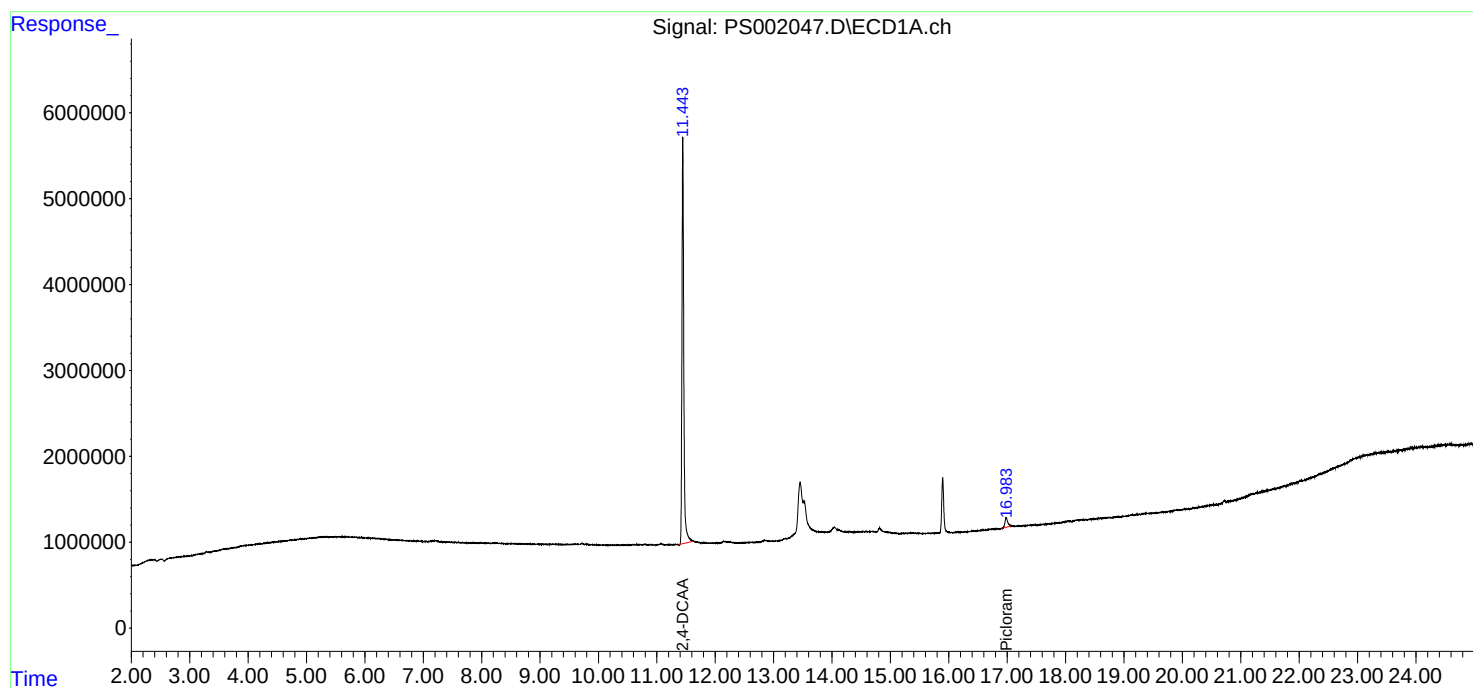


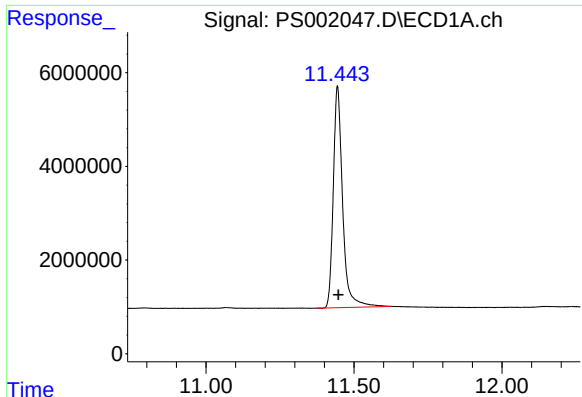

#4 2,4-DCAA


R.T.: 11.444 min
Delta R.T.: -0.003 min
Response: 103701214
Conc: 490.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

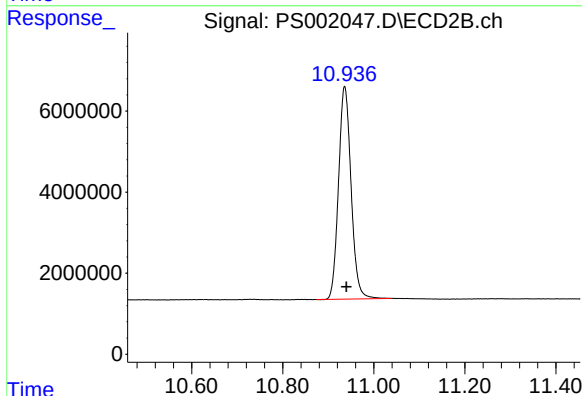


#4 2,4-DCAA

R.T.: 10.936 min
Delta R.T.: -0.004 min
Response: 100316203
Conc: 420.60 ng/ml

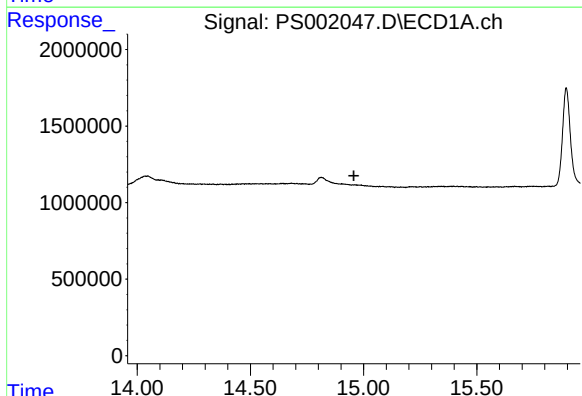


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.957 min
Response: 0
Conc: N.D.

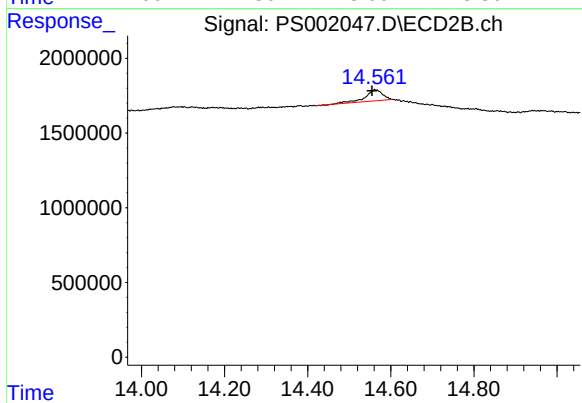

#12 2,4,5-T


R.T.: 14.561 min
Delta R.T.: 0.006 min
Response: 2197070
Conc: 2.01 ng/ml

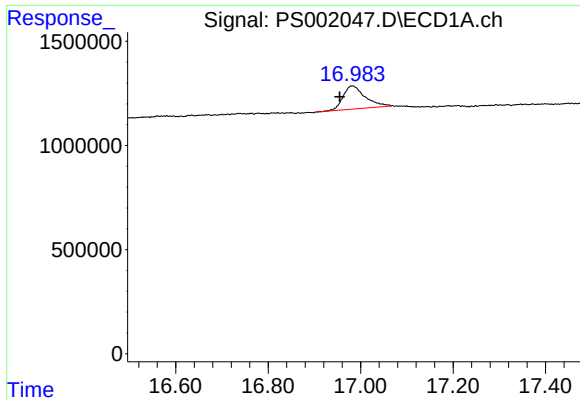

#15 Picloram


R.T.: 16.982 min
Delta R.T.: 0.027 min
Response: 3710981
Conc: 2.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

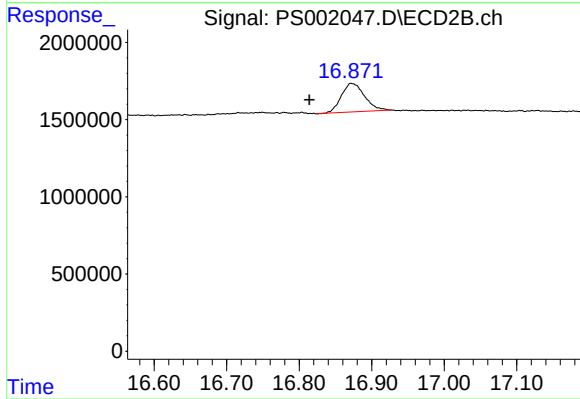


#15 Picloram

R.T.: 16.871 min
Delta R.T.: 0.057 min
Response: 4073184
Conc: 2.57 ng/ml

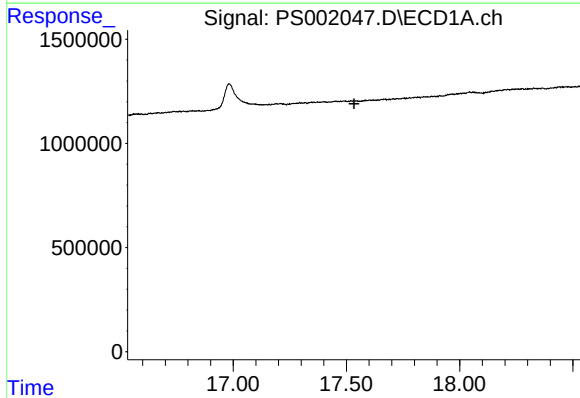

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.533 min
Response: 0
Conc: N.D.

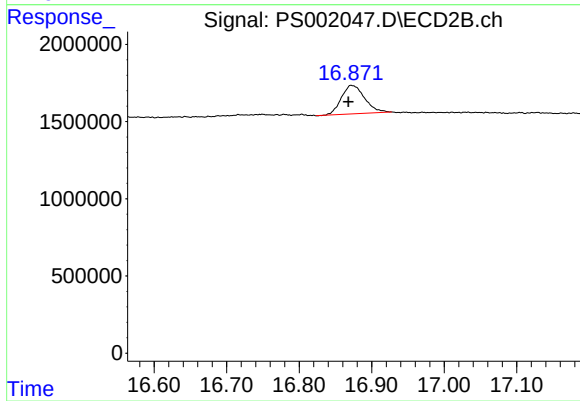

#16 DCPA

R.T.: 16.871 min
Delta R.T.: 0.004 min
Response: 4073184
Conc: 2.25 ng/ml