

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101918\
 Data File : PS002064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2018 01:50
 Operator : EI\SJ
 Sample : J5538-24
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 04:31:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
 Quant Title : 8080.M
 QLast Update : Wed Oct 17 08:59:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.454	10.950	54603137	53467379	258.290	224.175
Target Compounds							
1) T	Dalapon	2.894	2.391	157.8E6	684.0E6	517.055	2342.863 #
3) T	4-Nitroph...	11.031	0.000	49267693	0	365.121	N.D. #
5) T	DICAMBA	11.823	11.191	11059342	68558112	14.051	83.435 #
6) T	MCP	12.142	11.451	22327388	2448518	39.874	4.486 #
7) T	MCPA	0.000	11.883	0	15953730	N.D.	19.378 #
9) T	2,4-D	0.000	12.819	0	23428640	N.D.	78.405 #
10) T	Pentachlo...	13.673	0.000	12791696	0	4.520	N.D. #
12) T	2,4,5-T	14.905	14.612	5824577	47641210	4.967	43.495 #
13) T	2,4-DB	15.670	15.165	56451469	28719675	359.402	182.435 #
15) T	Picloram	16.969	16.816	7822897	10821266	4.576	6.822 #
16) T	DCPA	0.000	16.902	0	39213397	N.D.	21.674 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101918\
Data File : PS002064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2018 01:50
Operator : EI\SJ
Sample : J5538-24
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 04:31:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101518.M
Quant Title : 8080.M
QLast Update : Wed Oct 17 08:59:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

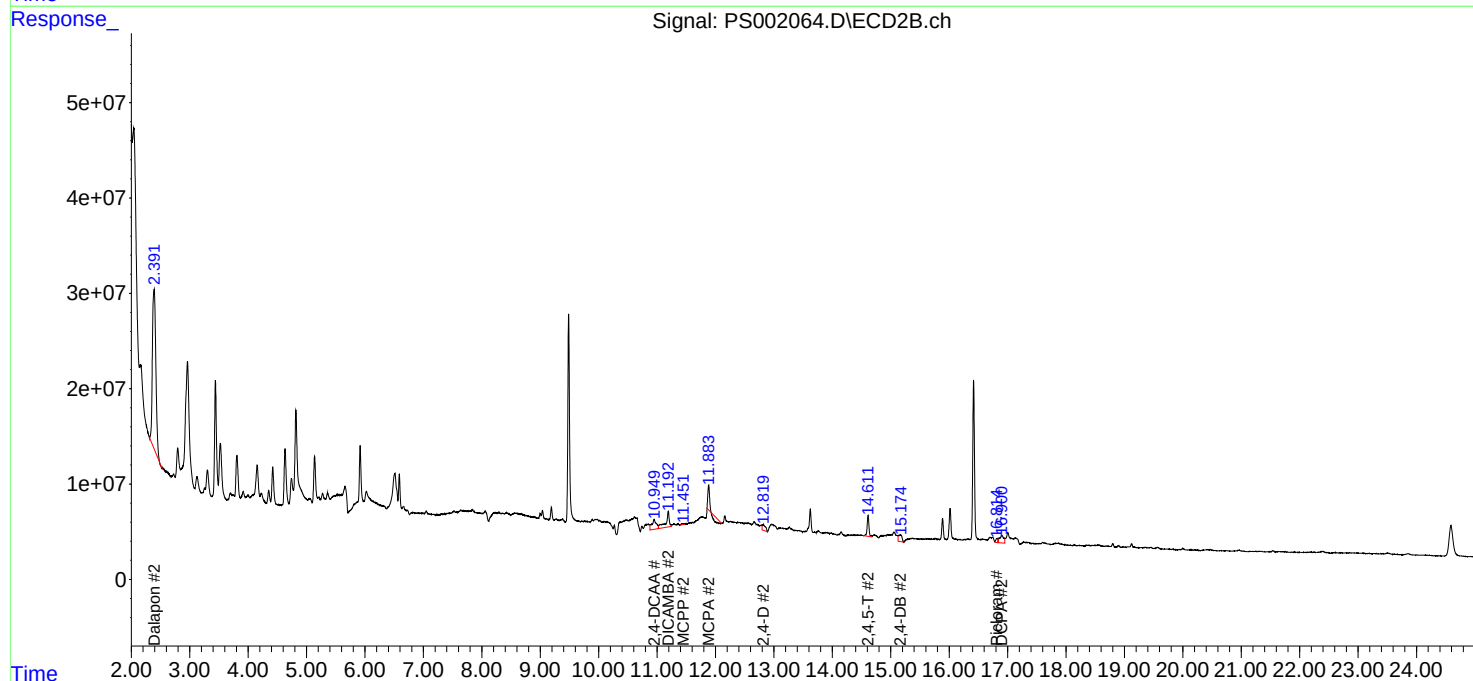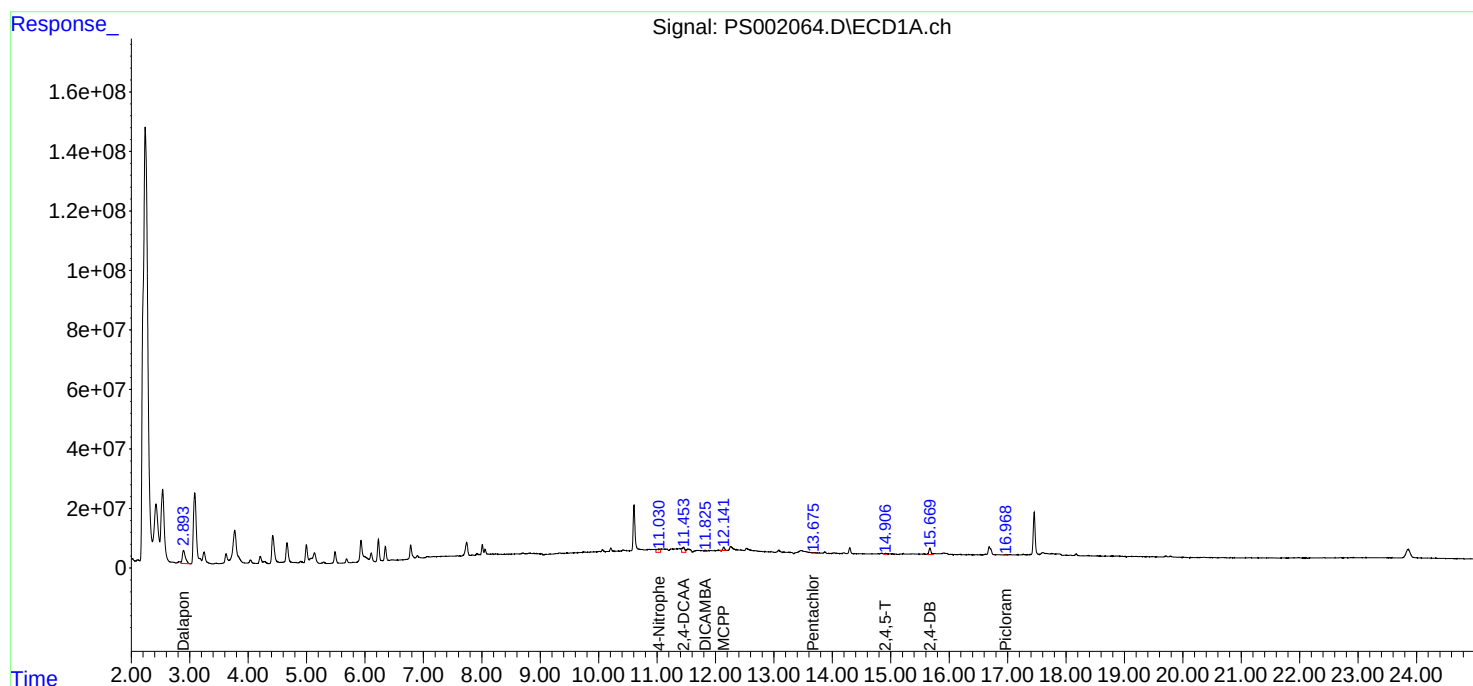


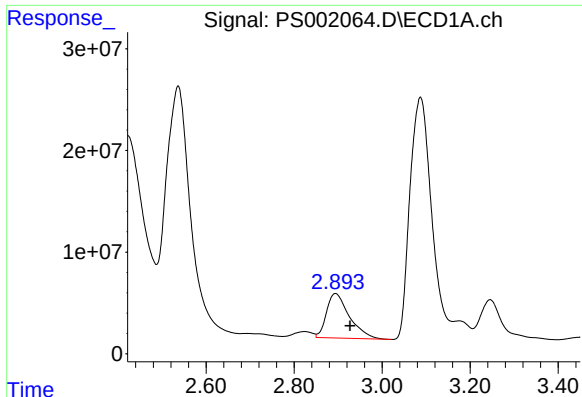

#1 Dalapon


R.T.: 2.894 min
Delta R.T.: -0.033 min
Response: 157783053
Conc: 517.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

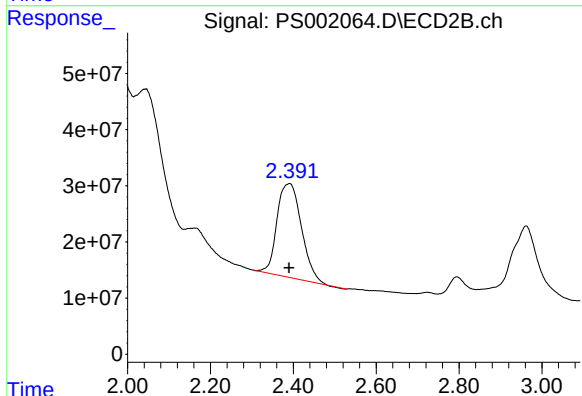


#1 Dalapon

R.T.: 2.391 min
Delta R.T.: 0.001 min
Response: 684038448
Conc: 2342.86 ng/ml

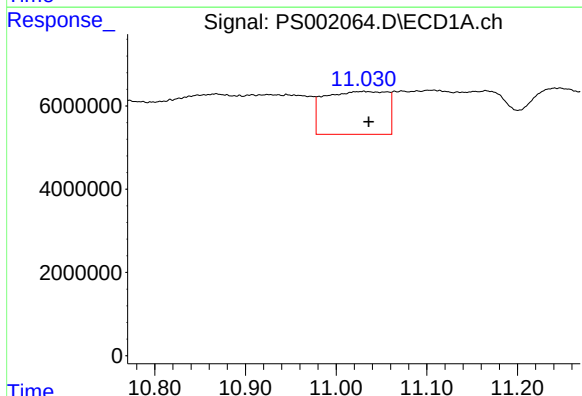


#3 4-Nitrophenol

R.T.: 11.031 min
Delta R.T.: -0.005 min
Response: 49267693
Conc: 365.12 ng/ml

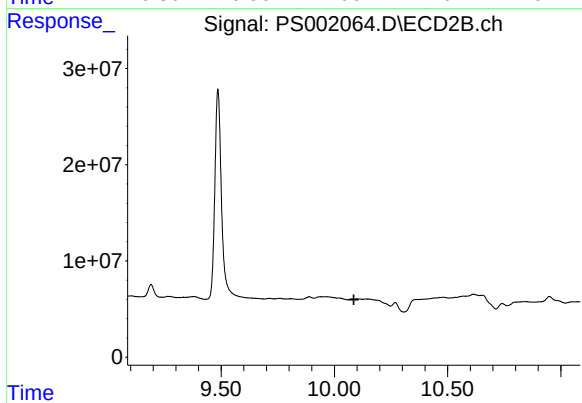

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.086 min
Response: 0
Conc: N.D.

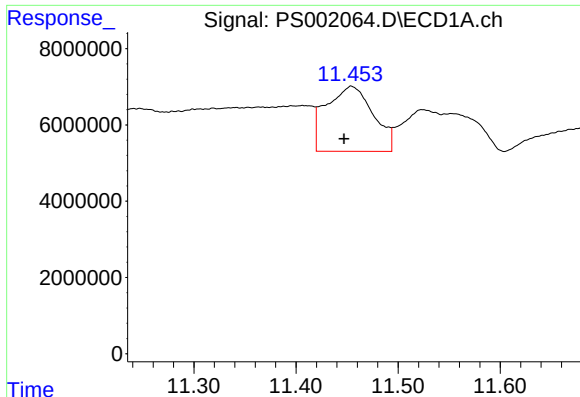

#4 2,4-DCAA


R.T.: 11.454 min
Delta R.T.: 0.008 min
Response: 54603137
Conc: 258.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

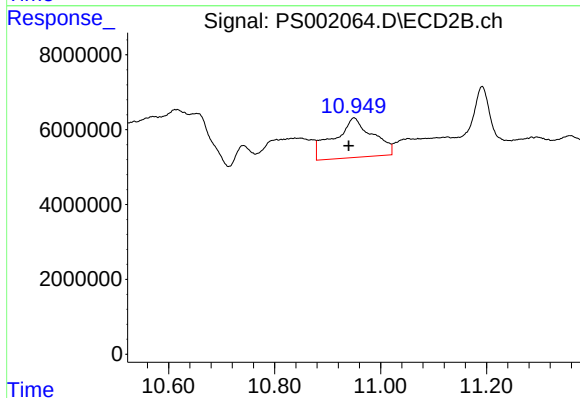


#4 2,4-DCAA

R.T.: 10.950 min
Delta R.T.: 0.010 min
Response: 53467379
Conc: 224.18 ng/ml

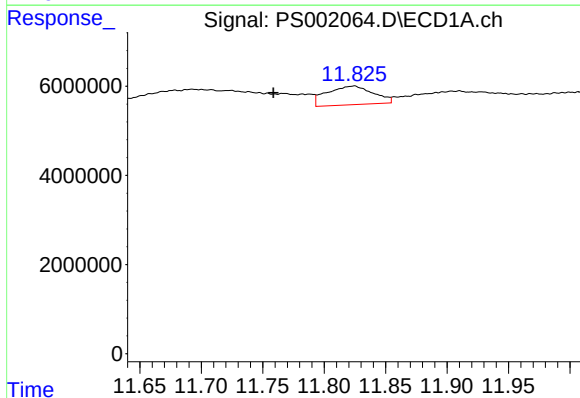


#5 DICAMBA

R.T.: 11.823 min
Delta R.T.: 0.065 min
Response: 11059342
Conc: 14.05 ng/ml

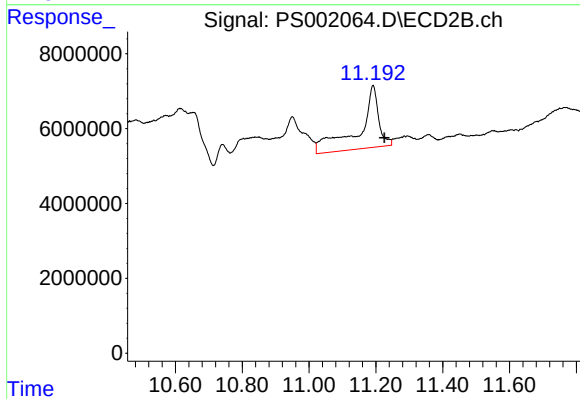

#5 DICAMBA


R.T.: 11.191 min
Delta R.T.: -0.034 min
Response: 68558112
Conc: 83.43 ng/ml

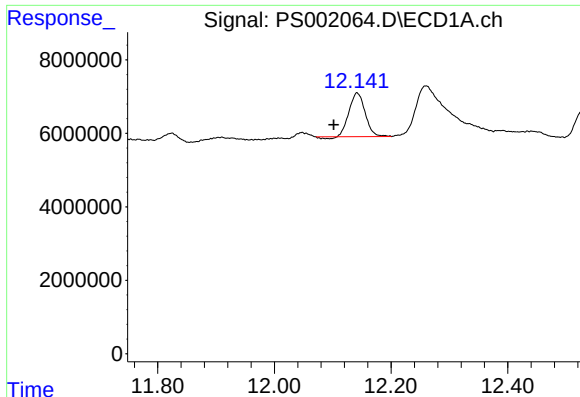

#6 MCPP


R.T.: 12.142 min
Delta R.T.: 0.040 min
Response: 22327388
Conc: 39.87 ug/ml

Instrument :
ECD_S
ClientSampleId :

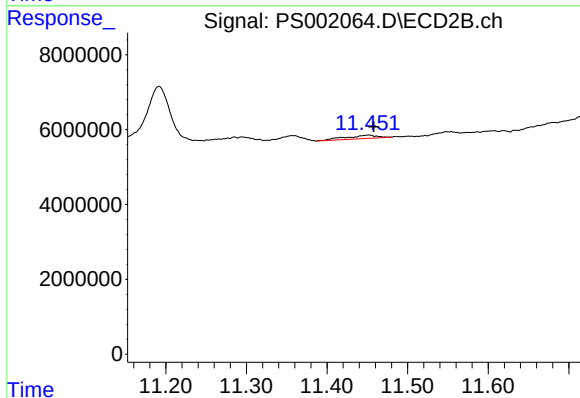


#6 MCPP

R.T.: 11.451 min
Delta R.T.: -0.007 min
Response: 2448518
Conc: 4.49 ug/ml

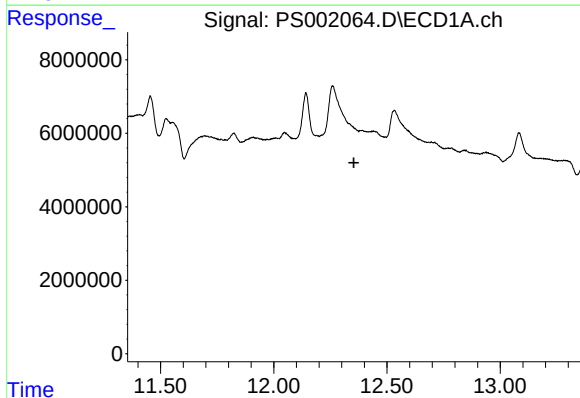


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.354 min
Response: 0
Conc: N.D.

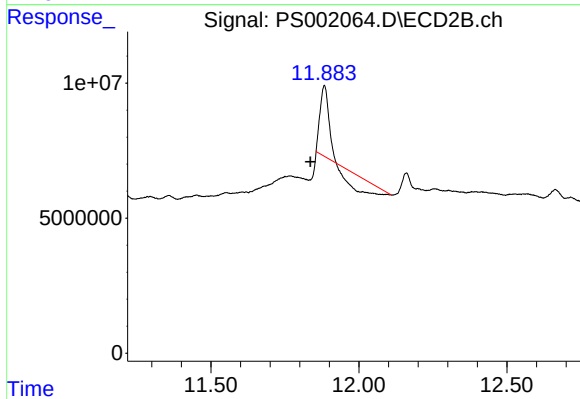

#7 MCPA


R.T.: 11.883 min
Delta R.T.: 0.047 min
Response: 15953730
Conc: 19.38 ug/ml

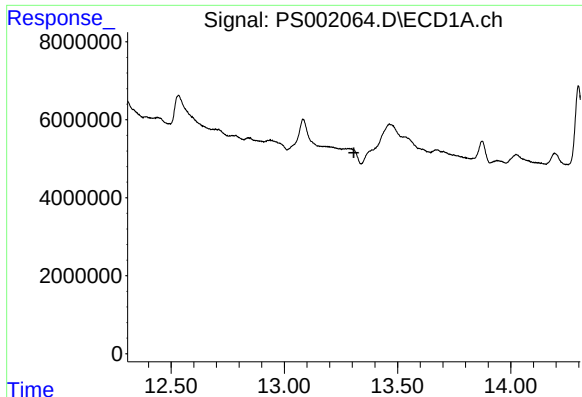

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.307 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

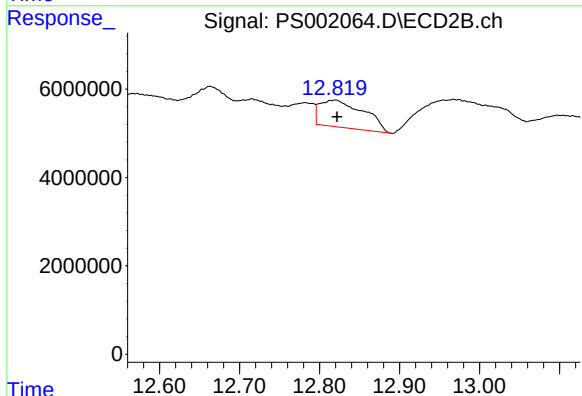


#9 2,4-D

R.T.: 12.819 min
Delta R.T.: -0.003 min
Response: 23428640
Conc: 78.41 ng/ml

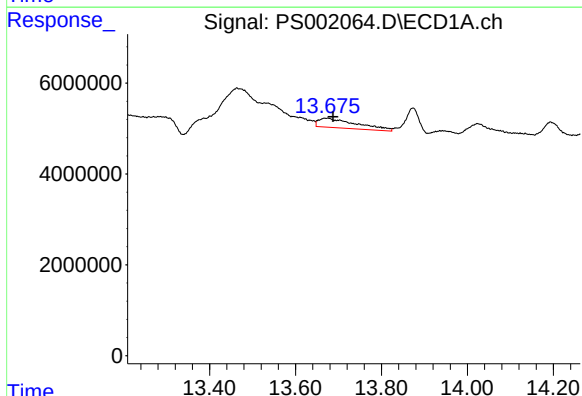


#10 Pentachlorophenol

R.T.: 13.673 min
Delta R.T.: -0.014 min
Response: 12791696
Conc: 4.52 ng/ml

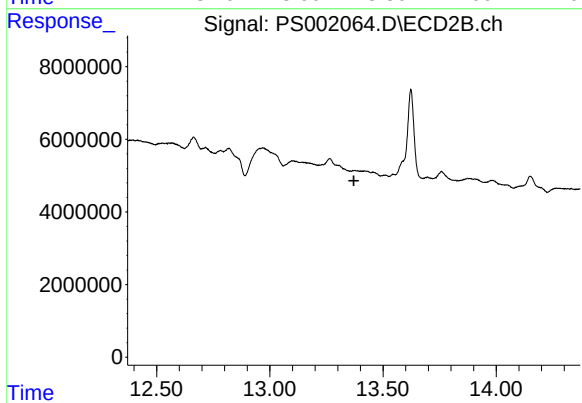

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.371 min
Response: 0
Conc: N.D.

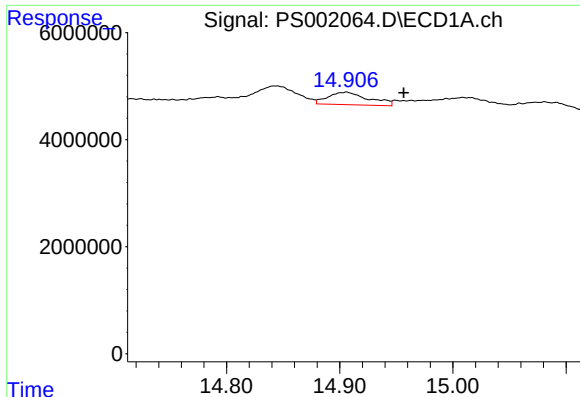

#12 2,4,5-T


R.T.: 14.905 min
Delta R.T.: -0.052 min
Response: 5824577
Conc: 4.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

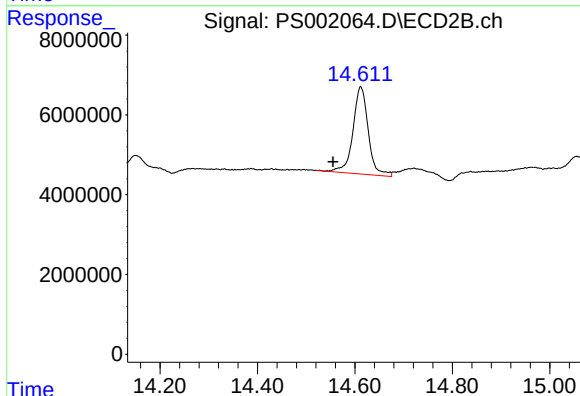


#12 2,4,5-T

R.T.: 14.612 min
Delta R.T.: 0.057 min
Response: 47641210
Conc: 43.50 ng/ml

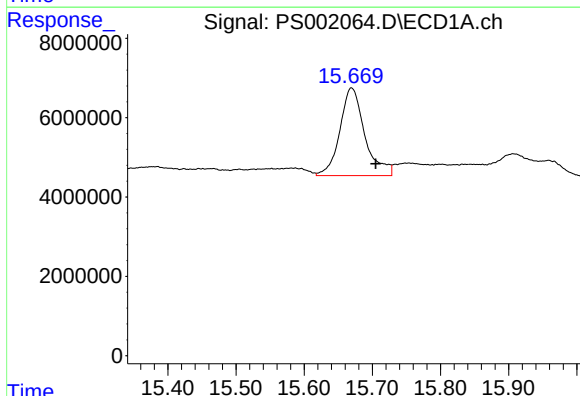


#13 2,4-DB

R.T.: 15.670 min
Delta R.T.: -0.035 min
Response: 56451469
Conc: 359.40 ng/ml

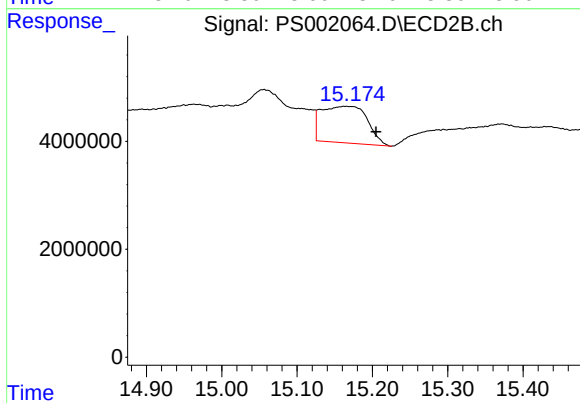

#13 2,4-DB


R.T.: 15.165 min
Delta R.T.: -0.040 min
Response: 28719675
Conc: 182.44 ng/ml

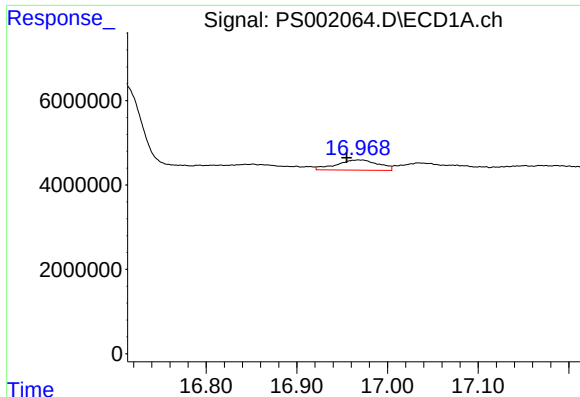

#15 Picloram


R.T.: 16.969 min
Delta R.T.: 0.014 min
Response: 7822897
Conc: 4.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

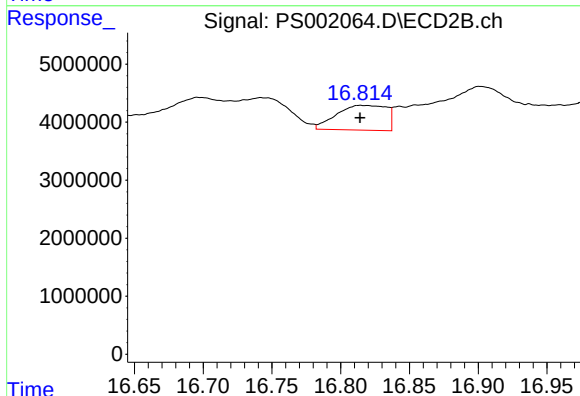


#15 Picloram

R.T.: 16.816 min
Delta R.T.: 0.002 min
Response: 10821266
Conc: 6.82 ng/ml

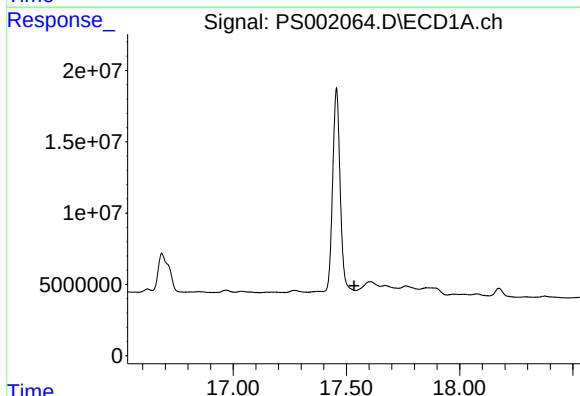

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.533 min
Response: 0
Conc: N.D.

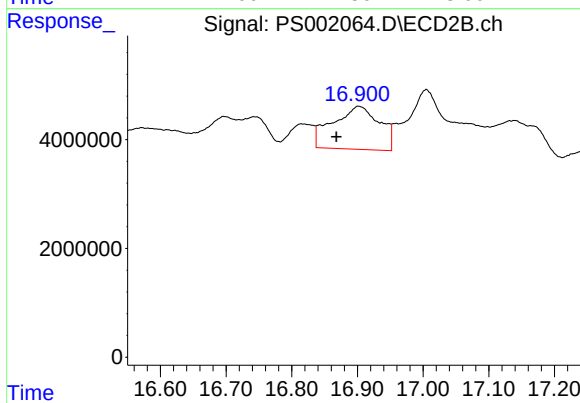

#16 DCPA

R.T.: 16.902 min
Delta R.T.: 0.034 min
Response: 39213397
Conc: 21.67 ng/ml