

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101922\
 Data File : PS020829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2022 09:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 22:18:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
 Quant Title : 8080.M
 QLast Update : Fri Oct 07 06:09:52 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.417	6.860	956.5E6	675.3E6	507.048	504.319
Target Compounds							
1) T	Dalapon	2.497	0.000	137230	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.800	0.000	675127	0	<MDL	N.D. #
5) T	DICAMBA	6.577	0.000	488670	0	<MDL	N.D. #
6) T	MCP	6.745	0.000	2596126	0	<MDL	N.D. #
7) T	MCPA	6.918f	0.000	168560	0	<MDL	N.D. #
8) T	DICHLORPROP	7.211f	7.675	1175837	802864	<MDL	<MDL #
9) T	2,4-D	7.380	0.000	146663	0	<MDL	N.D. #
10) T	Pentachlo...	7.649f	0.000	323243	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.138	0.000	1006580	0	<MDL	N.D. #
12) T	2,4,5-T	8.405	9.164	3070085	1907561	<MDL	<MDL #
13) T	2,4-DB	8.877	0.000	1056782	0	<MDL	N.D. #
14) T	DINOSEB	9.970	0.000	552126	0	<MDL	N.D. #
15) T	Picloram	9.784	10.929	12329589	7262694	<MDL	<MDL #
16) T	DCPA	10.224	10.929	2131167	7262694	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS101922\
Data File : PS020829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2022 09:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 22:18:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS100622.M
Quant Title : 8080.M
QLast Update : Fri Oct 07 06:09:52 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

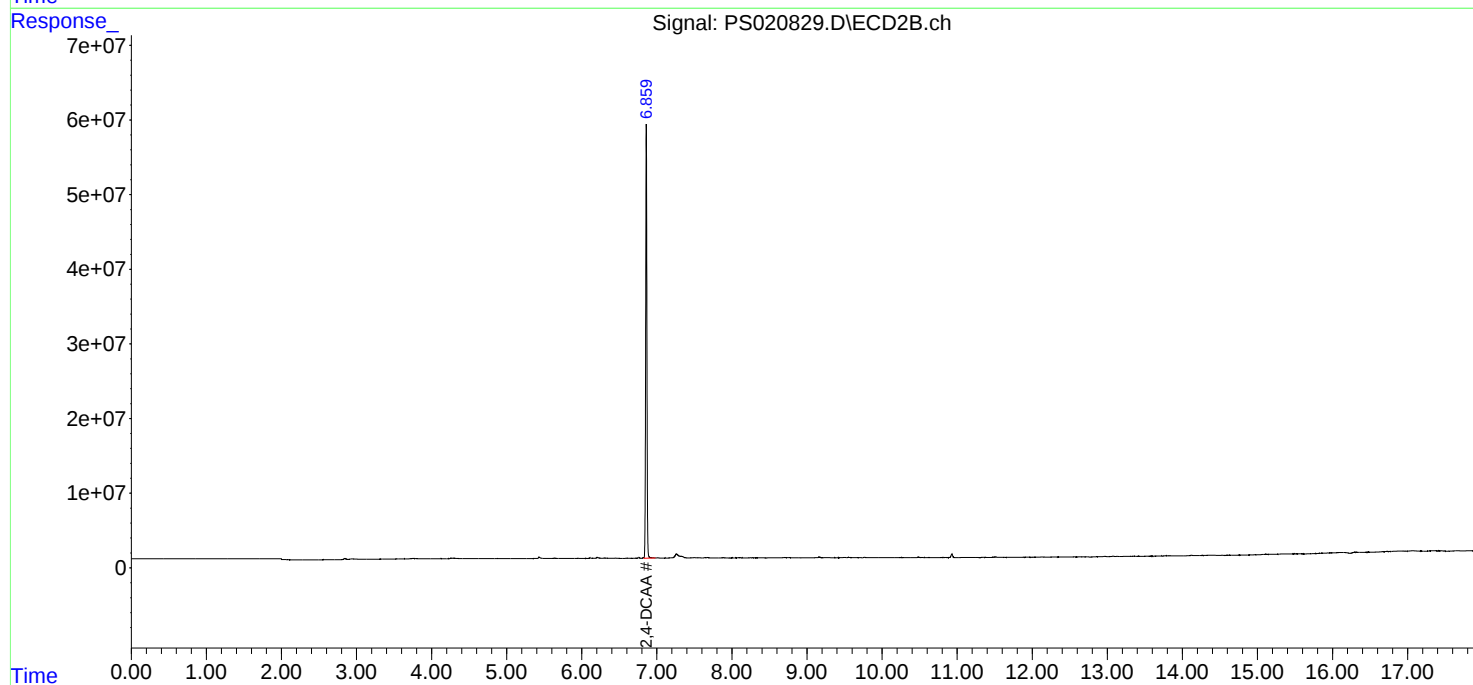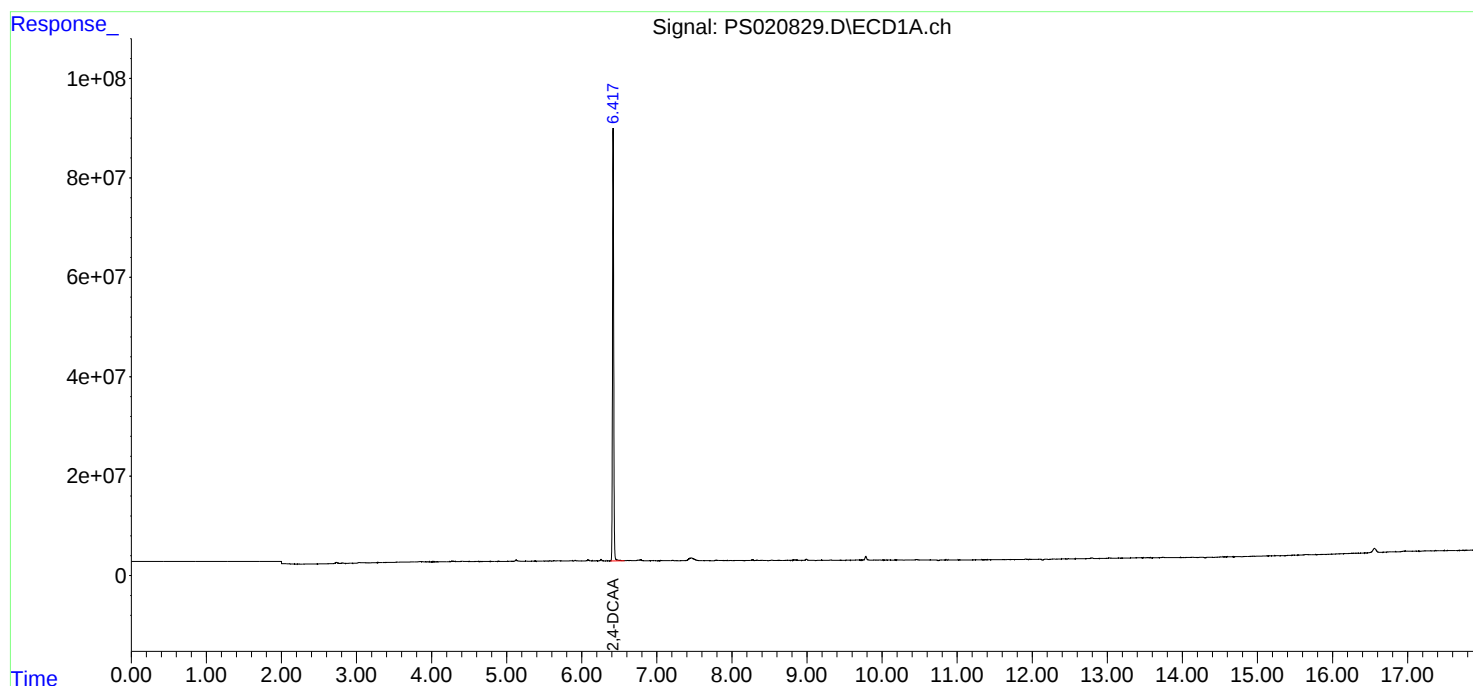


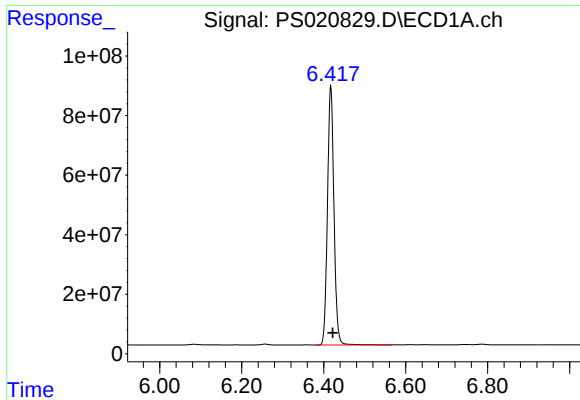

#4 2,4-DCAA

R.T.: 6.417 min
Delta R.T.: -0.005 min
Response: 956520266
Conc: 507.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

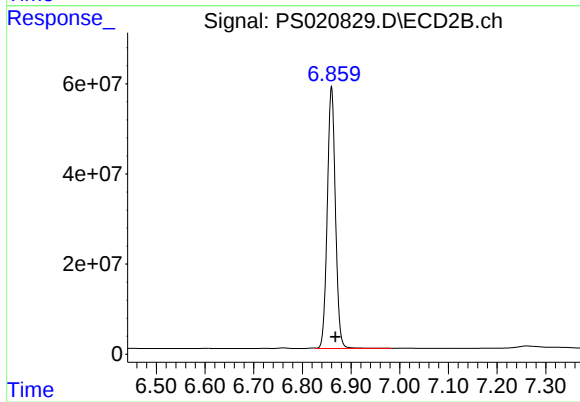

#4 2,4-DCAA

R.T.: 6.860 min
Delta R.T.: -0.008 min
Response: 675273061
Conc: 504.32 ng/ml